

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031723\
 Data File : PL081540.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2023 13:35
 Operator : AR\AJ
 Sample : 01954-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SV-TP5-0316

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 22:18:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:48:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.332	2.661	21120284	18622729	9.775	9.202
28)	SA Decachlor...	8.760	7.786	14185724	17937373	9.305	9.364
Target Compounds							
10)	B gamma-Chl...	5.709	4.853	1161278	421421	0.509m	0.172m#
11)	B alpha-Chl...	5.790	4.914	4896642	2366263	2.173m	0.966m#
12)	B 4,4'-DDE	5.964	5.105	1650910	1793297	0.844	0.914m
17)	MA 4,4'-DDT	6.791	5.910	1322836	1407350	0.833m	0.877



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031723\
Data File : PL081540.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2023 13:35
Operator : AR\AJ
Sample : 01954-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SV-TP5-0316

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 22:18:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:48:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

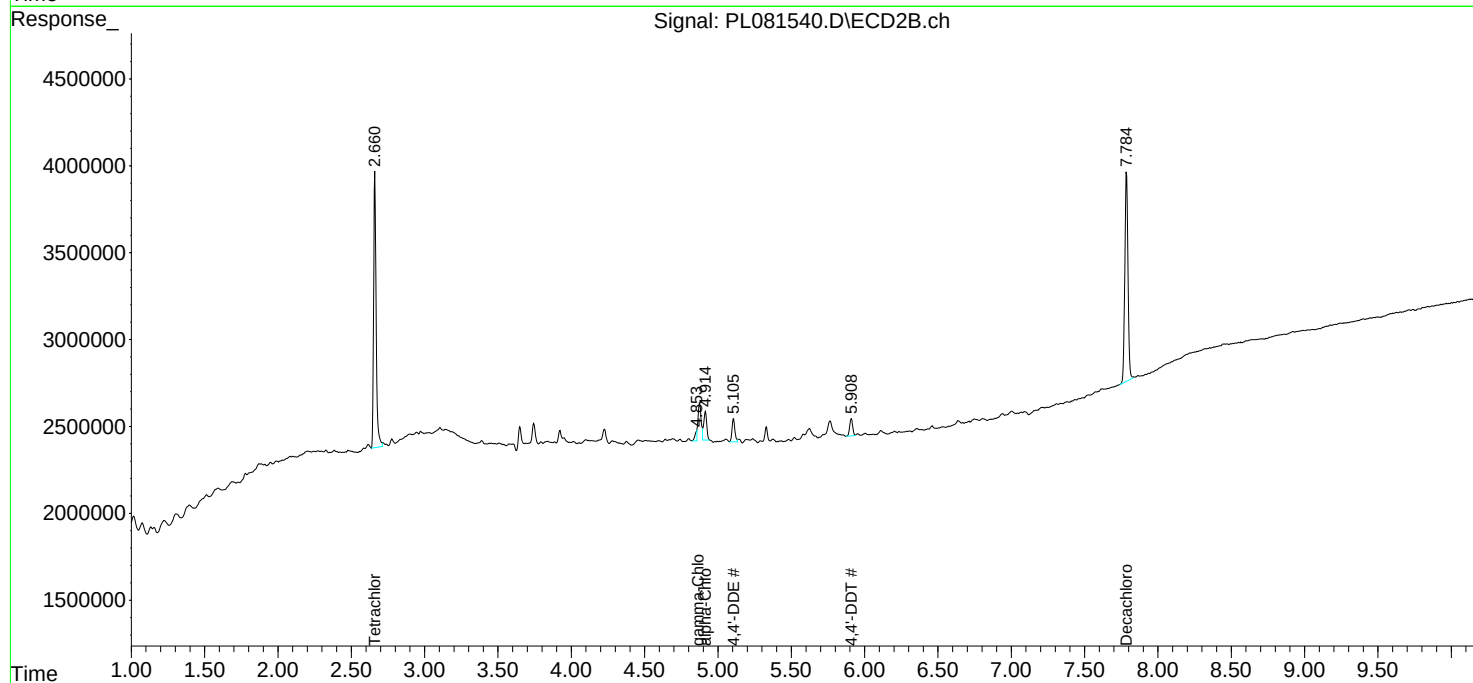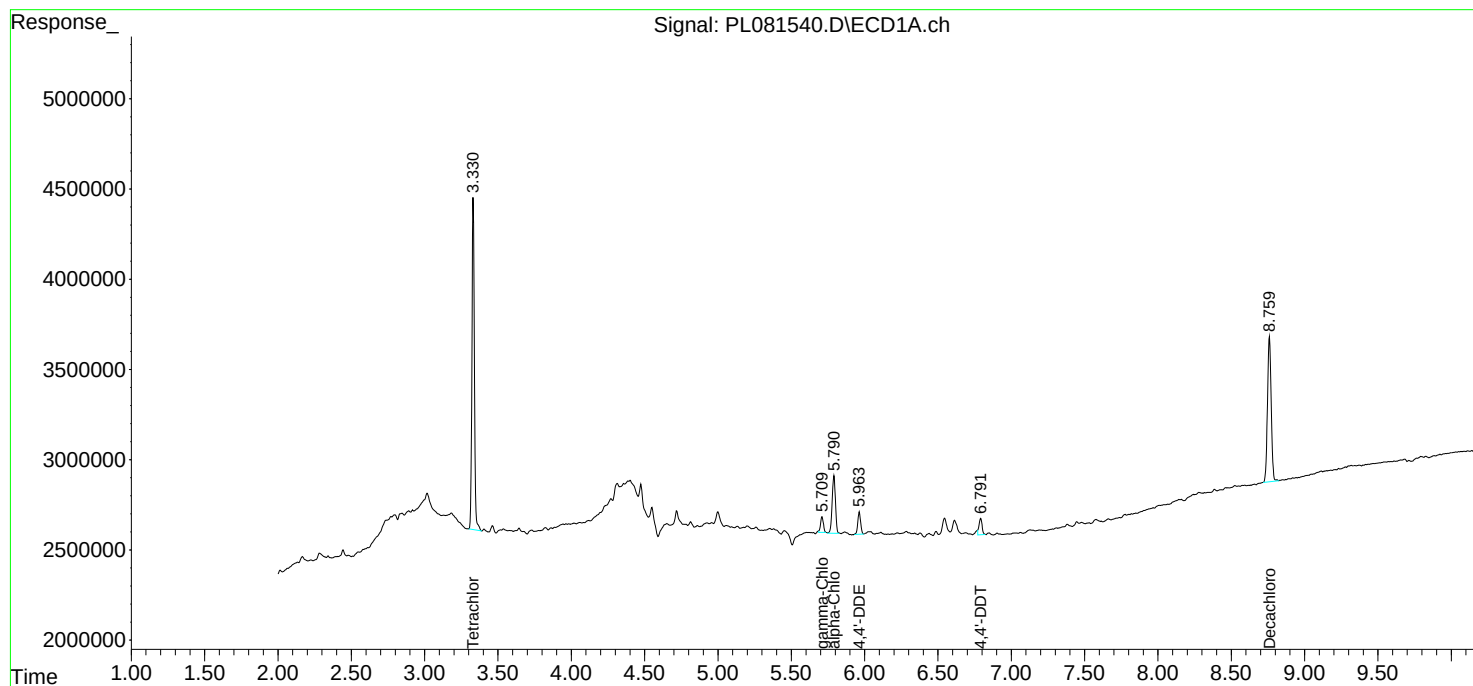


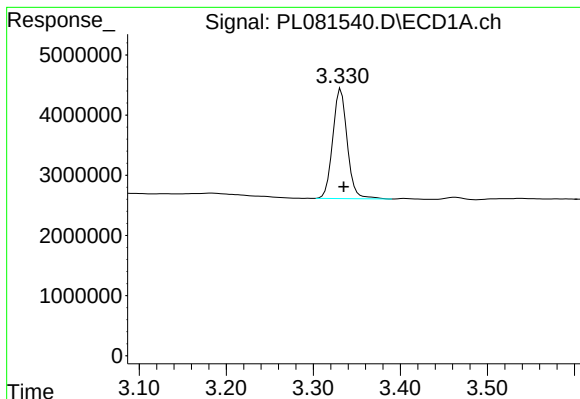

#1 Tetrachloro-m-xylene


R.T.: 3.332 min
Delta R.T.: -0.003 min
Response: 21120284
Conc: 9.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
SV-TP5-0316

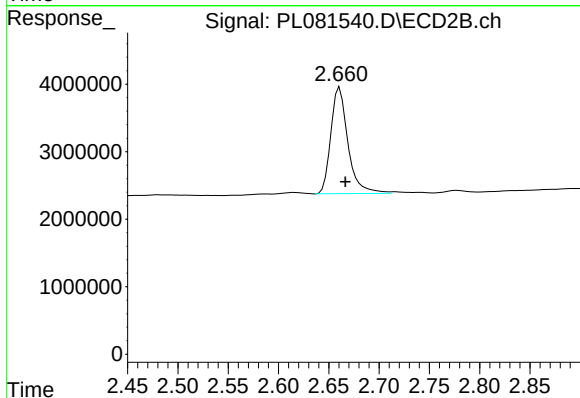


#1 Tetrachloro-m-xylene

R.T.: 2.661 min
Delta R.T.: -0.005 min
Response: 18622729
Conc: 9.20 ng/ml

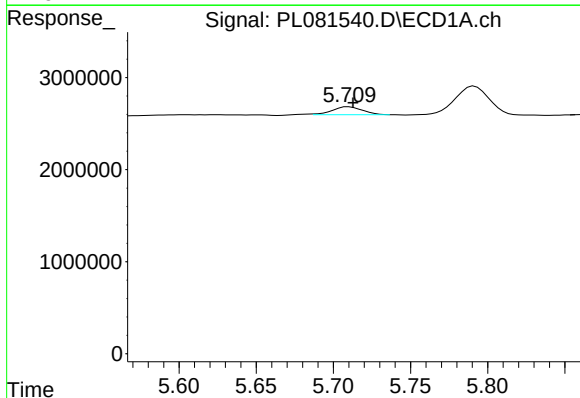


#10 gamma-Chlordane

R.T.: 5.709 min
Delta R.T.: -0.004 min
Response: 1161278
Conc: 0.51 ng/ml m

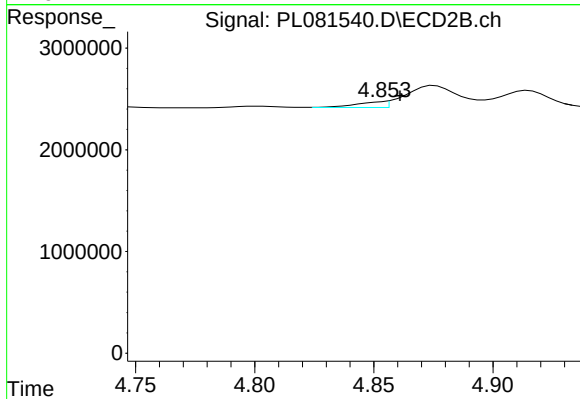

#10 gamma-Chlordane


R.T.: 4.853 min
Delta R.T.: -0.008 min
Response: 421421
Conc: 0.17 ng/ml m

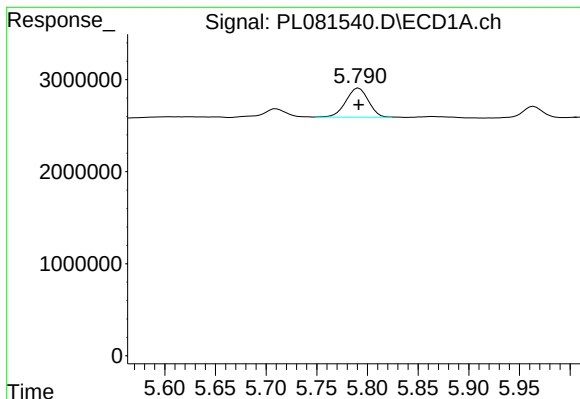

#11 alpha-Chlordane


R.T.: 5.790 min
Delta R.T.: -0.001 min
Response: 4896642
Conc: 2.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
SV-TP5-0316

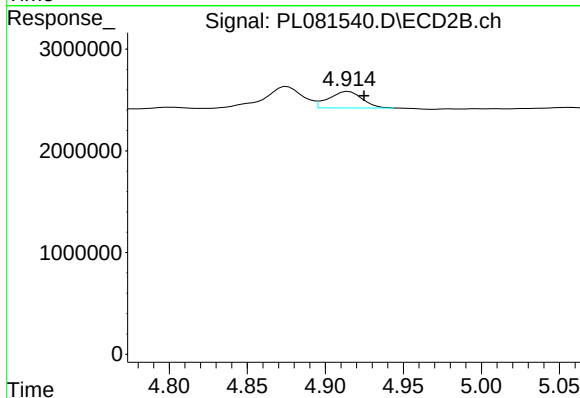


#11 alpha-Chlordane

R.T.: 4.914 min
Delta R.T.: -0.011 min
Response: 2366263
Conc: 0.97 ng/ml m

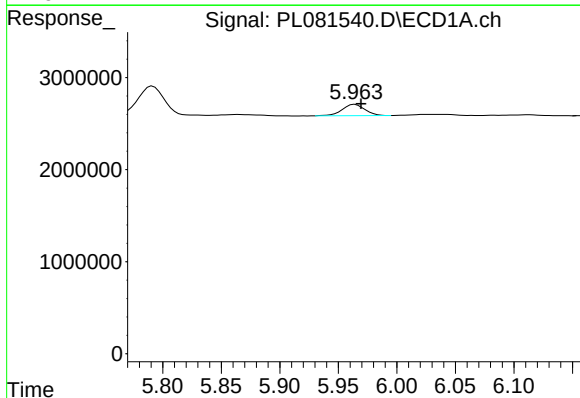


#12 4,4'-DDE

R.T.: 5.964 min
Delta R.T.: -0.005 min
Response: 1650910
Conc: 0.84 ng/ml

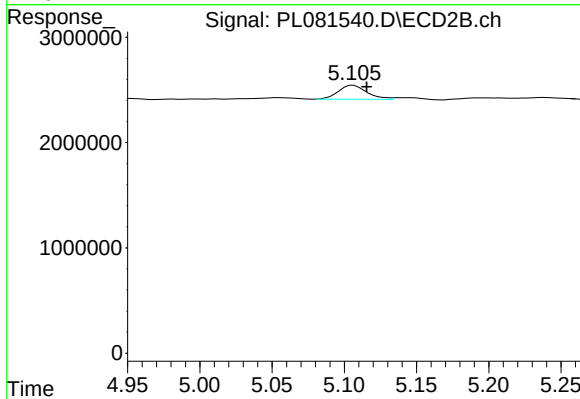

#12 4,4'-DDE


R.T.: 5.105 min
Delta R.T.: -0.010 min
Response: 1793297
Conc: 0.91 ng/ml m

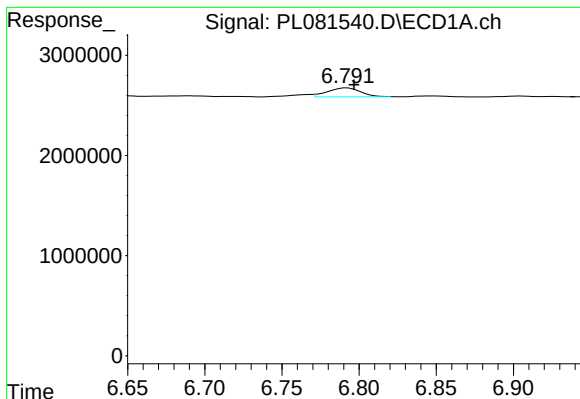

#17 4,4'-DDT


R.T.: 6.791 min
Delta R.T.: -0.006 min
Response: 1322836
Conc: 0.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
SV-TP5-0316

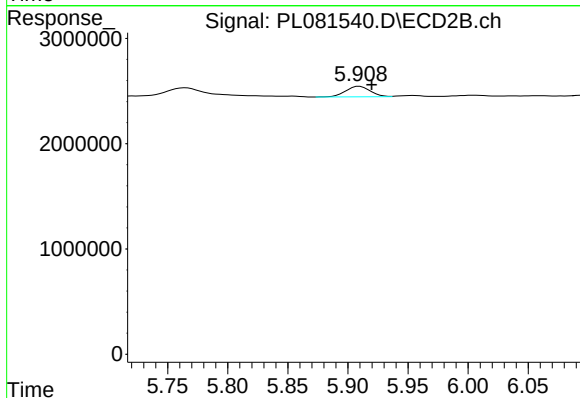


#17 4,4'-DDT

R.T.: 5.910 min
Delta R.T.: -0.010 min
Response: 1407350
Conc: 0.88 ng/ml

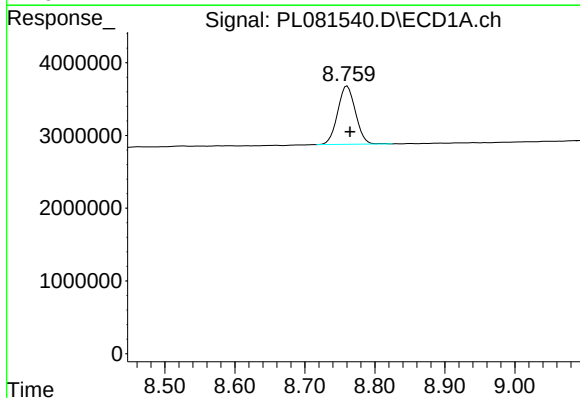

#28 Decachlorobiphenyl

R.T.: 8.760 min
Delta R.T.: -0.004 min
Response: 14185724
Conc: 9.30 ng/ml

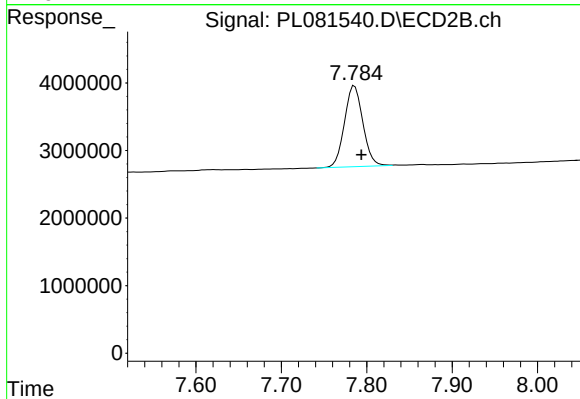

#28 Decachlorobiphenyl

R.T.: 7.786 min
Delta R.T.: -0.008 min
Response: 17937373
Conc: 9.36 ng/ml