

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031723\
 Data File : PL081550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2023 15:54
 Operator : AR\AJ
 Sample : 01965-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 22:27:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:48:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	2.680	37018850	33368584	17.134	16.488
28)	SA Decachlor...	8.755	7.802	19706952	25113321	12.926	13.110
Target Compounds							
12)	B 4,4'-DDE	5.963	5.123	1386002	1517536	0.708	0.773m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031723\
Data File : PL081550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2023 15:54
Operator : AR\AJ
Sample : 01965-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 22:27:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:48:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

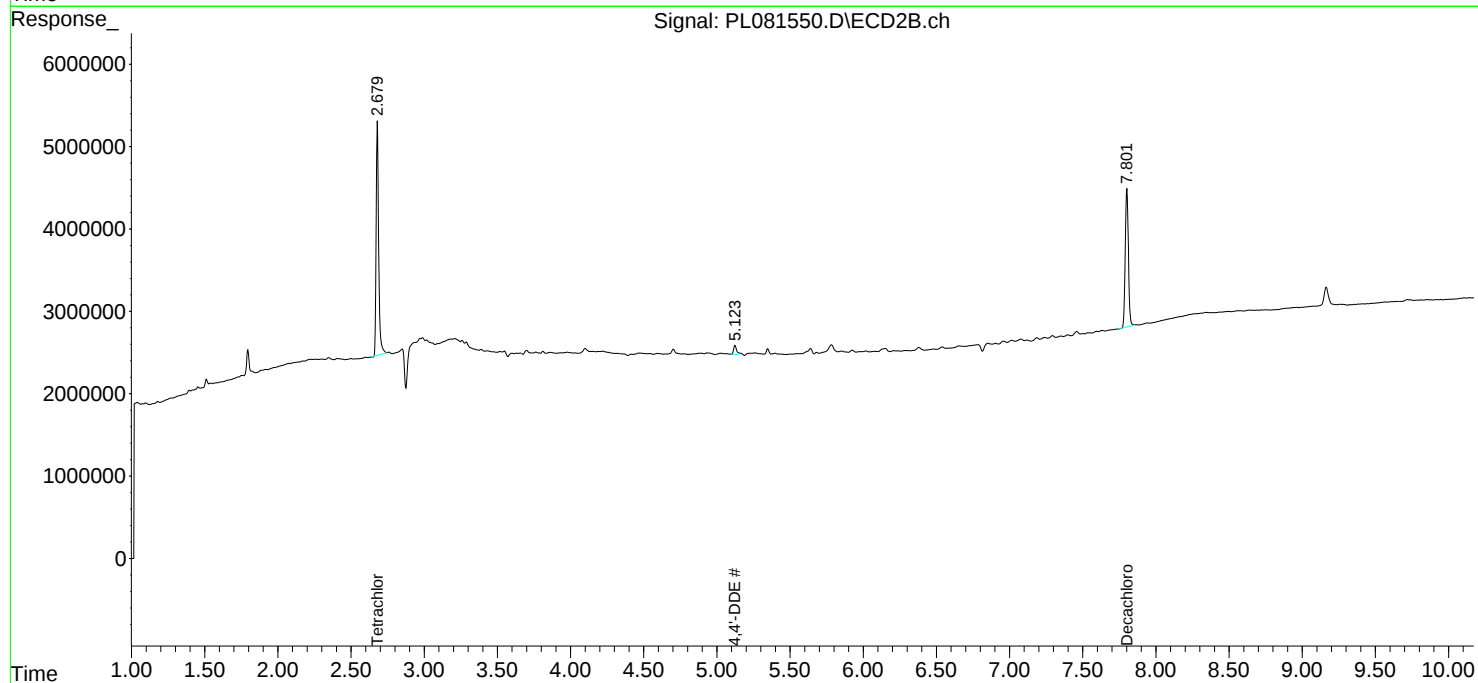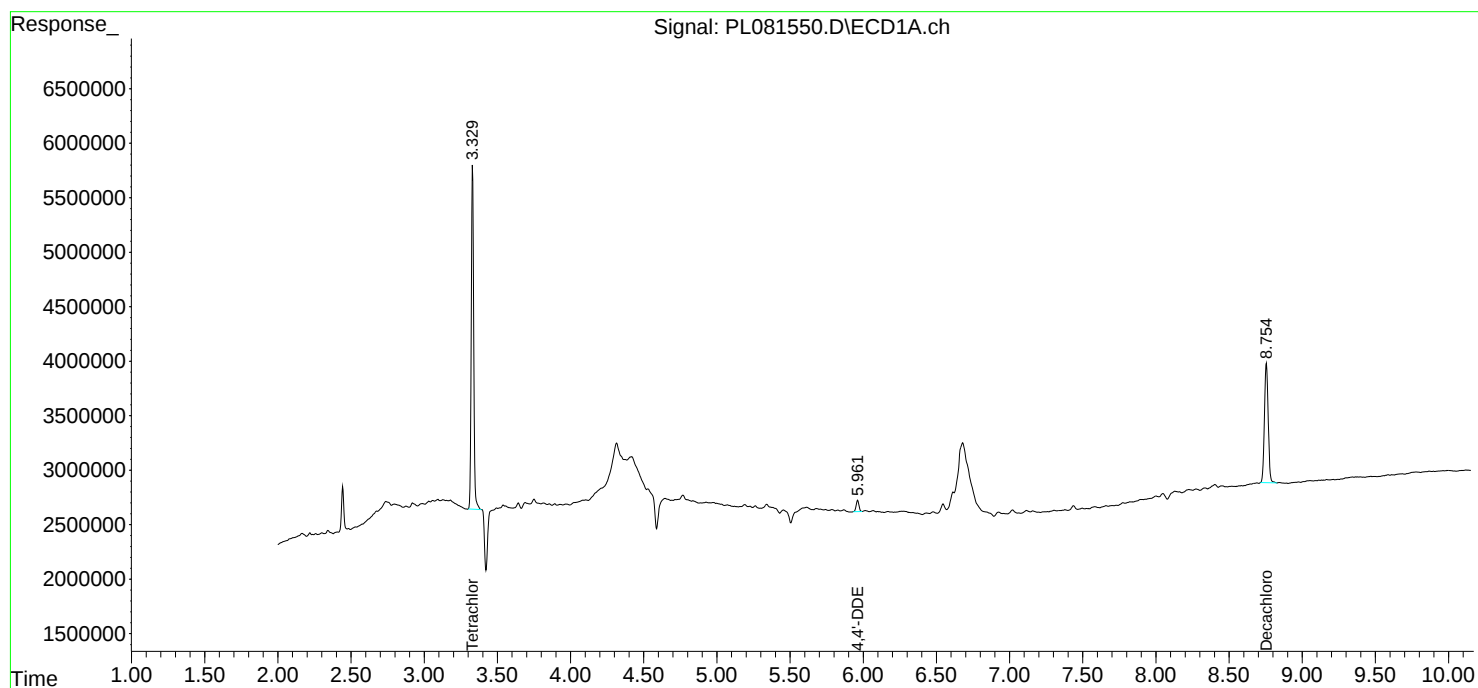


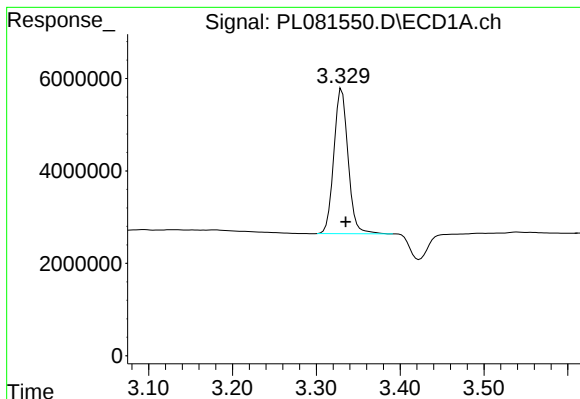

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: -0.005 min
Response: 37018850
Conc: 17.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

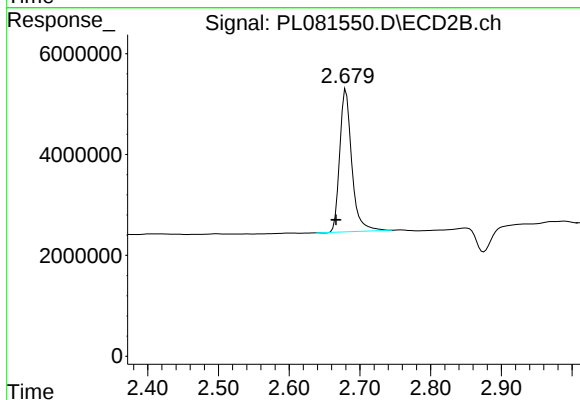


#1 Tetrachloro-m-xylene

R.T.: 2.680 min
Delta R.T.: 0.014 min
Response: 33368584
Conc: 16.49 ng/ml

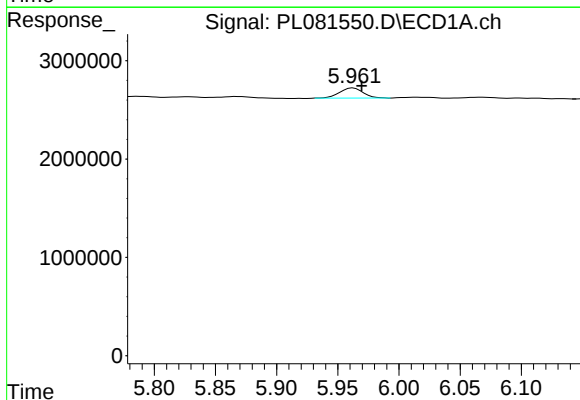


#12 4,4'-DDE

R.T.: 5.963 min
Delta R.T.: -0.007 min
Response: 1386002
Conc: 0.71 ng/ml

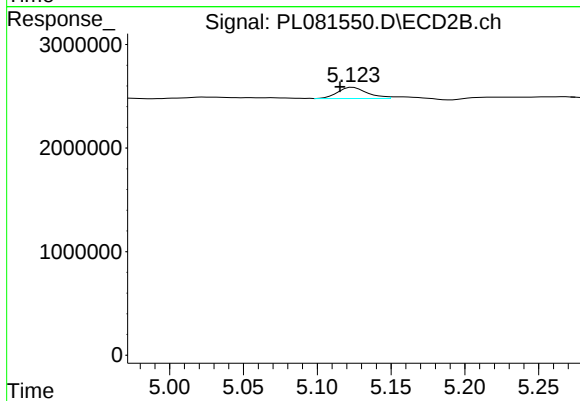

#12 4,4'-DDE


R.T.: 5.123 min
Delta R.T.: 0.007 min
Response: 1517536
Conc: 0.77 ng/ml m

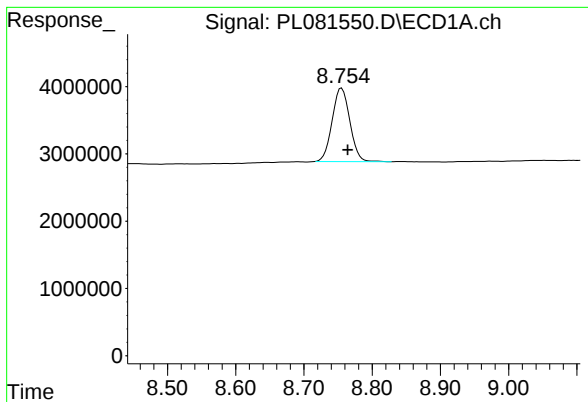

#28 Decachlorobiphenyl

R.T.: 8.755 min
Delta R.T.: -0.009 min
Response: 19706952
Conc: 12.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

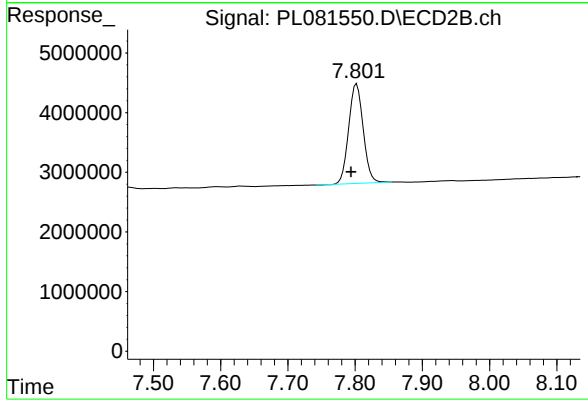

#28 Decachlorobiphenyl

R.T.: 7.802 min
Delta R.T.: 0.008 min
Response: 25113321
Conc: 13.11 ng/ml