

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031819\
 Data File : PL046077.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2019 14:26
 Operator : AJ\SJ
 Sample : K1930-01DL 2X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 00:55:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.980	52184794	15521585	7.586	7.248
28)	SA Decachlor...	8.043	9.036	41545133	11550025	4.965	5.055
Target Compounds							
10)	B gamma-Chl...	5.261	0.000	7076194	0	0.723	N.D. #
12)	B 4,4'-DDE	5.482	6.316	657.3E6	161.0E6	74.881	68.942
13)	MA Dieldrin	5.606	6.465	377.0E6	88474715	39.447	34.430
14)	MA Endrin	5.864	6.710f	55199754	9745583	6.129	4.283 #
16)	A 4,4'-DDD	5.993	6.805	101.1E6	24714385	13.813	12.851
17)	MA 4,4'-DDT	6.228	7.104	374.8E6	95252079	49.973	48.267
19)	B Endosulfa...	0.000	7.239	0	2253672	N.D.	1.002 #
25)	Chlordane-3	5.261	0.000	7076194	0	6.169	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031819\
Data File : PL046077.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2019 14:26
Operator : AJ\SJ
Sample : K1930-01DL 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-3DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 00:55:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

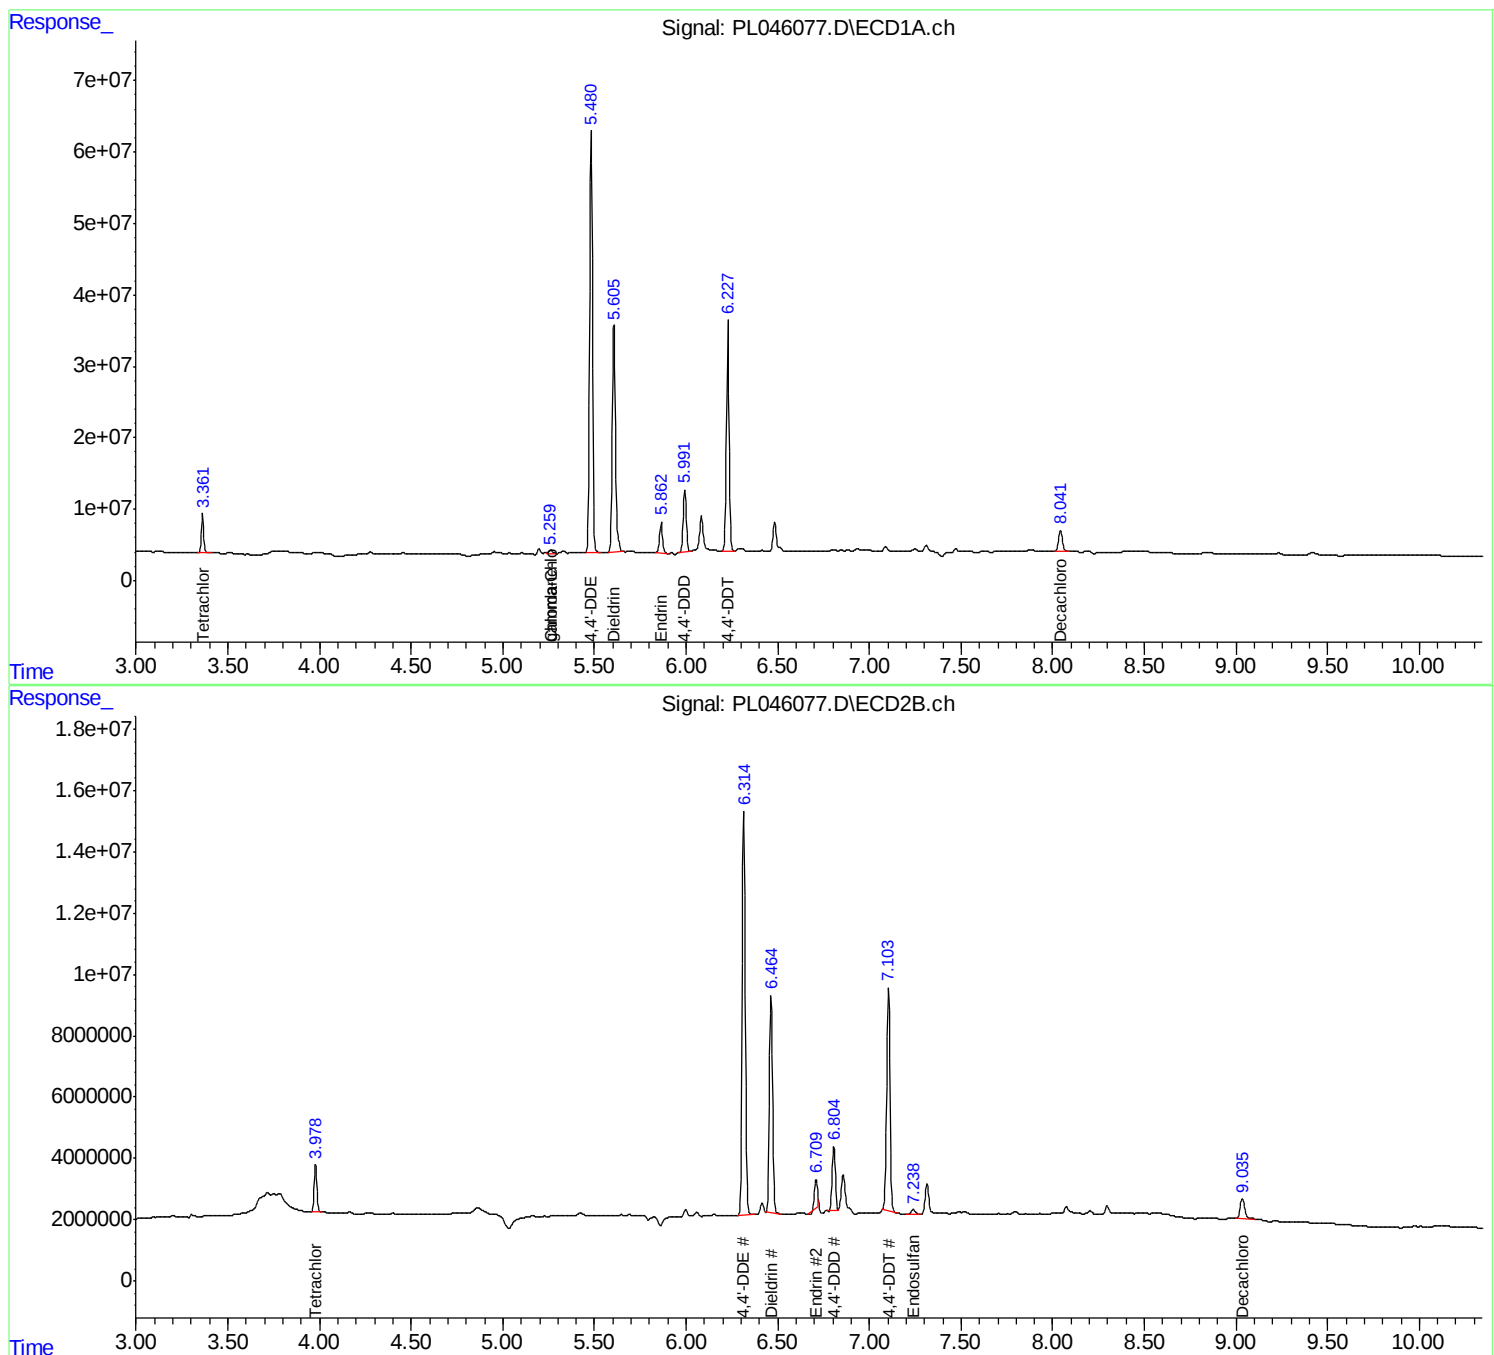


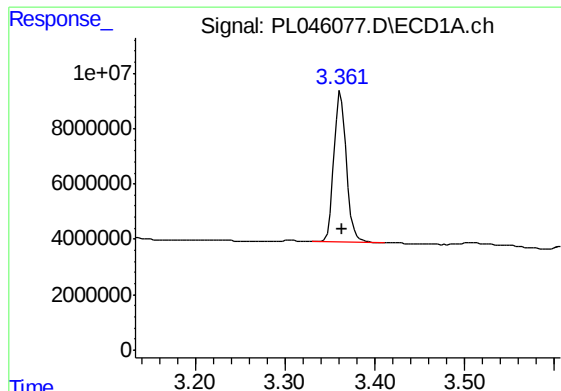

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 52184794
Conc: 7.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3DL

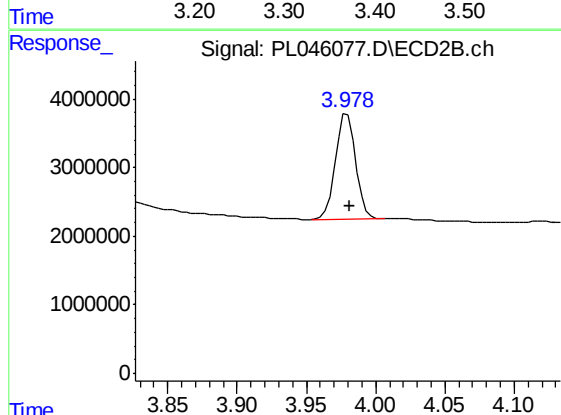


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 15521585
Conc: 7.25 ng/ml

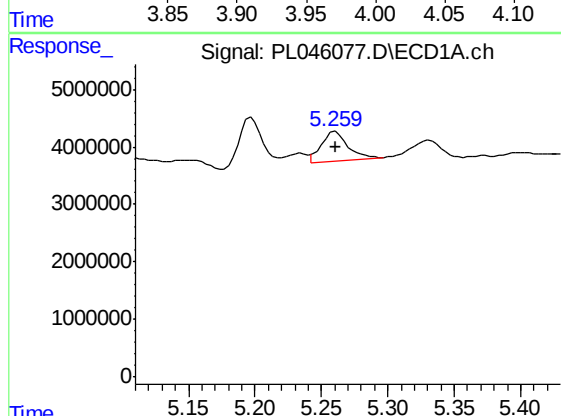


#10 gamma-Chlordane

R.T.: 5.261 min
Delta R.T.: 0.000 min
Response: 7076194
Conc: 0.72 ng/ml

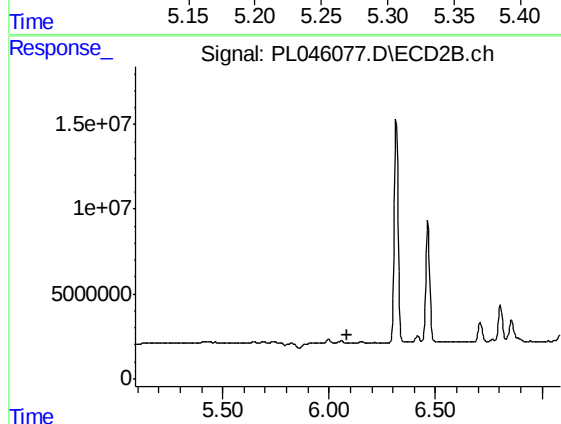

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

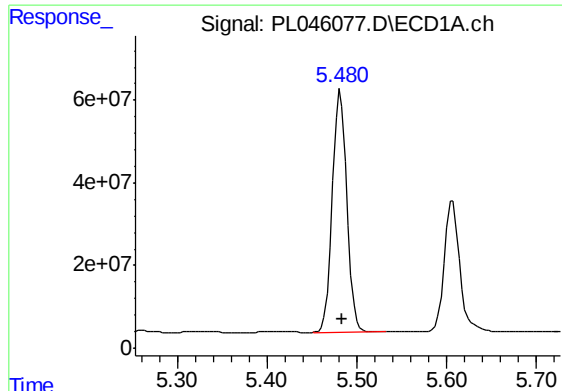

#12 4,4'-DDE


R.T.: 5.482 min
Delta R.T.: -0.002 min
Response: 657324056
Conc: 74.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3DL

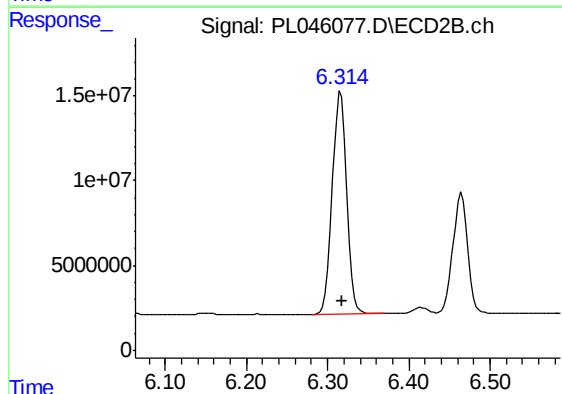


#12 4,4'-DDE

R.T.: 6.316 min
Delta R.T.: -0.002 min
Response: 161040582
Conc: 68.94 ng/ml

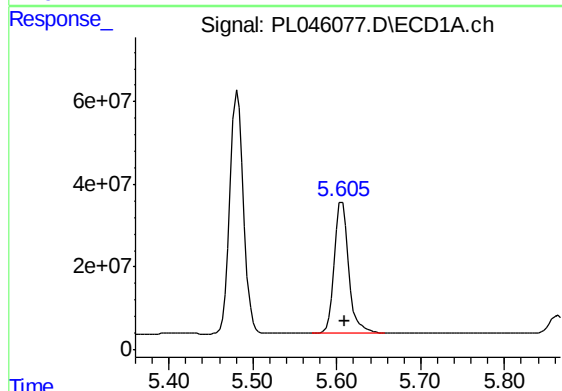


#13 Dieldrin

R.T.: 5.606 min
Delta R.T.: -0.003 min
Response: 377029455
Conc: 39.45 ng/ml

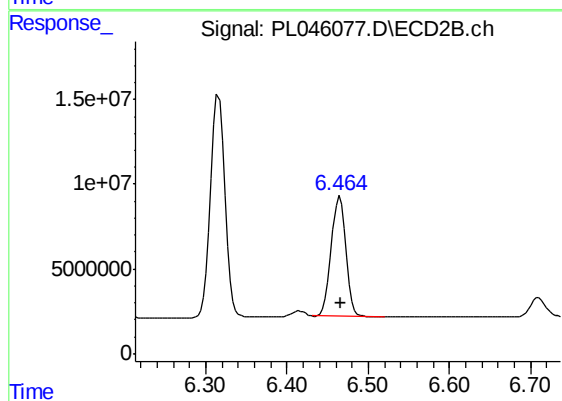

#13 Dieldrin


R.T.: 6.465 min
Delta R.T.: -0.002 min
Response: 88474715
Conc: 34.43 ng/ml

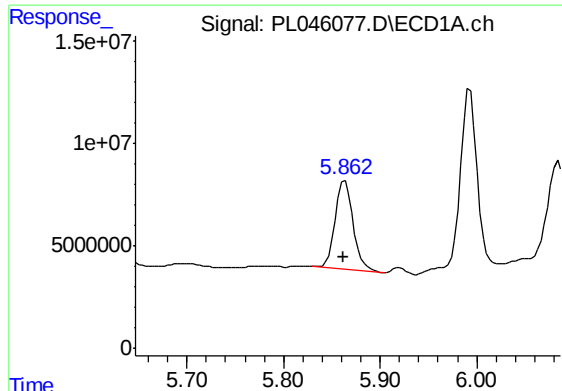

#14 Endrin


R.T.: 5.864 min
Delta R.T.: 0.001 min
Response: 55199754
Conc: 6.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3DL

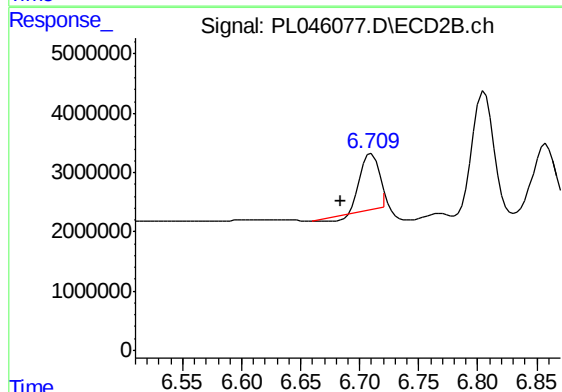


#14 Endrin

R.T.: 6.710 min
Delta R.T.: 0.026 min
Response: 9745583
Conc: 4.28 ng/ml

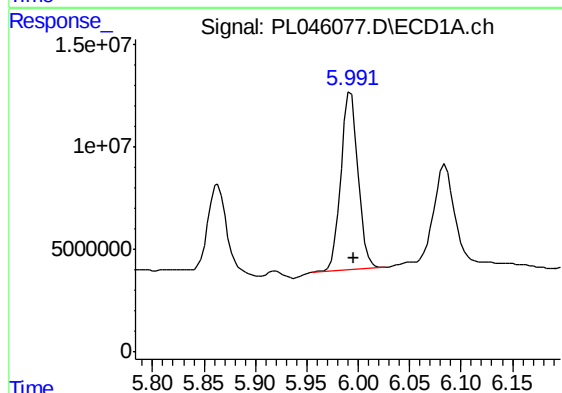


#16 4,4'-DDD

R.T.: 5.993 min
Delta R.T.: -0.003 min
Response: 101139275
Conc: 13.81 ng/ml

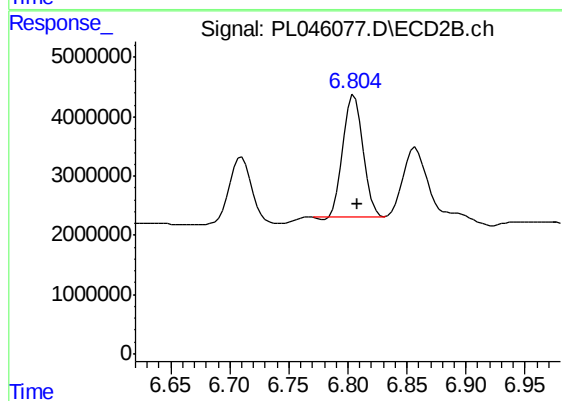

#16 4,4'-DDD


R.T.: 6.805 min
Delta R.T.: -0.002 min
Response: 24714385
Conc: 12.85 ng/ml

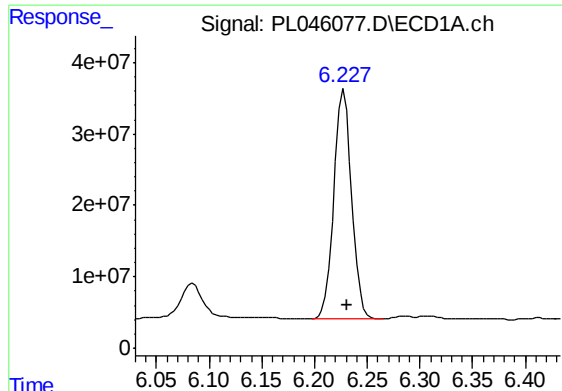

#17 4,4'-DDT


R.T.: 6.228 min
Delta R.T.: -0.003 min
Response: 374804000
Conc: 49.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3DL

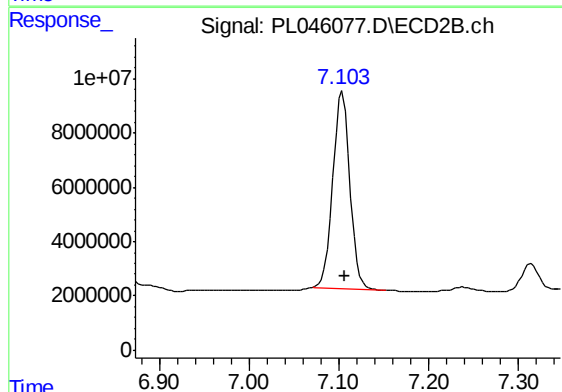


#17 4,4'-DDT

R.T.: 7.104 min
Delta R.T.: -0.002 min
Response: 95252079
Conc: 48.27 ng/ml

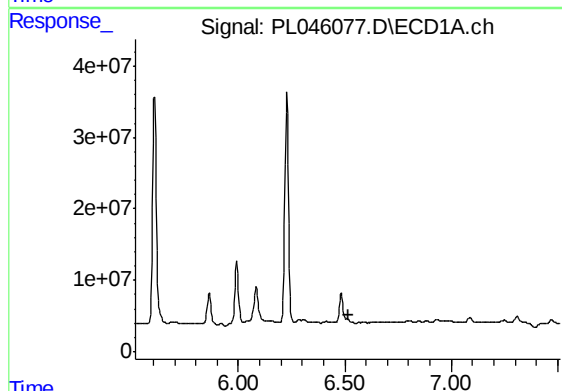


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.515 min
Response: 0
Conc: N.D.

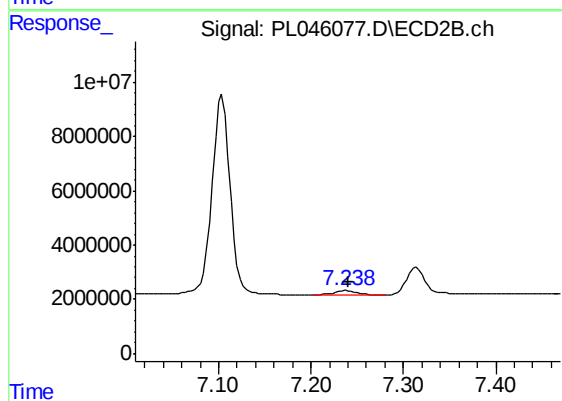

#19 Endosulfan Sulfate


R.T.: 7.239 min
Delta R.T.: -0.001 min
Response: 2253672
Conc: 1.00 ng/ml

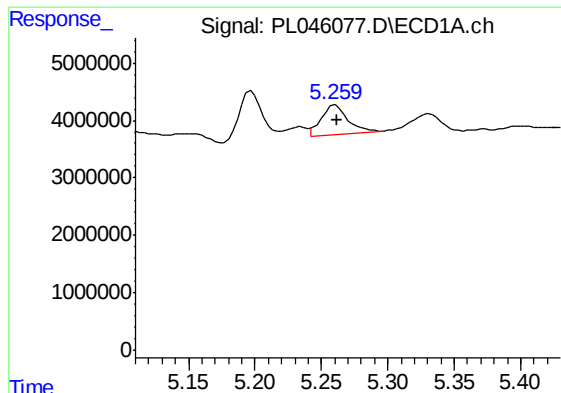

#25 Chlordane-3


R.T.: 5.261 min
Delta R.T.: -0.001 min
Response: 7076194
Conc: 6.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3DL

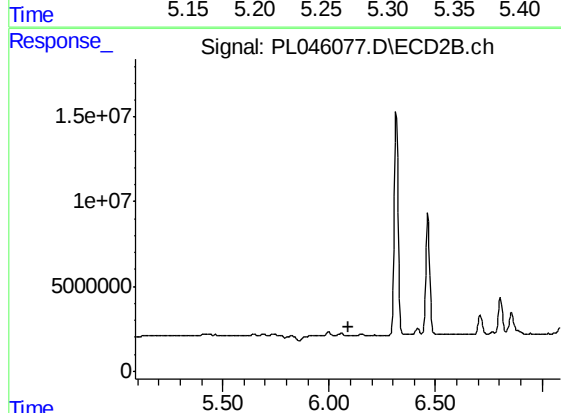


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

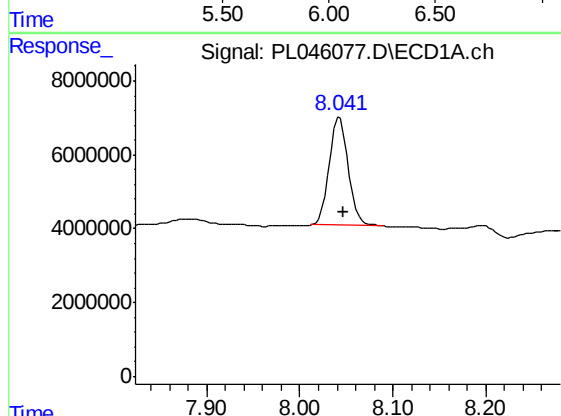

#28 Decachlorobiphenyl

R.T.: 8.043 min
Delta R.T.: -0.005 min
Response: 41545133
Conc: 4.97 ng/ml

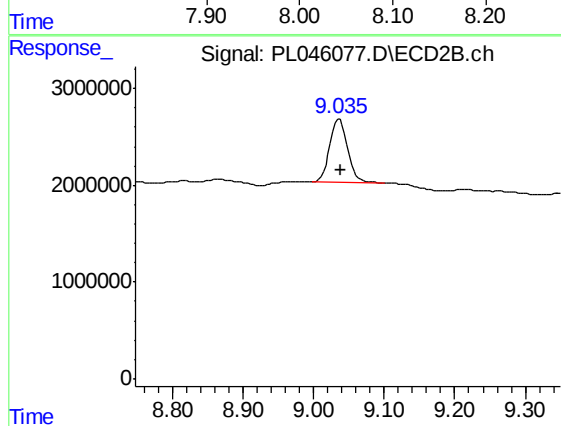

#28 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: -0.003 min
Response: 11550025
Conc: 5.05 ng/ml