

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031819\
 Data File : PL046087.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2019 16:47
 Operator : AJ\SJ
 Sample : K1691-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-01-031519-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 00:58:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.979	65858068	20604512	9.573	9.621
28)	SA Decachlor...	8.041	9.034	76756534	23639842	9.173	10.346
Target Compounds							
10)	B gamma-Chl...	5.276	0.000	9310267	0	0.951	N.D. #
11)	B alpha-Chl...	0.000	6.159	0	3125525	N.D.	1.159 #
12)	B 4,4'-DDE	5.479	6.315	42257481	12816865	4.814	5.487
16)	A 4,4'-DDD	0.000	6.807	0	881516	N.D.	0.458 #
17)	MA 4,4'-DDT	6.225	7.103	16063678	4816855	2.142	2.441
24)	Chlordane-2	0.000	5.436	0	1779045	N.D.	14.724 #
25)	Chlordane-3	5.276	0.000	9310267	0	8.117	N.D. #
26)	Chlordane-4	0.000	6.159	0	3125525	N.D.	6.681 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031819\
Data File : PL046087.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2019 16:47
Operator : AJ\SJ
Sample : K1691-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CL-01-031519-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 00:58:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

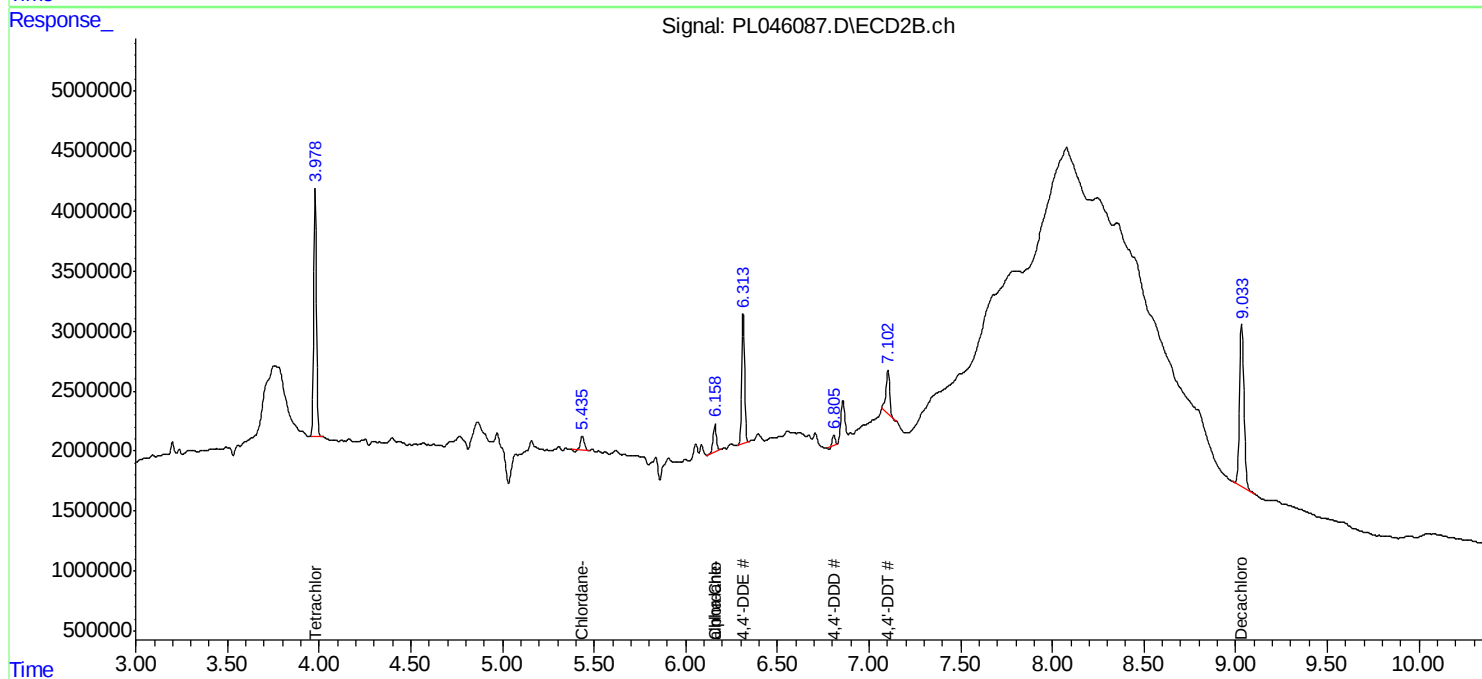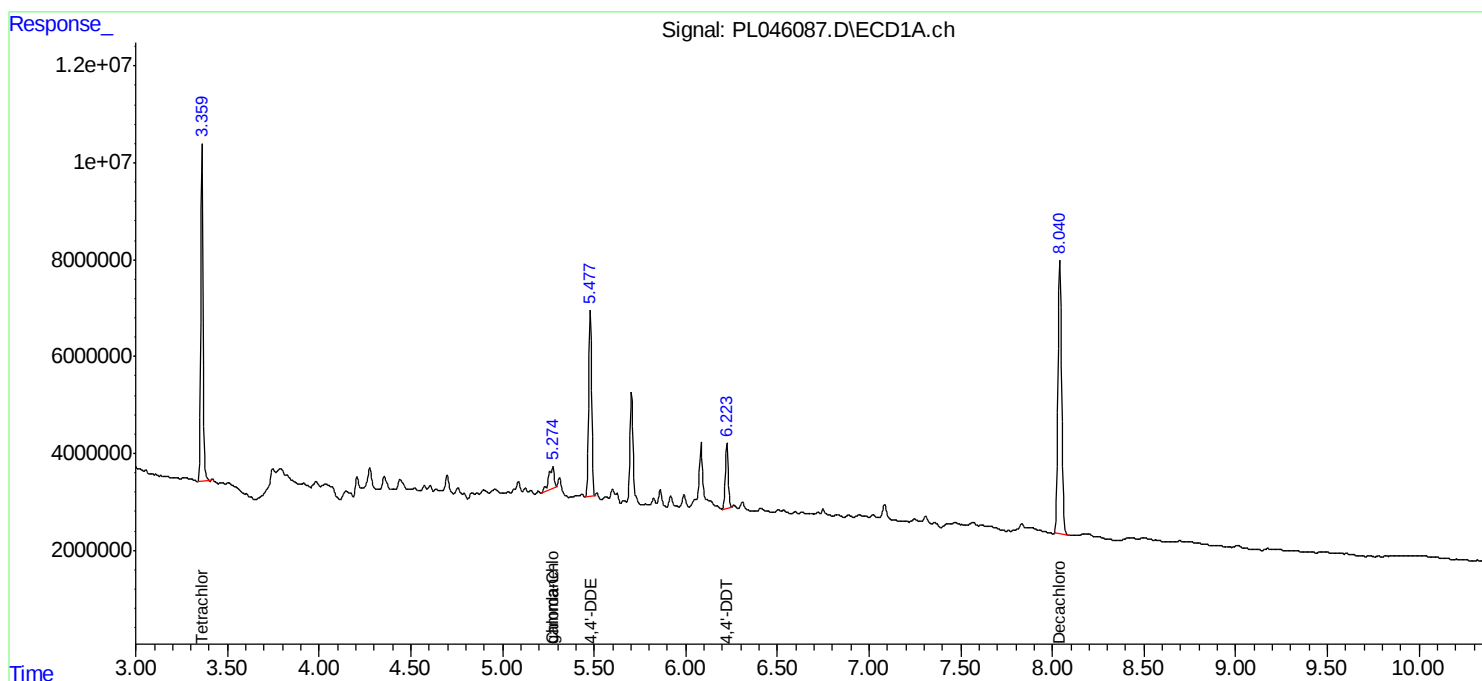


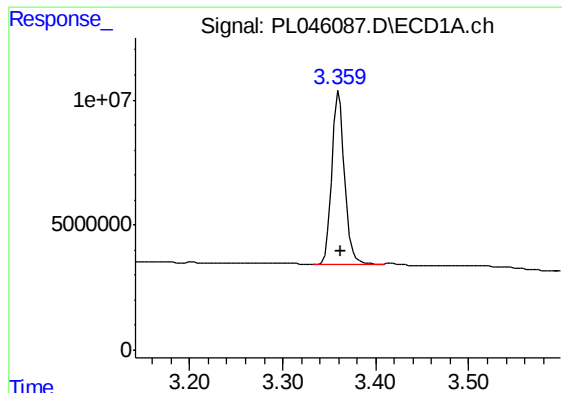

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: -0.002 min
Response: 65858068
Conc: 9.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-01-031519-B

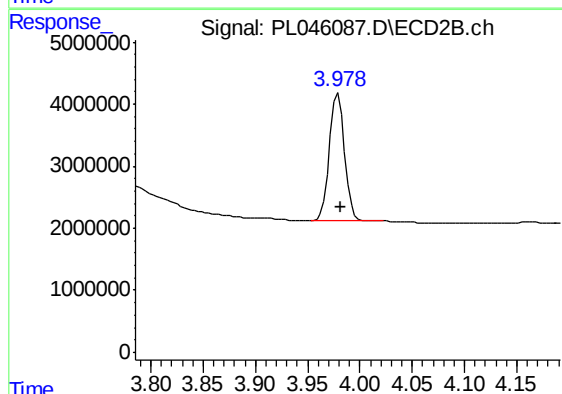


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.003 min
Response: 20604512
Conc: 9.62 ng/ml

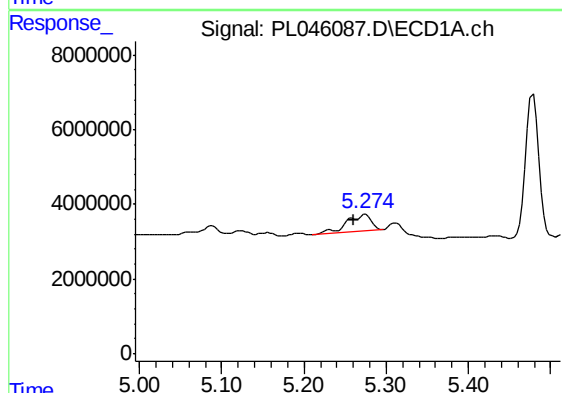


#10 gamma-Chlordane

R.T.: 5.276 min
Delta R.T.: 0.015 min
Response: 9310267
Conc: 0.95 ng/ml

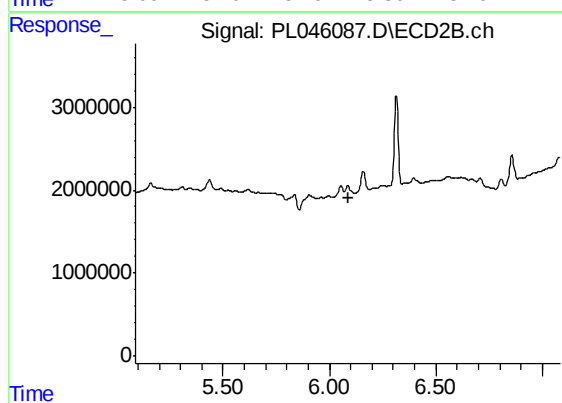

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

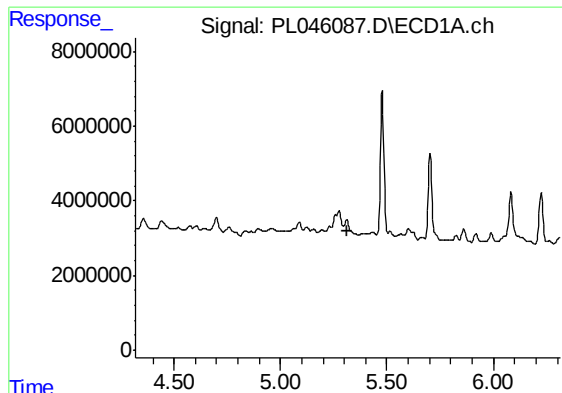

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CL-01-031519-B

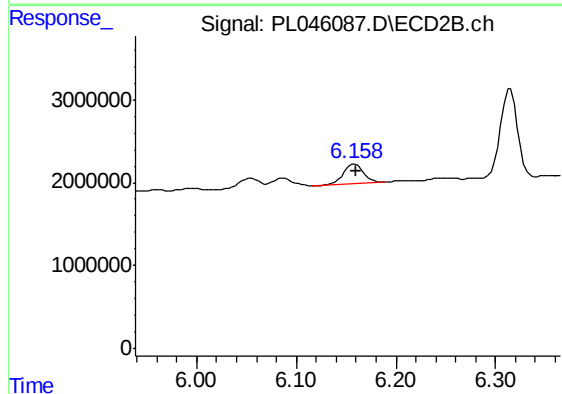


#11 alpha-Chlordane

R.T.: 6.159 min
Delta R.T.: -0.001 min
Response: 3125525
Conc: 1.16 ng/ml

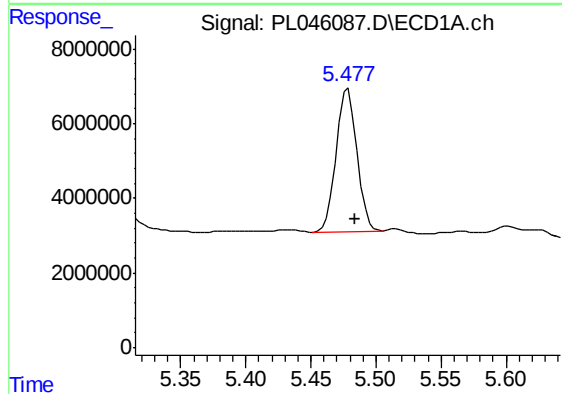


#12 4,4'-DDE

R.T.: 5.479 min
Delta R.T.: -0.005 min
Response: 42257481
Conc: 4.81 ng/ml

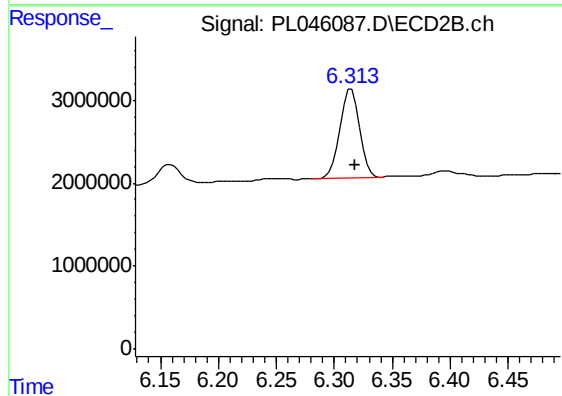

#12 4,4'-DDE


R.T.: 6.315 min
Delta R.T.: -0.003 min
Response: 12816865
Conc: 5.49 ng/ml

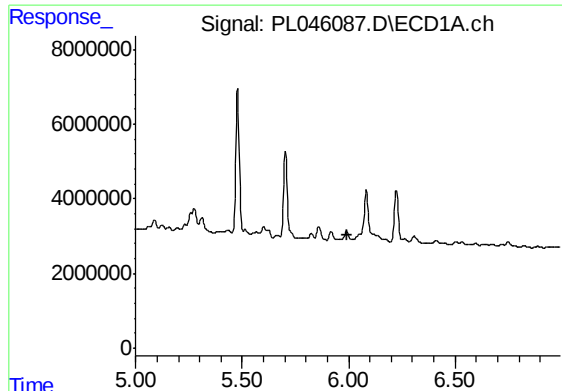

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CL-01-031519-B

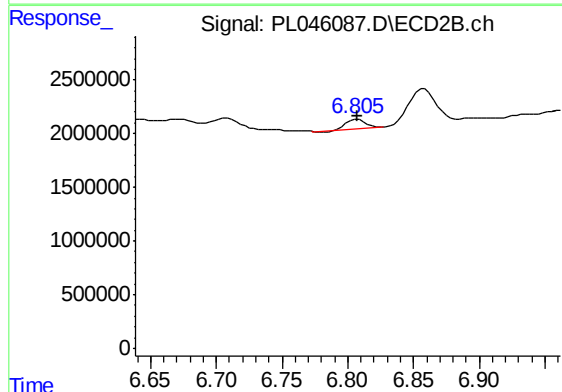


#16 4,4'-DDD

R.T.: 6.807 min
Delta R.T.: 0.000 min
Response: 881516
Conc: 0.46 ng/ml

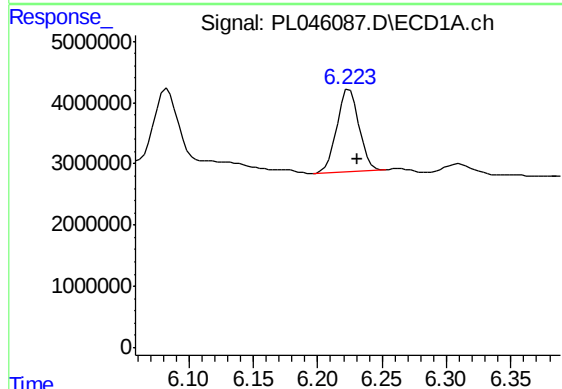


#17 4,4'-DDT

R.T.: 6.225 min
Delta R.T.: -0.006 min
Response: 16063678
Conc: 2.14 ng/ml

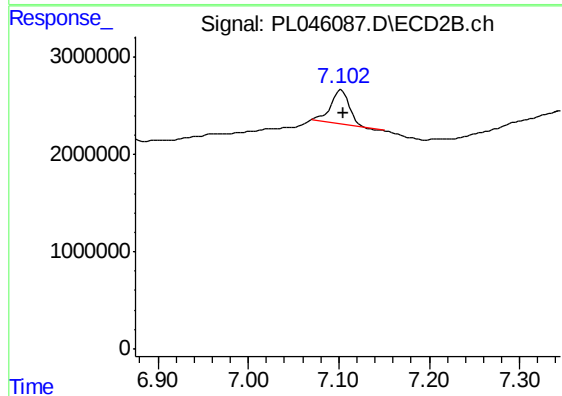

#17 4,4'-DDT


R.T.: 7.103 min
Delta R.T.: -0.003 min
Response: 4816855
Conc: 2.44 ng/ml

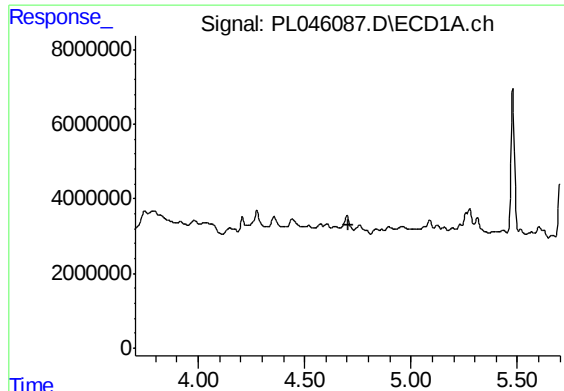

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CL-01-031519-B

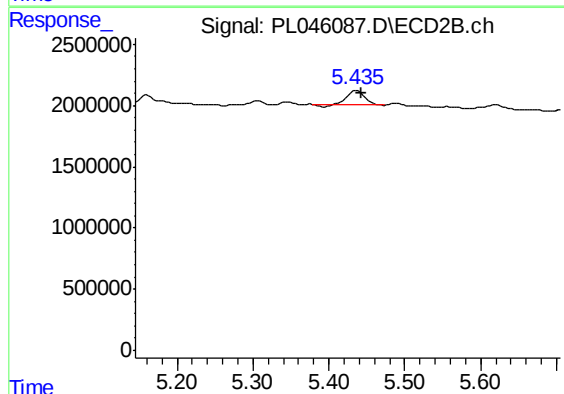


#24 Chlordane-2

R.T.: 5.436 min
Delta R.T.: -0.007 min
Response: 1779045
Conc: 14.72 ng/ml

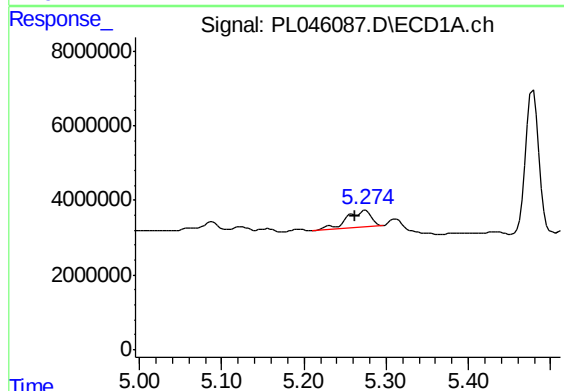


#25 Chlordane-3

R.T.: 5.276 min
Delta R.T.: 0.014 min
Response: 9310267
Conc: 8.12 ng/ml

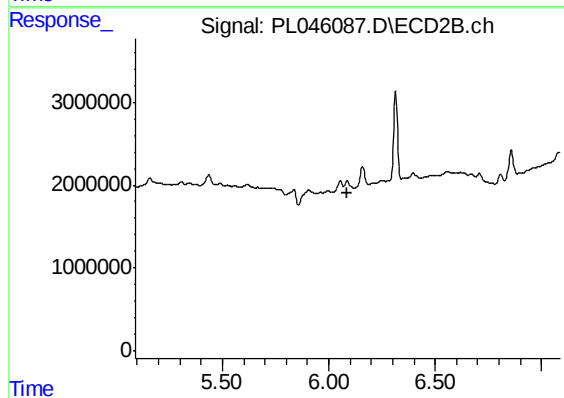

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

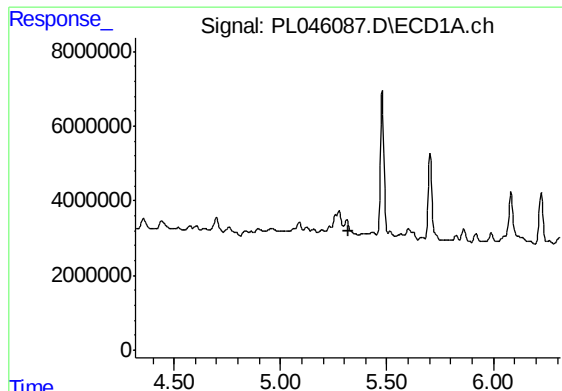

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CL-01-031519-B

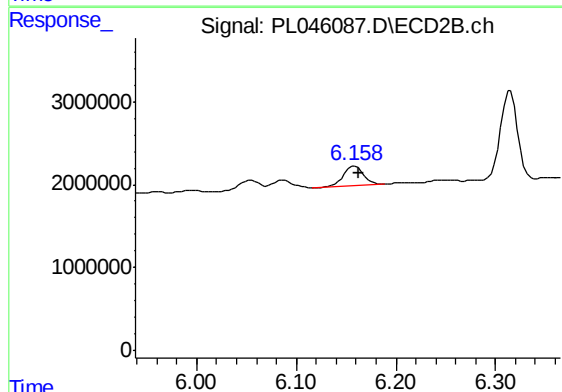


#26 Chlordane-4

R.T.: 6.159 min
Delta R.T.: -0.003 min
Response: 3125525
Conc: 6.68 ng/ml

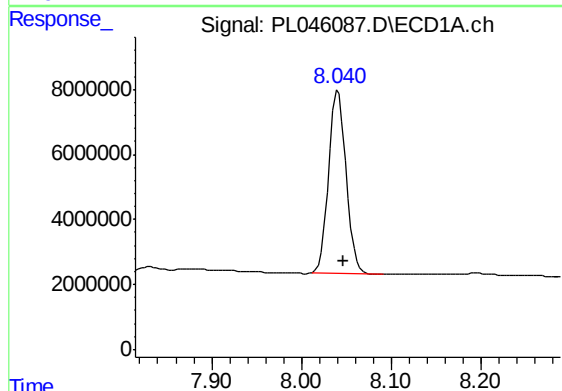

#28 Decachlorobiphenyl

R.T.: 8.041 min
Delta R.T.: -0.006 min
Response: 76756534
Conc: 9.17 ng/ml

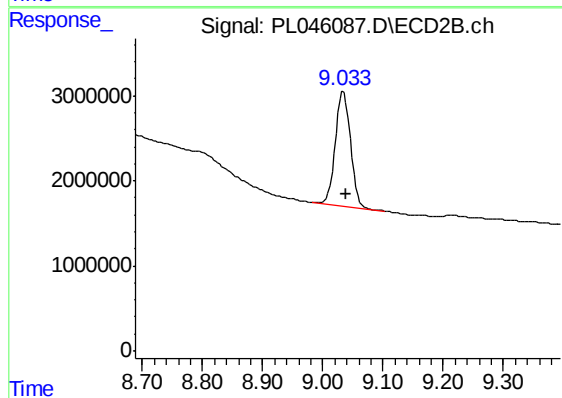

#28 Decachlorobiphenyl

R.T.: 9.034 min
Delta R.T.: -0.005 min
Response: 23639842
Conc: 10.35 ng/ml