

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031819\
 Data File : PL046093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2019 18:12
 Operator : AJ\SJ
 Sample : K1951-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-GF-03-006-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 00:59:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.360	3.979	51974031	16145422	7.555	7.539
28)	SA Decachlor...	8.040	9.035	75240273	23077730	8.992	10.100
Target Compounds							
4)	MA Heptachlor	4.354	5.160	5537755	1985310	0.525	0.667 #
10)	B gamma-Chl...	5.275	0.000	6214263	0	0.635	N.D. #
11)	B alpha-Chl...	0.000	6.159	0	3003209	N.D.	1.113 #
12)	B 4,4'-DDE	5.479	6.314	4721311	1619492	0.538	0.693 #
23)	Chlordane-1	4.207	4.970	11647276	1928721	34.568	17.104 #
24)	Chlordane-2	4.699	5.437	6251242	2357696	16.161	19.512
25)	Chlordane-3	5.275	0.000	6214263	0	5.418	N.D. #
26)	Chlordane-4	0.000	6.159	0	3003209	N.D.	6.420 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031819\
Data File : PL046093.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2019 18:12
Operator : AJ\SJ
Sample : K1951-03
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-GF-03-006-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 00:59:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

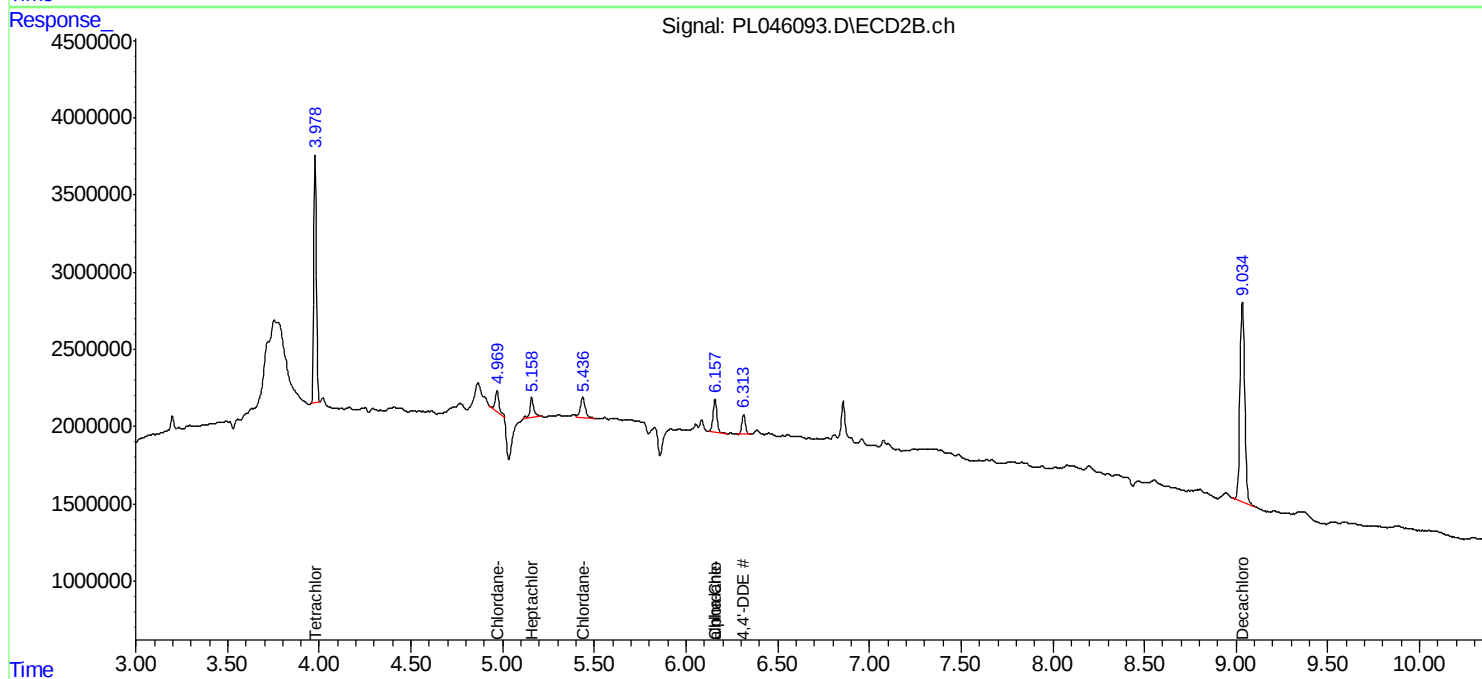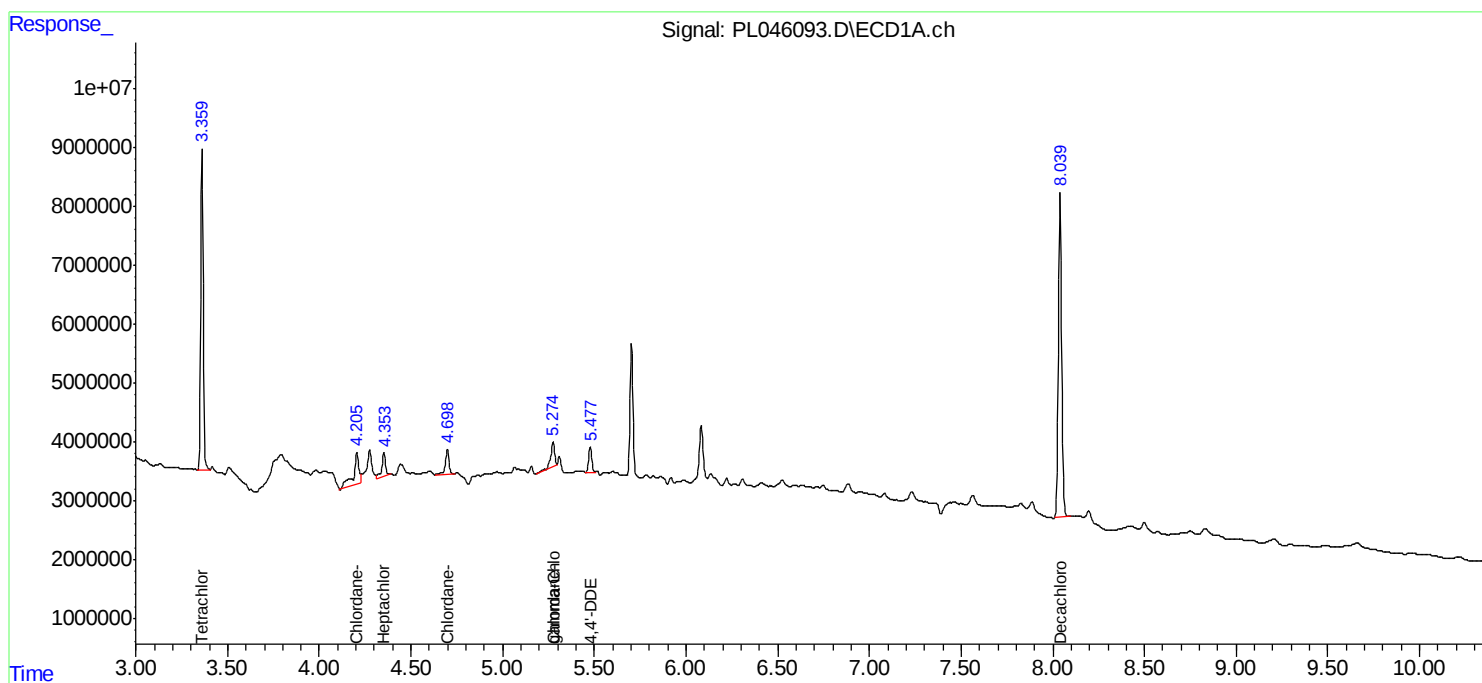


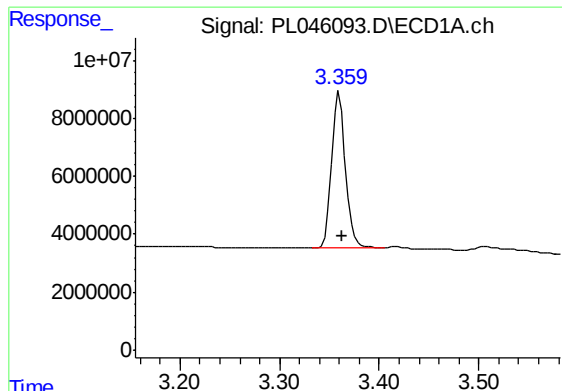

#1 Tetrachloro-m-xylene


R.T.: 3.360 min
Delta R.T.: -0.003 min
Response: 51974031
Conc: 7.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-GF-03-006-B

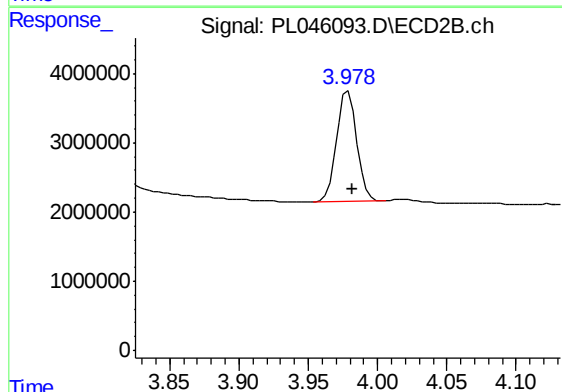


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.003 min
Response: 16145422
Conc: 7.54 ng/ml

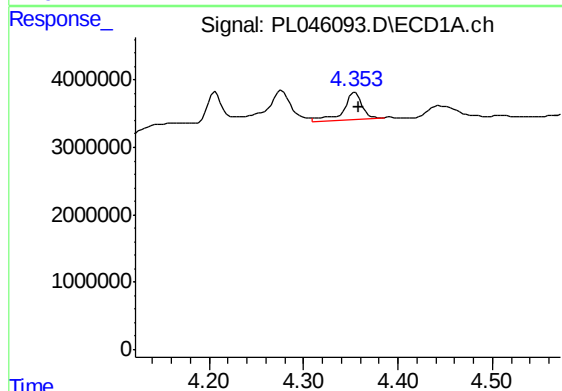


#4 Heptachlor

R.T.: 4.354 min
Delta R.T.: -0.004 min
Response: 5537755
Conc: 0.52 ng/ml

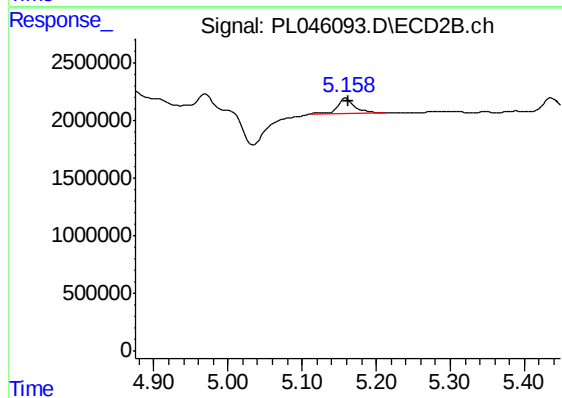

#4 Heptachlor


R.T.: 5.160 min
Delta R.T.: -0.003 min
Response: 1985310
Conc: 0.67 ng/ml

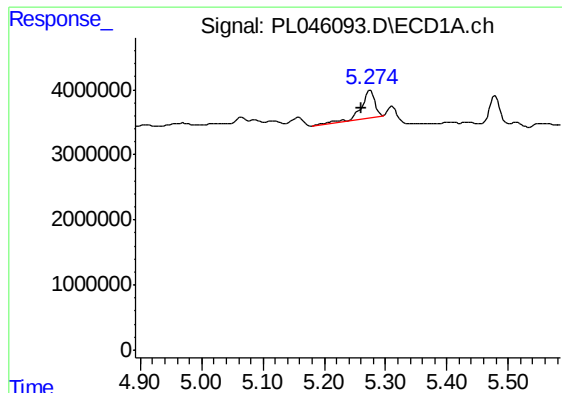

#10 gamma-Chlordane


R.T.: 5.275 min
Delta R.T.: 0.015 min
Response: 6214263
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-GF-03-006-B

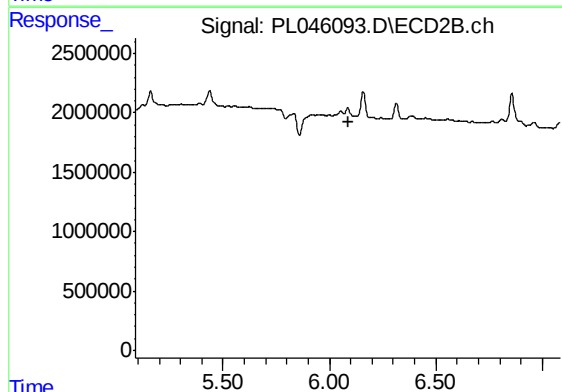


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

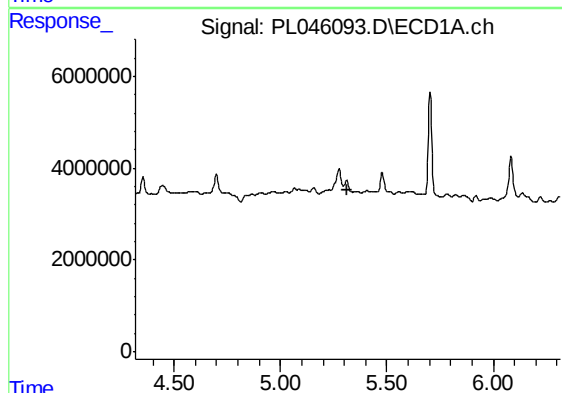


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.317 min
Response: 0
Conc: N.D.

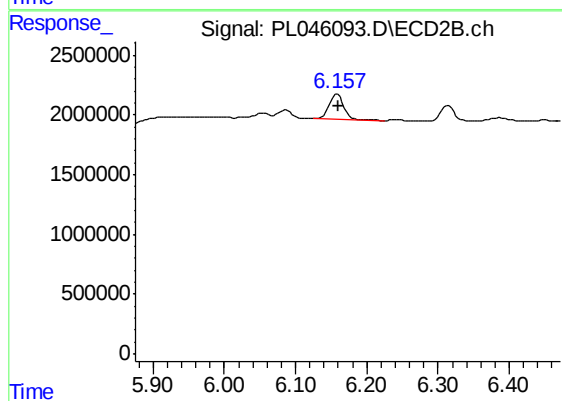

#11 alpha-Chlordane


R.T.: 6.159 min
Delta R.T.: -0.001 min
Response: 3003209
Conc: 1.11 ng/ml

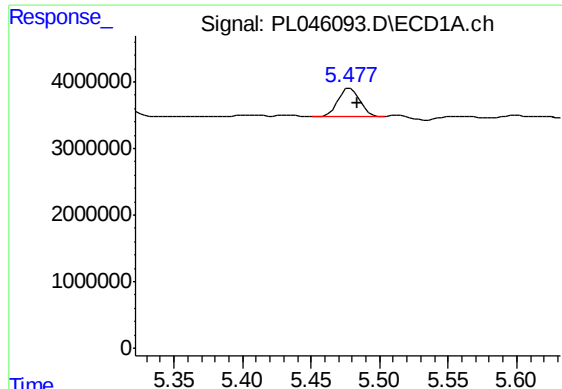

#12 4,4'-DDE


R.T.: 5.479 min
Delta R.T.: -0.005 min
Response: 4721311
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-GF-03-006-B

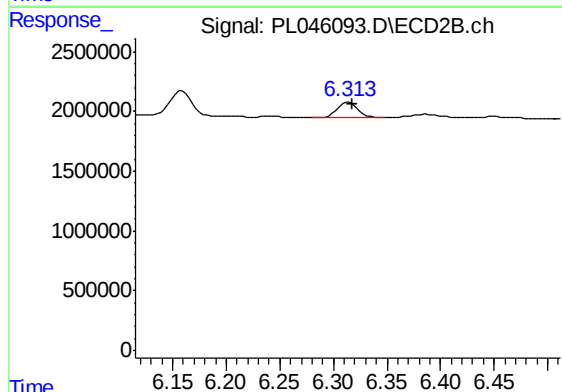


#12 4,4'-DDE

R.T.: 6.314 min
Delta R.T.: -0.004 min
Response: 1619492
Conc: 0.69 ng/ml

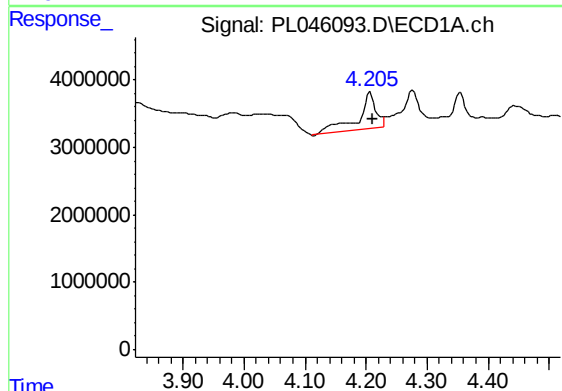


#23 Chlordane-1

R.T.: 4.207 min
Delta R.T.: -0.005 min
Response: 11647276
Conc: 34.57 ng/ml

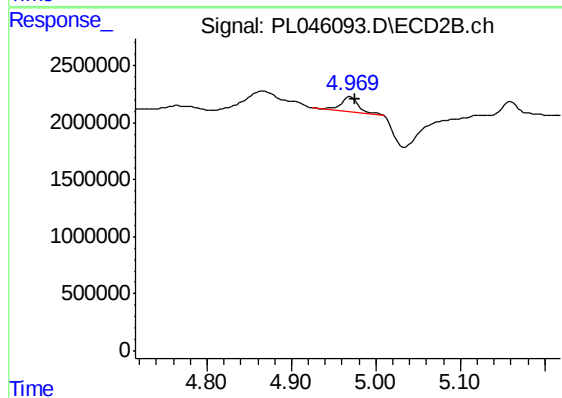

#23 Chlordane-1


R.T.: 4.970 min
Delta R.T.: -0.005 min
Response: 1928721
Conc: 17.10 ng/ml

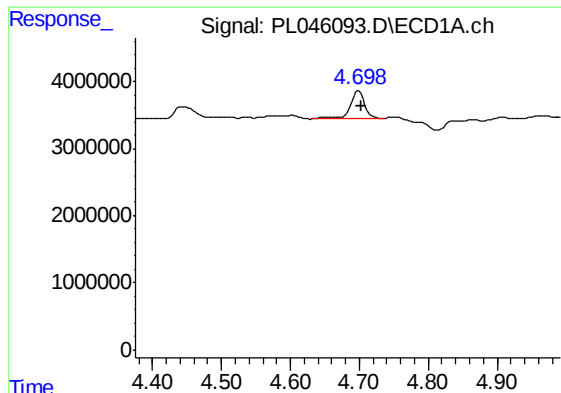

#24 Chlordane-2


R.T.: 4.699 min
Delta R.T.: -0.005 min
Response: 6251242
Conc: 16.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-GF-03-006-B

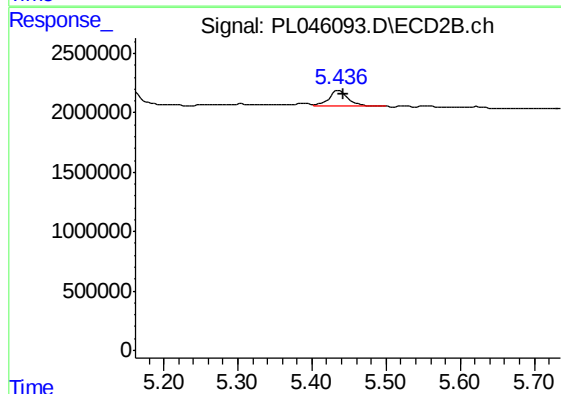


#24 Chlordane-2

R.T.: 5.437 min
Delta R.T.: -0.006 min
Response: 2357696
Conc: 19.51 ng/ml

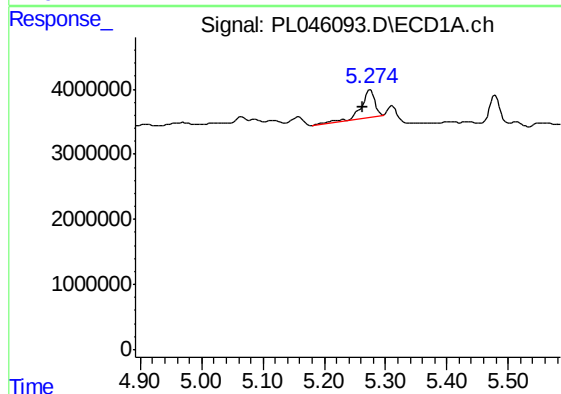


#25 Chlordane-3

R.T.: 5.275 min
Delta R.T.: 0.014 min
Response: 6214263
Conc: 5.42 ng/ml

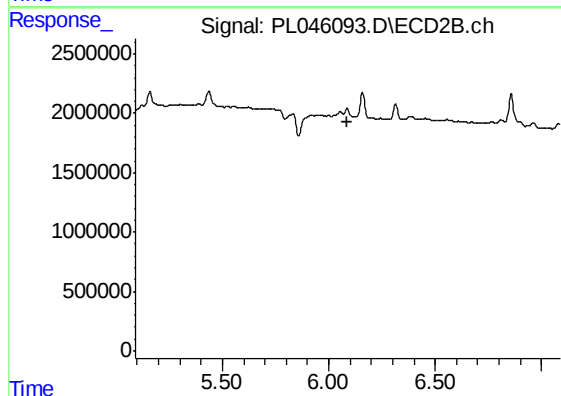

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

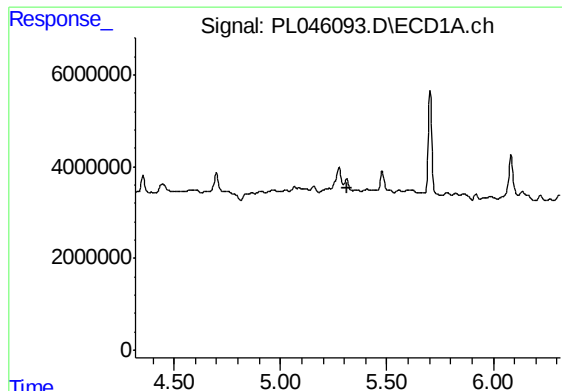

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-GF-03-006-B

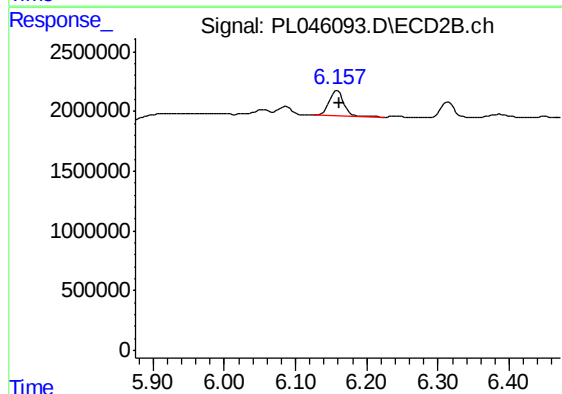


#26 Chlordane-4

R.T.: 6.159 min
Delta R.T.: -0.003 min
Response: 3003209
Conc: 6.42 ng/ml

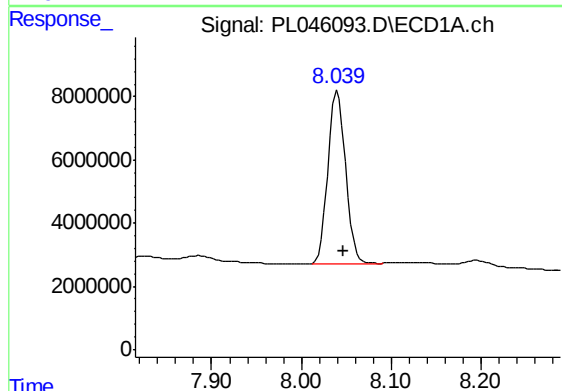

#28 Decachlorobiphenyl

R.T.: 8.040 min
Delta R.T.: -0.007 min
Response: 75240273
Conc: 8.99 ng/ml

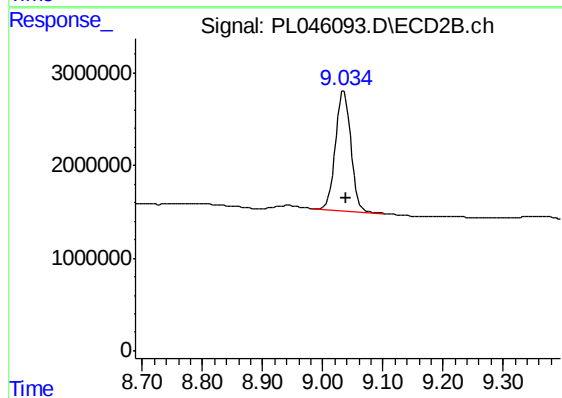

#28 Decachlorobiphenyl

R.T.: 9.035 min
Delta R.T.: -0.004 min
Response: 23077730
Conc: 10.10 ng/ml