

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031819\
 Data File : PL046114.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2019 23:09
 Operator : AJ\SJ
 Sample : K1935-08
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-2(10-11)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:04:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.360	3.979	34021693	11843413	4.946	5.530
28)	SA Decachlor...	8.040	9.034	32340251	9302743	3.865	4.071
Target Compounds							
4)	MA Heptachlor	4.372	5.168	4670706	3779958	0.443	1.271 #
5)	MB Aldrin	4.584f	5.478	156.3E6	5032897	16.065	1.863 #
6)	B beta-BHC	4.341f	0.000	11685657	0	2.726	N.D. #
9)	A Endosulfan I	5.361	6.233f	23986405	3270906	2.684	1.313 #
11)	B alpha-Chl...	5.314	0.000	102.1E6	0	10.532	N.D. #
23)	Chlordane-1	4.230f	4.959f	13226429	4803866	39.255	42.602
24)	Chlordane-2	0.000	5.426f	0	4675503	N.D.	38.695 #
26)	Chlordane-4	5.314	0.000	102.1E6	0	96.345	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031819\
Data File : PL046114.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2019 23:09
Operator : AJ\SJ
Sample : K1935-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
SB-2(10-11)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:04:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

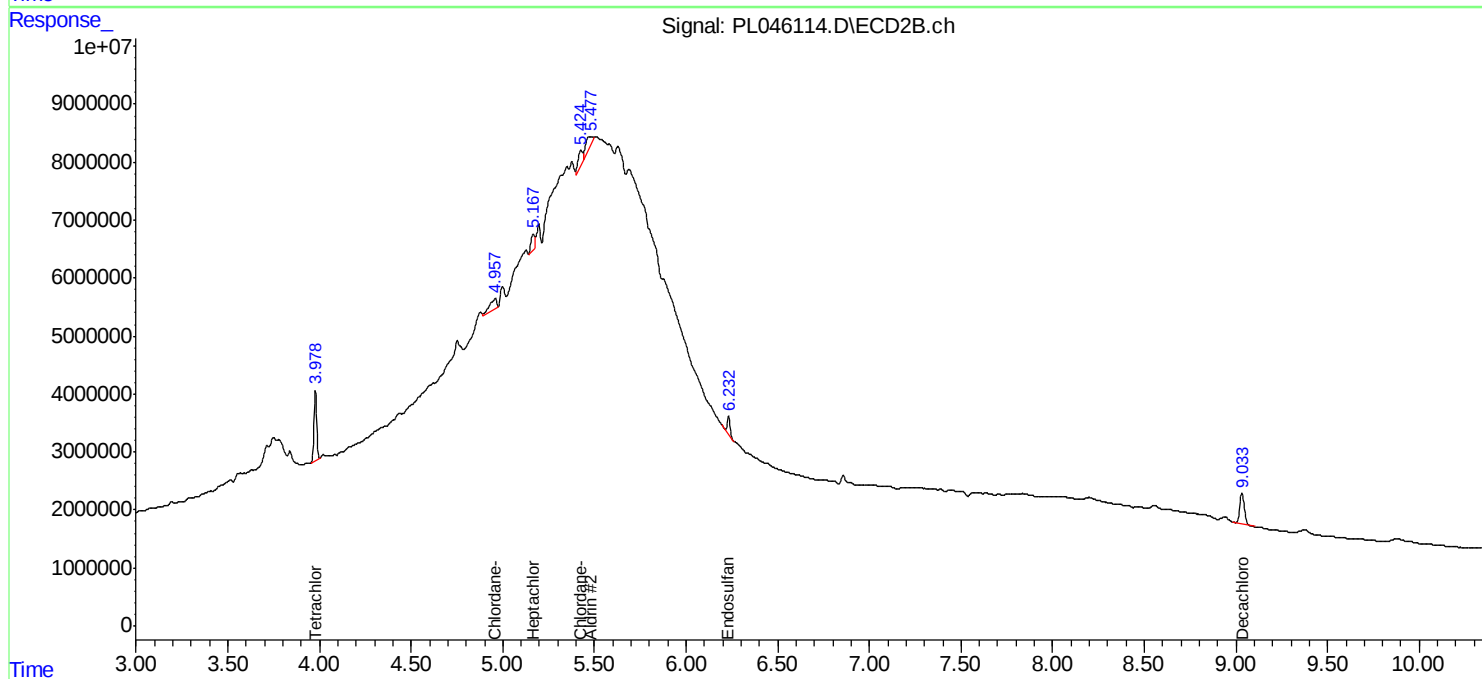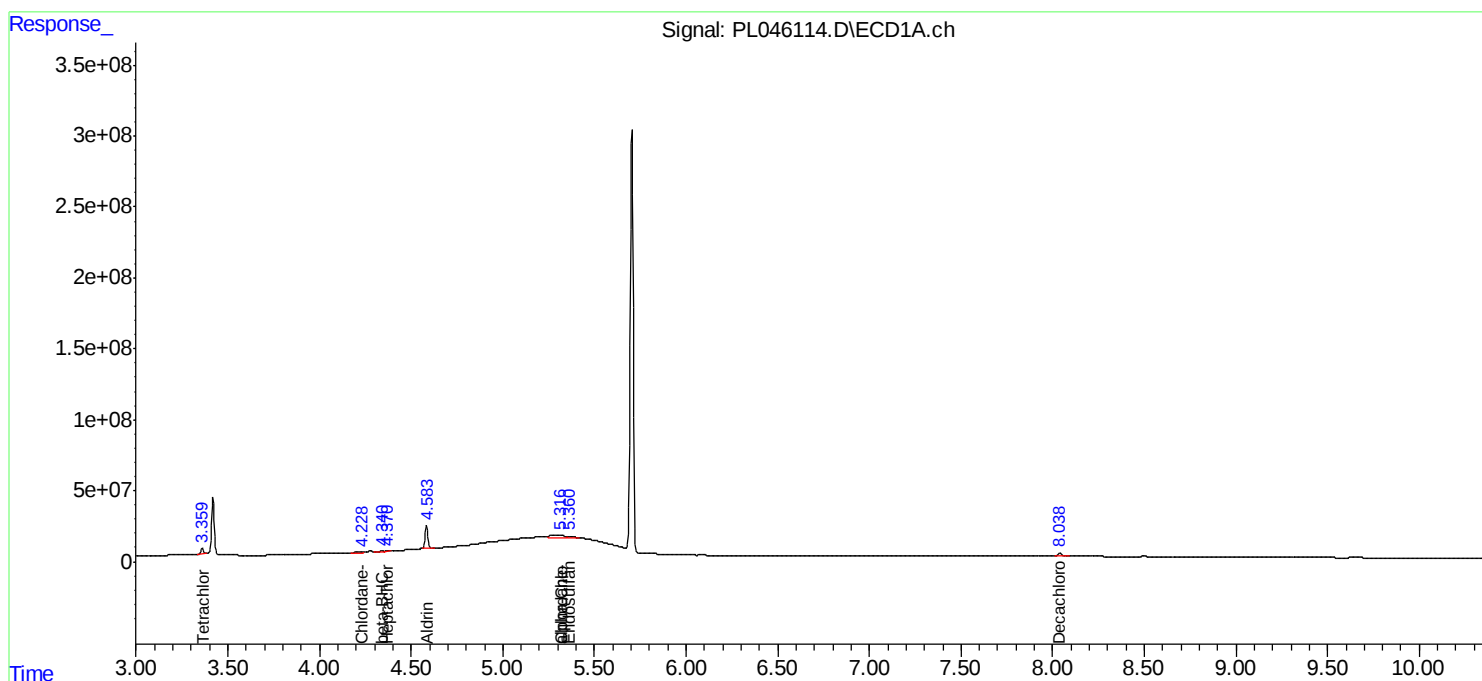


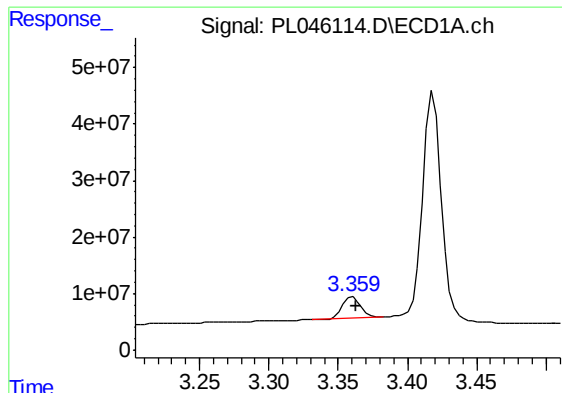

#1 Tetrachloro-m-xylene


R.T.: 3.360 min
Delta R.T.: -0.003 min
Response: 34021693
Conc: 4.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-2(10-11)

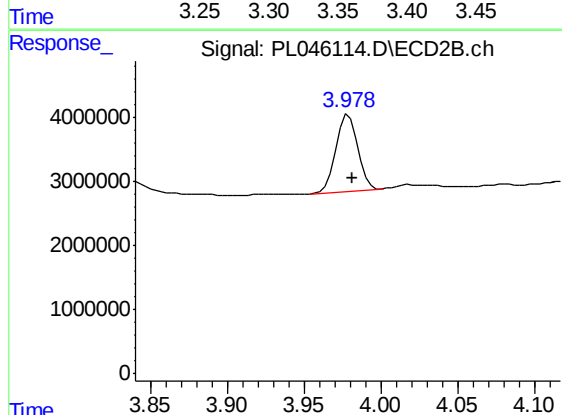


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.002 min
Response: 11843413
Conc: 5.53 ng/ml

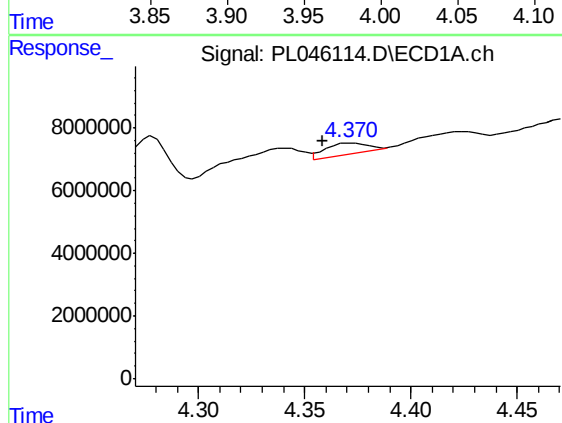


#4 Heptachlor

R.T.: 4.372 min
Delta R.T.: 0.014 min
Response: 4670706
Conc: 0.44 ng/ml

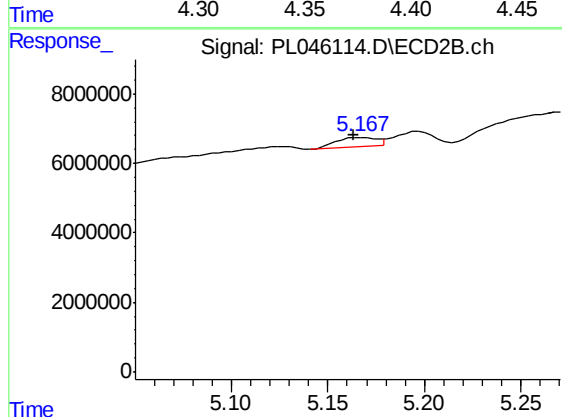

#4 Heptachlor


R.T.: 5.168 min
Delta R.T.: 0.005 min
Response: 3779958
Conc: 1.27 ng/ml

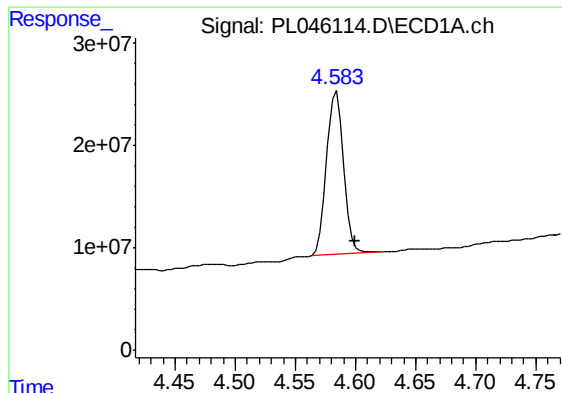

#5 Aldrin


R.T.: 4.584 min
Delta R.T.: -0.015 min
Response: 156250709
Conc: 16.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-2(10-11)

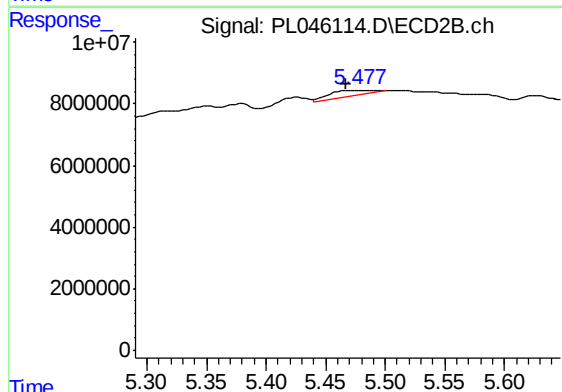


#5 Aldrin

R.T.: 5.478 min
Delta R.T.: 0.010 min
Response: 5032897
Conc: 1.86 ng/ml

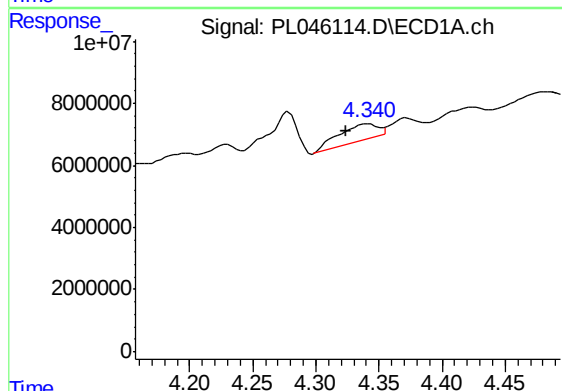


#6 beta-BHC

R.T.: 4.341 min
Delta R.T.: 0.018 min
Response: 11685657
Conc: 2.73 ng/ml

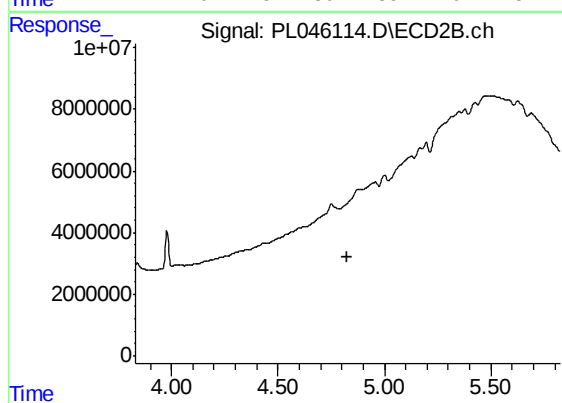

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.828 min
Response: 0
Conc: N.D.

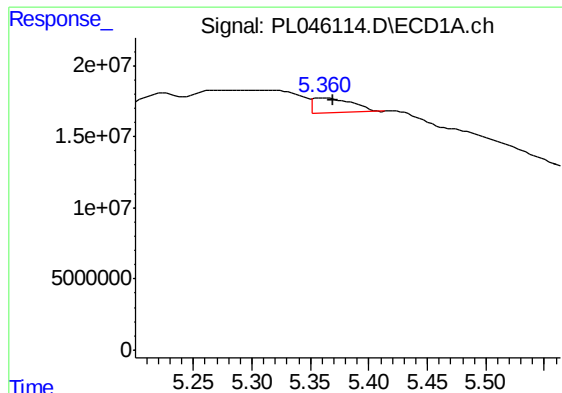

#9 Endosulfan I


R.T.: 5.361 min
Delta R.T.: -0.008 min
Response: 23986405
Conc: 2.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-2(10-11)

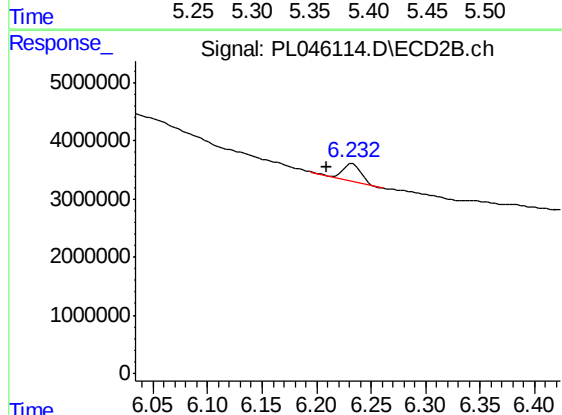


#9 Endosulfan I

R.T.: 6.233 min
Delta R.T.: 0.023 min
Response: 3270906
Conc: 1.31 ng/ml

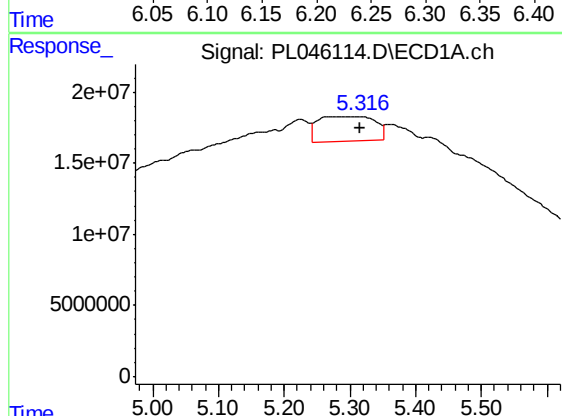


#11 alpha-Chlordane

R.T.: 5.314 min
Delta R.T.: -0.003 min
Response: 102131245
Conc: 10.53 ng/ml

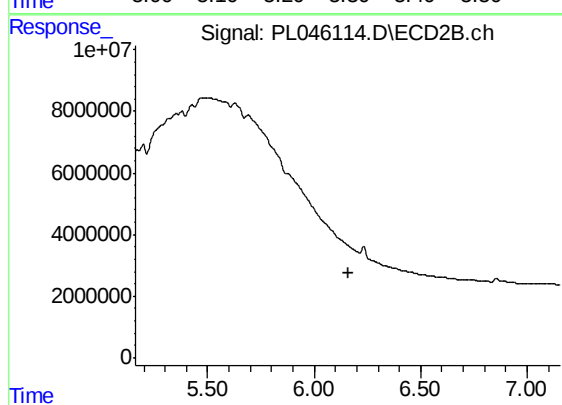

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.160 min
Response: 0
Conc: N.D.

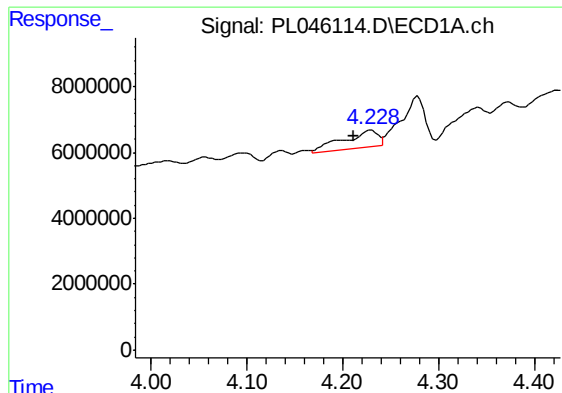

#23 Chlordane-1


R.T.: 4.230 min
Delta R.T.: 0.019 min
Response: 13226429
Conc: 39.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-2(10-11)

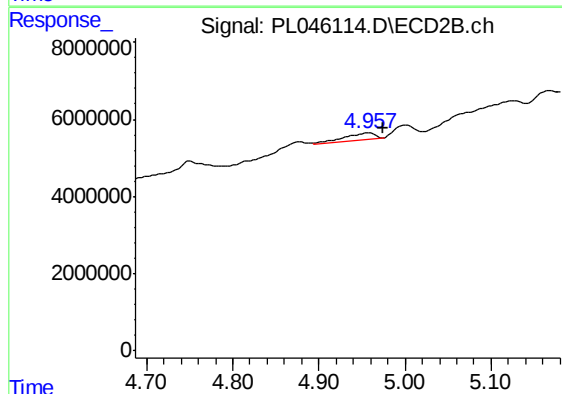


#23 Chlordane-1

R.T.: 4.959 min
Delta R.T.: -0.016 min
Response: 4803866
Conc: 42.60 ng/ml

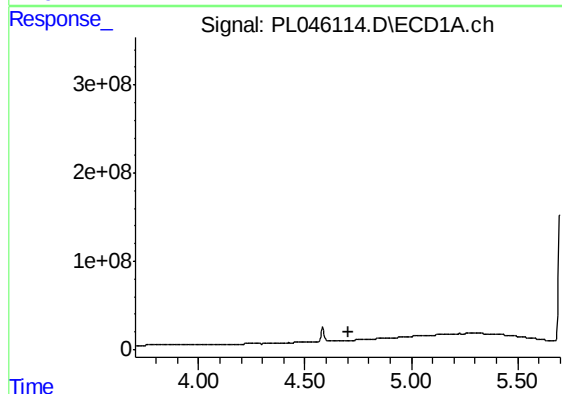


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

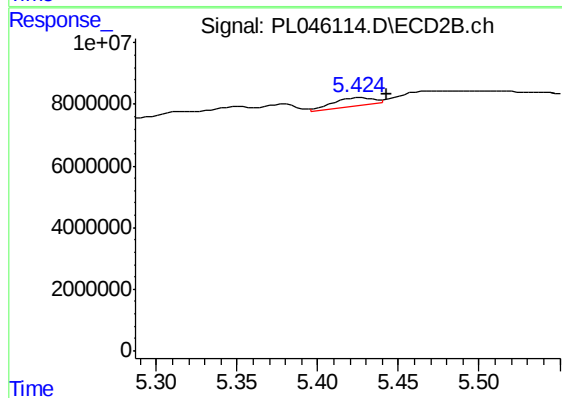

#24 Chlordane-2


R.T.: 5.426 min
Delta R.T.: -0.017 min
Response: 4675503
Conc: 38.69 ng/ml

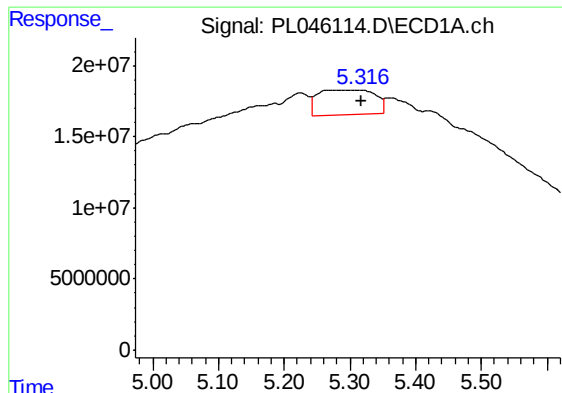

#26 Chlordane-4


R.T.: 5.314 min
Delta R.T.: -0.003 min
Response: 102131245
Conc: 96.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-2(10-11)

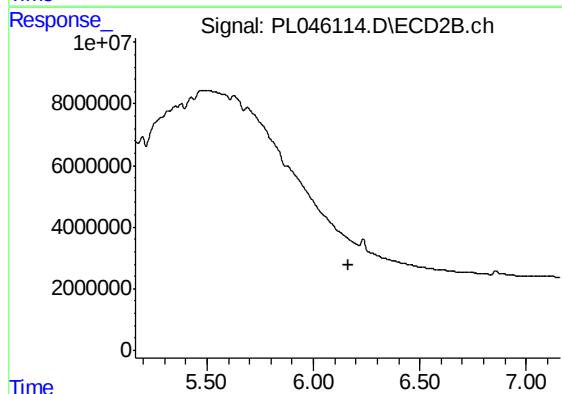


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

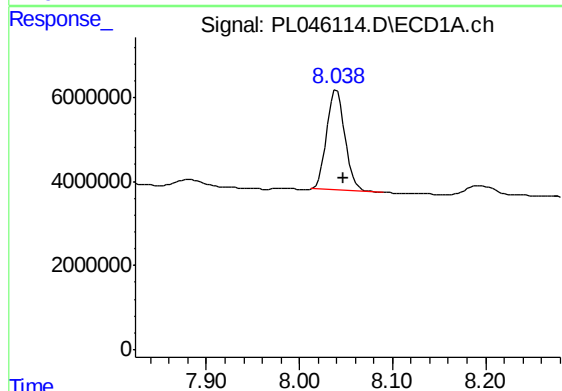

#28 Decachlorobiphenyl

R.T.: 8.040 min
Delta R.T.: -0.007 min
Response: 32340251
Conc: 3.87 ng/ml

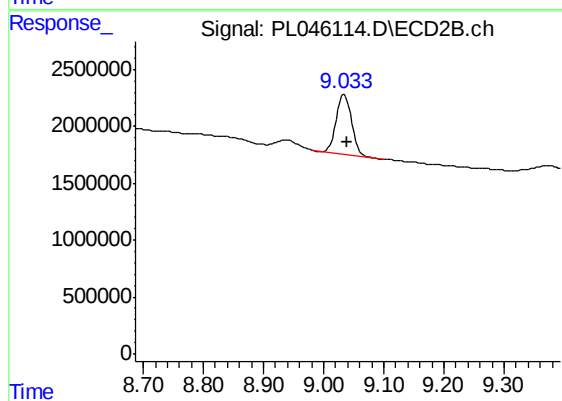

#28 Decachlorobiphenyl

R.T.: 9.034 min
Delta R.T.: -0.005 min
Response: 9302743
Conc: 4.07 ng/ml