

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031819\
 Data File : PL046116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2019 23:37
 Operator : AJ\SJ
 Sample : K1935-10
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-7(6-7)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:05:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1) SA	Tetrachlo...	3.361	3.979	42448485	13410787	6.170	6.262
28) SA	Decachlor...	8.040	9.035	69720726	20506561	8.332	8.975
Target Compounds							
4) MA	Heptachlor	0.000	5.164	0	1721146	N.D.	0.579 #
5) MB	Aldrin	4.585	5.470	65462841	4167167	6.730	1.543 #
7) B	delta-BHC	0.000	5.038	0	5247061	N.D.	2.439 #
8) B	Heptachlo...	5.060f	0.000	3782079	0	0.405	N.D. #
9) A	Endosulfan I	0.000	6.234f	0	1351719	N.D.	0.543 #
10) B	gamma-Chl...	5.284f	0.000	27958980	0	2.857	N.D. #
23)	Chlordane-1	4.235f	4.960f	6128663	2242943	18.189	19.891
24)	Chlordane-2	0.000	5.470f	0	4167167	N.D.	34.488 #
25)	Chlordane-3	5.284f	0.000	27958980	0	24.375	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031819\
Data File : PL046116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2019 23:37
Operator : AJ\SJ
Sample : K1935-10
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SB-7(6-7)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:05:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

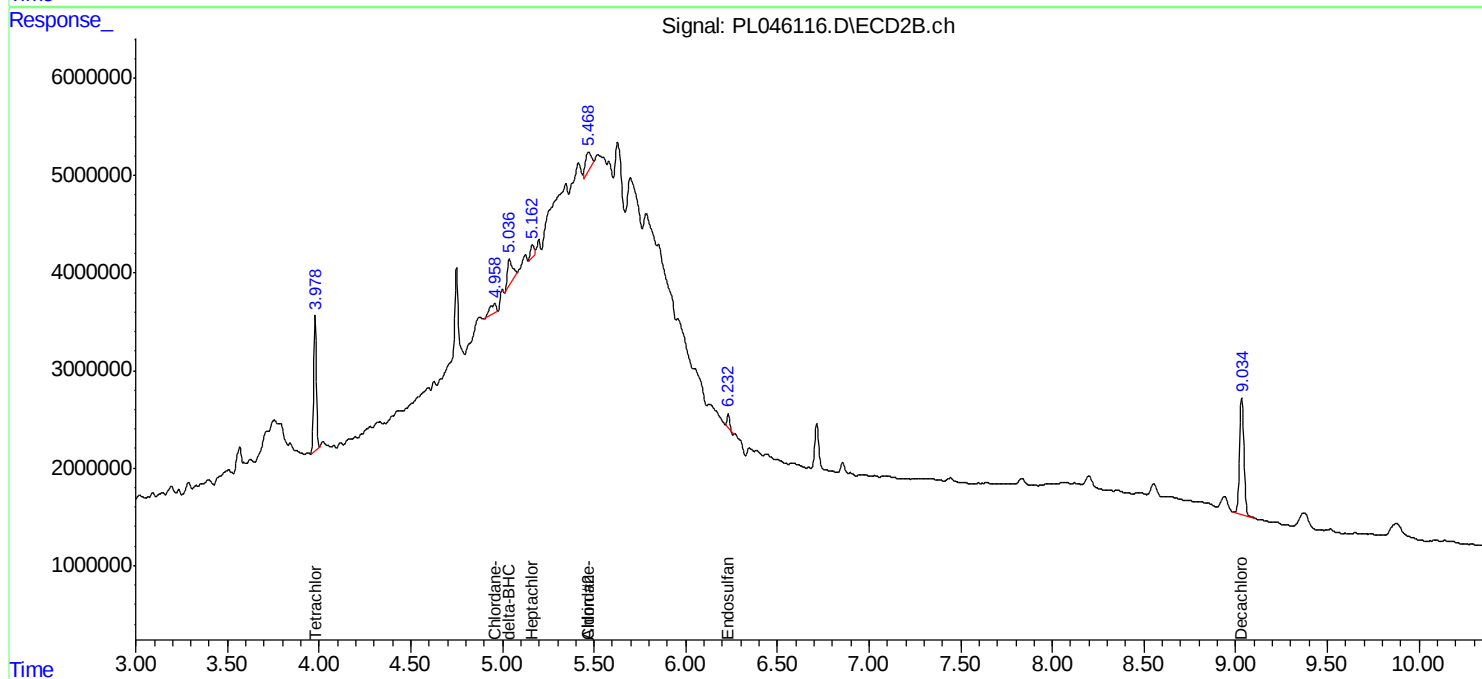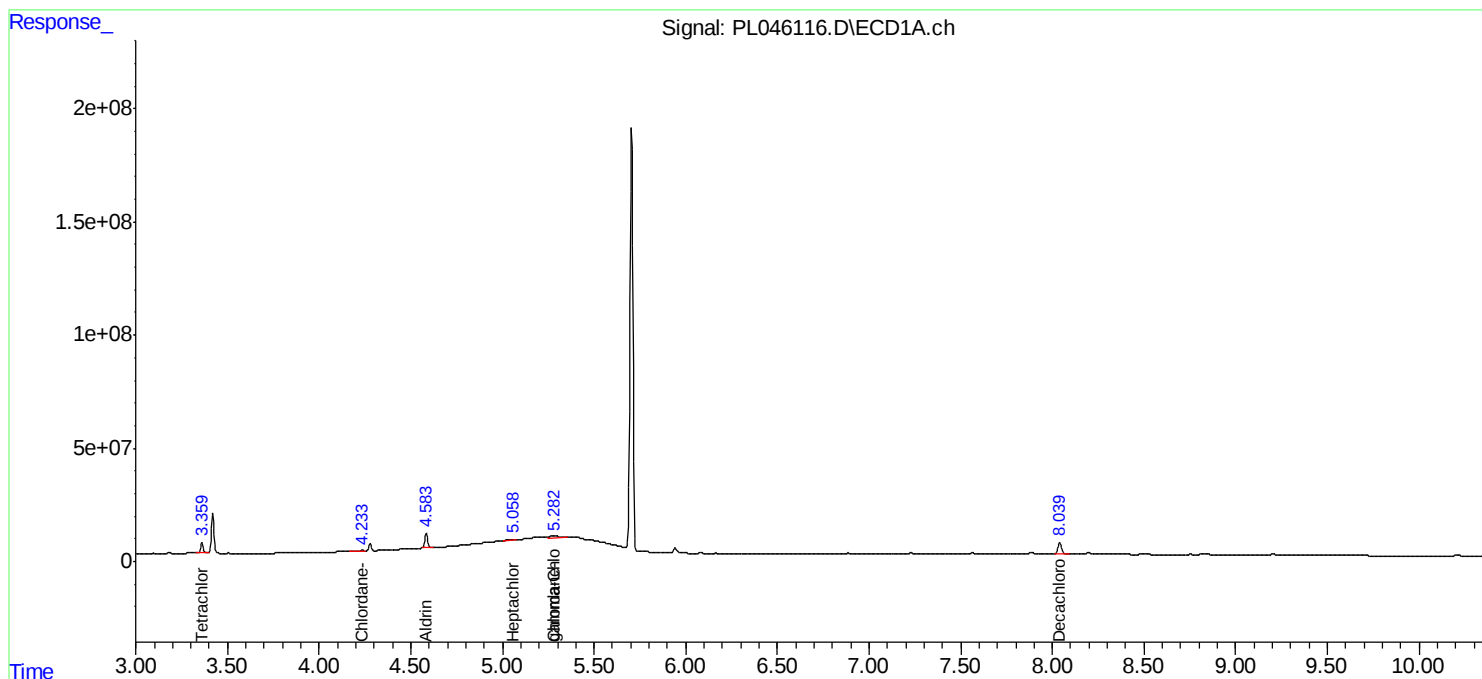


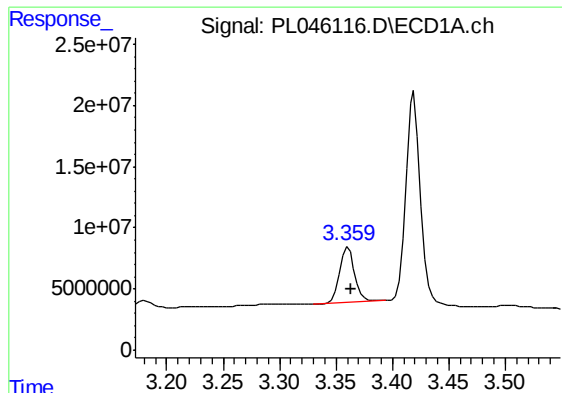

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: -0.002 min
Response: 42448485
Conc: 6.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7(6-7)

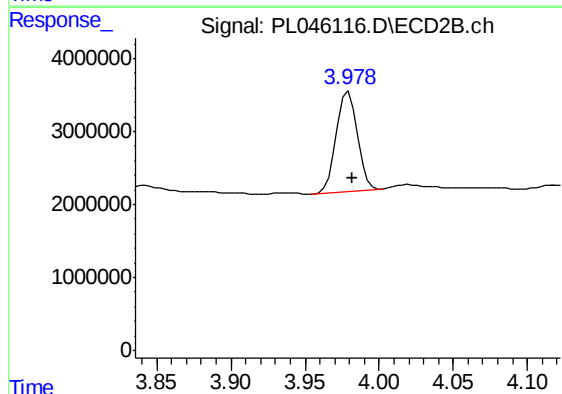


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.002 min
Response: 13410787
Conc: 6.26 ng/ml

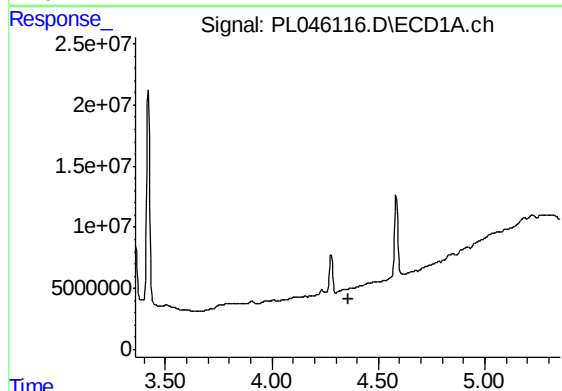


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.358 min
Response: 0
Conc: N.D.

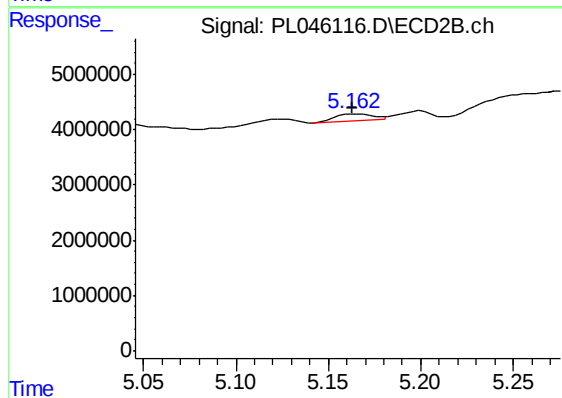

#4 Heptachlor


R.T.: 5.164 min
Delta R.T.: 0.001 min
Response: 1721146
Conc: 0.58 ng/ml

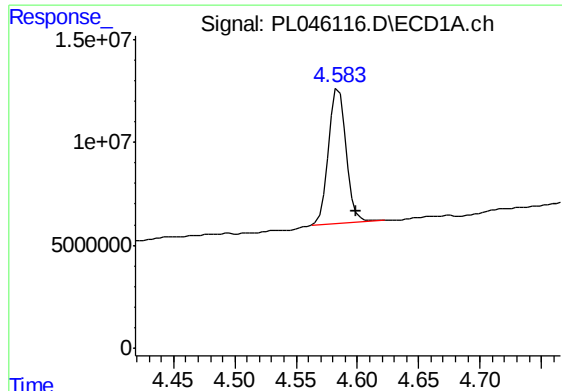

#5 Aldrin


R.T.: 4.585 min
Delta R.T.: -0.015 min
Response: 65462841
Conc: 6.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7(6-7)

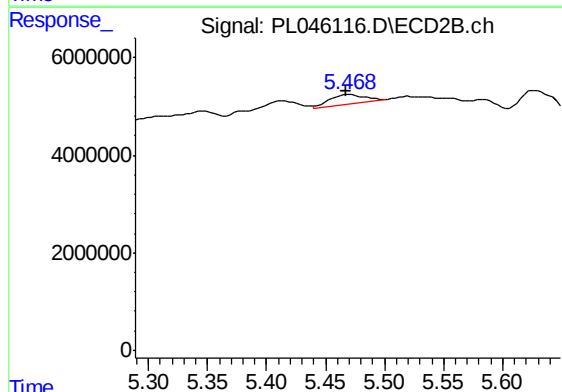


#5 Aldrin

R.T.: 5.470 min
Delta R.T.: 0.002 min
Response: 4167167
Conc: 1.54 ng/ml

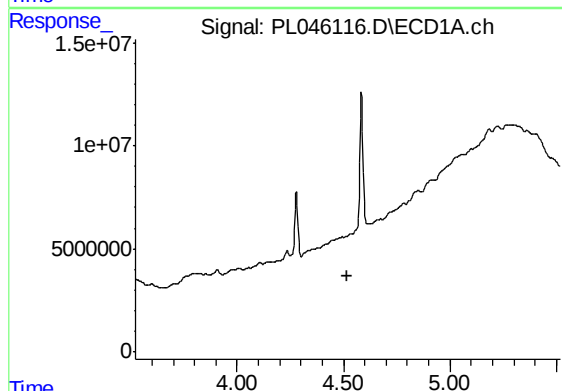


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.520 min
Response: 0
Conc: N.D.

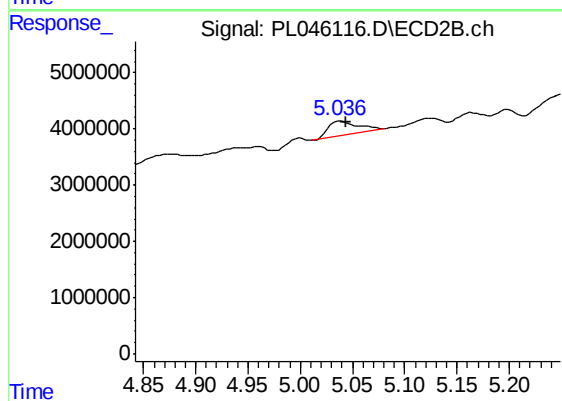

#7 delta-BHC


R.T.: 5.038 min
Delta R.T.: -0.006 min
Response: 5247061
Conc: 2.44 ng/ml

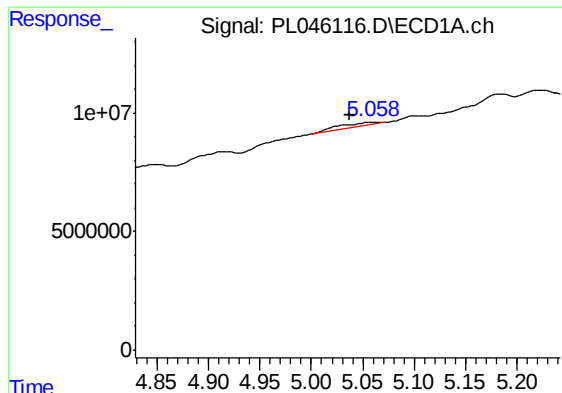

#8 Heptachlor epoxide


R.T.: 5.060 min
Delta R.T.: 0.022 min
Response: 3782079
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7(6-7)

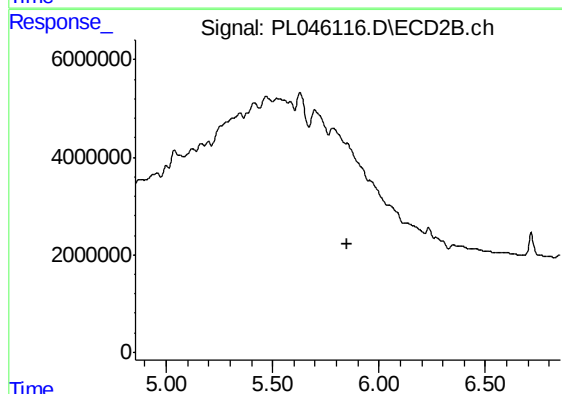


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.854 min
Response: 0
Conc: N.D.

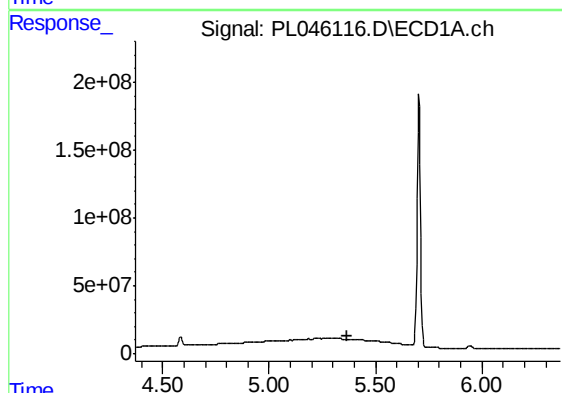


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.369 min
Response: 0
Conc: N.D.

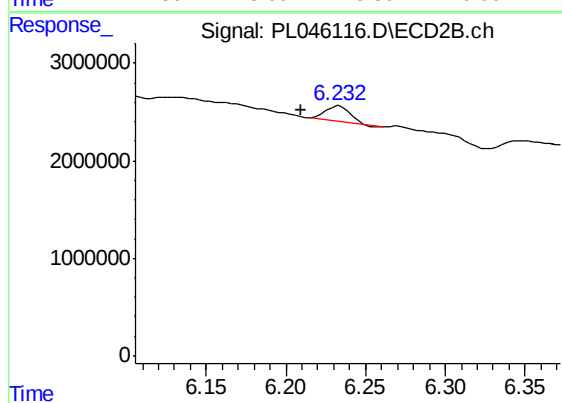

#9 Endosulfan I


R.T.: 6.234 min
Delta R.T.: 0.024 min
Response: 1351719
Conc: 0.54 ng/ml

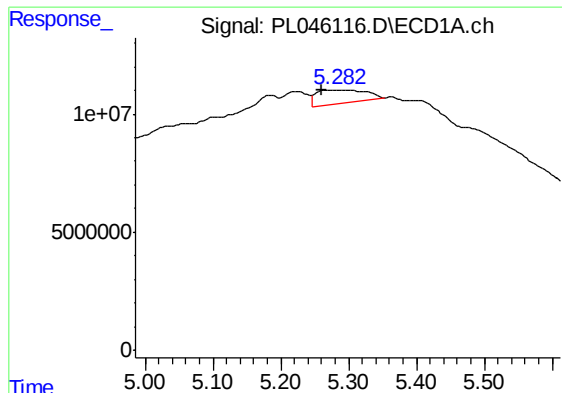

#10 gamma-Chlordane


R.T.: 5.284 min
Delta R.T.: 0.023 min
Response: 27958980
Conc: 2.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7(6-7)

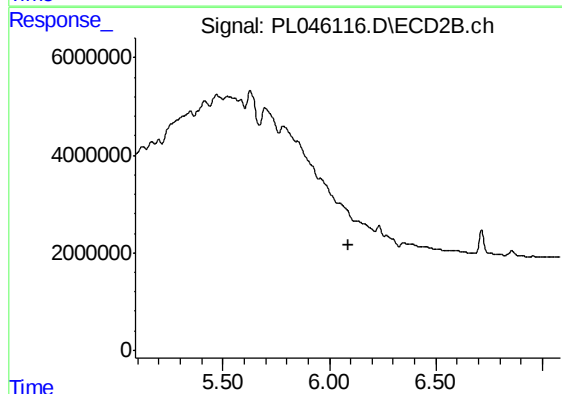


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

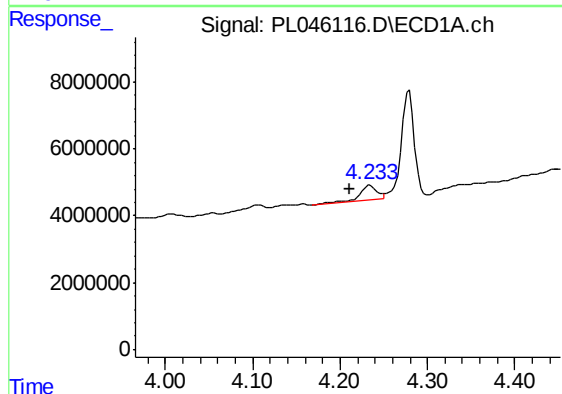


#23 Chlordane-1

R.T.: 4.235 min
Delta R.T.: 0.023 min
Response: 6128663
Conc: 18.19 ng/ml

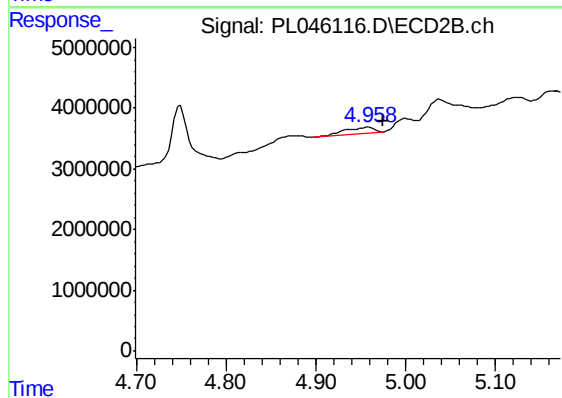

#23 Chlordane-1


R.T.: 4.960 min
Delta R.T.: -0.016 min
Response: 2242943
Conc: 19.89 ng/ml

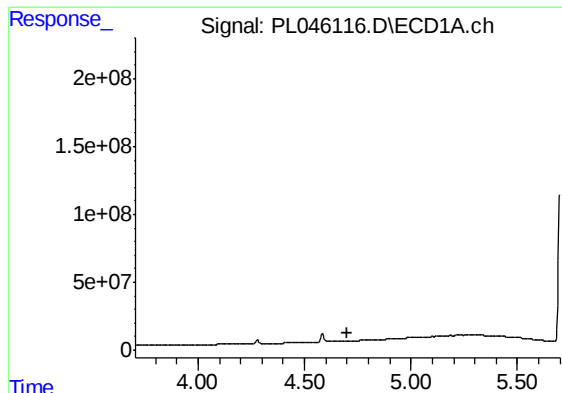

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-7(6-7)

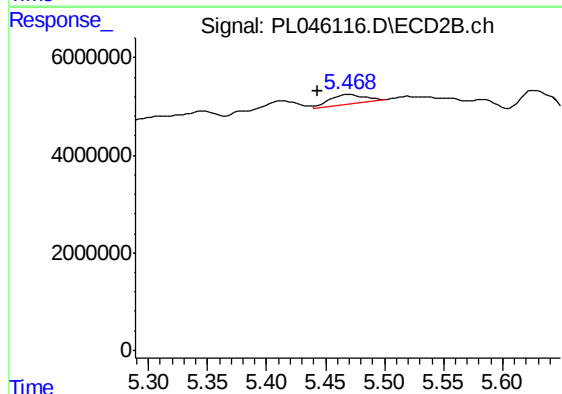


#24 Chlordane-2

R.T.: 5.470 min
Delta R.T.: 0.027 min
Response: 4167167
Conc: 34.49 ng/ml

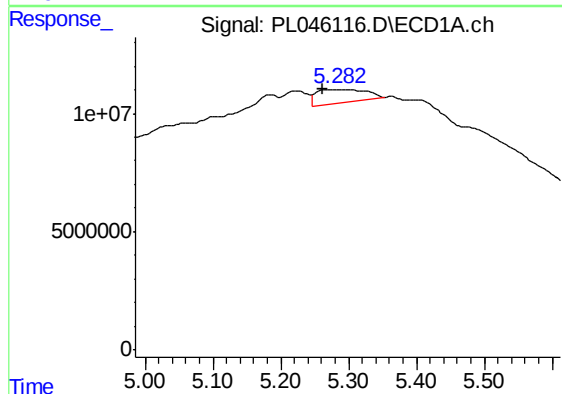


#25 Chlordane-3

R.T.: 5.284 min
Delta R.T.: 0.022 min
Response: 27958980
Conc: 24.38 ng/ml

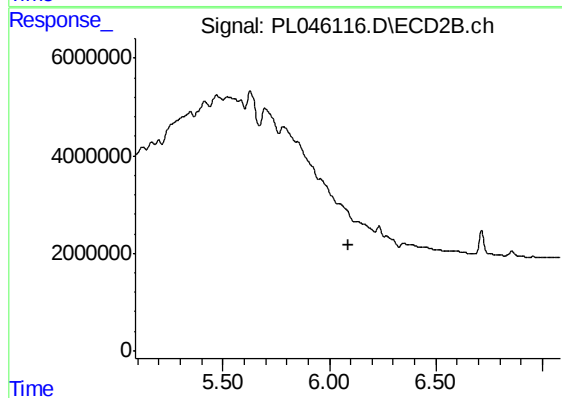

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

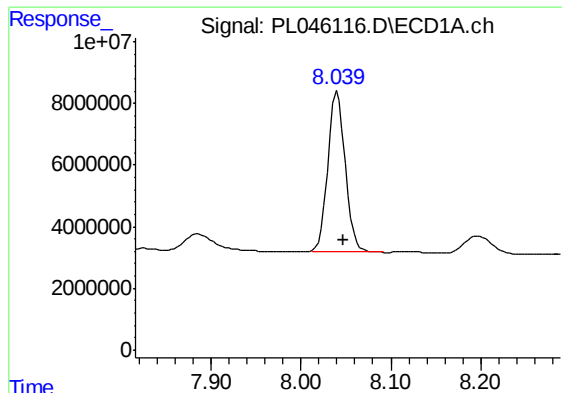

#28 Decachlorobiphenyl

R.T.: 8.040 min
Delta R.T.: -0.007 min
Response: 69720726
Conc: 8.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-7(6-7)

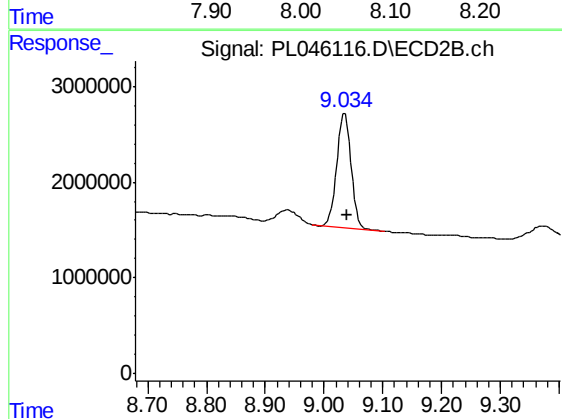

#28 Decachlorobiphenyl

R.T.: 9.035 min
Delta R.T.: -0.004 min
Response: 20506561
Conc: 8.97 ng/ml