

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031819\
 Data File : PL046089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2019 17:16
 Operator : AJ\SJ
 Sample : K1933-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S-3

Manual Integrations
 APPROVED

Sohil
 3/19/2019 2:06:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 09:46:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.360	3.979	43065977	13525015	6.260	6.316
2) SA Decachlor...	8.041	9.034	50283594	13882873	6.009	6.076
Target Compounds						
10) B gamma-Chl...	5.262	6.083	199.3E6	83071144	20.365m	30.963m#
11) B alpha-Chl...	5.312	6.159	515.4E6	208.0E6	53.153	77.110 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031819\
Data File : PL046089.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2019 17:16
Operator : AJ\SJ
Sample : K1933-03
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
S-3


Manual Integrations
APPROVED

Sohil
3/19/2019 2:06:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 09:46:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

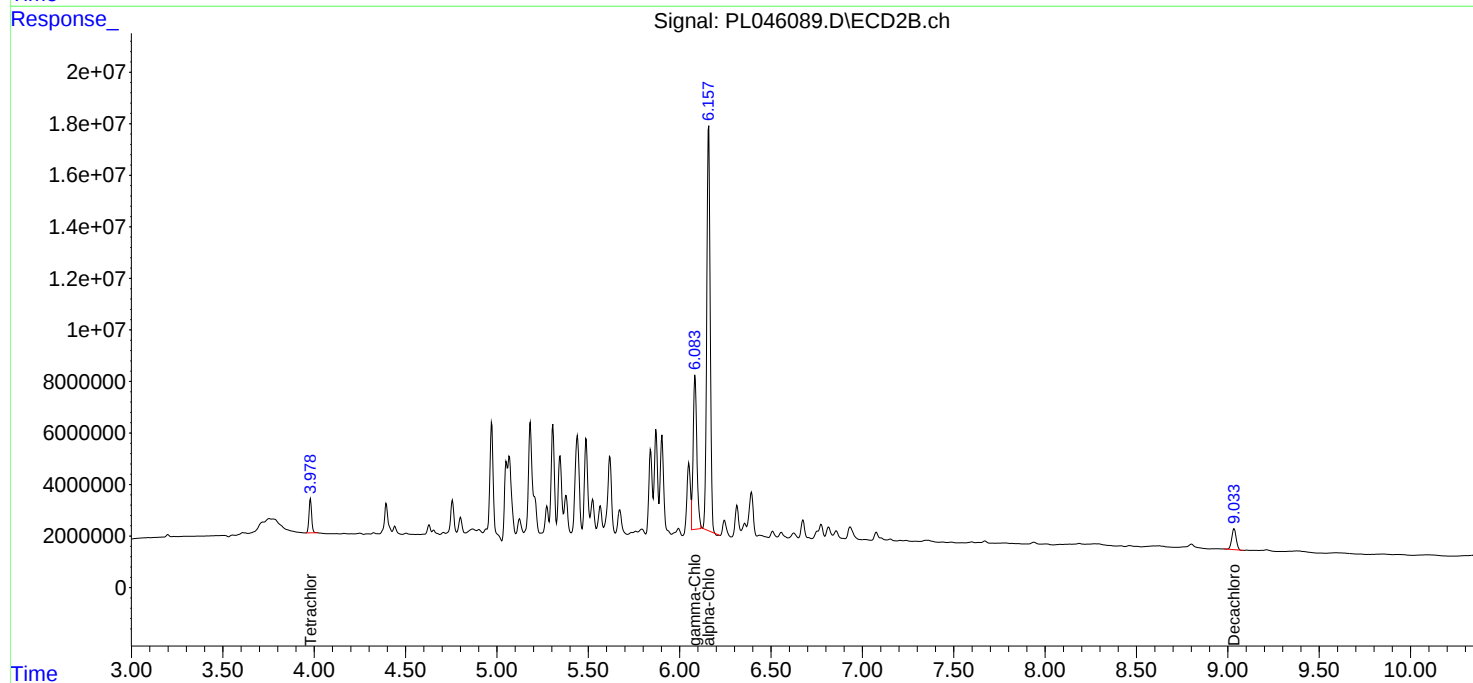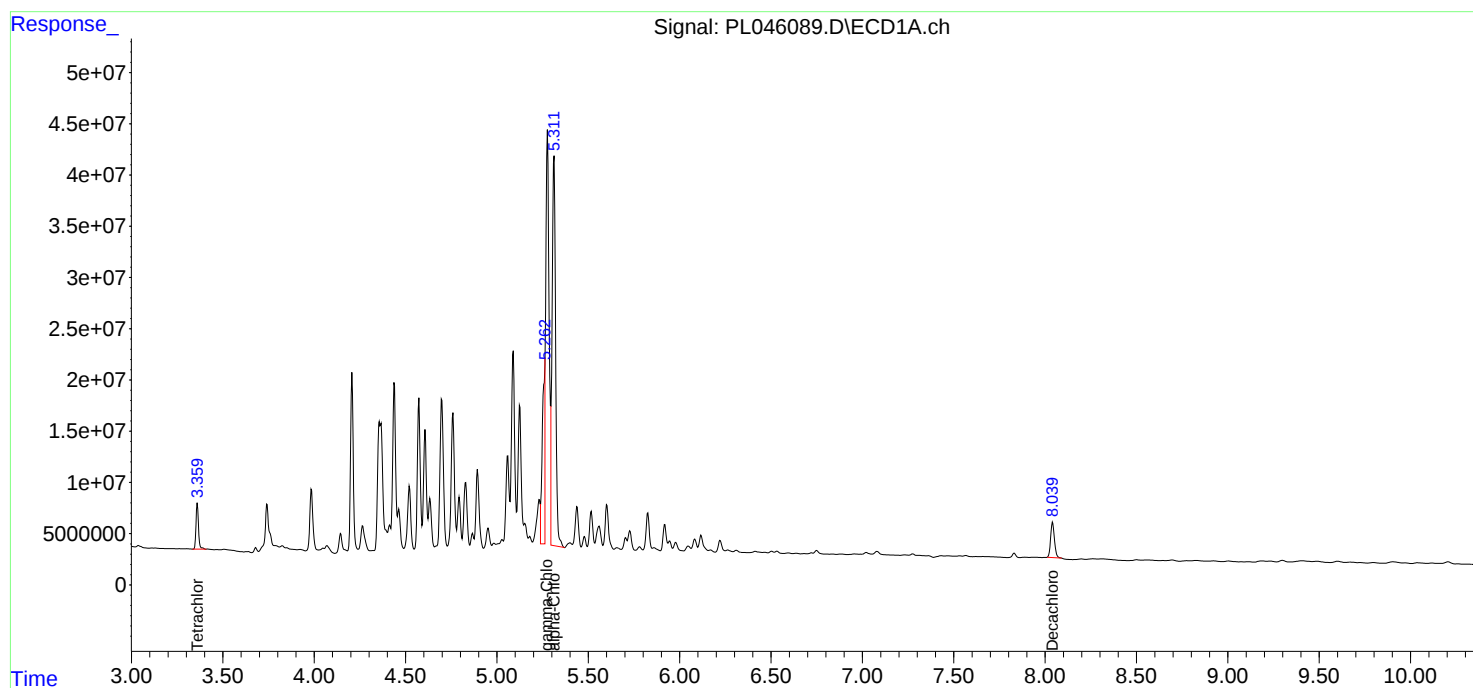

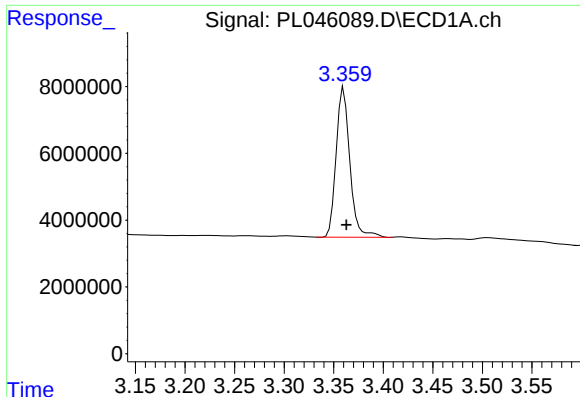


#1 Tetrachloro-m-xylene

R.T.: 3.360 min
Delta R.T.: -0.003 min
Response: 43065977
Conc: 6.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-3


Manual Integrations
APPROVED

Sohil
3/19/2019 2:06:30 PM

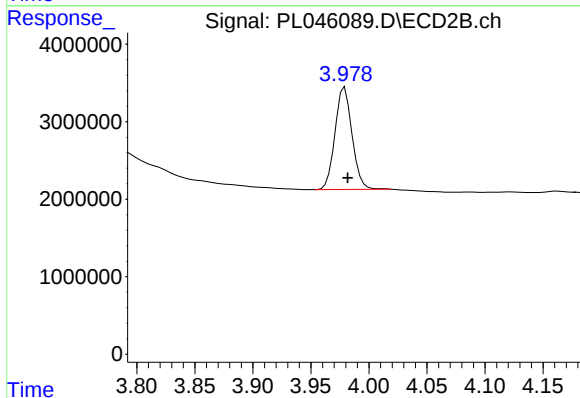


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.003 min
Response: 13525015
Conc: 6.32 ng/ml

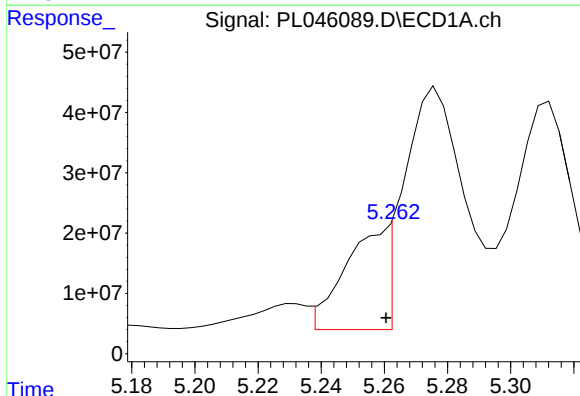


#10 gamma-Chlordane

R.T.: 5.262 min
Delta R.T.: 0.001 min
Response: 199313434
Conc: 20.37 ng/ml m

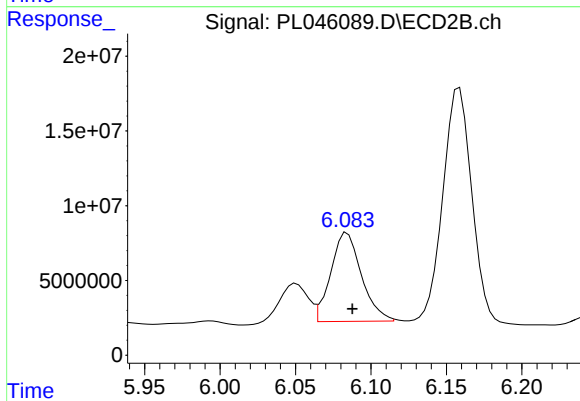

#10 gamma-Chlordane

R.T.: 6.083 min
Delta R.T.: -0.005 min
Response: 83071144
Conc: 30.96 ng/ml m

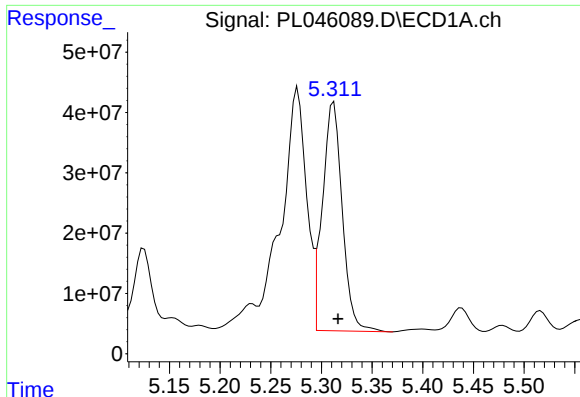


#11 alpha-Chlordane

R.T.: 5.312 min
Delta R.T.: -0.004 min
Response: 515419548
Conc: 53.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
S-3


Manual Integrations
APPROVED

Sohil
3/19/2019 2:06:30 PM

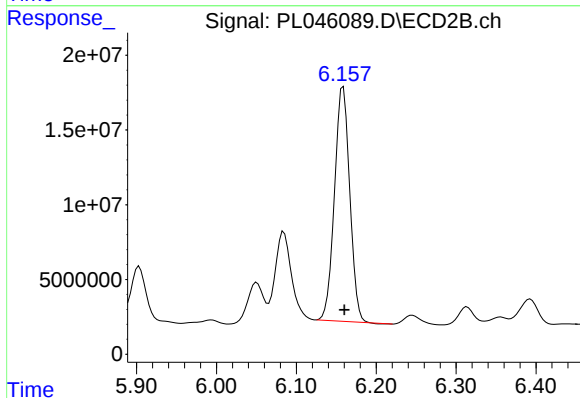


#11 alpha-Chlordane

R.T.: 6.159 min
Delta R.T.: -0.001 min
Response: 208019958
Conc: 77.11 ng/ml

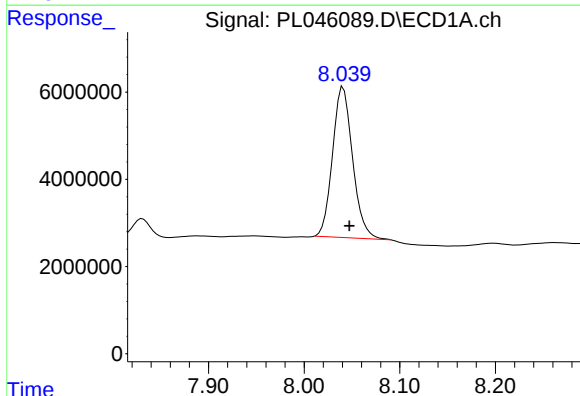

#28 Decachlorobiphenyl

R.T.: 8.041 min
Delta R.T.: -0.006 min
Response: 50283594
Conc: 6.01 ng/ml

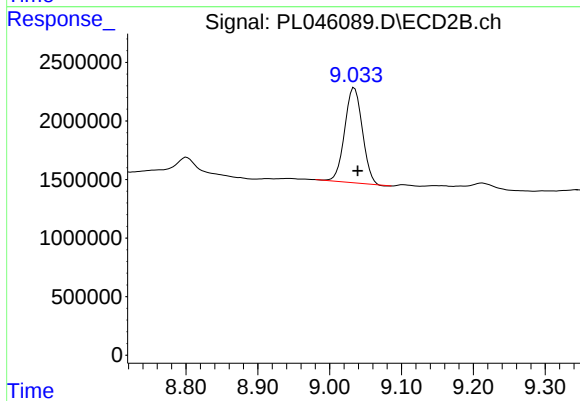

#28 Decachlorobiphenyl

R.T.: 9.034 min
Delta R.T.: -0.005 min
Response: 13882873
Conc: 6.08 ng/ml