

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
 Data File : PL065374.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2021 10:34
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 15:50:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 18 15:40:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
6) B	beta-BHC	0.000	4.645	0	3321422	N.D. 1.928 #
9) A	Endosulfan I	0.000	6.005f	0	4722908	N.D. 1.794 #
10) B	gamma-Chl...	0.000	5.839f	0	19688933	N.D. 7.055 #
15) B	Endosulfa...	0.000	6.637f	0	7502345	N.D. 3.324 #
25)	Chlordane-3	0.000	5.839f	0	19688933	N.D. 48.301 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
Data File : PL065374.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2021 10:34
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 15:50:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Thu Mar 18 15:40:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

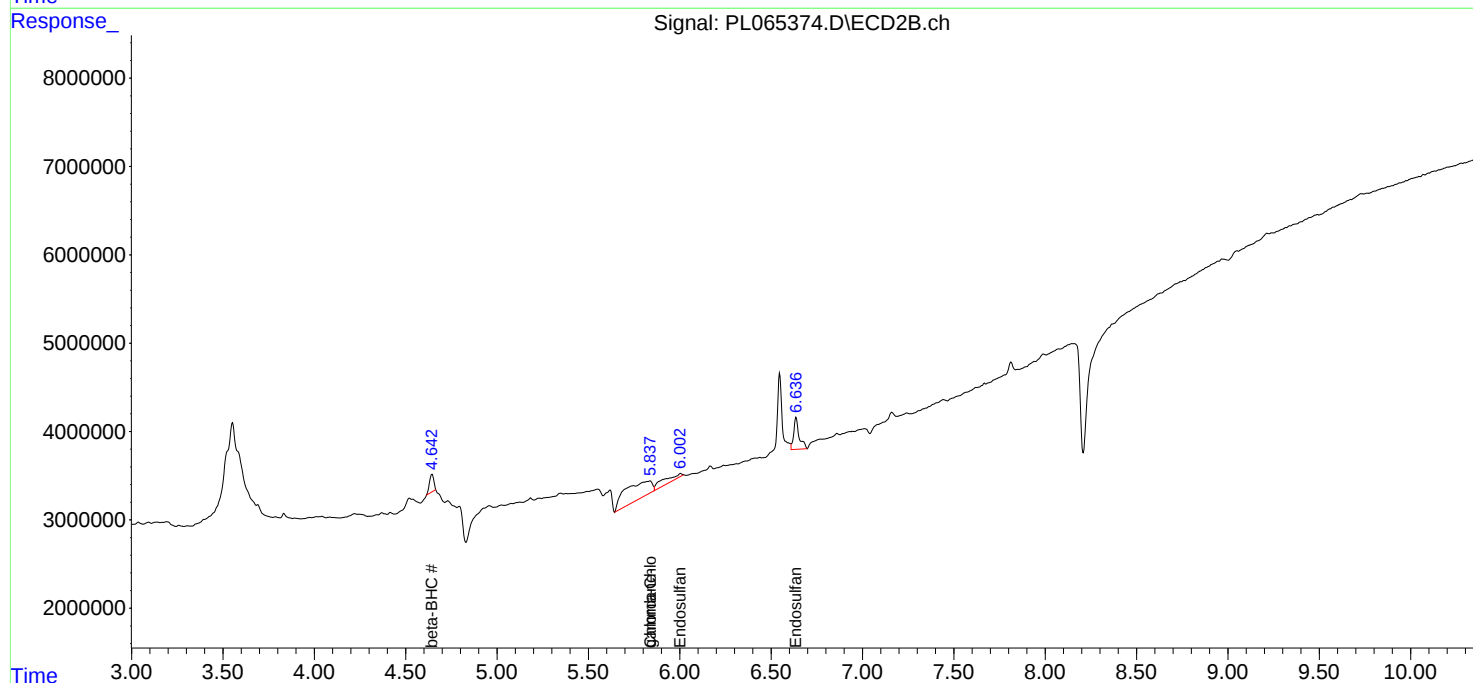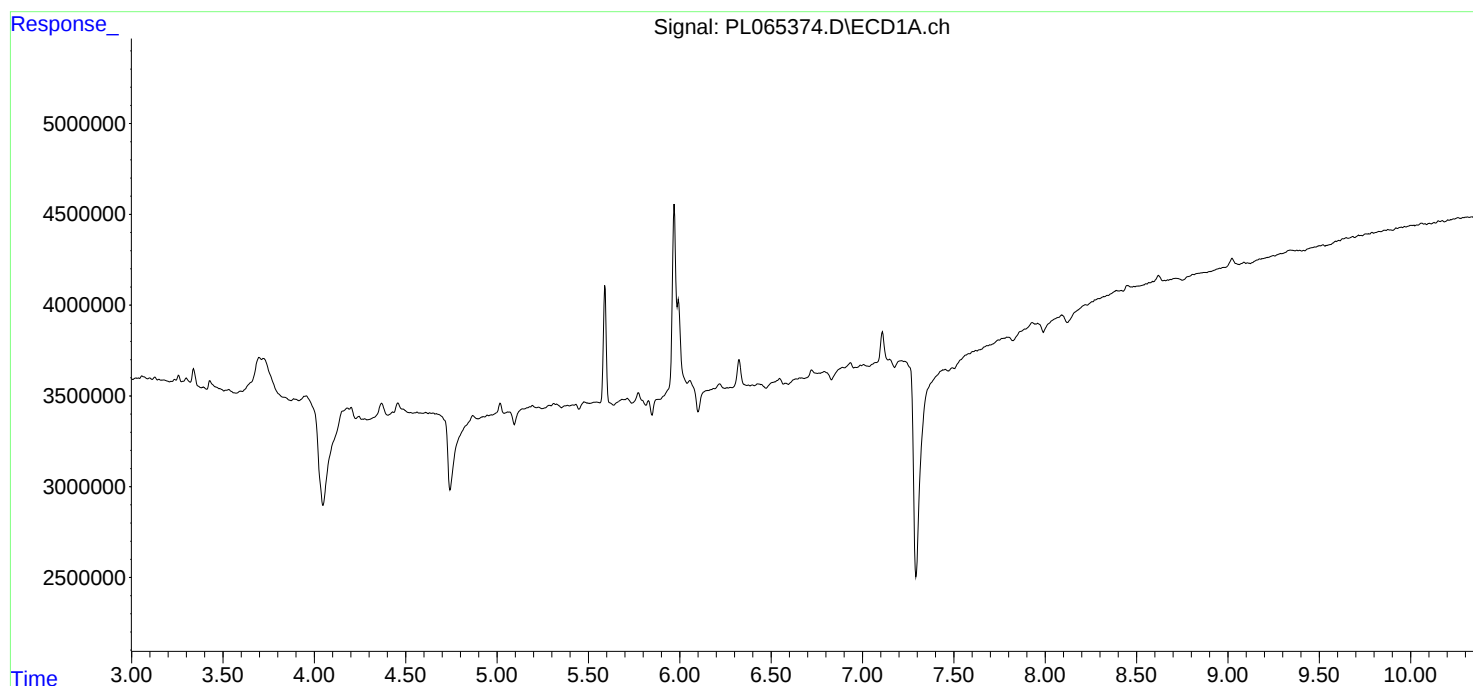


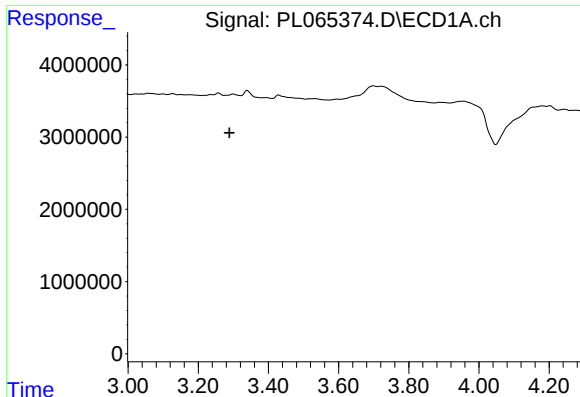

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.289 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

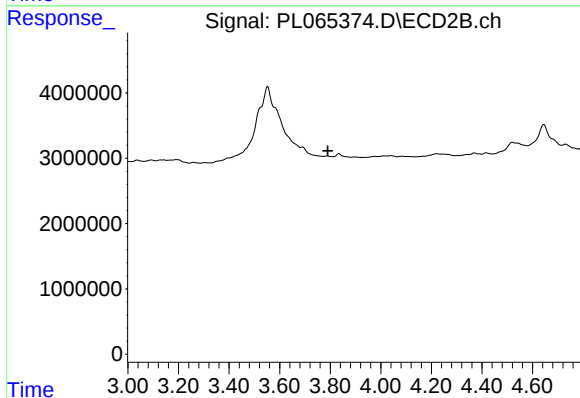


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.790 min
Response: 0
Conc: N.D.

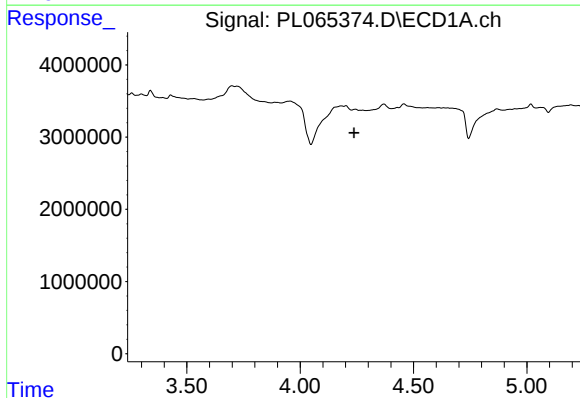


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.238 min
Response: 0
Conc: N.D.

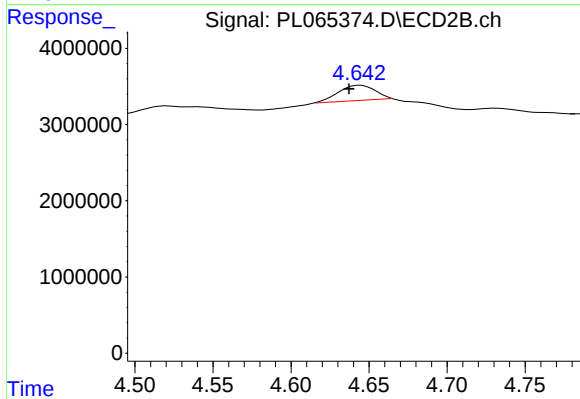

#6 beta-BHC


R.T.: 4.645 min
Delta R.T.: 0.007 min
Response: 3321422
Conc: 1.93 ng/ml

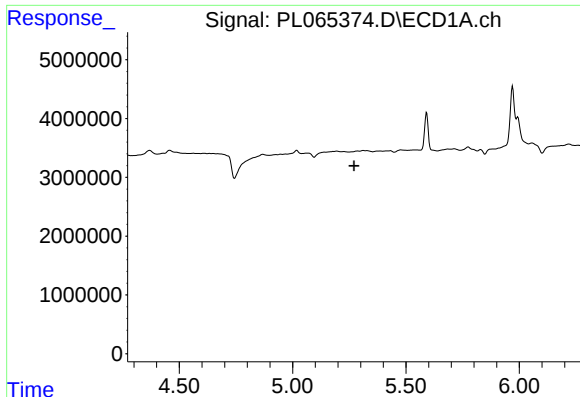

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.271 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

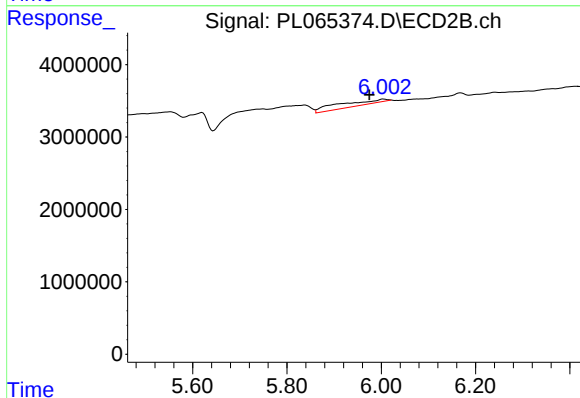


#9 Endosulfan I

R.T.: 6.005 min
Delta R.T.: 0.030 min
Response: 4722908
Conc: 1.79 ng/ml

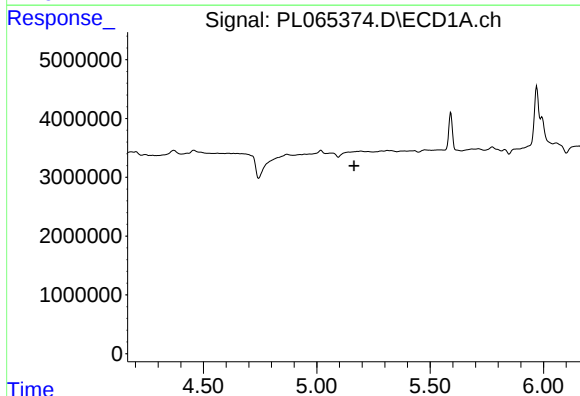


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.165 min
Response: 0
Conc: N.D.

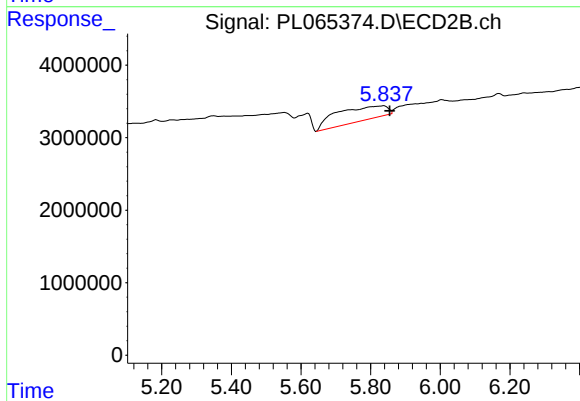

#10 gamma-Chlordane


R.T.: 5.839 min
Delta R.T.: -0.017 min
Response: 19688933
Conc: 7.06 ng/ml

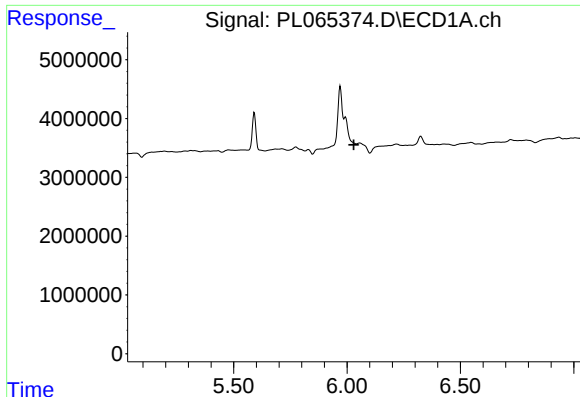

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.030 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

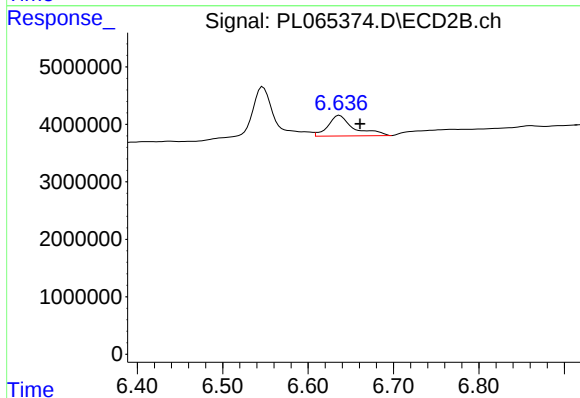


#15 Endosulfan II

R.T.: 6.637 min
Delta R.T.: -0.024 min
Response: 7502345
Conc: 3.32 ng/ml

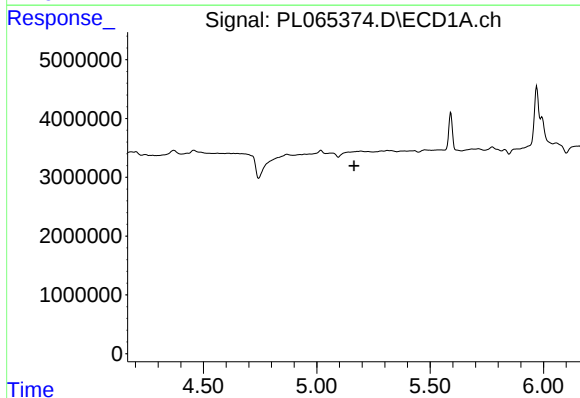


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.165 min
Response: 0
Conc: N.D.

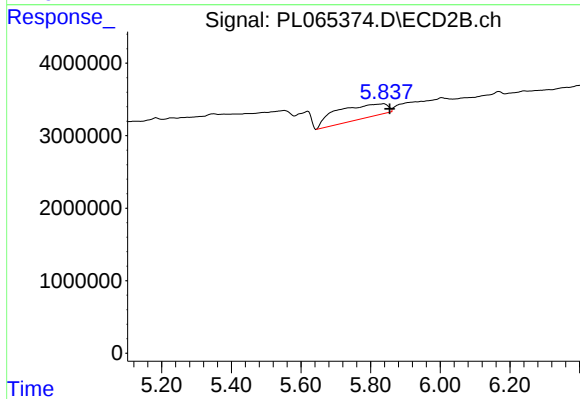

#25 Chlordane-3


R.T.: 5.839 min
Delta R.T.: -0.016 min
Response: 19688933
Conc: 48.30 ng/ml

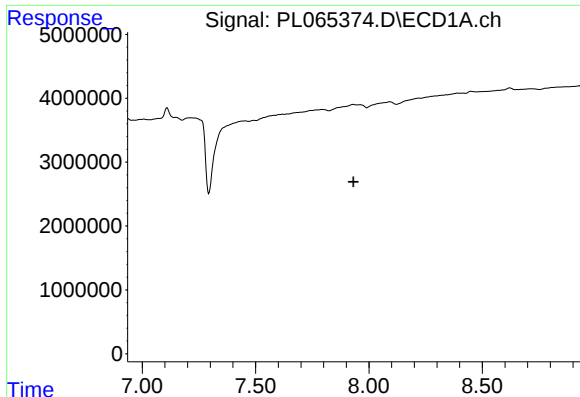

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.932 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

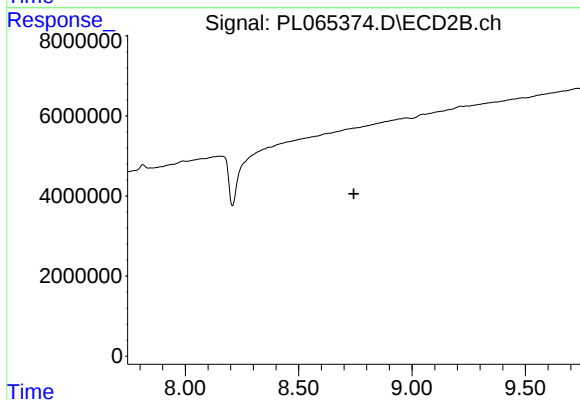

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.744 min
Response: 0
Conc: N.D.