

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
 Data File : PL065384.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2021 13:26
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:06:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:02:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.790	200.8E6	202.2E6	75.412	75.001
28)	SA Decachlor...	7.933	8.744	172.7E6	141.9E6	74.686	74.592
Target Compounds							
23)	Chlordane-1	4.127	4.756	66482673	84159310	753.112	749.039
24)	Chlordane-2	4.614	5.219	79230996	77665052	747.876	747.090
25)	Chlordane-3	5.166	5.856	226.7E6	303.7E6	749.659	748.431
26)	Chlordane-4	5.221	5.926	203.0E6	355.7E6	739.384	747.565
27)	Chlordane-5	6.034	6.724	72309466	60477199	736.243	749.148



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
Data File : PL065384.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2021 13:26
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:06:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:02:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

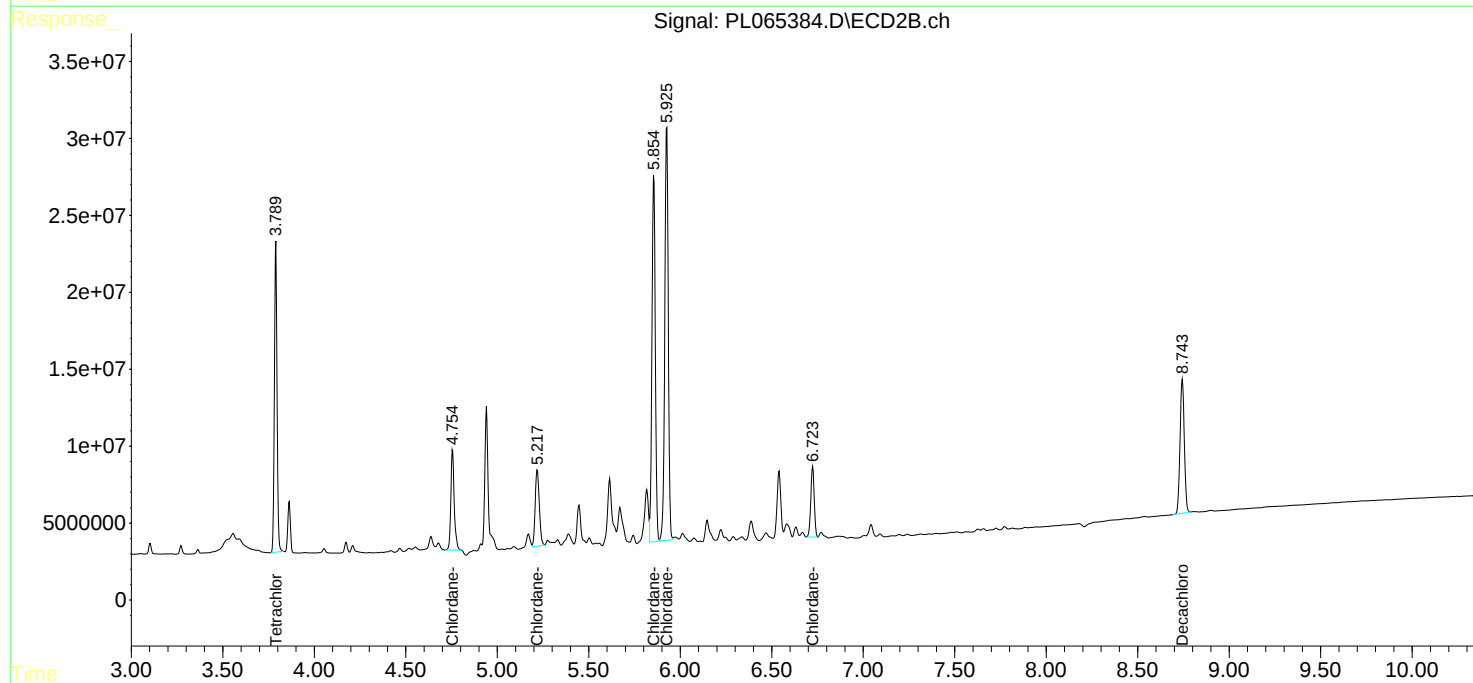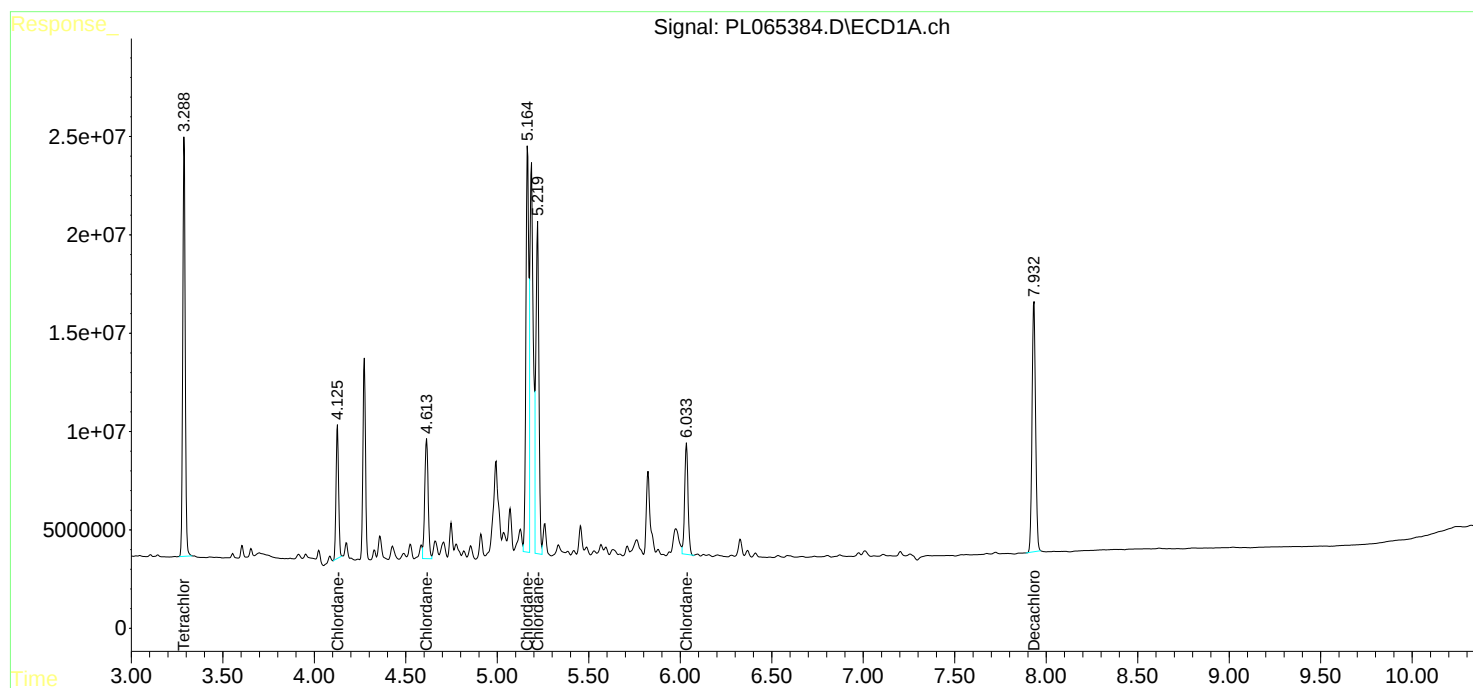


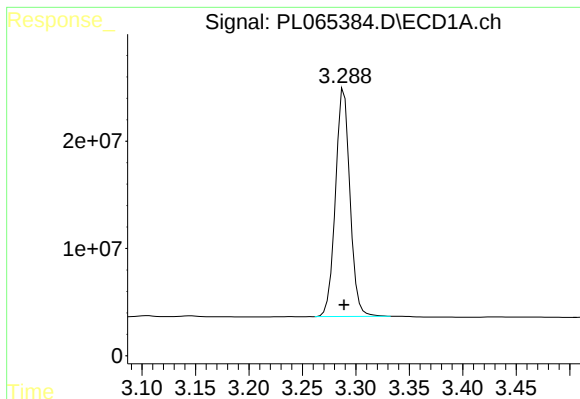

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 200790324
Conc: 75.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

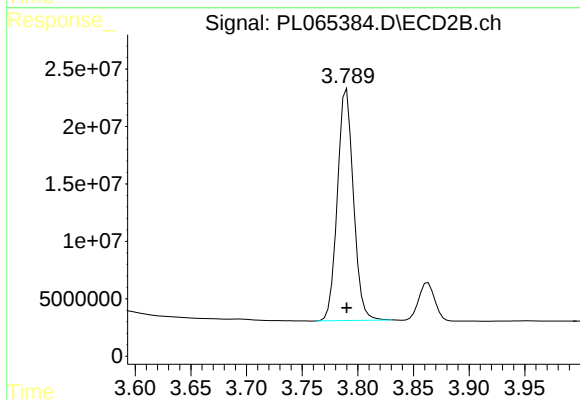


#1 Tetrachloro-m-xylene

R.T.: 3.790 min
Delta R.T.: 0.000 min
Response: 202245772
Conc: 75.00 ng/ml

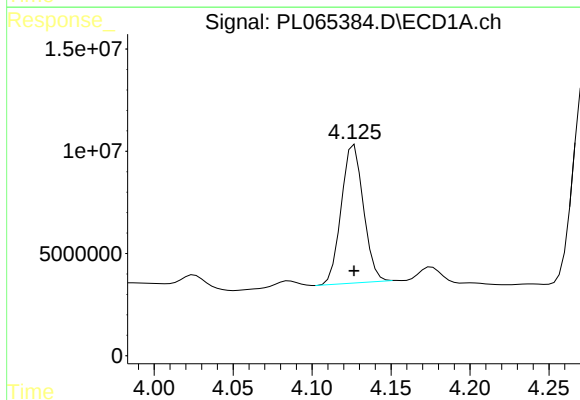


#23 Chlordane-1

R.T.: 4.127 min
Delta R.T.: 0.000 min
Response: 66482673
Conc: 753.11 ng/ml

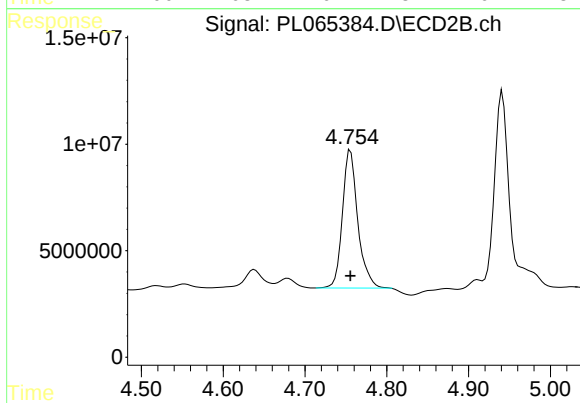

#23 Chlordane-1


R.T.: 4.756 min
Delta R.T.: 0.000 min
Response: 84159310
Conc: 749.04 ng/ml

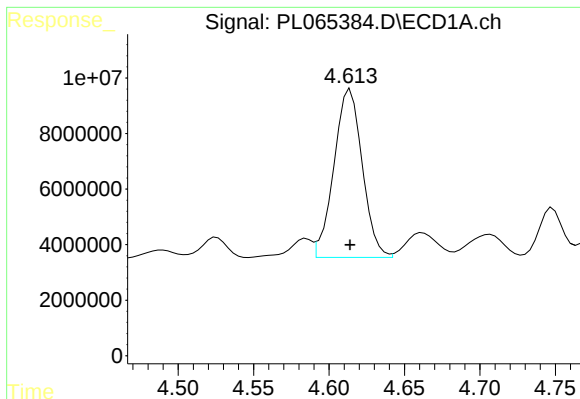

#24 Chlordane-2


R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 79230996
Conc: 747.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

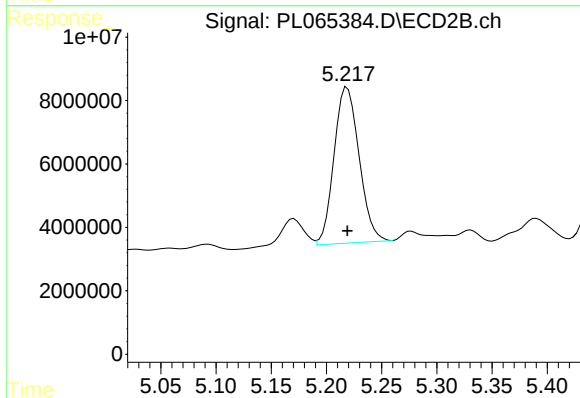


#24 Chlordane-2

R.T.: 5.219 min
Delta R.T.: 0.000 min
Response: 77665052
Conc: 747.09 ng/ml

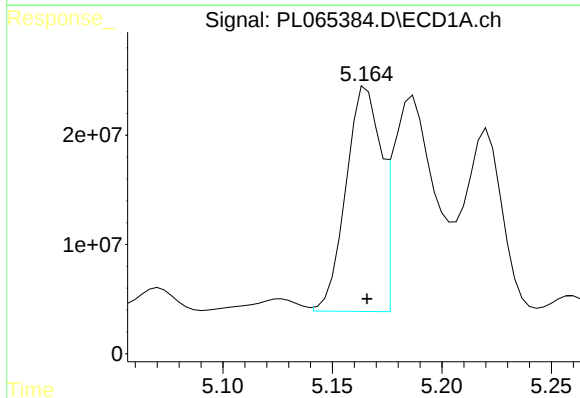


#25 Chlordane-3

R.T.: 5.166 min
Delta R.T.: 0.000 min
Response: 226712017
Conc: 749.66 ng/ml

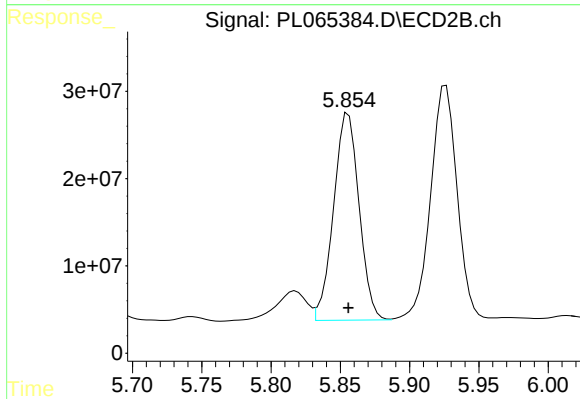

#25 Chlordane-3


R.T.: 5.856 min
Delta R.T.: 0.000 min
Response: 303727748
Conc: 748.43 ng/ml

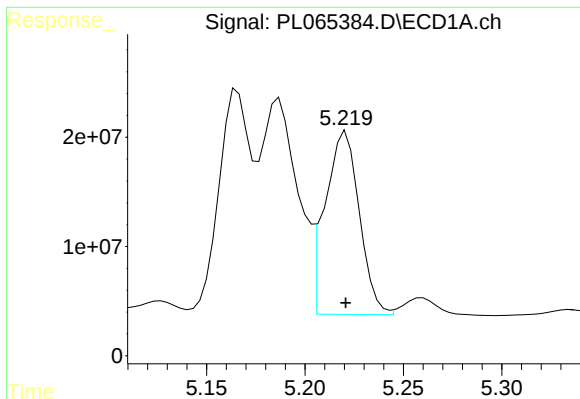

#26 Chlordane-4


R.T.: 5.221 min
Delta R.T.: 0.000 min
Response: 202967922
Conc: 739.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

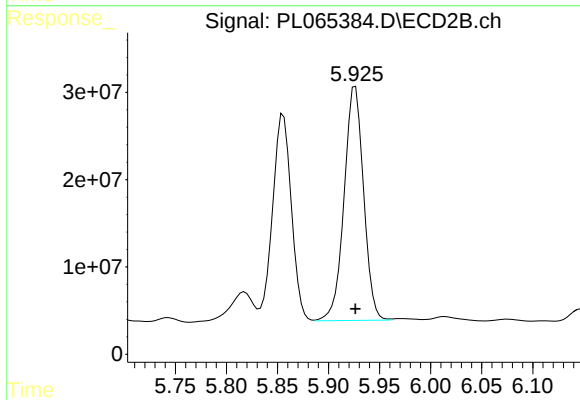


#26 Chlordane-4

R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 355673660
Conc: 747.56 ng/ml

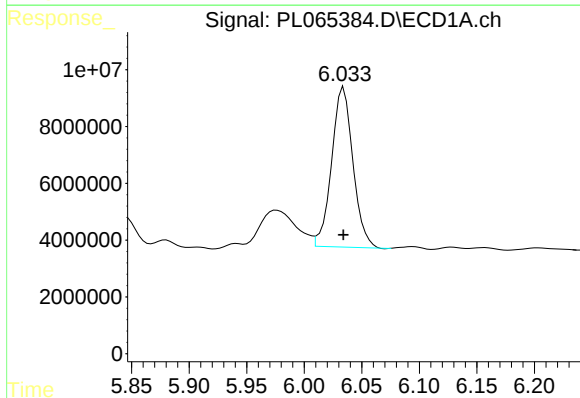


#27 Chlordane-5

R.T.: 6.034 min
Delta R.T.: 0.000 min
Response: 72309466
Conc: 736.24 ng/ml

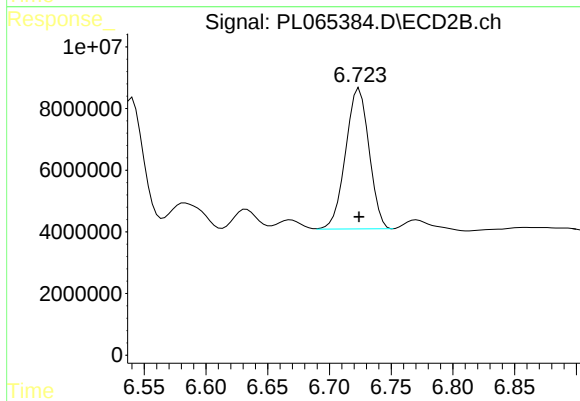

#27 Chlordane-5

R.T.: 6.724 min
Delta R.T.: 0.000 min
Response: 60477199
Conc: 749.15 ng/ml

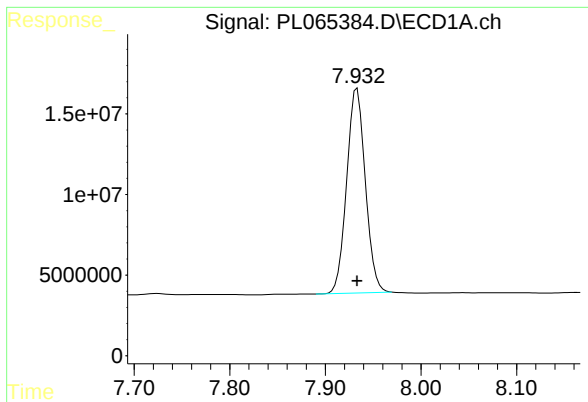

#28 Decachlorobiphenyl


R.T.: 7.933 min

Delta R.T.: 0.000 min

Response: 172688452

Conc: 74.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

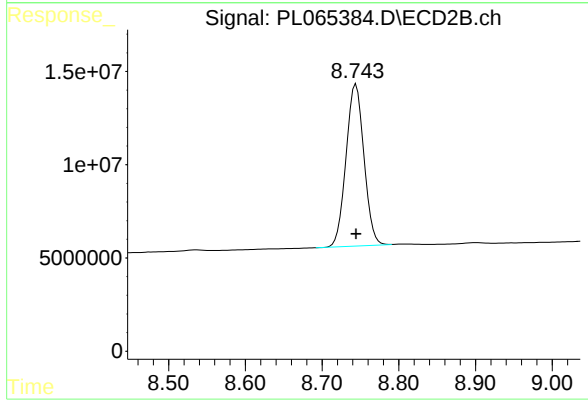

#28 Decachlorobiphenyl

R.T.: 8.744 min

Delta R.T.: 0.000 min

Response: 141867485

Conc: 74.59 ng/ml