

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
 Data File : PL065385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2021 13:40
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:02:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:02:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.790	133.3E6	138.6E6	50.000	50.000
28)	SA Decachlor...	7.933	8.743	120.0E6	98208659	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.126	4.756	45113673	57896361	500.000	500.000
24)	Chlordane-2	4.614	5.219	55241469	54258722	500.000	500.000
25)	Chlordane-3	5.166	5.856	154.9E6	206.6E6	500.000	500.000
26)	Chlordane-4	5.221	5.926	140.9E6	243.3E6	500.000	500.000
27)	Chlordane-5	6.035	6.724	50296431	40957570	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
Data File : PL065385.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2021 13:40
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:02:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:02:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

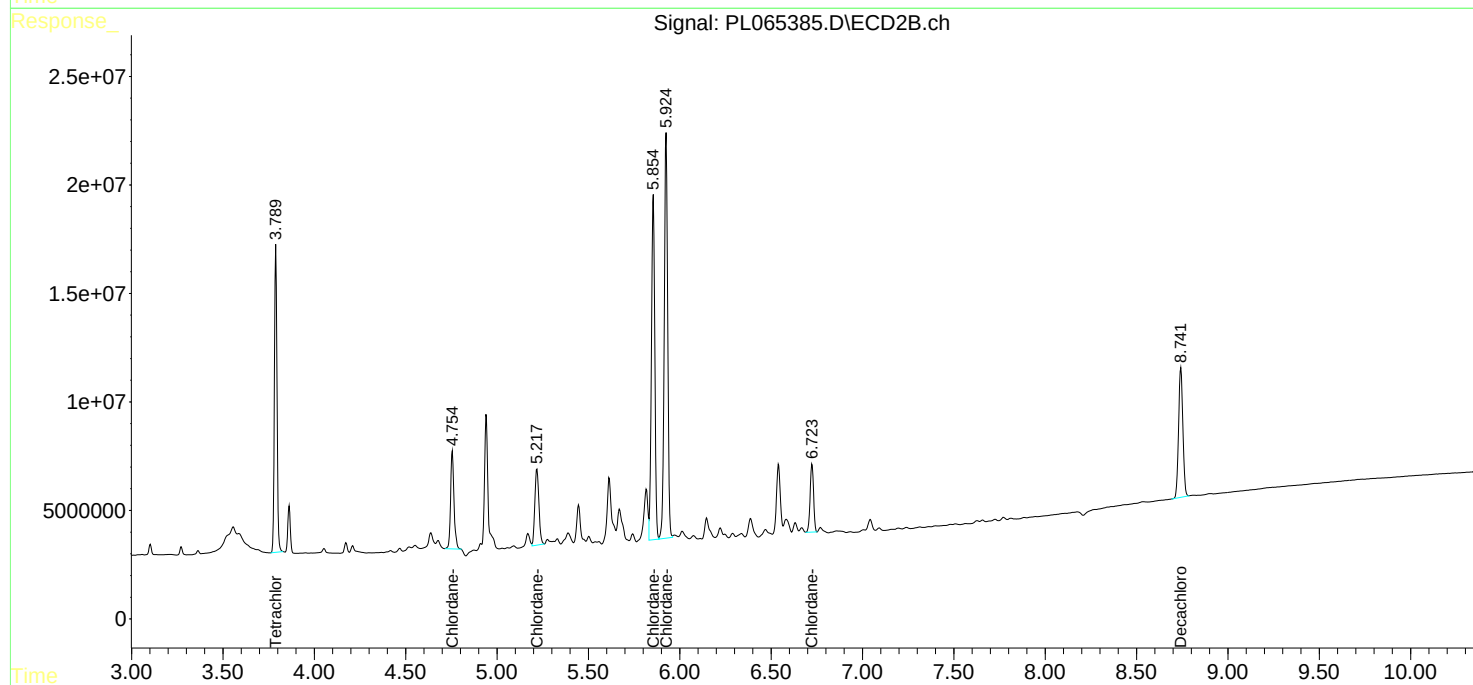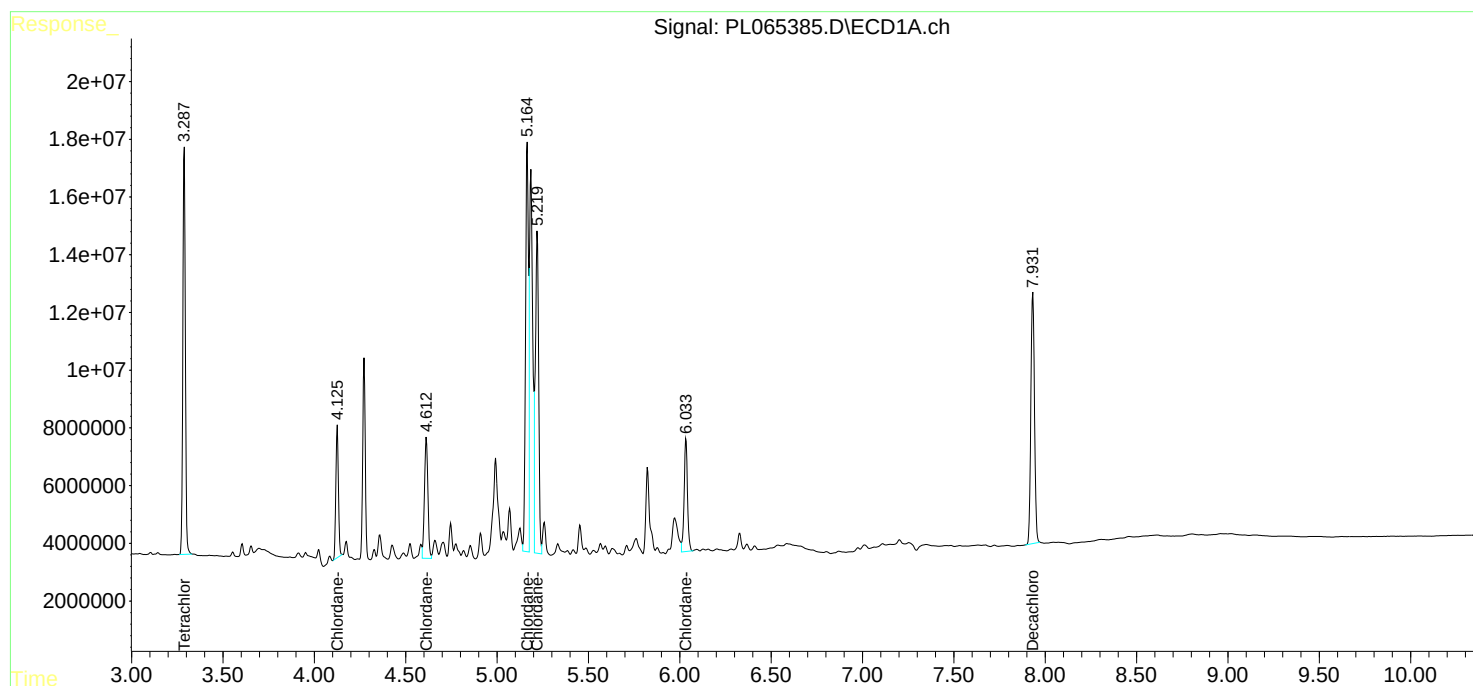


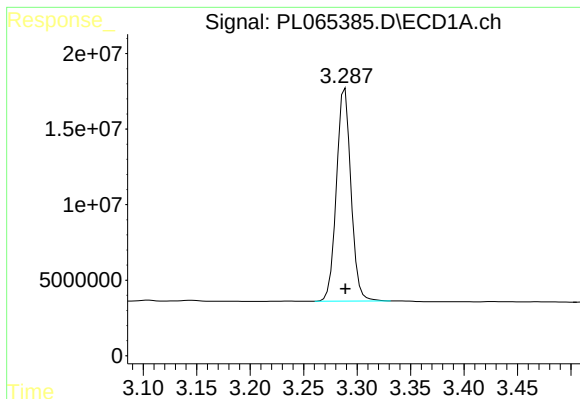

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 133269246
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

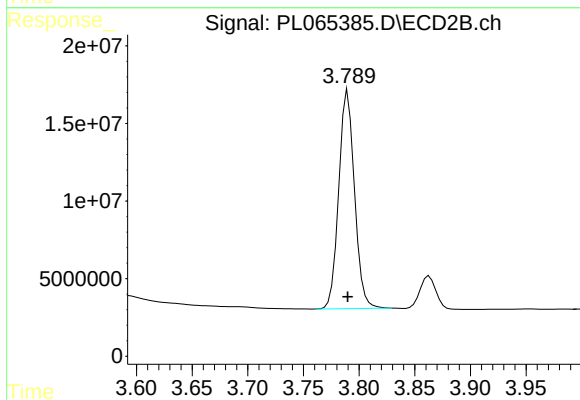


#1 Tetrachloro-m-xylene

R.T.: 3.790 min
Delta R.T.: 0.000 min
Response: 138598738
Conc: 50.00 ng/ml

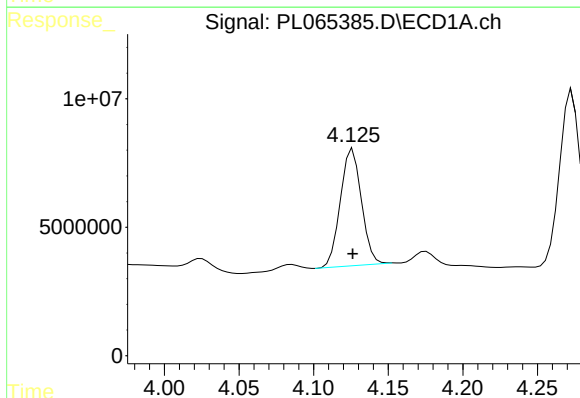


#23 Chlordane-1

R.T.: 4.126 min
Delta R.T.: 0.000 min
Response: 45113673
Conc: 500.00 ng/ml

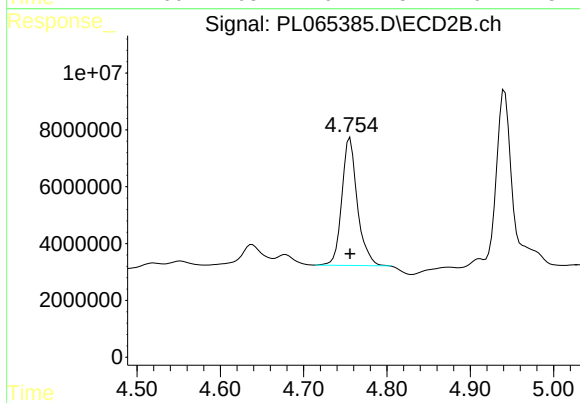

#23 Chlordane-1


R.T.: 4.756 min
Delta R.T.: 0.000 min
Response: 57896361
Conc: 500.00 ng/ml

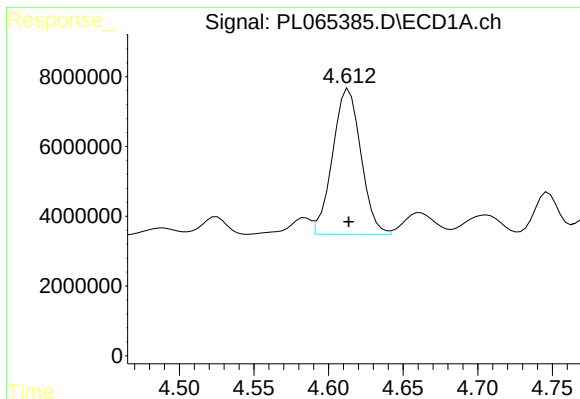

#24 Chlordane-2


R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 55241469
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

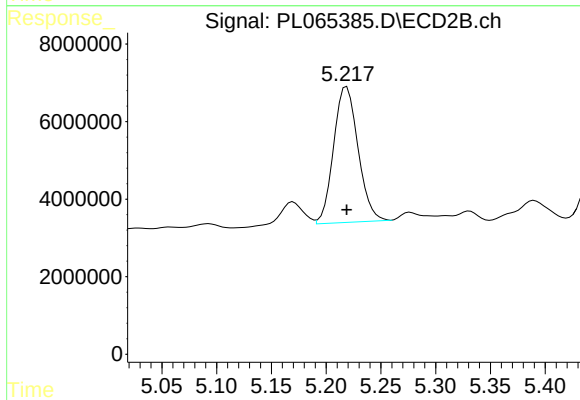


#24 Chlordane-2

R.T.: 5.219 min
Delta R.T.: 0.000 min
Response: 54258722
Conc: 500.00 ng/ml

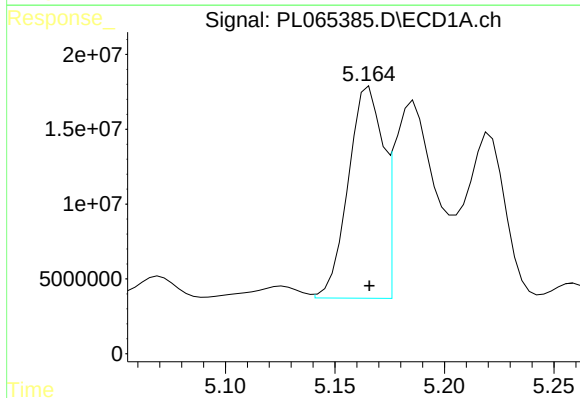


#25 Chlordane-3

R.T.: 5.166 min
Delta R.T.: 0.000 min
Response: 154853293
Conc: 500.00 ng/ml

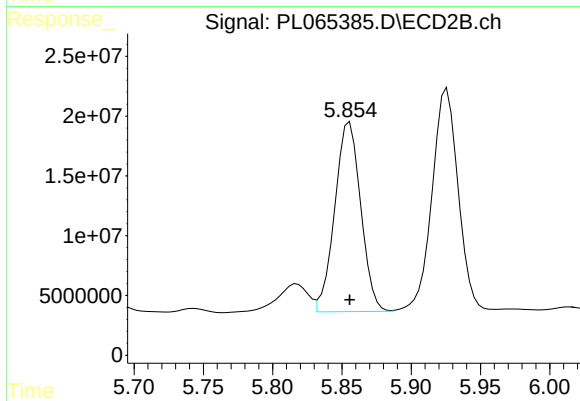

#25 Chlordane-3


R.T.: 5.856 min
Delta R.T.: 0.000 min
Response: 206647165
Conc: 500.00 ng/ml

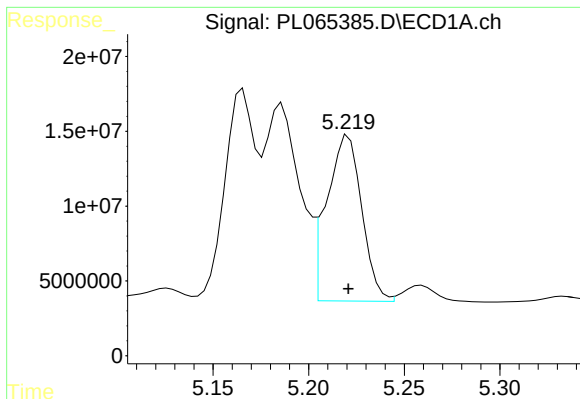

#26 Chlordane-4


R.T.: 5.221 min
Delta R.T.: 0.000 min
Response: 140949257
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

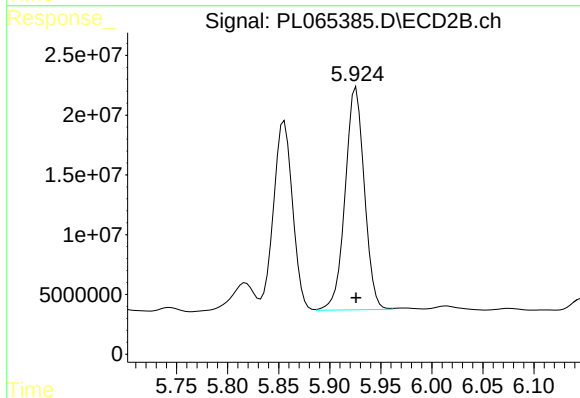


#26 Chlordane-4

R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 243333577
Conc: 500.00 ng/ml

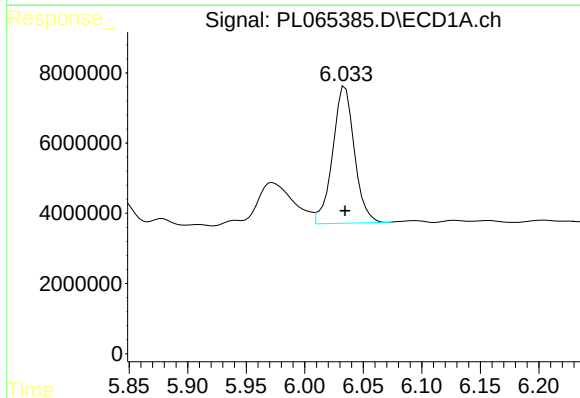


#27 Chlordane-5

R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 50296431
Conc: 500.00 ng/ml

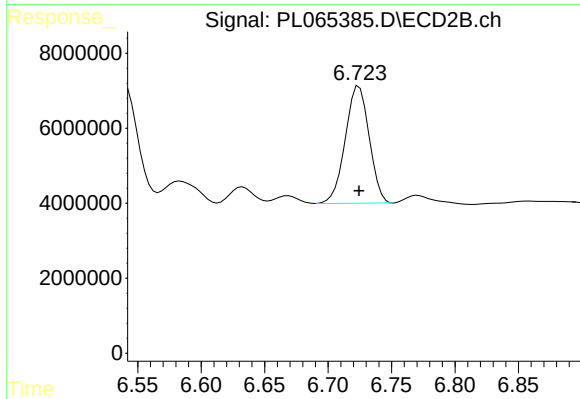

#27 Chlordane-5


R.T.: 6.724 min
Delta R.T.: 0.000 min
Response: 40957570
Conc: 500.00 ng/ml

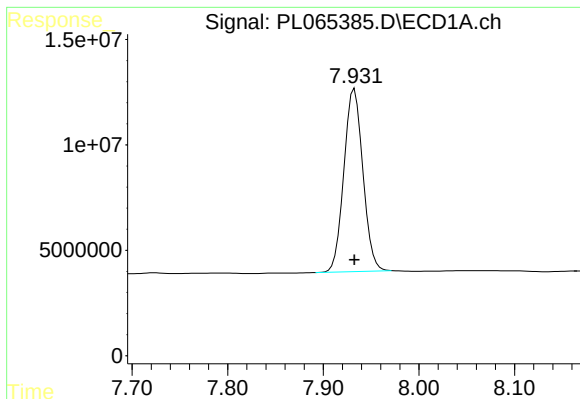

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.000 min
Response: 120029663
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

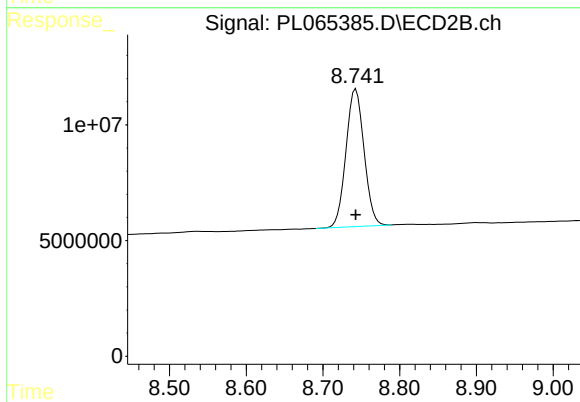

#28 Decachlorobiphenyl

R.T.: 8.743 min
Delta R.T.: 0.000 min
Response: 98208659
Conc: 50.00 ng/ml