

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
 Data File : PL065387.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2021 14:09
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:10:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:02:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.790	12082646	14419074	4.674	5.245
28)	SA Decachlor...	7.932	8.743	13374032	9899191	5.537	5.123
Target Compounds							
23)	Chlordane-1	4.126	4.755	4037937	5406790	46.871	47.937
24)	Chlordane-2	4.614	5.219	5625864	6082811	51.870	55.850
25)	Chlordane-3	5.165	5.855	14433974	20969282	48.376	51.442
26)	Chlordane-4	5.220	5.926	13333521	25164693	48.942	52.310
27)	Chlordane-5	6.033	6.724	5354060	3907532	53.553	48.833



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
Data File : PL065387.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2021 14:09
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:10:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:02:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

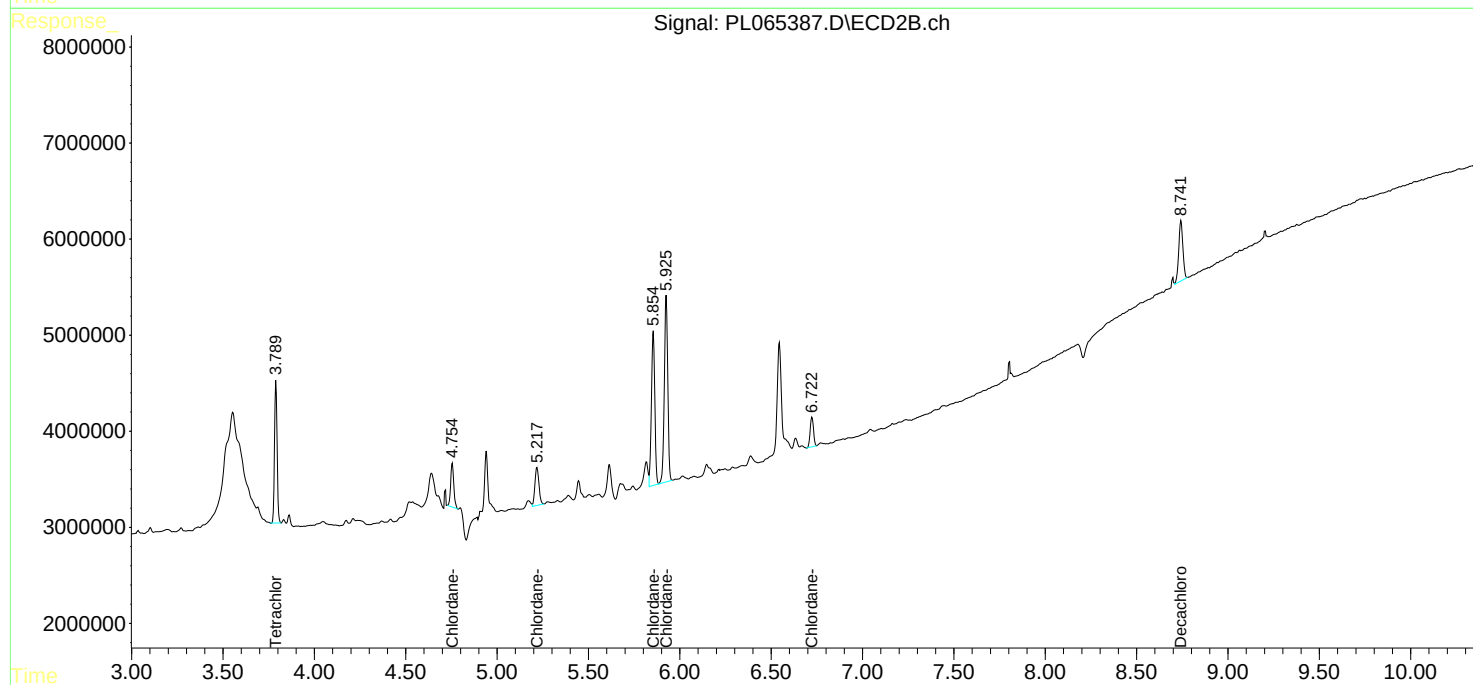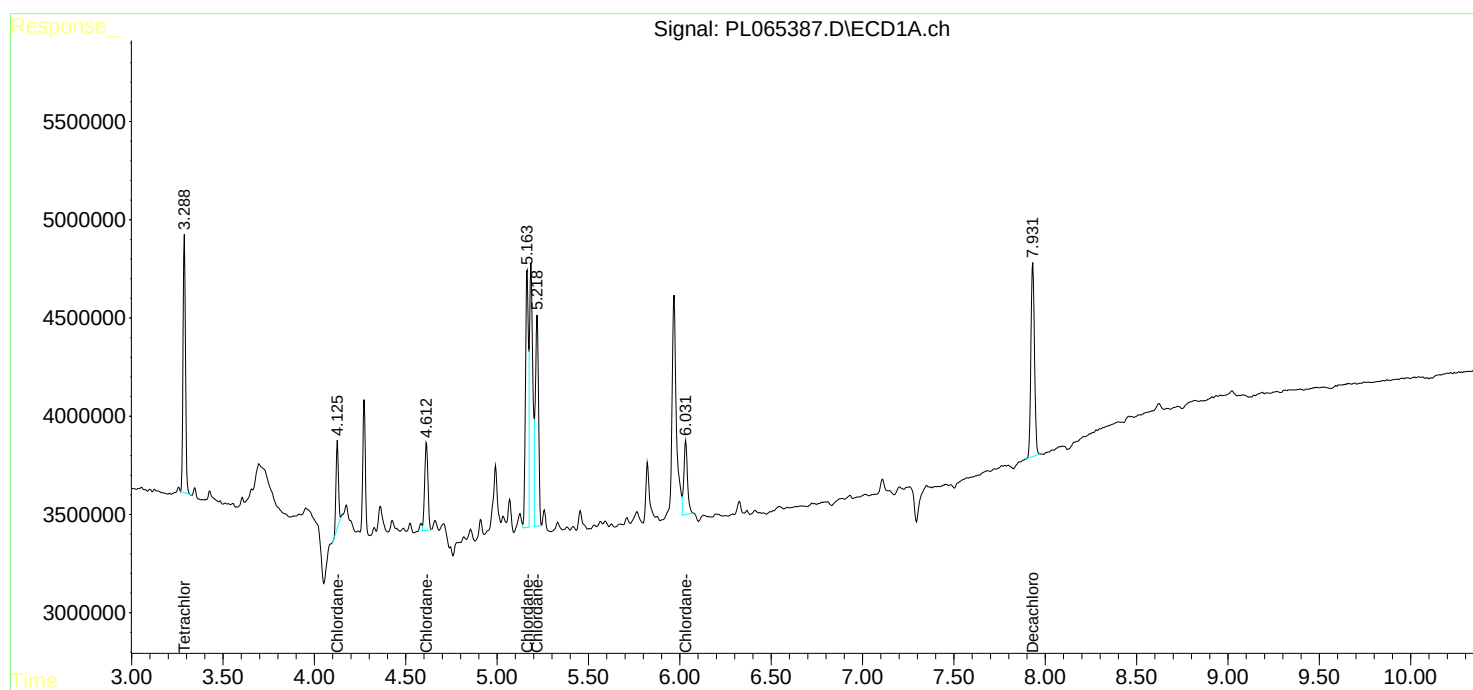


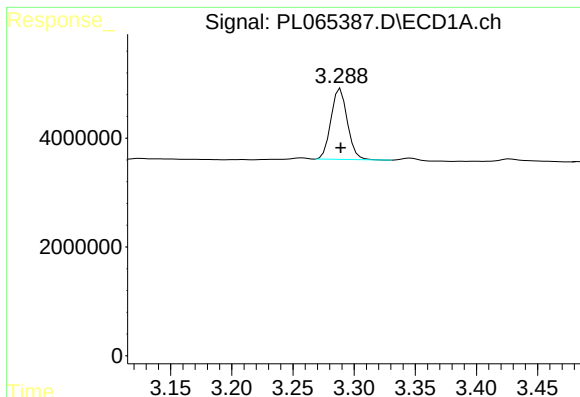

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 12082646
Conc: 4.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

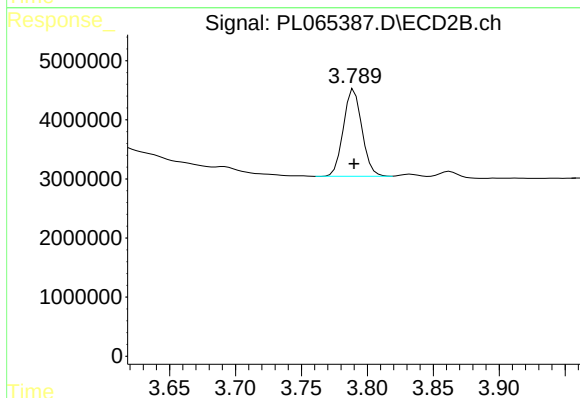


#1 Tetrachloro-m-xylene

R.T.: 3.790 min
Delta R.T.: 0.000 min
Response: 14419074
Conc: 5.25 ng/ml

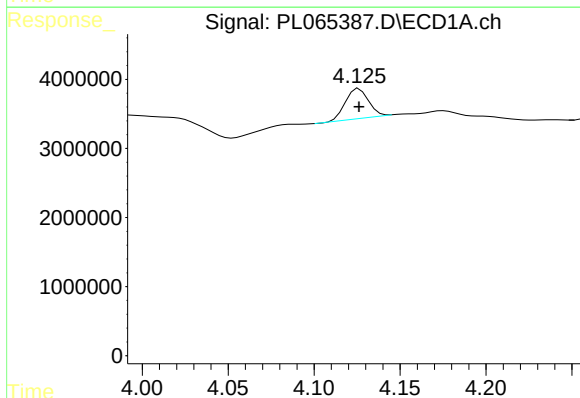


#23 Chlordane-1

R.T.: 4.126 min
Delta R.T.: 0.000 min
Response: 4037937
Conc: 46.87 ng/ml

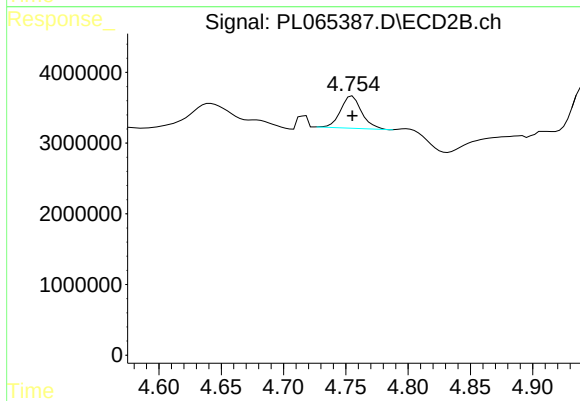

#23 Chlordane-1


R.T.: 4.755 min
Delta R.T.: 0.000 min
Response: 5406790
Conc: 47.94 ng/ml

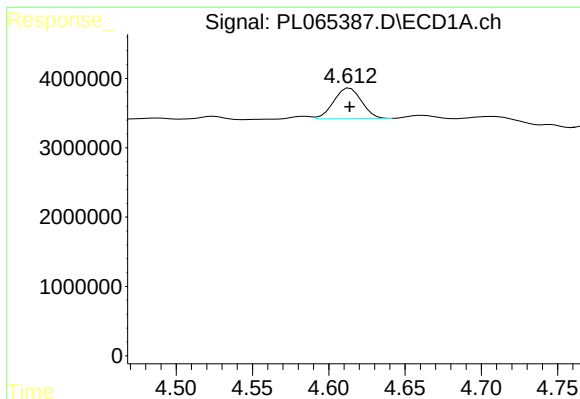

#24 Chlordane-2


R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 5625864
Conc: 51.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

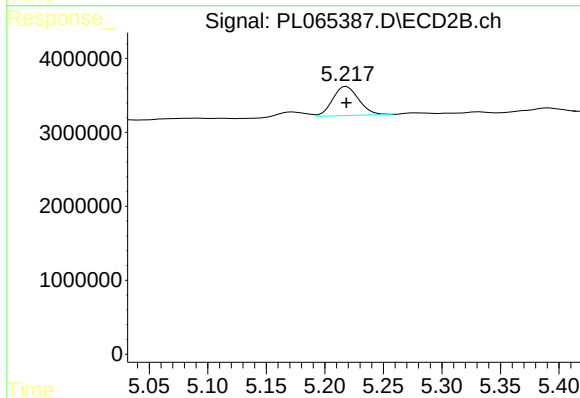


#24 Chlordane-2

R.T.: 5.219 min
Delta R.T.: 0.000 min
Response: 6082811
Conc: 55.85 ng/ml

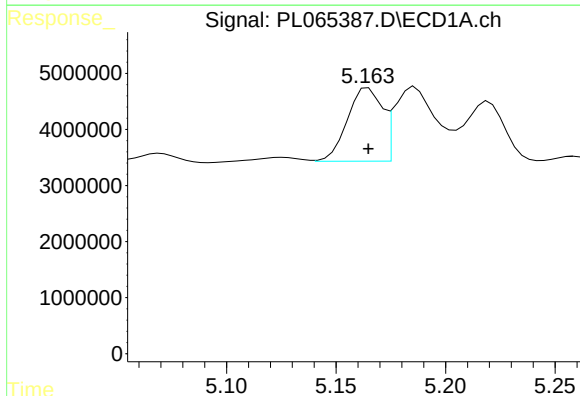


#25 Chlordane-3

R.T.: 5.165 min
Delta R.T.: 0.000 min
Response: 14433974
Conc: 48.38 ng/ml

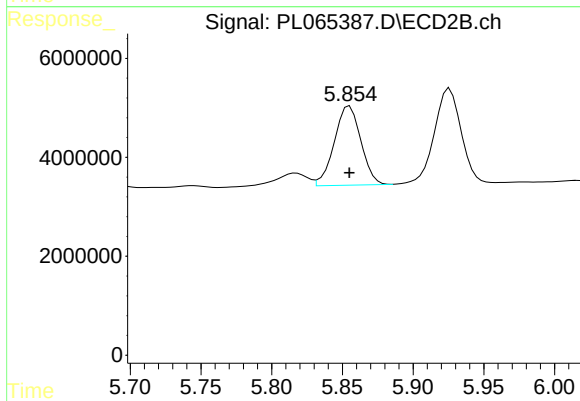

#25 Chlordane-3


R.T.: 5.855 min
Delta R.T.: 0.000 min
Response: 20969282
Conc: 51.44 ng/ml

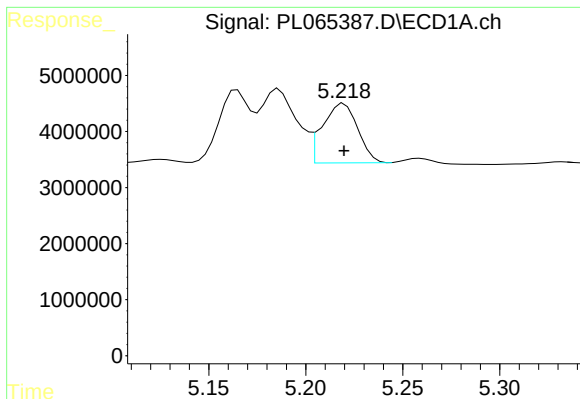

#26 Chlordane-4


R.T.: 5.220 min
Delta R.T.: 0.000 min
Response: 13333521
Conc: 48.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

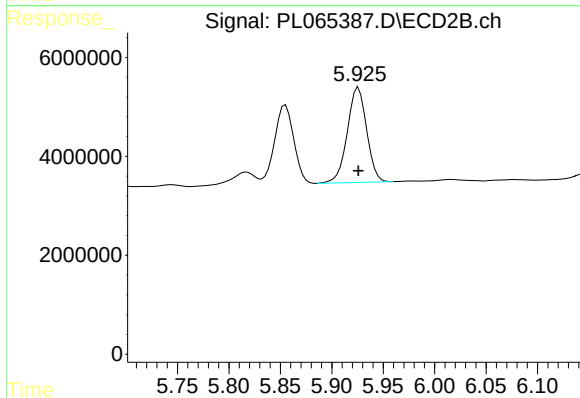


#26 Chlordane-4

R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 25164693
Conc: 52.31 ng/ml

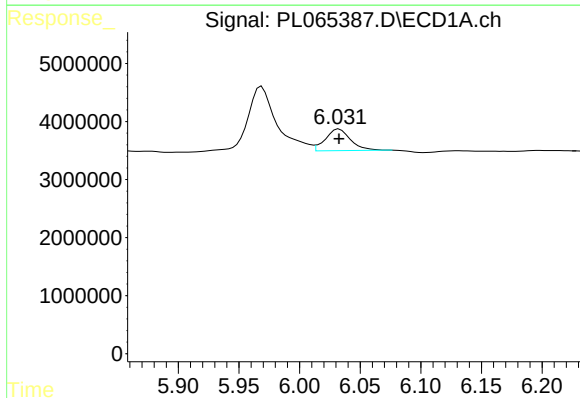


#27 Chlordane-5

R.T.: 6.033 min
Delta R.T.: 0.000 min
Response: 5354060
Conc: 53.55 ng/ml

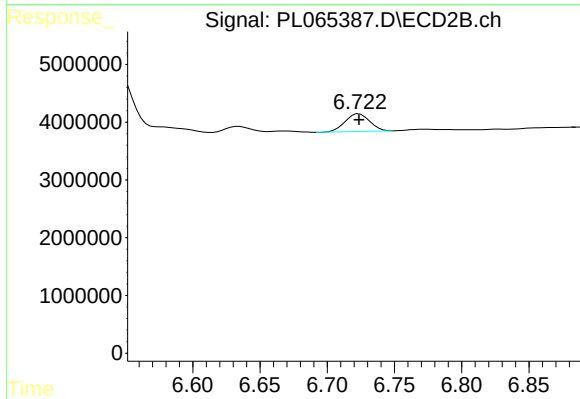

#27 Chlordane-5


R.T.: 6.724 min
Delta R.T.: 0.000 min
Response: 3907532
Conc: 48.83 ng/ml

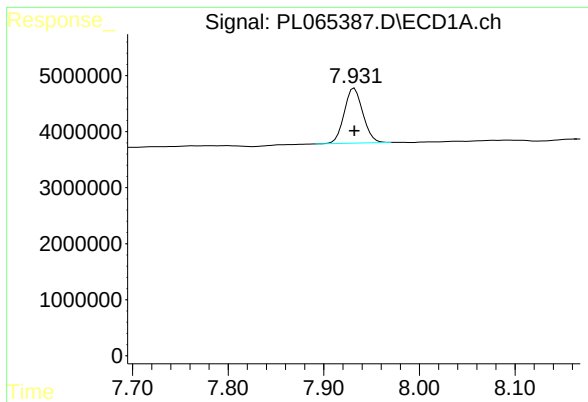

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: 0.000 min
Response: 13374032
Conc: 5.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

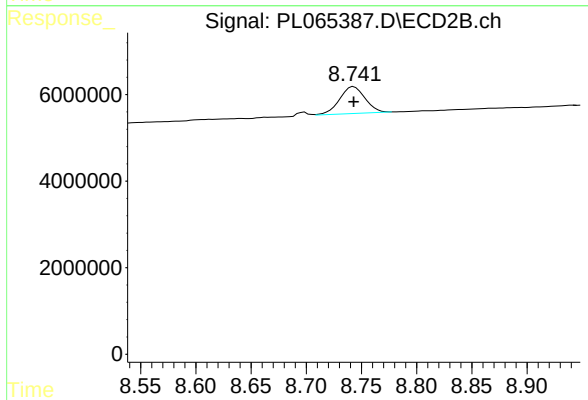

#28 Decachlorobiphenyl

R.T.: 8.743 min
Delta R.T.: 0.000 min
Response: 9899191
Conc: 5.12 ng/ml