

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
 Data File : PL065383.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2021 13:12
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:04:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:02:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.790	264.5E6	262.1E6	99.620	97.204
28)	SA Decachlor...	7.933	8.744	223.3E6	185.0E6	96.393	97.006
Target Compounds							
23)	Chlordane-1	4.126	4.756	85960882	109.1E6	975.785	970.076
24)	Chlordane-2	4.614	5.219	101.7E6	99799228	958.605	958.149
25)	Chlordane-3	5.165	5.856	295.3E6	399.2E6	976.139	982.644
26)	Chlordane-4	5.221	5.926	271.0E6	466.4E6	980.300	978.768
27)	Chlordane-5	6.034	6.724	97636827	79632480	985.088	985.870



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
Data File : PL065383.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2021 13:12
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:04:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:02:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

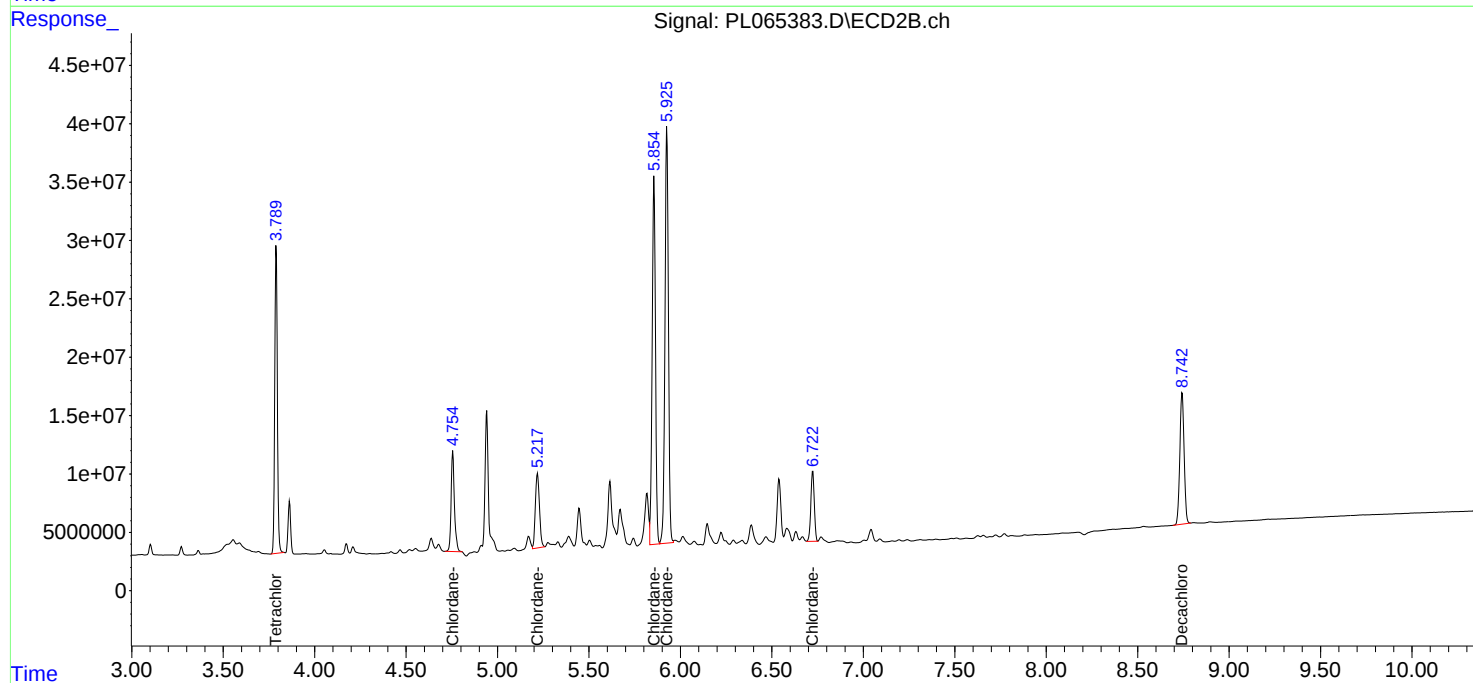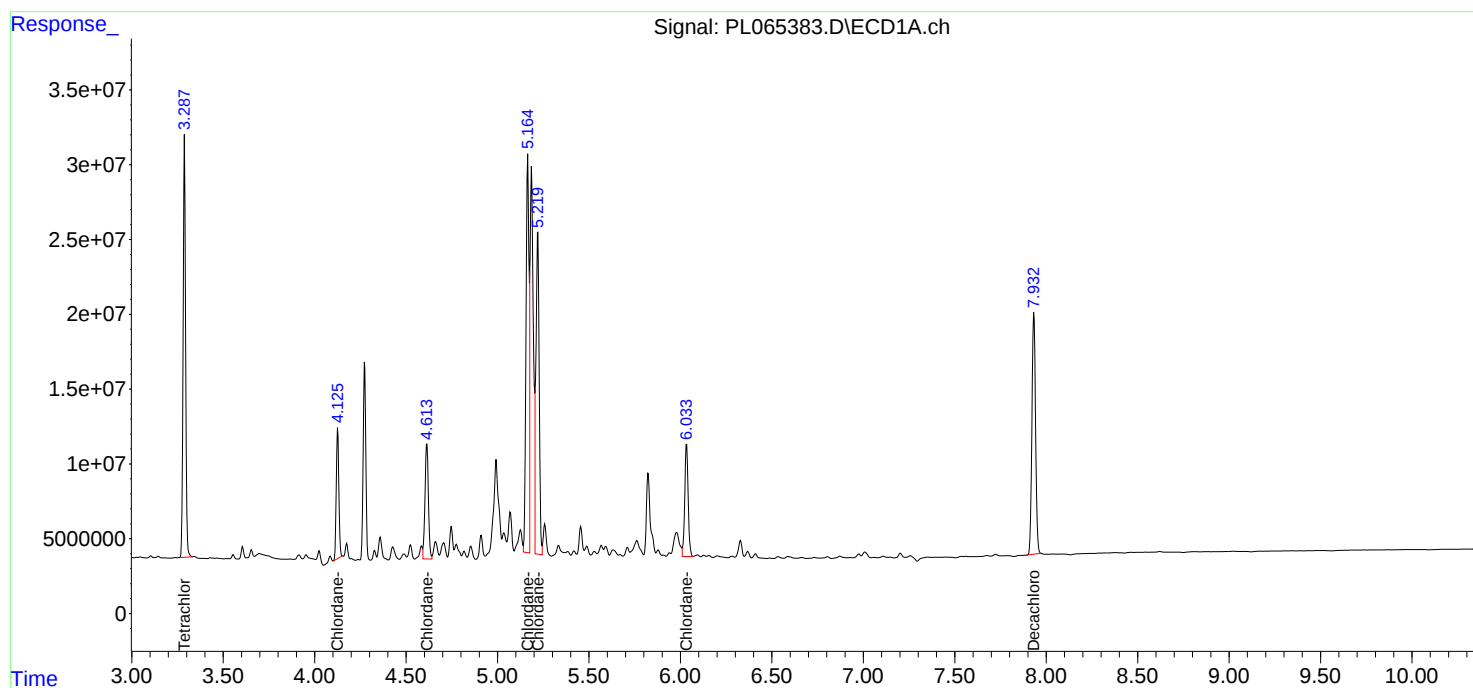


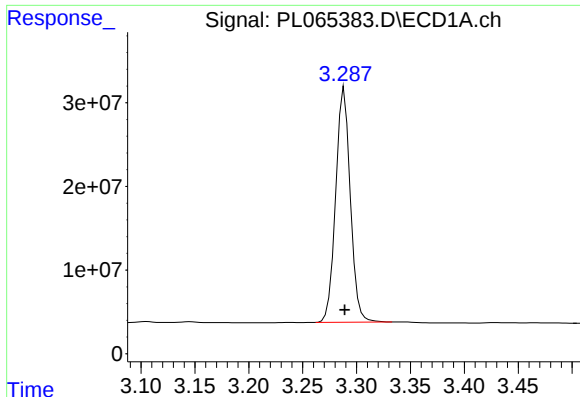

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 264518854
Conc: 99.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

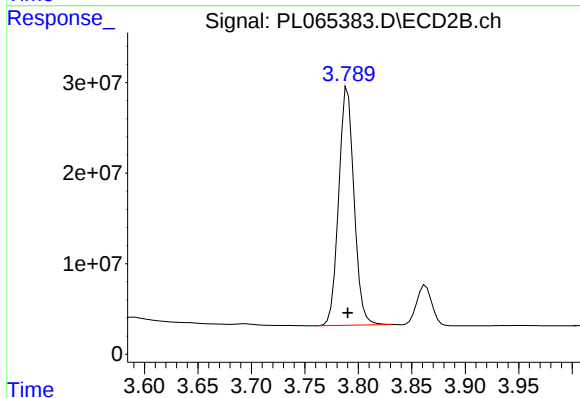


#1 Tetrachloro-m-xylene

R.T.: 3.790 min
Delta R.T.: 0.000 min
Response: 262117237
Conc: 97.20 ng/ml

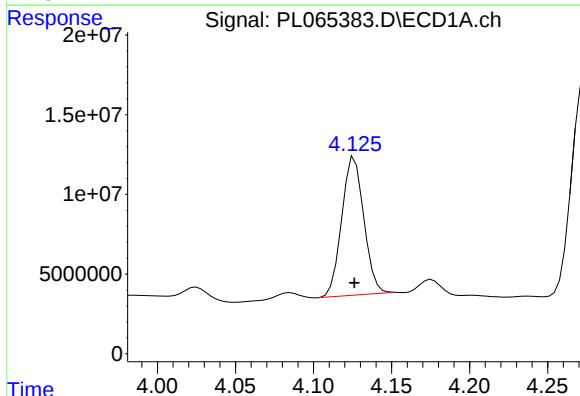


#23 Chlordane-1

R.T.: 4.126 min
Delta R.T.: 0.000 min
Response: 85960882
Conc: 975.78 ng/ml

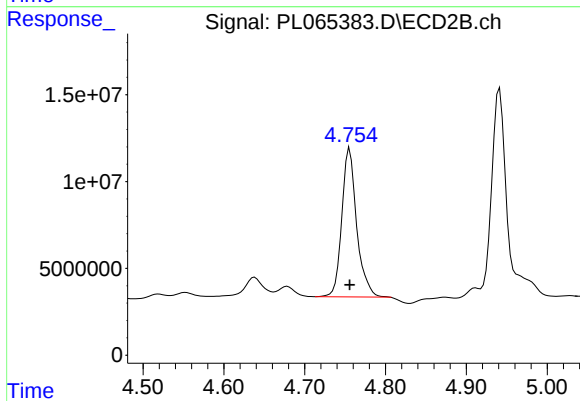

#23 Chlordane-1


R.T.: 4.756 min
Delta R.T.: 0.000 min
Response: 109064058
Conc: 970.08 ng/ml

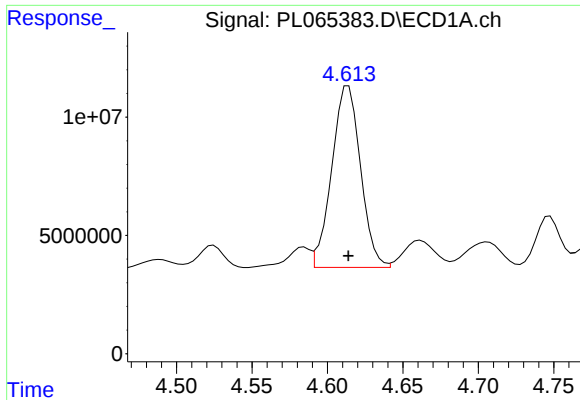

#24 Chlordane-2


R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 101699674
Conc: 958.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

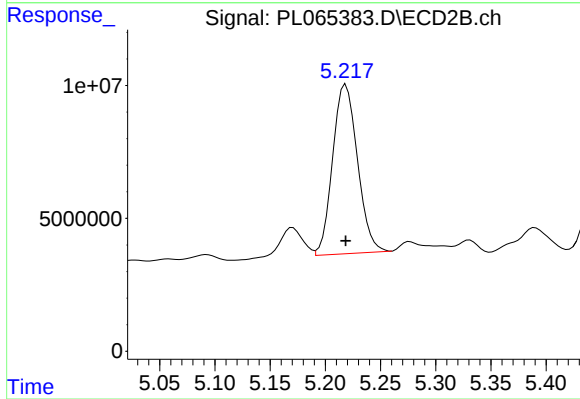


#24 Chlordane-2

R.T.: 5.219 min
Delta R.T.: 0.000 min
Response: 99799228
Conc: 958.15 ng/ml

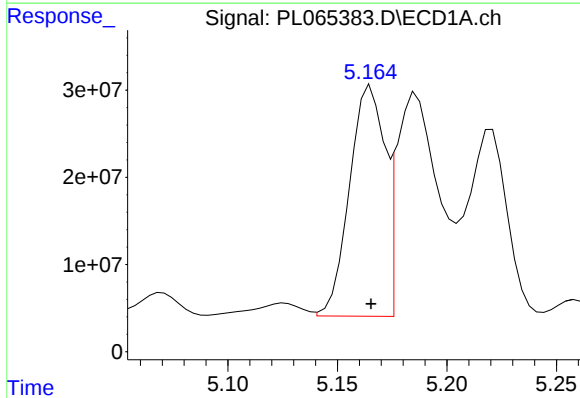


#25 Chlordane-3

R.T.: 5.165 min
Delta R.T.: 0.000 min
Response: 295271043
Conc: 976.14 ng/ml

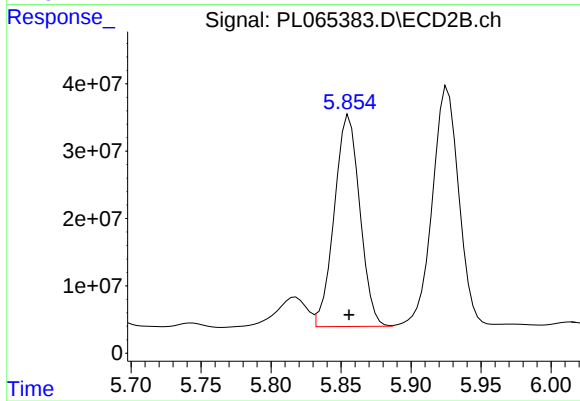

#25 Chlordane-3


R.T.: 5.856 min
Delta R.T.: 0.000 min
Response: 399192669
Conc: 982.64 ng/ml

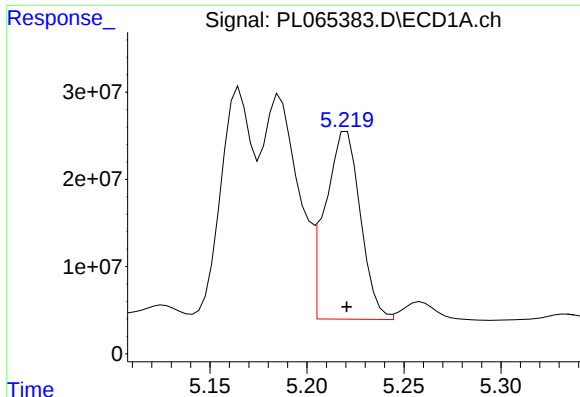

#26 Chlordane-4


R.T.: 5.221 min
Delta R.T.: 0.000 min
Response: 271006197
Conc: 980.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

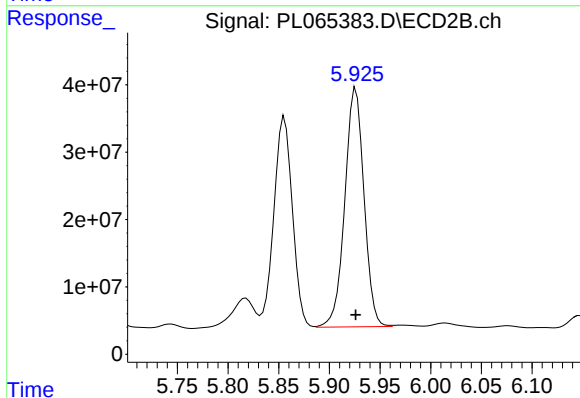


#26 Chlordane-4

R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 466430624
Conc: 978.77 ng/ml

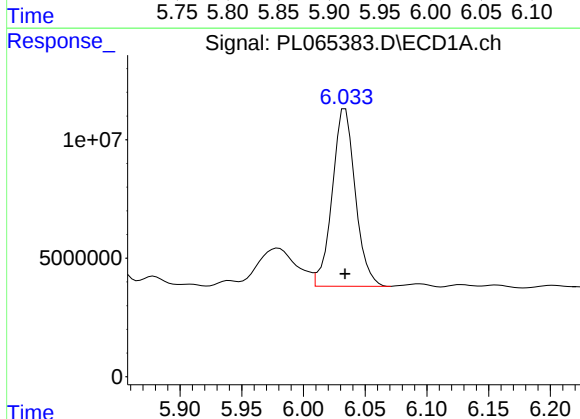


#27 Chlordane-5

R.T.: 6.034 min
Delta R.T.: 0.000 min
Response: 97636827
Conc: 985.09 ng/ml

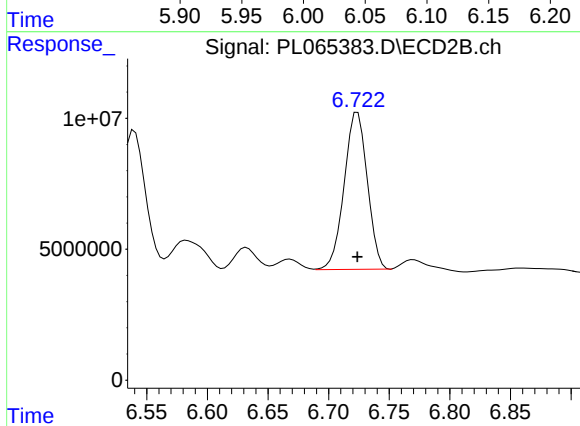

#27 Chlordane-5


R.T.: 6.724 min
Delta R.T.: 0.000 min
Response: 79632480
Conc: 985.87 ng/ml

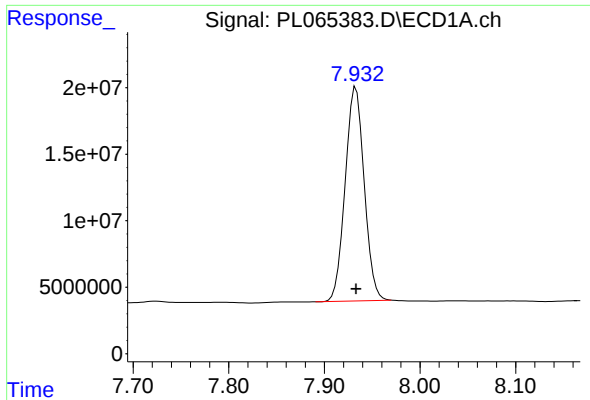

#28 Decachlorobiphenyl

R.T.: 7.933 min
Delta R.T.: 0.000 min
Response: 223343266
Conc: 96.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

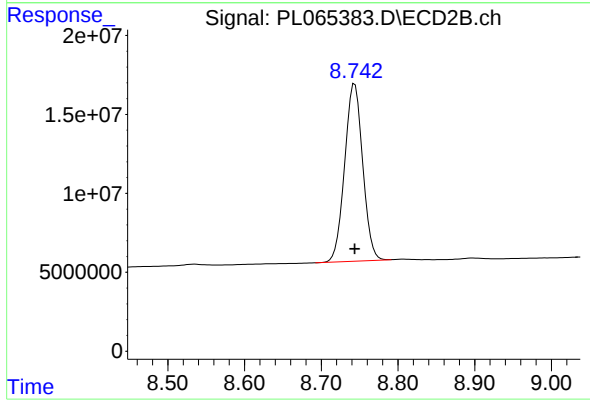

#28 Decachlorobiphenyl

R.T.: 8.744 min
Delta R.T.: 0.000 min
Response: 184996651
Conc: 97.01 ng/ml