

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
 Data File : PL065386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2021 13:55
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:08:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:02:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.790	63061237	69285934	24.000	25.517
28)	SA Decachlor...	7.932	8.743	61620931	49419831	26.218	25.731
Target Compounds							
23)	Chlordane-1	4.126	4.756	21289364	29687082	243.314	260.517
24)	Chlordane-2	4.614	5.218	27990860	27759763	260.509	262.560
25)	Chlordane-3	5.165	5.855	73978381	100.3E6	245.944	247.901
26)	Chlordane-4	5.220	5.926	67993206	118.7E6	248.263	249.590
27)	Chlordane-5	6.034	6.724	24540918	19939296	249.904	247.738



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
Data File : PL065386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2021 13:55
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:08:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:02:00 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

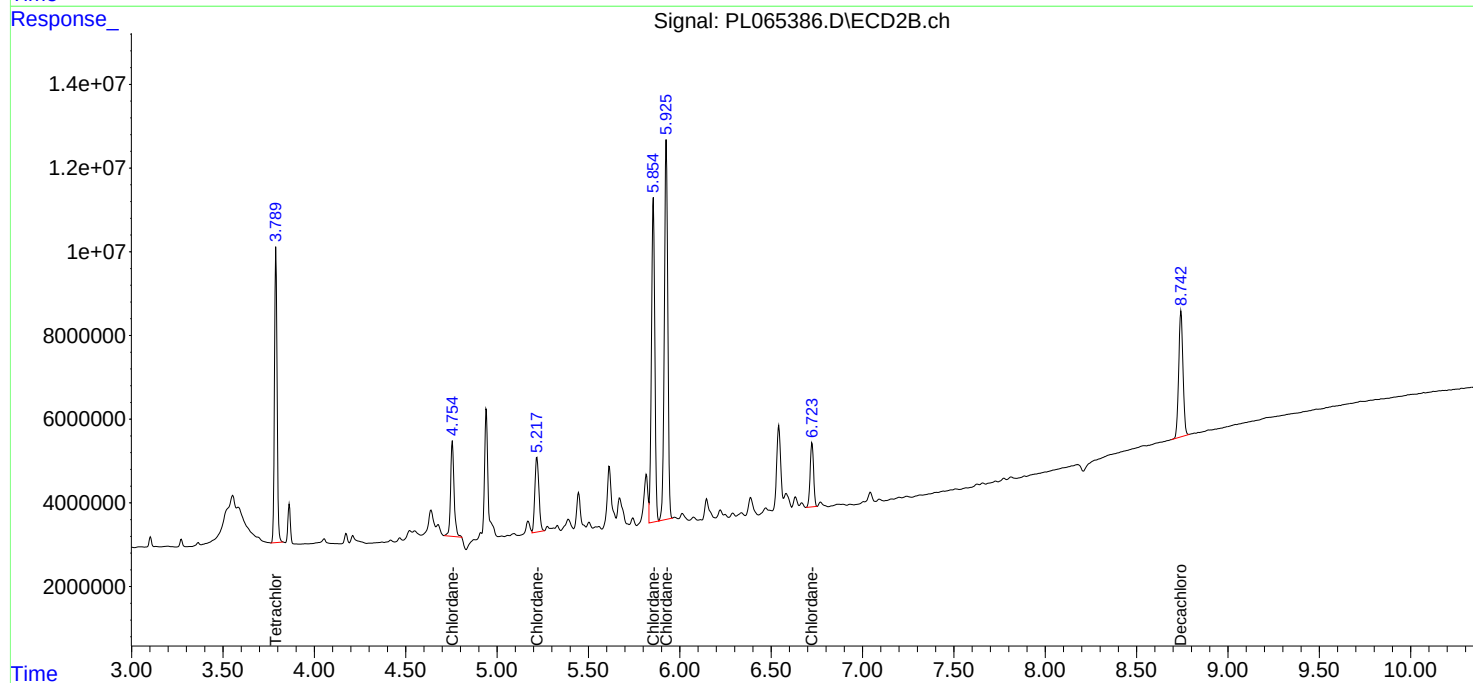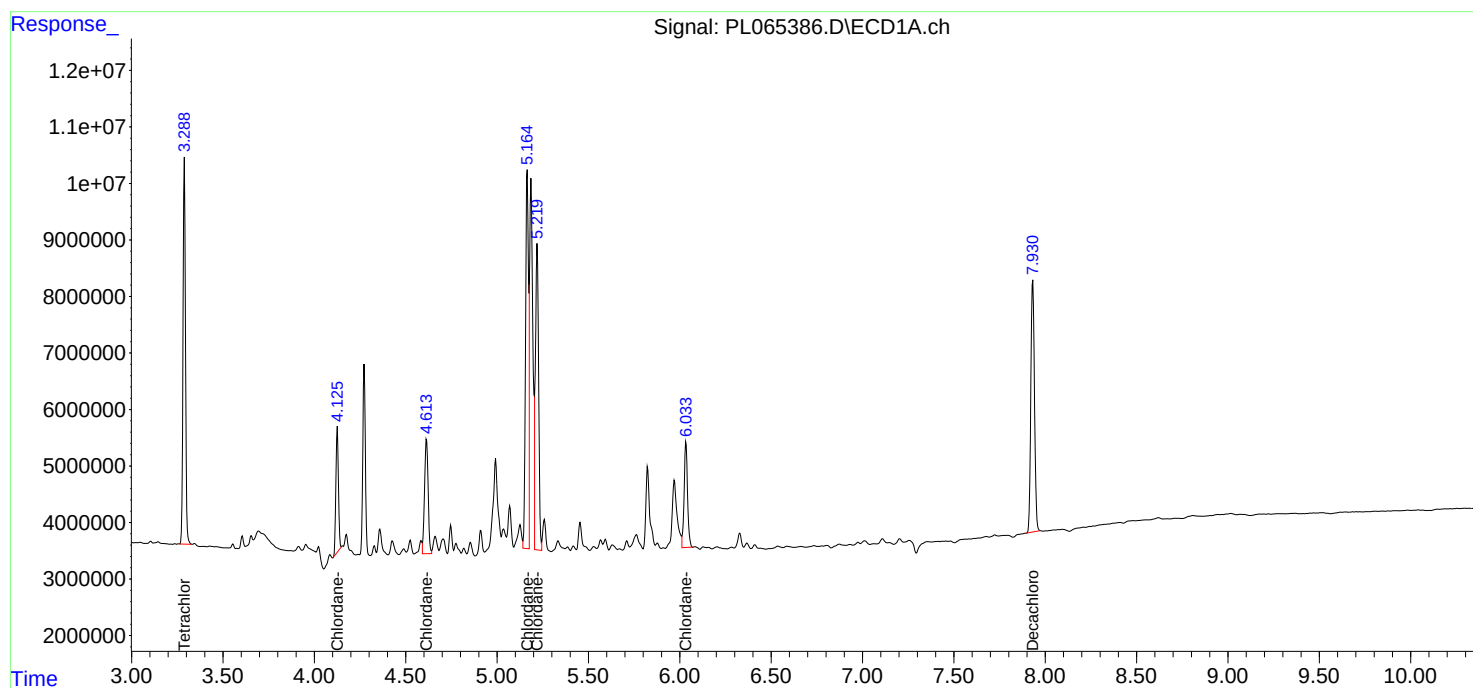


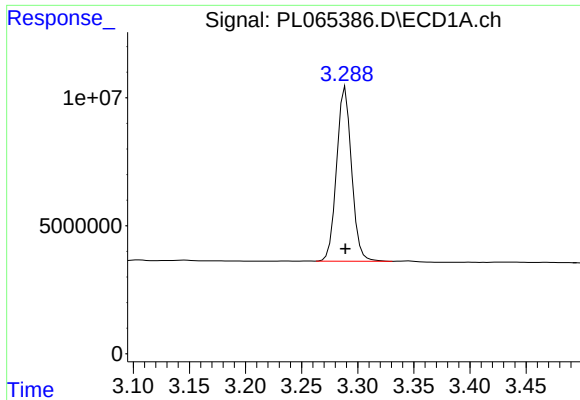

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 63061237
Conc: 24.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

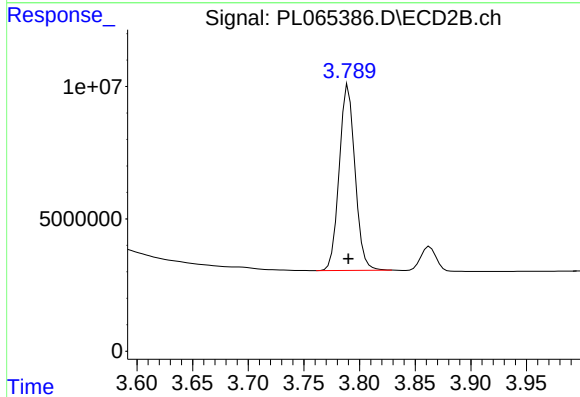


#1 Tetrachloro-m-xylene

R.T.: 3.790 min
Delta R.T.: 0.000 min
Response: 69285934
Conc: 25.52 ng/ml

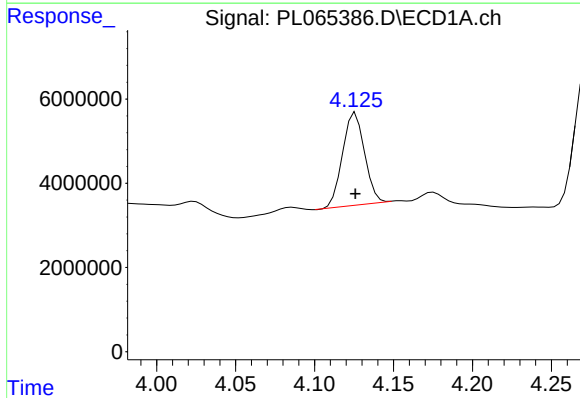


#23 Chlordane-1

R.T.: 4.126 min
Delta R.T.: 0.000 min
Response: 21289364
Conc: 243.31 ng/ml

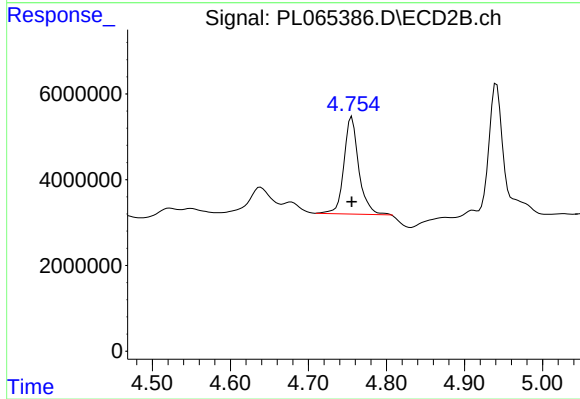

#23 Chlordane-1


R.T.: 4.756 min
Delta R.T.: 0.000 min
Response: 29687082
Conc: 260.52 ng/ml

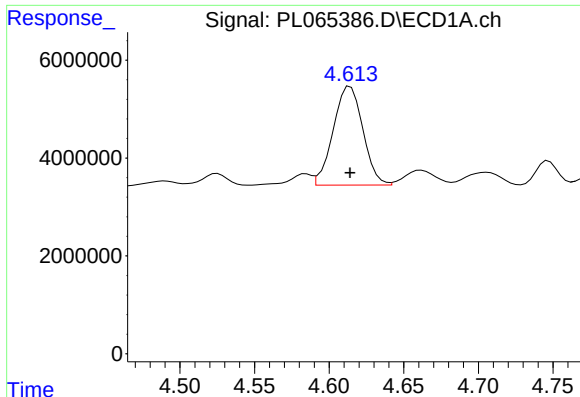

#24 Chlordane-2


R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 27990860
Conc: 260.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

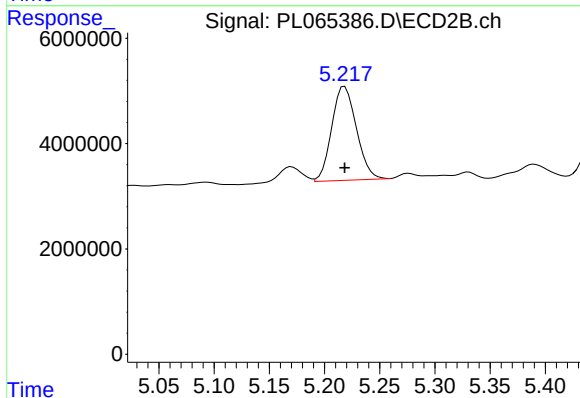


#24 Chlordane-2

R.T.: 5.218 min
Delta R.T.: 0.000 min
Response: 27759763
Conc: 262.56 ng/ml

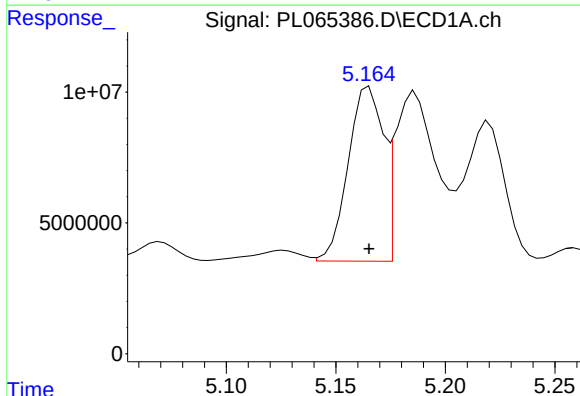


#25 Chlordane-3

R.T.: 5.165 min
Delta R.T.: 0.000 min
Response: 73978381
Conc: 245.94 ng/ml

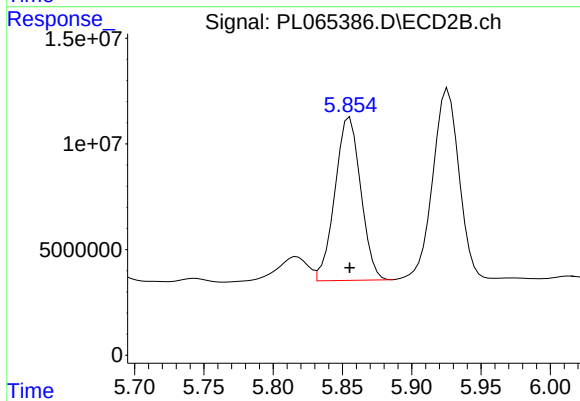

#25 Chlordane-3


R.T.: 5.855 min
Delta R.T.: 0.000 min
Response: 100322318
Conc: 247.90 ng/ml

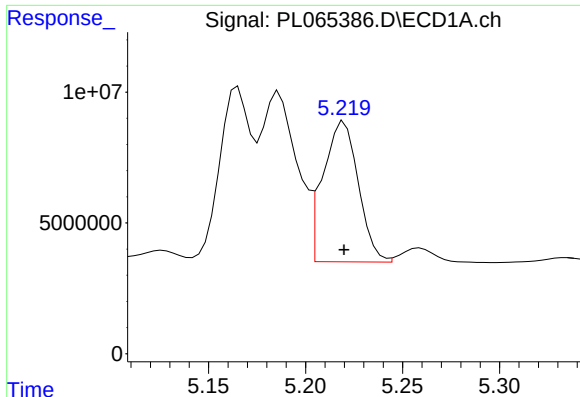

#26 Chlordane-4


R.T.: 5.220 min
Delta R.T.: 0.000 min
Response: 67993206
Conc: 248.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

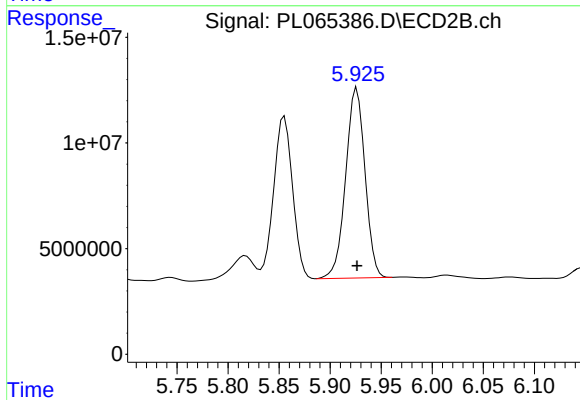


#26 Chlordane-4

R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 118684420
Conc: 249.59 ng/ml

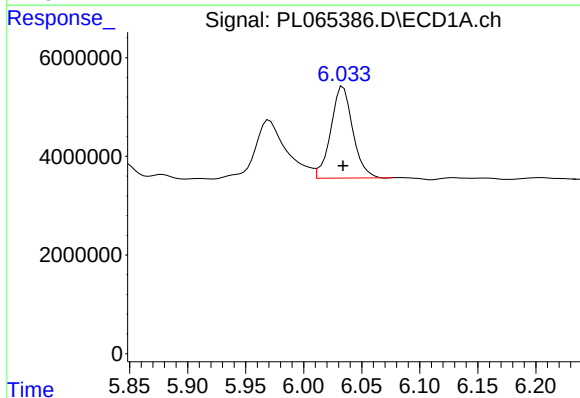


#27 Chlordane-5

R.T.: 6.034 min
Delta R.T.: 0.000 min
Response: 24540918
Conc: 249.90 ng/ml

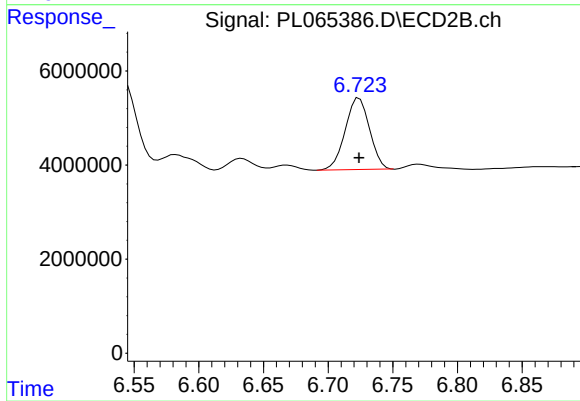

#27 Chlordane-5


R.T.: 6.724 min
Delta R.T.: 0.000 min
Response: 19939296
Conc: 247.74 ng/ml

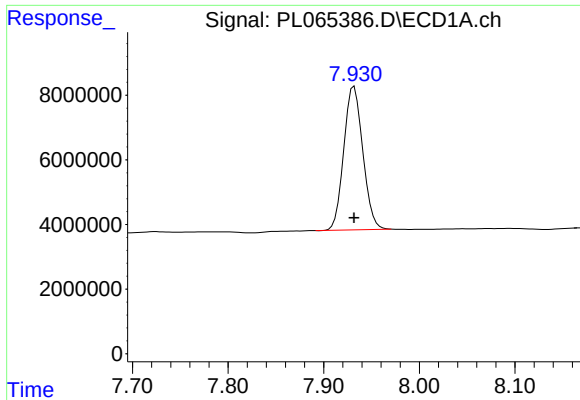

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: 0.000 min
Response: 61620931
Conc: 26.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

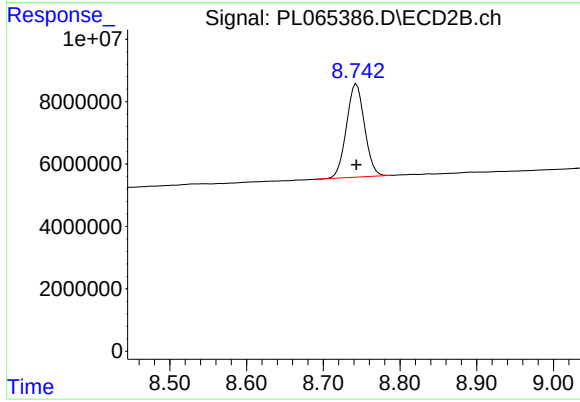

#28 Decachlorobiphenyl

R.T.: 8.743 min
Delta R.T.: 0.000 min
Response: 49419831
Conc: 25.73 ng/ml