

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
 Data File : PL065394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2021 16:04
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL031821

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 02:11:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:11:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.289	3.790	135.6E6	139.2E6	52.465	50.649
28)	SA Decachlor...	7.932	8.744	122.4E6	100.6E6	50.690	52.048
Target Compounds							
23)	Chlordane-1	4.126	4.756	46402406	60200798	538.626	533.739
24)	Chlordane-2	4.614	5.219	56460041	56196289	520.556	515.974
25)	Chlordane-3	5.165	5.856	156.8E6	216.1E6	525.496	530.182
26)	Chlordane-4	5.220	5.926	140.4E6	251.2E6	515.505	522.246
27)	Chlordane-5	6.034	6.724	51480328	45289095	514.919	565.984



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
Data File : PL065394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2021 16:04
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL031821

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 02:11:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:11:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

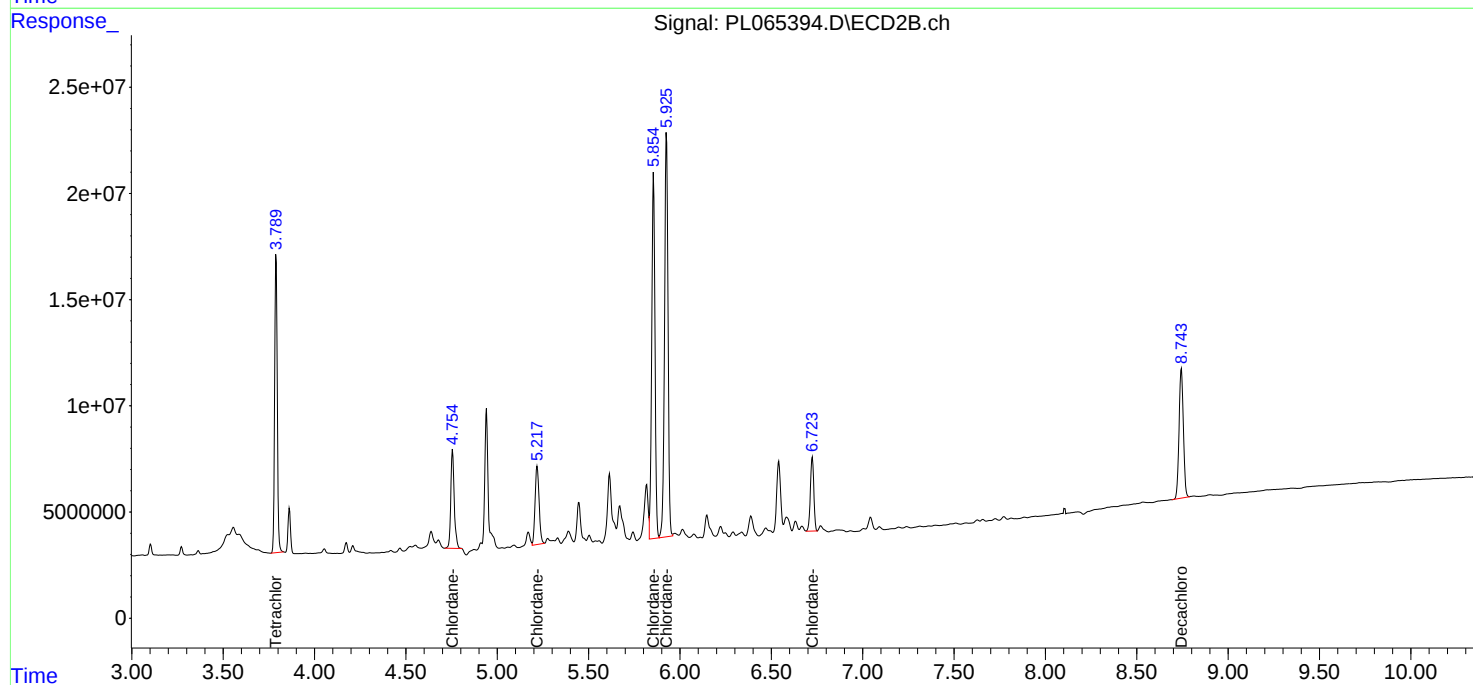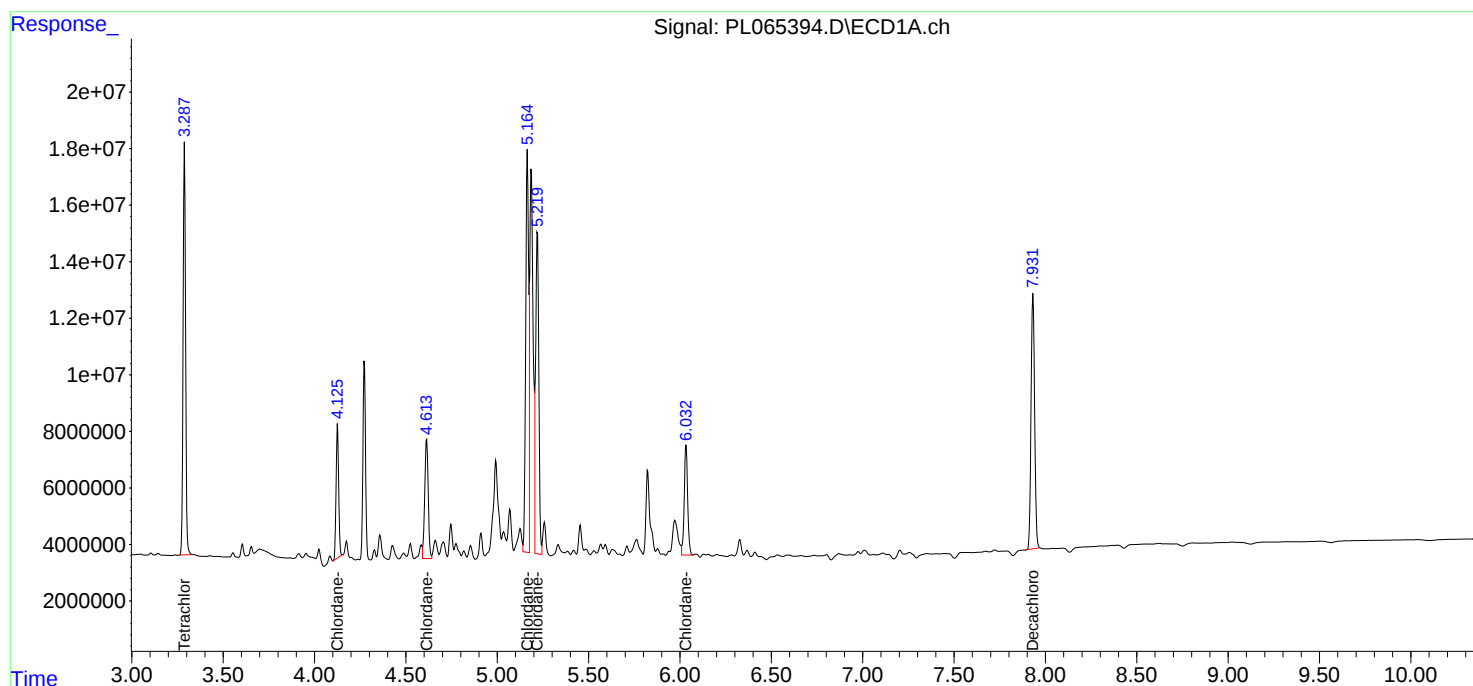


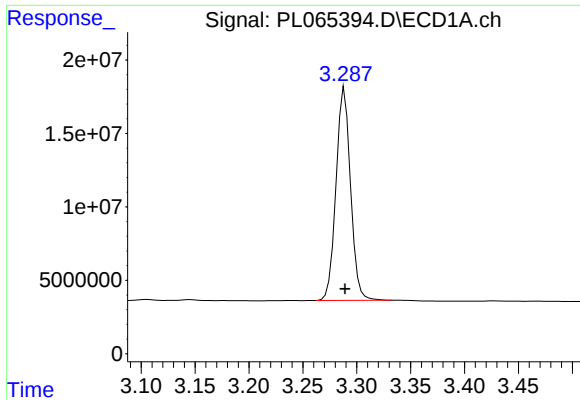

#1 Tetrachloro-m-xylene


R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 135640586
Conc: 52.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL031821

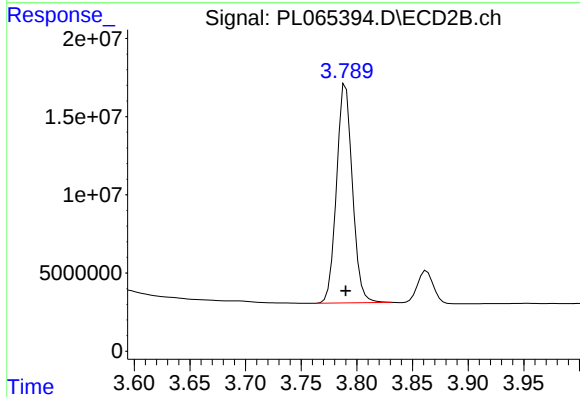


#1 Tetrachloro-m-xylene

R.T.: 3.790 min
Delta R.T.: 0.000 min
Response: 139234298
Conc: 50.65 ng/ml

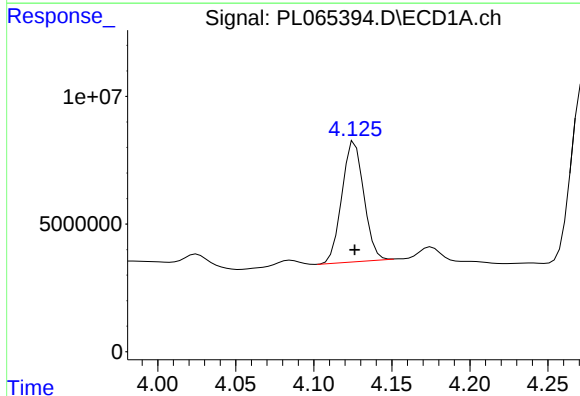


#23 Chlordane-1

R.T.: 4.126 min
Delta R.T.: 0.000 min
Response: 46402406
Conc: 538.63 ng/ml

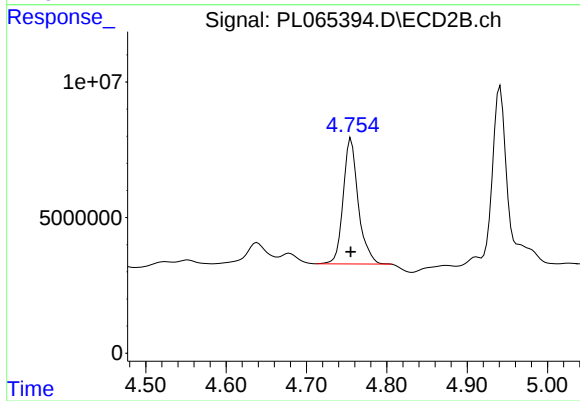

#23 Chlordane-1


R.T.: 4.756 min
Delta R.T.: 0.000 min
Response: 60200798
Conc: 533.74 ng/ml

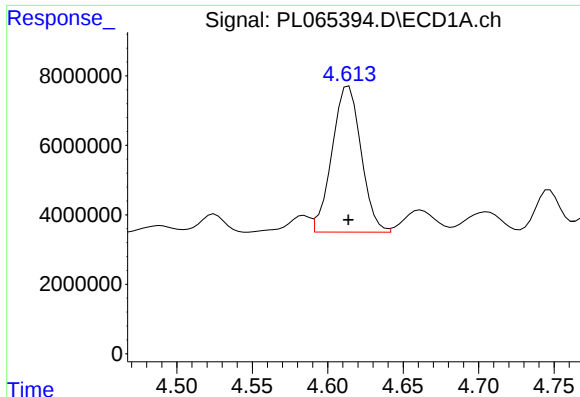

#24 Chlordane-2


R.T.: 4.614 min
Delta R.T.: 0.000 min
Response: 56460041
Conc: 520.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL031821

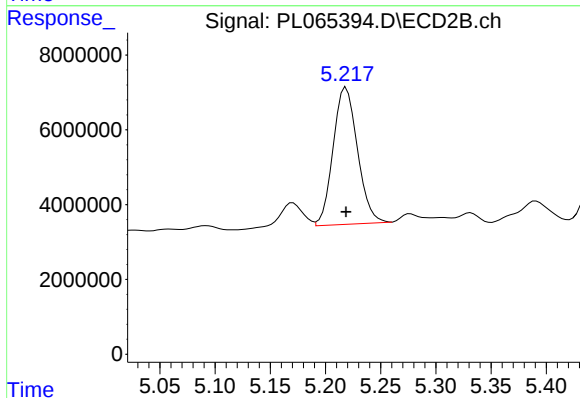


#24 Chlordane-2

R.T.: 5.219 min
Delta R.T.: 0.000 min
Response: 56196289
Conc: 515.97 ng/ml

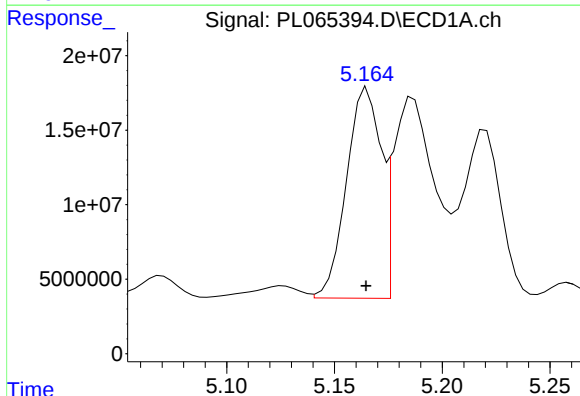


#25 Chlordane-3

R.T.: 5.165 min
Delta R.T.: 0.000 min
Response: 156792663
Conc: 525.50 ng/ml

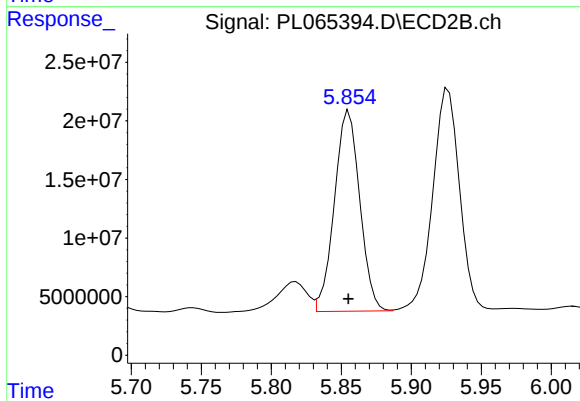

#25 Chlordane-3


R.T.: 5.856 min
Delta R.T.: 0.000 min
Response: 216116315
Conc: 530.18 ng/ml

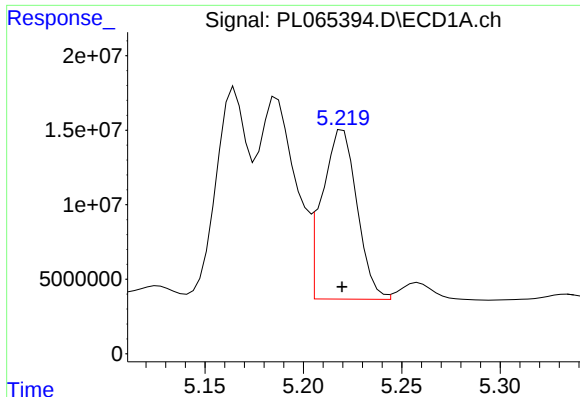

#26 Chlordane-4


R.T.: 5.220 min
Delta R.T.: 0.000 min
Response: 140441395
Conc: 515.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL031821

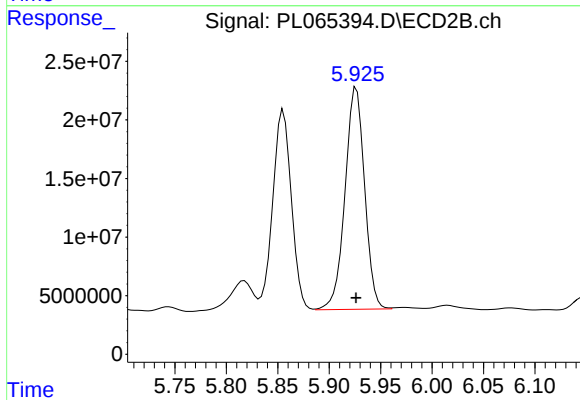


#26 Chlordane-4

R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 251237844
Conc: 522.25 ng/ml

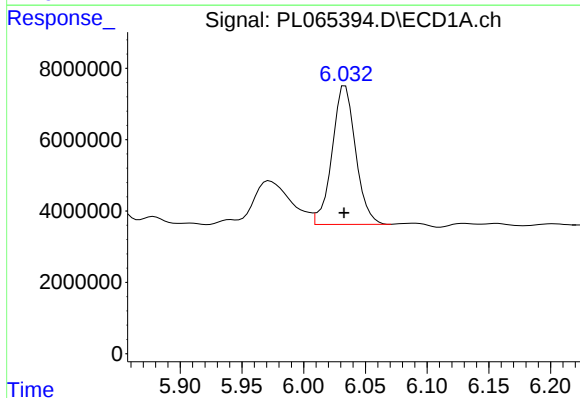


#27 Chlordane-5

R.T.: 6.034 min
Delta R.T.: 0.001 min
Response: 51480328
Conc: 514.92 ng/ml

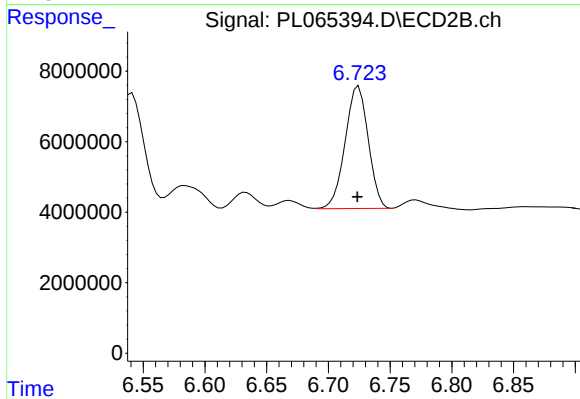

#27 Chlordane-5


R.T.: 6.724 min
Delta R.T.: 0.000 min
Response: 45289095
Conc: 565.98 ng/ml

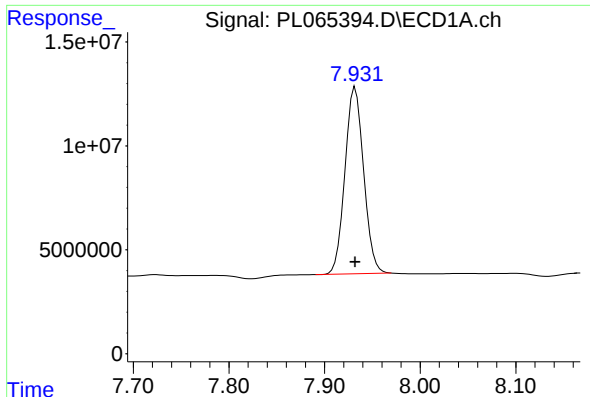

#28 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: 0.000 min
Response: 122428045
Conc: 50.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL031821

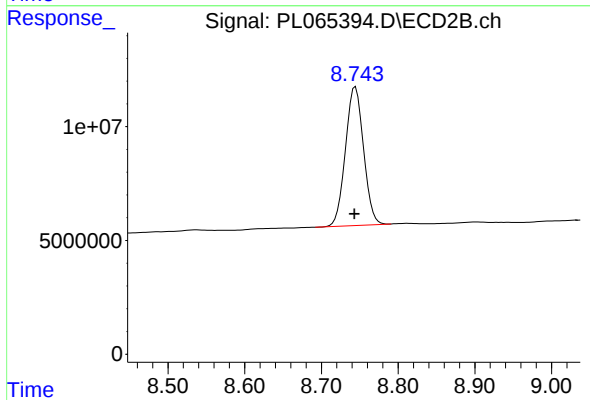

#28 Decachlorobiphenyl

R.T.: 8.744 min
Delta R.T.: 0.001 min
Response: 100581348
Conc: 52.05 ng/ml