

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
 Data File : PL065400.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2021 17:44
 Operator : AR\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PTOXCCC500

Manual Integrations
 APPROVED

Ankita
 3/19/2021 1:09:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 06:56:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\LTX031821.M
 Quant Title : GC Extractables
 QLast Update : Thu Mar 18 15:48:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticide 1 Signal #2 Phase: Rtx-CLPesticide 1
 Signal #1 Info : 30M x 0.32mm x0.3 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.289	3.789	119.8E6	123.1E6	50.136	44.716
7) SA Decachlor...	7.932	8.743	116.8E6	96848913	49.085	48.138
Target Compounds						
2) Toxaphene-1	5.475	6.132	7927803	7405703	506.865	456.801
3) Toxaphene-2	5.626	6.821	7197943	8952073	456.888	456.347
4) Toxaphene-3	6.301	6.900	19817152	17607193	500.948	471.469
5) Toxaphene-4	6.650	6.981	14428977	15042038	518.943	465.751m
6) Toxaphene-5	6.778	7.398	23477210	14591772	500.185	488.557

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031821\
Data File : PL065400.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2021 17:44
Operator : AR\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
PTOXCCC500


Manual Integrations
APPROVED

Ankita
3/19/2021 1:09:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 06:56:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\LTX031821.M
Quant Title : GC Extractables
QLast Update : Thu Mar 18 15:48:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticide 1 Signal #2 Phase: Rtx-CLPesticide 1
Signal #1 Info : 30M x 0.32mm x0.3 Signal #2 Info : 30M x 0.32mm x 0.25µm

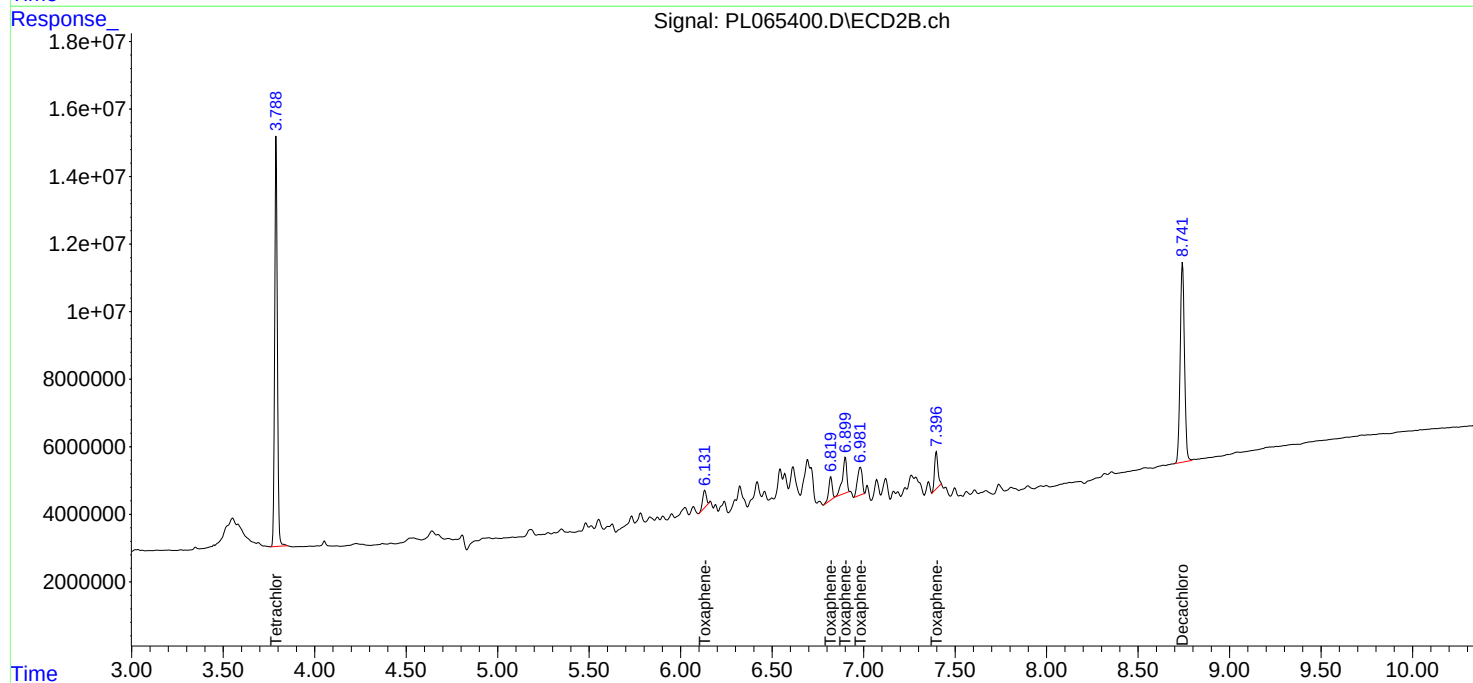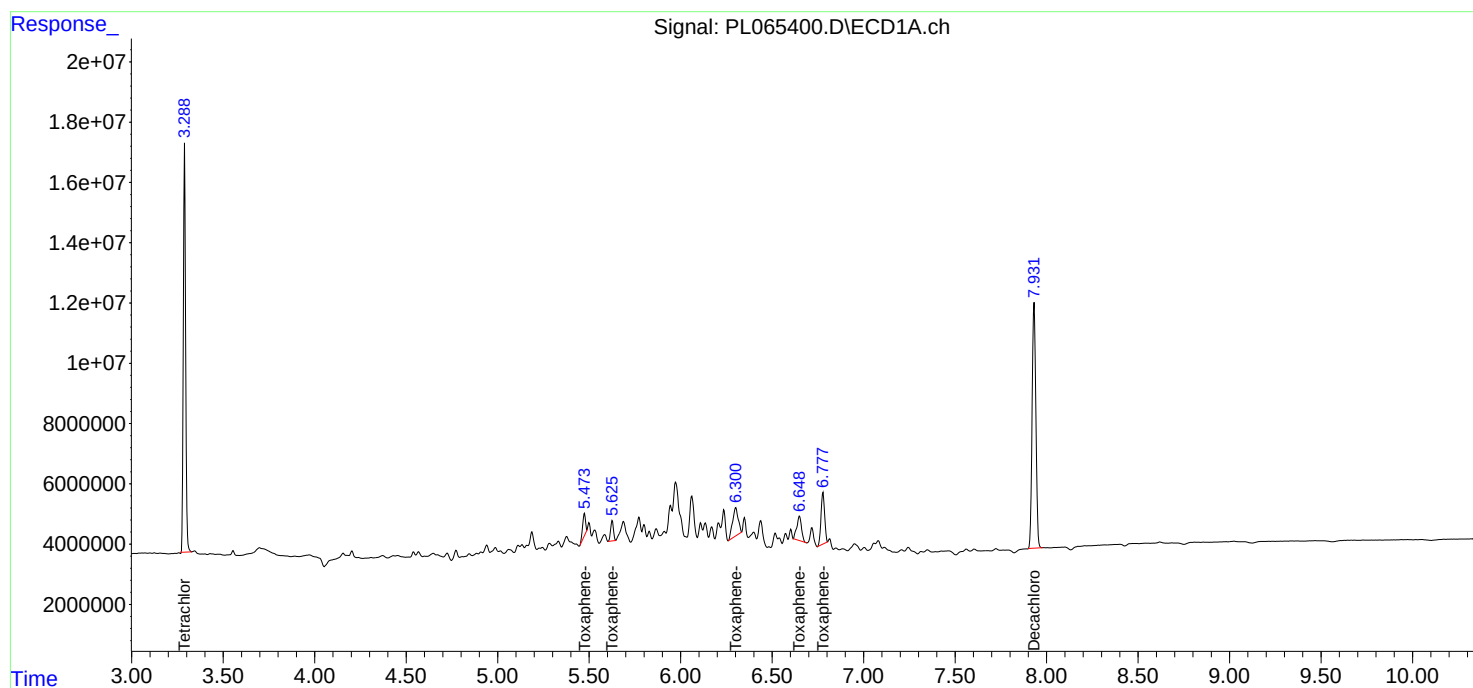

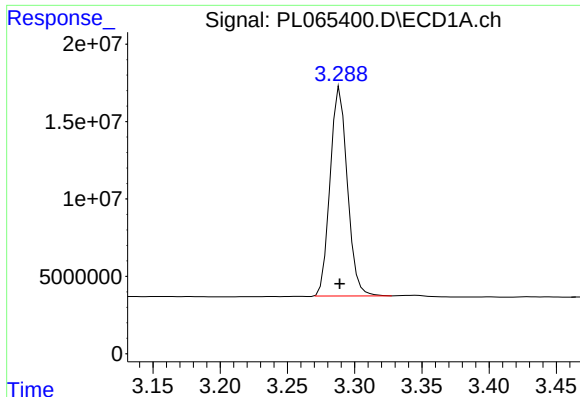


#1 Tetrachloro-m-xylene

R.T.: 3.289 min
Delta R.T.: 0.000 min
Response: 119796082
Conc: 50.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500


Manual Integrations
APPROVED

Ankita
3/19/2021 1:09:16 PM

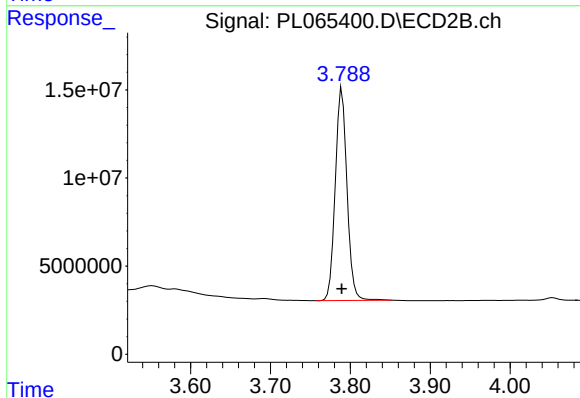


#1 Tetrachloro-m-xylene

R.T.: 3.789 min
Delta R.T.: 0.000 min
Response: 123143677
Conc: 44.72 ng/ml

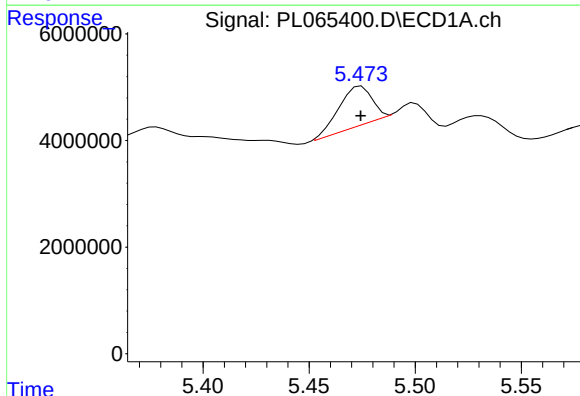


#2 Toxaphene-1

R.T.: 5.475 min
Delta R.T.: 0.000 min
Response: 7927803
Conc: 506.87 ng/ml

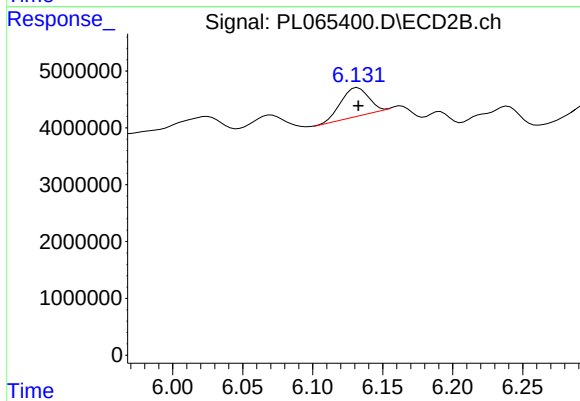

#2 Toxaphene-1

R.T.: 6.132 min
Delta R.T.: 0.000 min
Response: 7405703
Conc: 456.80 ng/ml

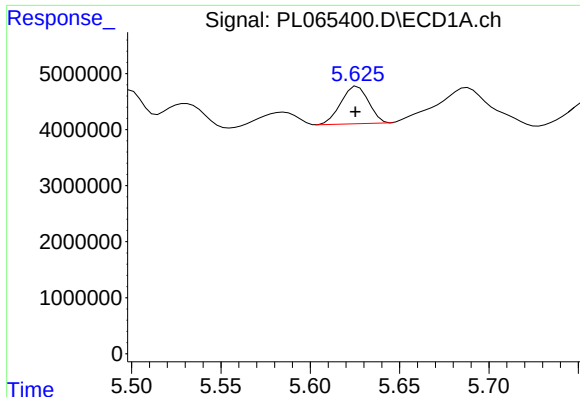


#3 Toxaphene-2

R.T.: 5.626 min
Delta R.T.: 0.001 min
Response: 7197943
Conc: 456.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500


Manual Integrations
APPROVED

Ankita
3/19/2021 1:09:16 PM

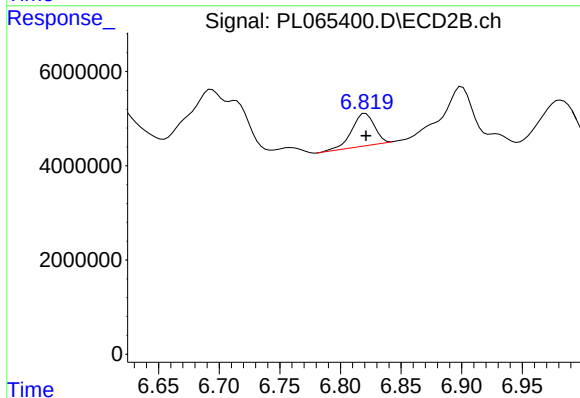


#3 Toxaphene-2

R.T.: 6.821 min
Delta R.T.: 0.000 min
Response: 8952073
Conc: 456.35 ng/ml

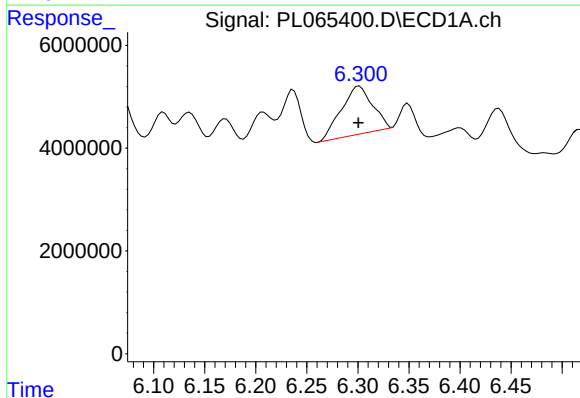


#4 Toxaphene-3

R.T.: 6.301 min
Delta R.T.: 0.000 min
Response: 19817152
Conc: 500.95 ng/ml

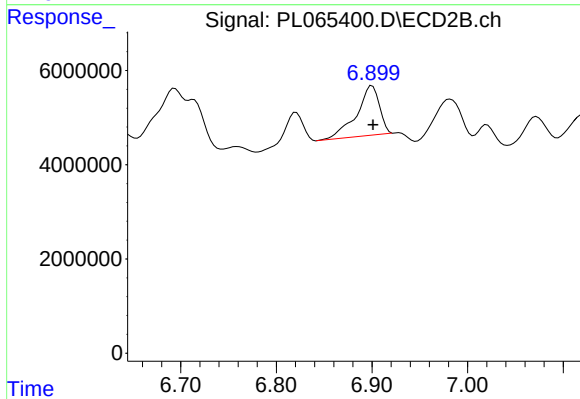

#4 Toxaphene-3

R.T.: 6.900 min
Delta R.T.: 0.000 min
Response: 17607193
Conc: 471.47 ng/ml

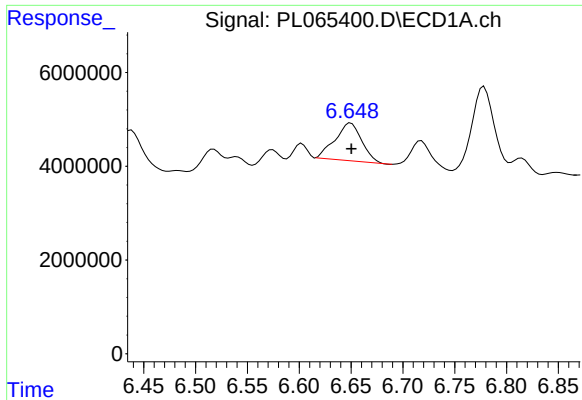


#5 Toxaphene-4

R.T.: 6.650 min
Delta R.T.: 0.000 min
Response: 14428977
Conc: 518.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500


Manual Integrations
APPROVED

Ankita
3/19/2021 1:09:16 PM

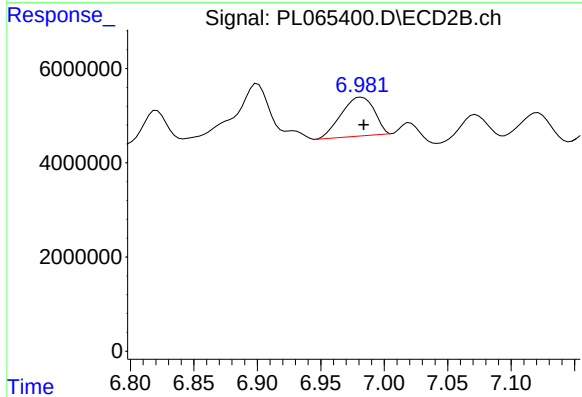


#5 Toxaphene-4

R.T.: 6.981 min
Delta R.T.: -0.003 min
Response: 15042038
Conc: 465.75 ng/ml m

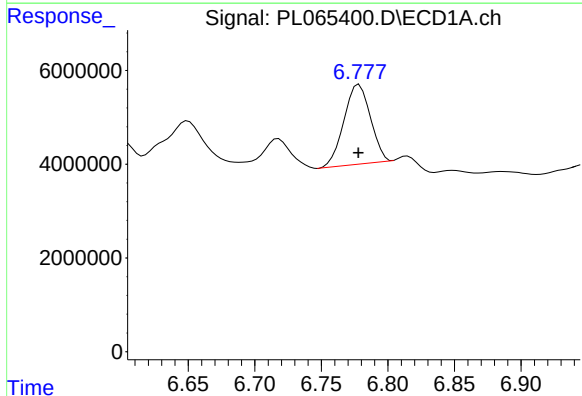


#6 Toxaphene-5

R.T.: 6.778 min
Delta R.T.: 0.000 min
Response: 23477210
Conc: 500.19 ng/ml

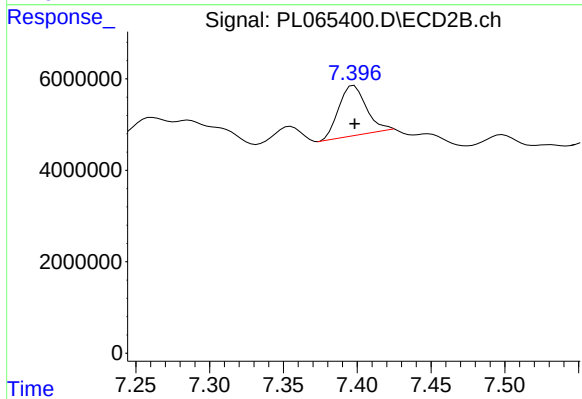

#6 Toxaphene-5

R.T.: 7.398 min
Delta R.T.: 0.000 min
Response: 14591772
Conc: 488.56 ng/ml

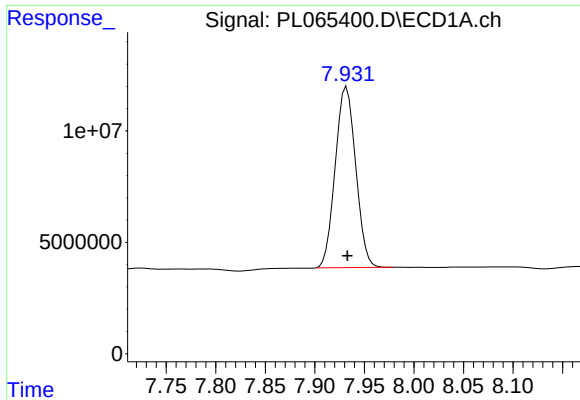


#7 Decachlorobiphenyl

R.T.: 7.932 min
Delta R.T.: 0.000 min
Response: 116753995
Conc: 49.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PTOXCCC500

Manual Integrations
APPROVED

Ankita
3/19/2021 1:09:16 PM

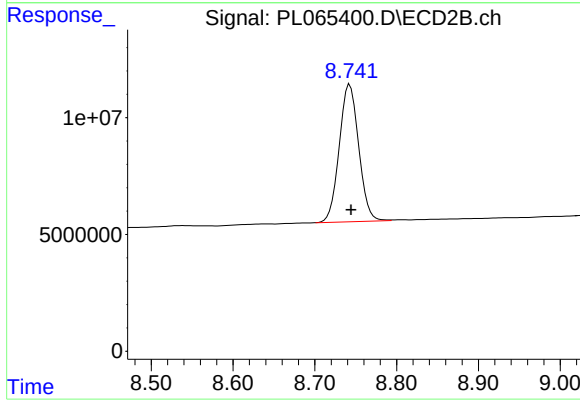

#7 Decachlorobiphenyl

R.T.: 8.743 min
Delta R.T.: -0.002 min
Response: 96848913
Conc: 48.14 ng/ml