

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
 Data File : PL073464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2022 12:56
 Operator : AR\AJ
 Sample : PB143235BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB143235BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 00:49:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.646	5.491	5924093	33515679	18.496	20.421
28)	SA Decachlor...	10.419	11.333	10360996	36394674	20.376	20.353
Target Compounds							
6)	B beta-BHC	6.131f	6.659f	70264	394964	0.341	0.379
7)	B delta-BHC	0.000	6.959	0	1344213	N.D.	0.624 #
8)	B Heptachlo...	0.000	7.927	0	8511516	N.D.	4.261 #
10)	B gamma-Chl...	7.340f	8.198	9627	9597811	0.022	4.699 #
13)	MA Dieldrin	7.785	0.000	207651	0	0.498	N.D. #
14)	MA Endrin	8.093f	0.000	696629	0	1.795	N.D. #
16)	A 4,4'-DDD	0.000	9.001	0	590090	N.D.	0.404 #
22)	Mirex	0.000	10.422f	0	445042	N.D.	0.328 #
23)	Chlordane-1	6.002f	0.000	19994	0	1.687	N.D. #
25)	Chlordane-3	7.340f	8.198	9627	9597811	0.236	35.399 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
Data File : PL073464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2022 12:56
Operator : AR\AJ
Sample : PB143235BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB143235BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 00:49:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

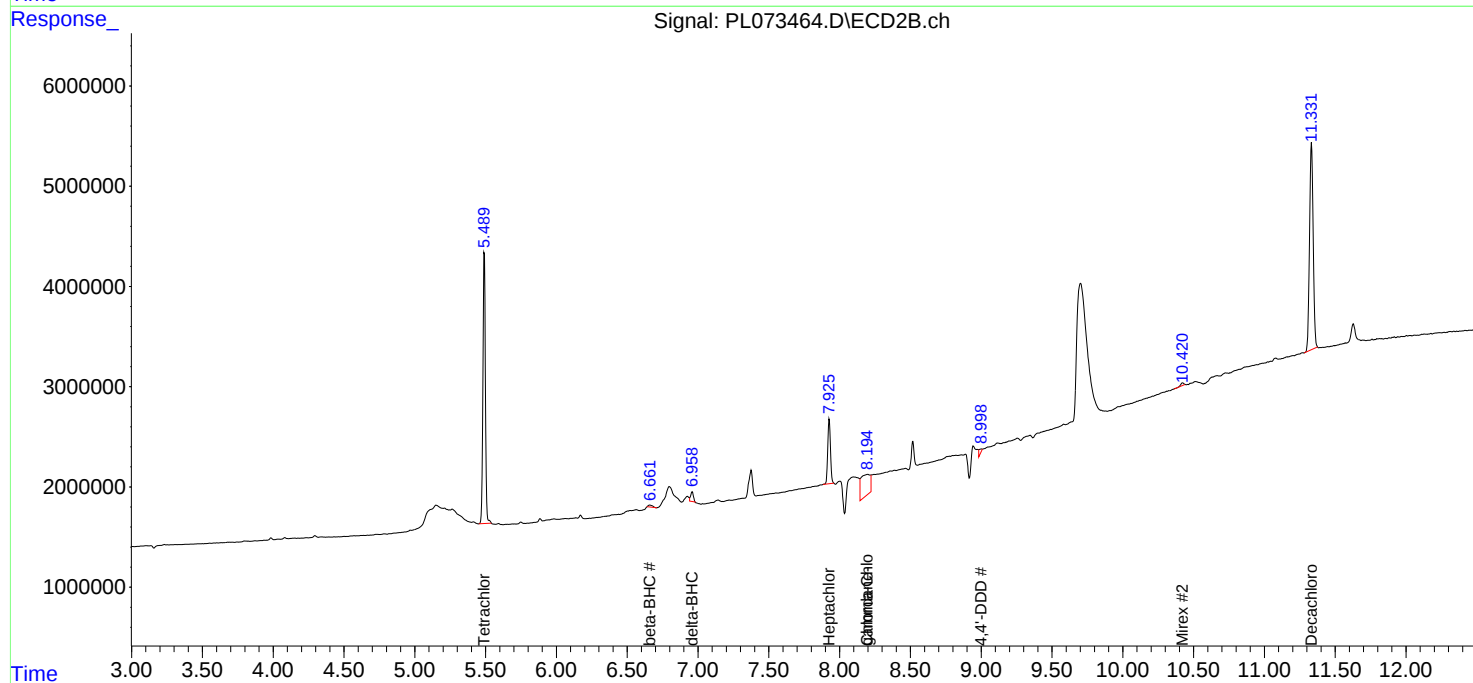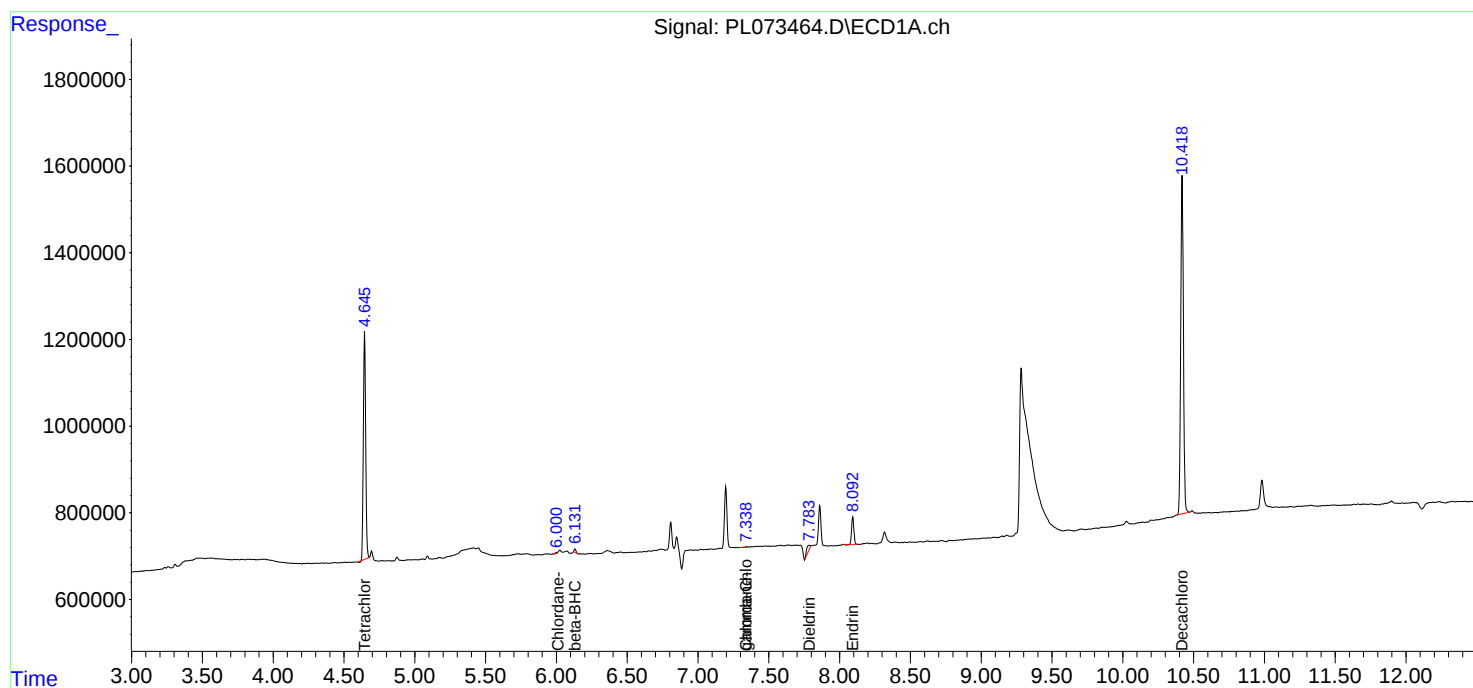


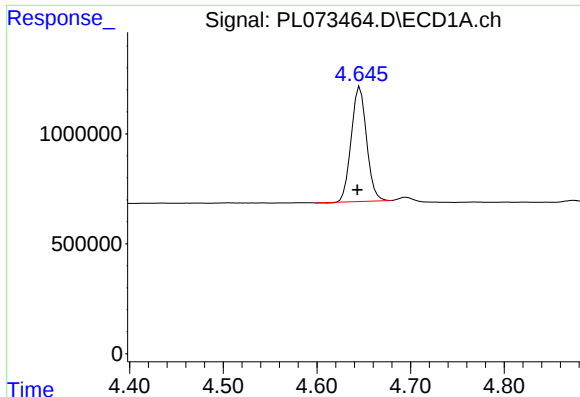

#1 Tetrachloro-m-xylene


R.T.: 4.646 min
Delta R.T.: 0.003 min
Response: 5924093
Conc: 18.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143235BL

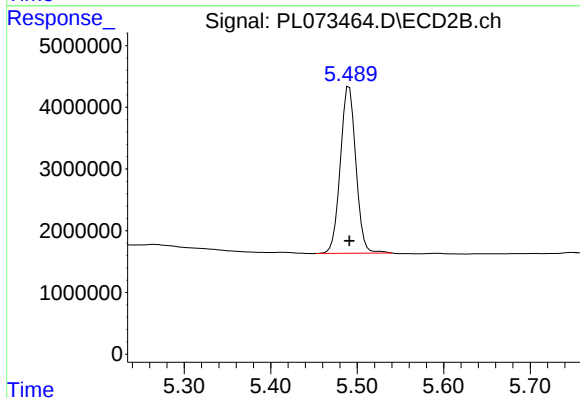


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 33515679
Conc: 20.42 ng/ml

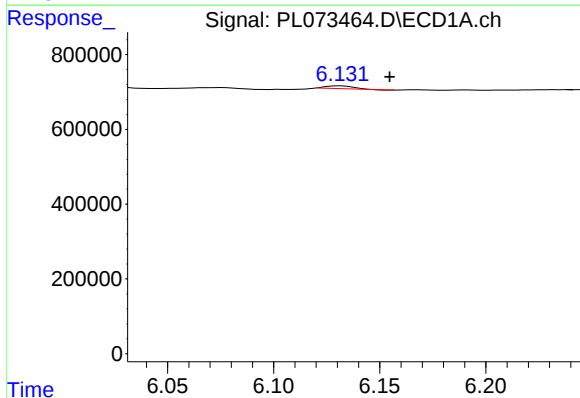


#6 beta-BHC

R.T.: 6.131 min
Delta R.T.: -0.023 min
Response: 70264
Conc: 0.34 ng/ml

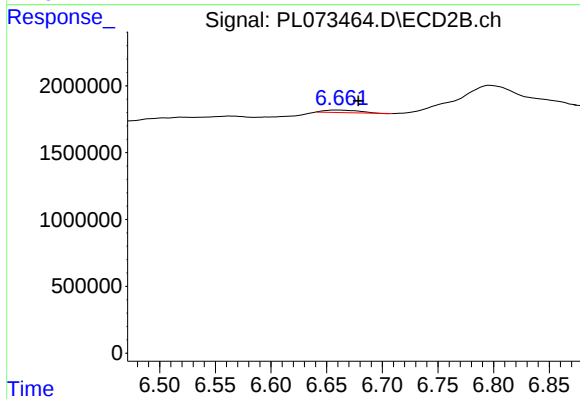

#6 beta-BHC


R.T.: 6.659 min
Delta R.T.: -0.019 min
Response: 394964
Conc: 0.38 ng/ml

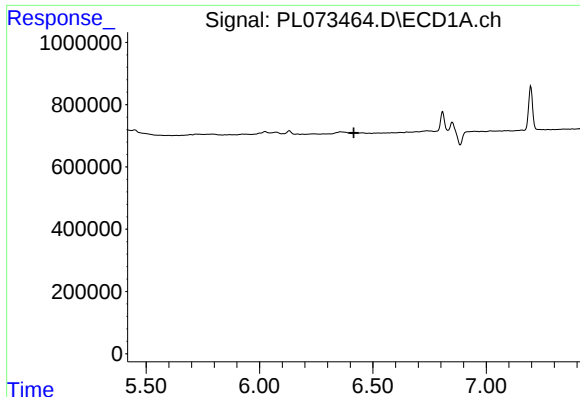

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143235BL

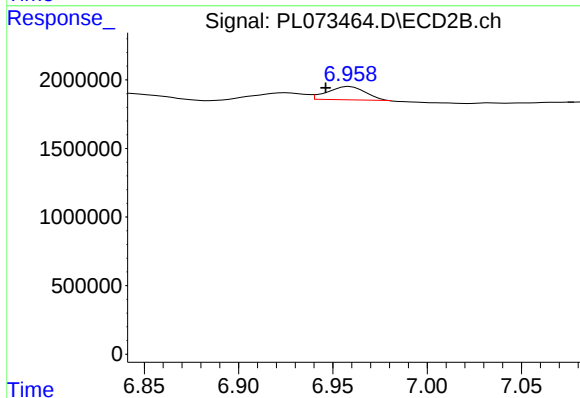


#7 delta-BHC

R.T.: 6.959 min
Delta R.T.: 0.013 min
Response: 1344213
Conc: 0.62 ng/ml

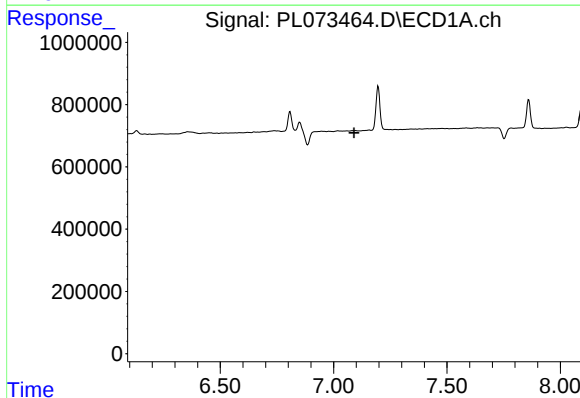


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.090 min
Response: 0
Conc: N.D.

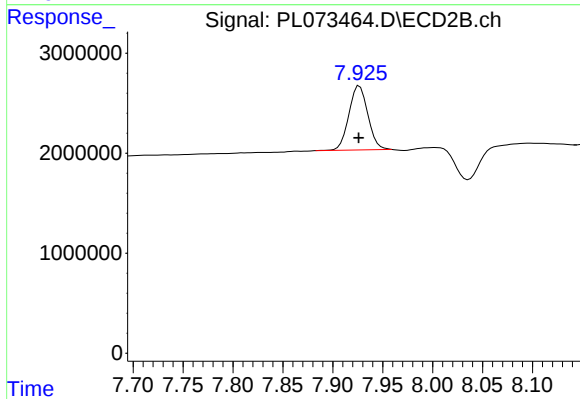

#8 Heptachlor epoxide


R.T.: 7.927 min
Delta R.T.: 0.000 min
Response: 8511516
Conc: 4.26 ng/ml

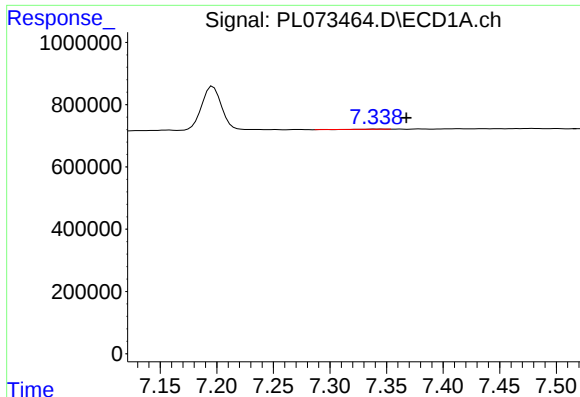

#10 gamma-Chlordane


R.T.: 7.340 min
Delta R.T.: -0.027 min
Response: 9627
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143235BL

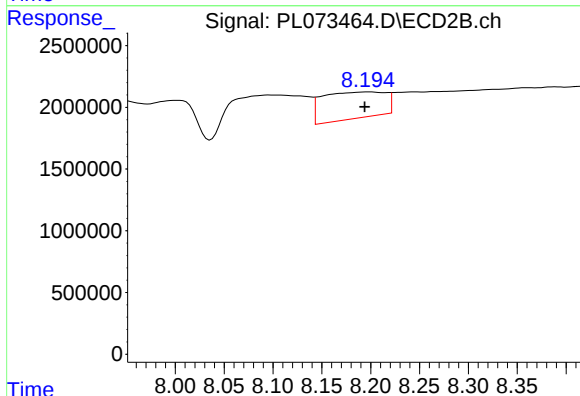


#10 gamma-Chlordane

R.T.: 8.198 min
Delta R.T.: 0.005 min
Response: 9597811
Conc: 4.70 ng/ml

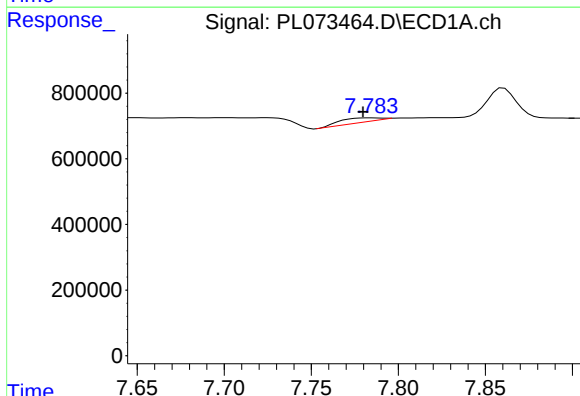


#13 Dieldrin

R.T.: 7.785 min
Delta R.T.: 0.005 min
Response: 207651
Conc: 0.50 ng/ml

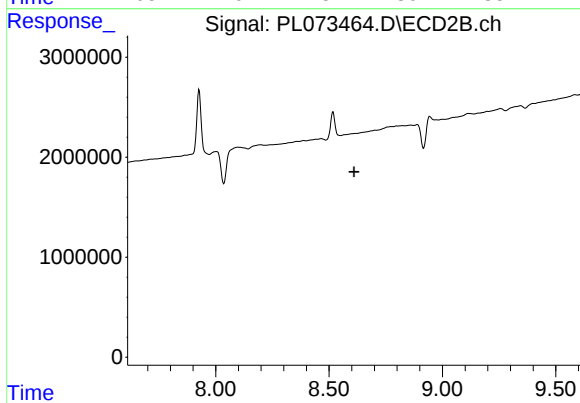

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.611 min
Response: 0
Conc: N.D.

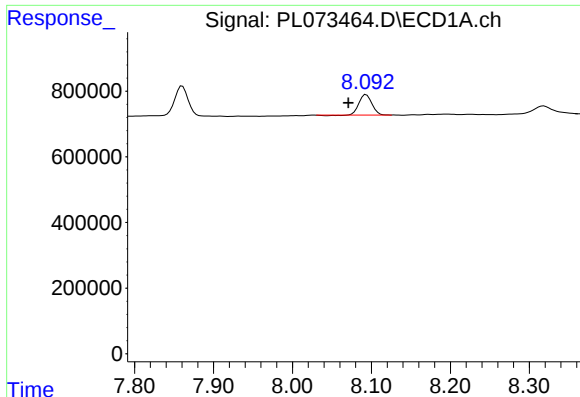

#14 Endrin


R.T.: 8.093 min
Delta R.T.: 0.023 min
Response: 696629
Conc: 1.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143235BL

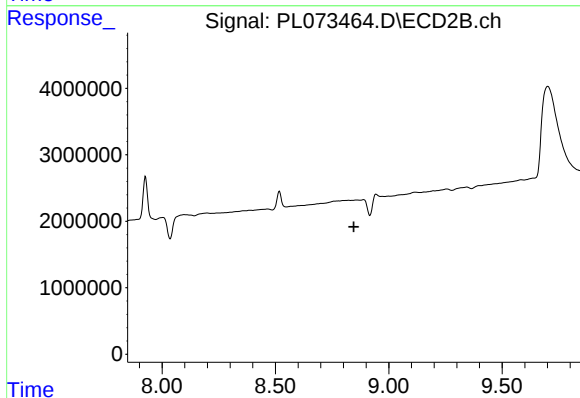


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.845 min
Response: 0
Conc: N.D.

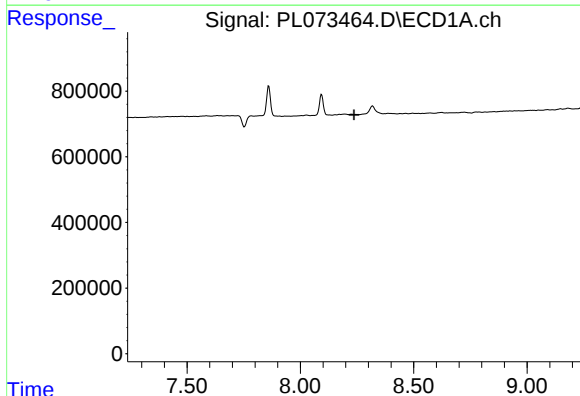


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.237 min
Response: 0
Conc: N.D.

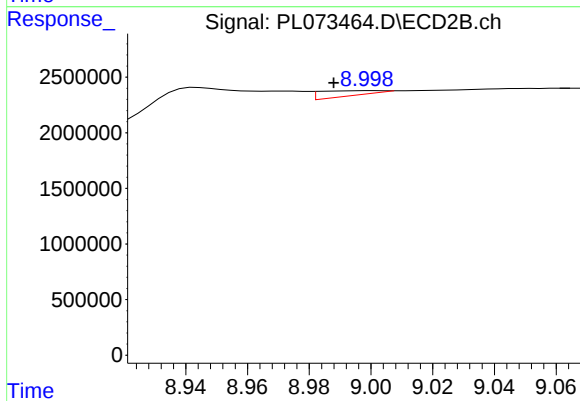

#16 4,4'-DDD


R.T.: 9.001 min
Delta R.T.: 0.013 min
Response: 590090
Conc: 0.40 ng/ml

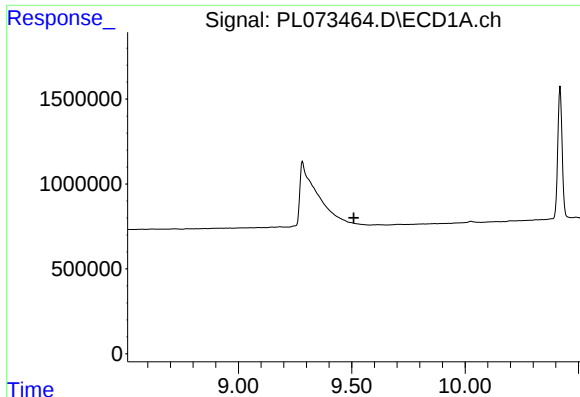

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143235BL

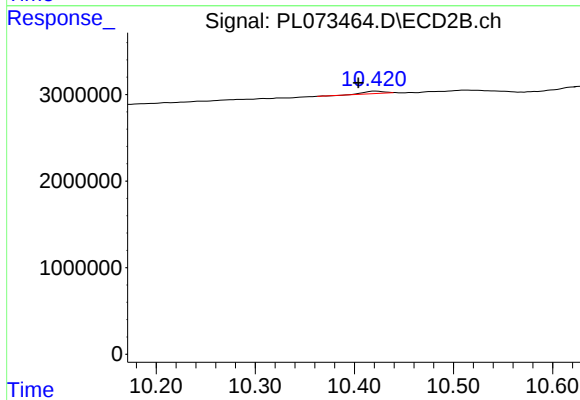


#22 Mirex

R.T.: 10.422 min
Delta R.T.: 0.017 min
Response: 445042
Conc: 0.33 ng/ml

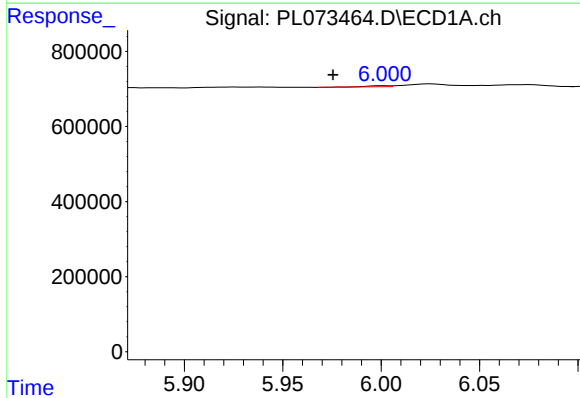


#23 Chlordane-1

R.T.: 6.002 min
Delta R.T.: 0.026 min
Response: 19994
Conc: 1.69 ng/ml

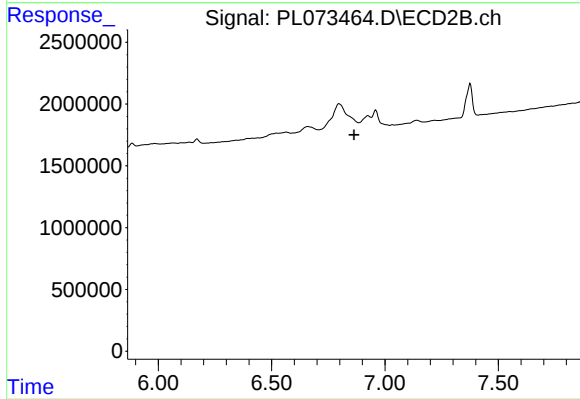

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 6.863 min
Response: 0
Conc: N.D.

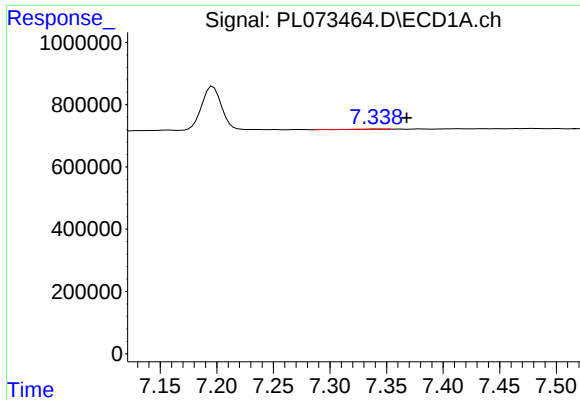

#25 Chlordane-3


R.T.: 7.340 min
Delta R.T.: -0.028 min
Response: 9627
Conc: 0.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143235BL

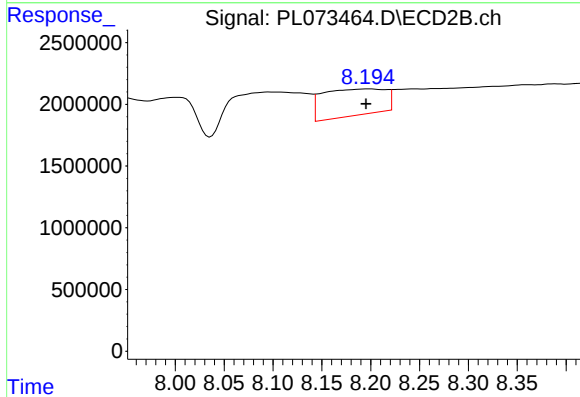


#25 Chlordane-3

R.T.: 8.198 min
Delta R.T.: 0.003 min
Response: 9597811
Conc: 35.40 ng/ml

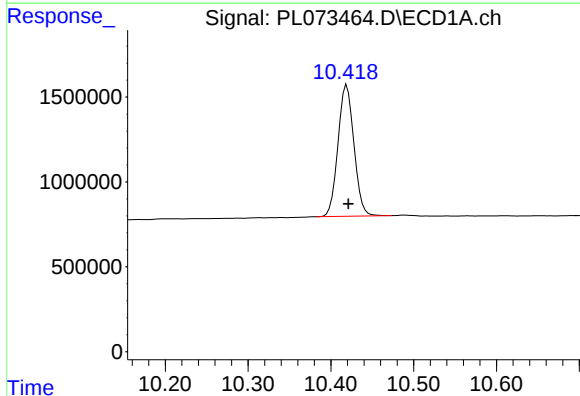

#28 Decachlorobiphenyl

R.T.: 10.419 min
Delta R.T.: -0.002 min
Response: 10360996
Conc: 20.38 ng/ml

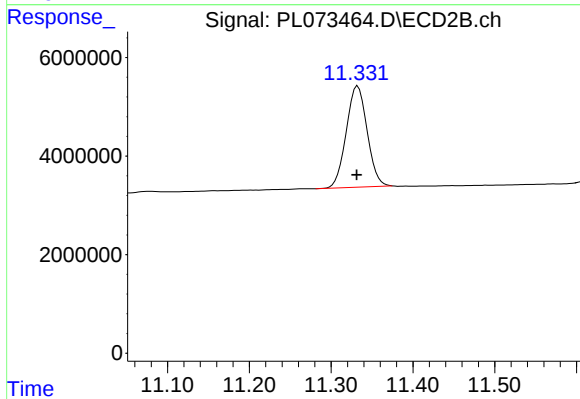

#28 Decachlorobiphenyl

R.T.: 11.333 min
Delta R.T.: 0.001 min
Response: 36394674
Conc: 20.35 ng/ml