

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
 Data File : PL073473.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2022 15:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 00:54:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.492	7823259	42915677	24.426	26.148
28)	SA Decachlor...	10.417	11.332	12156465	42583004	23.907	23.814
Target Compounds							
6)	B beta-BHC	6.128f	6.677	56254	749156	0.273	0.719 #
7)	B delta-BHC	0.000	6.959	0	2491819	N.D.	1.157 #
8)	B Heptachlo...	0.000	7.927	0	1582722	N.D.	0.792 #
10)	B gamma-Chl...	0.000	8.197	0	2596718	N.D.	1.271 #
13)	MA Dieldrin	7.779	0.000	136560	0	0.328	N.D. #
14)	MA Endrin	8.091f	0.000	219919	0	0.567	N.D. #
15)	B Endosulfa...	8.354f	9.063	36196	3561070	0.093	2.319 #
23)	Chlordane-1	0.000	6.849	0	1273666	N.D.	18.644 #
25)	Chlordane-3	0.000	8.197	0	2596718	N.D.	9.577 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
Data File : PL073473.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2022 15:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 00:54:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

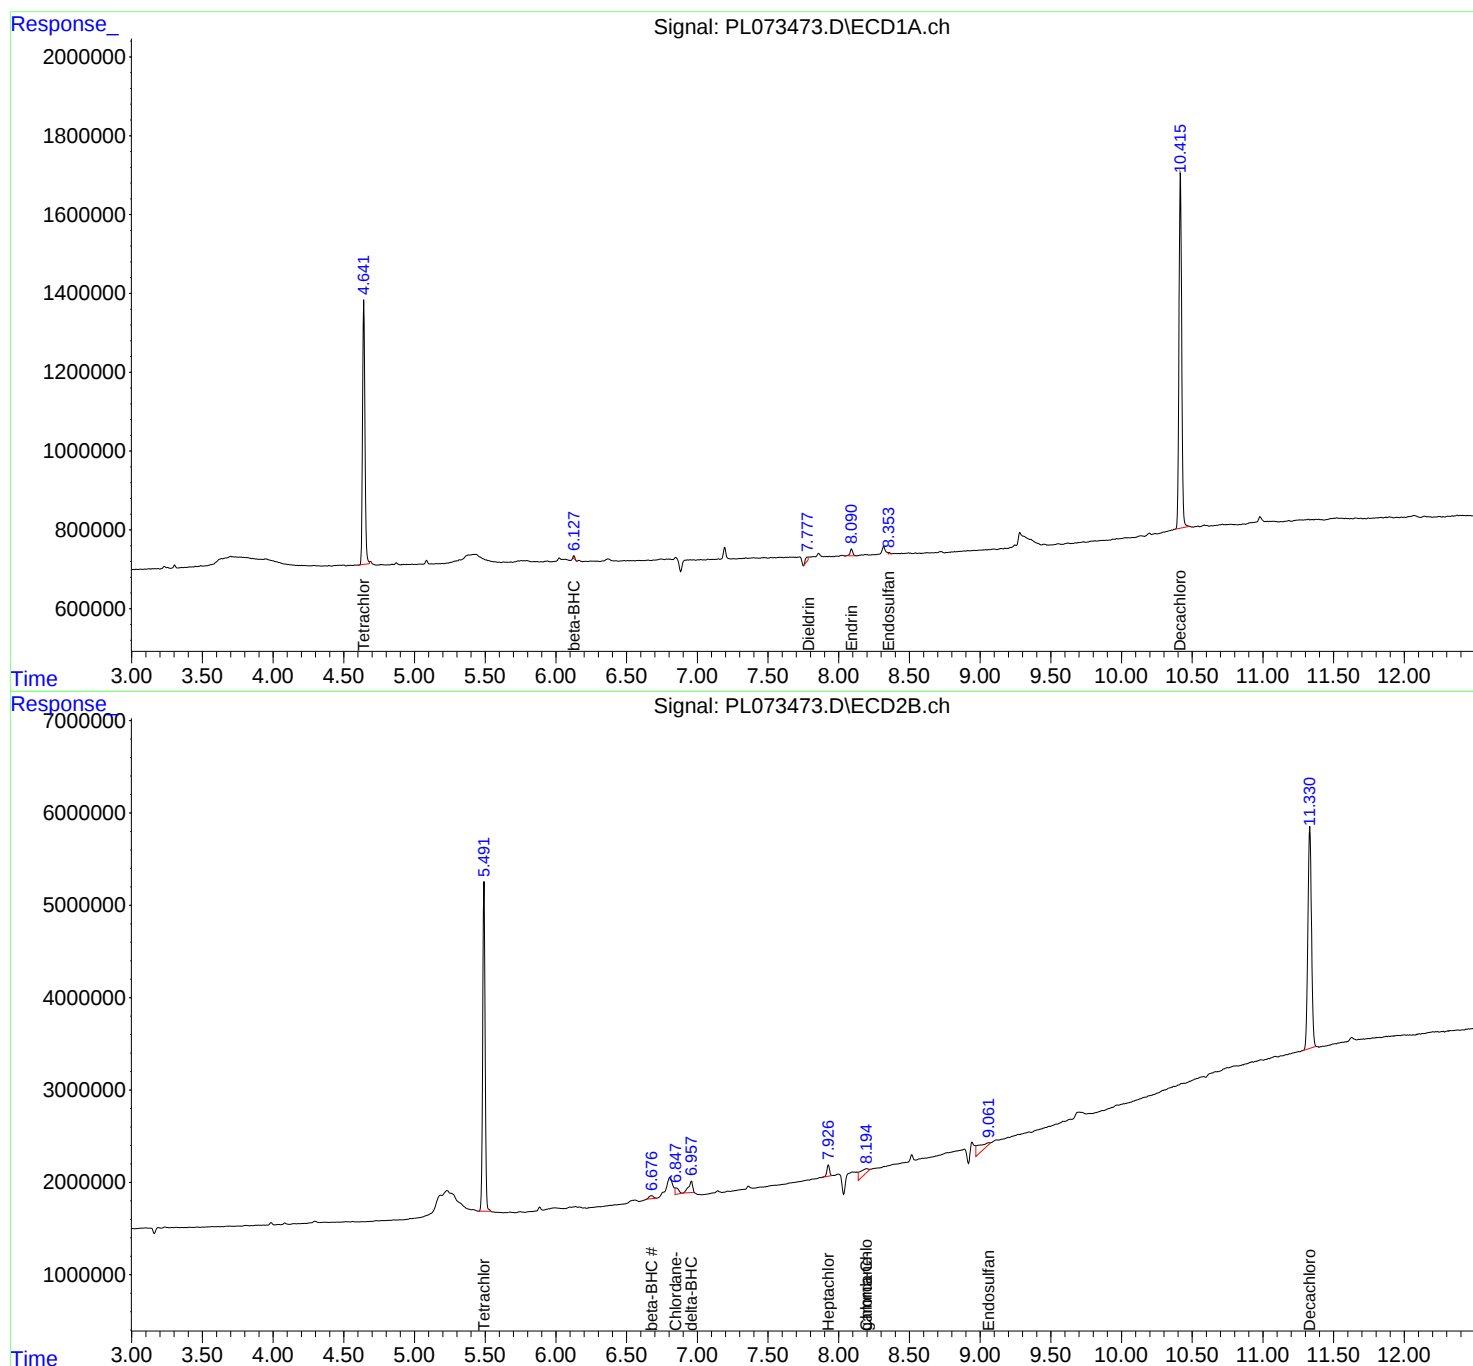


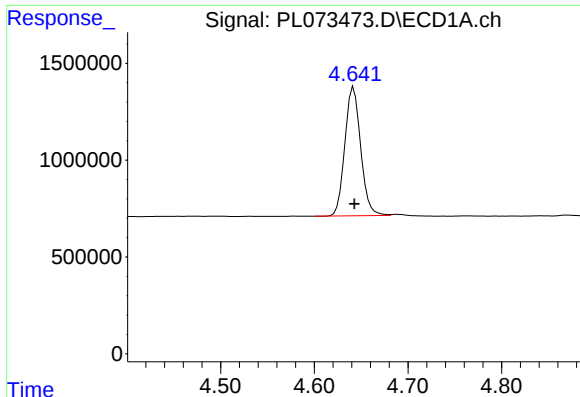

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 7823259
Conc: 24.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

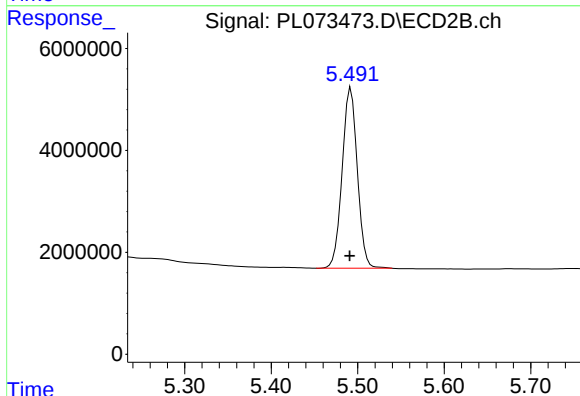


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.001 min
Response: 42915677
Conc: 26.15 ng/ml

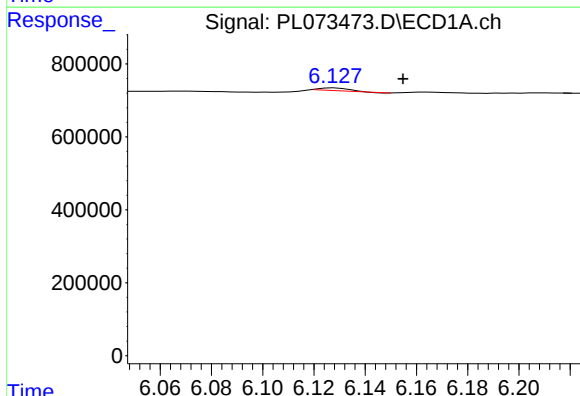


#6 beta-BHC

R.T.: 6.128 min
Delta R.T.: -0.027 min
Response: 56254
Conc: 0.27 ng/ml

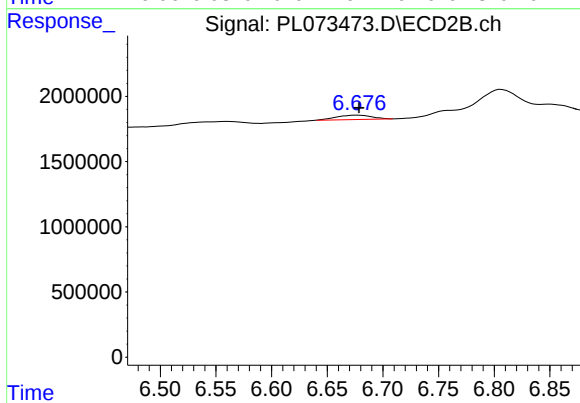

#6 beta-BHC


R.T.: 6.677 min
Delta R.T.: -0.001 min
Response: 749156
Conc: 0.72 ng/ml

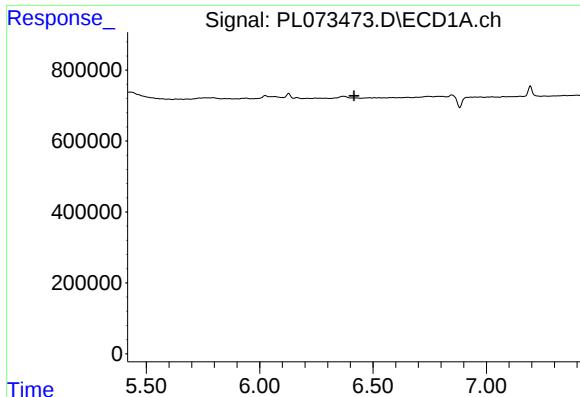

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

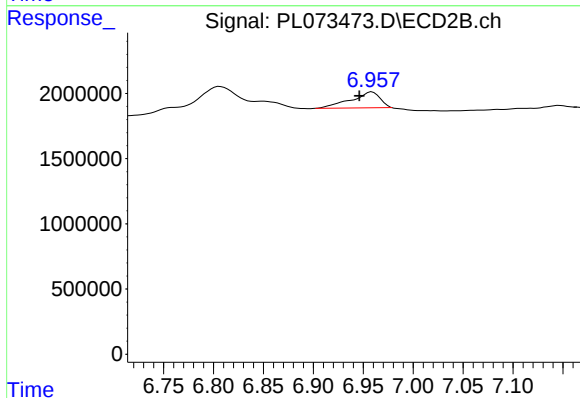


#7 delta-BHC

R.T.: 6.959 min
Delta R.T.: 0.013 min
Response: 2491819
Conc: 1.16 ng/ml

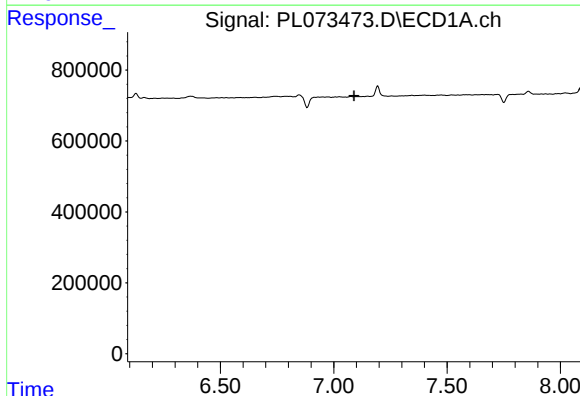


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.090 min
Response: 0
Conc: N.D.

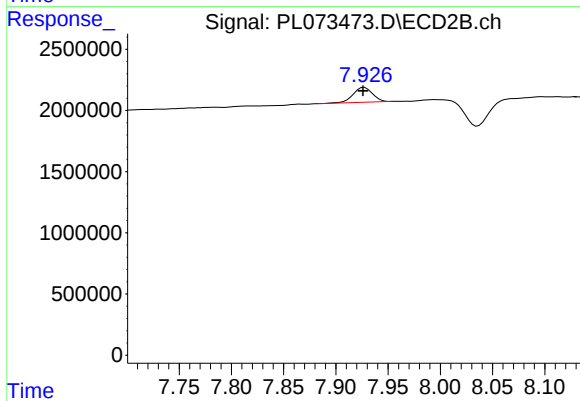

#8 Heptachlor epoxide


R.T.: 7.927 min
Delta R.T.: 0.001 min
Response: 1582722
Conc: 0.79 ng/ml

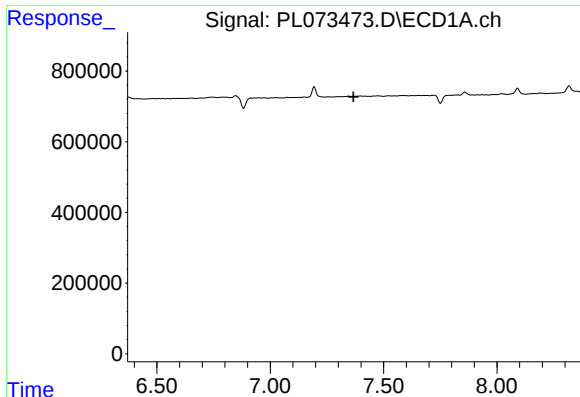

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

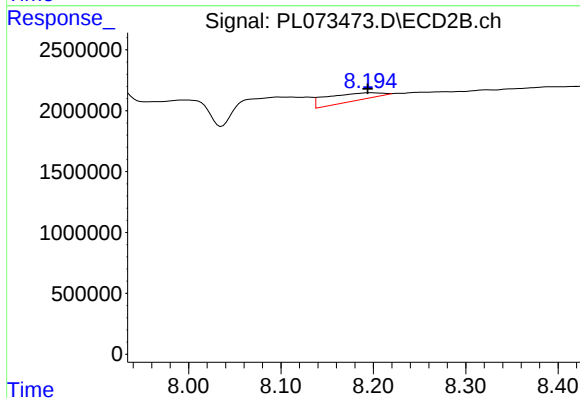


#10 gamma-Chlordane

R.T.: 8.197 min
Delta R.T.: 0.003 min
Response: 2596718
Conc: 1.27 ng/ml

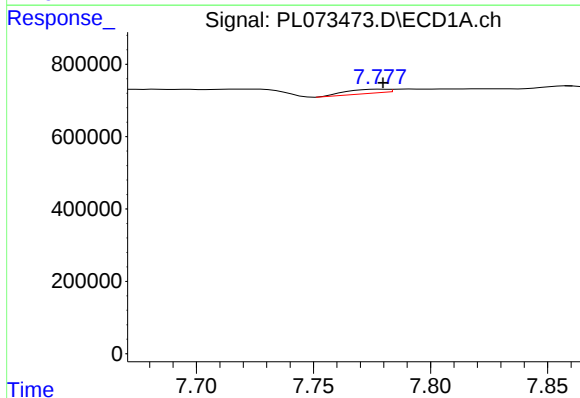


#13 Dieldrin

R.T.: 7.779 min
Delta R.T.: 0.000 min
Response: 136560
Conc: 0.33 ng/ml

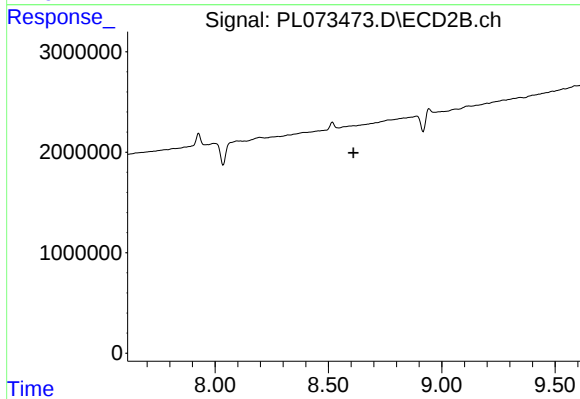

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 8.611 min
Response: 0
Conc: N.D.

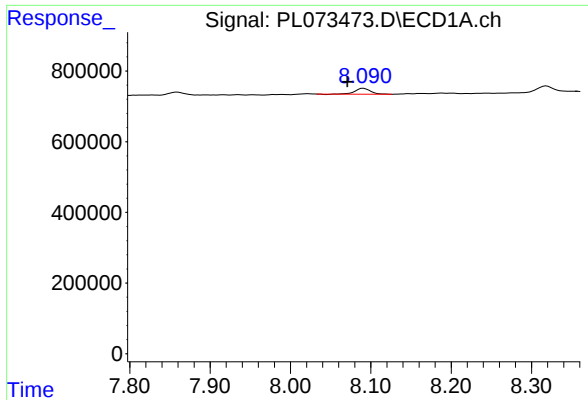

#14 Endrin


R.T.: 8.091 min
Delta R.T.: 0.020 min
Response: 219919
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

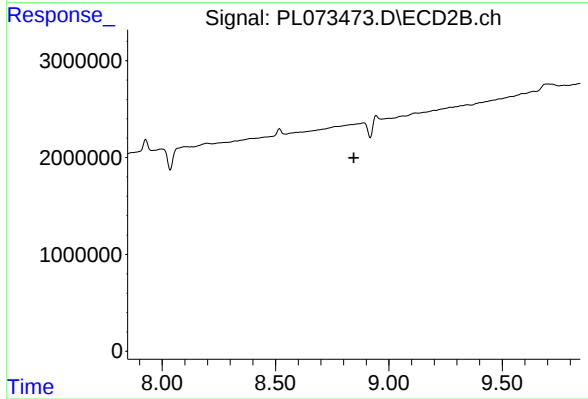


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.845 min
Response: 0
Conc: N.D.

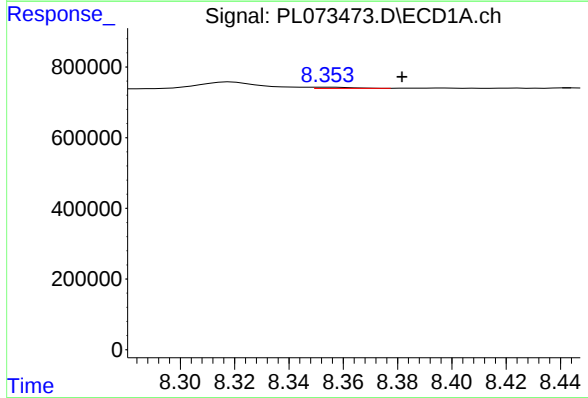


#15 Endosulfan II

R.T.: 8.354 min
Delta R.T.: -0.027 min
Response: 36196
Conc: 0.09 ng/ml

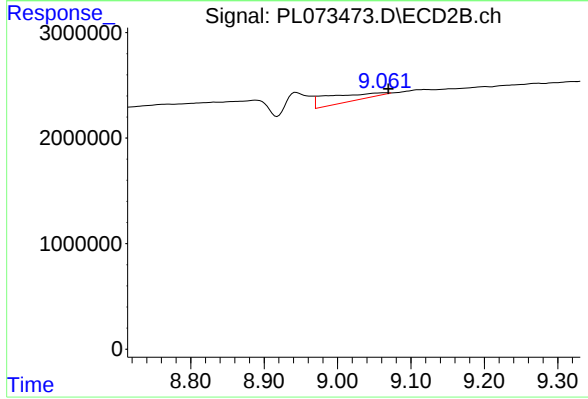

#15 Endosulfan II


R.T.: 9.063 min
Delta R.T.: -0.006 min
Response: 3561070
Conc: 2.32 ng/ml

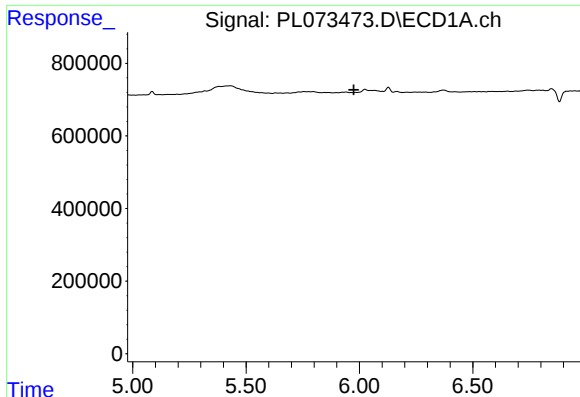

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

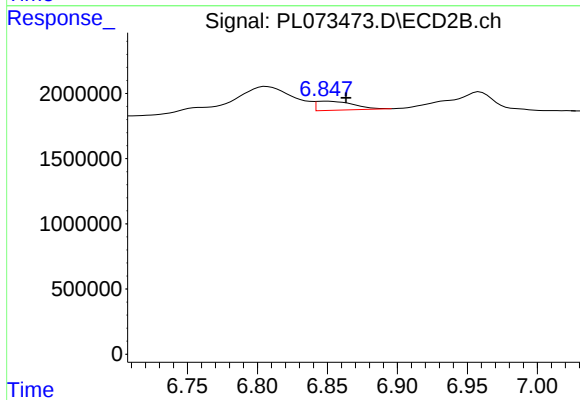


#23 Chlordane-1

R.T.: 6.849 min
Delta R.T.: -0.014 min
Response: 1273666
Conc: 18.64 ng/ml

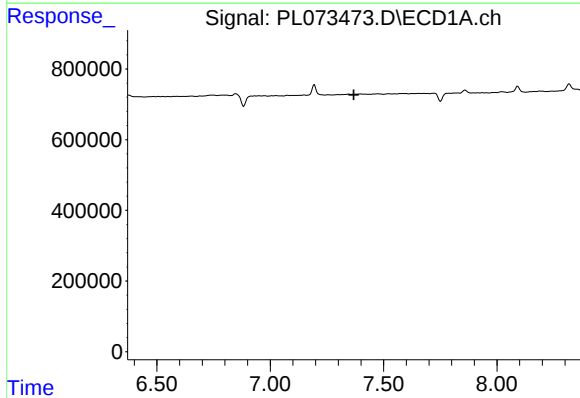


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

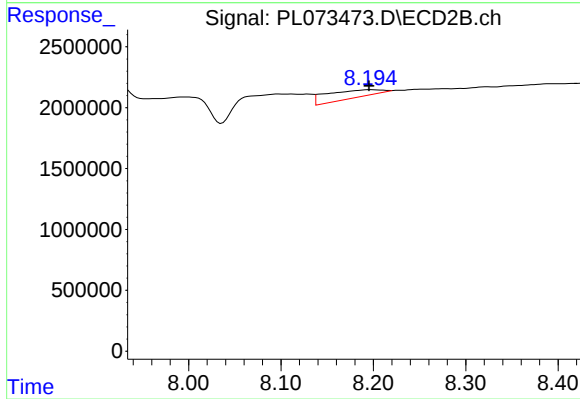

#25 Chlordane-3


R.T.: 8.197 min
Delta R.T.: 0.002 min
Response: 2596718
Conc: 9.58 ng/ml

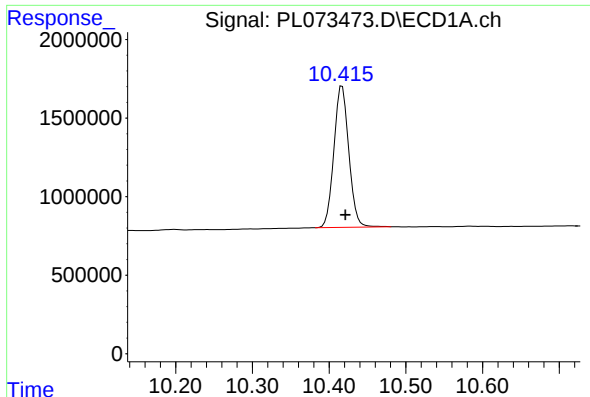

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.004 min
Response: 12156465
Conc: 23.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

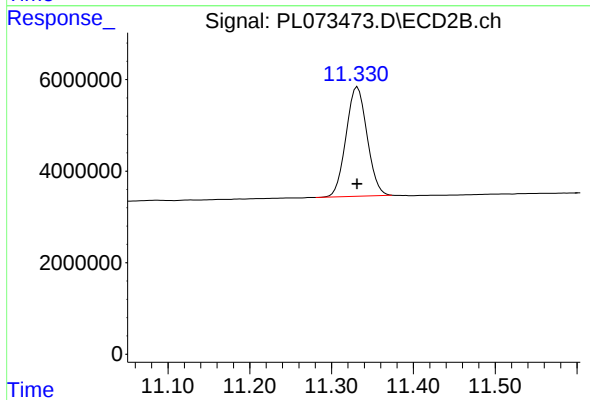

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 42583004
Conc: 23.81 ng/ml