

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
 Data File : PL073479.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2022 17:36
 Operator : AR\AJ
 Sample : PB143453BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB143454BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 00:55:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.492	5787205	31691386	18.069	19.309
28)	SA Decachlor...	10.417	11.331	9895166	34115157	19.460	19.078
Target Compounds							
6)	B beta-BHC	0.000	6.676	0	797344	N.D.	0.765 #
7)	B delta-BHC	0.000	6.957	0	1682057	N.D.	0.781 #
8)	B Heptachlo...	0.000	7.921	0	55358	N.D.	0.028 #
10)	B gamma-Chl...	0.000	8.202	0	669122	N.D.	0.328 #
11)	B alpha-Chl...	0.000	8.286	0	141721	N.D.	0.071 #
19)	B Endosulfa...	0.000	9.444	0	38538	N.D.	0.024 #
20)	A Methoxychlor	9.094	0.000	14151	0	0.055	N.D. #
21)	B Endrin ke...	0.000	9.923	0	77674	N.D.	0.047 #
23)	Chlordane-1	0.000	6.854	0	1300966	N.D.	19.044 #
25)	Chlordane-3	0.000	8.202	0	669122	N.D.	2.468 #
26)	Chlordane-4	0.000	8.286	0	141721	N.D.	0.428 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
Data File : PL073479.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2022 17:36
Operator : AR\AJ
Sample : PB143453BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB143454BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 00:55:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

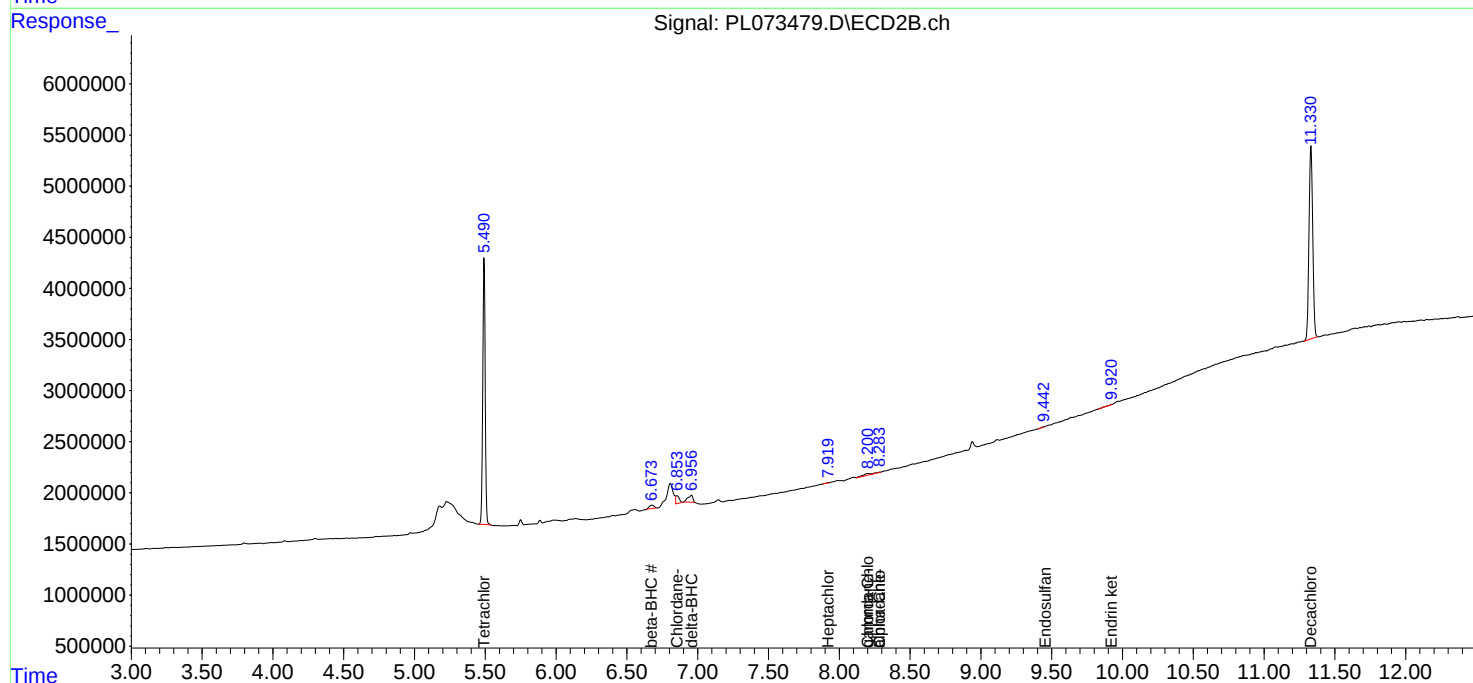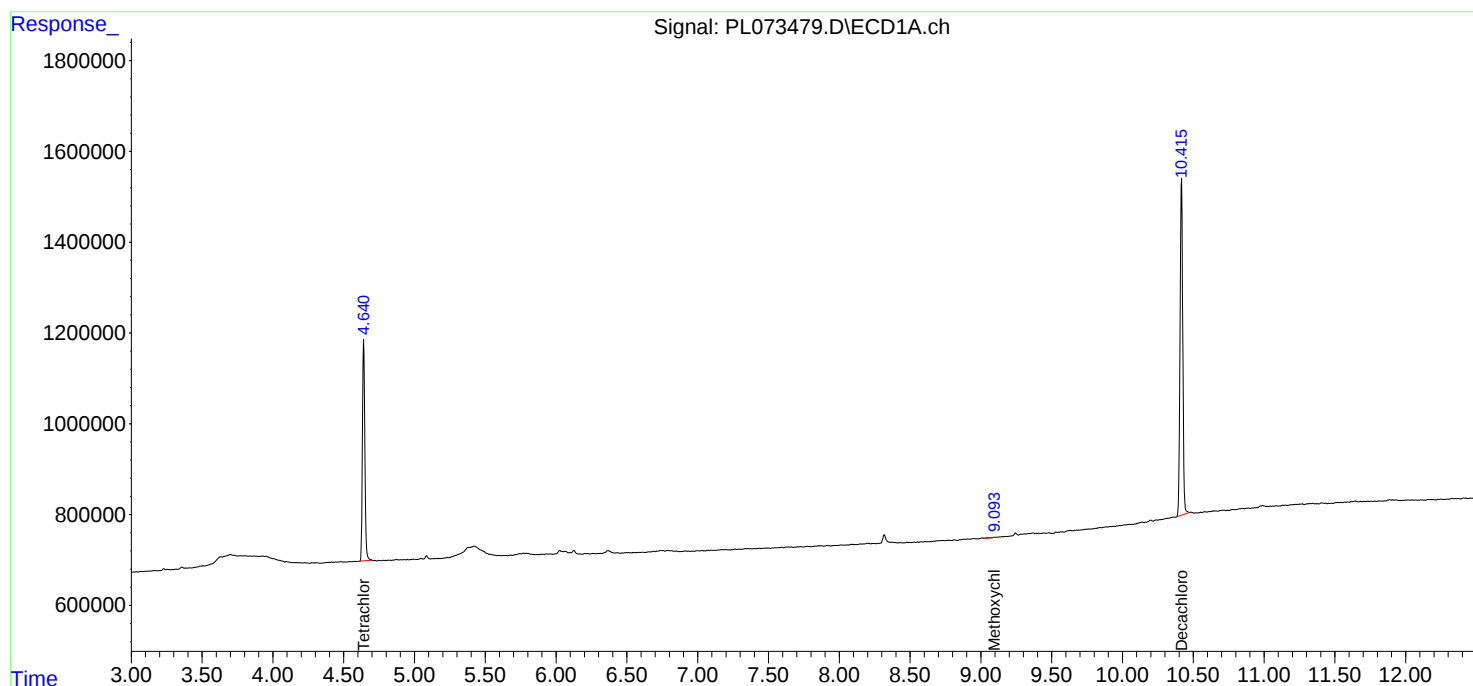


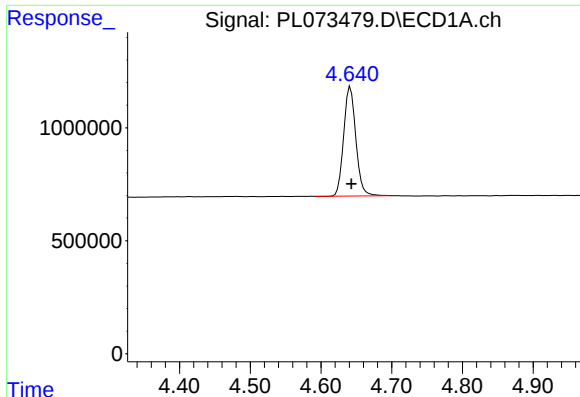

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.001 min
Response: 5787205
Conc: 18.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143454BL

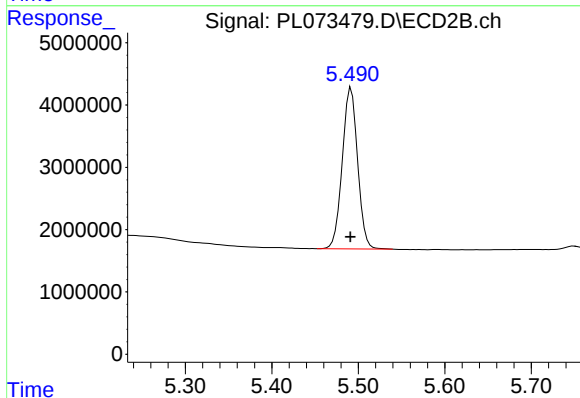


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 31691386
Conc: 19.31 ng/ml

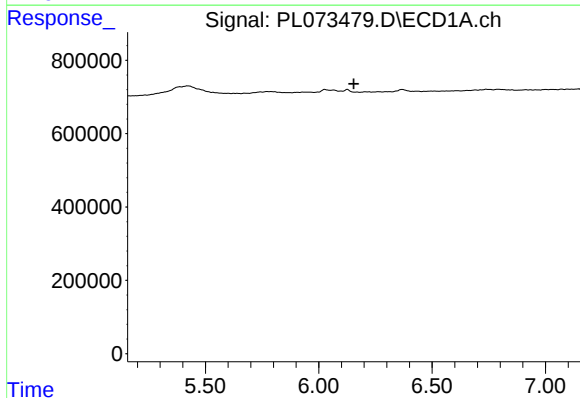


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

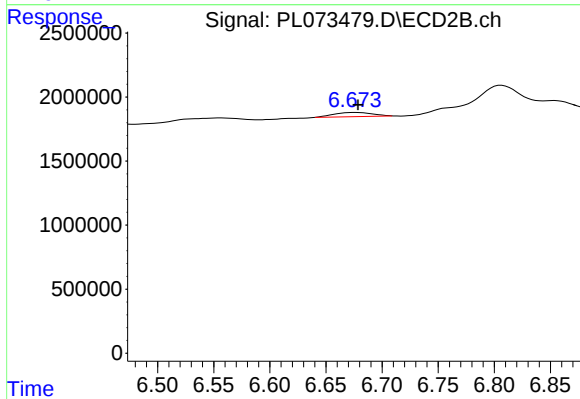

#6 beta-BHC


R.T.: 6.676 min
Delta R.T.: -0.003 min
Response: 797344
Conc: 0.76 ng/ml

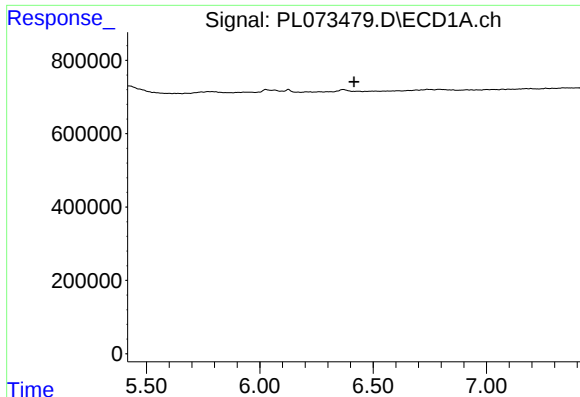

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143454BL

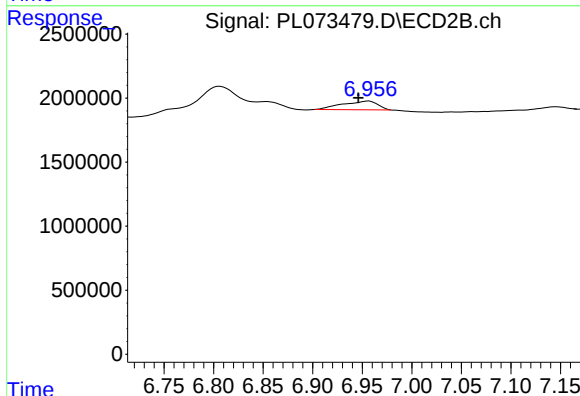


#7 delta-BHC

R.T.: 6.957 min
Delta R.T.: 0.011 min
Response: 1682057
Conc: 0.78 ng/ml

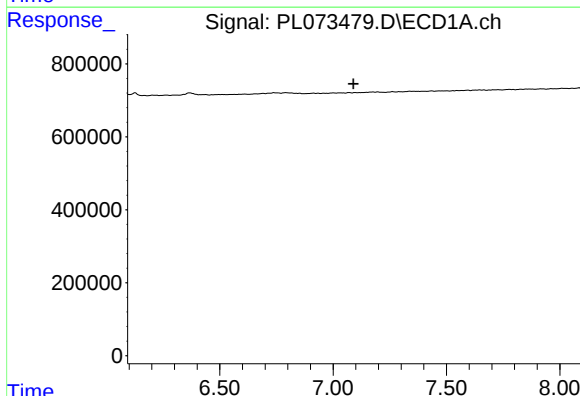


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.090 min
Response: 0
Conc: N.D.

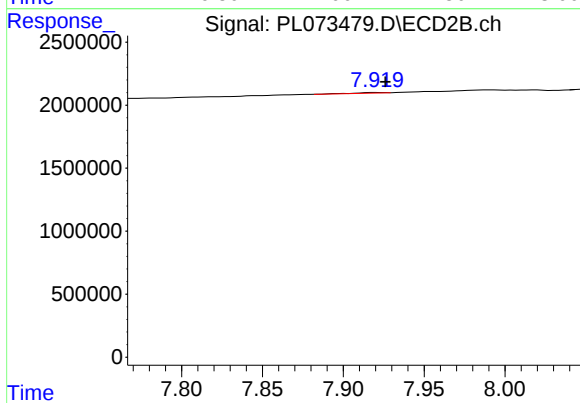

#8 Heptachlor epoxide


R.T.: 7.921 min
Delta R.T.: -0.006 min
Response: 55358
Conc: 0.03 ng/ml

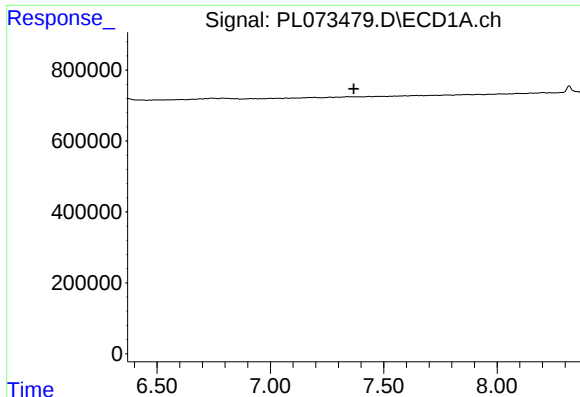

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143454BL

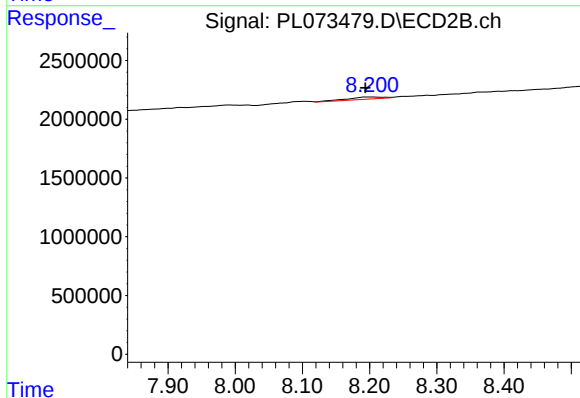


#10 gamma-Chlordane

R.T.: 8.202 min
Delta R.T.: 0.008 min
Response: 669122
Conc: 0.33 ng/ml

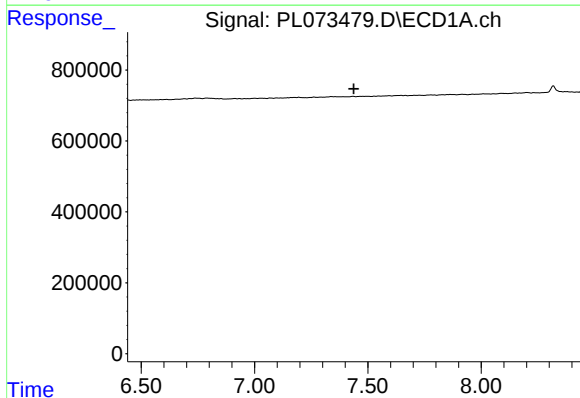


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

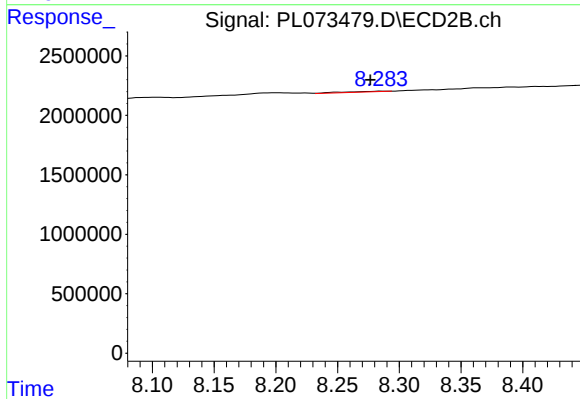

#11 alpha-Chlordane


R.T.: 8.286 min
Delta R.T.: 0.010 min
Response: 141721
Conc: 0.07 ng/ml

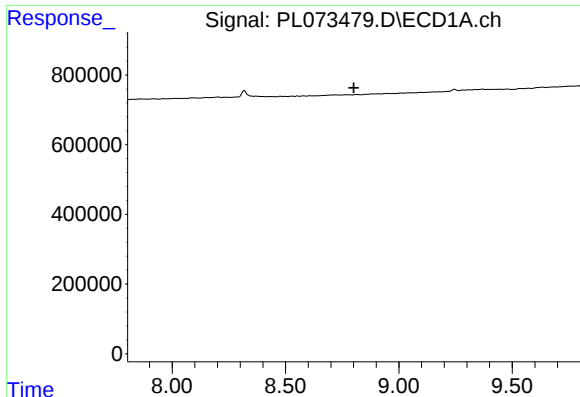

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143454BL

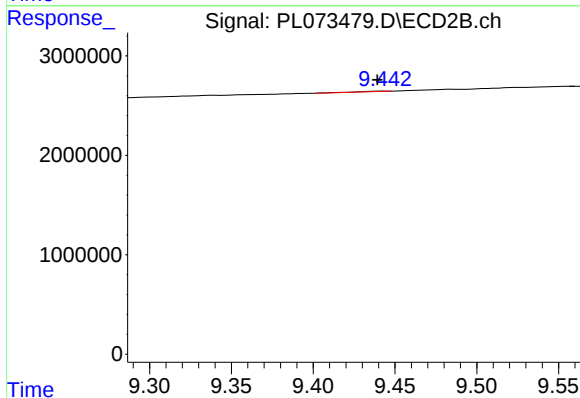


#19 Endosulfan Sulfate

R.T.: 9.444 min
Delta R.T.: 0.004 min
Response: 38538
Conc: 0.02 ng/ml

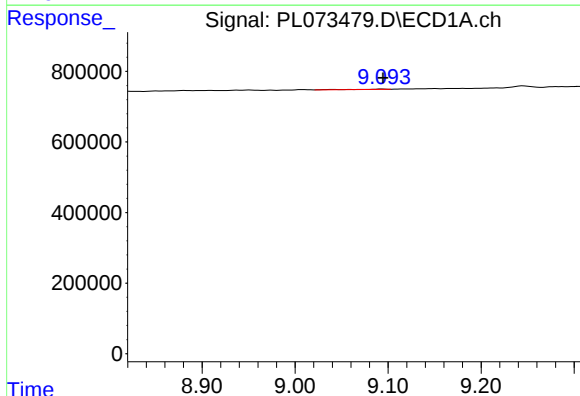


#20 Methoxychlor

R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 14151
Conc: 0.06 ng/ml

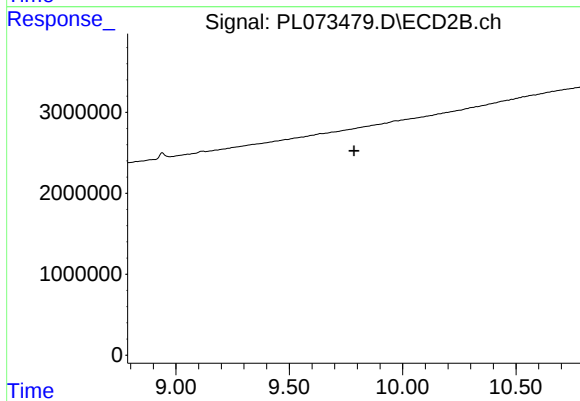

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.786 min
Response: 0
Conc: N.D.

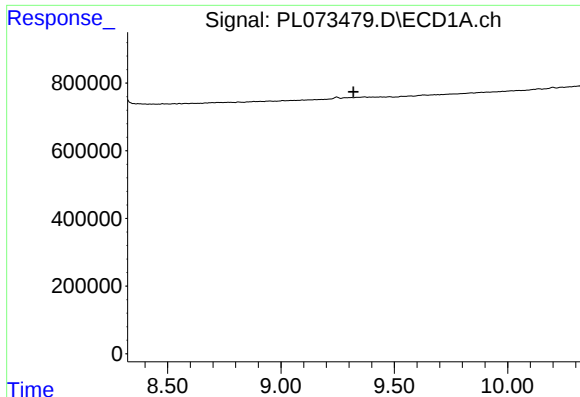

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 9.320 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143454BL

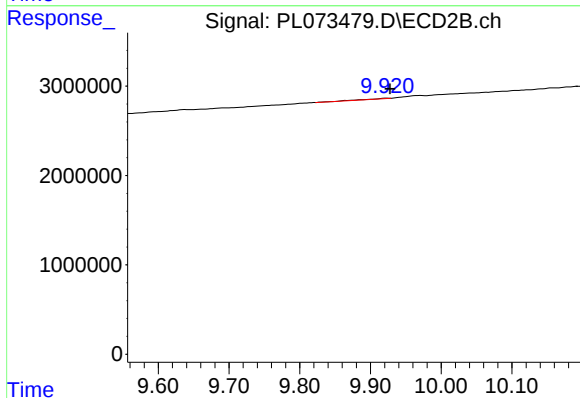


#21 Endrin ketone

R.T.: 9.923 min
Delta R.T.: -0.005 min
Response: 77674
Conc: 0.05 ng/ml

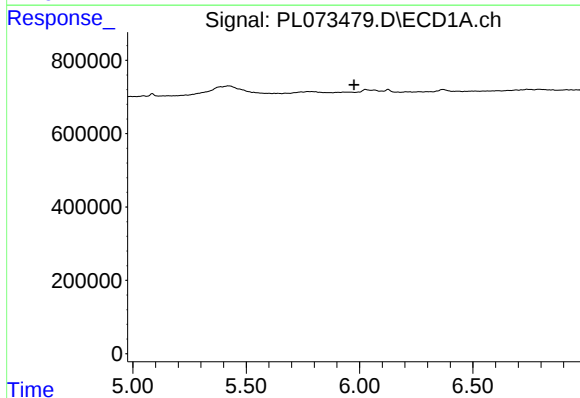


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

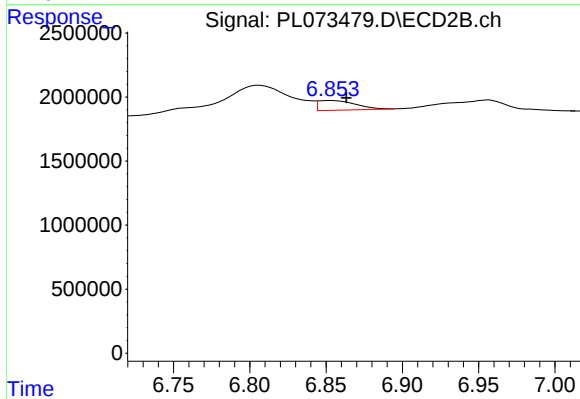

#23 Chlordane-1


R.T.: 6.854 min
Delta R.T.: -0.009 min
Response: 1300966
Conc: 19.04 ng/ml

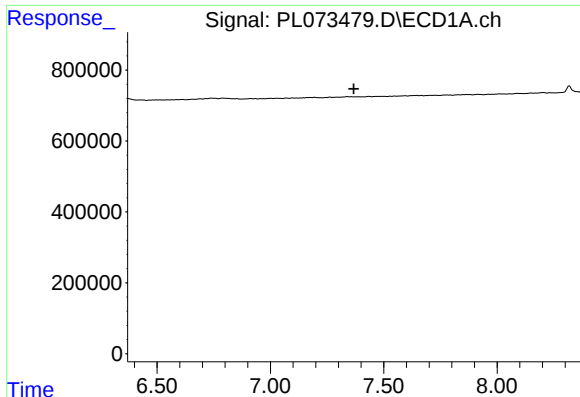

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143454BL

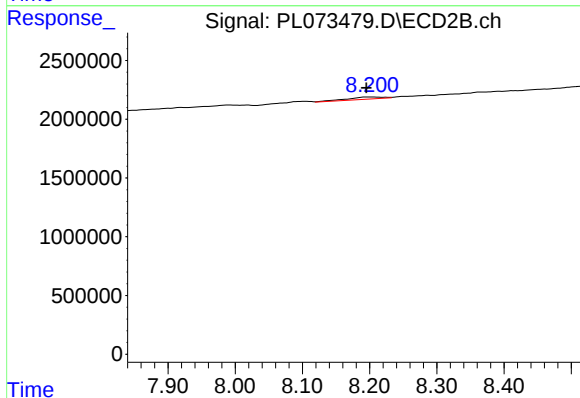


#25 Chlordane-3

R.T.: 8.202 min
Delta R.T.: 0.006 min
Response: 669122
Conc: 2.47 ng/ml

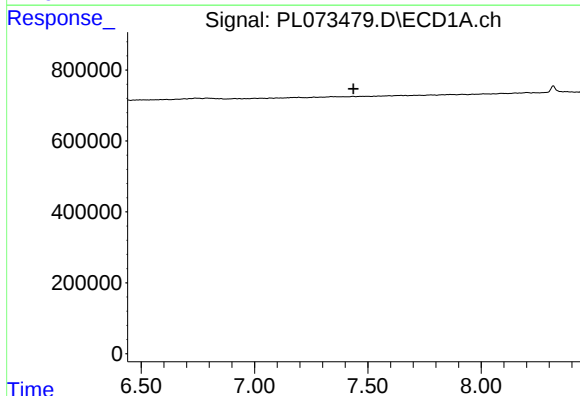


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

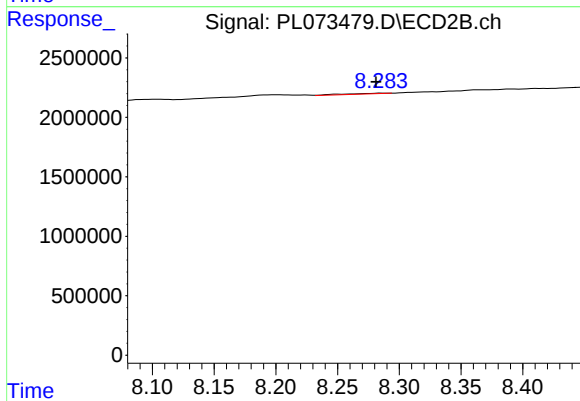

#26 Chlordane-4


R.T.: 8.286 min
Delta R.T.: 0.005 min
Response: 141721
Conc: 0.43 ng/ml

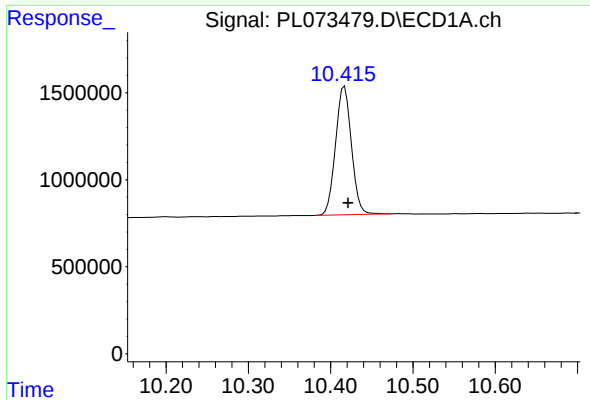

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.004 min
Response: 9895166
Conc: 19.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143454BL

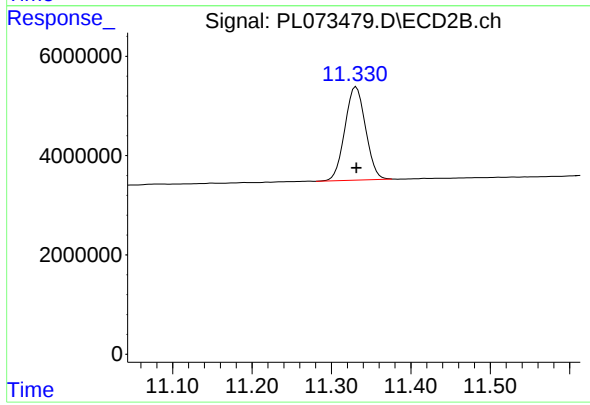

#28 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: 0.000 min
Response: 34115157
Conc: 19.08 ng/ml