

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
 Data File : PL073492.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2022 00:28
 Operator : AR\AJ
 Sample : PB143442BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB143442BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 02:52:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.492	5693158	30896675	17.775	18.825
28)	SA Decachlor...	10.418	11.332	9557368	33168883	18.795	18.549
Target Compounds							
6)	B beta-BHC	0.000	6.677	0	682277	N.D.	0.655 #
7)	B delta-BHC	0.000	6.954	0	1231198	N.D.	0.572 #
9)	A Endosulfan I	0.000	8.338	0	90414	N.D.	0.050 #
10)	B gamma-Chl...	0.000	8.200	0	504093	N.D.	0.247 #
13)	MA Dieldrin	0.000	8.605	0	10288	N.D.	0.006 #
15)	B Endosulfa...	8.357f	0.000	23057	0	0.059	N.D. #
20)	A Methoxychlor	9.111f	0.000	16210	0	0.063	N.D. #
23)	Chlordane-1	0.000	6.856	0	954369	N.D.	13.970 #
25)	Chlordane-3	0.000	8.200	0	504093	N.D.	1.859 #
27)	Chlordane-5	8.357f	0.000	23057	0	1.408	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
Data File : PL073492.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2022 00:28
Operator : AR\AJ
Sample : PB143442BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB143442BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 02:52:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

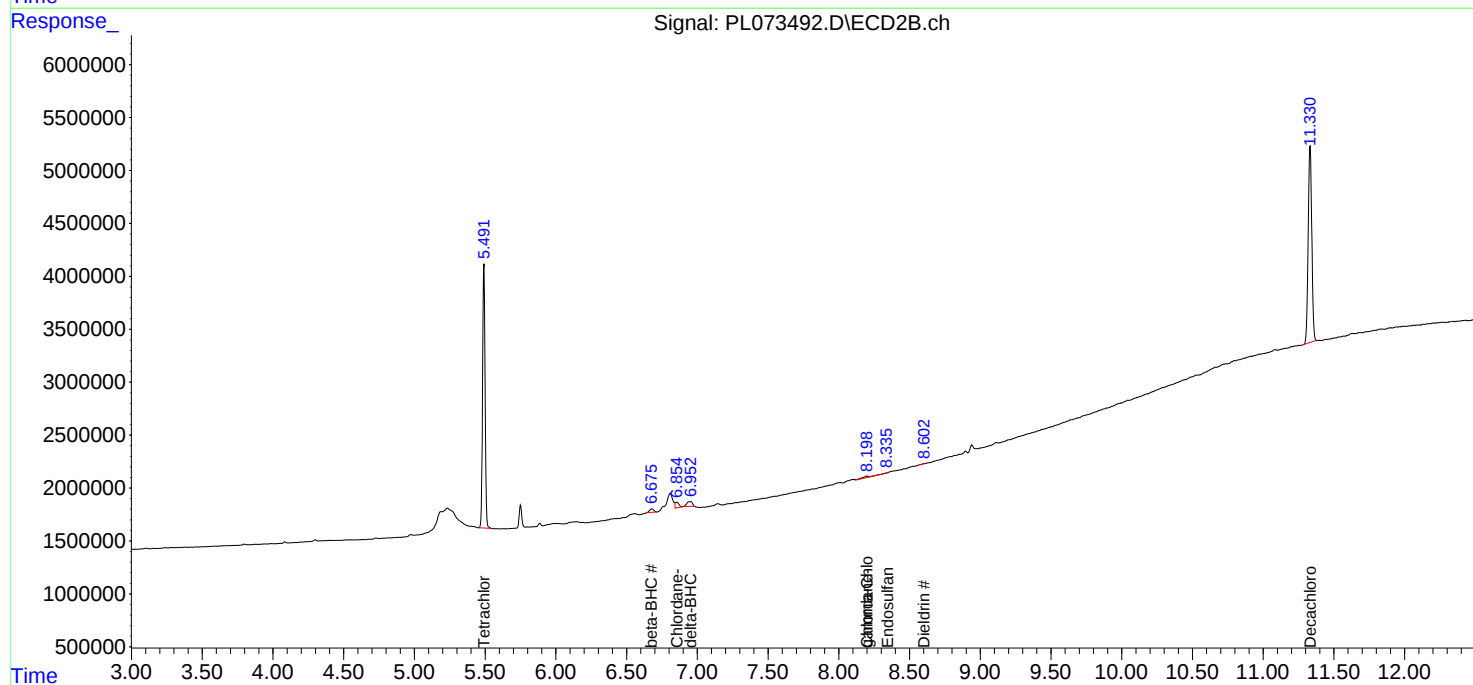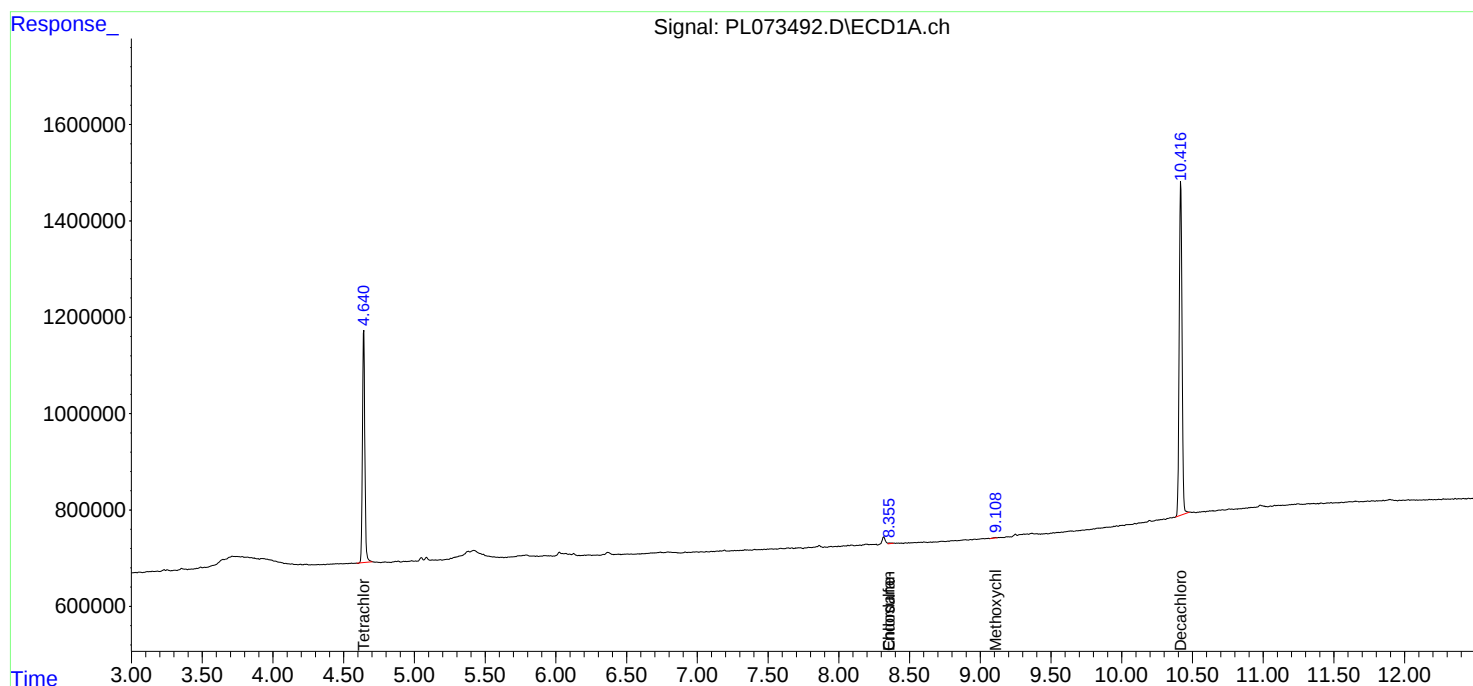


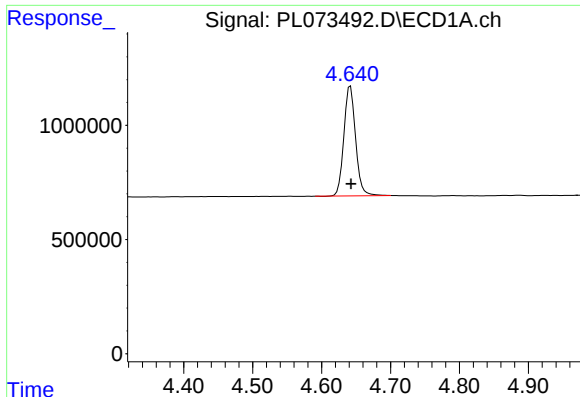

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.001 min
Response: 5693158
Conc: 17.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143442BL

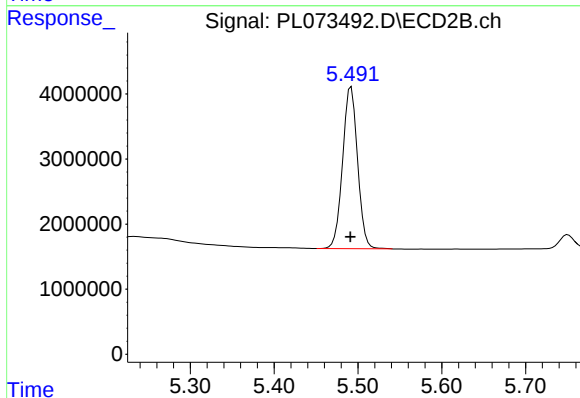


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 30896675
Conc: 18.83 ng/ml

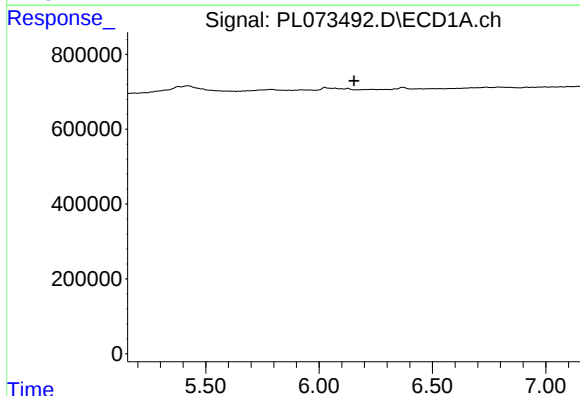


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

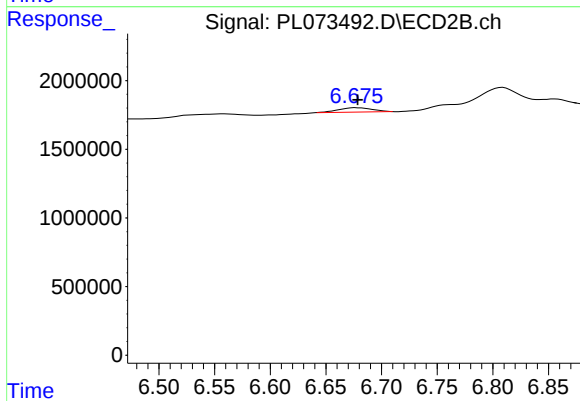

#6 beta-BHC


R.T.: 6.677 min
Delta R.T.: -0.002 min
Response: 682277
Conc: 0.65 ng/ml

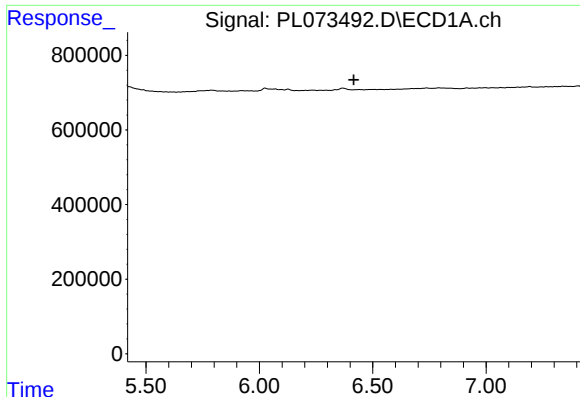

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143442BL

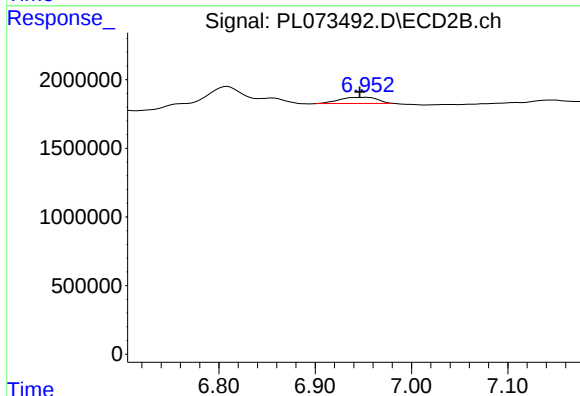


#7 delta-BHC

R.T.: 6.954 min
Delta R.T.: 0.007 min
Response: 1231198
Conc: 0.57 ng/ml

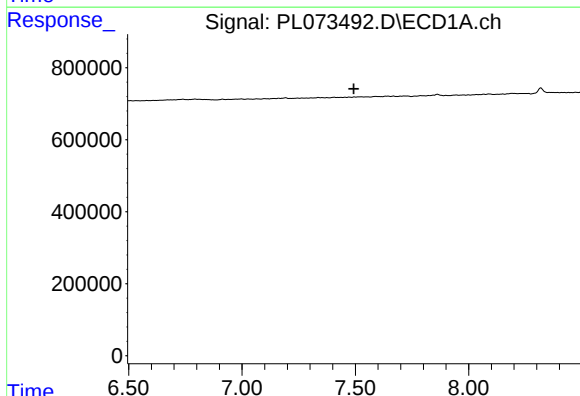


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.493 min
Response: 0
Conc: N.D.

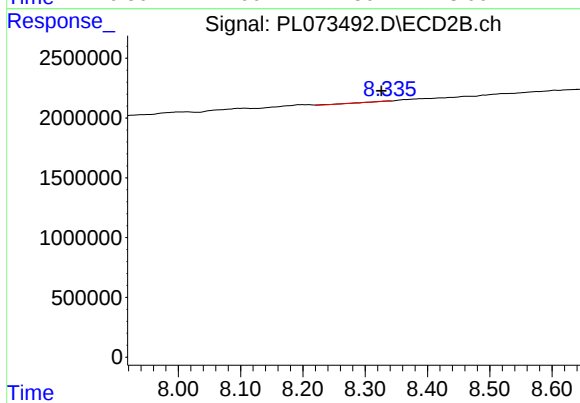

#9 Endosulfan I


R.T.: 8.338 min
Delta R.T.: 0.011 min
Response: 90414
Conc: 0.05 ng/ml

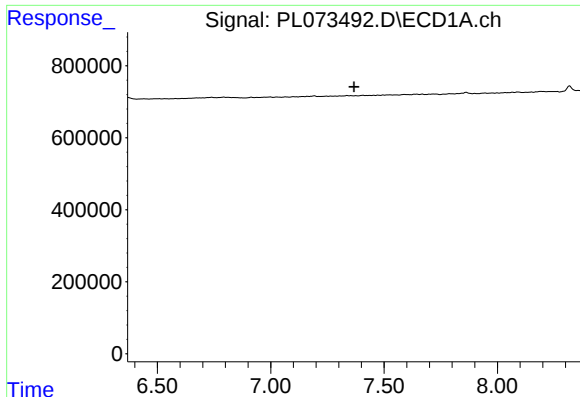

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143442BL

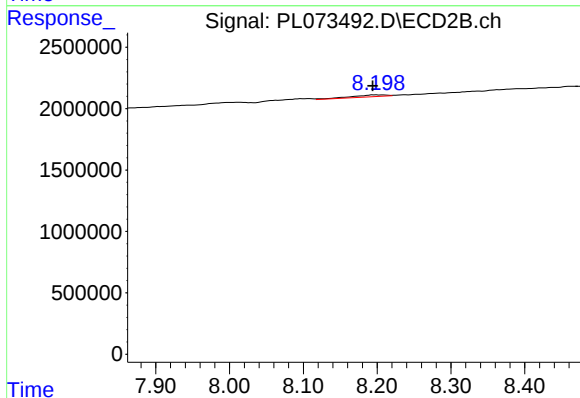


#10 gamma-Chlordane

R.T.: 8.200 min
Delta R.T.: 0.006 min
Response: 504093
Conc: 0.25 ng/ml

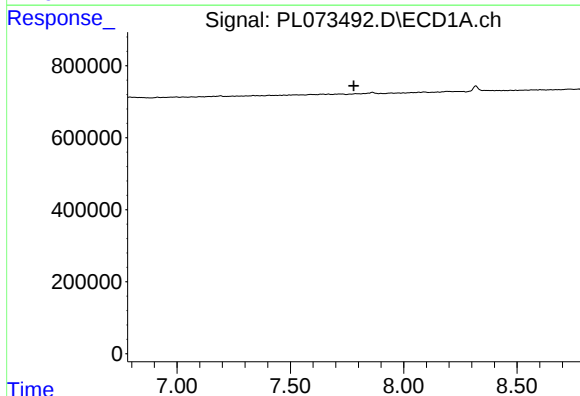


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.780 min
Response: 0
Conc: N.D.

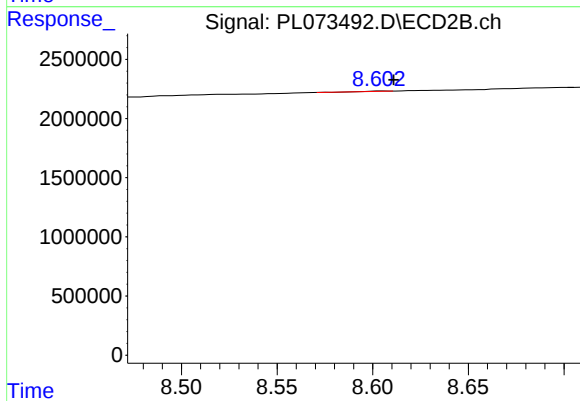

#13 Dieldrin


R.T.: 8.605 min
Delta R.T.: -0.006 min
Response: 10288
Conc: 0.01 ng/ml

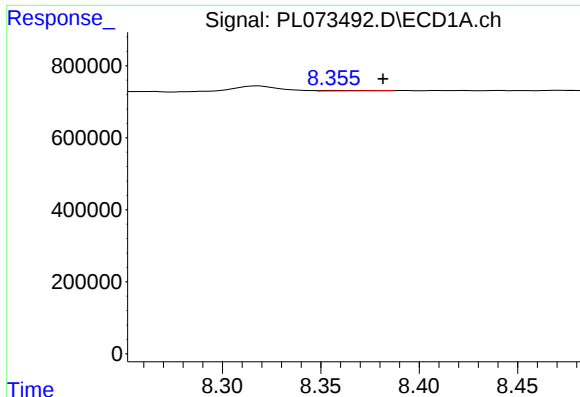

#15 Endosulfan II


R.T.: 8.357 min
Delta R.T.: -0.025 min
Response: 23057
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143442BL

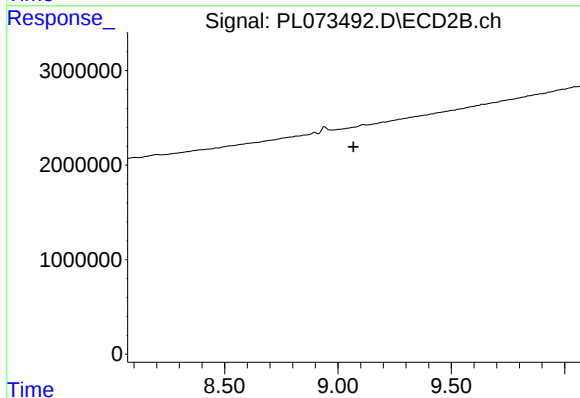


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.069 min
Response: 0
Conc: N.D.

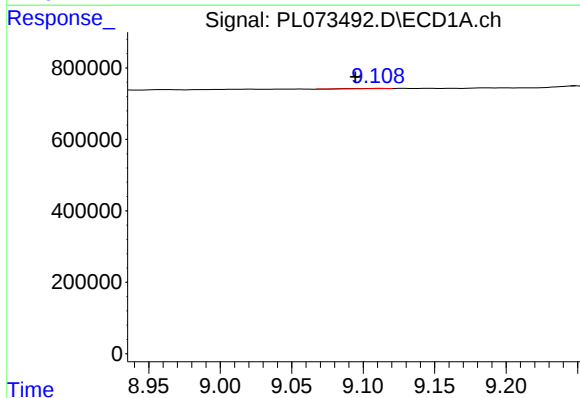


#20 Methoxychlor

R.T.: 9.111 min
Delta R.T.: 0.016 min
Response: 16210
Conc: 0.06 ng/ml

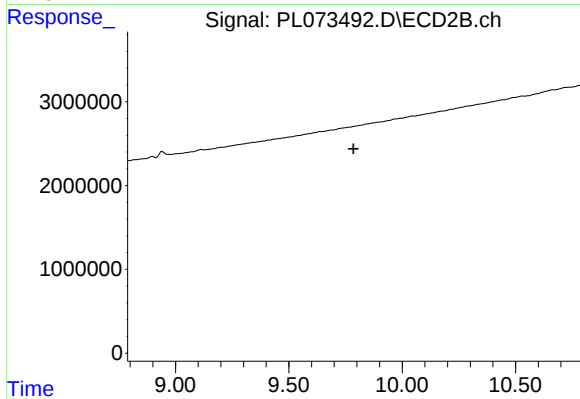

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 9.786 min
Response: 0
Conc: N.D.

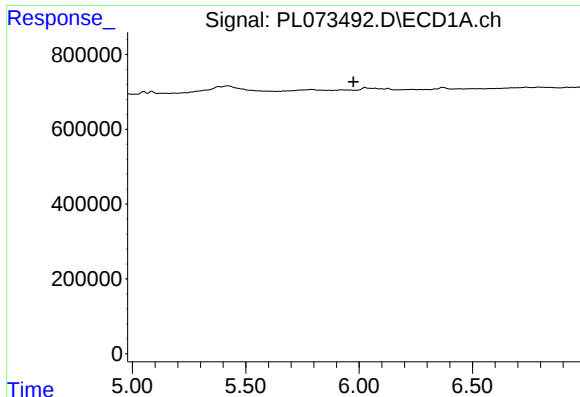

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143442BL

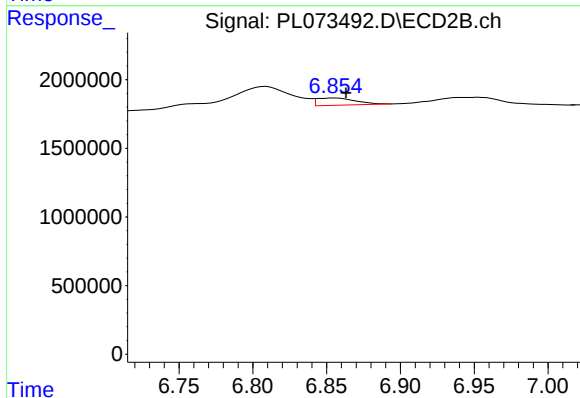


#23 Chlordane-1

R.T.: 6.856 min
Delta R.T.: -0.008 min
Response: 954369
Conc: 13.97 ng/ml

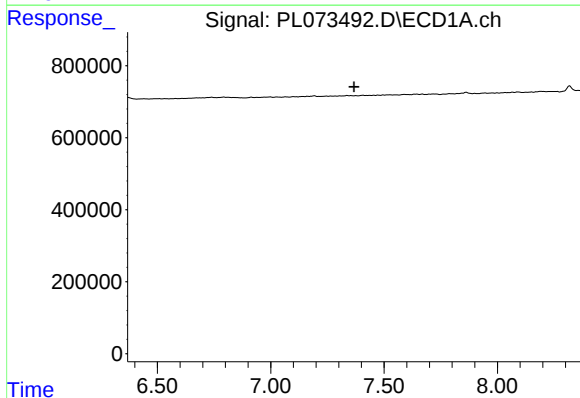


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

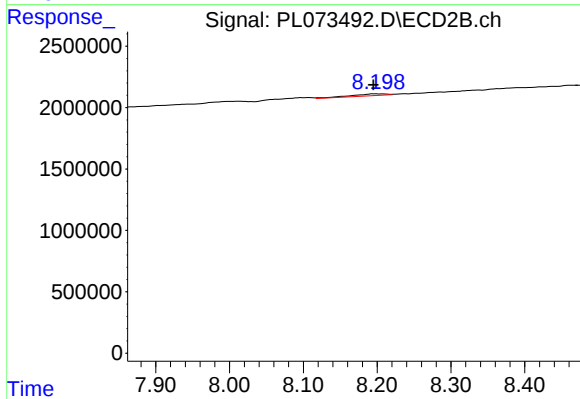

#25 Chlordane-3


R.T.: 8.200 min
Delta R.T.: 0.005 min
Response: 504093
Conc: 1.86 ng/ml

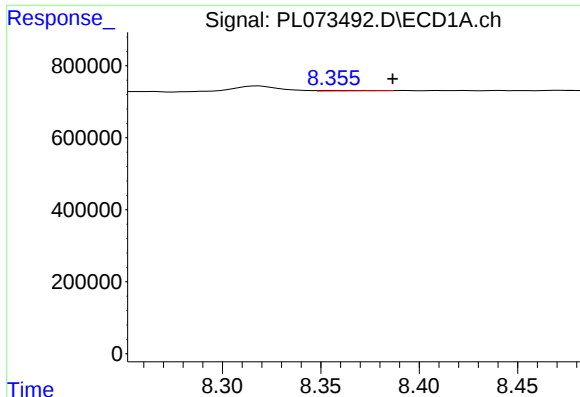

#27 Chlordane-5


R.T.: 8.357 min
Delta R.T.: -0.030 min
Response: 23057
Conc: 1.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143442BL

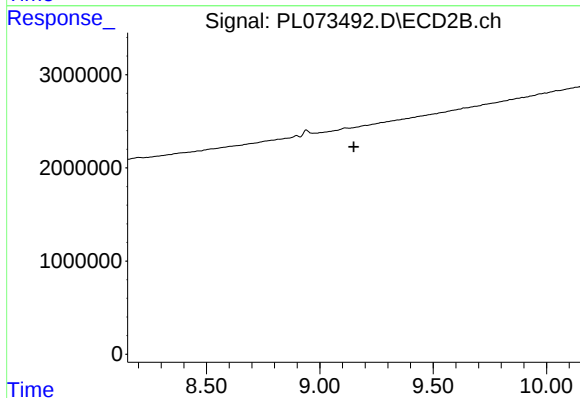


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.149 min
Response: 0
Conc: N.D.

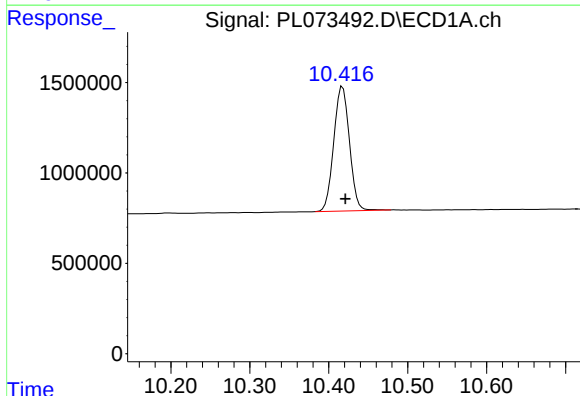

#28 Decachlorobiphenyl

R.T.: 10.418 min
Delta R.T.: -0.003 min
Response: 9557368
Conc: 18.80 ng/ml

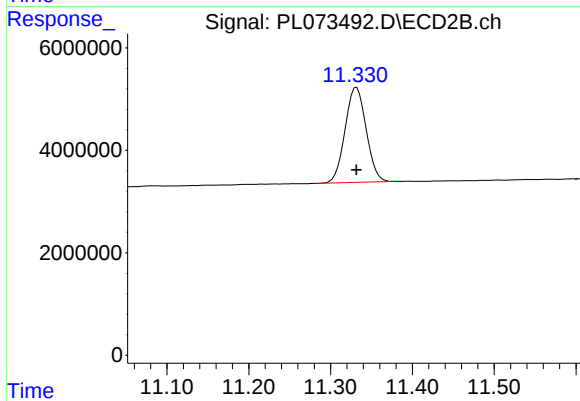

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 33168883
Conc: 18.55 ng/ml