

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
 Data File : PL073494.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2022 01:01
 Operator : AR\AJ
 Sample : PB143437TB
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB143437TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 02:53:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.492	5817744	31060757	18.164	18.925
28)	SA Decachlor...	10.416	11.332	9857448	33907895	19.385	18.962
Target Compounds							
6)	B beta-BHC	0.000	6.681	0	687183	N.D.	0.659 #
7)	B delta-BHC	0.000	6.958	0	1427769	N.D.	0.663 #
8)	B Heptachlo...	0.000	7.935	0	38557	N.D.	0.019 #
10)	B gamma-Chl...	0.000	8.194	0	435455	N.D.	0.213 #
11)	B alpha-Chl...	0.000	8.285	0	159053	N.D.	0.080 #
13)	MA Dieldrin	0.000	8.599	0	59375	N.D.	0.032 #
14)	MA Endrin	0.000	8.859	0	22811	N.D.	0.015 #
22)	Mirex	0.000	10.421f	0	110474	N.D.	0.081 #
23)	Chlordane-1	0.000	6.856	0	968693	N.D.	14.180 #
25)	Chlordane-3	0.000	8.194	0	435455	N.D.	1.606 #
26)	Chlordane-4	0.000	8.285	0	159053	N.D.	0.480 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
Data File : PL073494.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2022 01:01
Operator : AR\AJ
Sample : PB143437TB
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB143437TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 02:53:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

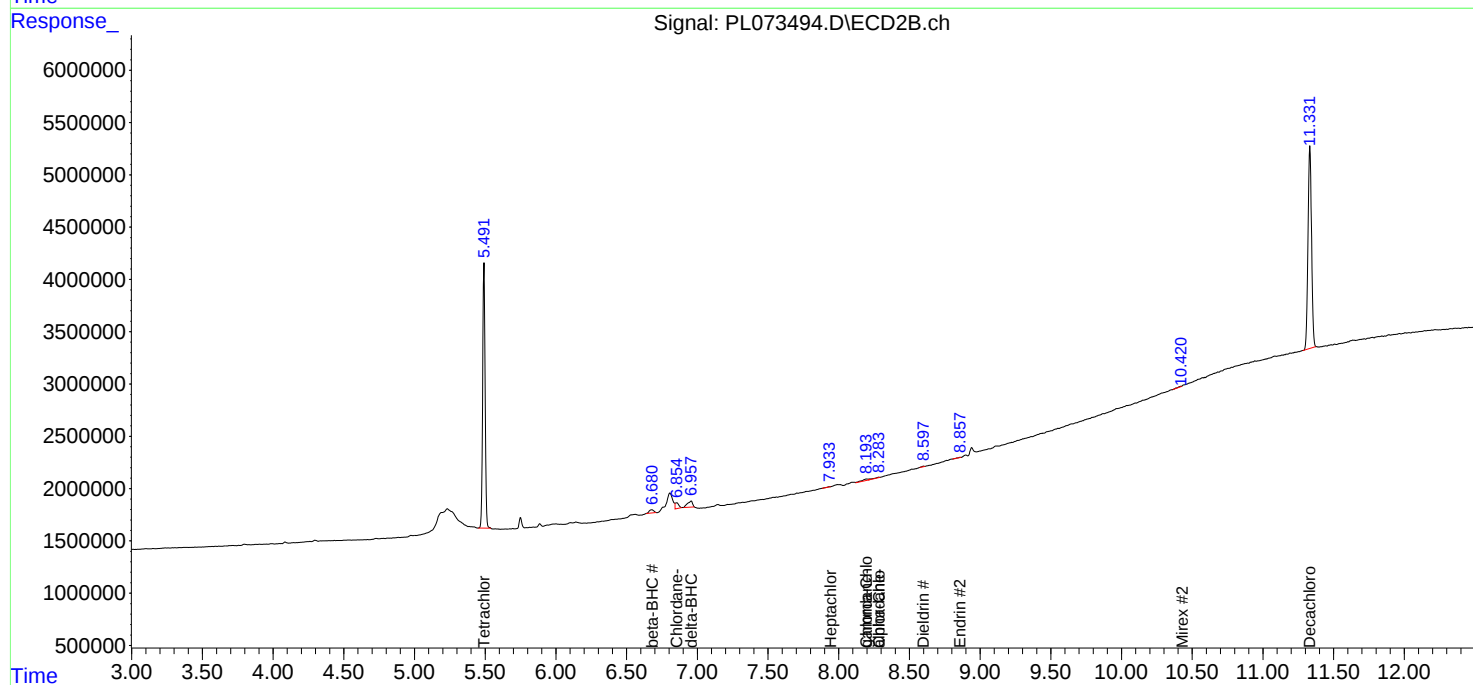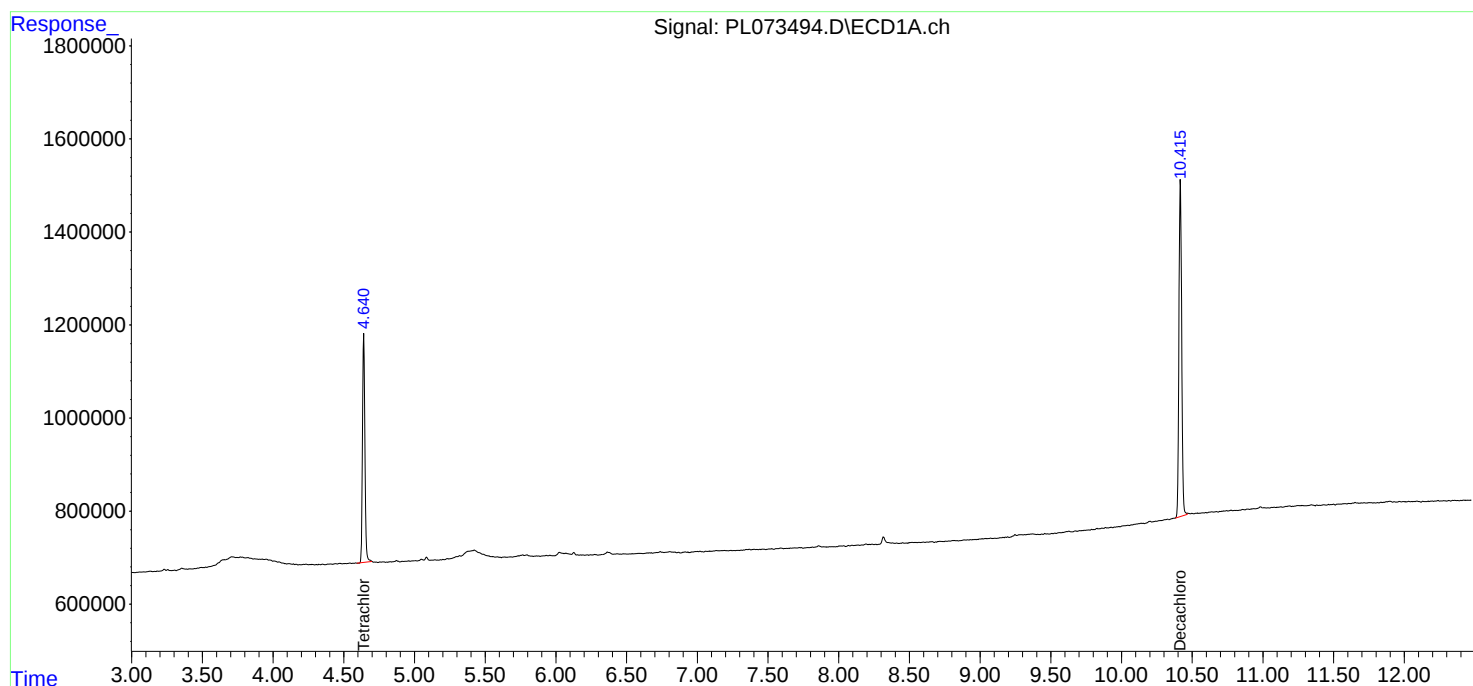


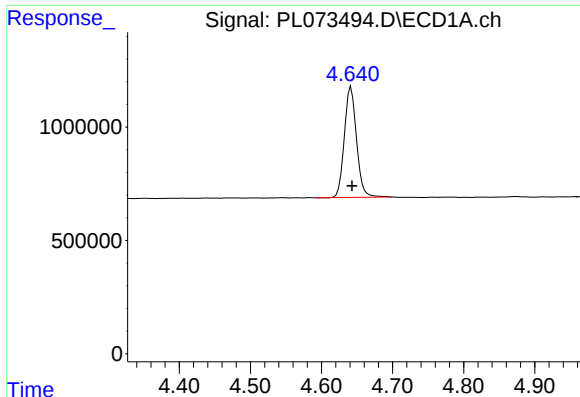

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.001 min
Response: 5817744
Conc: 18.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143437TB

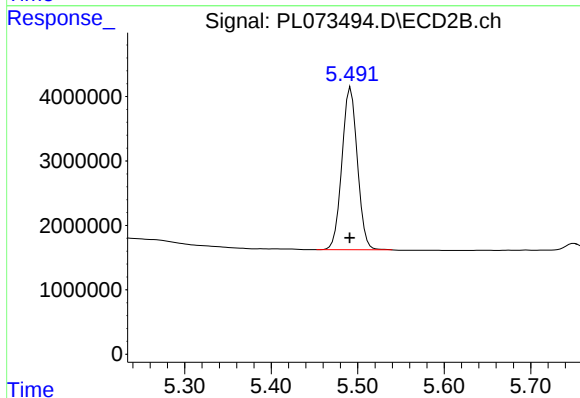


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 31060757
Conc: 18.93 ng/ml

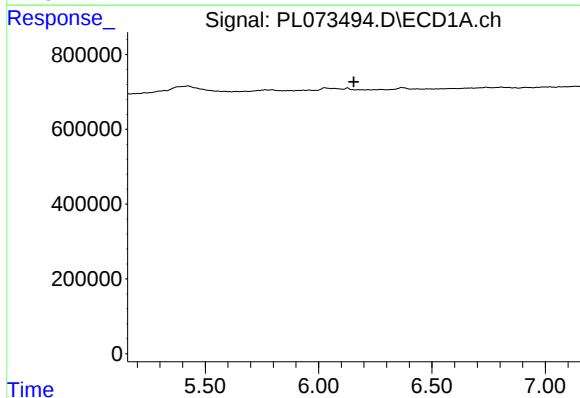


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

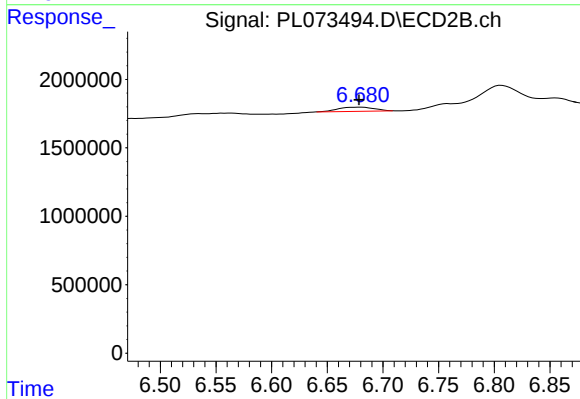

#6 beta-BHC


R.T.: 6.681 min
Delta R.T.: 0.002 min
Response: 687183
Conc: 0.66 ng/ml

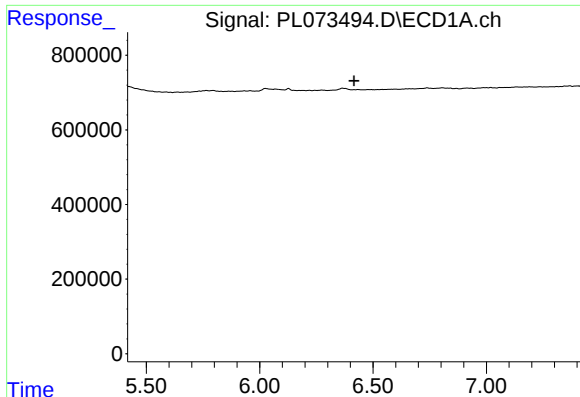

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143437TB

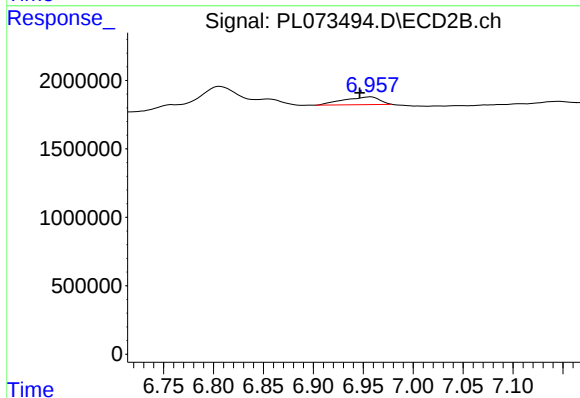


#7 delta-BHC

R.T.: 6.958 min
Delta R.T.: 0.011 min
Response: 1427769
Conc: 0.66 ng/ml

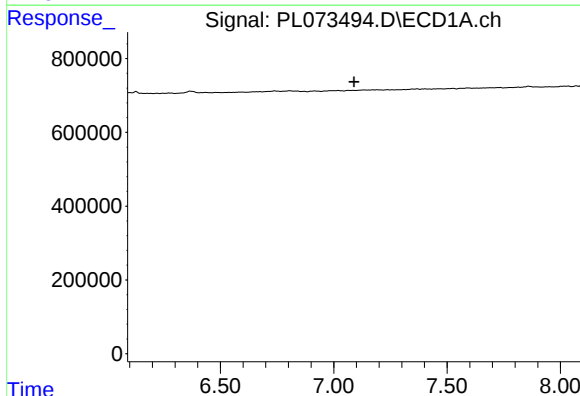


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.090 min
Response: 0
Conc: N.D.

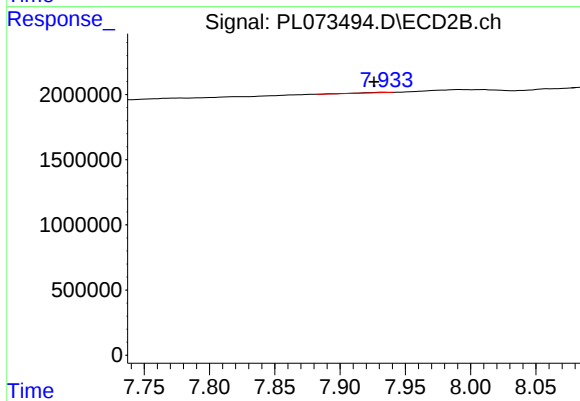

#8 Heptachlor epoxide


R.T.: 7.935 min
Delta R.T.: 0.009 min
Response: 38557
Conc: 0.02 ng/ml

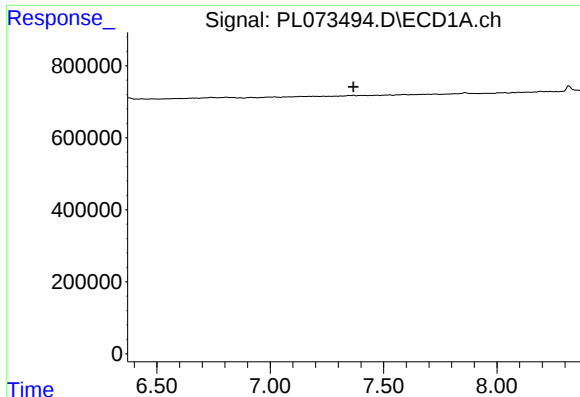

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143437TB

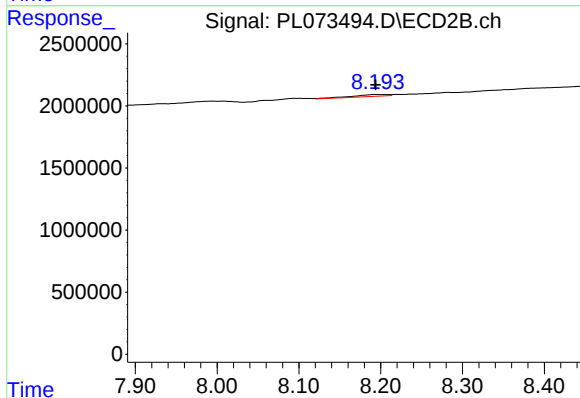


#10 gamma-Chlordane

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 435455
Conc: 0.21 ng/ml

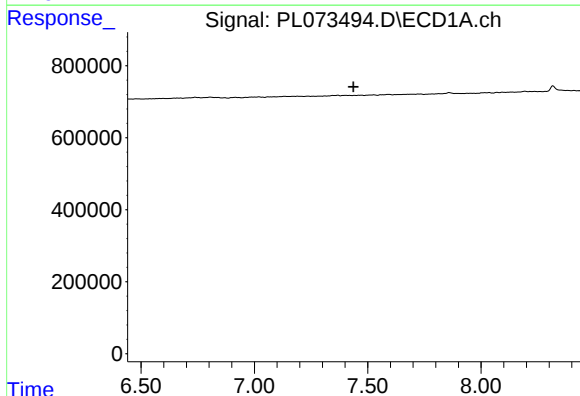


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

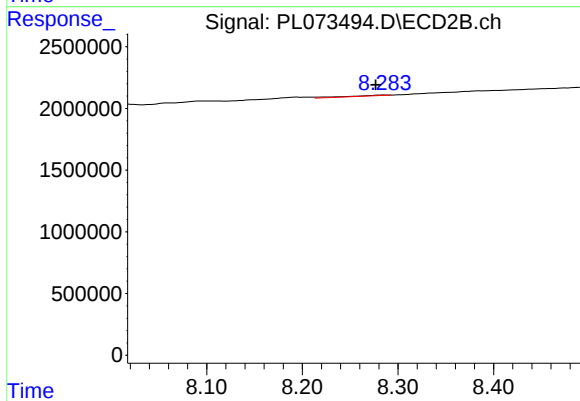

#11 alpha-Chlordane


R.T.: 8.285 min
Delta R.T.: 0.008 min
Response: 159053
Conc: 0.08 ng/ml

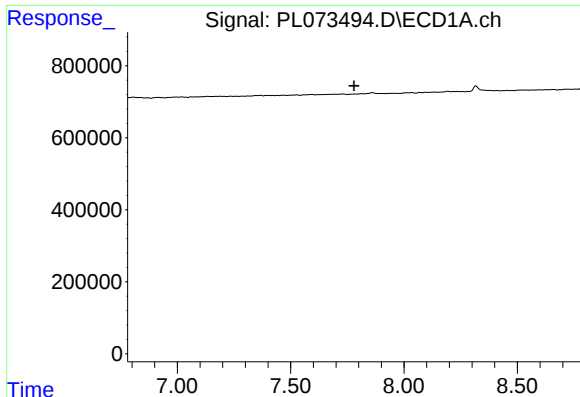

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 7.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143437TB

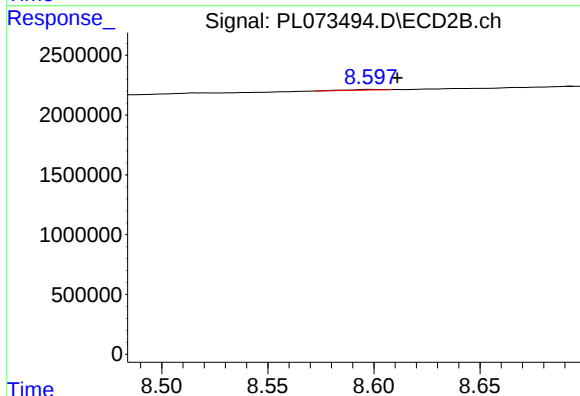


#13 Dieldrin

R.T.: 8.599 min
Delta R.T.: -0.012 min
Response: 59375
Conc: 0.03 ng/ml

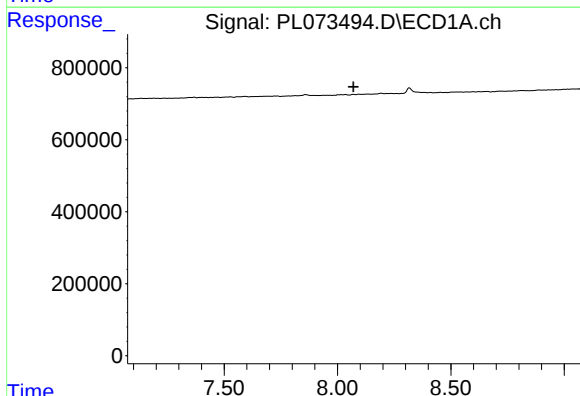


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 8.071 min
Response: 0
Conc: N.D.

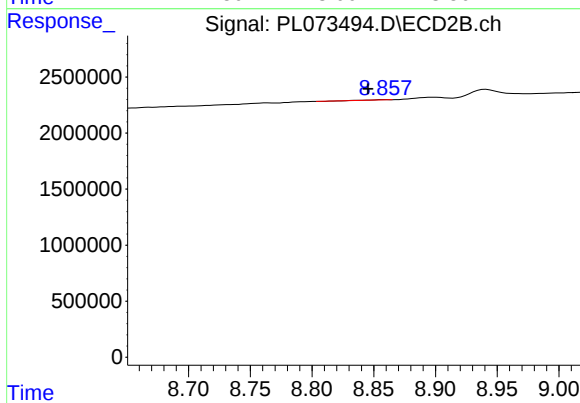

#14 Endrin


R.T.: 8.859 min
Delta R.T.: 0.014 min
Response: 22811
Conc: 0.01 ng/ml

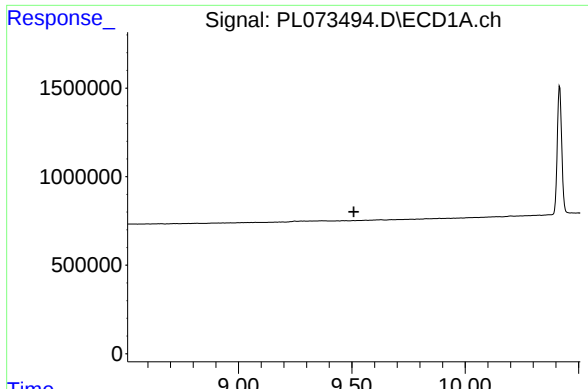

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143437TB

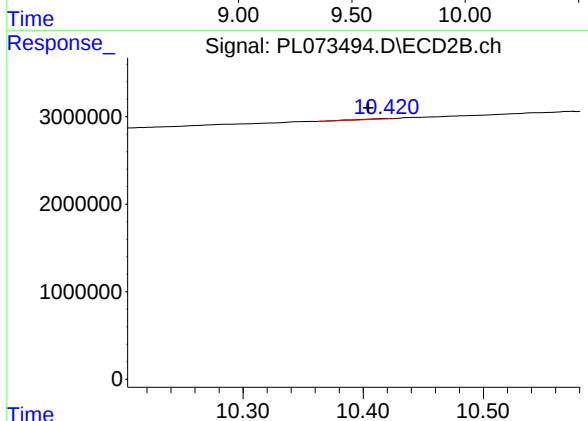


#22 Mirex

R.T.: 10.421 min
Delta R.T.: 0.016 min
Response: 110474
Conc: 0.08 ng/ml

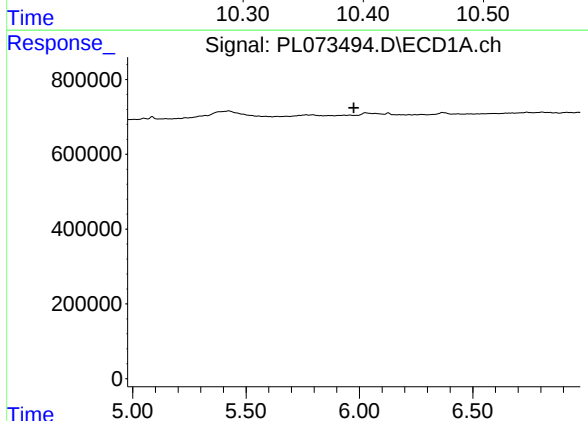


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

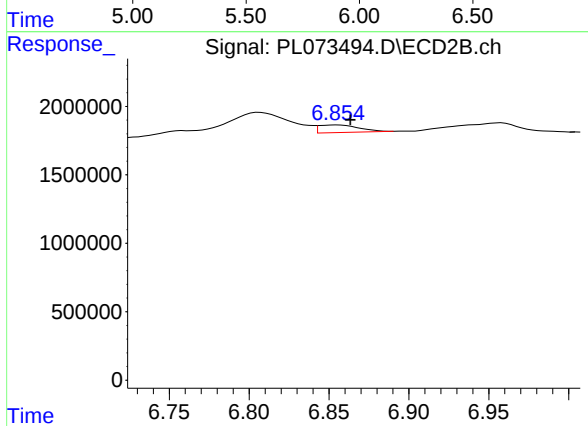

#23 Chlordane-1


R.T.: 6.856 min
Delta R.T.: -0.008 min
Response: 968693
Conc: 14.18 ng/ml

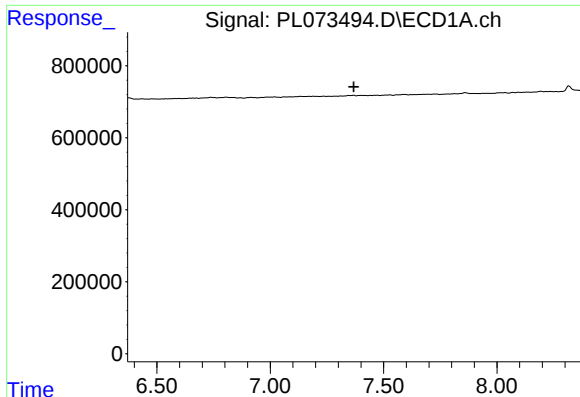

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143437TB

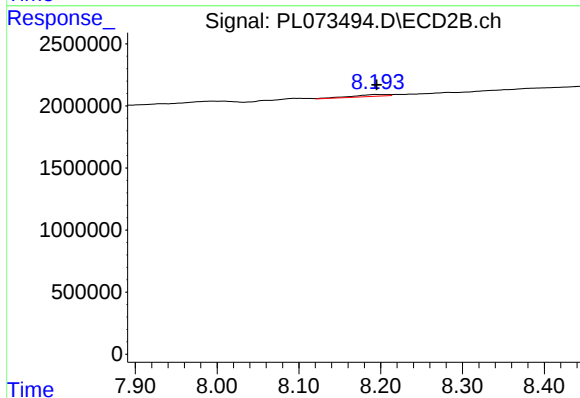


#25 Chlordane-3

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 435455
Conc: 1.61 ng/ml

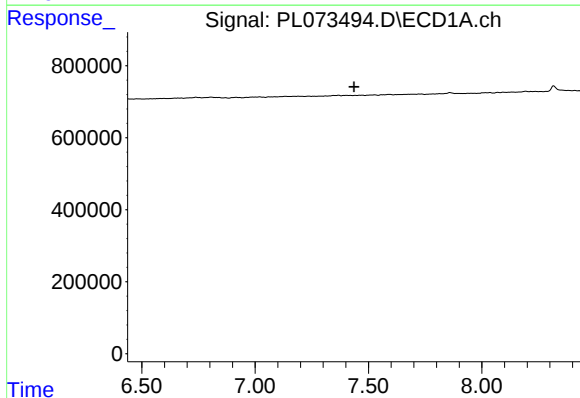


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

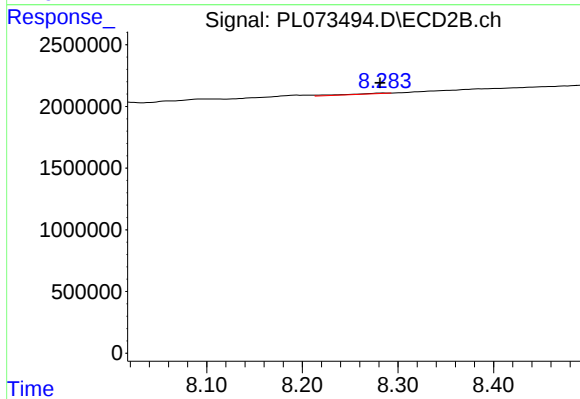

#26 Chlordane-4


R.T.: 8.285 min
Delta R.T.: 0.004 min
Response: 159053
Conc: 0.48 ng/ml

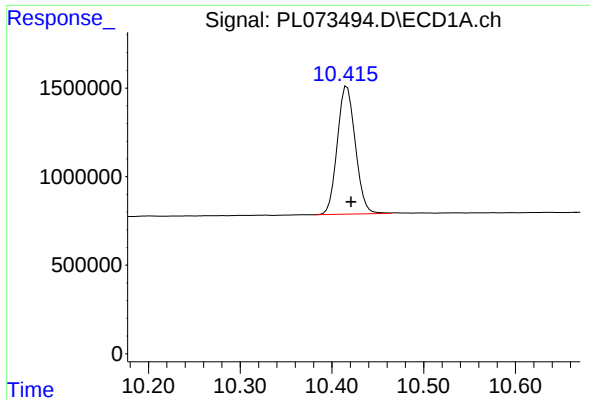

#28 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: -0.004 min
Response: 9857448
Conc: 19.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143437TB

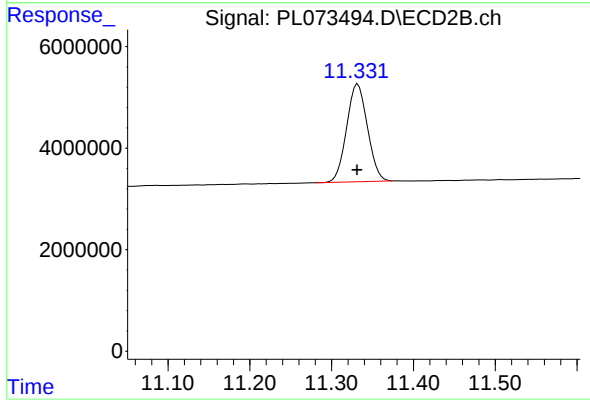

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 33907895
Conc: 18.96 ng/ml