

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
 Data File : PL073510.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2022 06:46
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 02:58:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.492	7963113	43953723	24.863	26.781
28)	SA Decachlor...	10.417	11.333	12008861	43231629	23.616	24.176
Target Compounds							
6)	B beta-BHC	0.000	6.679	0	720148	N.D.	0.691 #
7)	B delta-BHC	0.000	6.960	0	2555716	N.D.	1.187 #
8)	B Heptachlo...	0.000	7.927	0	2386704	N.D.	1.195 #
9)	A Endosulfan I	7.474f	0.000	15996	0	0.039	N.D. #
10)	B gamma-Chl...	7.355	8.194	45353	4295129	0.104	2.103 #
13)	MA Dieldrin	7.788	0.000	405316	0	0.973	N.D. #
14)	MA Endrin	8.092f	0.000	660558	0	1.702	N.D. #
15)	B Endosulfa...	0.000	9.055	0	3420699	N.D.	2.227 #
20)	A Methoxychlor	9.101	0.000	43488	0	0.170	N.D. #
23)	Chlordane-1	0.000	6.854	0	967231	N.D.	14.159 #
25)	Chlordane-3	7.355	8.194	45353	4295129	1.111	15.841 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
Data File : PL073510.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2022 06:46
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 02:58:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

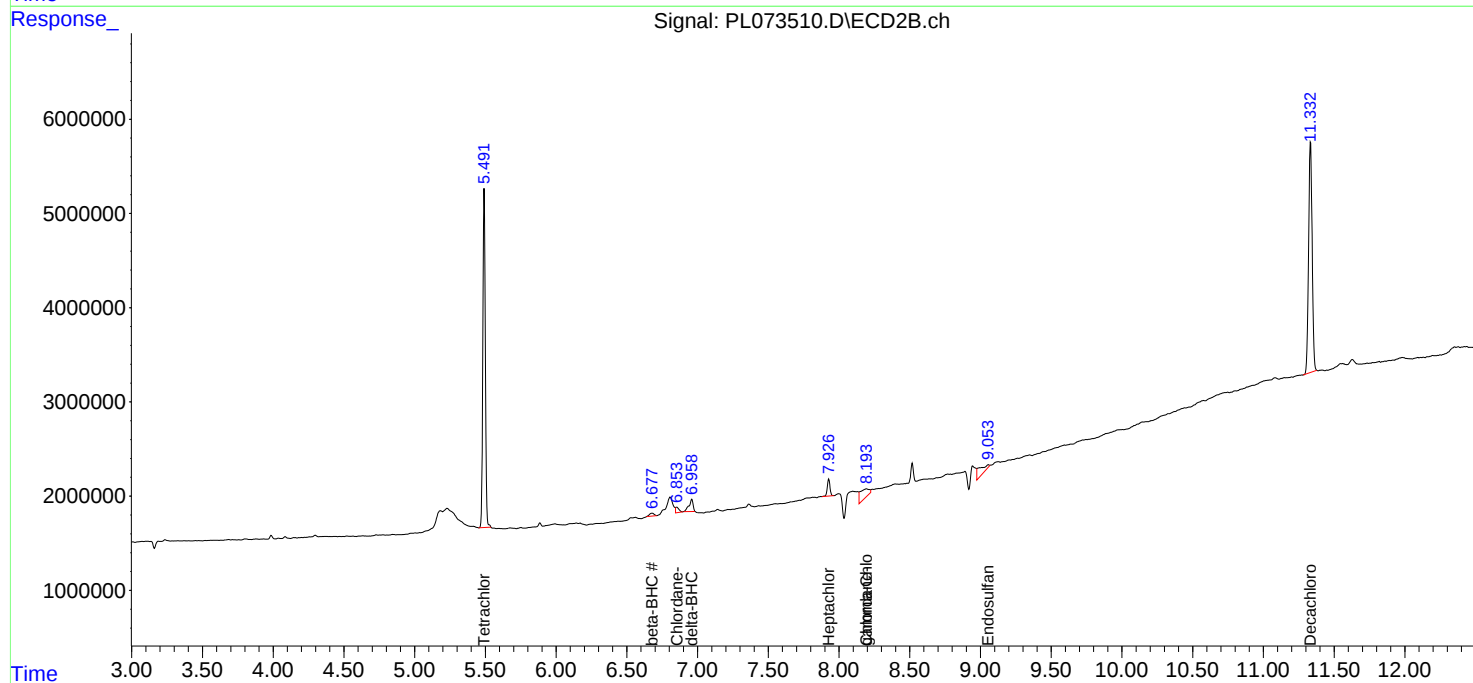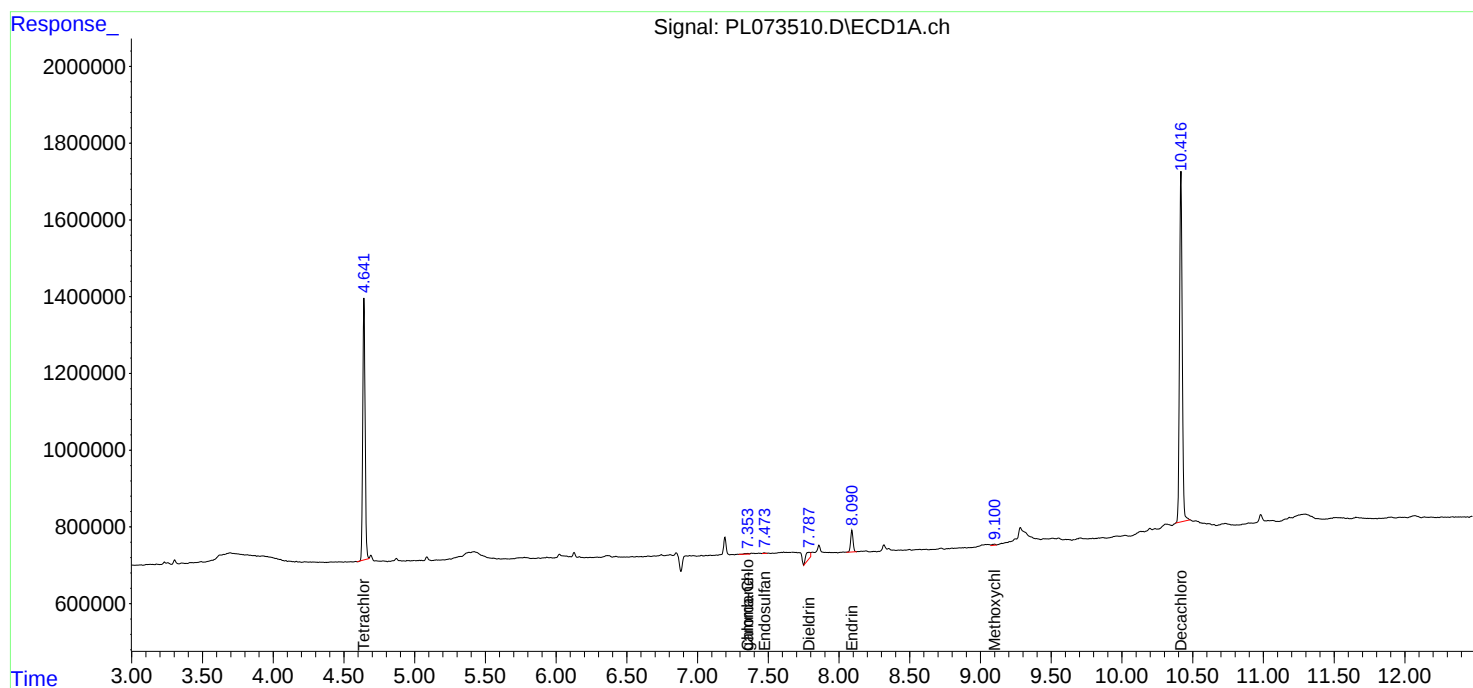


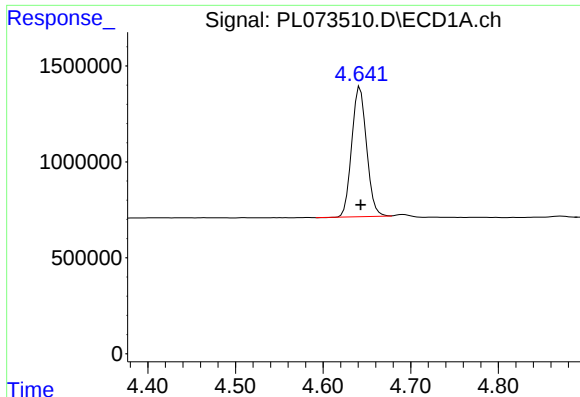

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 7963113
Conc: 24.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

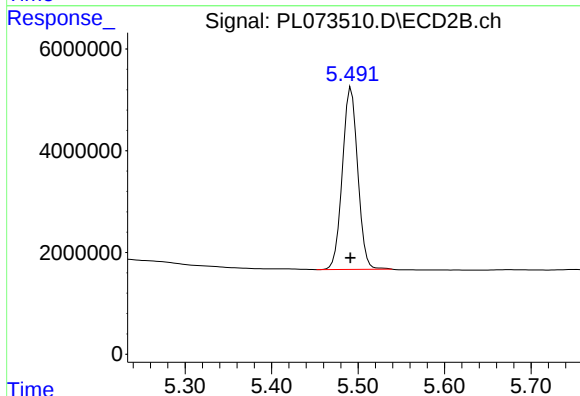


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 43953723
Conc: 26.78 ng/ml

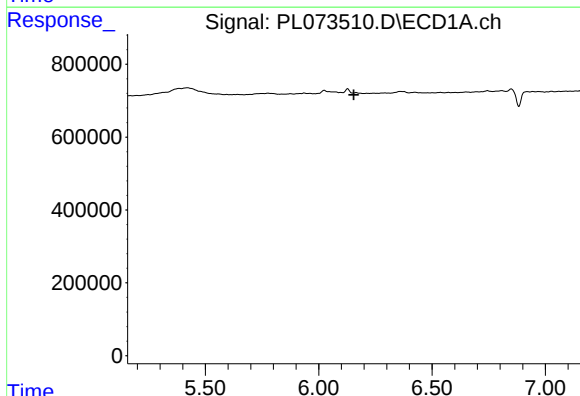


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

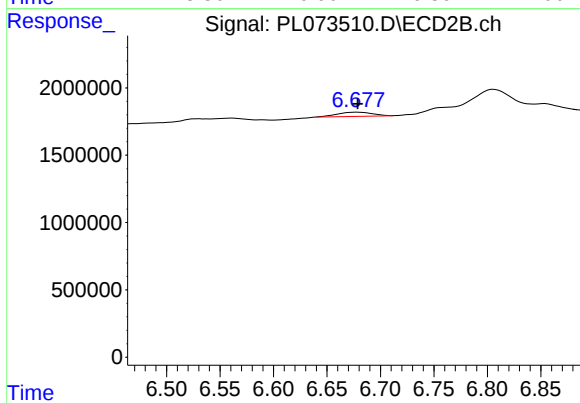

#6 beta-BHC


R.T.: 6.679 min
Delta R.T.: 0.000 min
Response: 720148
Conc: 0.69 ng/ml

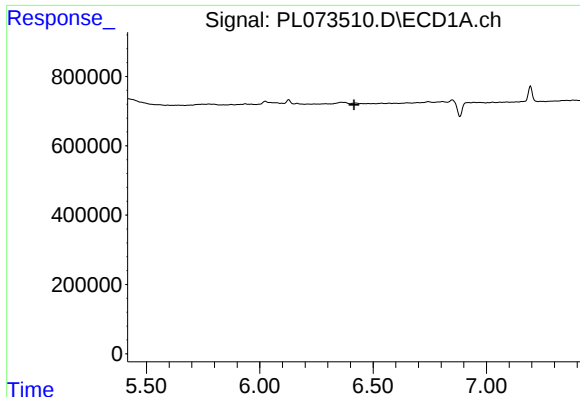

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

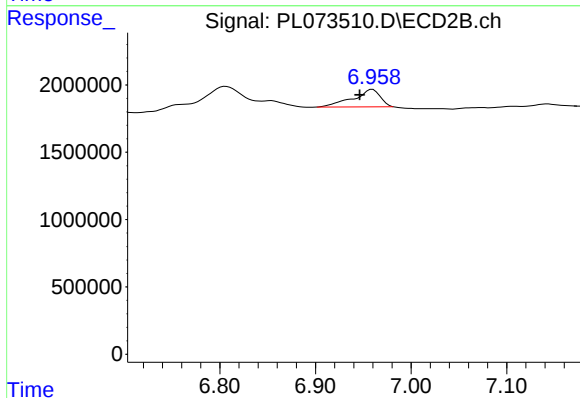


#7 delta-BHC

R.T.: 6.960 min
Delta R.T.: 0.013 min
Response: 2555716
Conc: 1.19 ng/ml

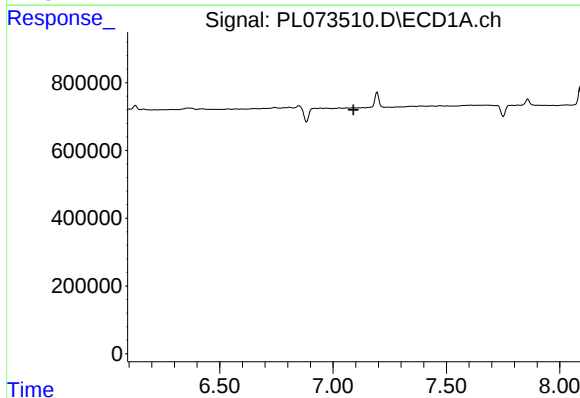


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 7.090 min
Response: 0
Conc: N.D.

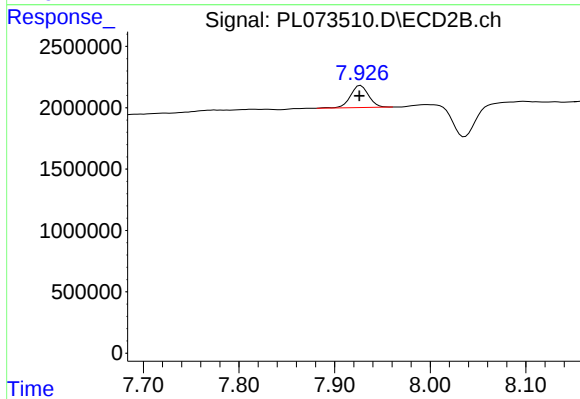

#8 Heptachlor epoxide


R.T.: 7.927 min
Delta R.T.: 0.001 min
Response: 2386704
Conc: 1.19 ng/ml

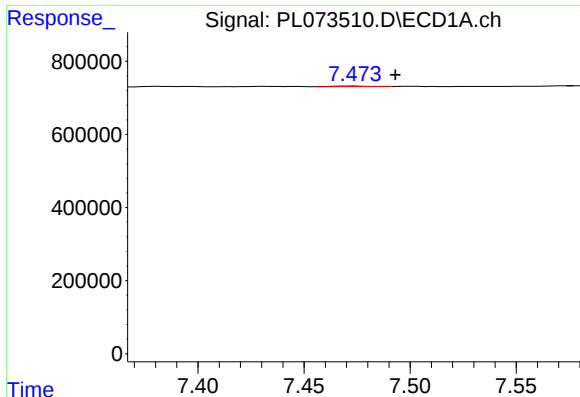

#9 Endosulfan I


R.T.: 7.474 min
Delta R.T.: -0.019 min
Response: 15996
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

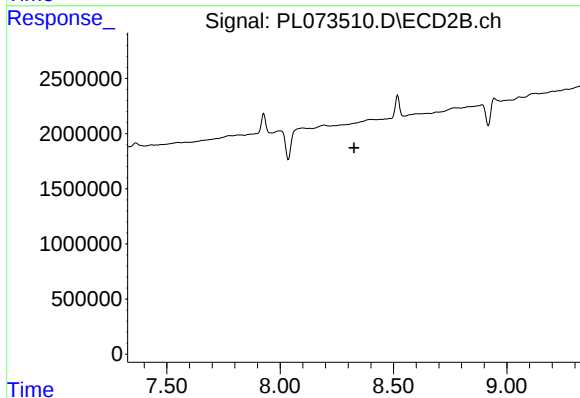


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 8.326 min
Response: 0
Conc: N.D.

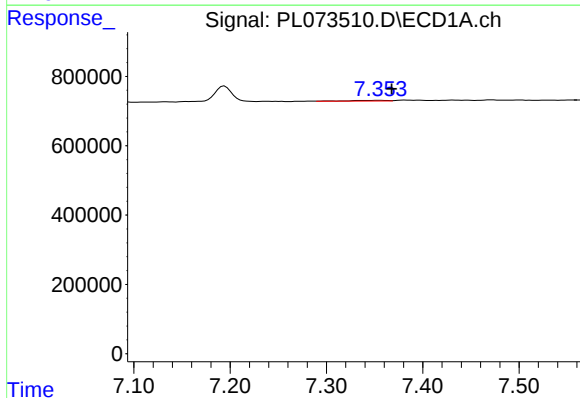


#10 gamma-Chlordane

R.T.: 7.355 min
Delta R.T.: -0.013 min
Response: 45353
Conc: 0.10 ng/ml

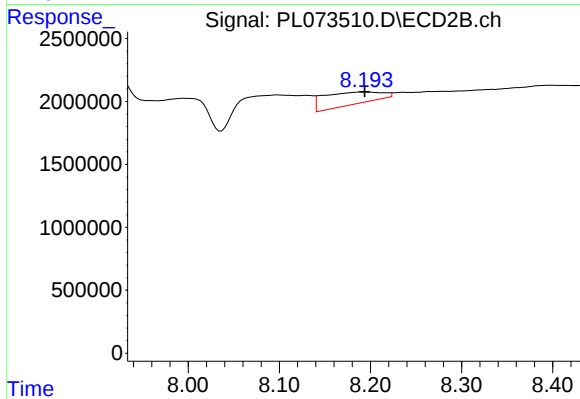

#10 gamma-Chlordane


R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 4295129
Conc: 2.10 ng/ml

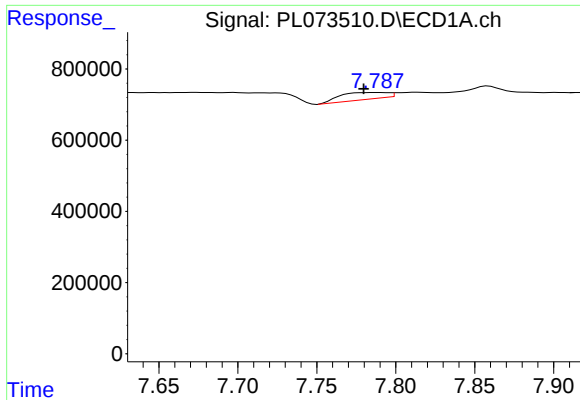

#13 Dieldrin


R.T.: 7.788 min
Delta R.T.: 0.009 min
Response: 405316
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

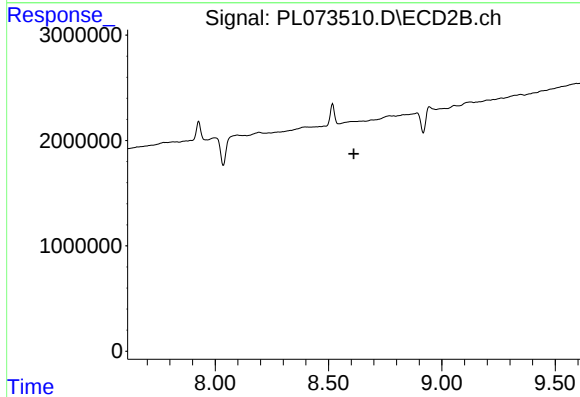


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.611 min
Response: 0
Conc: N.D.

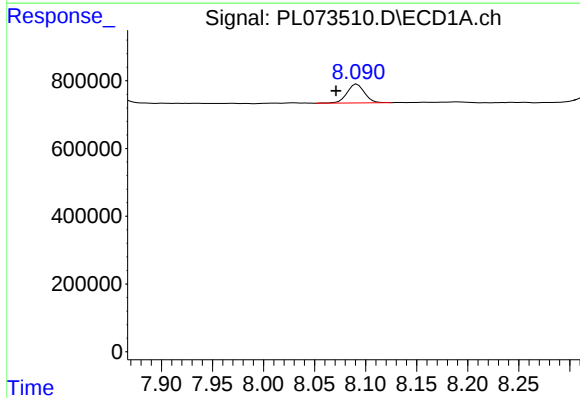


#14 Endrin

R.T.: 8.092 min
Delta R.T.: 0.021 min
Response: 660558
Conc: 1.70 ng/ml

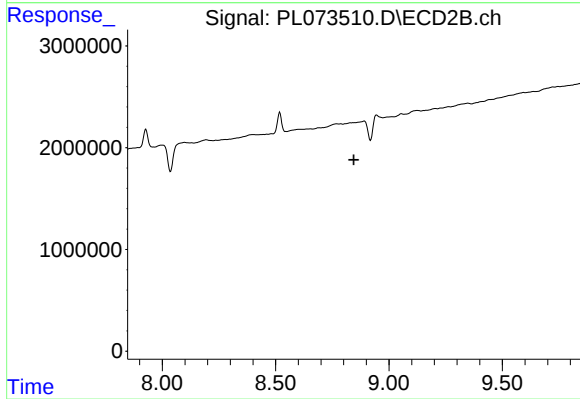

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.845 min
Response: 0
Conc: N.D.

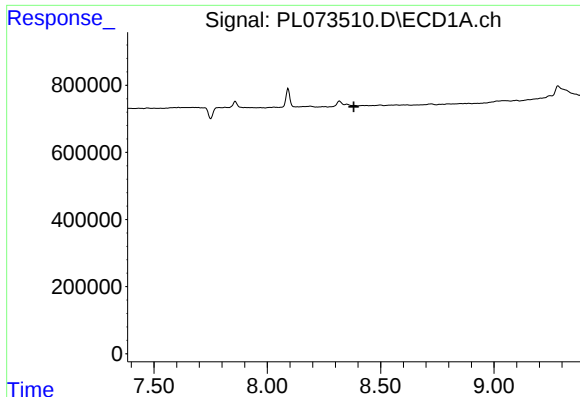

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

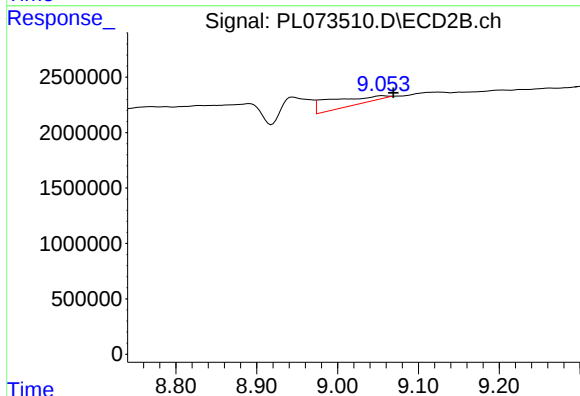


#15 Endosulfan II

R.T.: 9.055 min
Delta R.T.: -0.014 min
Response: 3420699
Conc: 2.23 ng/ml

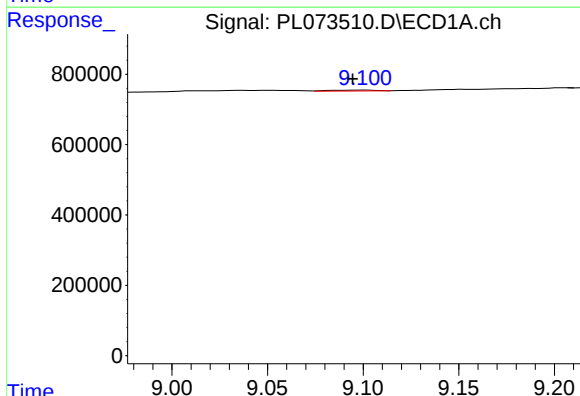


#20 Methoxychlor

R.T.: 9.101 min
Delta R.T.: 0.006 min
Response: 43488
Conc: 0.17 ng/ml

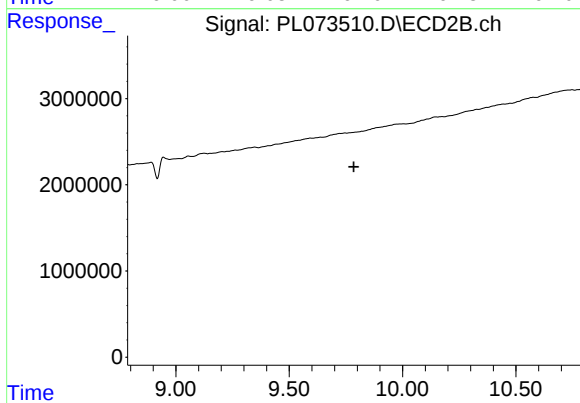

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.786 min
Response: 0
Conc: N.D.

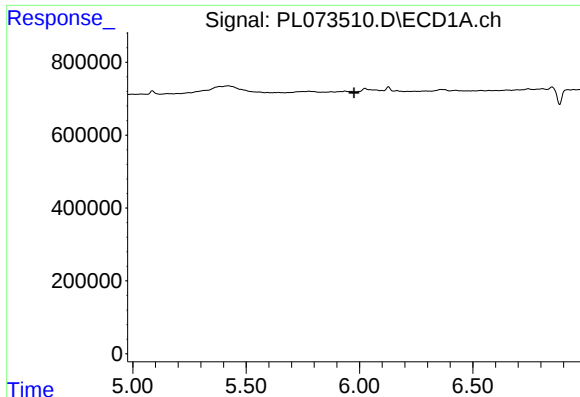

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

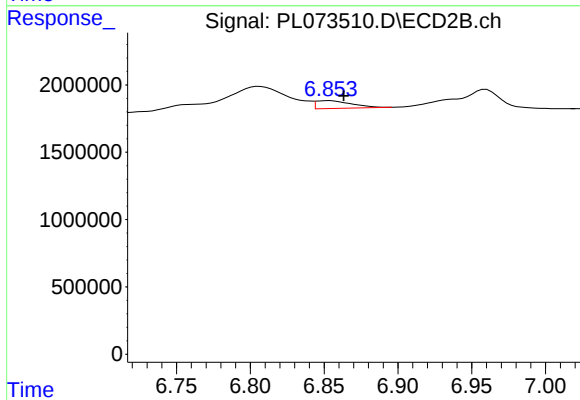


#23 Chlordane-1

R.T.: 6.854 min
Delta R.T.: -0.009 min
Response: 967231
Conc: 14.16 ng/ml

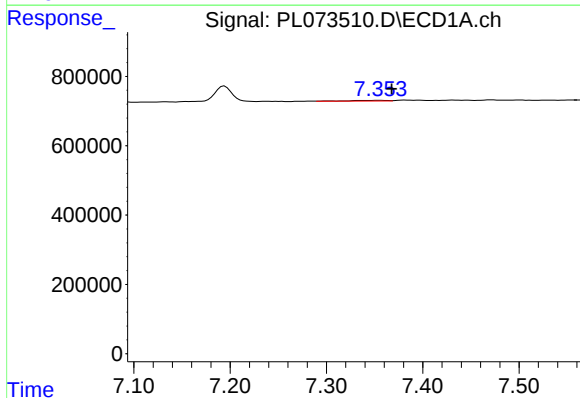


#25 Chlordane-3

R.T.: 7.355 min
Delta R.T.: -0.013 min
Response: 45353
Conc: 1.11 ng/ml

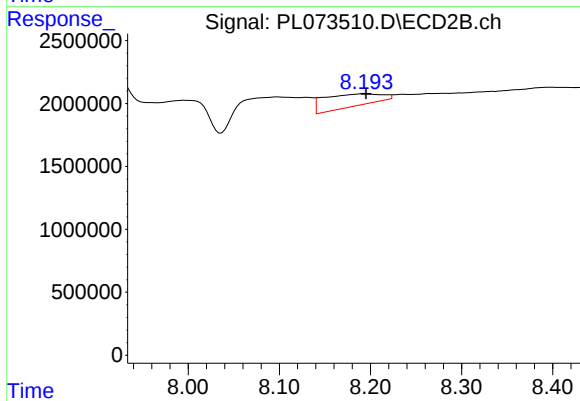

#25 Chlordane-3


R.T.: 8.194 min
Delta R.T.: -0.001 min
Response: 4295129
Conc: 15.84 ng/ml

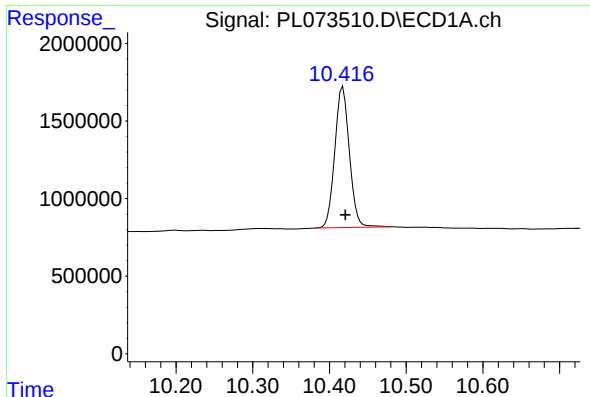

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.004 min
Response: 12008861
Conc: 23.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

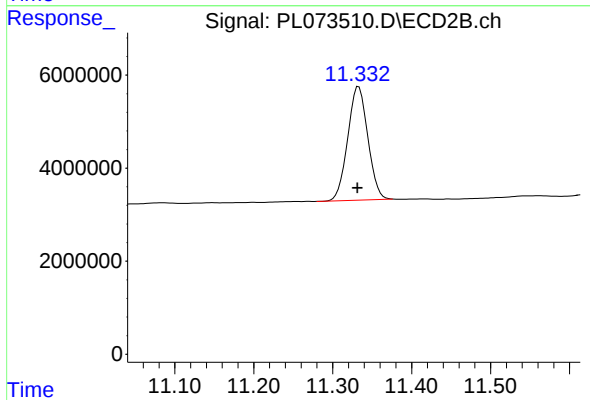

#28 Decachlorobiphenyl

R.T.: 11.333 min
Delta R.T.: 0.002 min
Response: 43231629
Conc: 24.18 ng/ml