

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
 Data File : PL073475.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2022 16:30
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 00:54:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.492	18325860	83972164	57.217	51.164
28)	SA Decachlor...	10.418	11.332	22848371	79600745	44.933	44.515
Target Compounds							
23)	Chlordane-1	5.974	6.864	5329261	32816520	449.537	480.383
24)	Chlordane-2	6.663	7.445	7279950	34877895	446.270	485.266
25)	Chlordane-3	7.366	8.195	18100166	136.1E6	443.261	501.859
26)	Chlordane-4	7.434	8.281	19460209	164.7E6	439.076	497.342
27)	Chlordane-5	8.384	9.150	7206691	25890354	440.096	477.001



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
Data File : PL073475.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2022 16:30
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 00:54:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

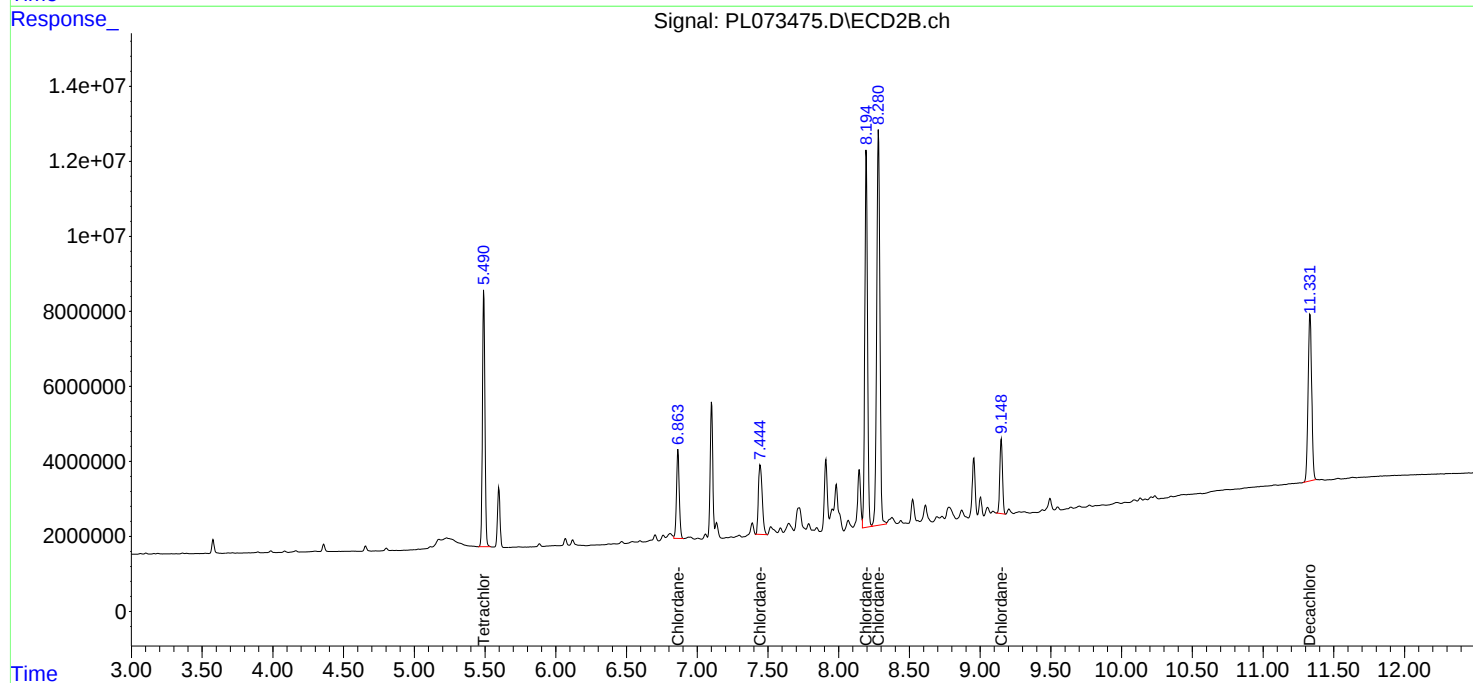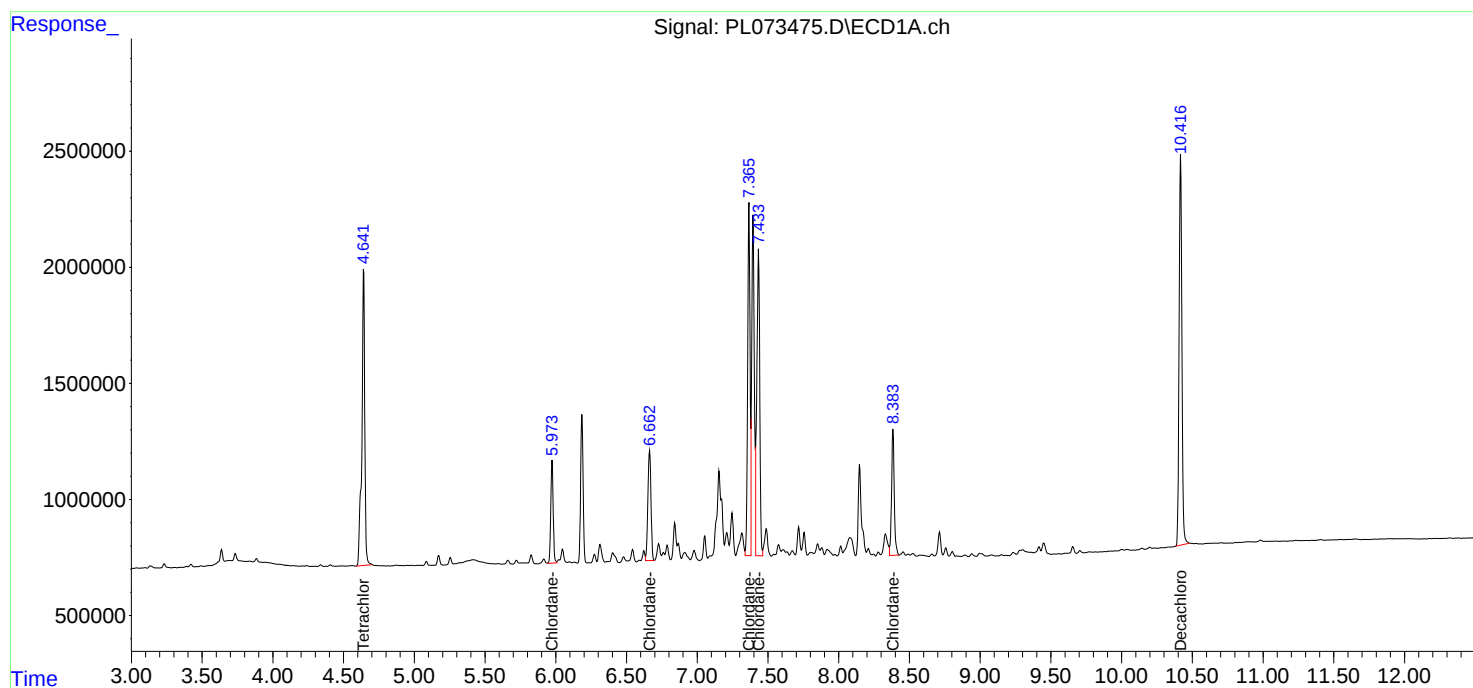


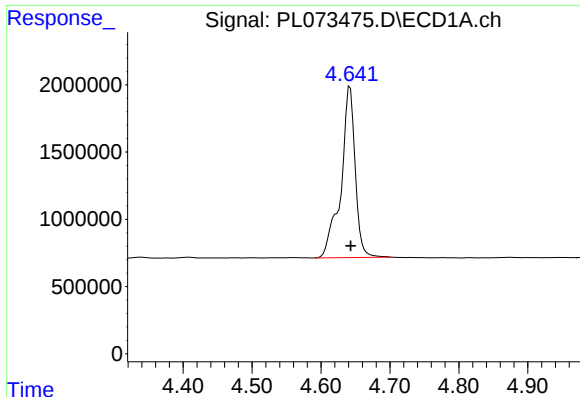

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 18325860
Conc: 57.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

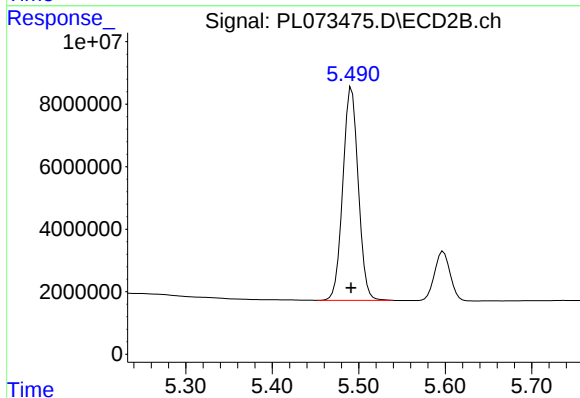


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 83972164
Conc: 51.16 ng/ml

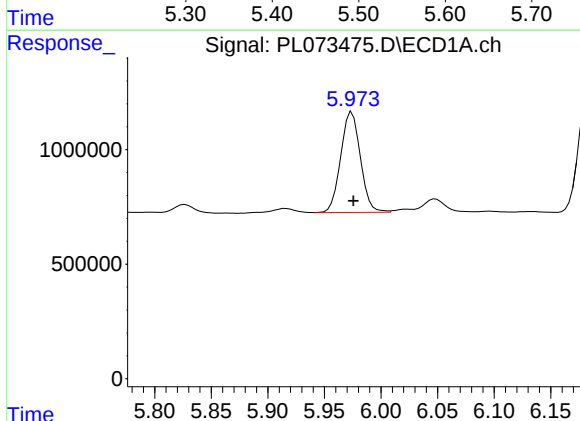


#23 Chlordane-1

R.T.: 5.974 min
Delta R.T.: -0.001 min
Response: 5329261
Conc: 449.54 ng/ml

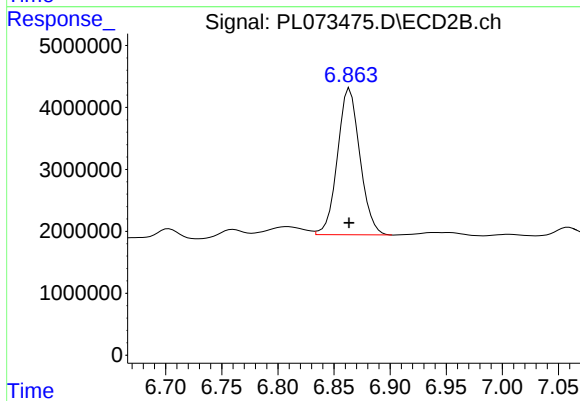

#23 Chlordane-1


R.T.: 6.864 min
Delta R.T.: 0.000 min
Response: 32816520
Conc: 480.38 ng/ml

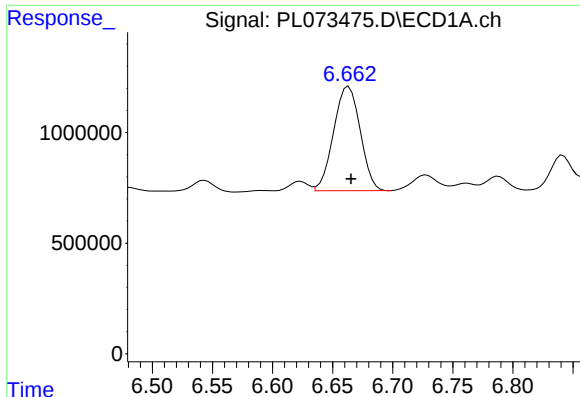

#24 Chlordane-2


R.T.: 6.663 min
Delta R.T.: -0.002 min
Response: 7279950
Conc: 446.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

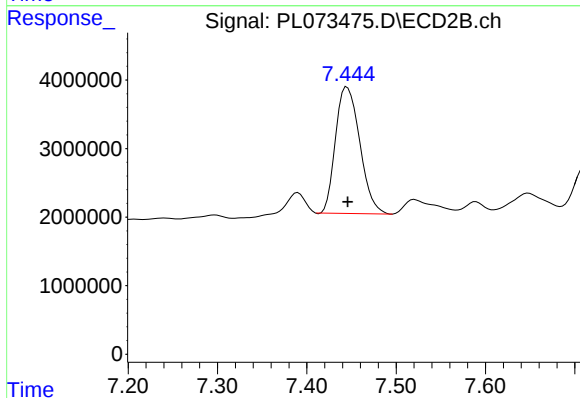


#24 Chlordane-2

R.T.: 7.445 min
Delta R.T.: 0.000 min
Response: 34877895
Conc: 485.27 ng/ml

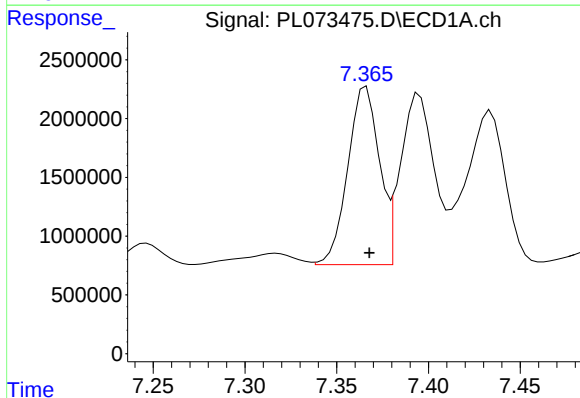


#25 Chlordane-3

R.T.: 7.366 min
Delta R.T.: -0.002 min
Response: 18100166
Conc: 443.26 ng/ml

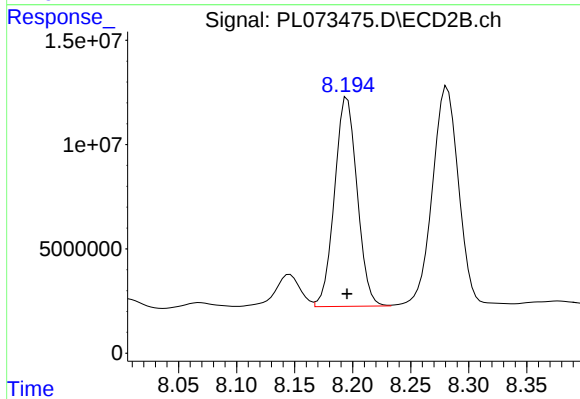

#25 Chlordane-3


R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 136070265
Conc: 501.86 ng/ml

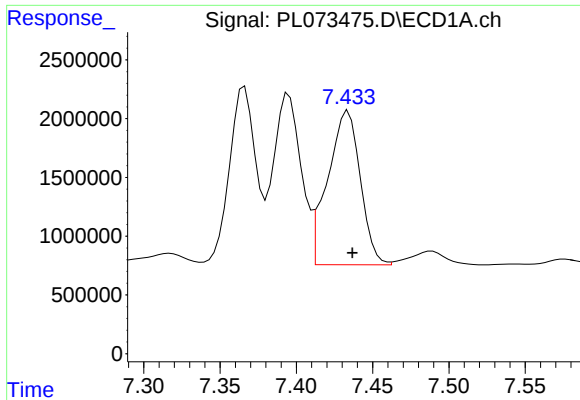

#26 Chlordane-4


R.T.: 7.434 min
Delta R.T.: -0.003 min
Response: 19460209
Conc: 439.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

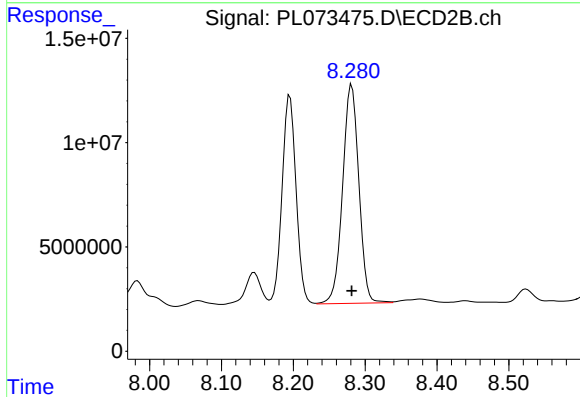


#26 Chlordane-4

R.T.: 8.281 min
Delta R.T.: 0.000 min
Response: 164745771
Conc: 497.34 ng/ml

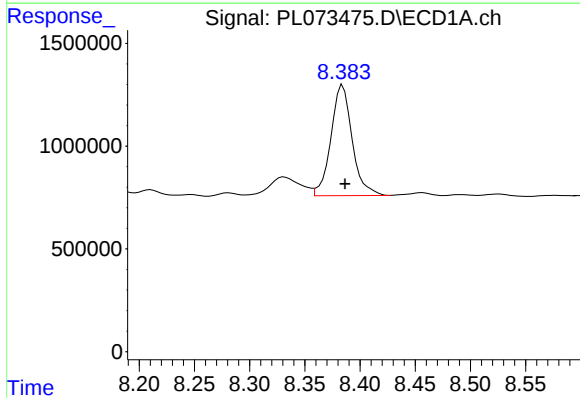


#27 Chlordane-5

R.T.: 8.384 min
Delta R.T.: -0.002 min
Response: 7206691
Conc: 440.10 ng/ml

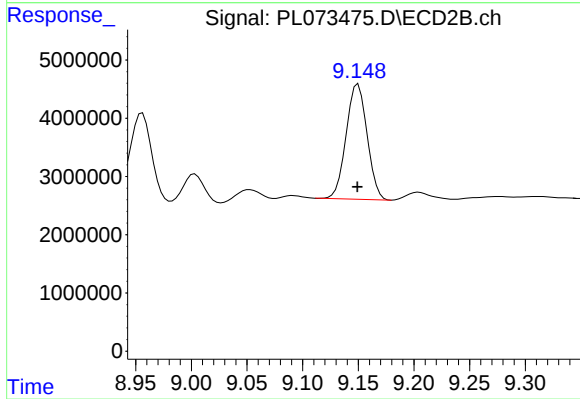

#27 Chlordane-5


R.T.: 9.150 min
Delta R.T.: 0.000 min
Response: 25890354
Conc: 477.00 ng/ml

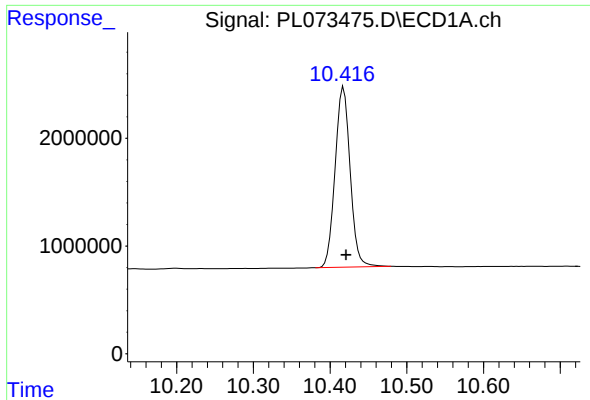

#28 Decachlorobiphenyl

R.T.: 10.418 min
Delta R.T.: -0.003 min
Response: 22848371
Conc: 44.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

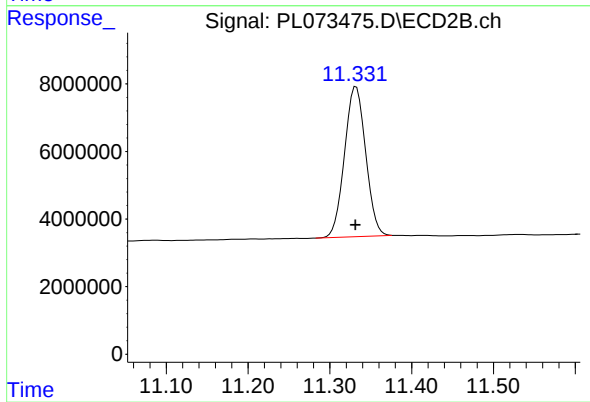

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 79600745
Conc: 44.52 ng/ml