

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
 Data File : PL073490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Mar 2022 20:37
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 19 01:18:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.492	17592257	80008686	54.927	48.749
28)	SA Decachlor...	10.416	11.332	22134806	78333183	43.530	43.806
Target Compounds							
23)	Chlordane-1	5.974	6.864	5112417	31889211	431.246	466.808
24)	Chlordane-2	6.663	7.447	7067798	33402911	433.264	464.744
25)	Chlordane-3	7.365	8.196	17392225	132.0E6	425.924	486.905
26)	Chlordane-4	7.434	8.282	18797572	158.9E6	424.125	479.698
27)	Chlordane-5	8.384	9.150	6881567	25094746	420.241	462.342



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031822\
Data File : PL073490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Mar 2022 20:37
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 19 01:18:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

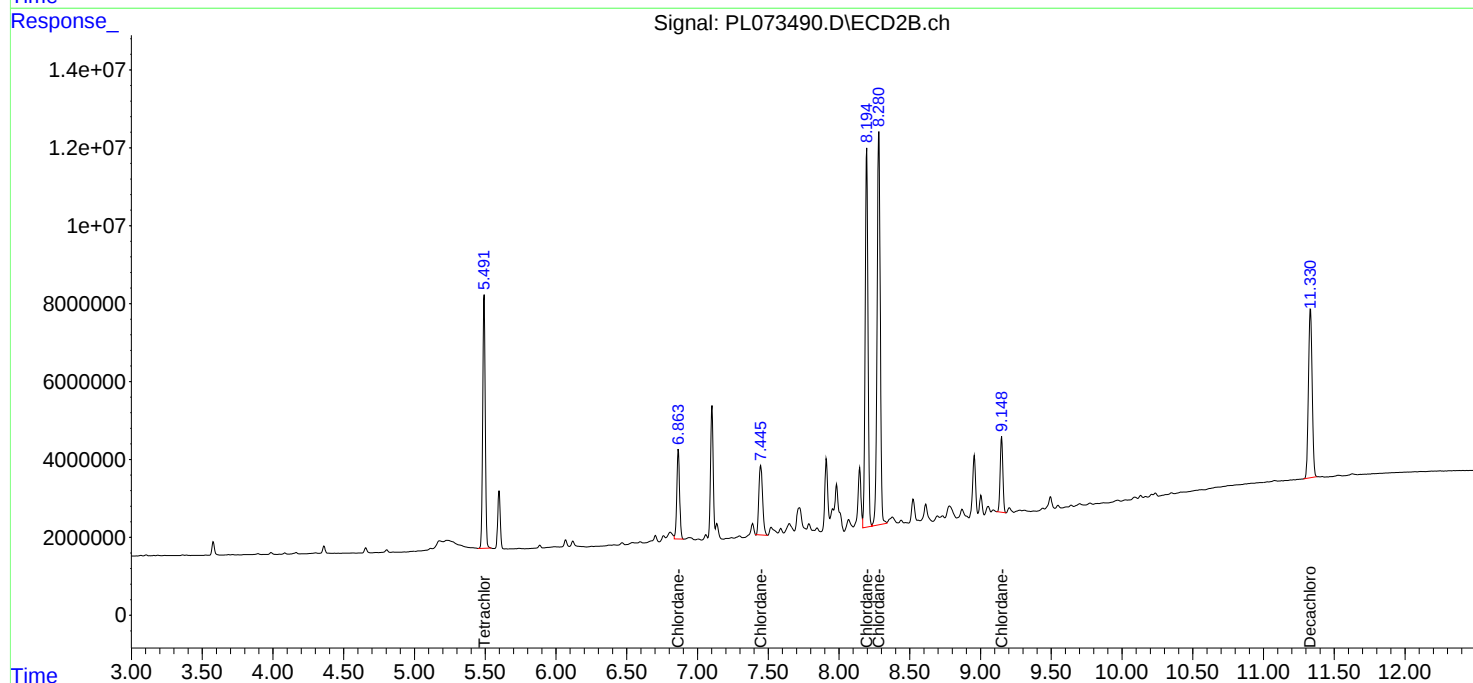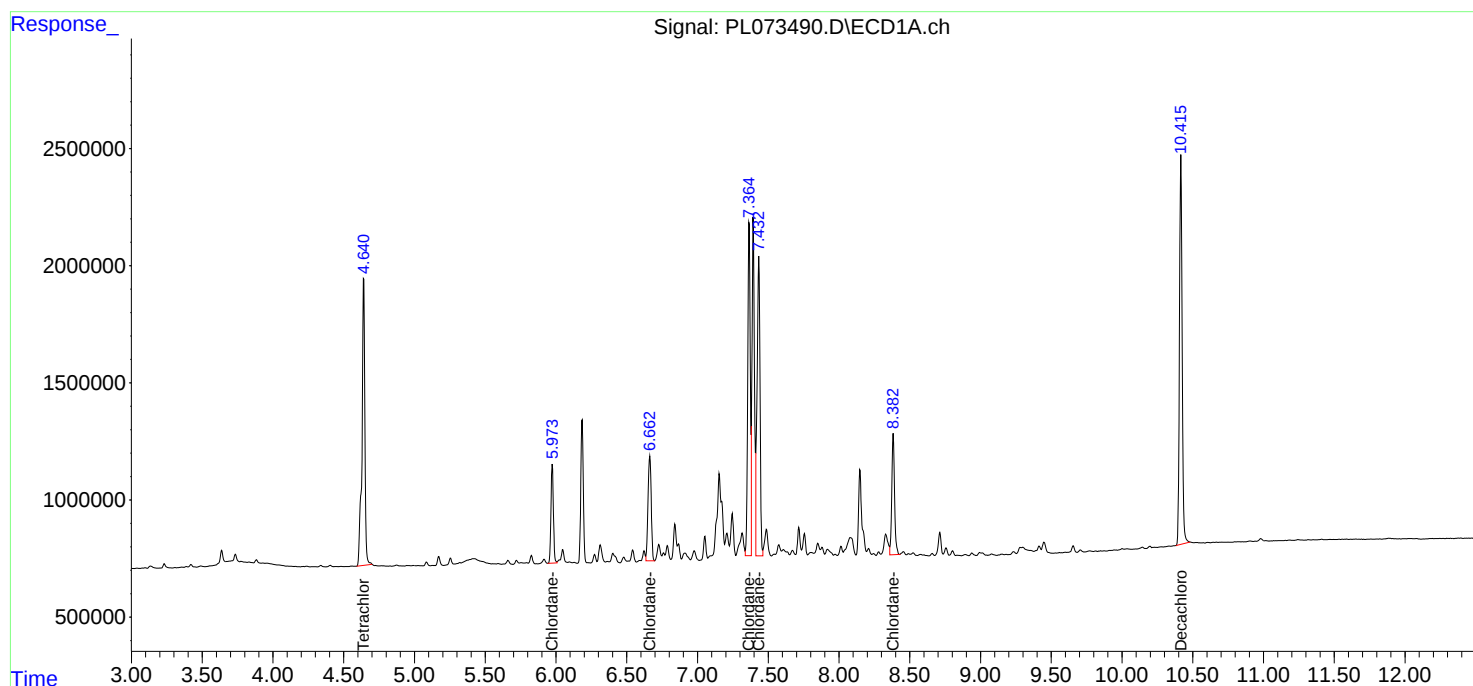


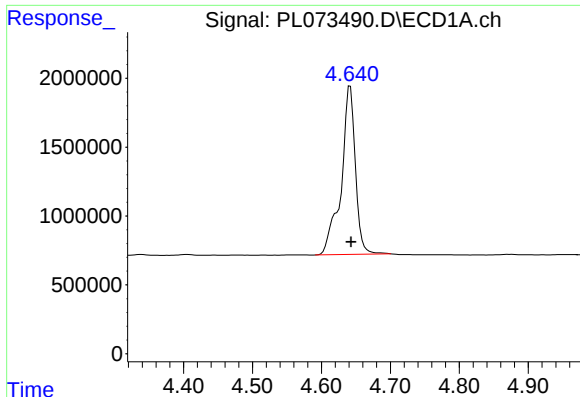

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: -0.001 min
Response: 17592257
Conc: 54.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

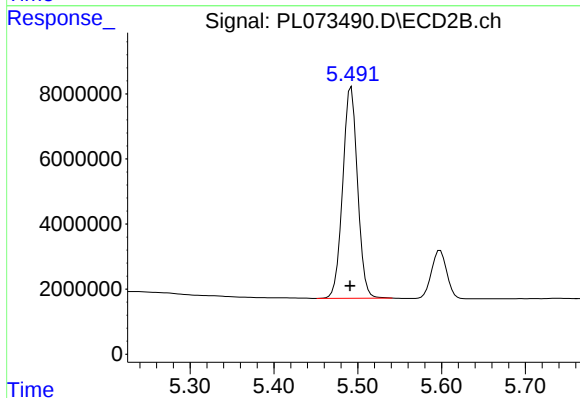


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.001 min
Response: 80008686
Conc: 48.75 ng/ml

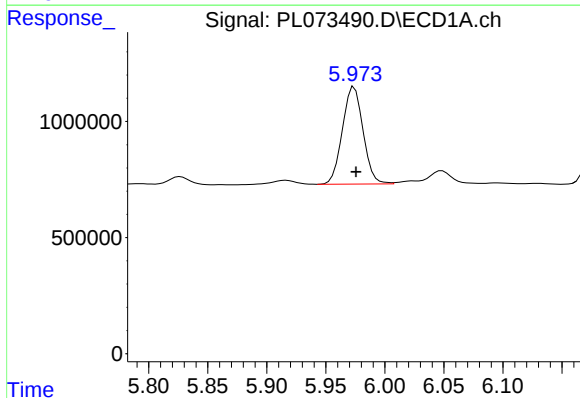


#23 Chlordane-1

R.T.: 5.974 min
Delta R.T.: -0.001 min
Response: 5112417
Conc: 431.25 ng/ml

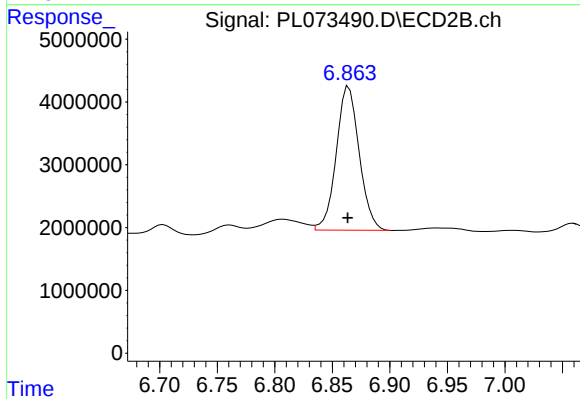

#23 Chlordane-1


R.T.: 6.864 min
Delta R.T.: 0.001 min
Response: 31889211
Conc: 466.81 ng/ml

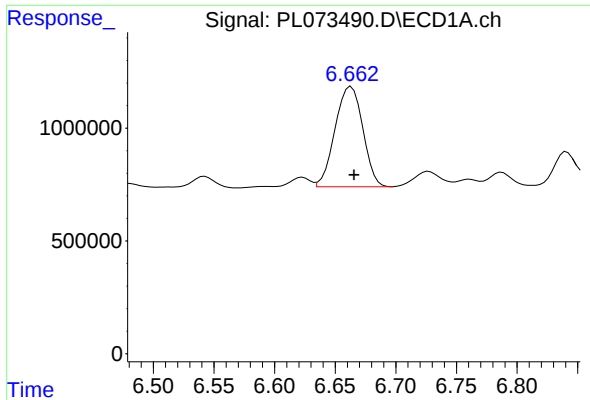

#24 Chlordane-2


R.T.: 6.663 min
Delta R.T.: -0.002 min
Response: 7067798
Conc: 433.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

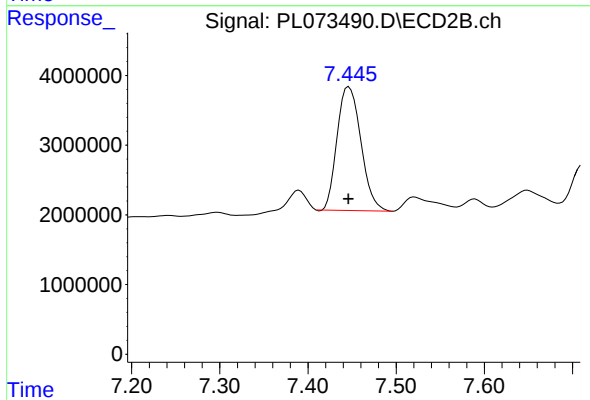


#24 Chlordane-2

R.T.: 7.447 min
Delta R.T.: 0.000 min
Response: 33402911
Conc: 464.74 ng/ml

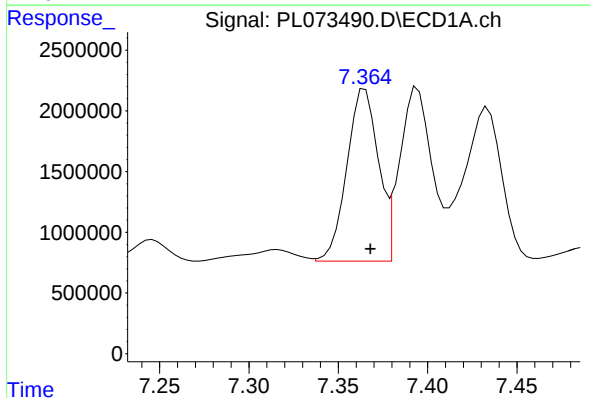


#25 Chlordane-3

R.T.: 7.365 min
Delta R.T.: -0.003 min
Response: 17392225
Conc: 425.92 ng/ml

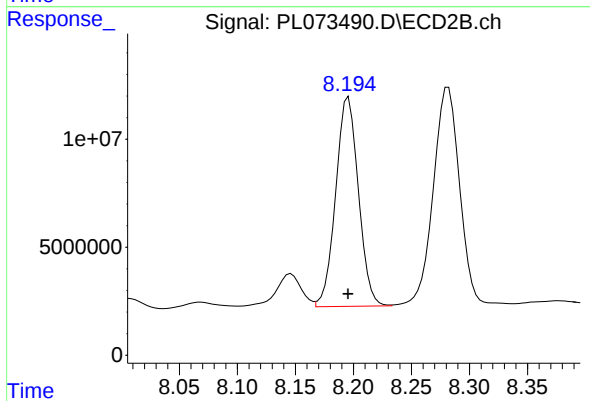

#25 Chlordane-3


R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 132015492
Conc: 486.90 ng/ml

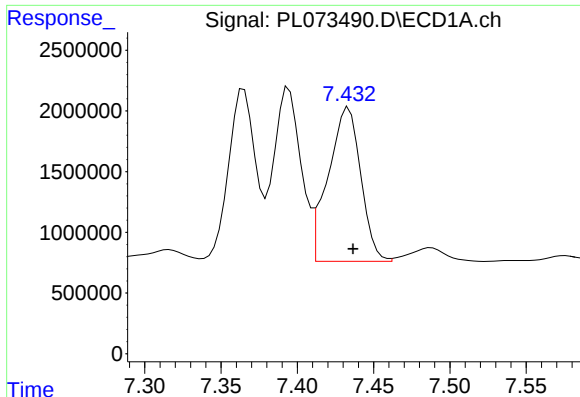

#26 Chlordane-4


R.T.: 7.434 min
Delta R.T.: -0.003 min
Response: 18797572
Conc: 424.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

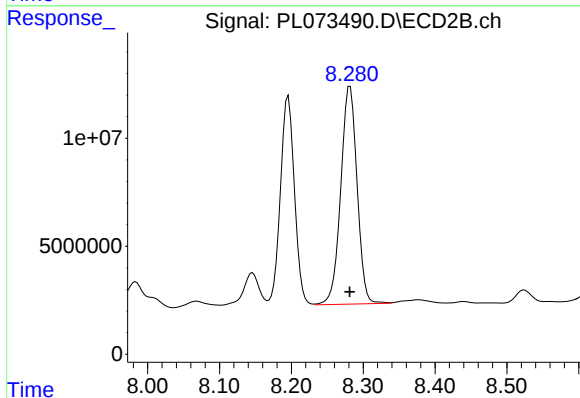


#26 Chlordane-4

R.T.: 8.282 min
Delta R.T.: 0.000 min
Response: 158901274
Conc: 479.70 ng/ml

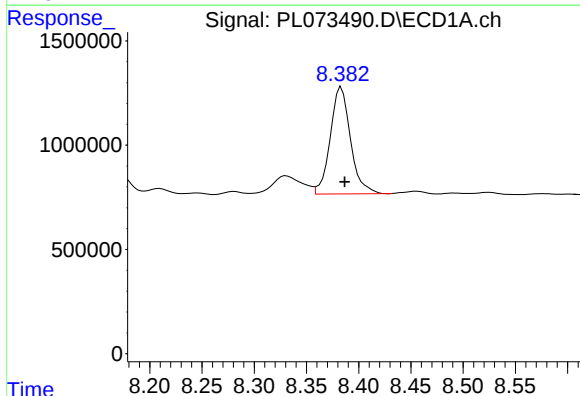


#27 Chlordane-5

R.T.: 8.384 min
Delta R.T.: -0.003 min
Response: 6881567
Conc: 420.24 ng/ml

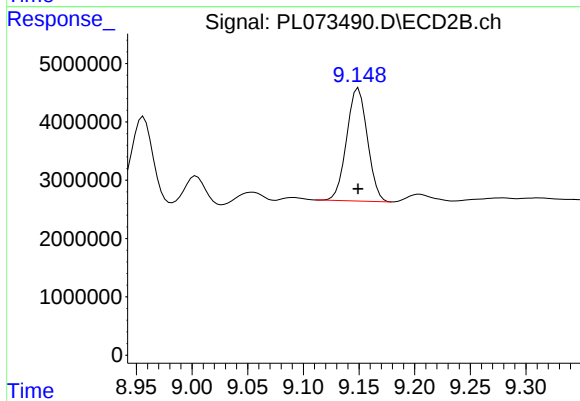

#27 Chlordane-5


R.T.: 9.150 min
Delta R.T.: 0.000 min
Response: 25094746
Conc: 462.34 ng/ml

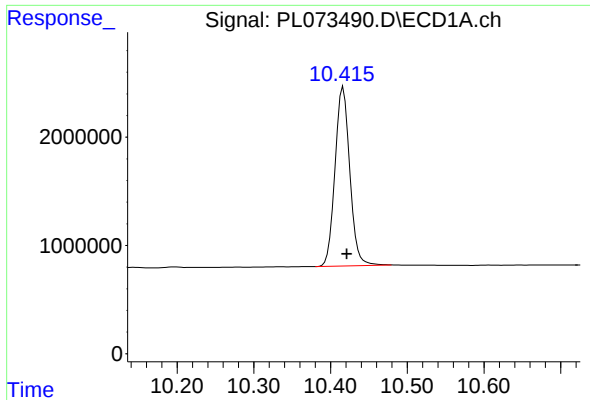

#28 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: -0.005 min
Response: 22134806
Conc: 43.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

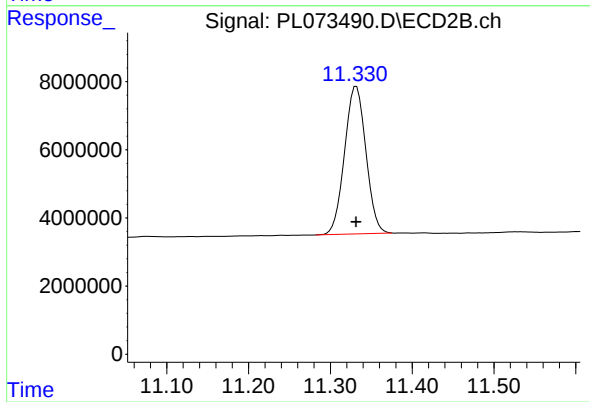

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 78333183
Conc: 43.81 ng/ml