

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031919\
 Data File : PL046161.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2019 18:30
 Operator : AJ\SJ
 Sample : K1971-10
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-15(6-7)-031519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 02:14:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.980	31536460	19051843	4.584	8.896 #
28)	SA Decachlor...	8.044	9.037	71009905	20144650	8.486	8.816
Target Compounds							
5)	MB Aldrin	4.586	5.465	657.9E6	65425753	67.640	24.223 #
9)	A Endosulfan I	0.000	6.234f	0	10810847	N.D.	4.341 #
10)	B gamma-Chl...	5.283f	0.000	906.8E6	0	92.649	N.D. #
11)	B alpha-Chl...	5.320	0.000	651.5E6	0	67.190	N.D. #
24)	Chlordane-2	0.000	5.465f	0	65425753	N.D.	541.469 #
25)	Chlordane-3	5.283f	0.000	906.8E6	0	790.528	N.D. #
26)	Chlordane-4	5.320	0.000	651.5E6	0	614.633	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031919\
Data File : PL046161.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2019 18:30
Operator : AJ\SJ
Sample : K1971-10
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SB-15(6-7)-031519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 02:14:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

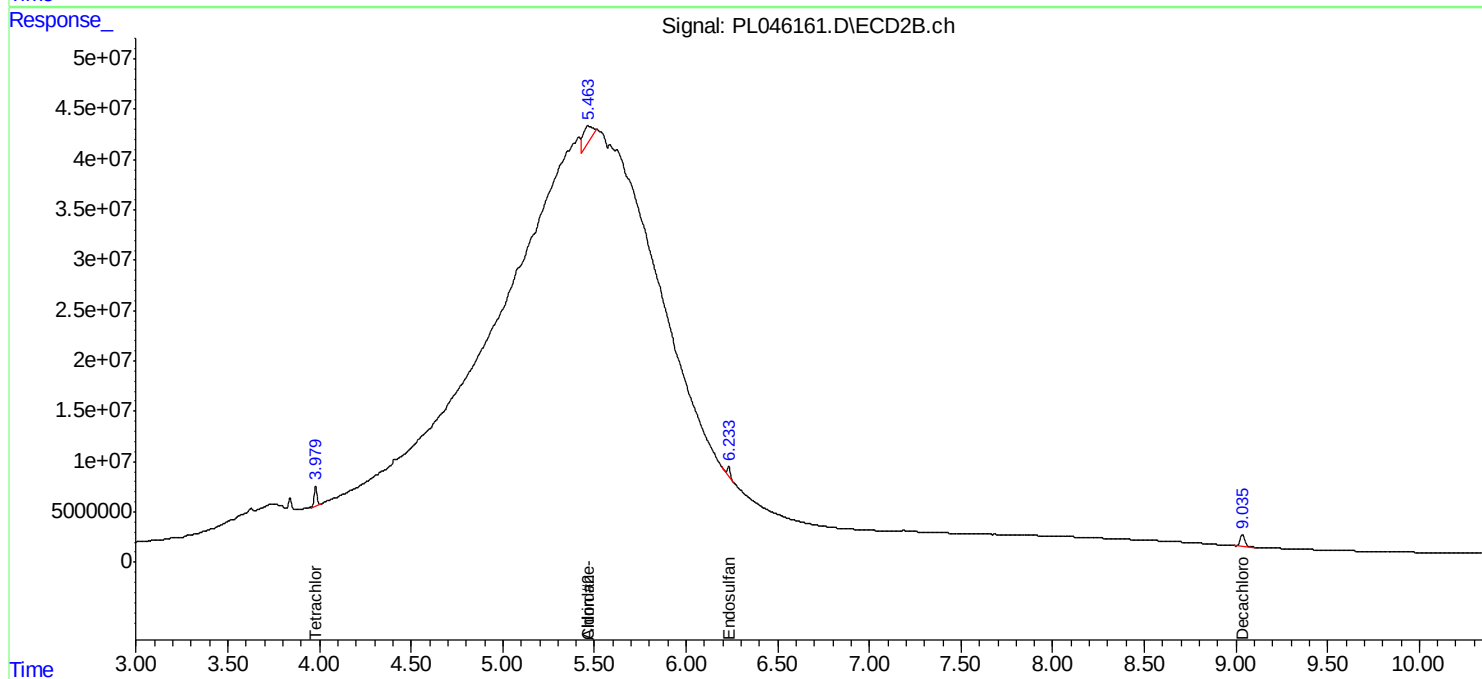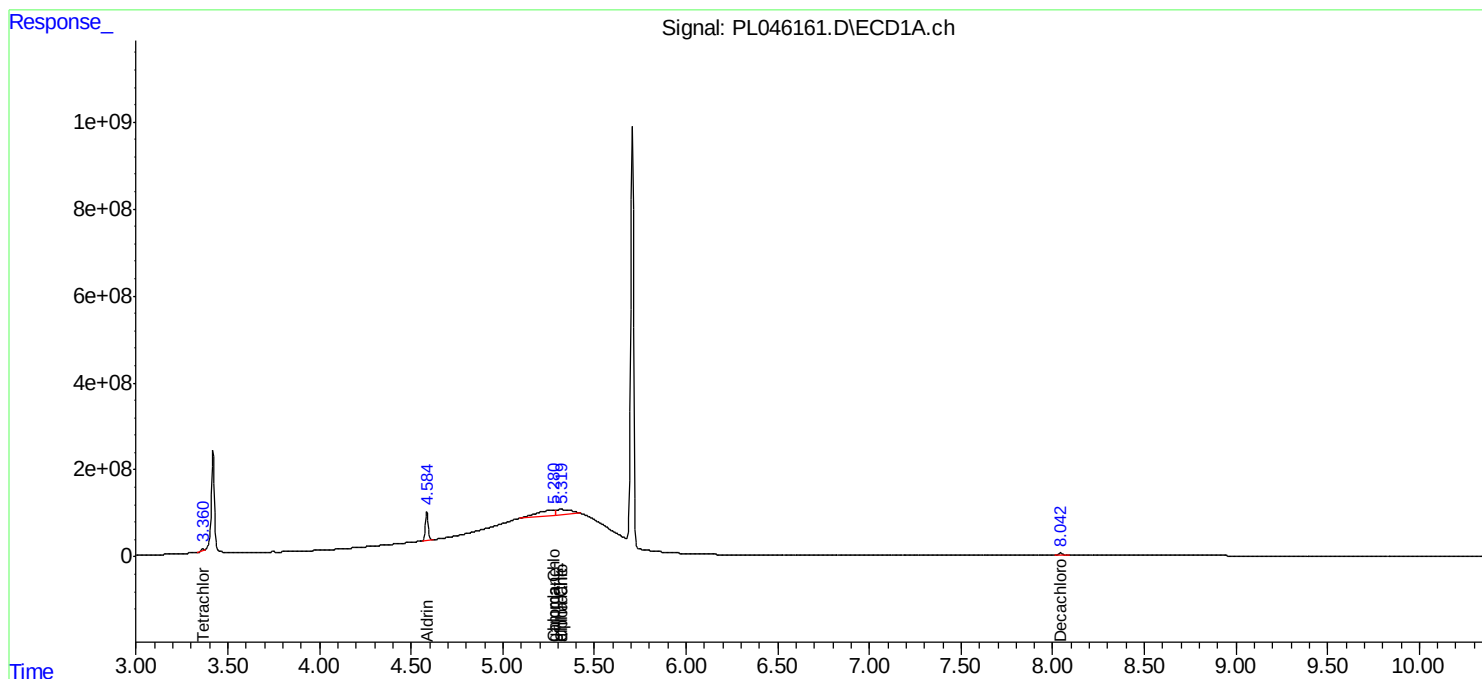


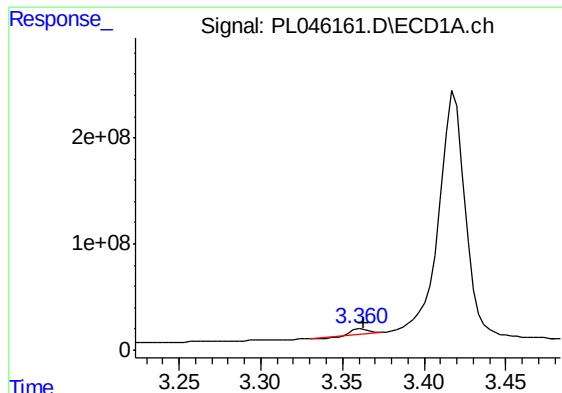

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 31536460
Conc: 4.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-15(6-7)-031519

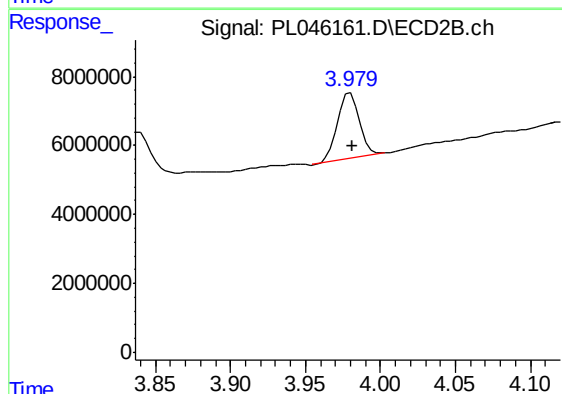


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 19051843
Conc: 8.90 ng/ml

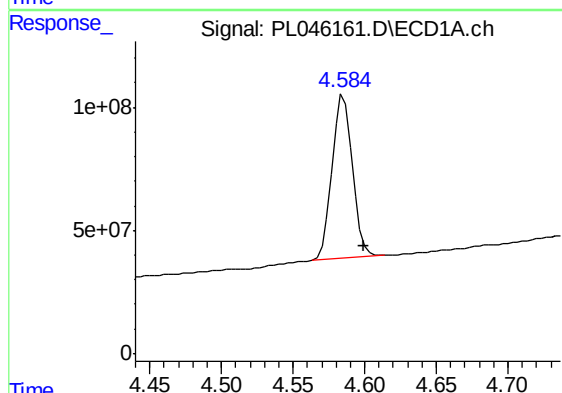


#5 Aldrin

R.T.: 4.586 min
Delta R.T.: -0.014 min
Response: 657895346
Conc: 67.64 ng/ml

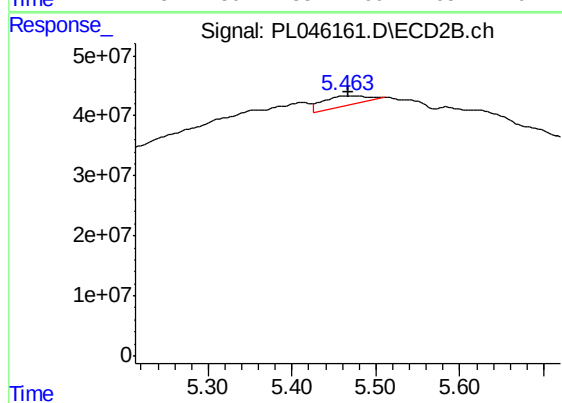

#5 Aldrin


R.T.: 5.465 min
Delta R.T.: -0.003 min
Response: 65425753
Conc: 24.22 ng/ml

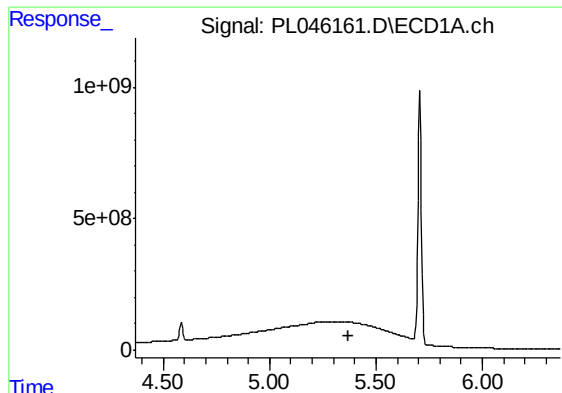

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SB-15(6-7)-031519

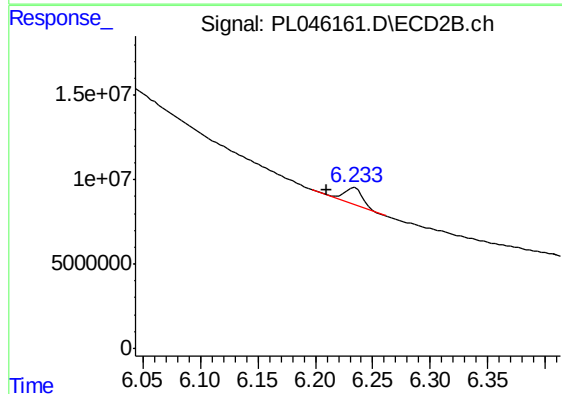


#9 Endosulfan I

R.T.: 6.234 min
Delta R.T.: 0.024 min
Response: 10810847
Conc: 4.34 ng/ml

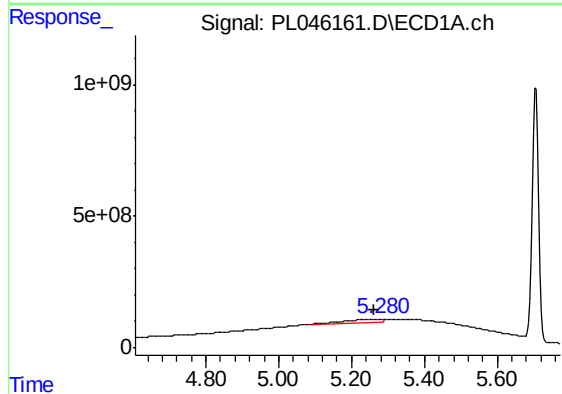


#10 gamma-Chlordane

R.T.: 5.283 min
Delta R.T.: 0.022 min
Response: 906752171
Conc: 92.65 ng/ml

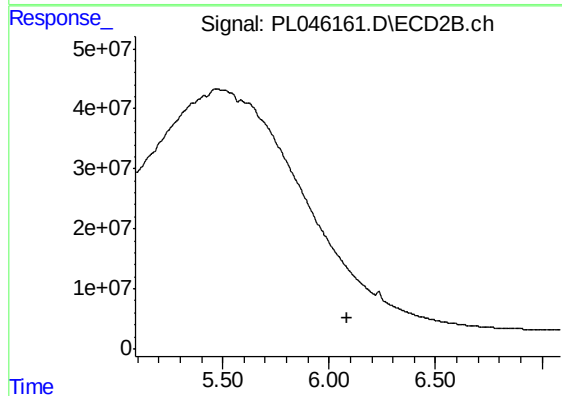

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.088 min
Response: 0
Conc: N.D.

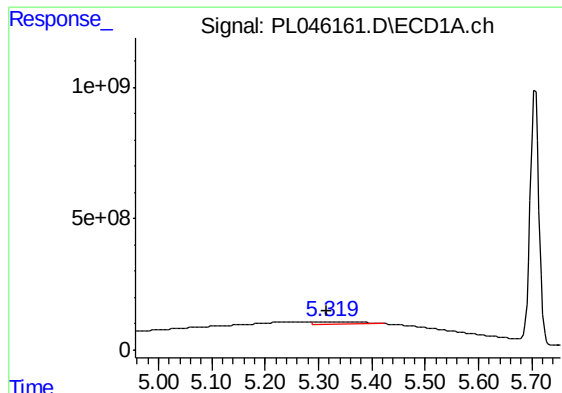

#11 alpha-Chlordane


R.T.: 5.320 min
Delta R.T.: 0.004 min
Response: 651543570
Conc: 67.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-15(6-7)-031519

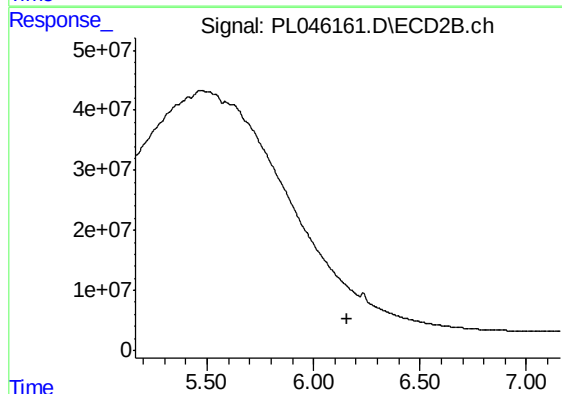


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.160 min
Response: 0
Conc: N.D.

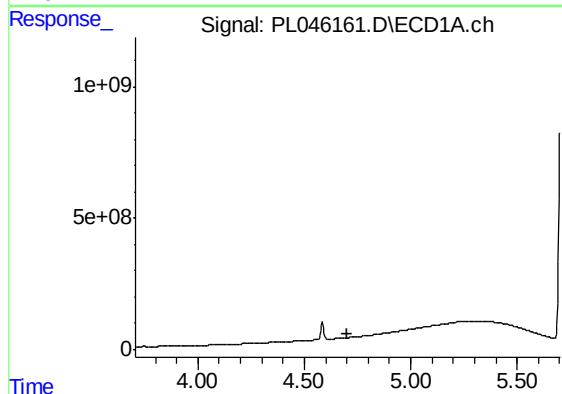


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.704 min
Response: 0
Conc: N.D.

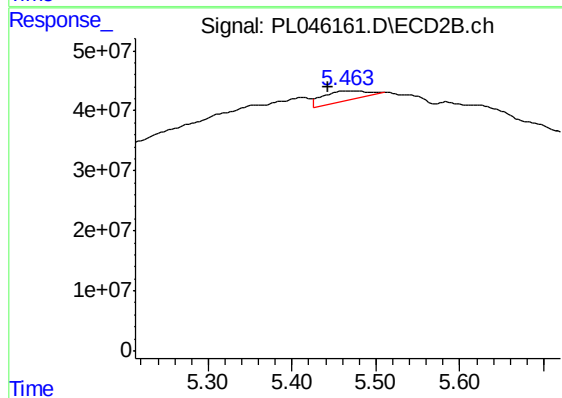

#24 Chlordane-2


R.T.: 5.465 min
Delta R.T.: 0.022 min
Response: 65425753
Conc: 541.47 ng/ml

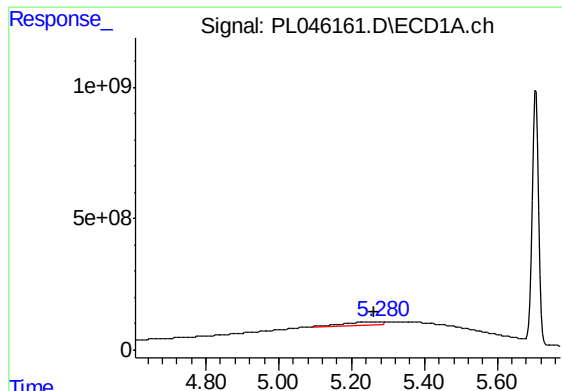

#25 Chlordane-3


R.T.: 5.283 min
Delta R.T.: 0.021 min
Response: 906752171
Conc: 790.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-15(6-7)-031519

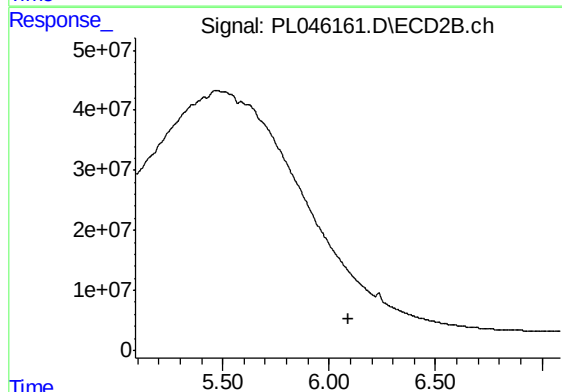


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

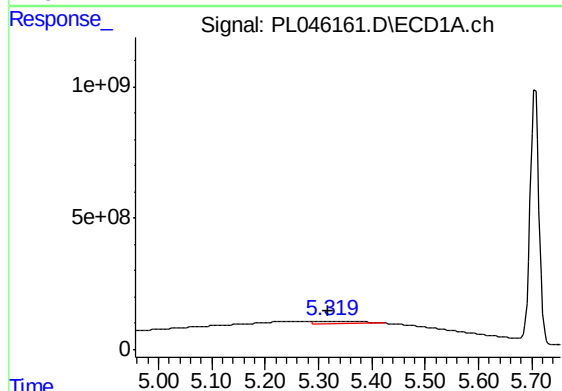


#26 Chlordane-4

R.T.: 5.320 min
Delta R.T.: 0.003 min
Response: 651543570
Conc: 614.63 ng/ml

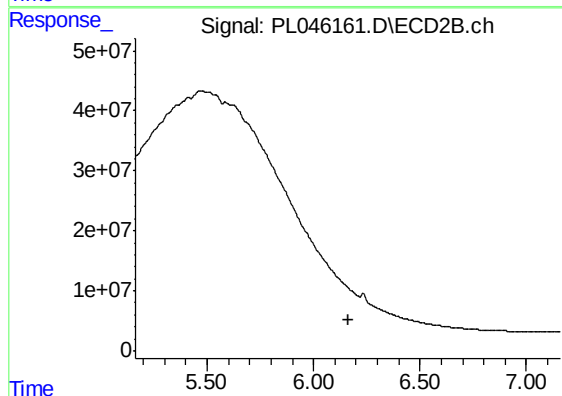

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

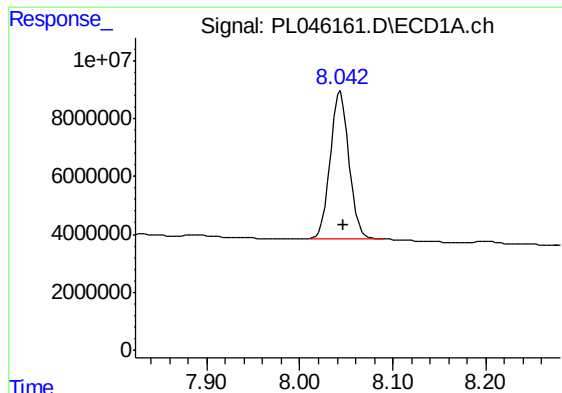

#28 Decachlorobiphenyl

R.T.: 8.044 min
Delta R.T.: -0.003 min
Response: 71009905
Conc: 8.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-15(6-7)-031519

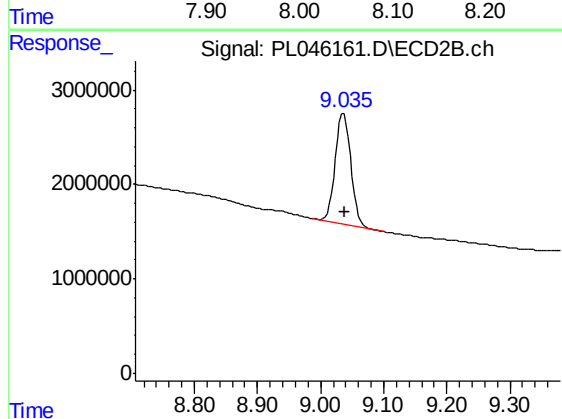

#28 Decachlorobiphenyl

R.T.: 9.037 min
Delta R.T.: -0.002 min
Response: 20144650
Conc: 8.82 ng/ml