

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031921\
 Data File : PL065448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2021 16:28
 Operator : AR\AJ
 Sample : PB135246BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB135246BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 00:58:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.787	43015123	42469794	18.113	15.473
28)	SA Decachlor...	7.929	8.737	40343161	34619018	16.698	17.466
Target Compounds							
4)	MA Heptachlor	0.000	4.947	0	753765	N.D.	0.226 #
5)	MB Aldrin	0.000	5.234	0	44100	N.D.	0.013 #
6)	B beta-BHC	0.000	4.639	0	1312700	N.D.	0.762 #
10)	B gamma-Chl...	0.000	5.848	0	848049	N.D.	0.304 #
11)	B alpha-Chl...	0.000	5.926	0	174263	N.D.	0.063 #
19)	B Endosulfa...	6.427f	0.000	124142	0	0.050	N.D. #
24)	Chlordane-2	0.000	5.234f	0	44100	N.D.	0.405 #
25)	Chlordane-3	0.000	5.848	0	848049	N.D.	2.080 #
26)	Chlordane-4	0.000	5.926	0	174263	N.D.	0.362 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031921\
Data File : PL065448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2021 16:28
Operator : AR\AJ
Sample : PB135246BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB135246BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 00:58:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

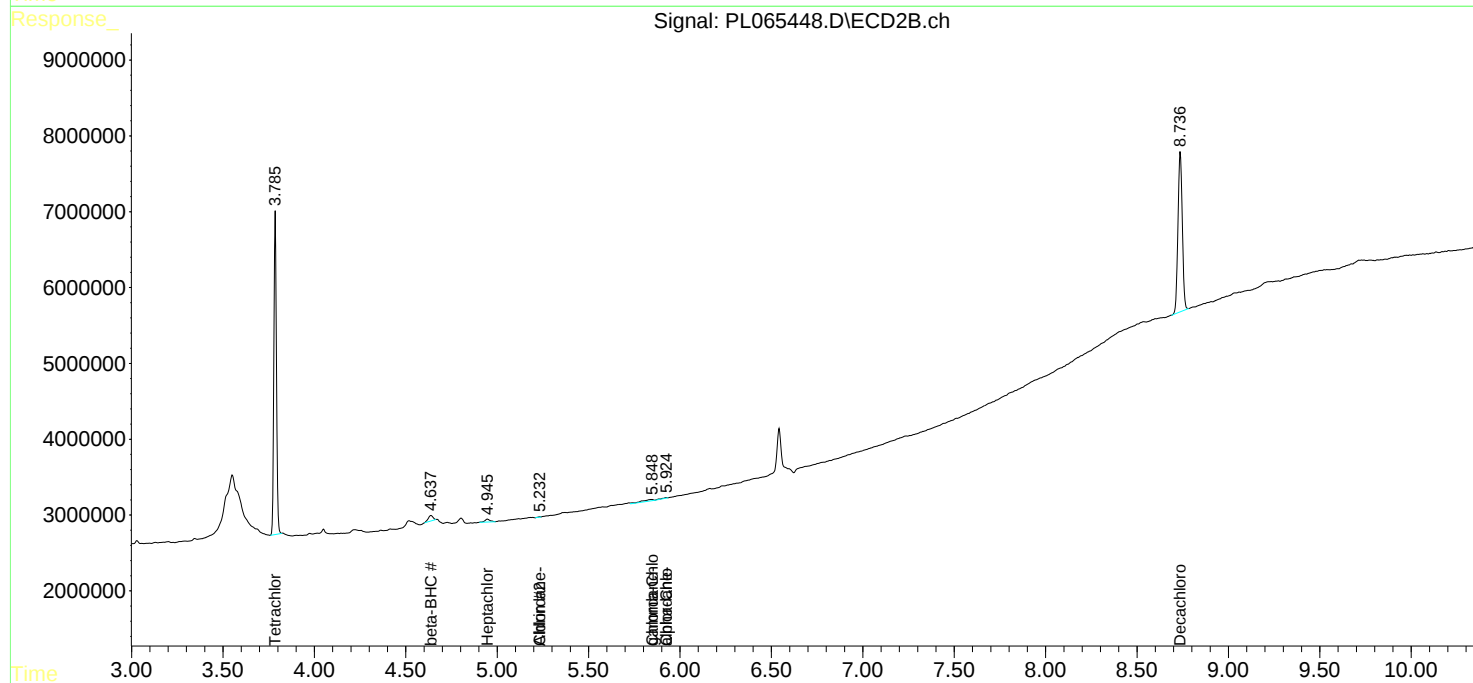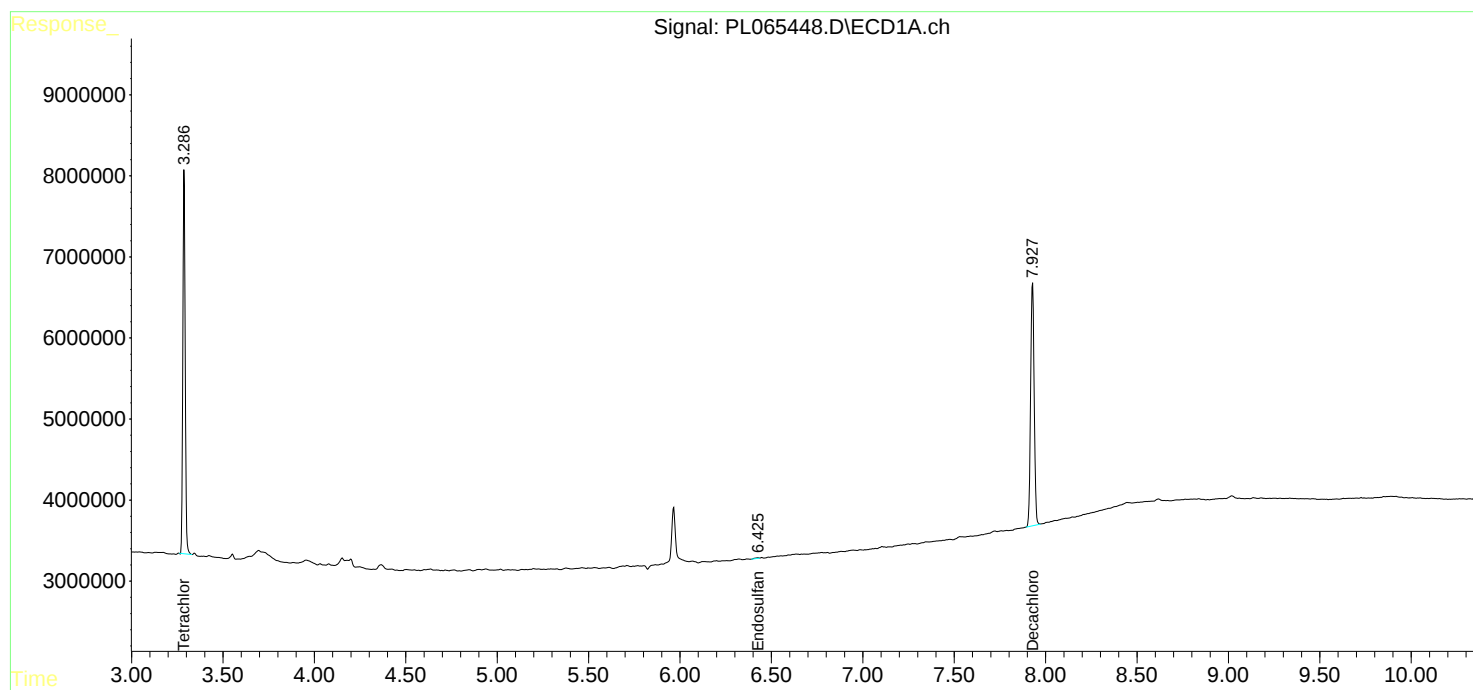


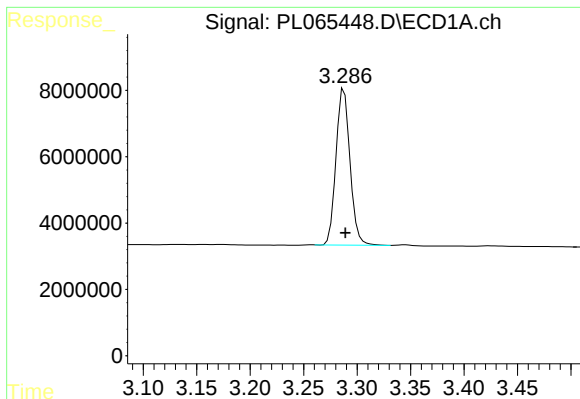

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: -0.001 min
Response: 43015123
Conc: 18.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135246BL

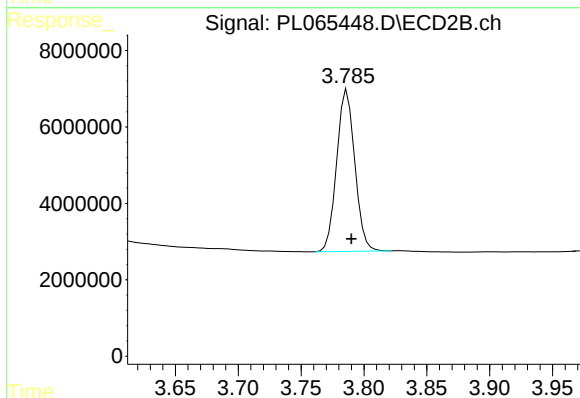


#1 Tetrachloro-m-xylene

R.T.: 3.787 min
Delta R.T.: -0.003 min
Response: 42469794
Conc: 15.47 ng/ml

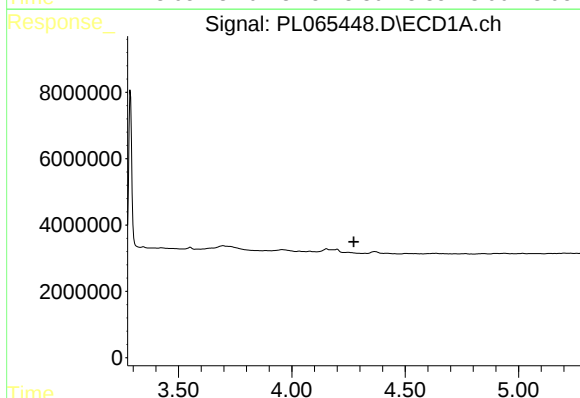


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.274 min
Response: 0
Conc: N.D.

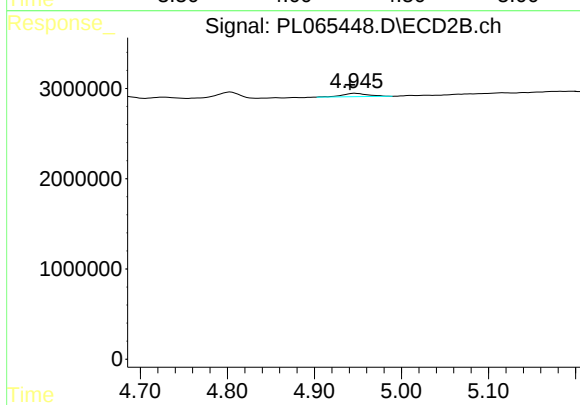

#4 Heptachlor


R.T.: 4.947 min
Delta R.T.: 0.006 min
Response: 753765
Conc: 0.23 ng/ml

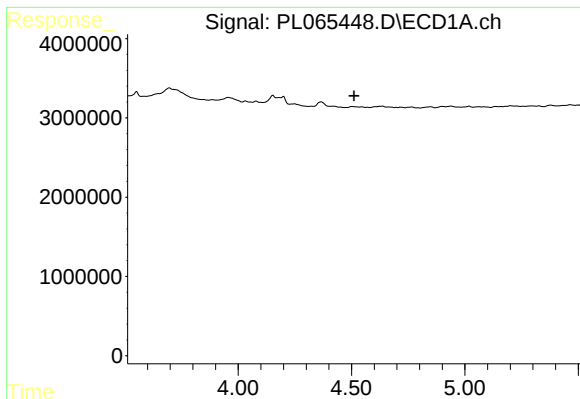

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.511 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB135246BL

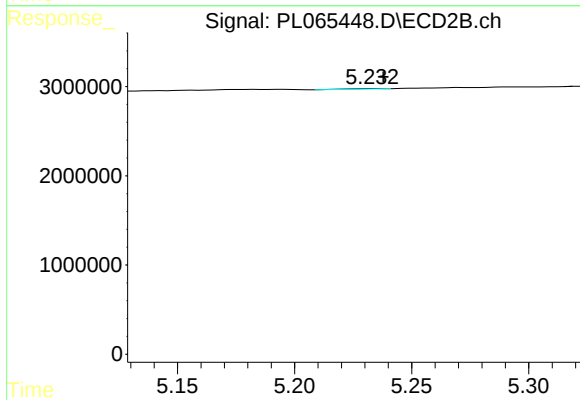


#5 Aldrin

R.T.: 5.234 min
Delta R.T.: -0.004 min
Response: 44100
Conc: 0.01 ng/ml

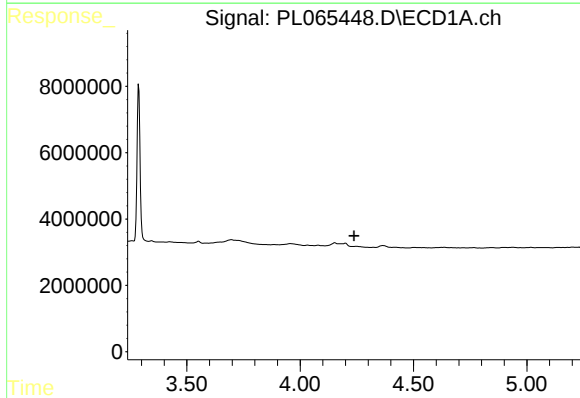


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.238 min
Response: 0
Conc: N.D.

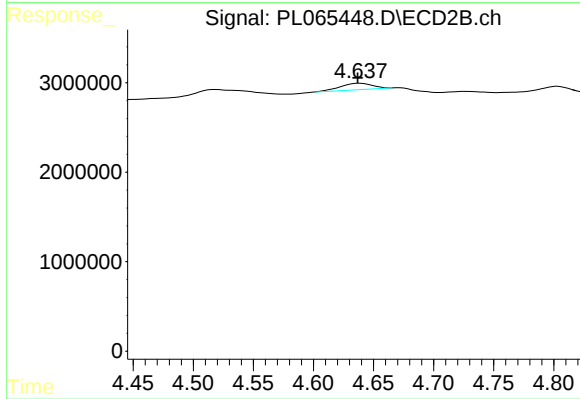

#6 beta-BHC


R.T.: 4.639 min
Delta R.T.: 0.002 min
Response: 1312700
Conc: 0.76 ng/ml

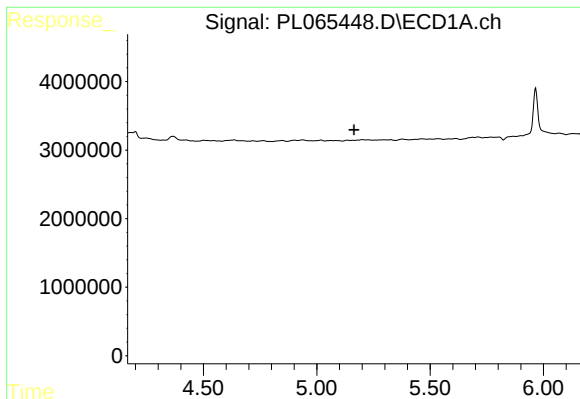

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.165 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB135246BL

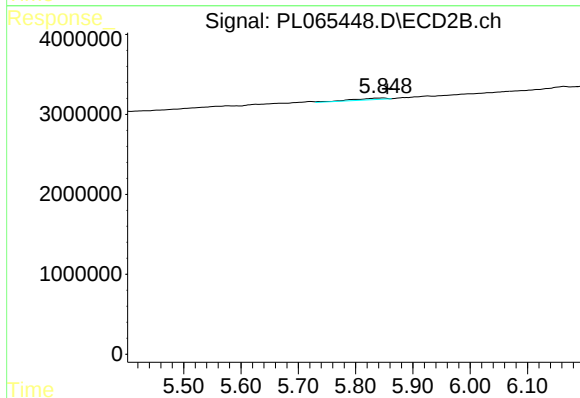


#10 gamma-Chlordane

R.T.: 5.848 min
Delta R.T.: -0.007 min
Response: 848049
Conc: 0.30 ng/ml

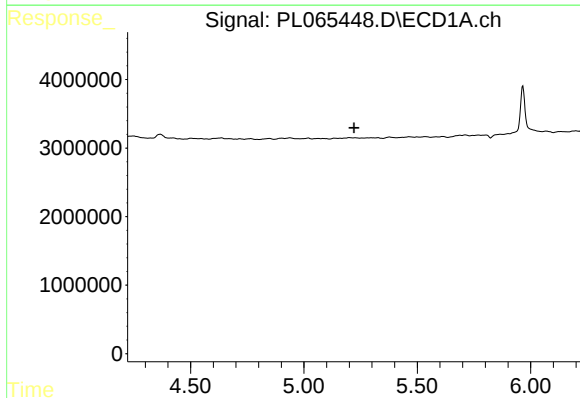


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.221 min
Response: 0
Conc: N.D.

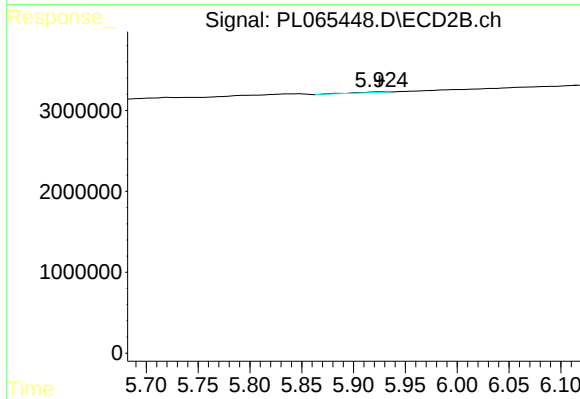

#11 alpha-Chlordane


R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 174263
Conc: 0.06 ng/ml

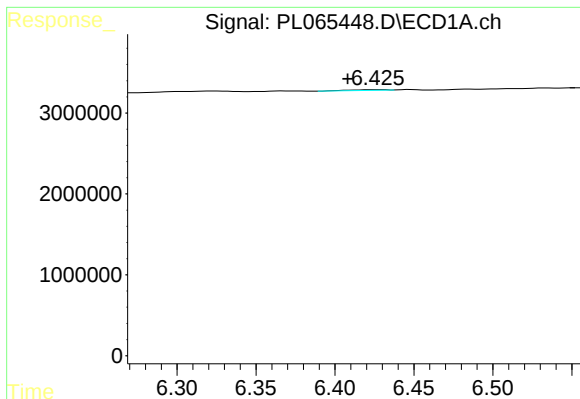

#19 Endosulfan Sulfate


R.T.: 6.427 min
Delta R.T.: 0.019 min
Response: 124142
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135246BL

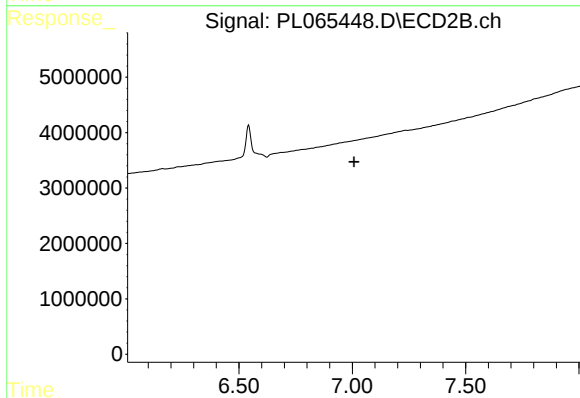


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.009 min
Response: 0
Conc: N.D.

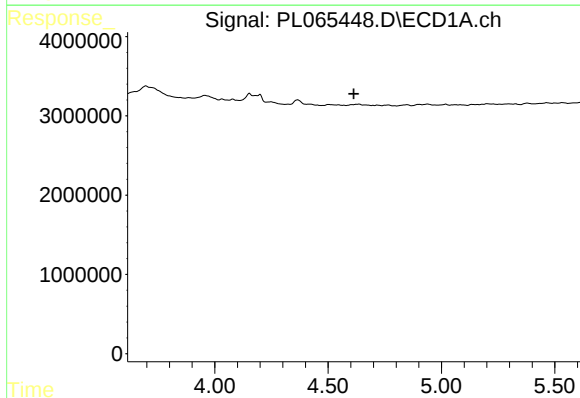


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.614 min
Response: 0
Conc: N.D.

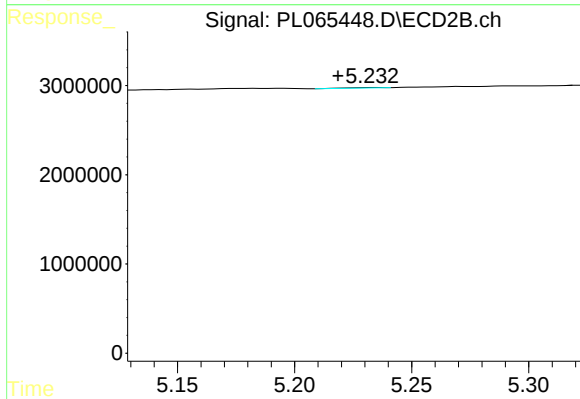

#24 Chlordane-2


R.T.: 5.234 min
Delta R.T.: 0.015 min
Response: 44100
Conc: 0.40 ng/ml

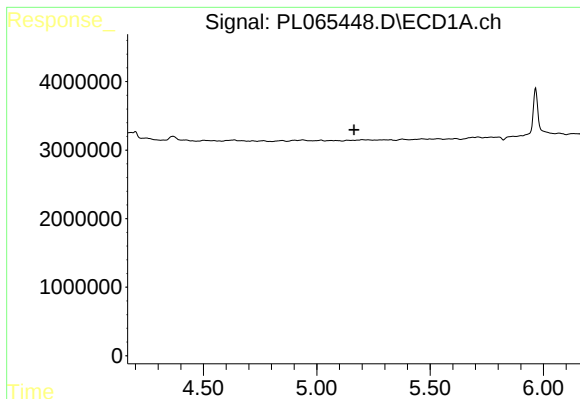

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.165 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB135246BL

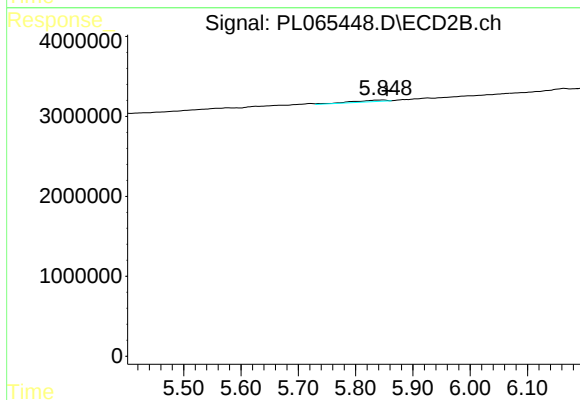


#25 Chlordane-3

R.T.: 5.848 min
Delta R.T.: -0.007 min
Response: 848049
Conc: 2.08 ng/ml

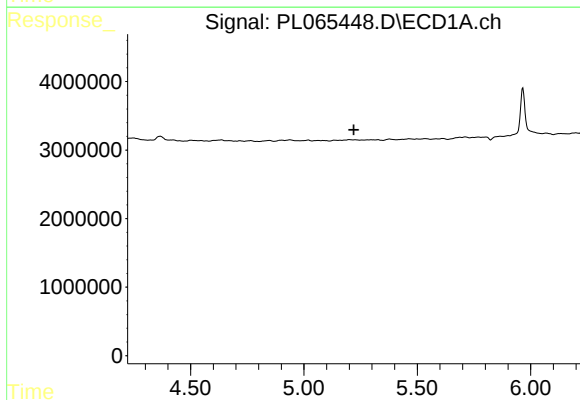


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.220 min
Response: 0
Conc: N.D.

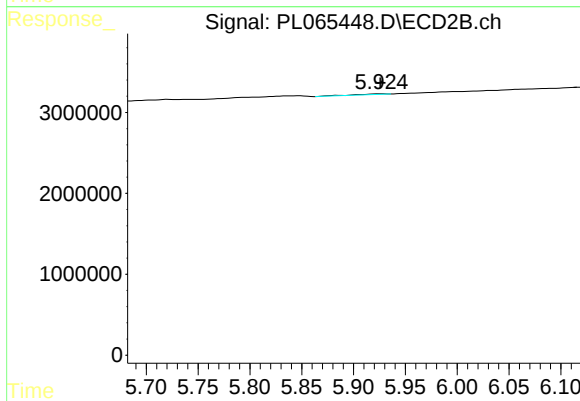

#26 Chlordane-4


R.T.: 5.926 min
Delta R.T.: 0.000 min
Response: 174263
Conc: 0.36 ng/ml

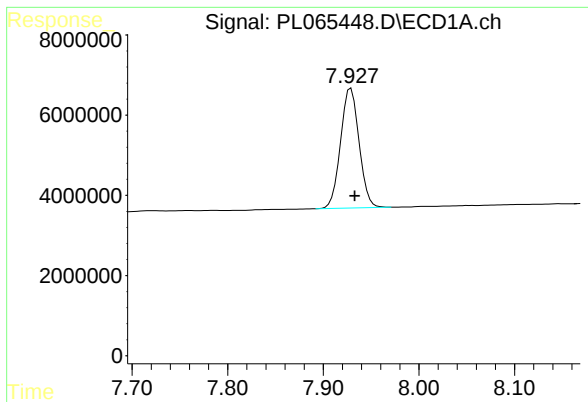

#28 Decachlorobiphenyl

R.T.: 7.929 min
Delta R.T.: -0.004 min
Response: 40343161
Conc: 16.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB135246BL

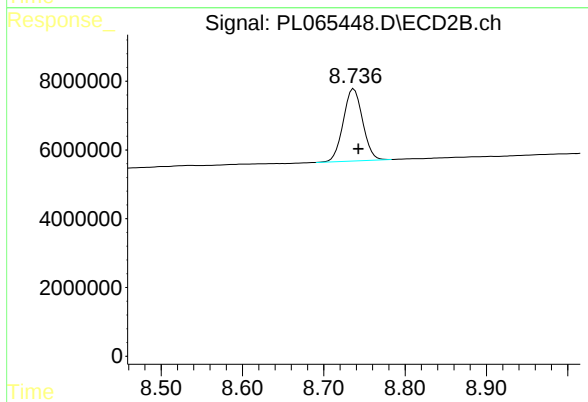

#28 Decachlorobiphenyl

R.T.: 8.737 min
Delta R.T.: -0.006 min
Response: 34619018
Conc: 17.47 ng/ml