

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031921\
 Data File : PL065449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2021 16:42
 Operator : AR\AJ
 Sample : M1721-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-05-031821

Manual Integrations
 APPROVED

Ankita
 3/22/2021 11:16:33 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 00:59:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.787	46832425	46217642	19.721	16.839
28)	SA Decachlor...	7.928	8.738	32935361	31017006	13.632	15.648
Target Compounds							
12)	B 4,4'-DDE	5.384	6.081	4167607	2964854	1.584m	1.190m
16)	A 4,4'-DDD	5.900	6.570	6974008	4105961	3.155m	1.867m#
17)	MA 4,4'-DDT	6.124	6.866	4494489	8190861	2.375	4.173 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031921\
Data File : PL065449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2021 16:42
Operator : AR\AJ
Sample : M1721-01
Misc :
ALS Vial : 23 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
TR-05-031821


Manual Integrations
APPROVED

Ankita
3/22/2021 11:16:33 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 00:59:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

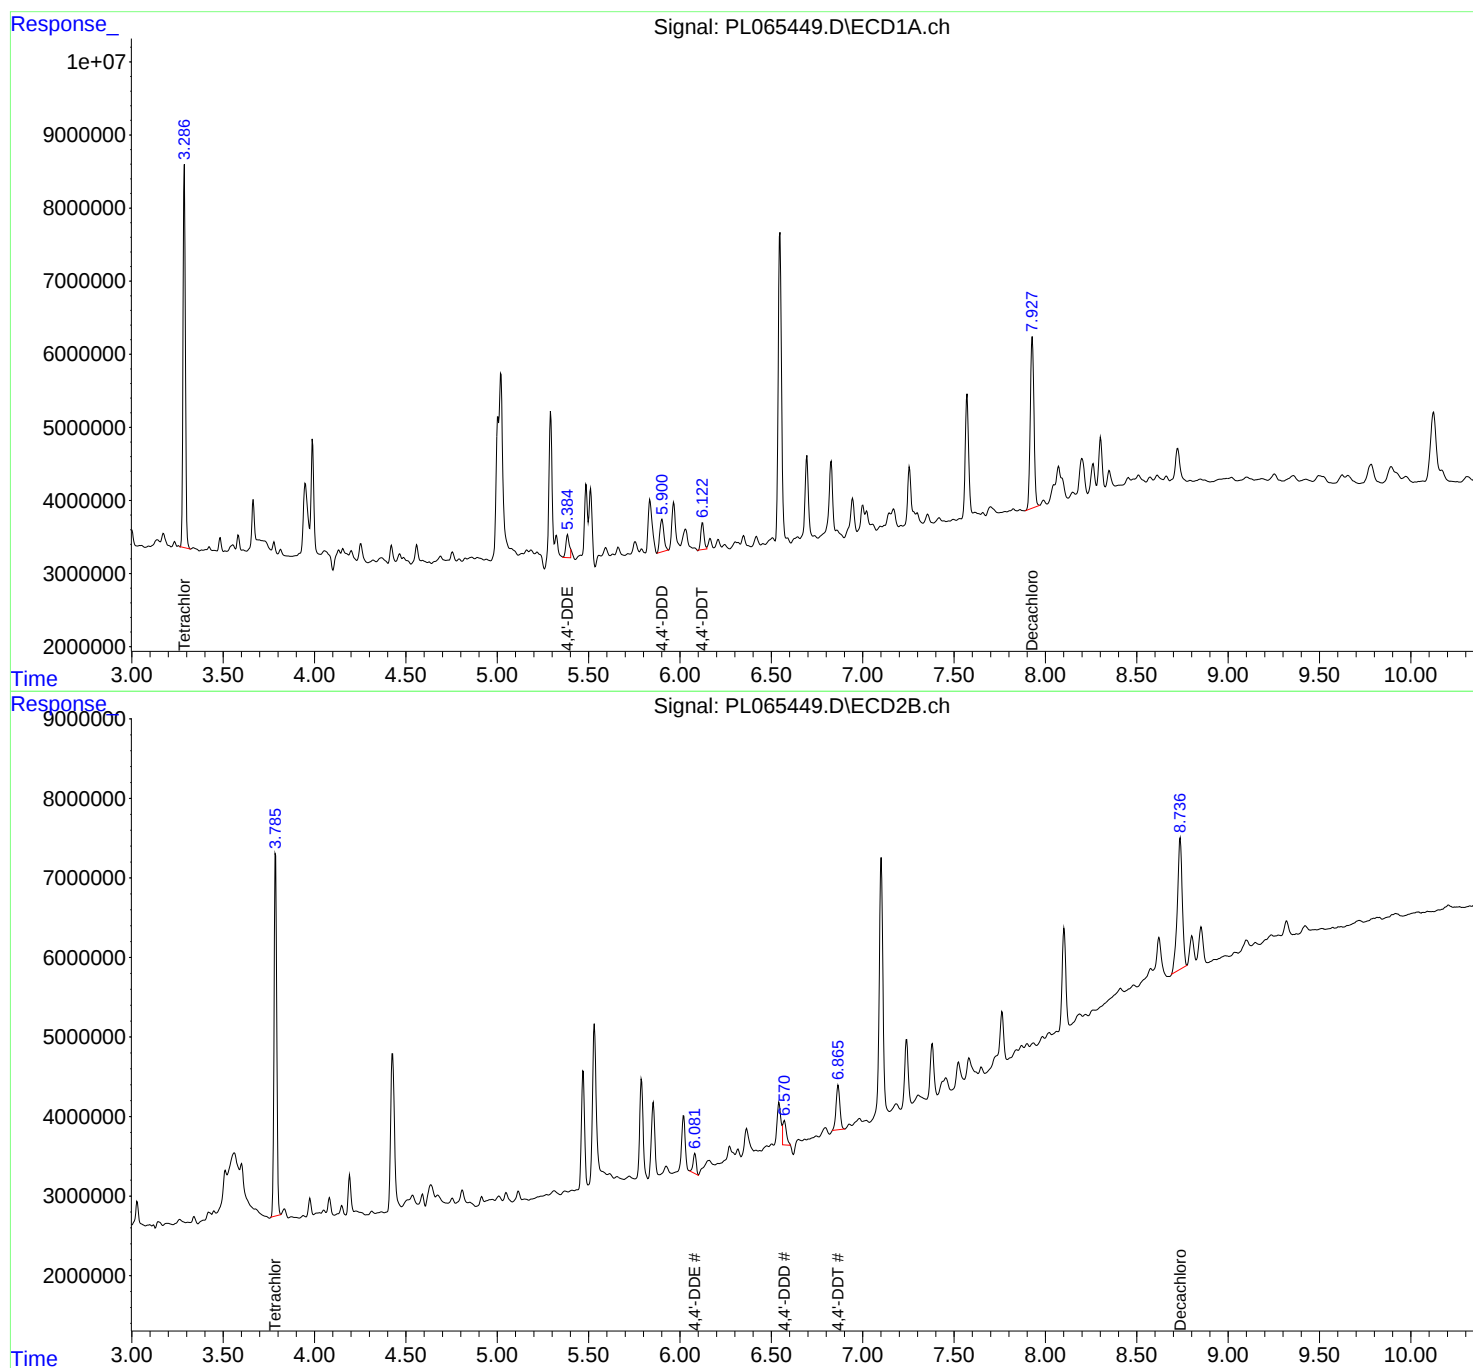

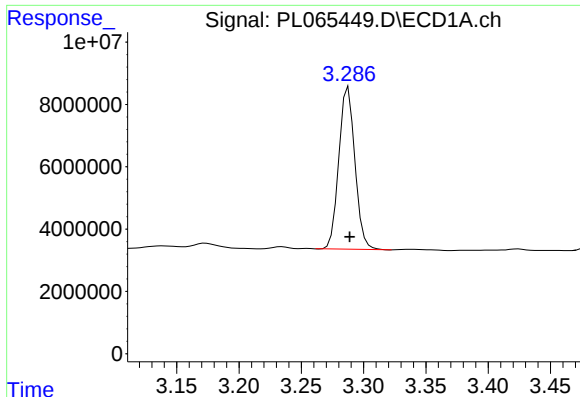


#1 Tetrachloro-m-xylene

R.T.: 3.288 min
Delta R.T.: -0.001 min
Response: 46832425
Conc: 19.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-031821


Manual Integrations
APPROVED

Ankita
3/22/2021 11:16:33 AM

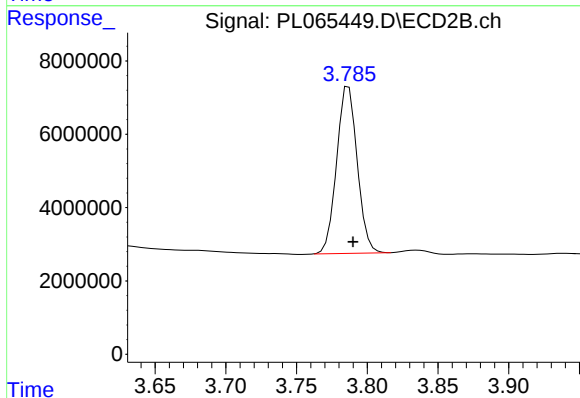


#1 Tetrachloro-m-xylene

R.T.: 3.787 min
Delta R.T.: -0.003 min
Response: 46217642
Conc: 16.84 ng/ml

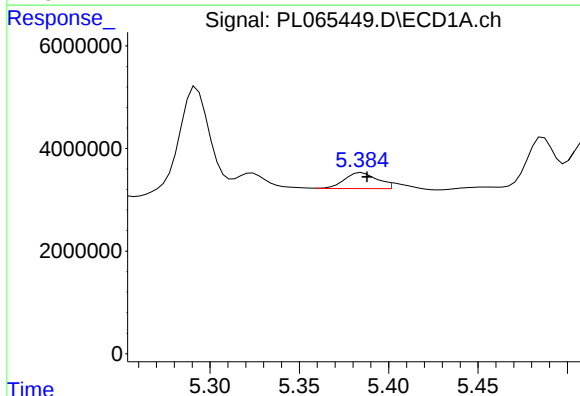


#12 4,4'-DDE

R.T.: 5.384 min
Delta R.T.: -0.004 min
Response: 4167607
Conc: 1.58 ng/ml m

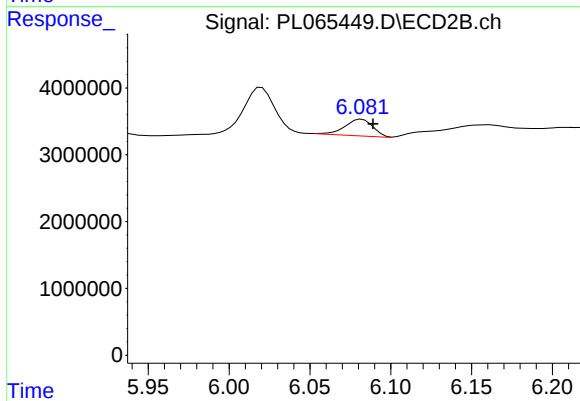

#12 4,4'-DDE

R.T.: 6.081 min
Delta R.T.: -0.008 min
Response: 2964854
Conc: 1.19 ng/ml m

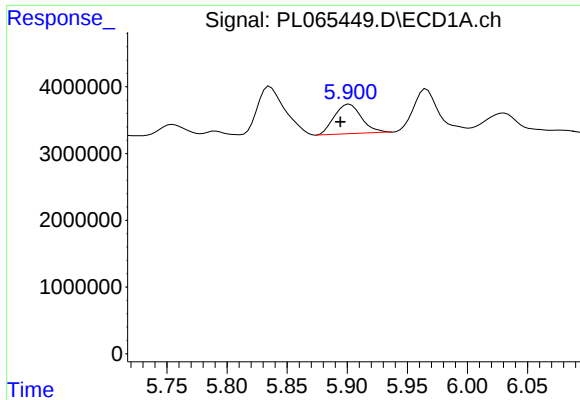


#16 4,4'-DDD

R.T.: 5.900 min
Delta R.T.: 0.006 min
Response: 6974008
Conc: 3.16 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TR-05-031821


Manual Integrations
APPROVED

Ankita
3/22/2021 11:16:33 AM

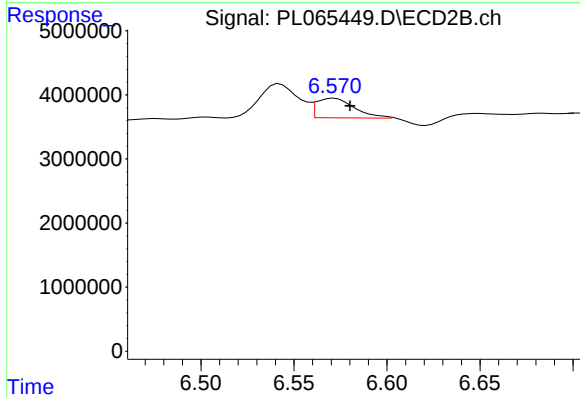


#16 4,4'-DDD

R.T.: 6.570 min
Delta R.T.: -0.010 min
Response: 4105961
Conc: 1.87 ng/ml m

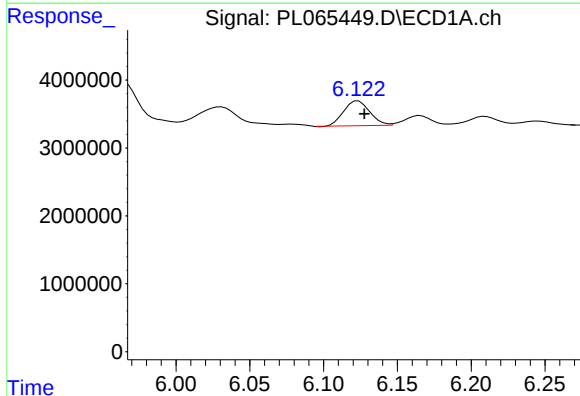


#17 4,4'-DDT

R.T.: 6.124 min
Delta R.T.: -0.004 min
Response: 4494489
Conc: 2.37 ng/ml

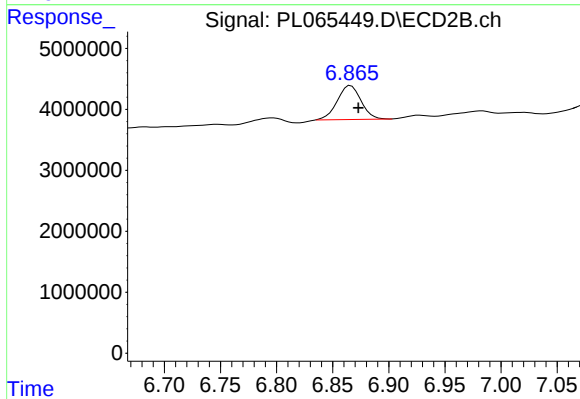

#17 4,4'-DDT

R.T.: 6.866 min
Delta R.T.: -0.007 min
Response: 8190861
Conc: 4.17 ng/ml

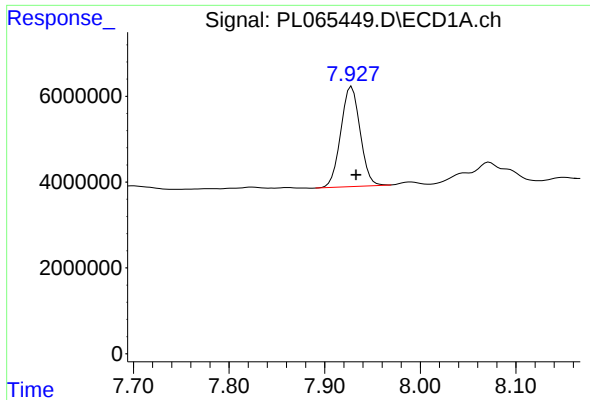


#28 Decachlorobiphenyl

R.T.: 7.928 min
Delta R.T.: -0.005 min
Response: 32935361
Conc: 13.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-05-031821

Manual Integrations
APPROVED

Ankita
3/22/2021 11:16:33 AM

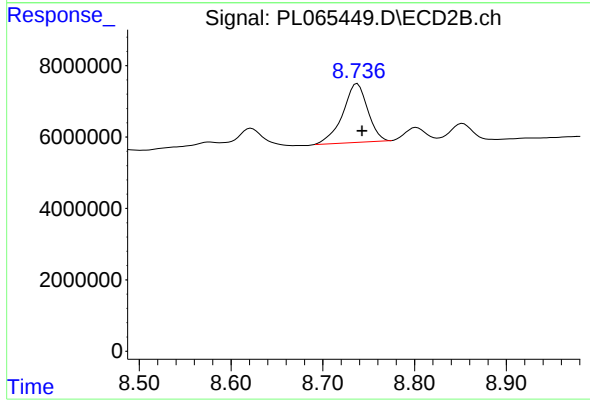

#28 Decachlorobiphenyl

R.T.: 8.738 min
Delta R.T.: -0.005 min
Response: 31017006
Conc: 15.65 ng/ml