

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031921\
 Data File : PL065456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2021 18:22
 Operator : AR\AJ
 Sample : M1724-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 26207

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 01:01:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.288	3.787	17138899	17892153	7.217	6.519
28)	SA Decachlor...	7.928	8.738	15005051	13869751	6.211	6.997
Target Compounds							
20)	A Methoxychlor	6.684	7.332	7900361	8827395	6.891	8.452



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031921\
Data File : PL065456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2021 18:22
Operator : AR\AJ
Sample : M1724-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
26207

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 01:01:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

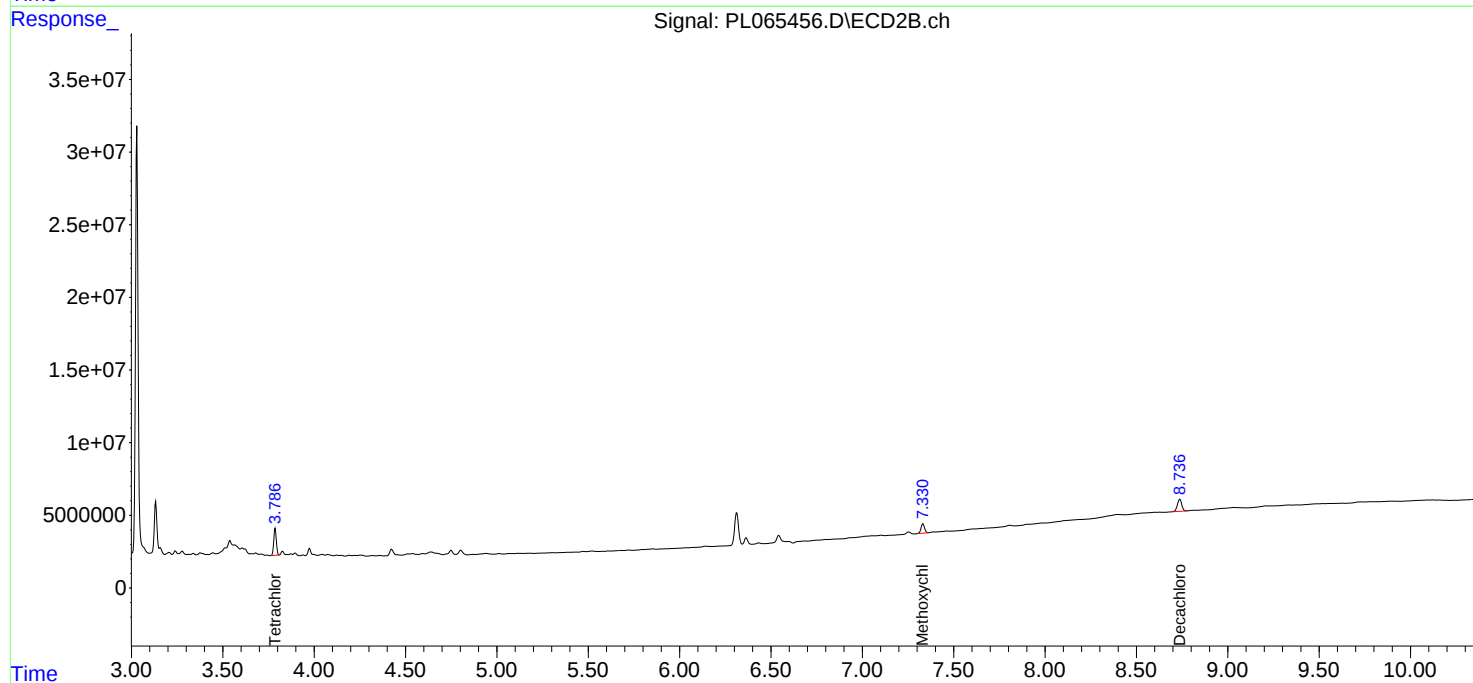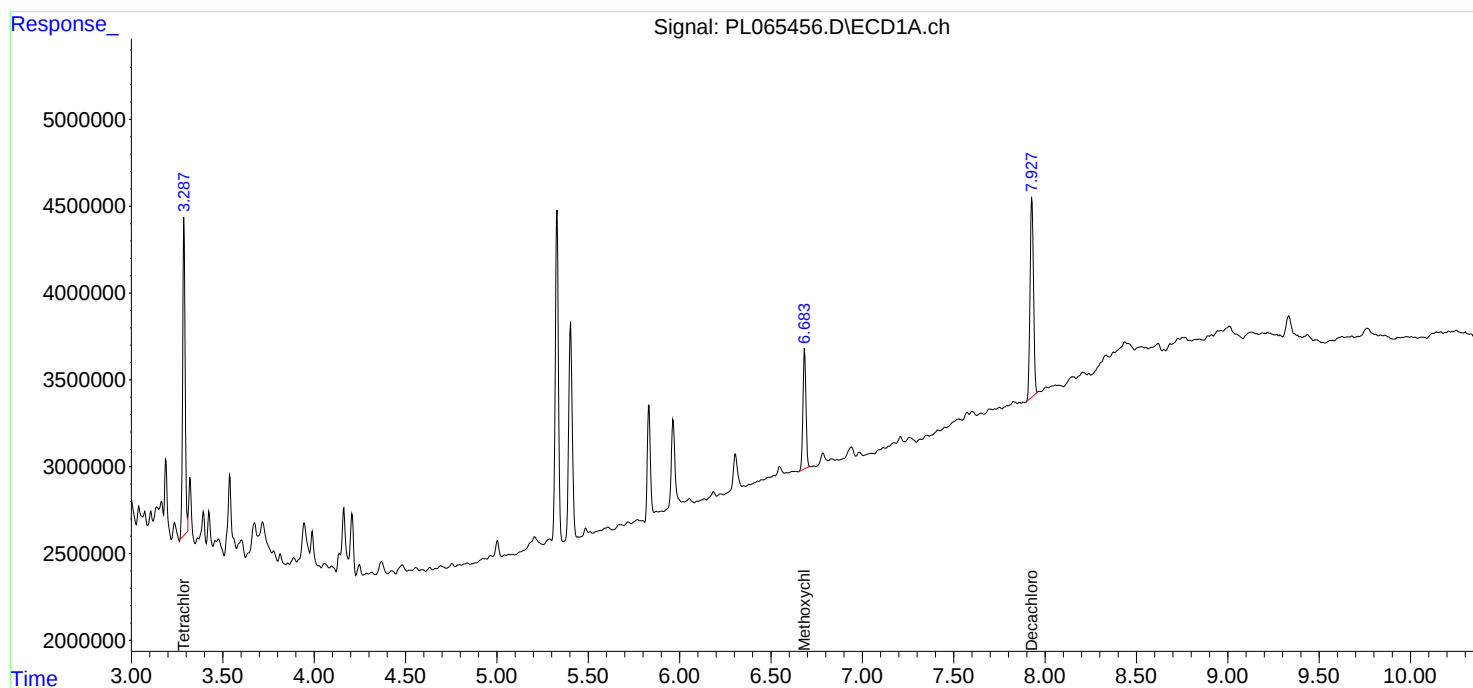


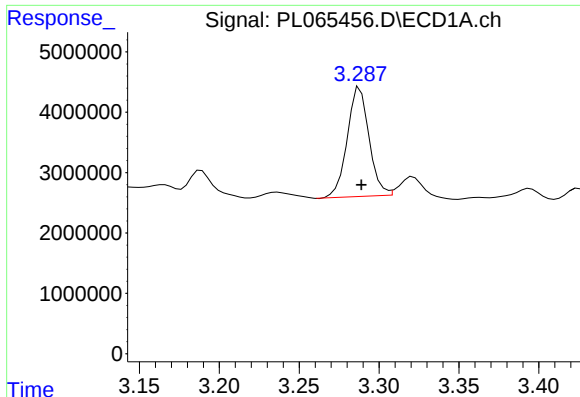

#1 Tetrachloro-m-xylene


R.T.: 3.288 min
Delta R.T.: 0.000 min
Response: 17138899
Conc: 7.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
26207

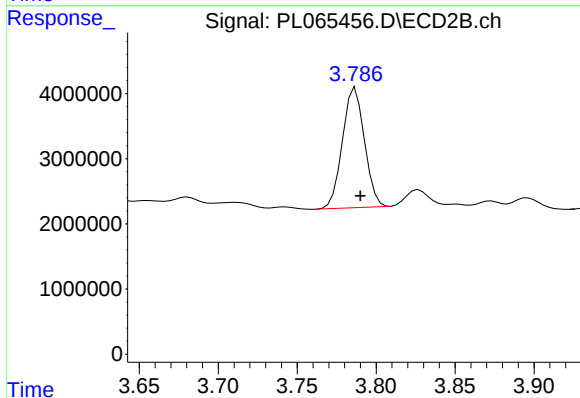


#1 Tetrachloro-m-xylene

R.T.: 3.787 min
Delta R.T.: -0.003 min
Response: 17892153
Conc: 6.52 ng/ml

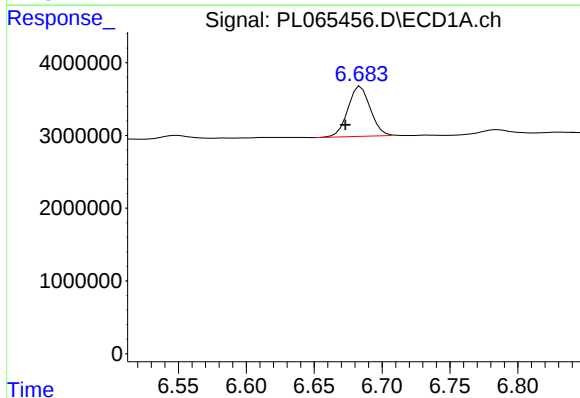


#20 Methoxychlor

R.T.: 6.684 min
Delta R.T.: 0.011 min
Response: 7900361
Conc: 6.89 ng/ml

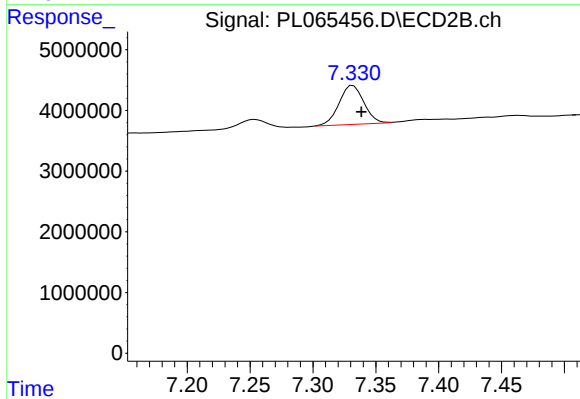

#20 Methoxychlor


R.T.: 7.332 min
Delta R.T.: -0.007 min
Response: 8827395
Conc: 8.45 ng/ml

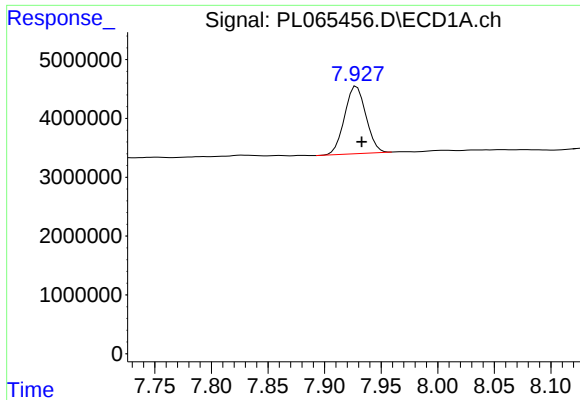

#28 Decachlorobiphenyl

R.T.: 7.928 min
Delta R.T.: -0.005 min
Response: 15005051
Conc: 6.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
26207

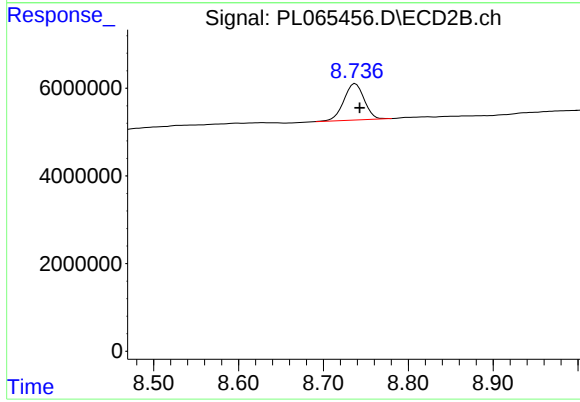

#28 Decachlorobiphenyl

R.T.: 8.738 min
Delta R.T.: -0.005 min
Response: 13869751
Conc: 7.00 ng/ml