

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031924\
 Data File : PL088677.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2024 14:23
 Operator : AR\AJ
 Sample : P1616-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 146-BAY-AVENUE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/20/2024
 Supervised By :Ankita Jodhani 03/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 01:06:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.634	2.850	25947655	12792290	9.792	9.598m
2) SA Decachlor...	9.306	8.082	18070568	8990156	7.310	6.630

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031924\
Data File : PL088677.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2024 14:23
Operator : AR\AJ
Sample : P1616-03
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
146-BAY-AVENUE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/20/2024
Supervised By : Ankita Jodhani 03/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 01:06:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

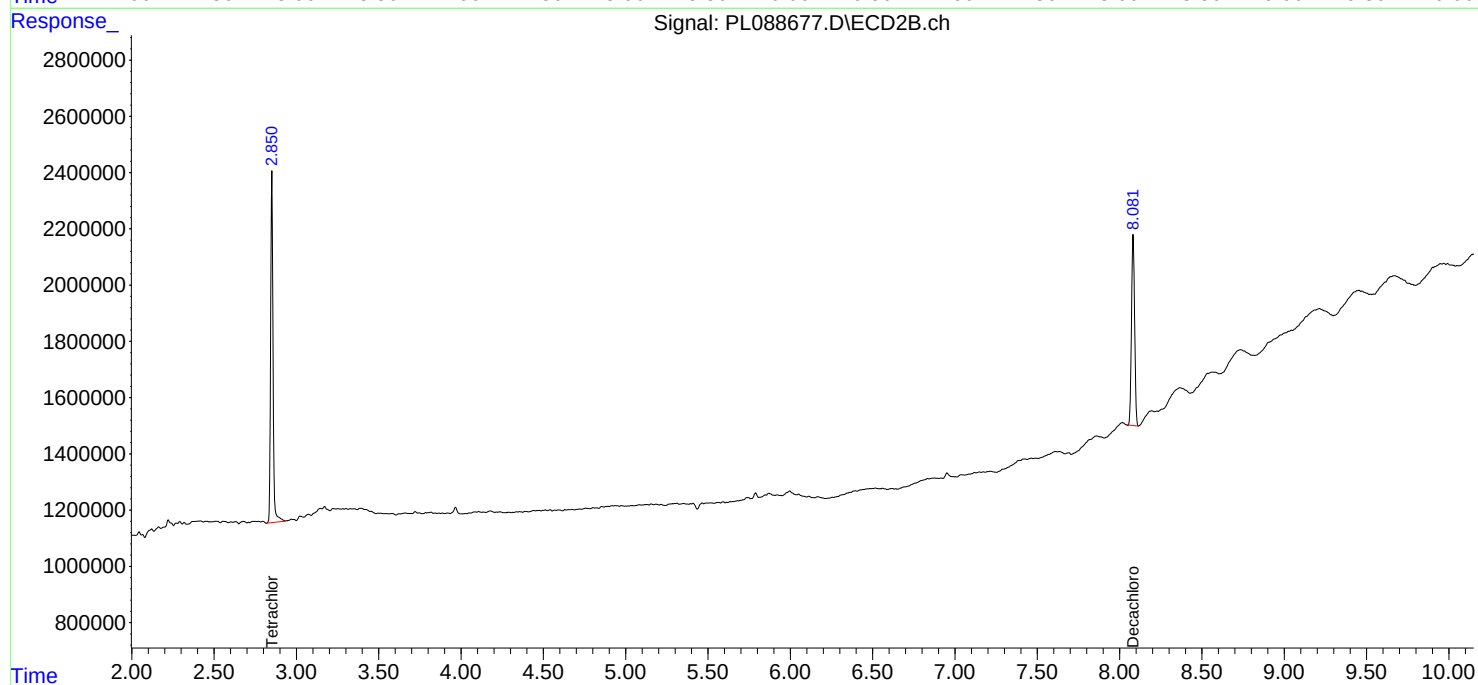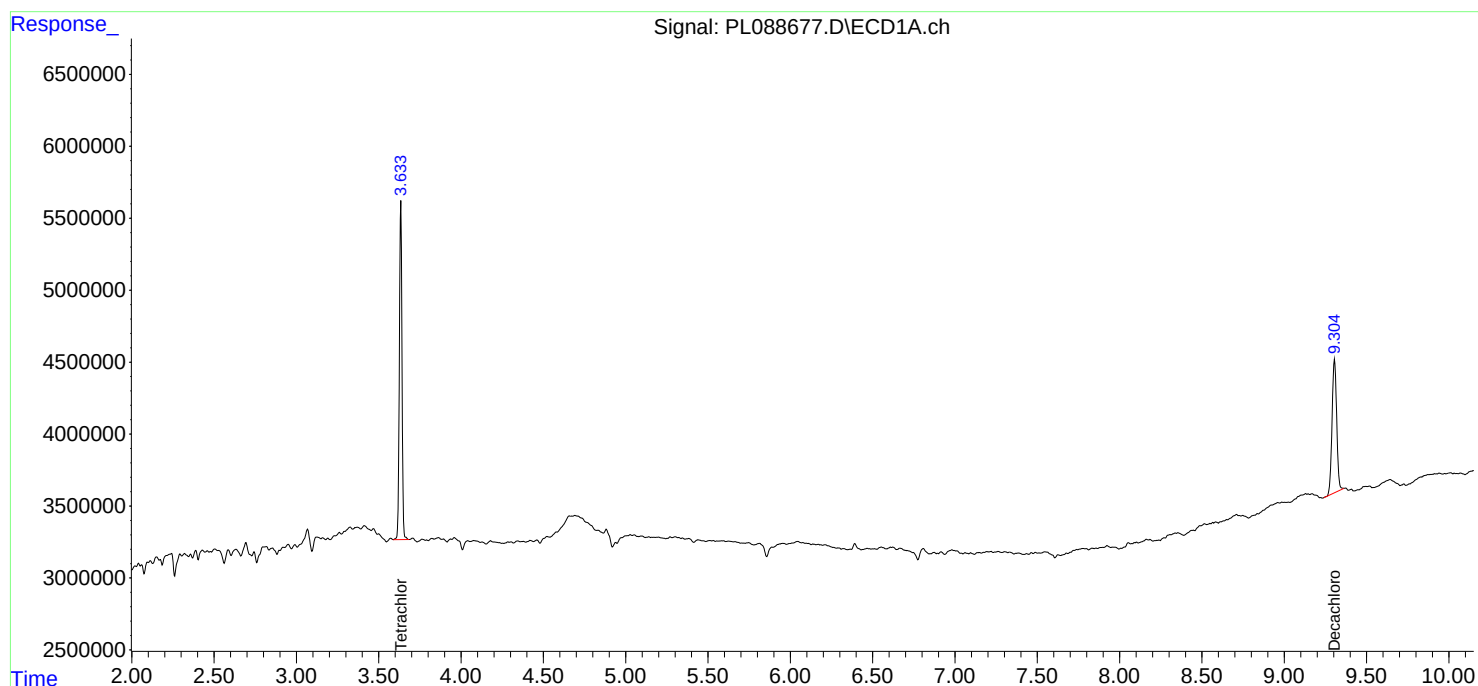

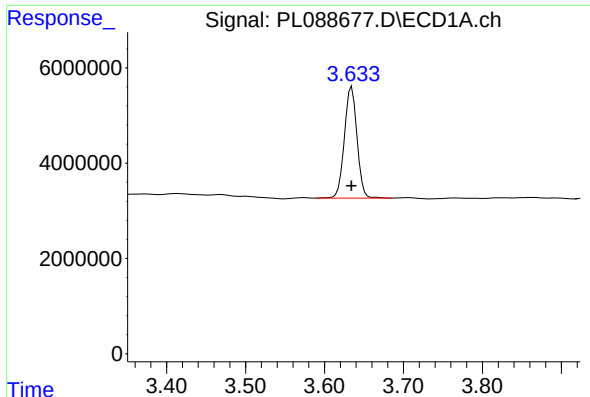


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 25947655
Conc: 9.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
146-BAY-AVENUE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/20/2024
Supervised By :Ankita Jodhani 03/20/2024

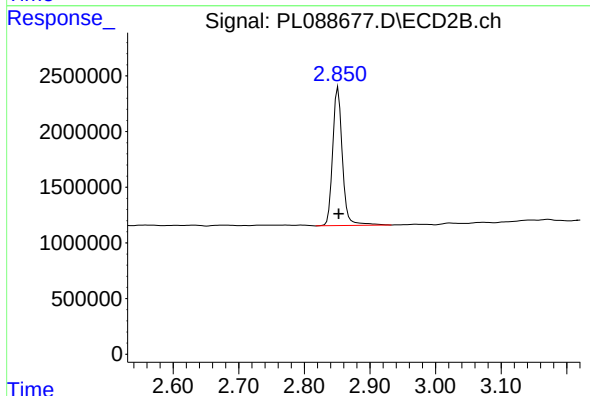


#1 Tetrachloro-m-xylene

R.T.: 2.850 min
Delta R.T.: -0.002 min
Response: 12792290
Conc: 9.60 ng/ml m

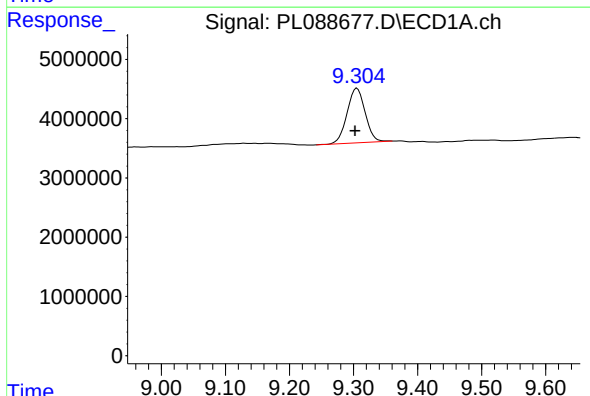

#28 Decachlorobiphenyl

R.T.: 9.306 min
Delta R.T.: 0.003 min
Response: 18070568
Conc: 7.31 ng/ml

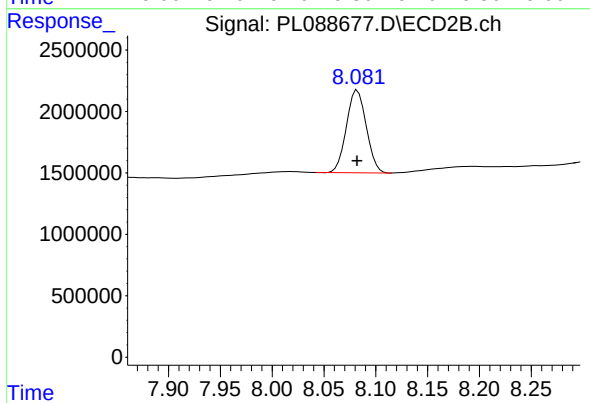

#28 Decachlorobiphenyl

R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 8990156
Conc: 6.63 ng/ml