

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031924\
 Data File : PL088682.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2024 15:32
 Operator : AR\AJ
 Sample : P1786-02 5X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-22

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/20/2024
 Supervised By : Ankita Jodhani 03/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 01:11:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.634	2.851	13440985	6304186	5.072	4.730
2) SA Decachlor...	9.304	8.082	9592447	5626222	3.881m	4.149

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031924\
Data File : PL088682.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2024 15:32
Operator : AR\AJ
Sample : P1786-02 5X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-22


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/20/2024
Supervised By : Ankita Jodhani 03/20/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 01:11:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

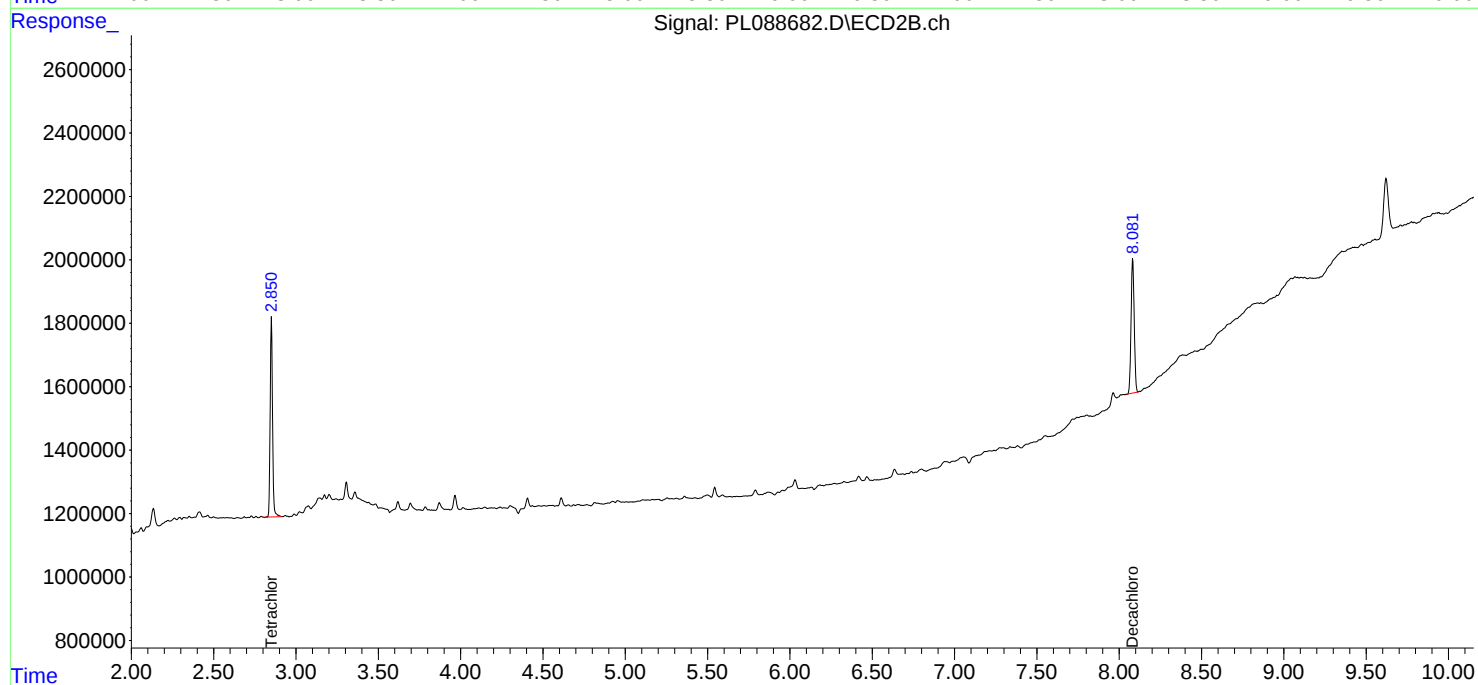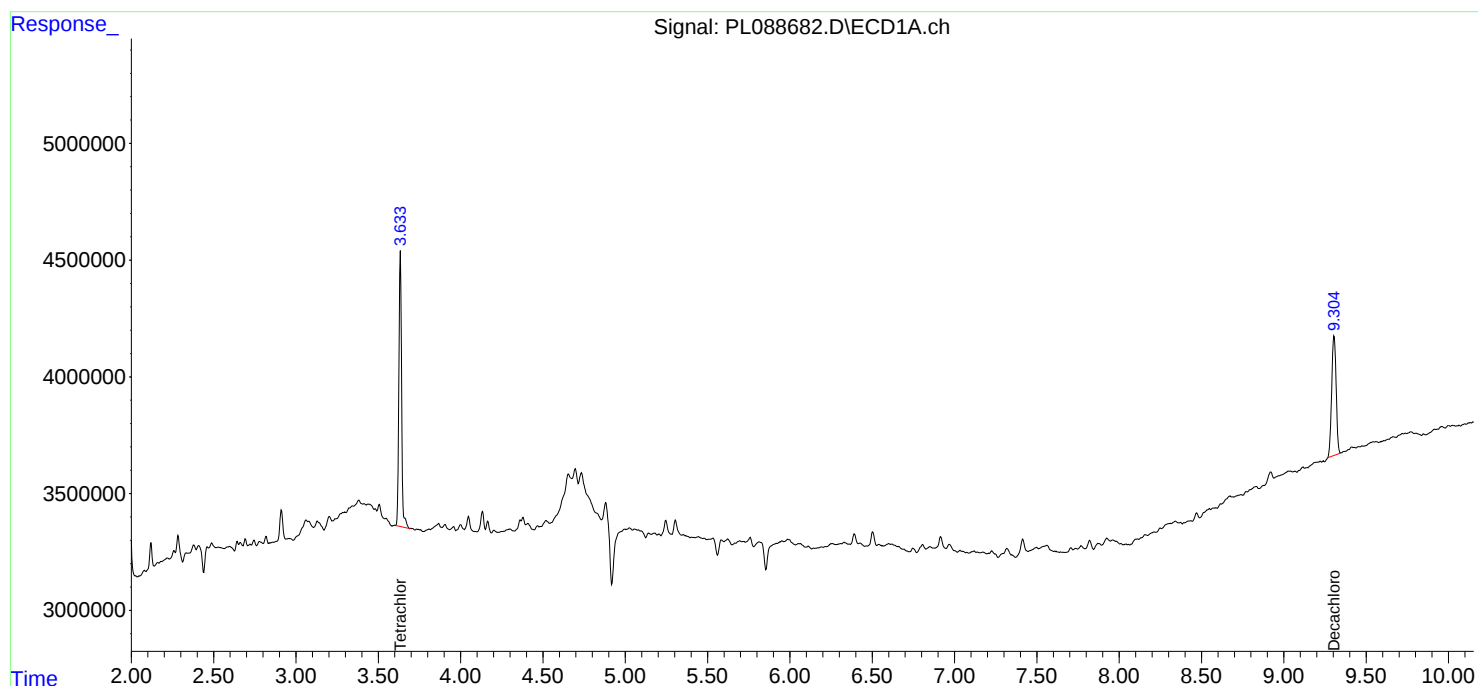

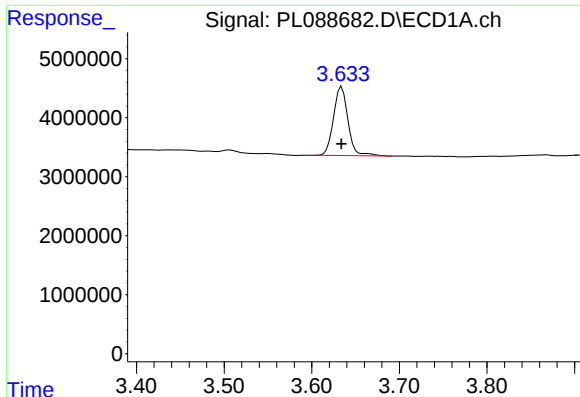


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 13440985
Conc: 5.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-22


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/20/2024
Supervised By :Ankita Jodhani 03/20/2024

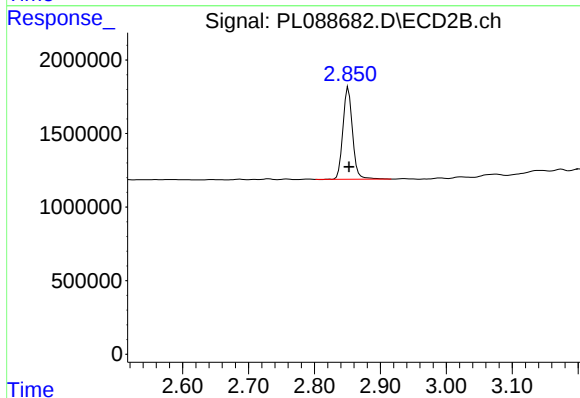


#1 Tetrachloro-m-xylene

R.T.: 2.851 min
Delta R.T.: 0.000 min
Response: 6304186
Conc: 4.73 ng/ml

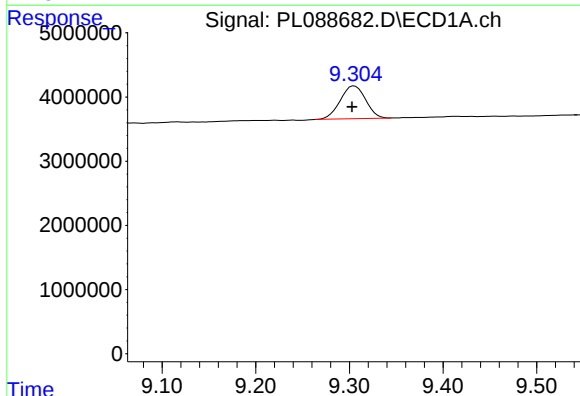

#28 Decachlorobiphenyl

R.T.: 9.304 min
Delta R.T.: 0.001 min
Response: 9592447
Conc: 3.88 ng/ml m

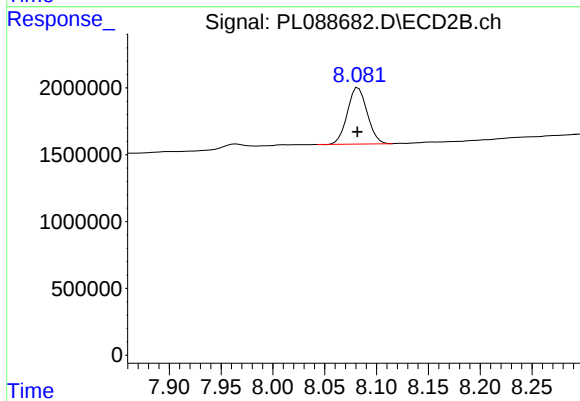

#28 Decachlorobiphenyl

R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 5626222
Conc: 4.15 ng/ml