

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031925\
 Data File : PL094748.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2025 18:36
 Operator : AR\AJ
 Sample : Q1597-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2-CONCRETE-SLAB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 02:08:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.771	50883659	81818174	17.976	22.923 #
28)	SA Decachlor...	9.051	7.904	38466691	77567652	18.253	19.203
Target Compounds							
3)	MA gamma-BHC...	0.000	3.611	0	6271744	N.D.	1.220 #
7)	B delta-BHC	4.760	0.000	9774440	0	2.510	N.D. #
12)	B 4,4'-DDE	0.000	5.206f	0	19975532	N.D.	4.297 #
14)	MA Endrin	0.000	5.650f	0	34612214	N.D.	7.932 #
18)	B Endrin al...	0.000	6.119	0	3883911	N.D.	1.154 #
20)	A Methoxychlor	0.000	6.597	0	69471707	N.D.	32.753 #
21)	B Endrin ke...	0.000	6.824	0	141.8E6	N.D.	29.721 #
23)	Chlordane-1	0.000	3.780	0	2484524	N.D.	16.450 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031925\
Data File : PL094748.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2025 18:36
Operator : AR\AJ
Sample : Q1597-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
2-CONCRETE-SLAB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 02:08:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

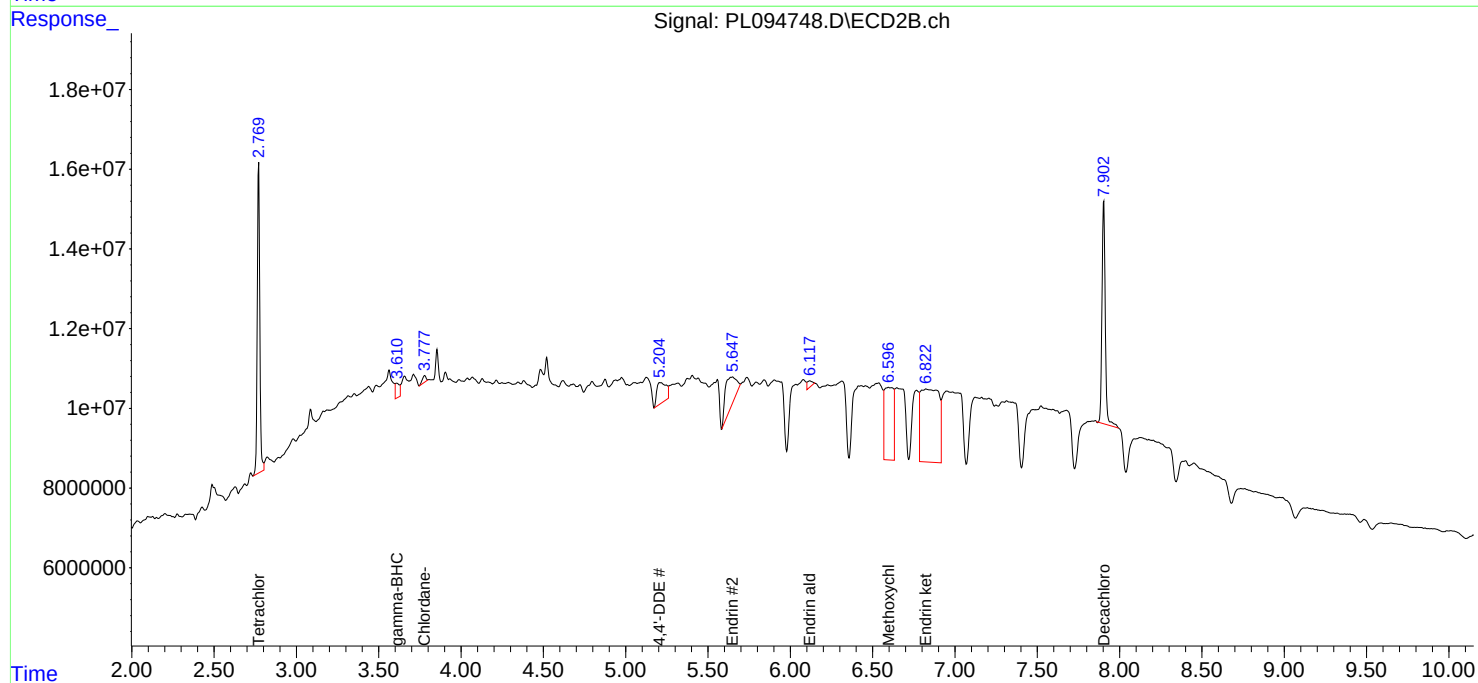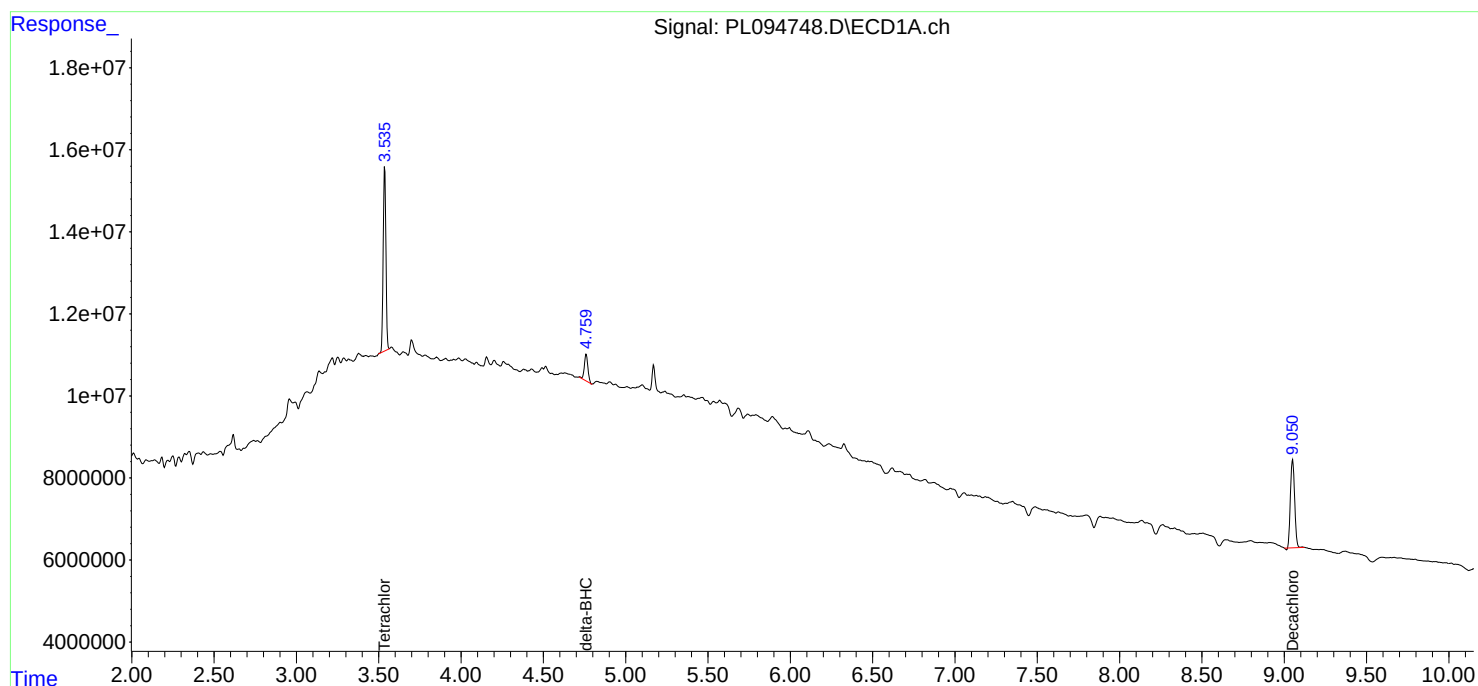


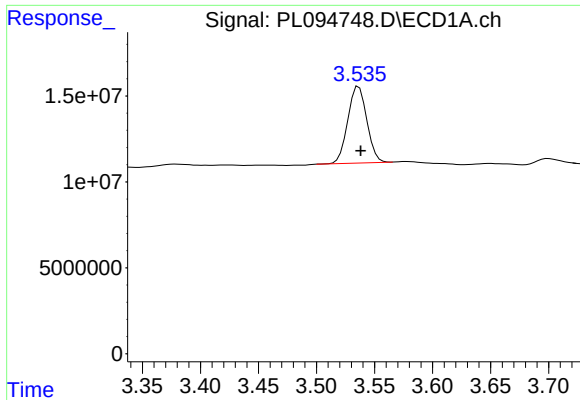

#1 Tetrachloro-m-xylene


R.T.: 3.536 min
Delta R.T.: -0.002 min
Response: 50883659
Conc: 17.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
2-CONCRETE-SLAB

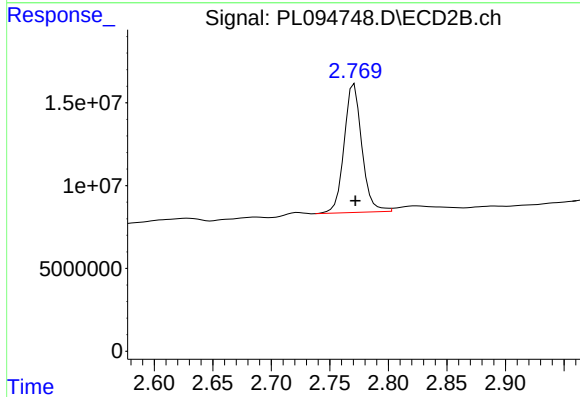


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: -0.001 min
Response: 81818174
Conc: 22.92 ng/ml

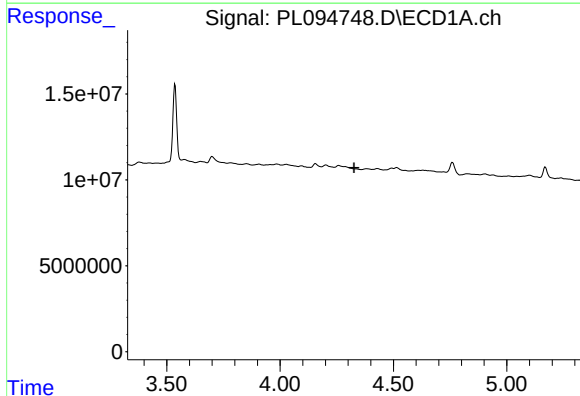


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.327 min
Response: 0
Conc: N.D.

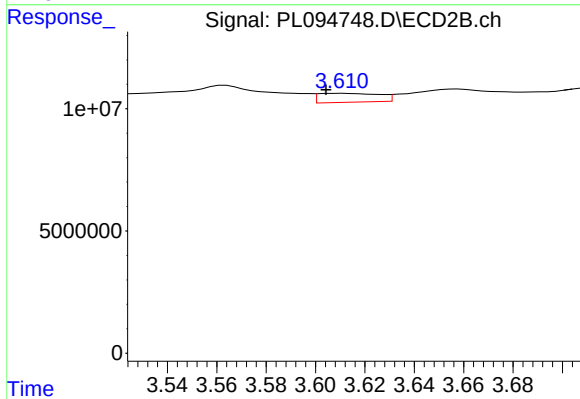

#3 gamma-BHC (Lindane)


R.T.: 3.611 min
Delta R.T.: 0.006 min
Response: 6271744
Conc: 1.22 ng/ml

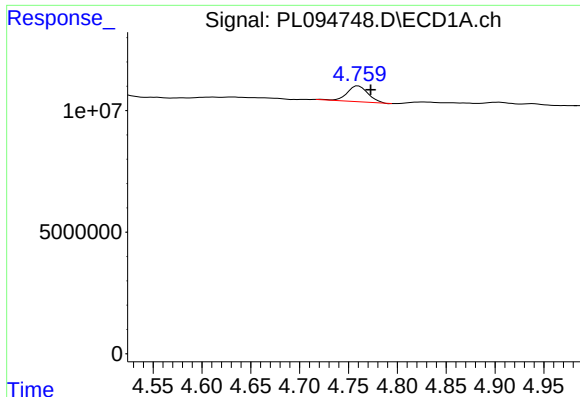

#7 delta-BHC


R.T.: 4.760 min
Delta R.T.: -0.013 min
Response: 9774440
Conc: 2.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
2-CONCRETE-SLAB

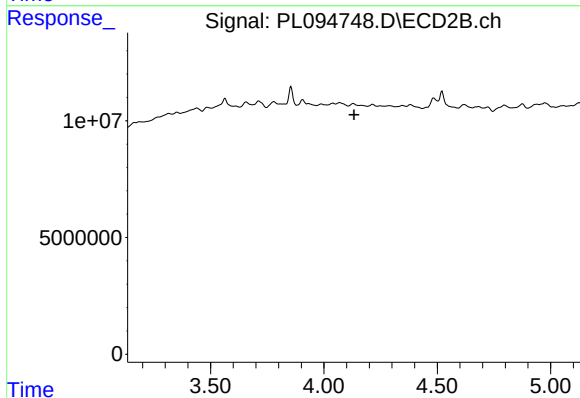


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.133 min
Response: 0
Conc: N.D.

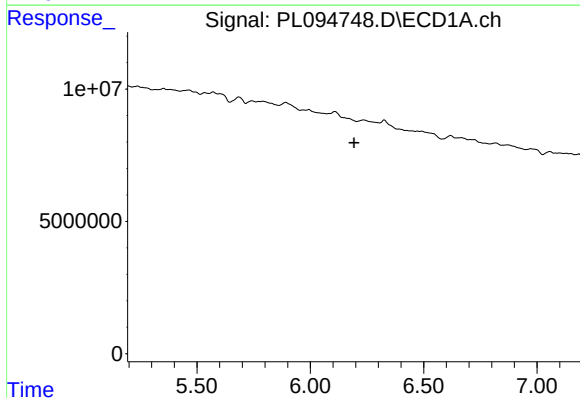


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.193 min
Response: 0
Conc: N.D.

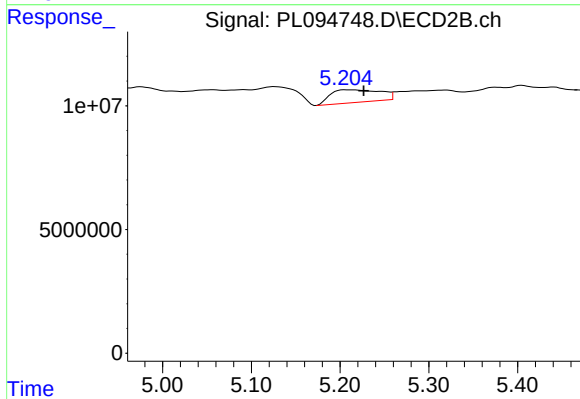

#12 4,4'-DDE


R.T.: 5.206 min
Delta R.T.: -0.021 min
Response: 19975532
Conc: 4.30 ng/ml

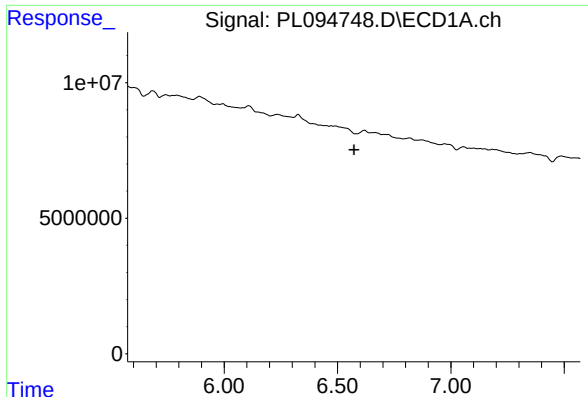

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
2-CONCRETE-SLAB

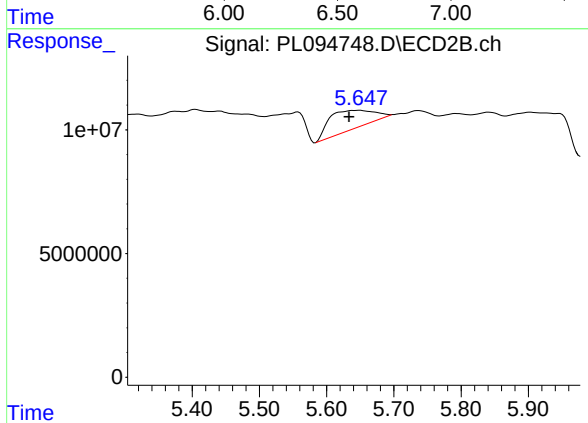


#14 Endrin

R.T.: 5.650 min
Delta R.T.: 0.016 min
Response: 34612214
Conc: 7.93 ng/ml

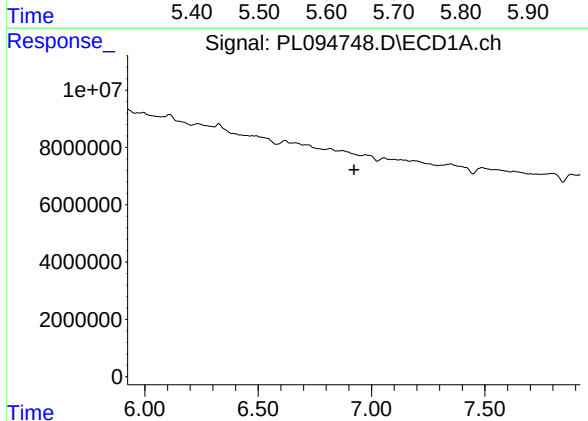


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.924 min
Response: 0
Conc: N.D.

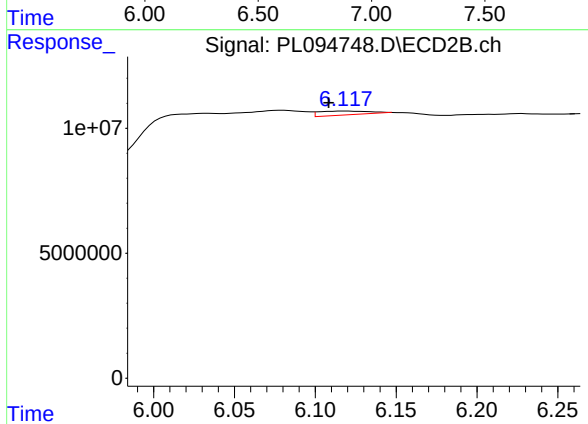

#18 Endrin aldehyde


R.T.: 6.119 min
Delta R.T.: 0.011 min
Response: 3883911
Conc: 1.15 ng/ml

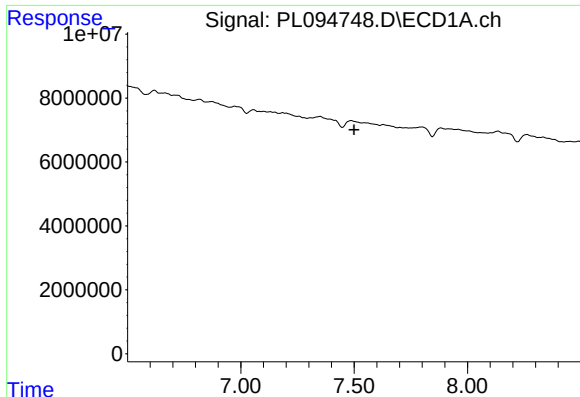

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.500 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
2-CONCRETE-SLAB

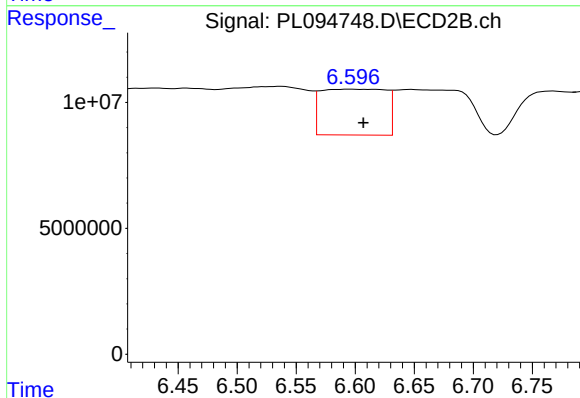


#20 Methoxychlor

R.T.: 6.597 min
Delta R.T.: -0.010 min
Response: 69471707
Conc: 32.75 ng/ml

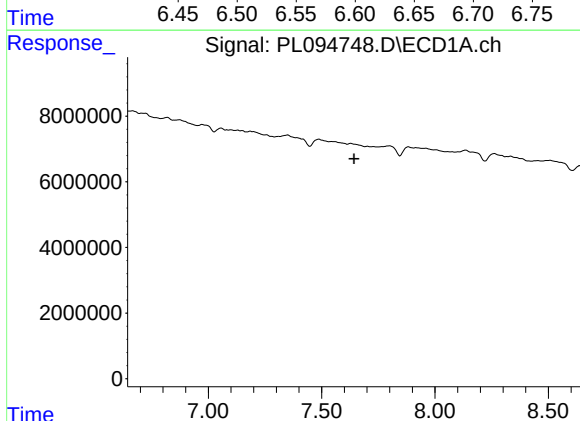


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 7.644 min
Response: 0
Conc: N.D.

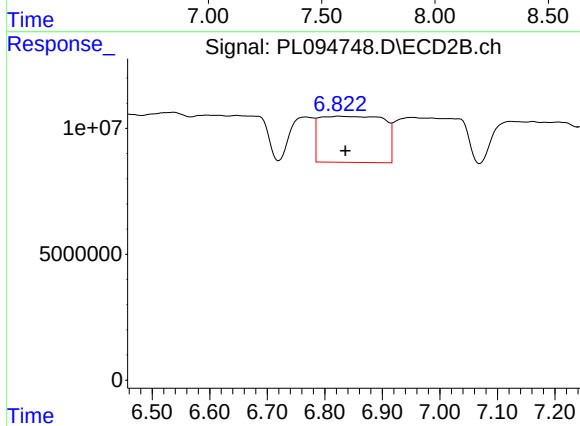

#21 Endrin ketone


R.T.: 6.824 min
Delta R.T.: -0.012 min
Response: 141845181
Conc: 29.72 ng/ml

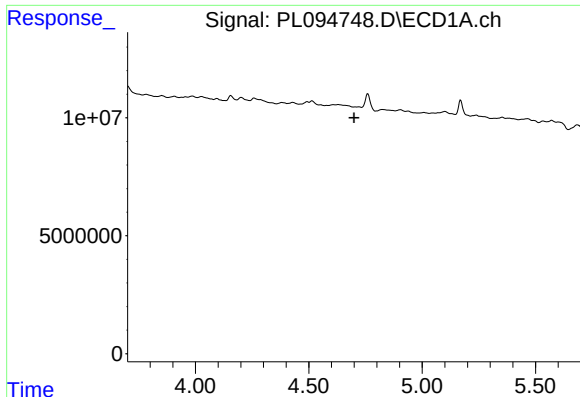

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.700 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
2-CONCRETE-SLAB

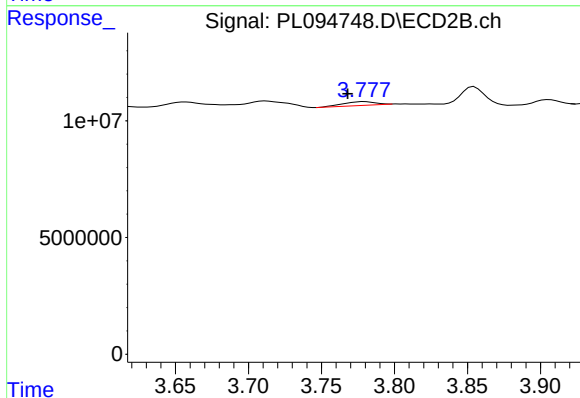


#23 Chlordane-1

R.T.: 3.780 min
Delta R.T.: 0.011 min
Response: 2484524
Conc: 16.45 ng/ml

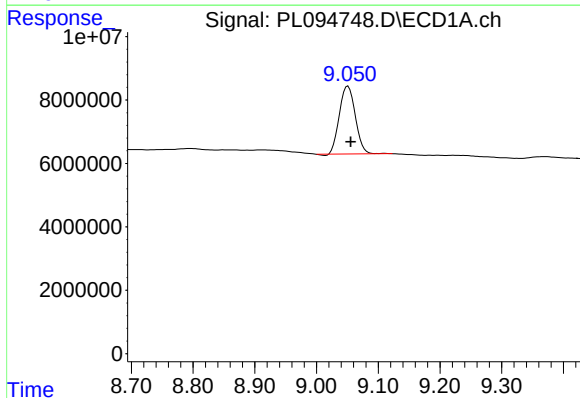

#28 Decachlorobiphenyl

R.T.: 9.051 min
Delta R.T.: -0.005 min
Response: 38466691
Conc: 18.25 ng/ml

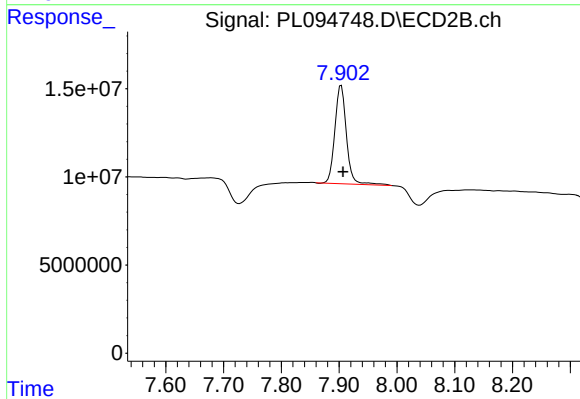

#28 Decachlorobiphenyl

R.T.: 7.904 min
Delta R.T.: -0.003 min
Response: 77567652
Conc: 19.20 ng/ml