

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031925\
 Data File : PL094761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Mar 2025 21:47
 Operator : AR\AJ
 Sample : PP24305
 Misc : PEST/PCB SURR 20/40PPB
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 01:13:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.770	63697497	84396614	22.503	23.645
28)	SA Decachlor...	9.049	7.902	59081456	103.9E6	28.034	25.713
Target Compounds							
7)	B delta-BHC	4.760	0.000	8584595	0	2.204	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031925\
Data File : PL094761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Mar 2025 21:47
Operator : AR\AJ
Sample : PP24305
Misc : PEST/PCB SURR 20/40PPB
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 01:13:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

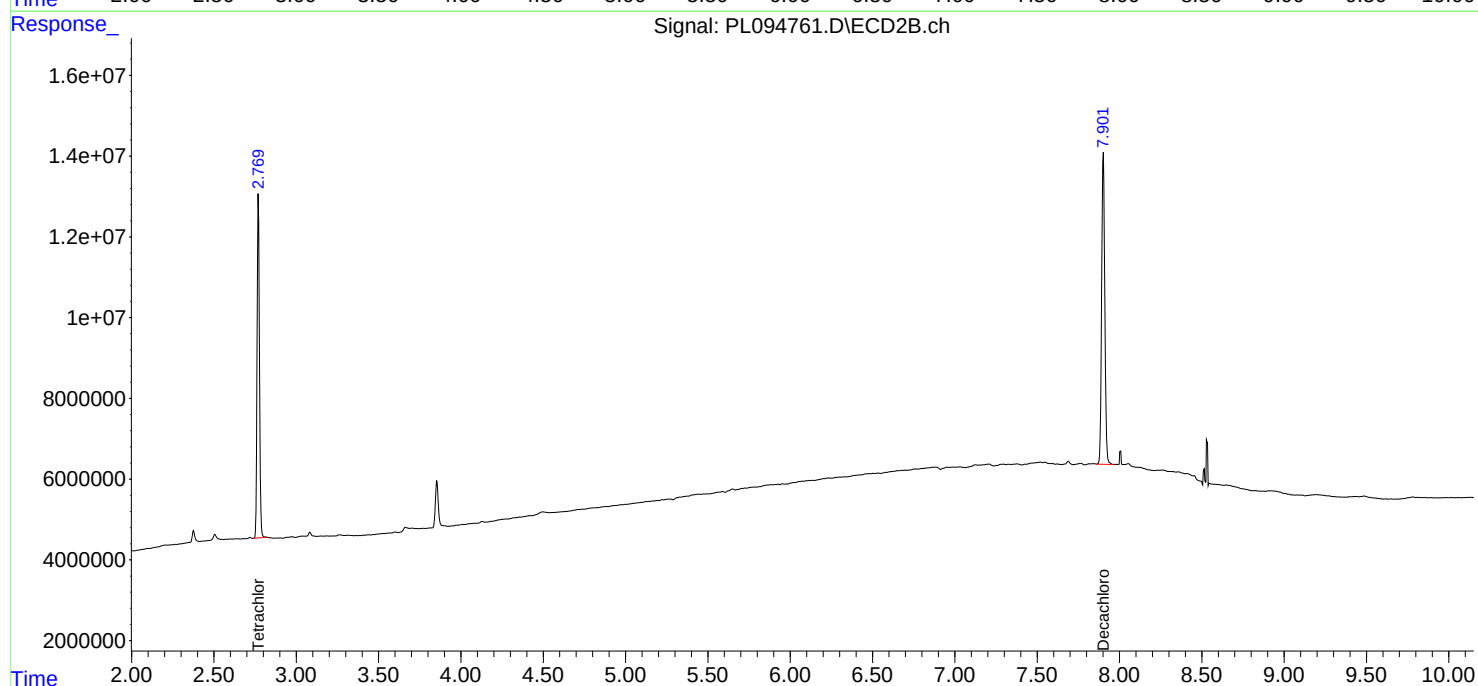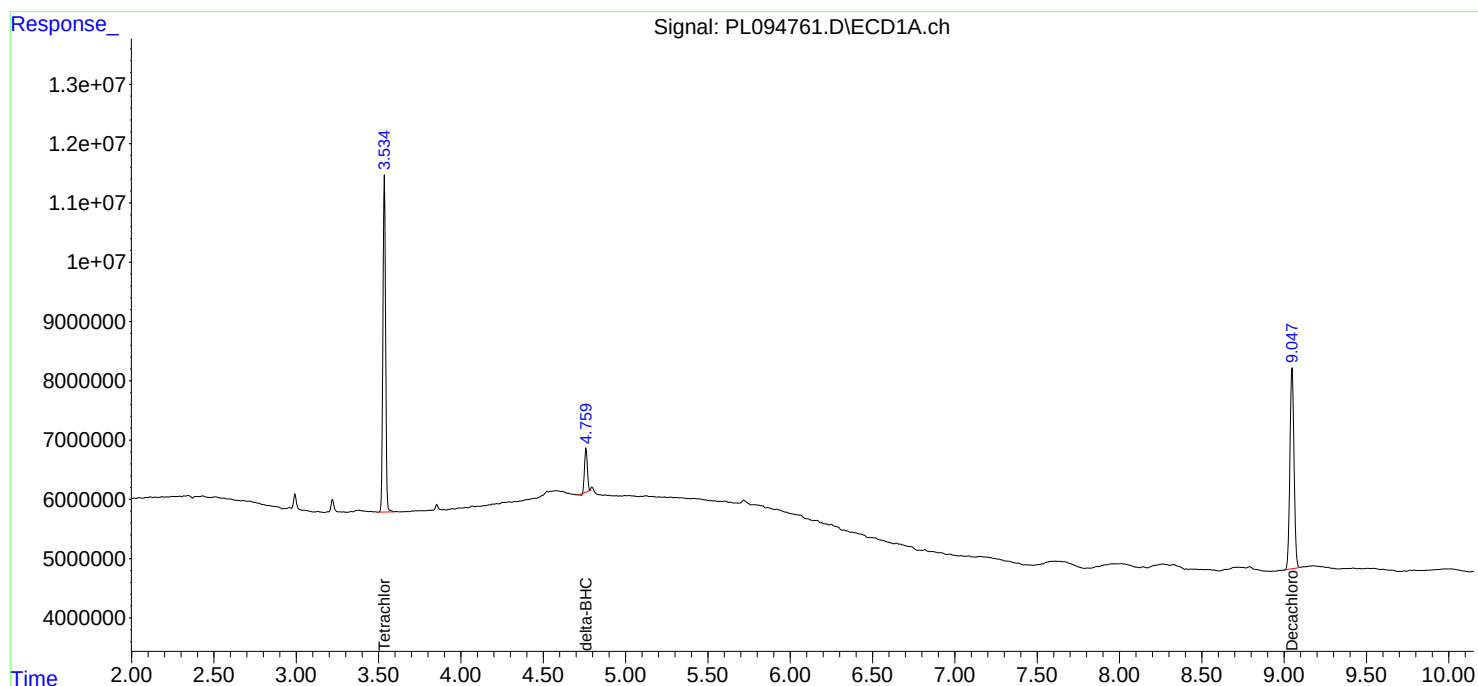


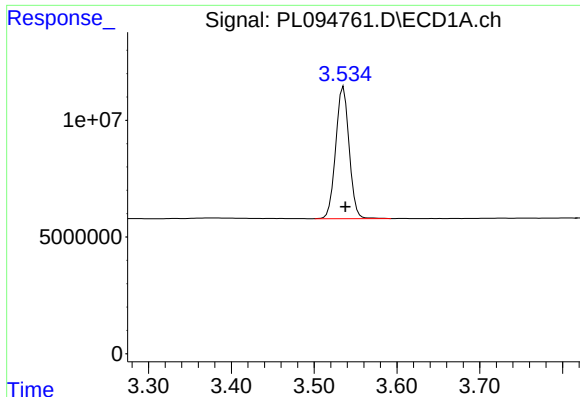

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: -0.003 min
Response: 63697497
Conc: 22.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

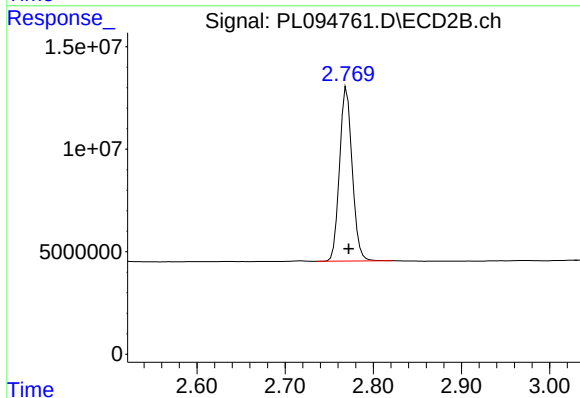


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.002 min
Response: 84396614
Conc: 23.65 ng/ml

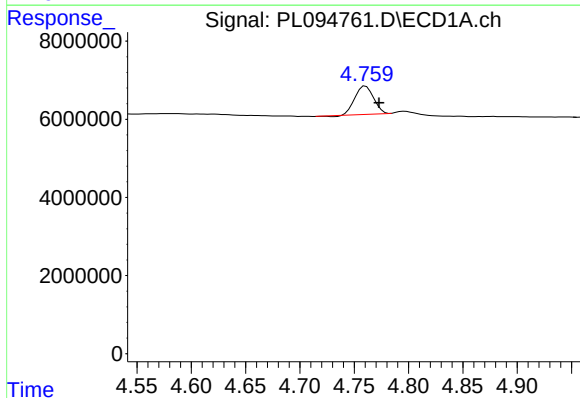


#7 delta-BHC

R.T.: 4.760 min
Delta R.T.: -0.012 min
Response: 8584595
Conc: 2.20 ng/ml

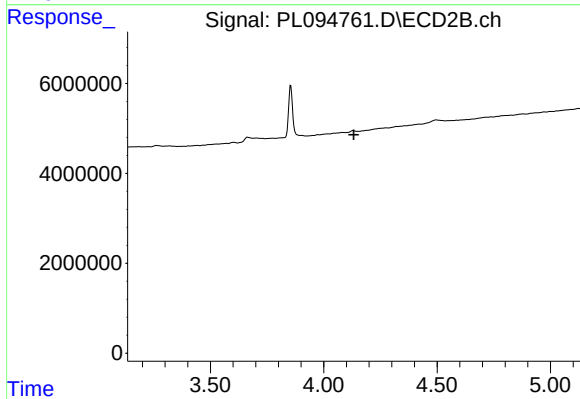

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.133 min
Response: 0
Conc: N.D.

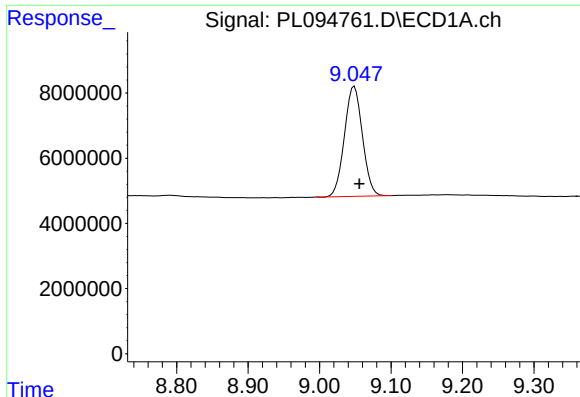

#28 Decachlorobiphenyl

R.T.: 9.049 min
Delta R.T.: -0.007 min
Response: 59081456
Conc: 28.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

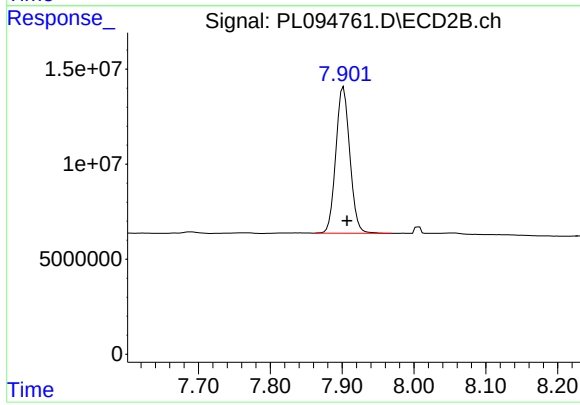

#28 Decachlorobiphenyl

R.T.: 7.902 min
Delta R.T.: -0.005 min
Response: 103863436
Conc: 25.71 ng/ml