

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032019\
 Data File : PL046186.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2019 09:30
 Operator : AJ\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 13:06:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	4.329f	5.149	16083773	4786137	1.524	1.609
6) B	beta-BHC	4.329	0.000	16083773	0	3.753	N.D. #
10) B	gamma-Chl...	5.287f	0.000	11534663	0	1.179	N.D. #
11) B	alpha-Chl...	5.287f	0.000	11534663	0	1.190	N.D. #
12) B	4,4'-DDE	0.000	6.317	0	4643148	N.D.	1.988 #
16) A	4,4'-DDD	0.000	6.826f	0	1737905	N.D.	0.904 #
21) B	Endrin ke...	7.020f	0.000	2344859	0	0.255	N.D. #
25)	Chlordane-3	5.287f	0.000	11534663	0	10.056	N.D. #
27)	Chlordane-5	0.000	6.979	0	3079087	N.D.	33.897 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032019\
Data File : PL046186.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2019 09:30
Operator : AJ\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 13:06:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

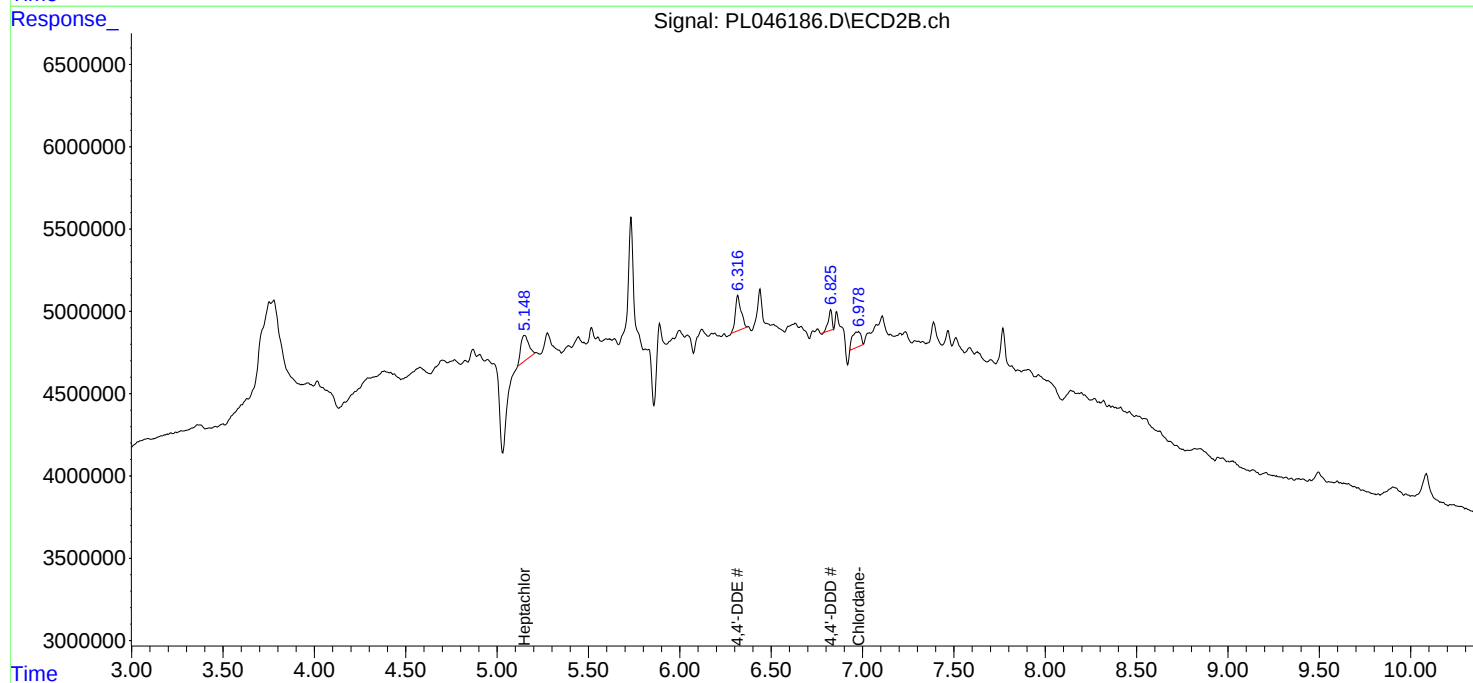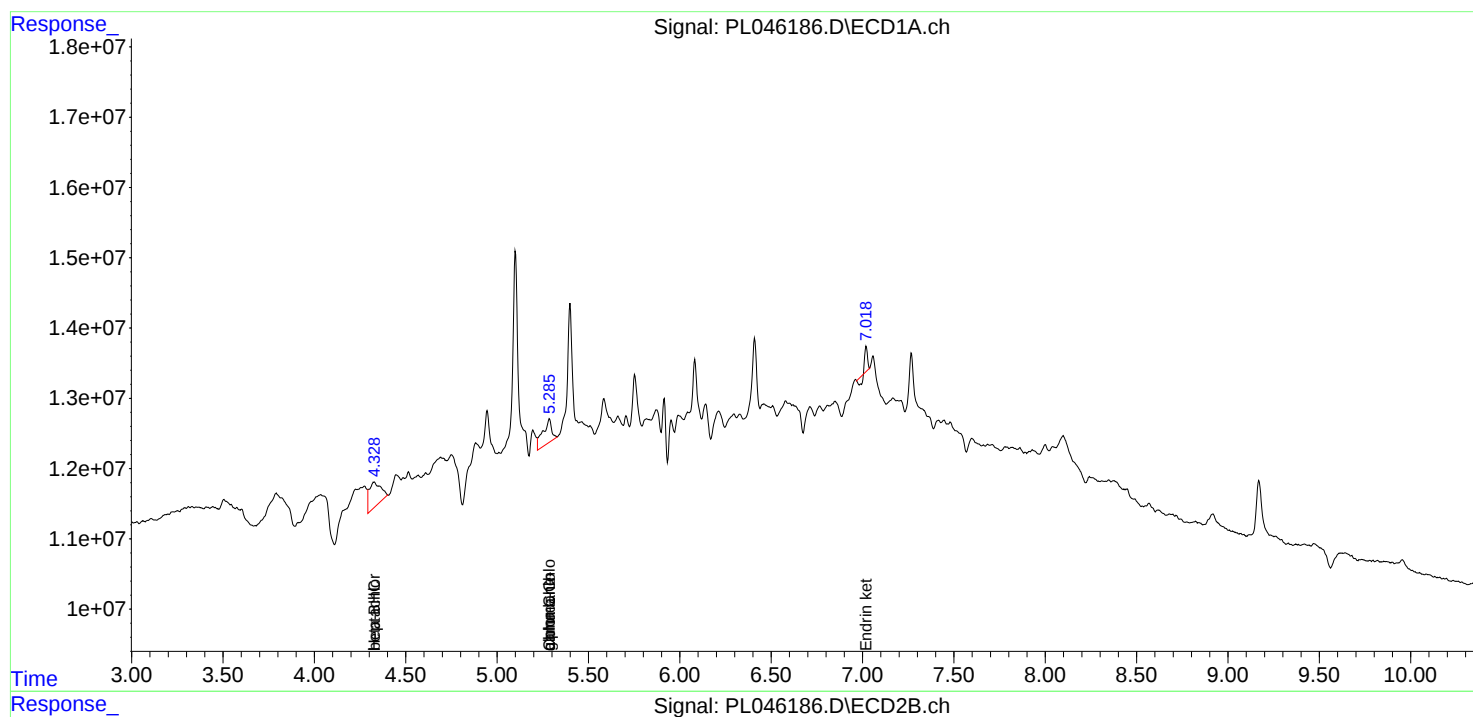


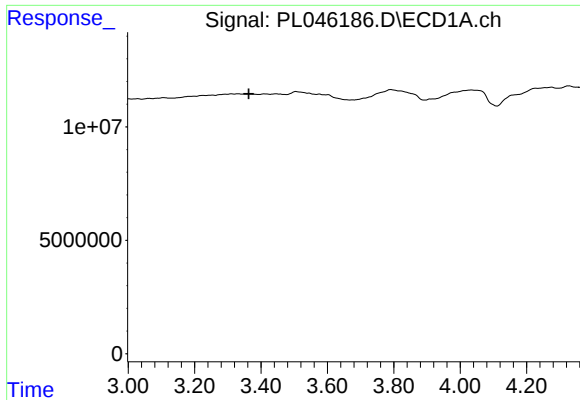

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

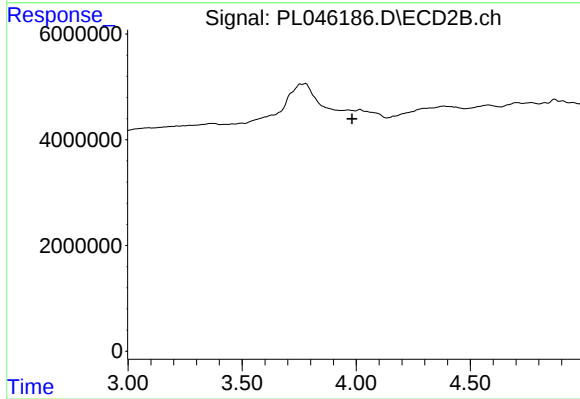


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.982 min
Response: 0
Conc: N.D.

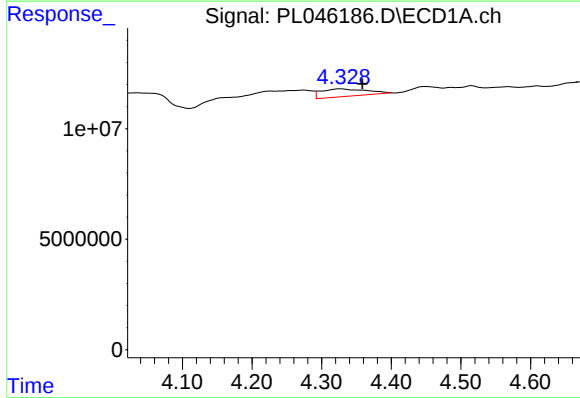


#4 Heptachlor

R.T.: 4.329 min
Delta R.T.: -0.030 min
Response: 16083773
Conc: 1.52 ng/ml

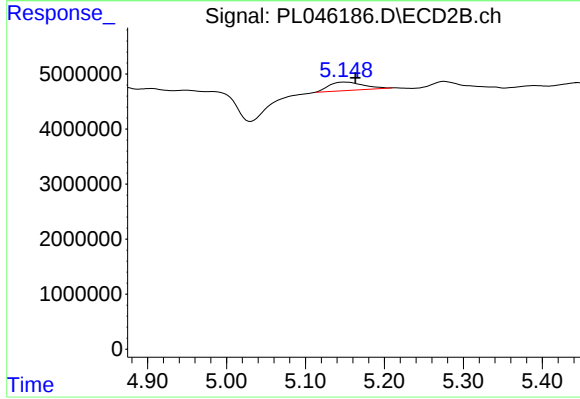

#4 Heptachlor


R.T.: 5.149 min
Delta R.T.: -0.014 min
Response: 4786137
Conc: 1.61 ng/ml

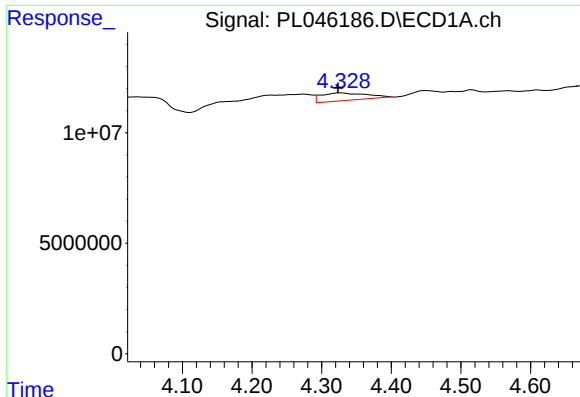

#6 beta-BHC


R.T.: 4.329 min
Delta R.T.: 0.005 min
Response: 16083773
Conc: 3.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

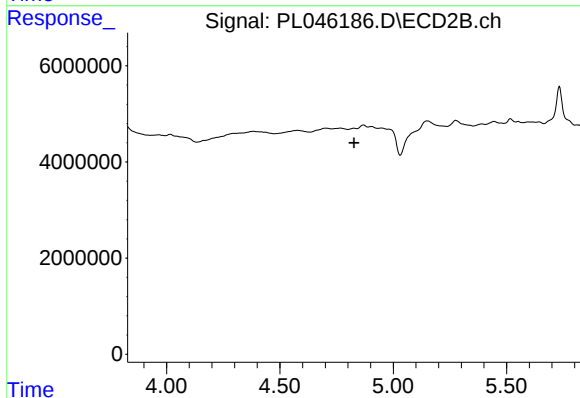


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.828 min
Response: 0
Conc: N.D.

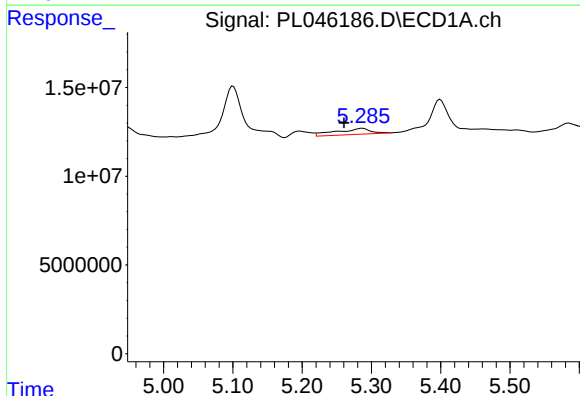


#10 gamma-Chlordane

R.T.: 5.287 min
Delta R.T.: 0.026 min
Response: 11534663
Conc: 1.18 ng/ml

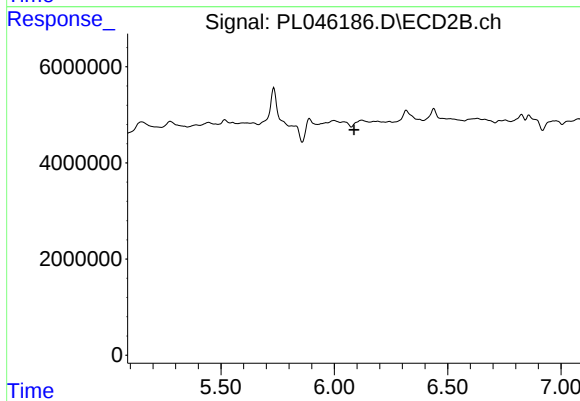

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

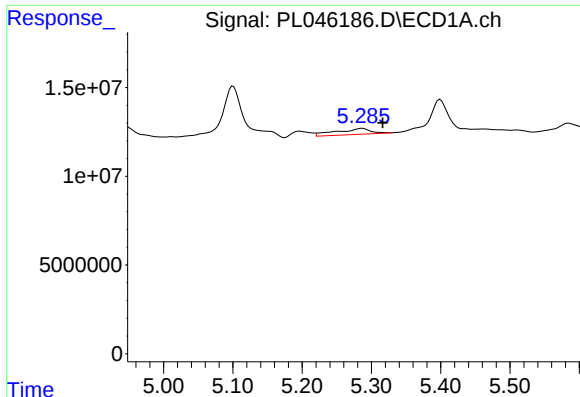

#11 alpha-Chlordane


R.T.: 5.287 min
Delta R.T.: -0.030 min
Response: 11534663
Conc: 1.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

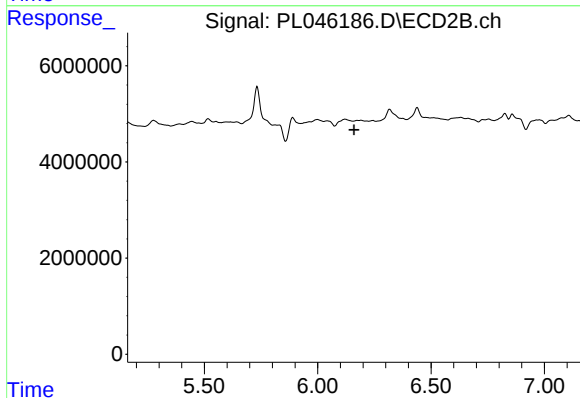


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.160 min
Response: 0
Conc: N.D.

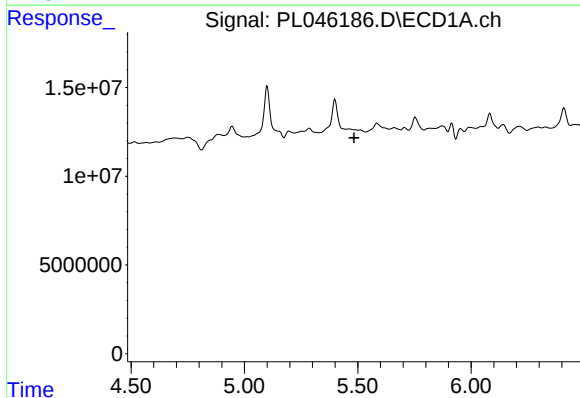


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.484 min
Response: 0
Conc: N.D.

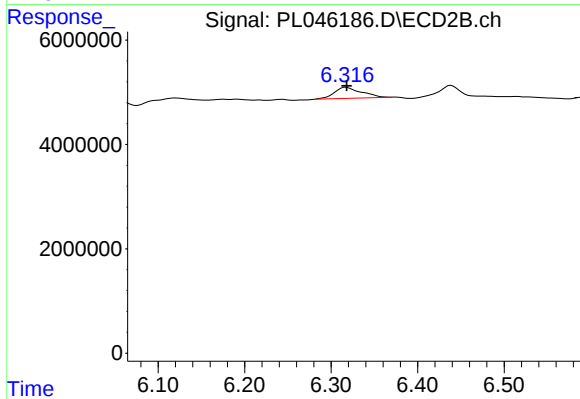

#12 4,4'-DDE


R.T.: 6.317 min
Delta R.T.: -0.001 min
Response: 4643148
Conc: 1.99 ng/ml

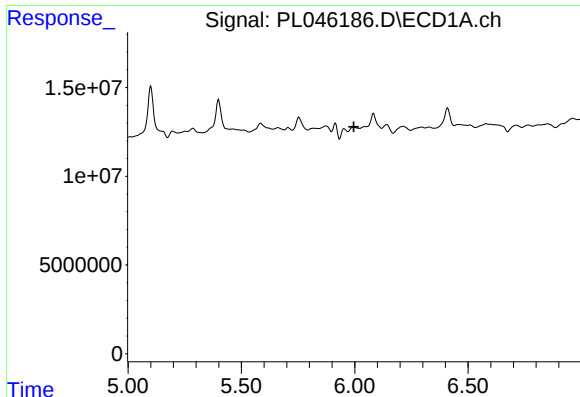

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

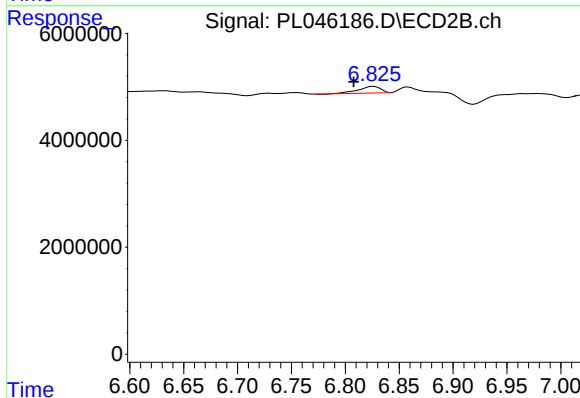


#16 4,4'-DDD

R.T.: 6.826 min
Delta R.T.: 0.019 min
Response: 1737905
Conc: 0.90 ng/ml

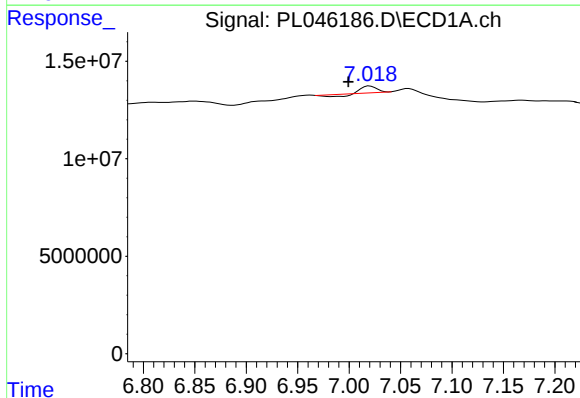


#21 Endrin ketone

R.T.: 7.020 min
Delta R.T.: 0.021 min
Response: 2344859
Conc: 0.25 ng/ml

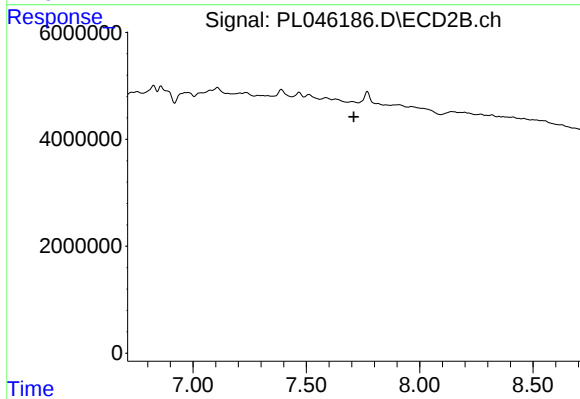

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.710 min
Response: 0
Conc: N.D.

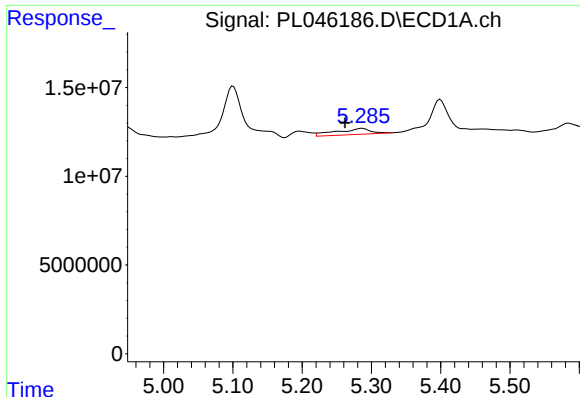

#25 Chlordane-3


R.T.: 5.287 min
Delta R.T.: 0.025 min
Response: 11534663
Conc: 10.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

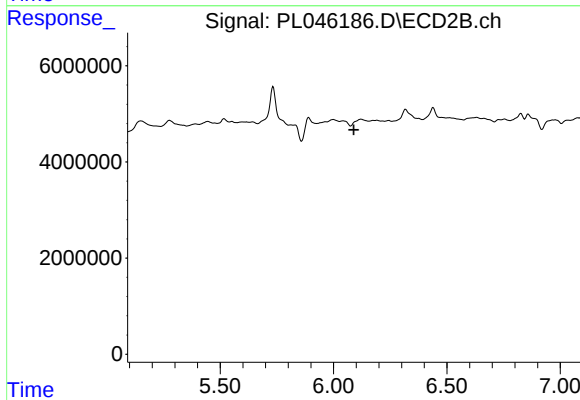


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

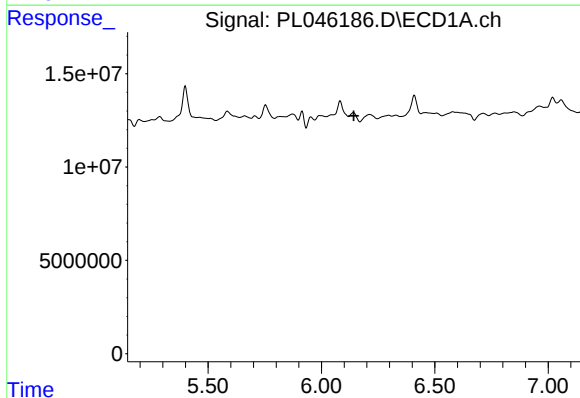


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.143 min
Response: 0
Conc: N.D.

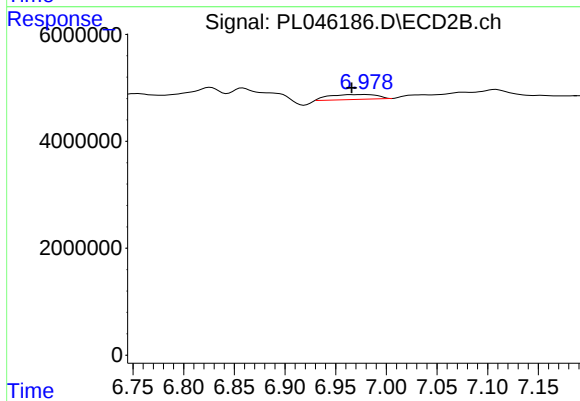

#27 Chlordane-5


R.T.: 6.979 min
Delta R.T.: 0.013 min
Response: 3079087
Conc: 33.90 ng/ml

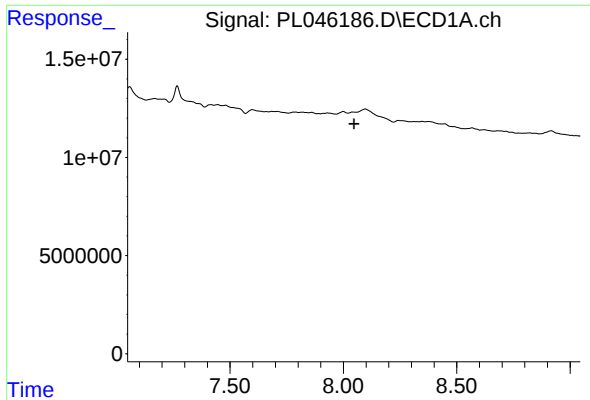

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.047 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

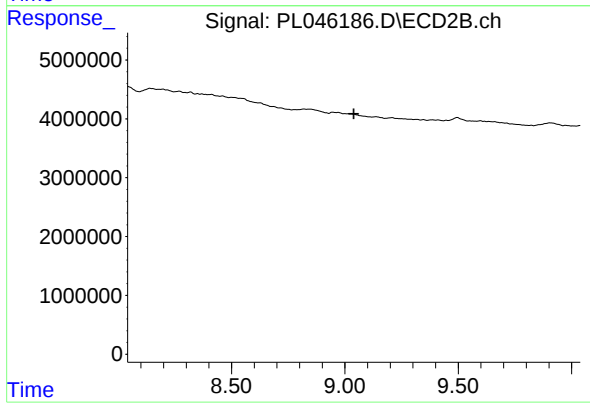

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.039 min
Response: 0
Conc: N.D.