

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032019\
 Data File : PL046196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2019 13:58
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 15:17:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.980	127.3E6	39488200	18.500	18.439
28)	SA Decachlor...	8.039	9.033	133.2E6	38630028	15.914	16.906
Target Compounds							
6)	B beta-BHC	4.326	0.000	2171381	0	0.507	N.D. #
9)	A Endosulfan I	5.398f	0.000	12295377	0	1.376	N.D. #
16)	A 4,4'-DDD	0.000	6.828f	0	3600373	N.D.	1.872 #
23)	Chlordane-1	4.239f	0.000	23543297	0	69.874	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032019\
Data File : PL046196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2019 13:58
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 15:17:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

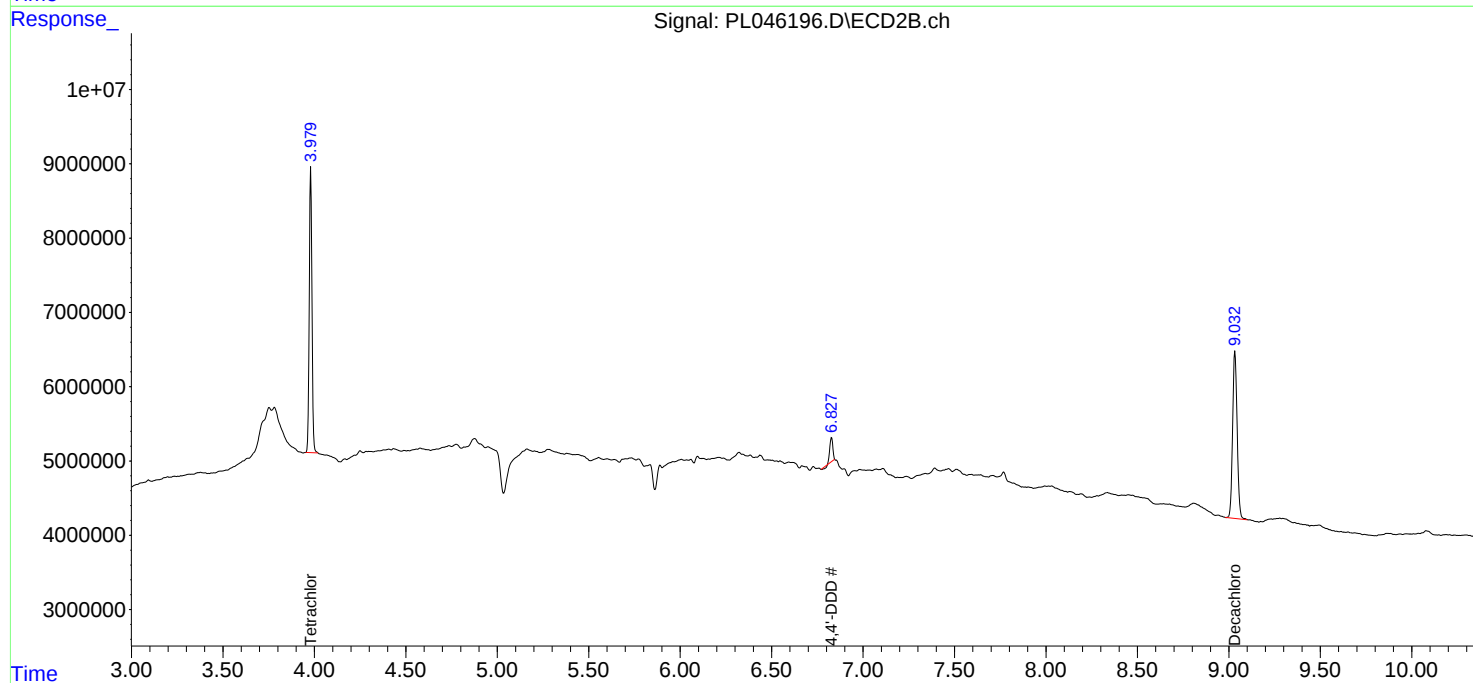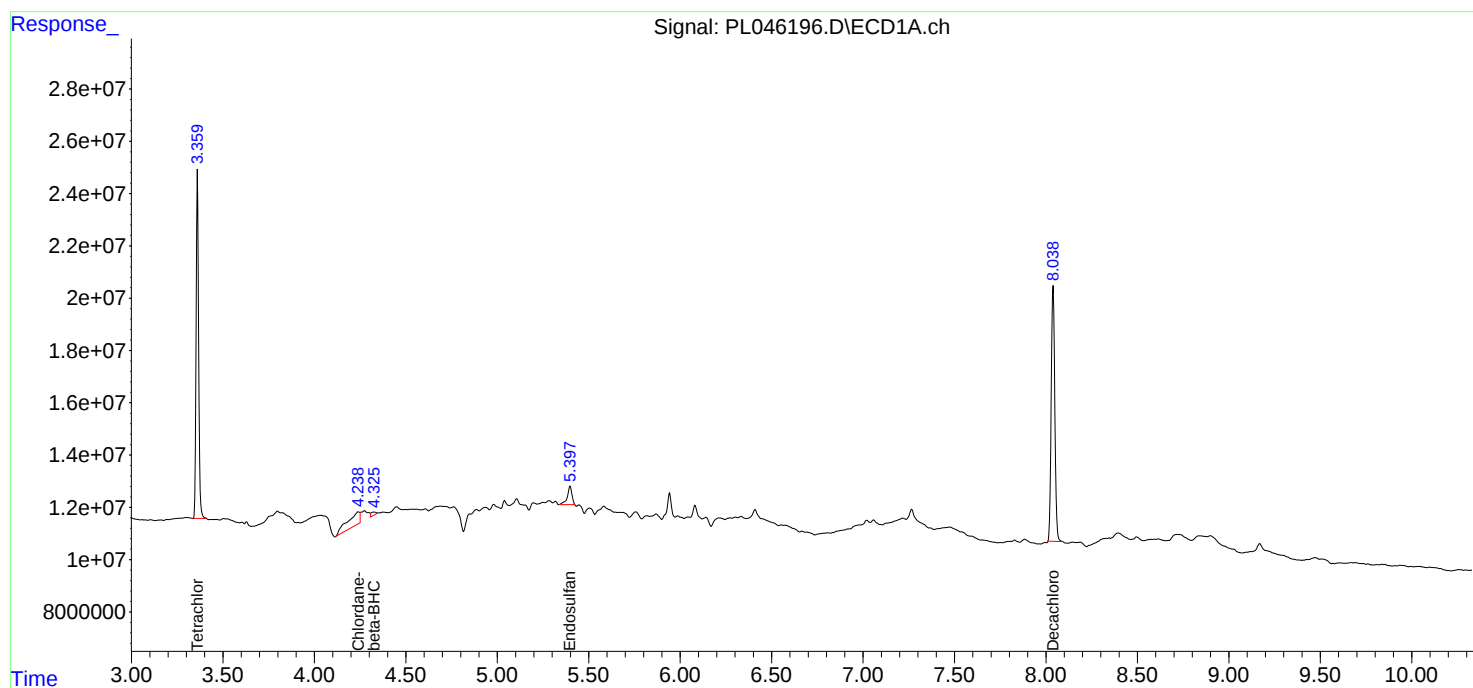


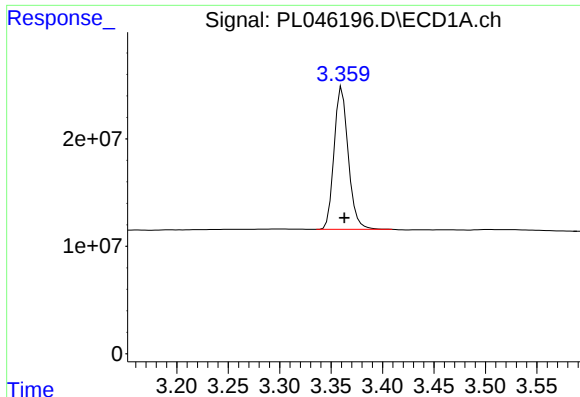

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: -0.002 min
Response: 127266823
Conc: 18.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

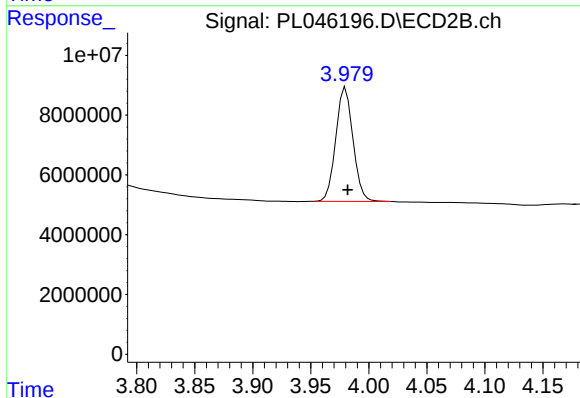


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 39488200
Conc: 18.44 ng/ml

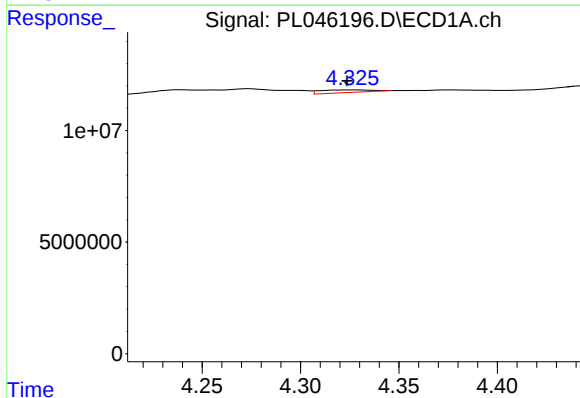


#6 beta-BHC

R.T.: 4.326 min
Delta R.T.: 0.003 min
Response: 2171381
Conc: 0.51 ng/ml

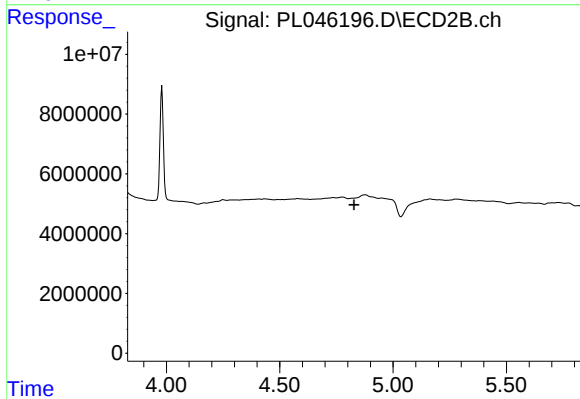

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.828 min
Response: 0
Conc: N.D.

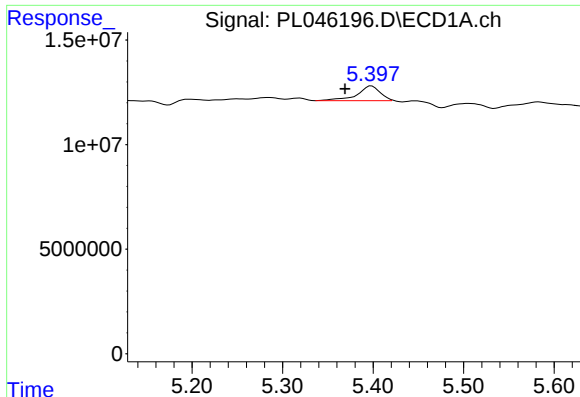

#9 Endosulfan I


R.T.: 5.398 min
Delta R.T.: 0.029 min
Response: 12295377
Conc: 1.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

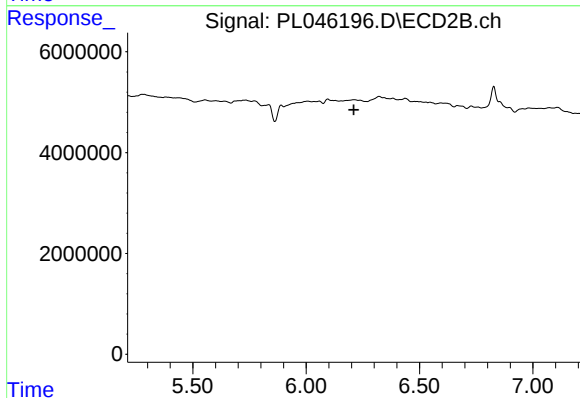


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.210 min
Response: 0
Conc: N.D.

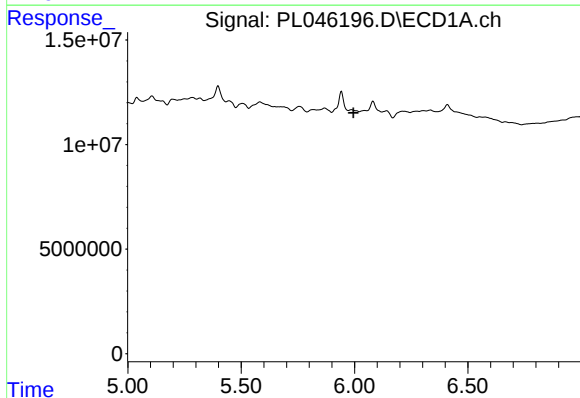


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

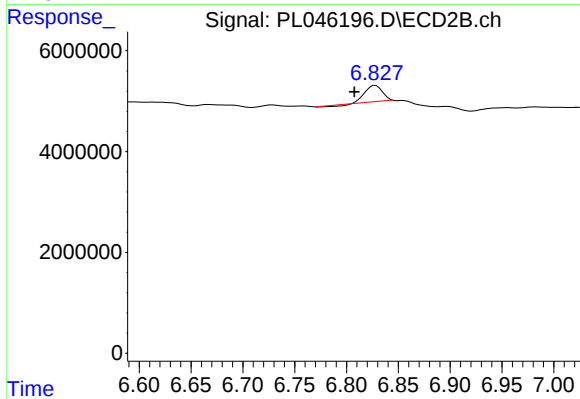

#16 4,4'-DDD


R.T.: 6.828 min
Delta R.T.: 0.020 min
Response: 3600373
Conc: 1.87 ng/ml

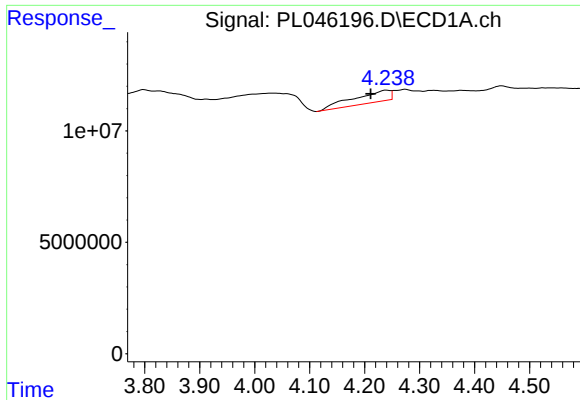

#23 Chlordane-1


R.T.: 4.239 min
Delta R.T.: 0.028 min
Response: 23543297
Conc: 69.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

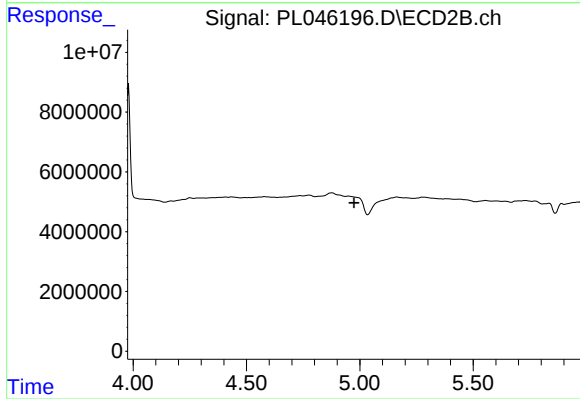


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.975 min
Response: 0
Conc: N.D.

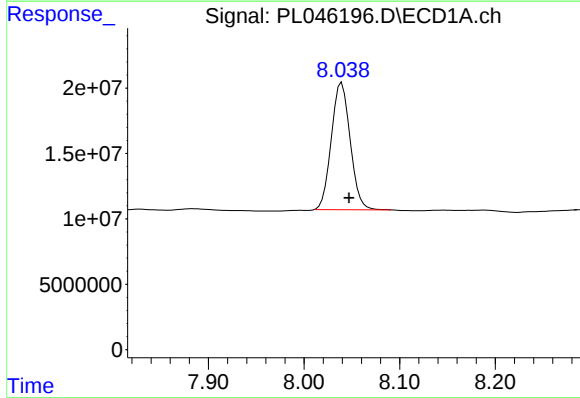

#28 Decachlorobiphenyl

R.T.: 8.039 min
Delta R.T.: -0.008 min
Response: 133155577
Conc: 15.91 ng/ml

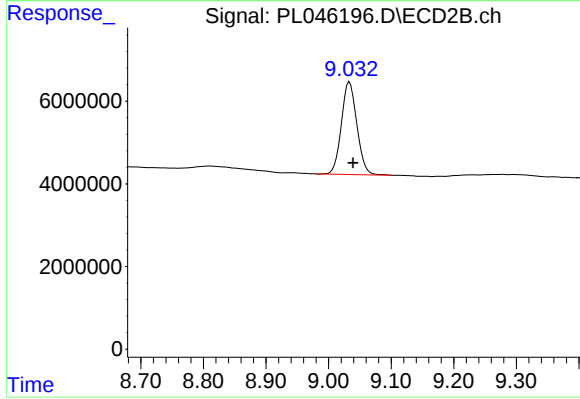

#28 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: -0.005 min
Response: 38630028
Conc: 16.91 ng/ml