

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032019\
 Data File : PL046246.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2019 04:20
 Operator : AJ\SJ
 Sample : K1688-21
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 08:38:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.980	60235557	18601465	8.756	8.686
28)	SA Decachlor...	8.039	9.034	74998486	22824526	8.963	9.989
Target Compounds							
10)	B gamma-Chl...	5.274	0.000	7041215	0	0.719	N.D. #
11)	B alpha-Chl...	0.000	6.158	0	3398983	N.D.	1.260 #
12)	B 4,4'-DDE	0.000	6.315	0	1877234	N.D.	0.804 #
25)	Chlordane-3	5.274	0.000	7041215	0	6.139	N.D. #
26)	Chlordane-4	0.000	6.158	0	3398983	N.D.	7.265 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032019\
Data File : PL046246.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2019 04:20
Operator : AJ\SJ
Sample : K1688-21
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 08:38:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

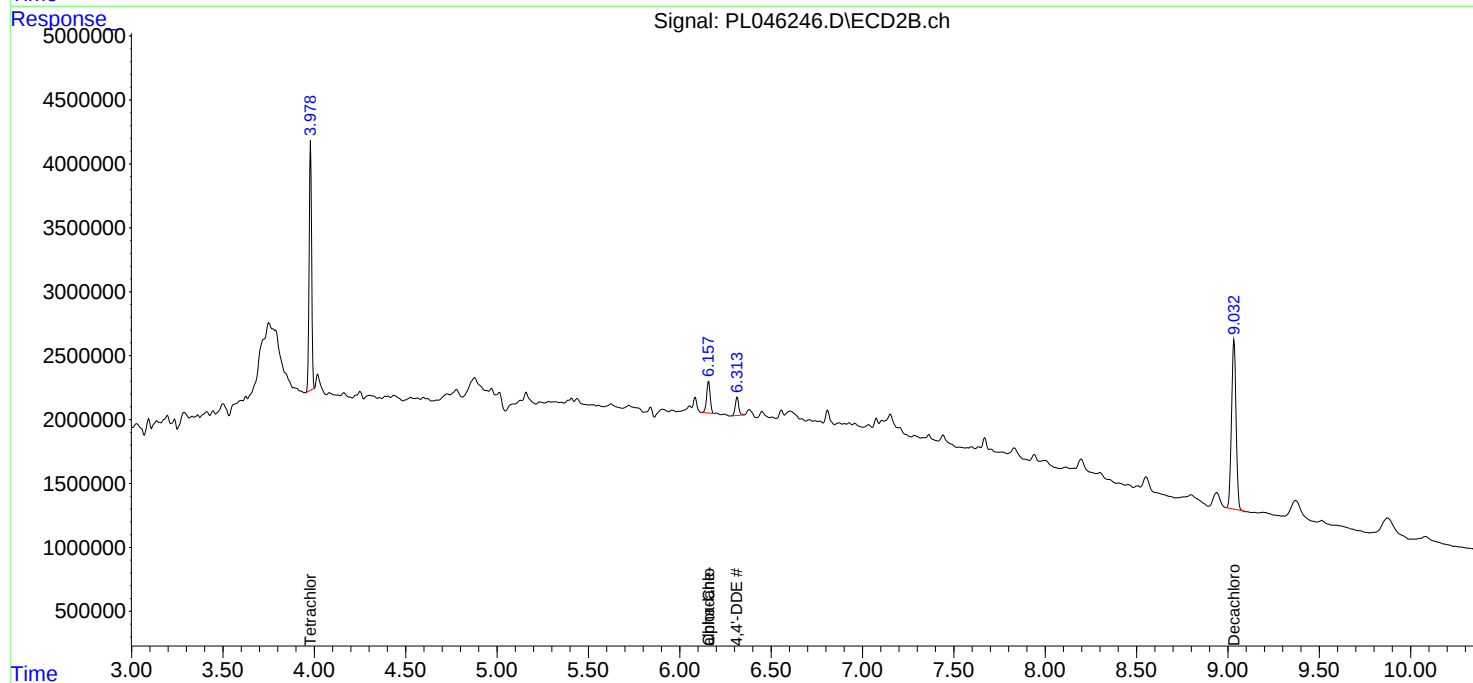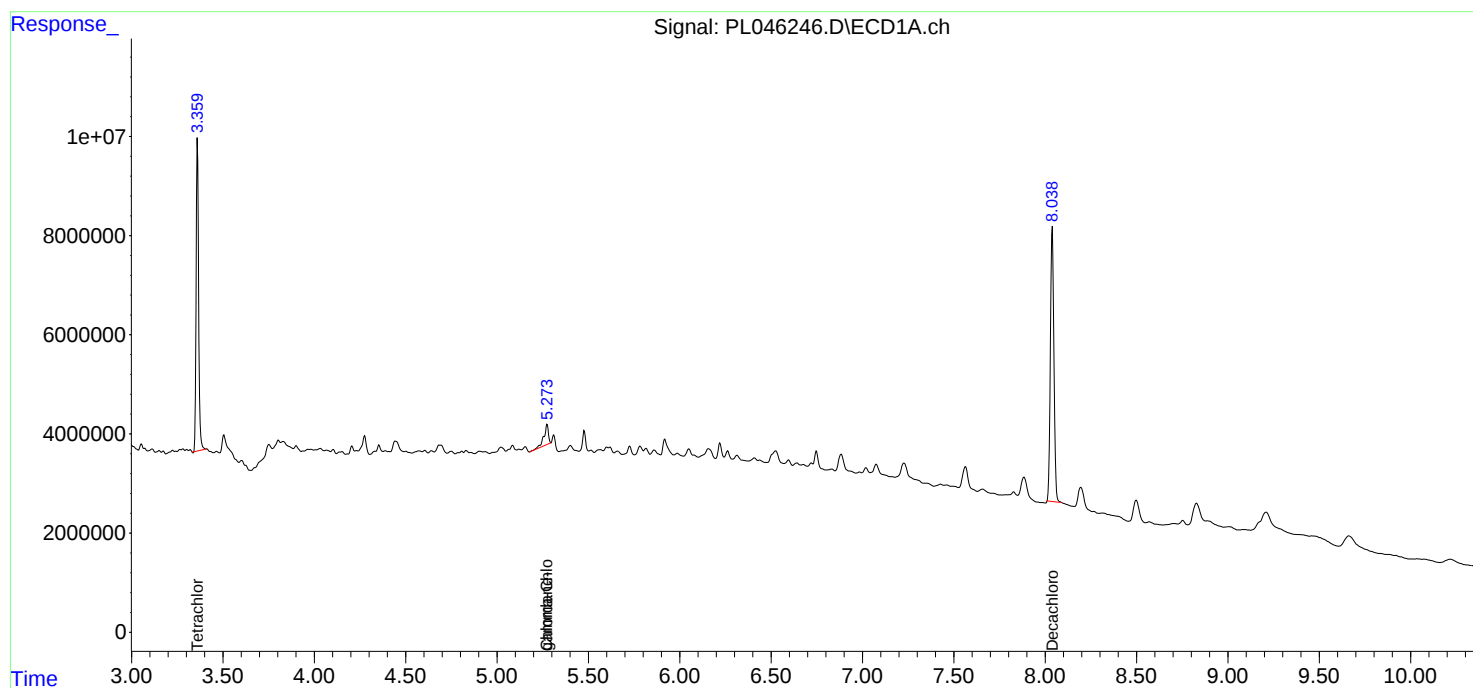


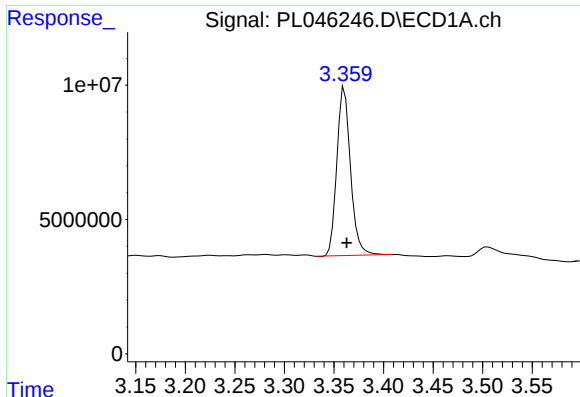

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: -0.002 min
Response: 60235557
Conc: 8.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

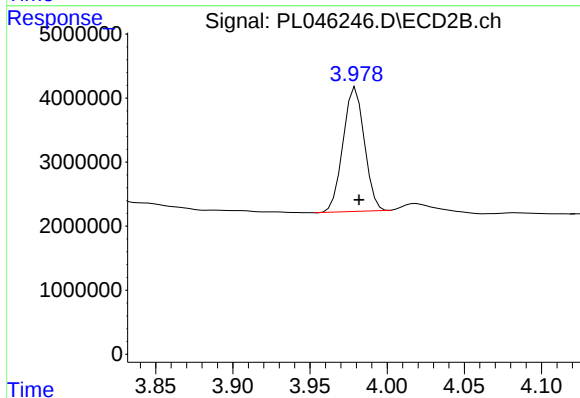


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 18601465
Conc: 8.69 ng/ml

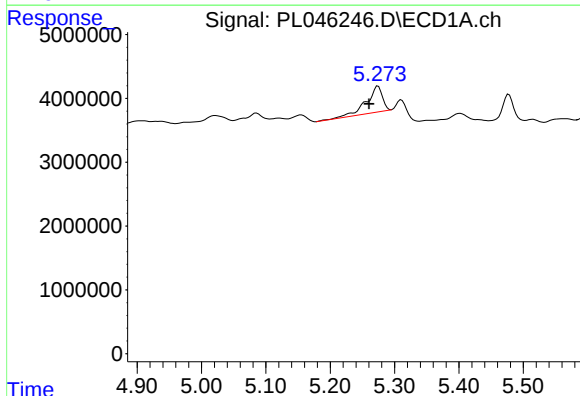


#10 gamma-Chlordane

R.T.: 5.274 min
Delta R.T.: 0.014 min
Response: 7041215
Conc: 0.72 ng/ml

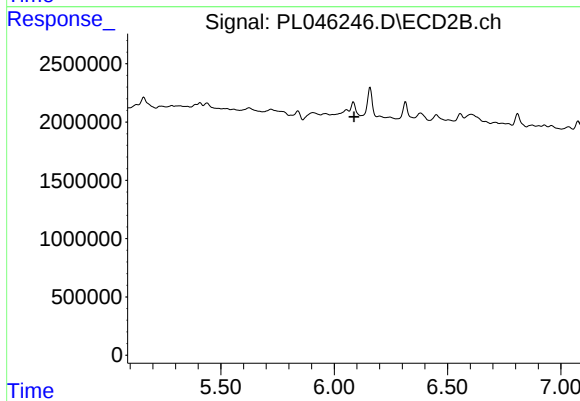

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.088 min
Response: 0
Conc: N.D.

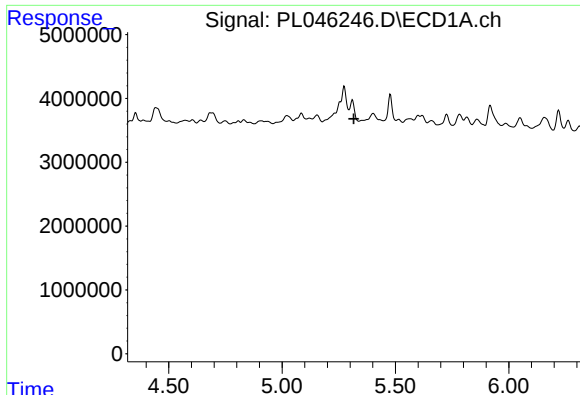

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

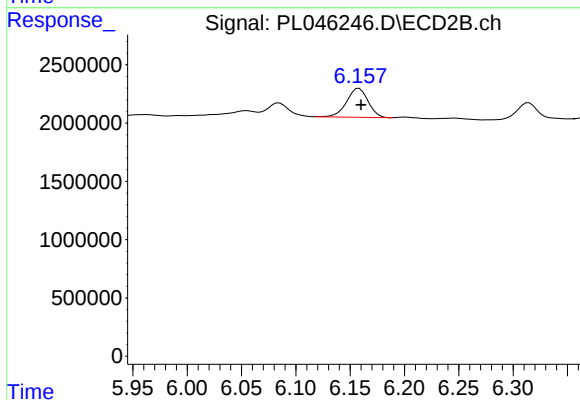


#11 alpha-Chlordane

R.T.: 6.158 min
Delta R.T.: -0.002 min
Response: 3398983
Conc: 1.26 ng/ml

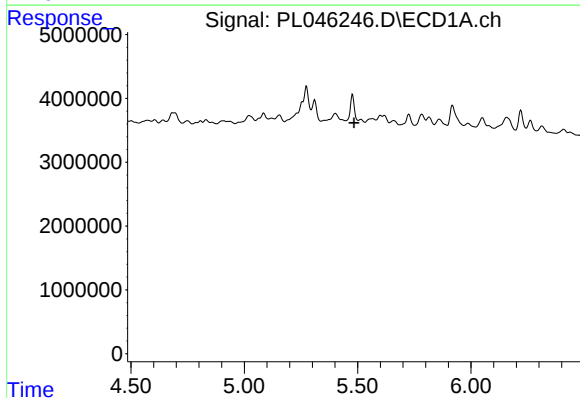


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.484 min
Response: 0
Conc: N.D.

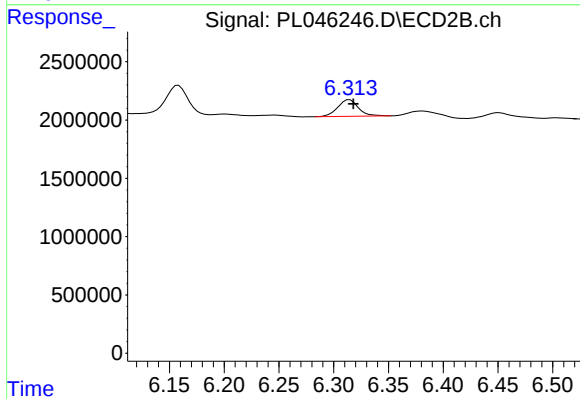

#12 4,4'-DDE


R.T.: 6.315 min
Delta R.T.: -0.004 min
Response: 1877234
Conc: 0.80 ng/ml

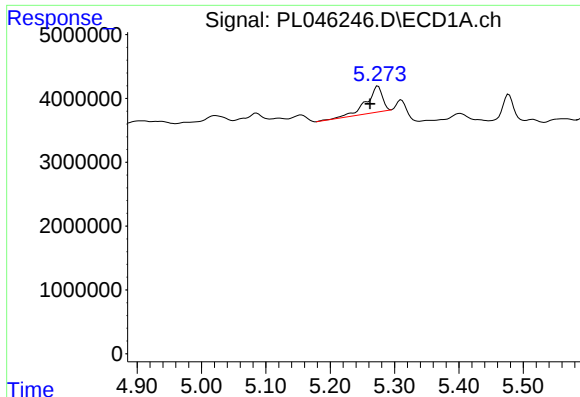

#25 Chlordane-3


R.T.: 5.274 min
Delta R.T.: 0.013 min
Response: 7041215
Conc: 6.14 ng/ml

Instrument :
ECD_L
ClientSampleId :

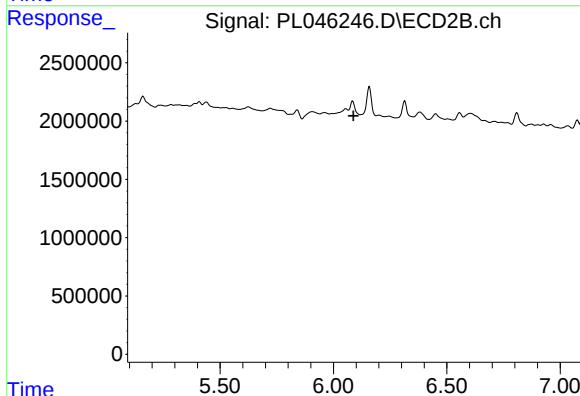


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

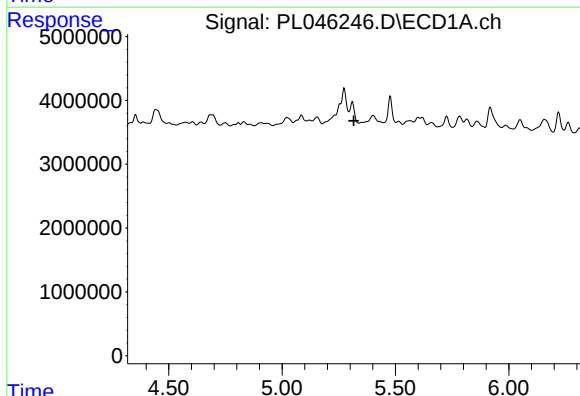


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.317 min
Response: 0
Conc: N.D.

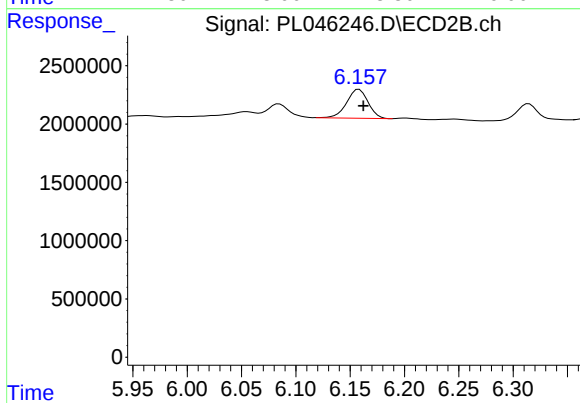

#26 Chlordane-4


R.T.: 6.158 min
Delta R.T.: -0.004 min
Response: 3398983
Conc: 7.27 ng/ml

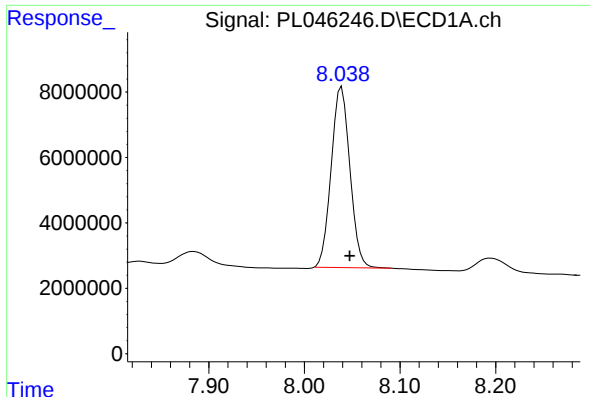

#28 Decachlorobiphenyl

R.T.: 8.039 min
Delta R.T.: -0.008 min
Response: 74998486
Conc: 8.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

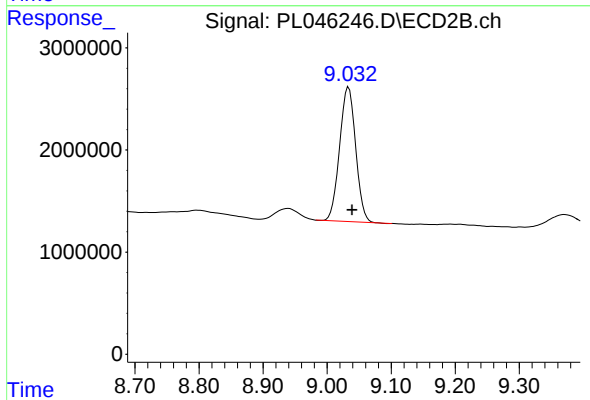

#28 Decachlorobiphenyl

R.T.: 9.034 min
Delta R.T.: -0.005 min
Response: 22824526
Conc: 9.99 ng/ml