

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032019\
 Data File : PL046251.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2019 05:32
 Operator : AJ\SJ
 Sample : K1688-37
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JC-02-031919-I

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 08:39:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.980	60603774	21223707	8.810	9.911
28)	SA Decachlor...	8.039	9.033	78603886	24525511	9.394	10.734
Target Compounds							
10)	B gamma-Chl...	5.275	0.000	6119245	0	0.625	N.D. #
11)	B alpha-Chl...	0.000	6.158	0	3171092	N.D.	1.175 #
12)	B 4,4'-DDE	0.000	6.314	0	1559316	N.D.	0.668 #
16)	A 4,4'-DDD	0.000	6.810	0	2242967	N.D.	1.166 #
17)	MA 4,4'-DDT	6.220	0.000	6226613	0	0.830	N.D. #
25)	Chlordane-3	5.275	0.000	6119245	0	5.335	N.D. #
26)	Chlordane-4	0.000	6.158	0	3171092	N.D.	6.778 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032019\
Data File : PL046251.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2019 05:32
Operator : AJ\SJ
Sample : K1688-37
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
JC-02-031919-I

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 08:39:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

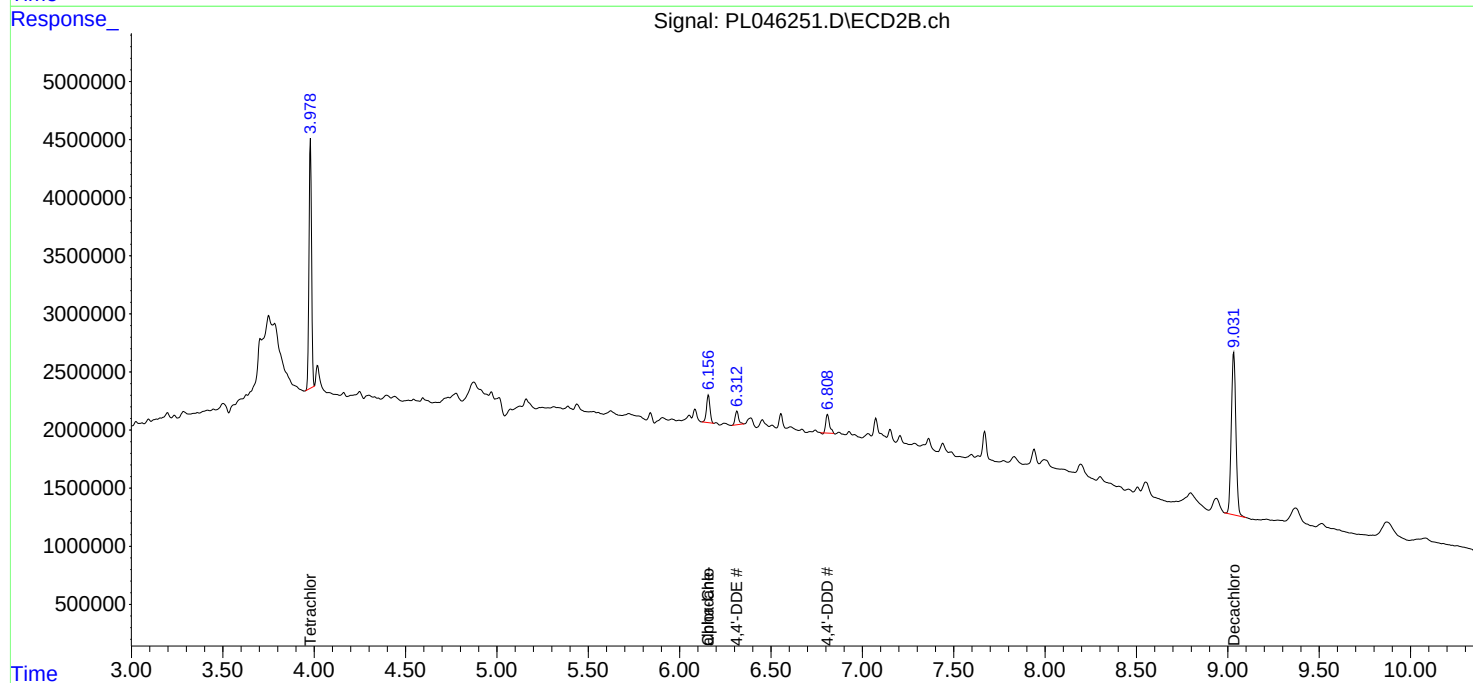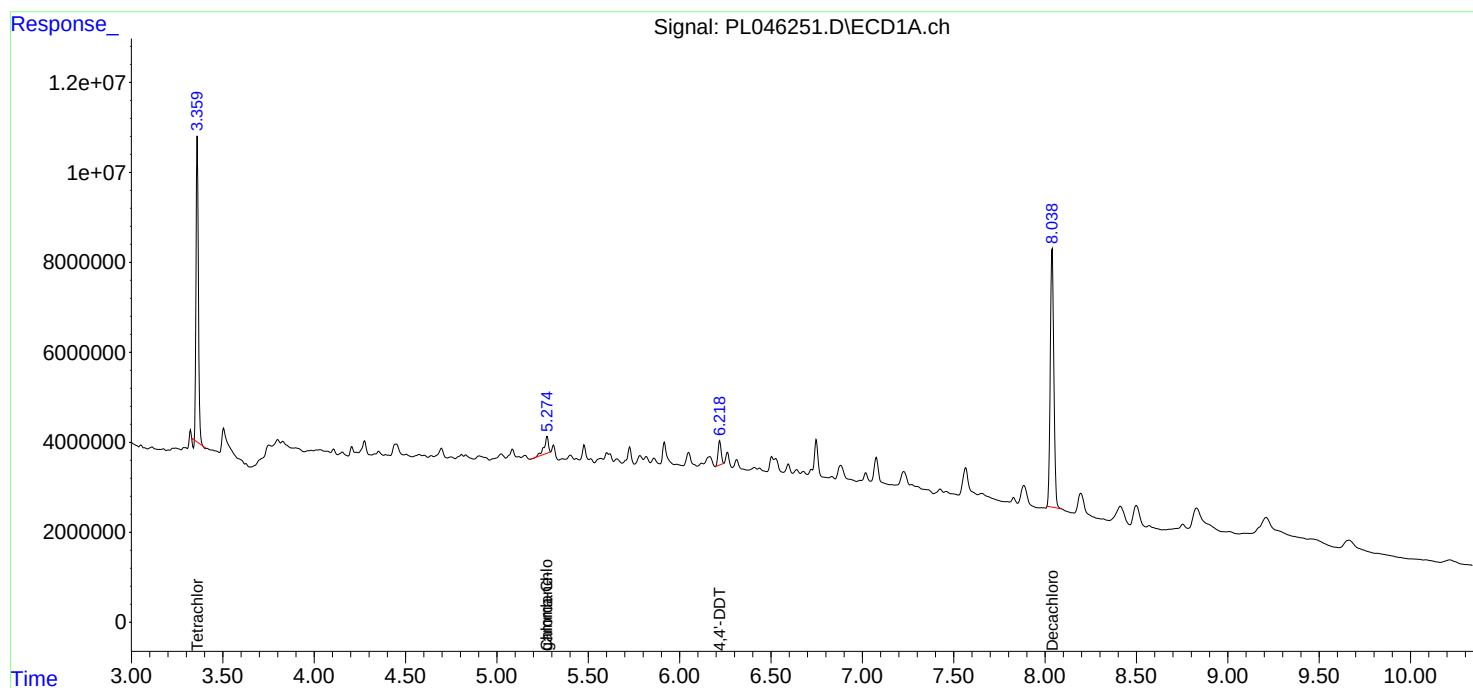


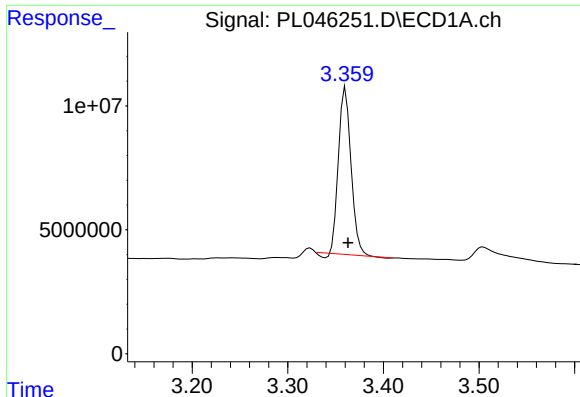

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: -0.002 min
Response: 60603774
Conc: 8.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-02-031919-I

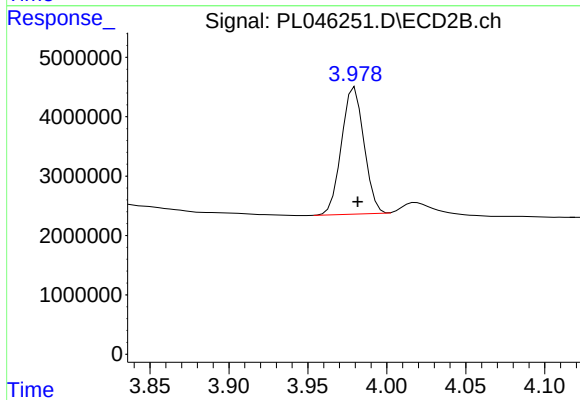


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 21223707
Conc: 9.91 ng/ml

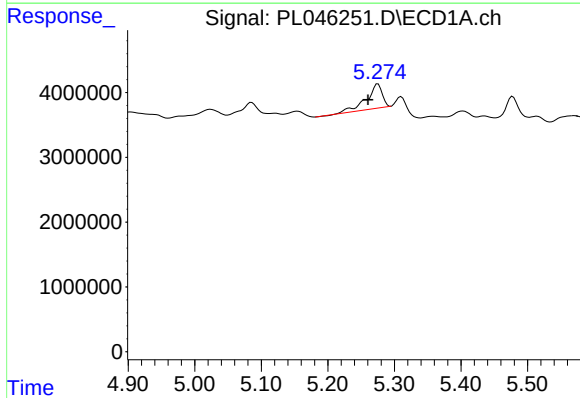


#10 gamma-Chlordane

R.T.: 5.275 min
Delta R.T.: 0.015 min
Response: 6119245
Conc: 0.63 ng/ml

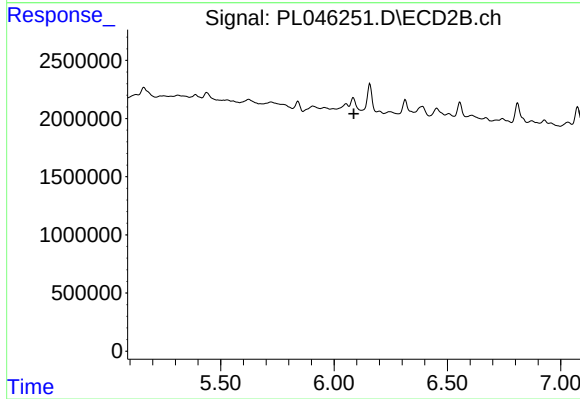

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.088 min
Response: 0
Conc: N.D.

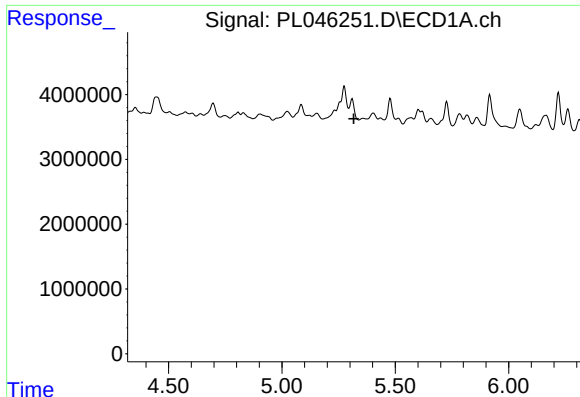

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JC-02-031919-I

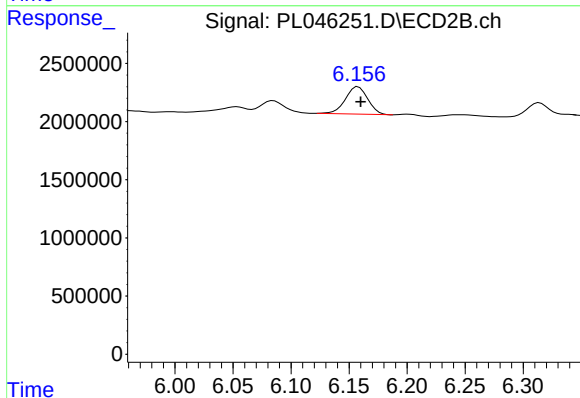


#11 alpha-Chlordane

R.T.: 6.158 min
Delta R.T.: -0.002 min
Response: 3171092
Conc: 1.18 ng/ml

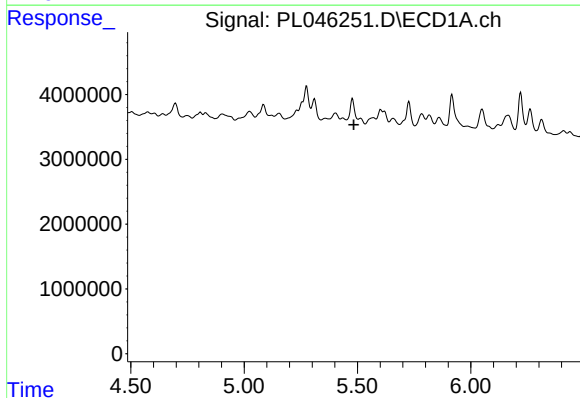


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 5.484 min
Response: 0
Conc: N.D.

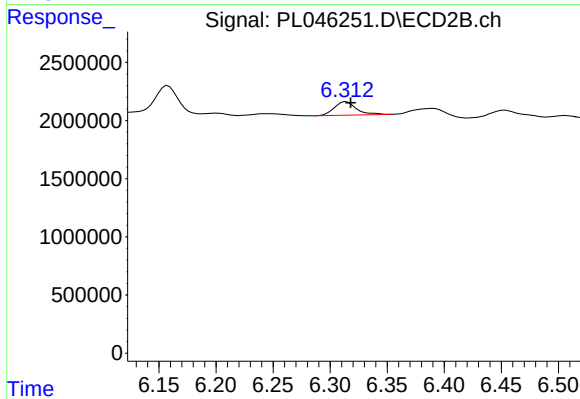

#12 4,4'-DDE


R.T.: 6.314 min
Delta R.T.: -0.004 min
Response: 1559316
Conc: 0.67 ng/ml

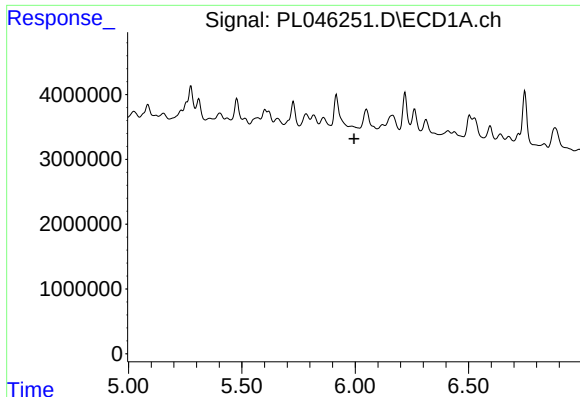

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JC-02-031919-I

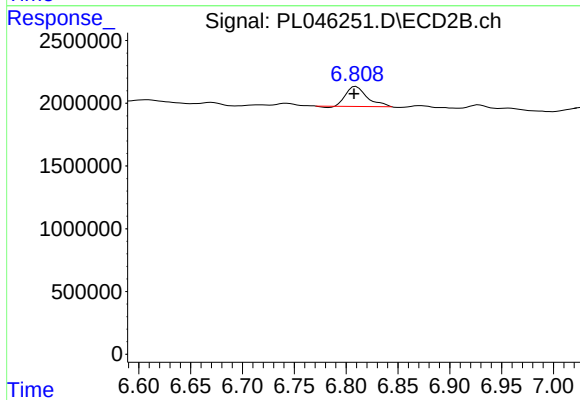


#16 4,4'-DDD

R.T.: 6.810 min
Delta R.T.: 0.002 min
Response: 2242967
Conc: 1.17 ng/ml

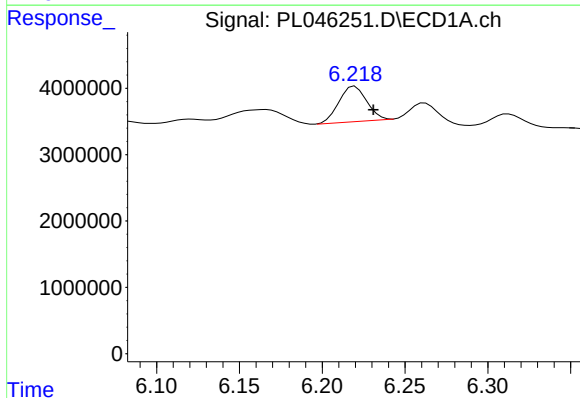


#17 4,4'-DDT

R.T.: 6.220 min
Delta R.T.: -0.011 min
Response: 6226613
Conc: 0.83 ng/ml

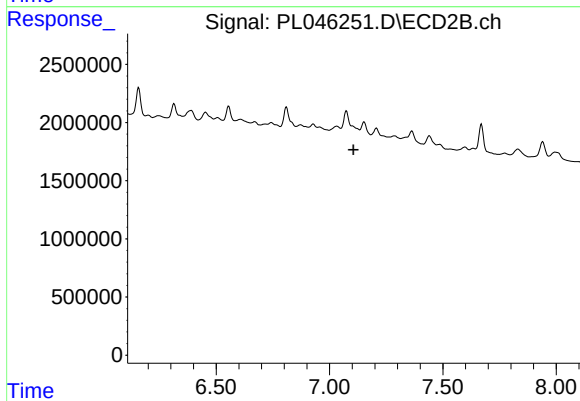

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.106 min
Response: 0
Conc: N.D.

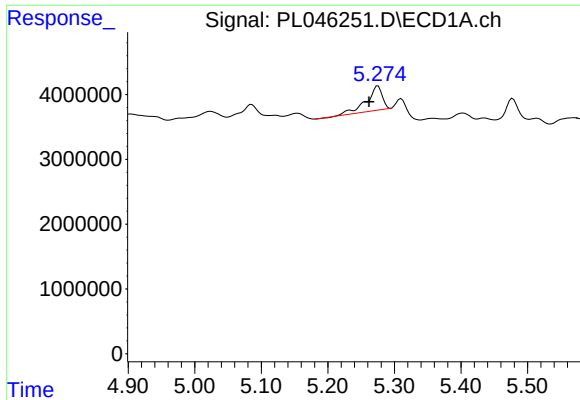

#25 Chlordane-3


R.T.: 5.275 min
Delta R.T.: 0.013 min
Response: 6119245
Conc: 5.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-02-031919-I

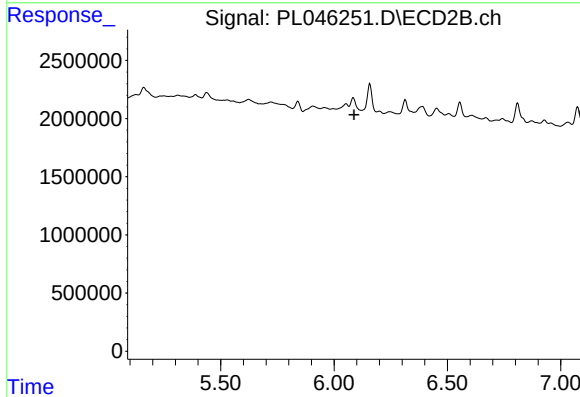


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

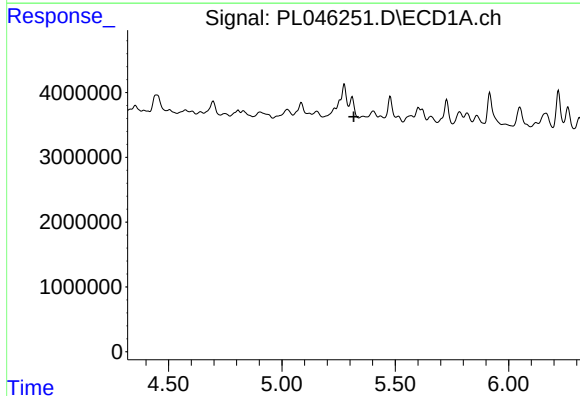


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.317 min
Response: 0
Conc: N.D.

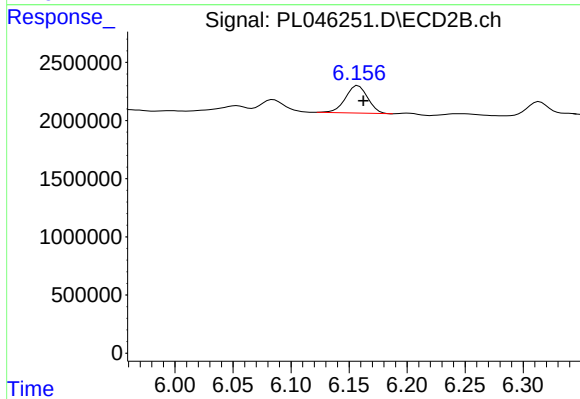

#26 Chlordane-4


R.T.: 6.158 min
Delta R.T.: -0.004 min
Response: 3171092
Conc: 6.78 ng/ml

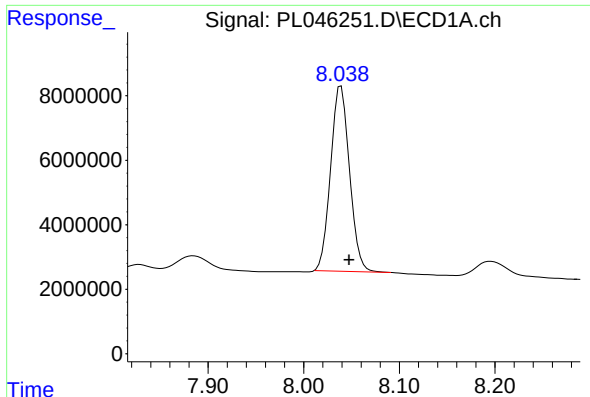

#28 Decachlorobiphenyl

R.T.: 8.039 min
Delta R.T.: -0.008 min
Response: 78603886
Conc: 9.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-02-031919-I

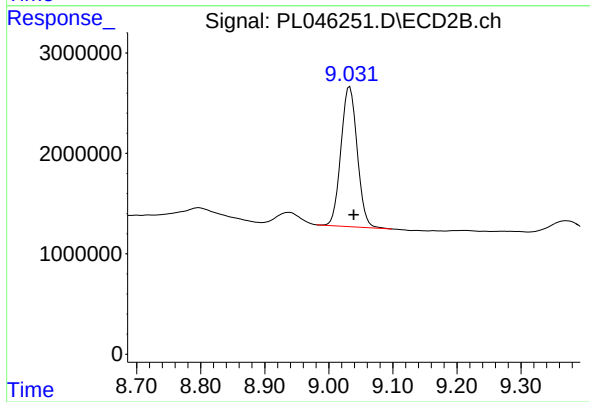

#28 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: -0.006 min
Response: 24525511
Conc: 10.73 ng/ml