

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032019\
 Data File : PL046193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Mar 2019 11:46
 Operator : AJ\SJ
 Sample : K1971-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-15(6-7)-031519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 20 13:07:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.360	3.979	59515753	19299521	8.651	9.012
28)	SA Decachlor...	8.040	9.033	68020290	23981950	8.129	10.496 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032019\
Data File : PL046193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Mar 2019 11:46
Operator : AJ\SJ
Sample : K1971-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SB-15(6-7)-031519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 20 13:07:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

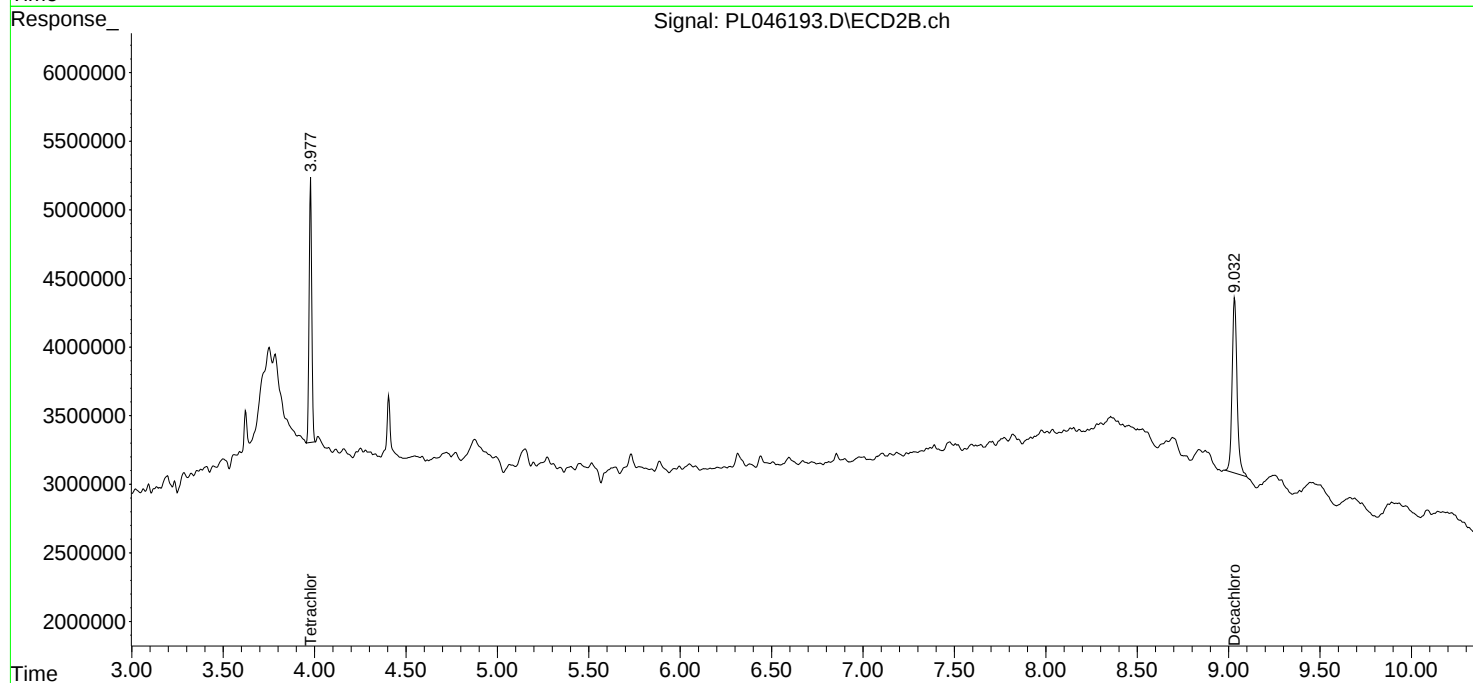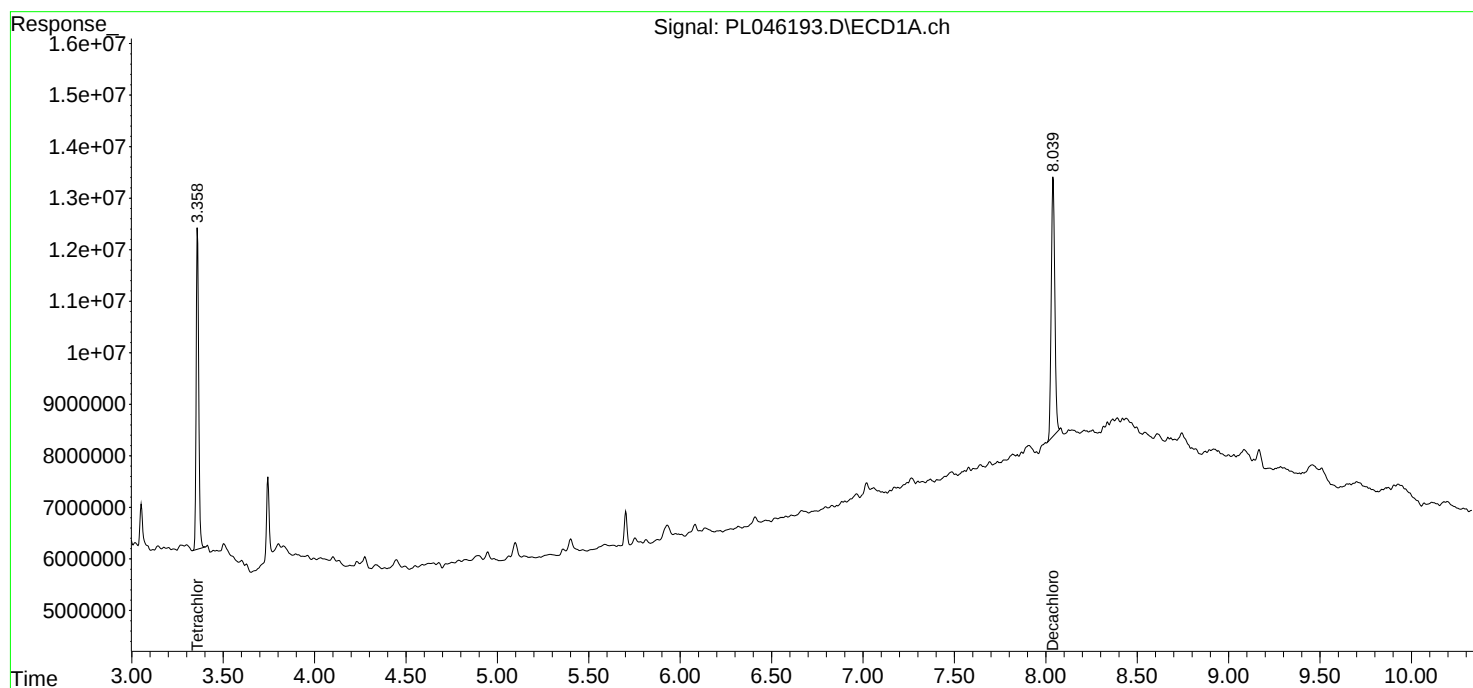


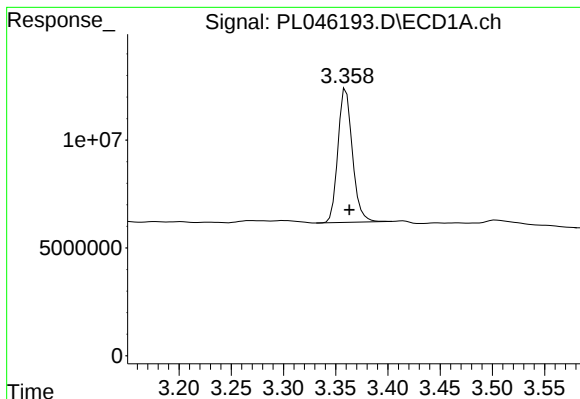

#1 Tetrachloro-m-xylene


R.T.: 3.360 min
Delta R.T.: -0.003 min
Response: 59515753
Conc: 8.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-15(6-7)-031519

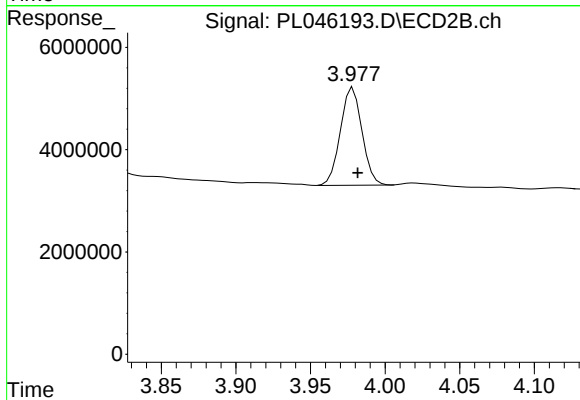


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.003 min
Response: 19299521
Conc: 9.01 ng/ml

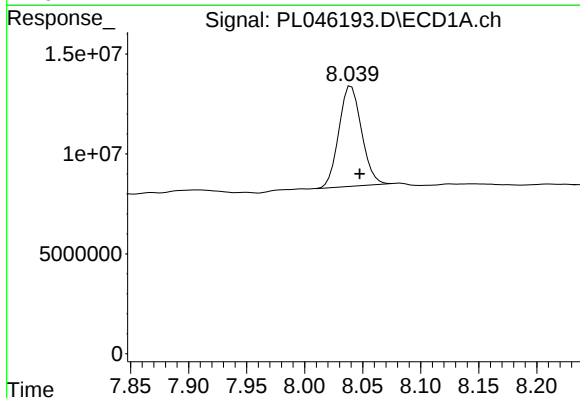

#28 Decachlorobiphenyl

R.T.: 8.040 min
Delta R.T.: -0.007 min
Response: 68020290
Conc: 8.13 ng/ml

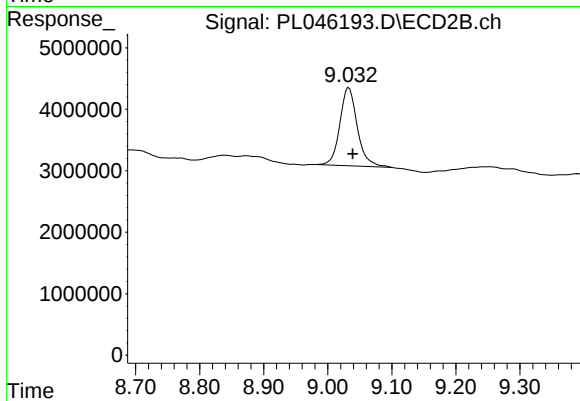

#28 Decachlorobiphenyl

R.T.: 9.033 min
Delta R.T.: -0.006 min
Response: 23981950
Conc: 10.50 ng/ml