

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032119\
 Data File : PL046272.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2019 14:28
 Operator : AJ\SJ
 Sample : K1694-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-02-032019-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 01:03:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.980	70720379	22480388	10.280	10.497
28)	SA Decachlor...	8.041	9.037	69703595	22041041	8.330	9.646
Target Compounds							
5)	MB Aldrin	0.000	5.438f	0	3683590	N.D.	1.364 #
10)	B gamma-Chl...	5.275	6.086	5673429	472495	0.580	0.176 #
11)	B alpha-Chl...	0.000	6.160	0	3167340	N.D.	1.174 #
12)	B 4,4'-DDE	5.479	6.314	9766051	4262336	1.113	1.825 #
16)	A 4,4'-DDD	0.000	6.807	0	1513994	N.D.	0.787 #
24)	Chlordane-2	0.000	5.438	0	3683590	N.D.	30.486 #
25)	Chlordane-3	5.275	6.086	5673429	472495	4.946	1.213 #
26)	Chlordane-4	0.000	6.160	0	3167340	N.D.	6.770 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032119\
Data File : PL046272.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2019 14:28
Operator : AJ\SJ
Sample : K1694-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EO-02-032019-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 01:03:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

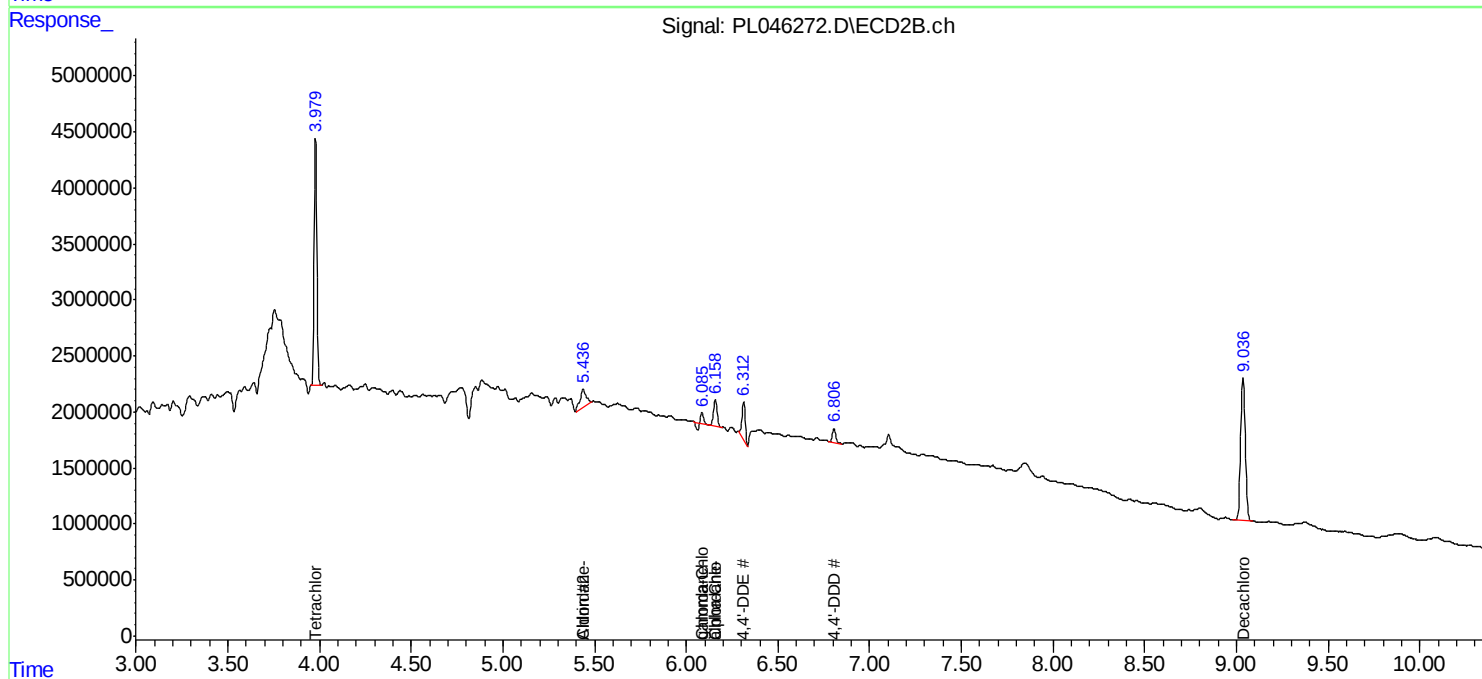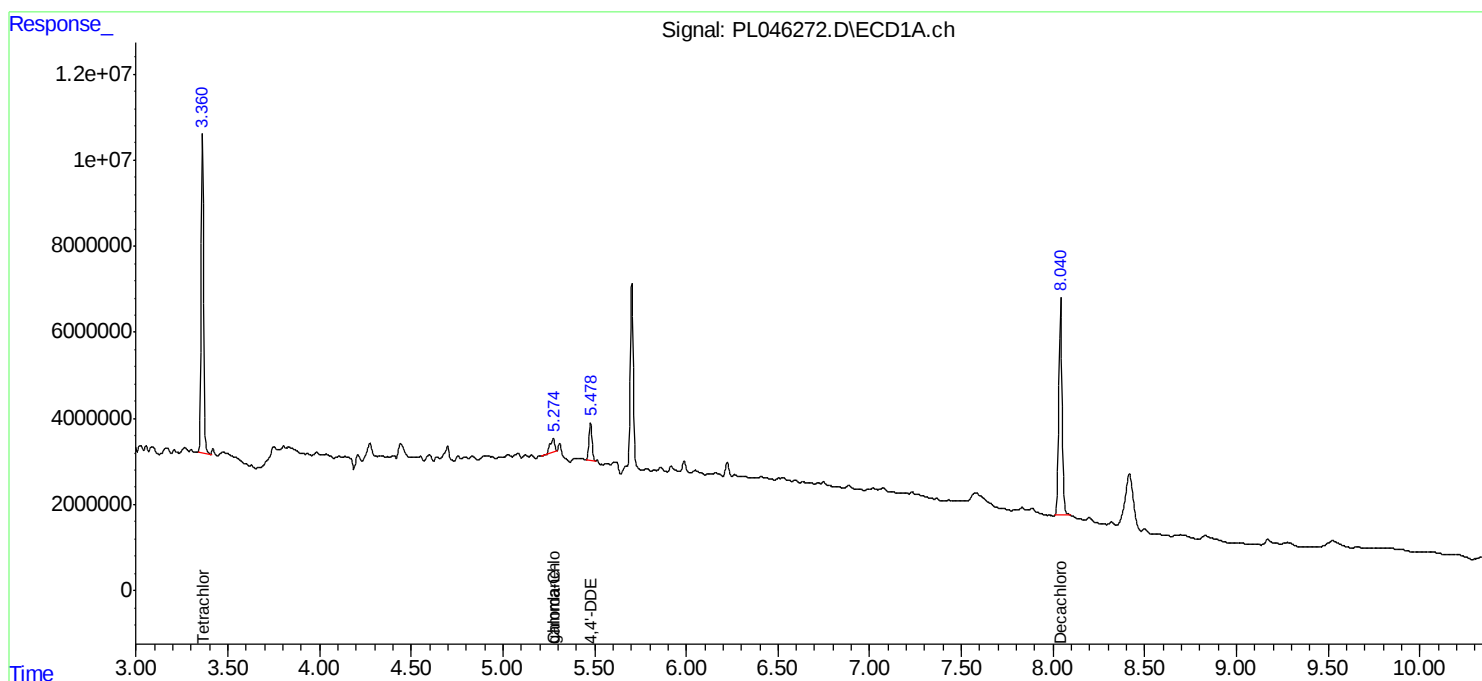


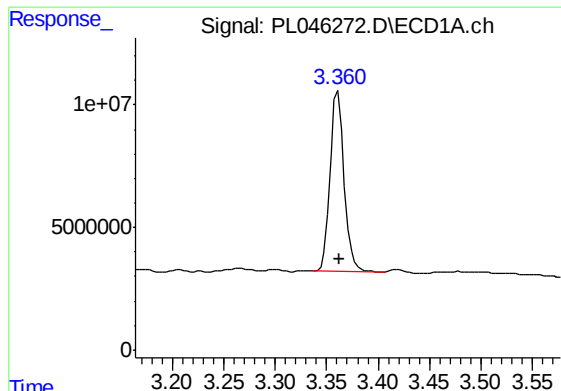

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: -0.002 min
Response: 70720379
Conc: 10.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-032019-B

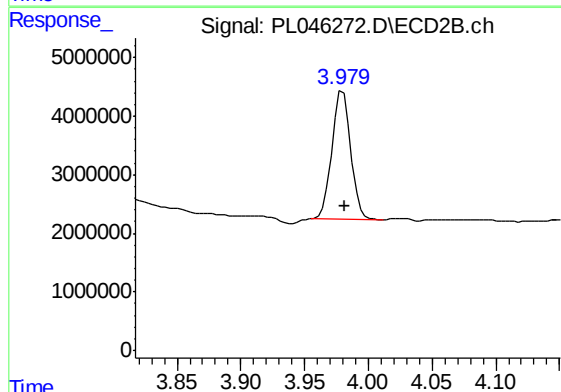


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 22480388
Conc: 10.50 ng/ml

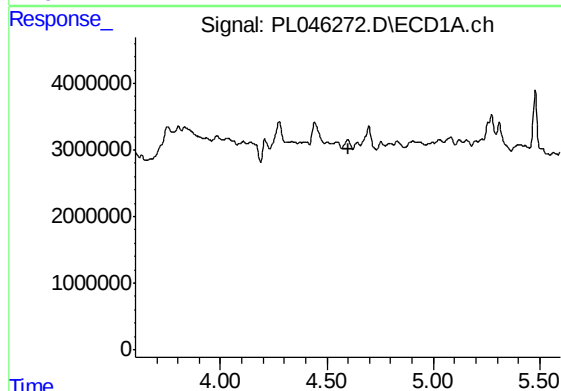


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.599 min
Response: 0
Conc: N.D.

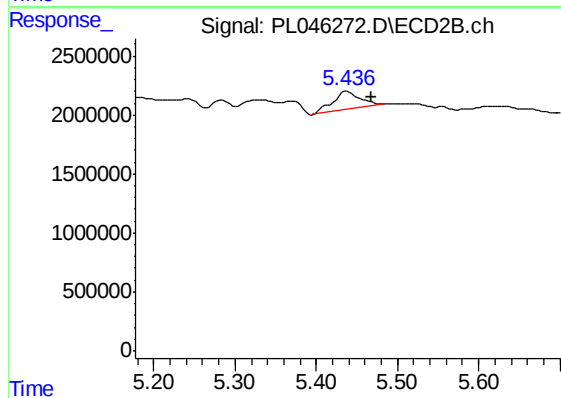

#5 Aldrin


R.T.: 5.438 min
Delta R.T.: -0.030 min
Response: 3683590
Conc: 1.36 ng/ml

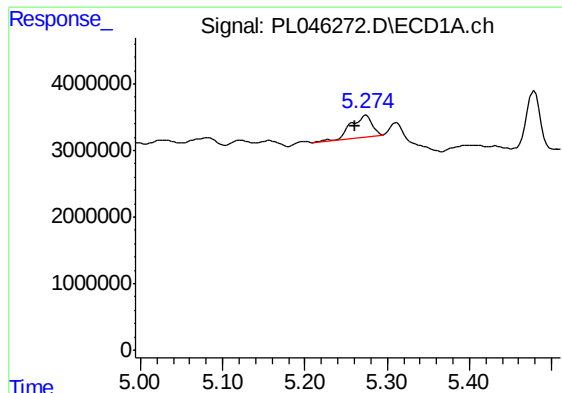

#10 gamma-Chlordane


R.T.: 5.275 min
Delta R.T.: 0.014 min
Response: 5673429
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-032019-B

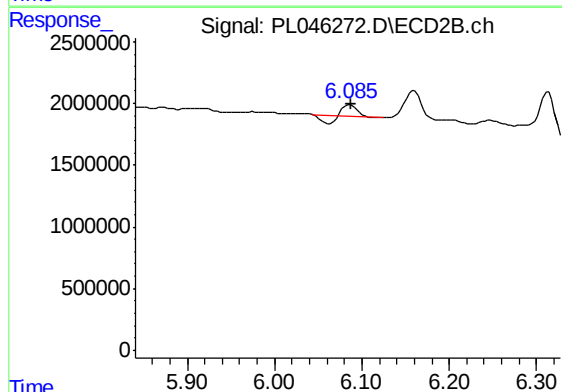


#10 gamma-Chlordane

R.T.: 6.086 min
Delta R.T.: -0.002 min
Response: 472495
Conc: 0.18 ng/ml

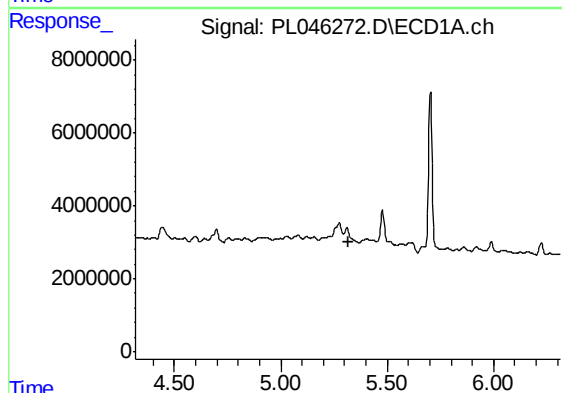


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.317 min
Response: 0
Conc: N.D.

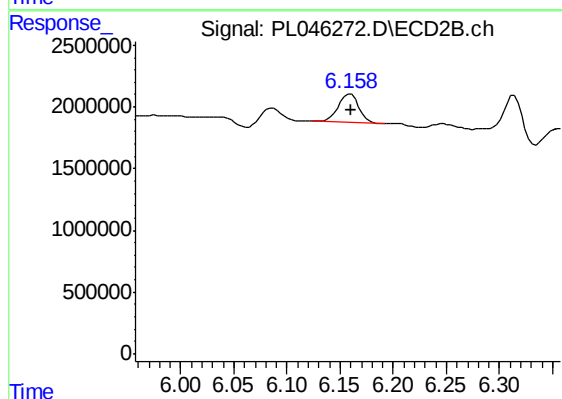

#11 alpha-Chlordane


R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 3167340
Conc: 1.17 ng/ml

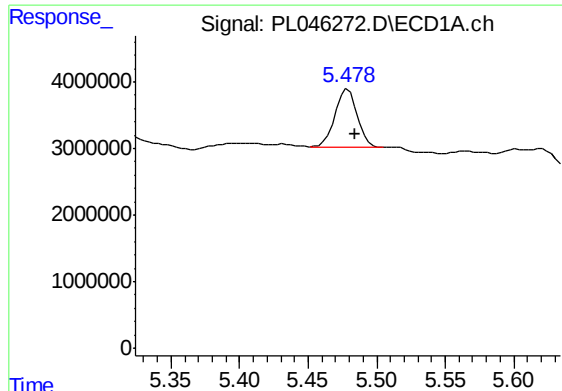

#12 4,4'-DDE


R.T.: 5.479 min
Delta R.T.: -0.005 min
Response: 9766051
Conc: 1.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-032019-B

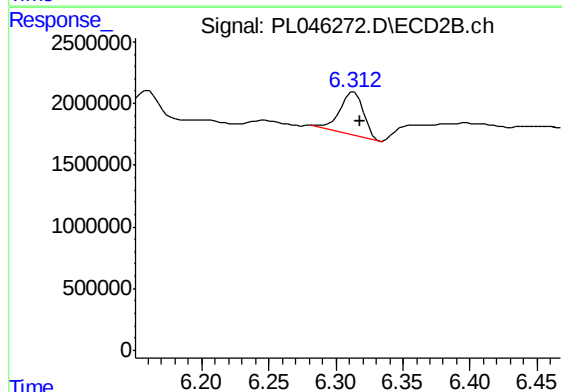


#12 4,4'-DDE

R.T.: 6.314 min
Delta R.T.: -0.004 min
Response: 4262336
Conc: 1.82 ng/ml

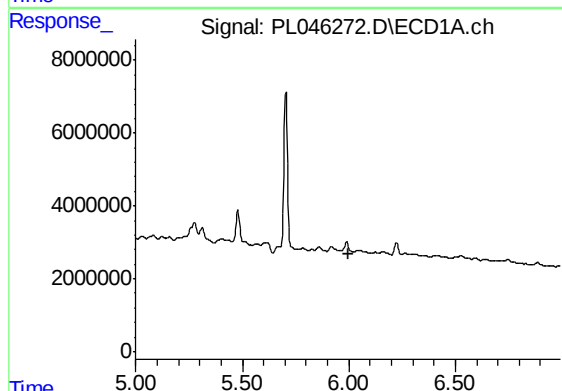


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

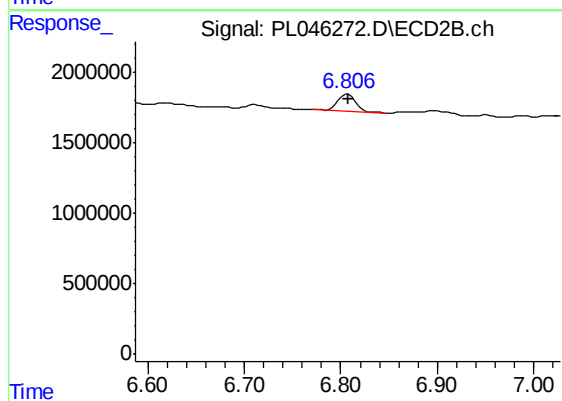

#16 4,4'-DDD


R.T.: 6.807 min
Delta R.T.: 0.000 min
Response: 1513994
Conc: 0.79 ng/ml

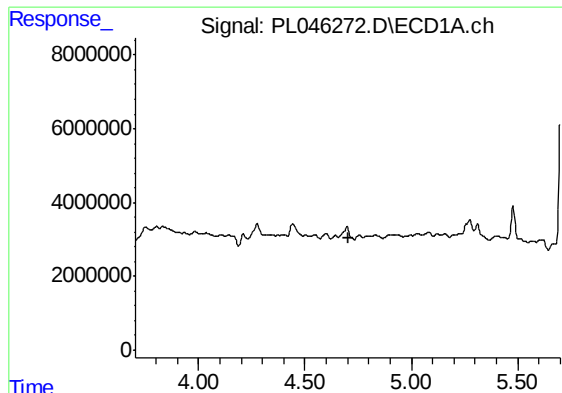

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.704 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-02-032019-B

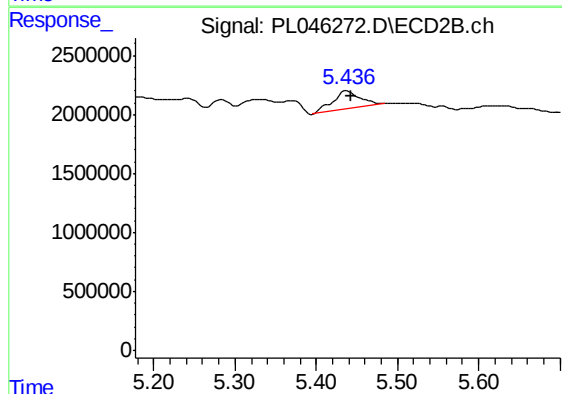


#24 Chlordane-2

R.T.: 5.438 min
Delta R.T.: -0.005 min
Response: 3683590
Conc: 30.49 ng/ml

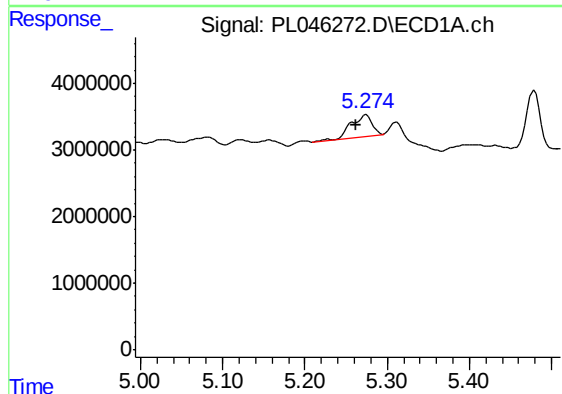


#25 Chlordane-3

R.T.: 5.275 min
Delta R.T.: 0.013 min
Response: 5673429
Conc: 4.95 ng/ml

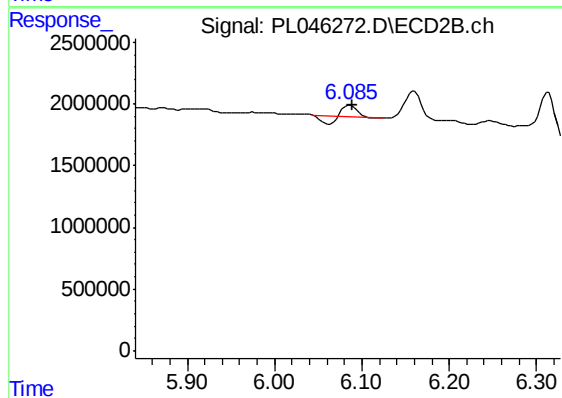

#25 Chlordane-3


R.T.: 6.086 min
Delta R.T.: -0.003 min
Response: 472495
Conc: 1.21 ng/ml

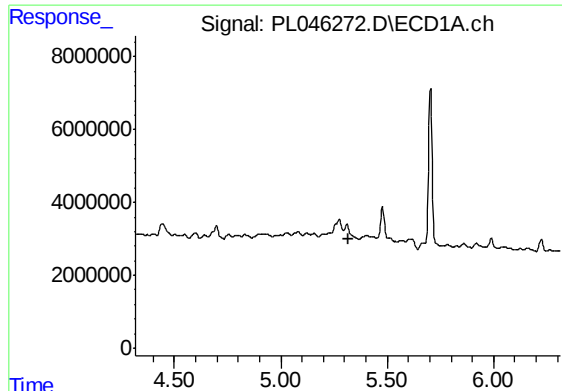

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-02-032019-B

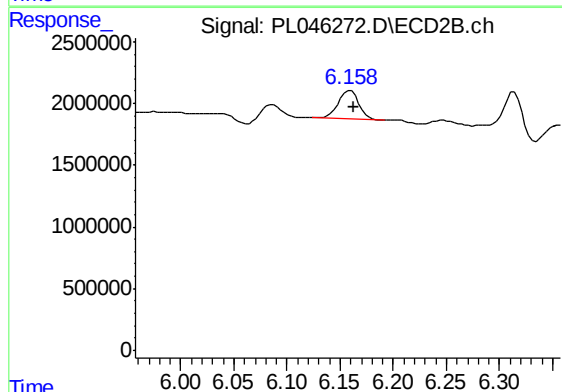


#26 Chlordane-4

R.T.: 6.160 min
Delta R.T.: -0.003 min
Response: 3167340
Conc: 6.77 ng/ml

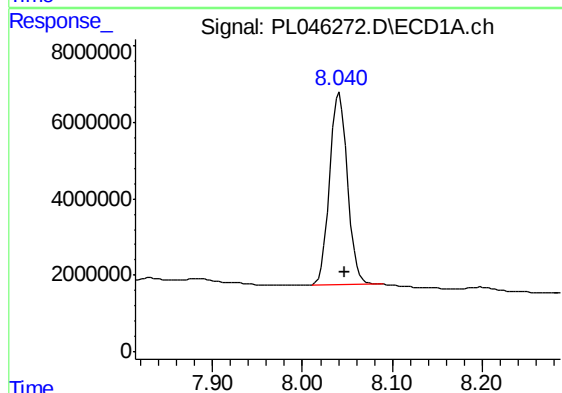

#28 Decachlorobiphenyl

R.T.: 8.041 min
Delta R.T.: -0.006 min
Response: 69703595
Conc: 8.33 ng/ml

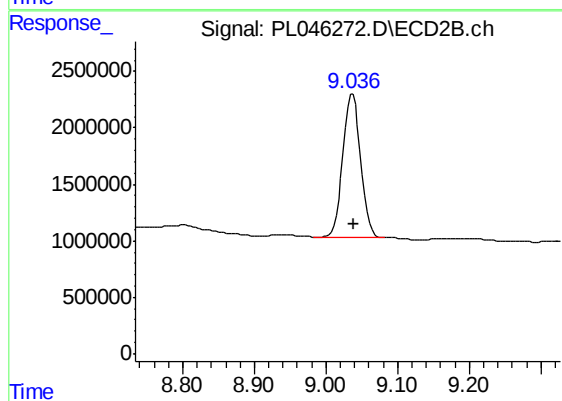

#28 Decachlorobiphenyl

R.T.: 9.037 min
Delta R.T.: -0.002 min
Response: 22041041
Conc: 9.65 ng/ml