

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032119\
 Data File : PL046279.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2019 16:08
 Operator : AJ\SJ
 Sample : K2002-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S4A(5-30)COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 01:05:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.981	127.0E6	41379398	18.467	19.322
28)	SA Decachlor...	8.040	9.036	113.3E6	31540564	13.545	13.804
Target Compounds							
2)	A alpha-BHC	0.000	4.395f	0	2334608	N.D.	0.768 #
3)	MA gamma-BHC...	4.076	0.000	3952900	0	0.391	N.D. #
9)	A Endosulfan I	5.394f	0.000	22380258	0	2.504	N.D. #
10)	B gamma-Chl...	0.000	6.073	0	5337158	N.D.	1.989 #
13)	MA Dieldrin	5.592f	0.000	24898322	0	2.605	N.D. #
15)	B Endosulfa...	0.000	6.905	0	2486587	N.D.	1.057 #
16)	A 4,4'-DDD	0.000	6.804	0	4070856	N.D.	2.117 #
25)	Chlordane-3	0.000	6.073f	0	5337158	N.D.	13.698 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032119\
Data File : PL046279.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2019 16:08
Operator : AJ\SJ
Sample : K2002-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
S4A(5-30)COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 01:05:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

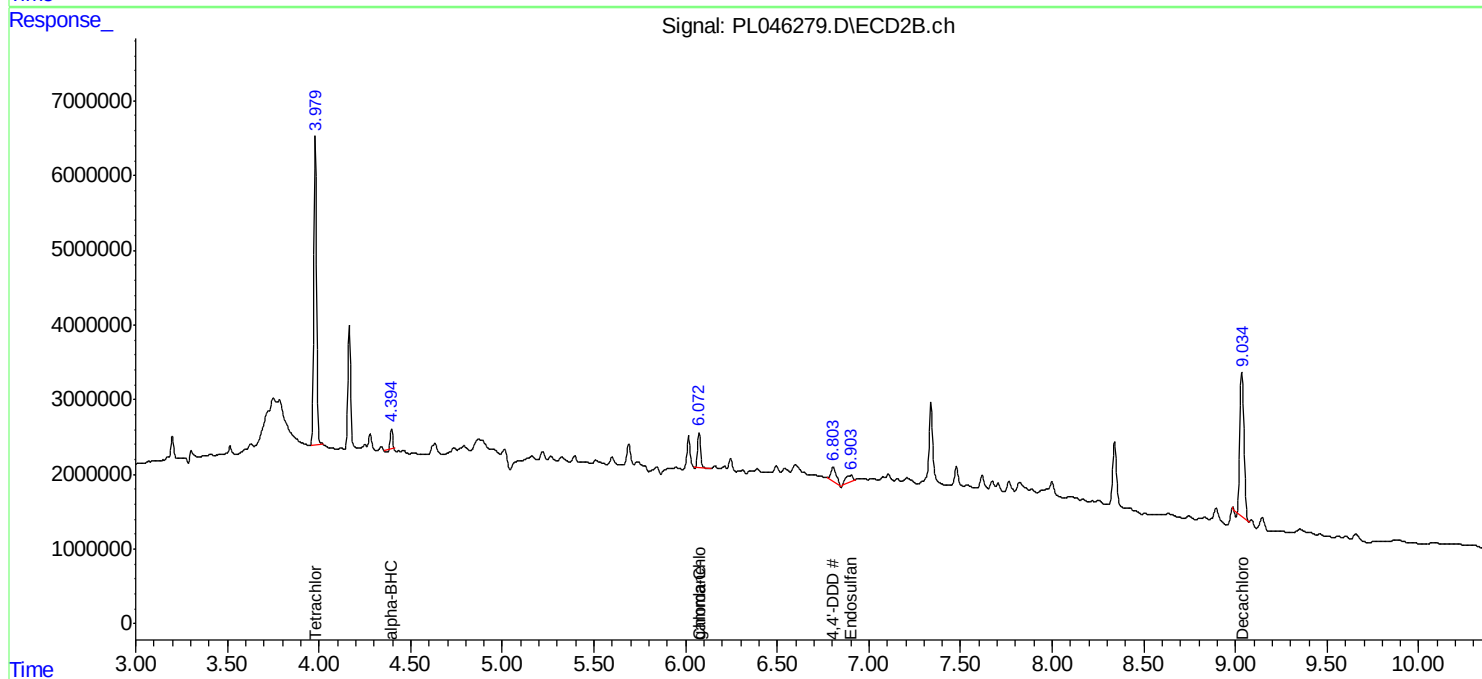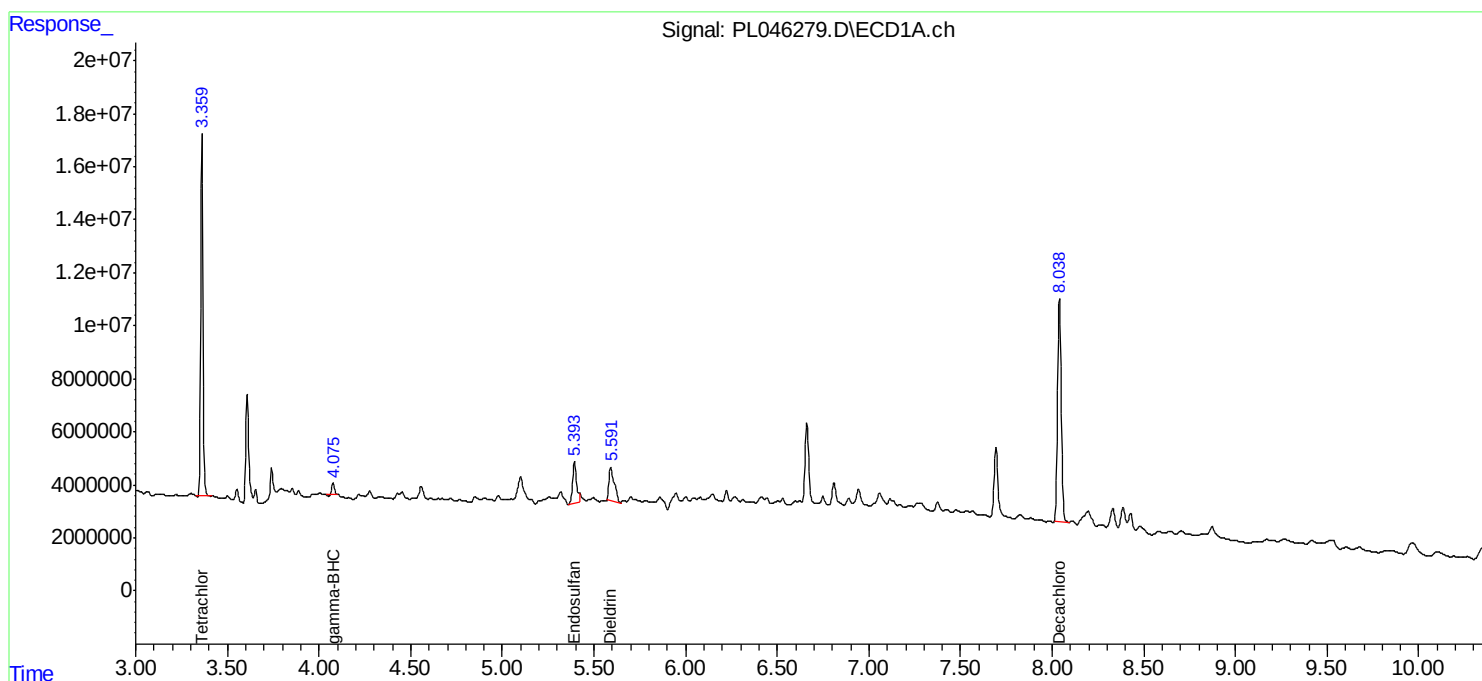


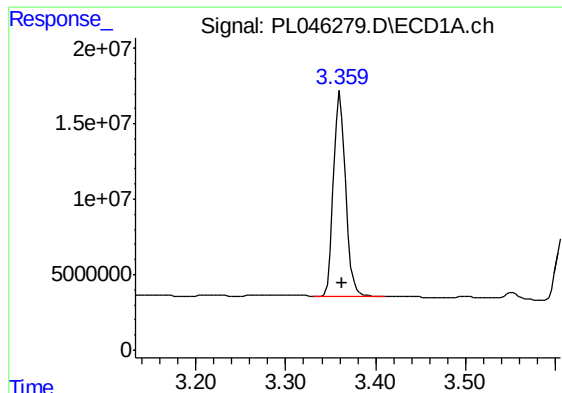

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: -0.002 min
Response: 127040680
Conc: 18.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
S4A(5-30)COMP

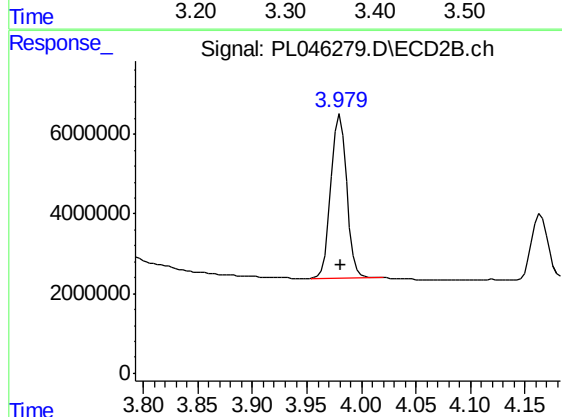


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: -0.001 min
Response: 41379398
Conc: 19.32 ng/ml

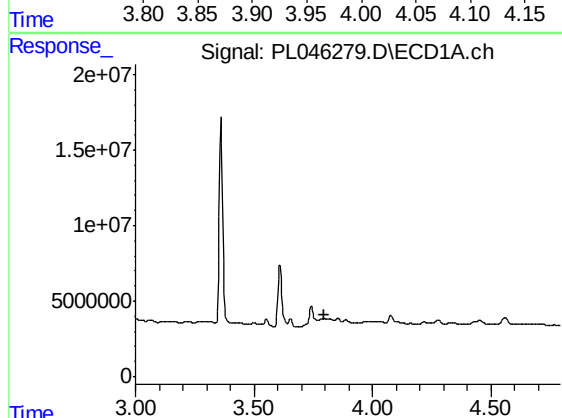


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.794 min
Response: 0
Conc: N.D.

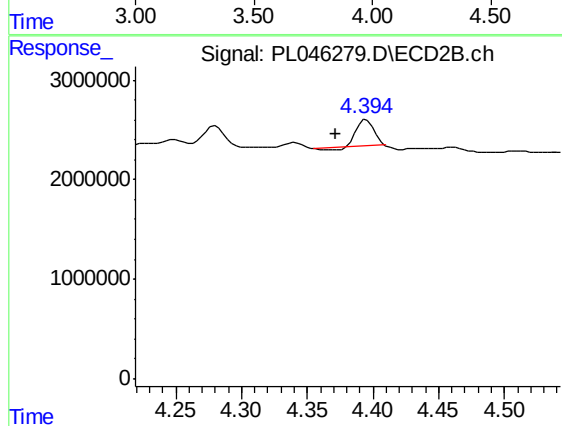

#2 alpha-BHC


R.T.: 4.395 min
Delta R.T.: 0.024 min
Response: 2334608
Conc: 0.77 ng/ml

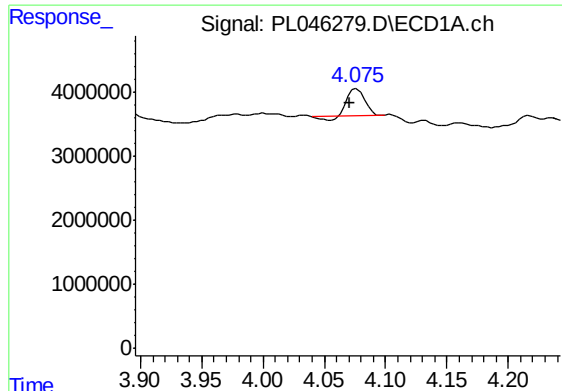

#3 gamma-BHC (Lindane)


R.T.: 4.076 min
Delta R.T.: 0.006 min
Response: 3952900
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
S4A(5-30)COMP

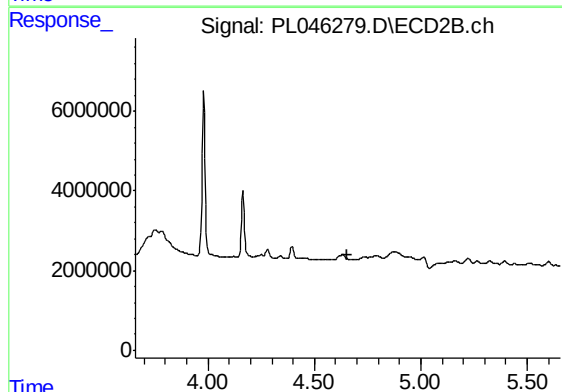


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.656 min
Response: 0
Conc: N.D.

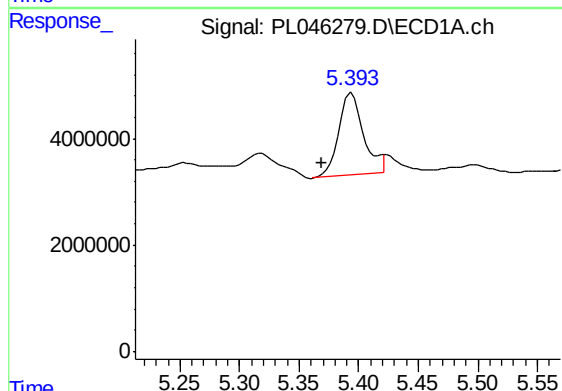


#9 Endosulfan I

R.T.: 5.394 min
Delta R.T.: 0.025 min
Response: 22380258
Conc: 2.50 ng/ml

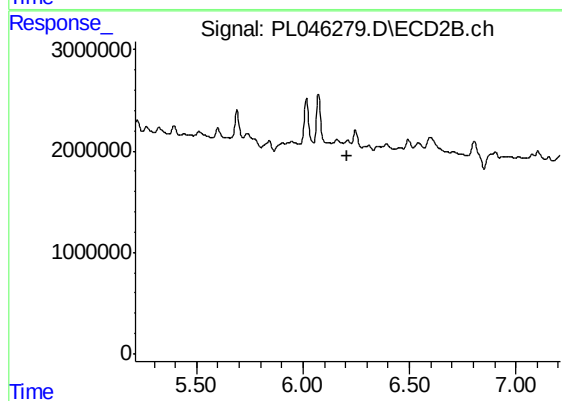

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.210 min
Response: 0
Conc: N.D.

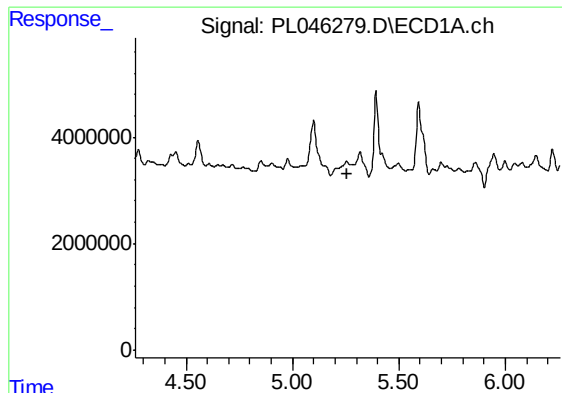

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S4A(5-30)COMP

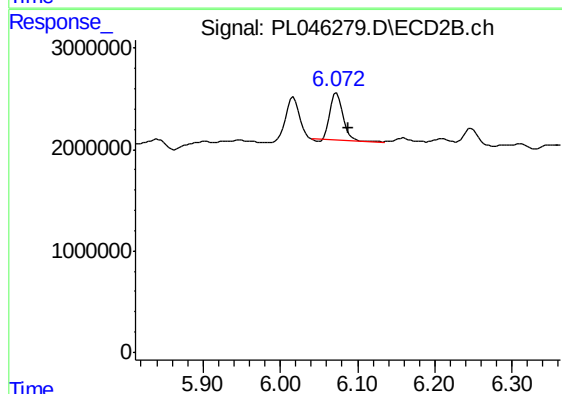


#10 gamma-Chlordane

R.T.: 6.073 min
Delta R.T.: -0.015 min
Response: 5337158
Conc: 1.99 ng/ml

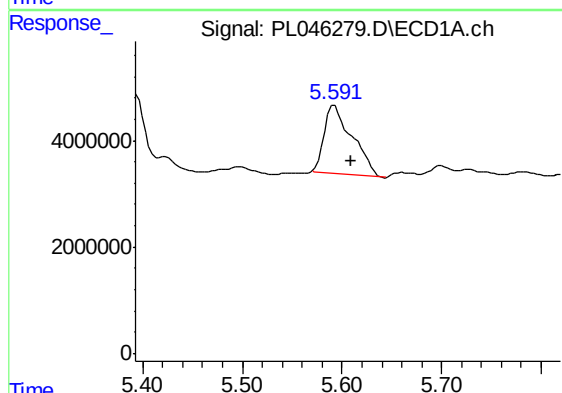


#13 Dieldrin

R.T.: 5.592 min
Delta R.T.: -0.017 min
Response: 24898322
Conc: 2.60 ng/ml

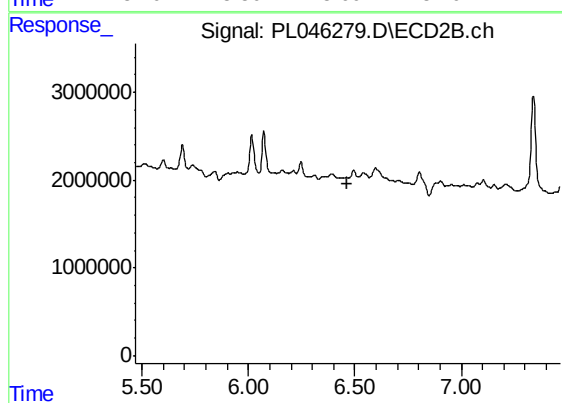

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.467 min
Response: 0
Conc: N.D.

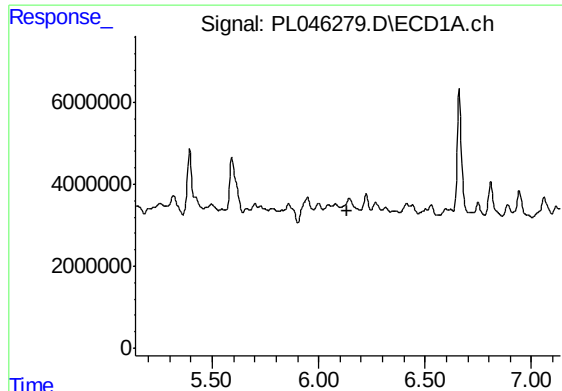

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.137 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S4A(5-30)COMP

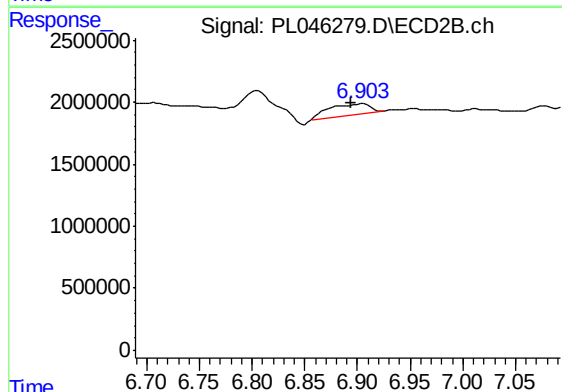


#15 Endosulfan II

R.T.: 6.905 min
Delta R.T.: 0.011 min
Response: 2486587
Conc: 1.06 ng/ml

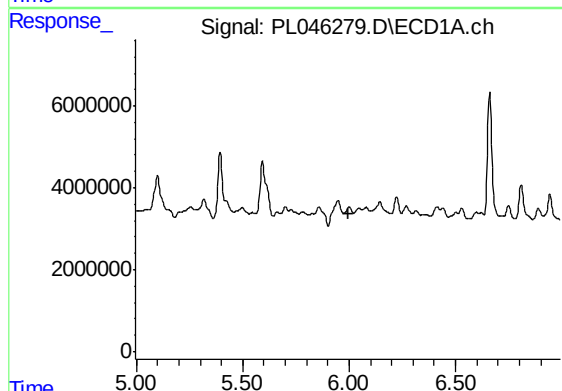


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.996 min
Response: 0
Conc: N.D.

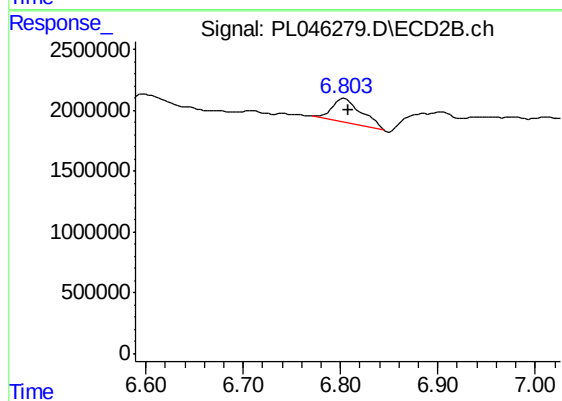

#16 4,4'-DDD


R.T.: 6.804 min
Delta R.T.: -0.004 min
Response: 4070856
Conc: 2.12 ng/ml

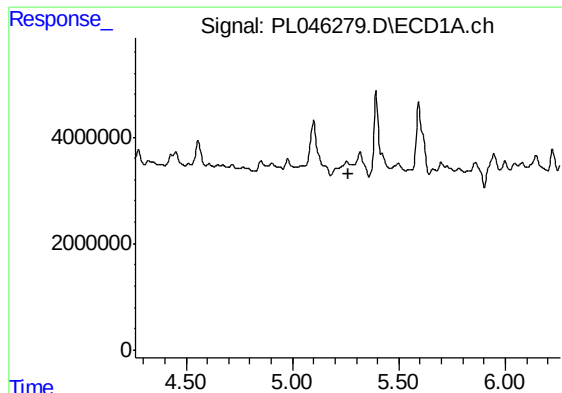

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.262 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S4A(5-30)COMP

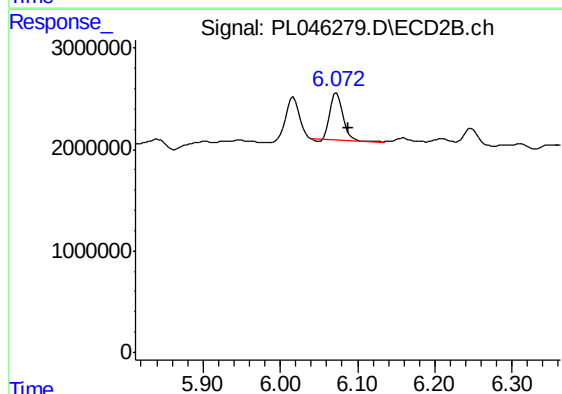


#25 Chlordane-3

R.T.: 6.073 min
Delta R.T.: -0.016 min
Response: 5337158
Conc: 13.70 ng/ml

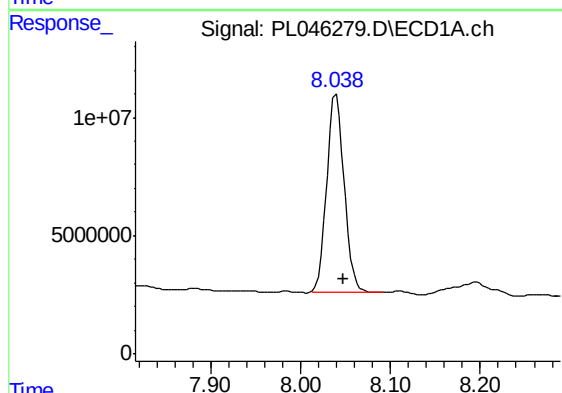

#28 Decachlorobiphenyl

R.T.: 8.040 min
Delta R.T.: -0.008 min
Response: 113339047
Conc: 13.55 ng/ml

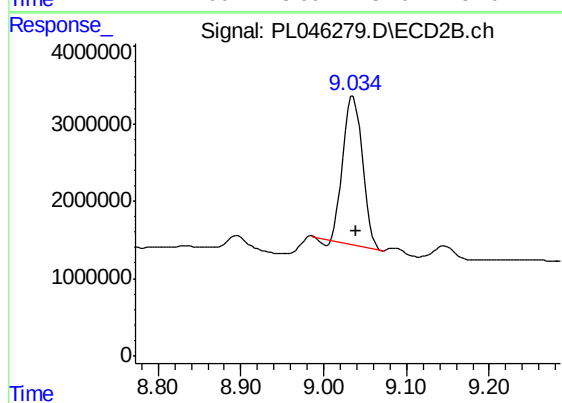

#28 Decachlorobiphenyl

R.T.: 9.036 min
Delta R.T.: -0.003 min
Response: 31540564
Conc: 13.80 ng/ml