

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032124\
 Data File : PL088712.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2024 14:36
 Operator : AR\AJ
 Sample : PB159707BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB159707BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/22/2024
 Supervised By : Ankita Jodhani 03/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 23:20:25 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.644	2.854	48805995	23849226	18.418	17.895
2)	SA Decachlor...	9.312	8.086	37052894	19457681	14.990m	14.350

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032124\
Data File : PL088712.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2024 14:36
Operator : AR\AJ
Sample : PB159707BL
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB159707BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/22/2024
Supervised By : Ankita Jodhani 03/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 23:20:25 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

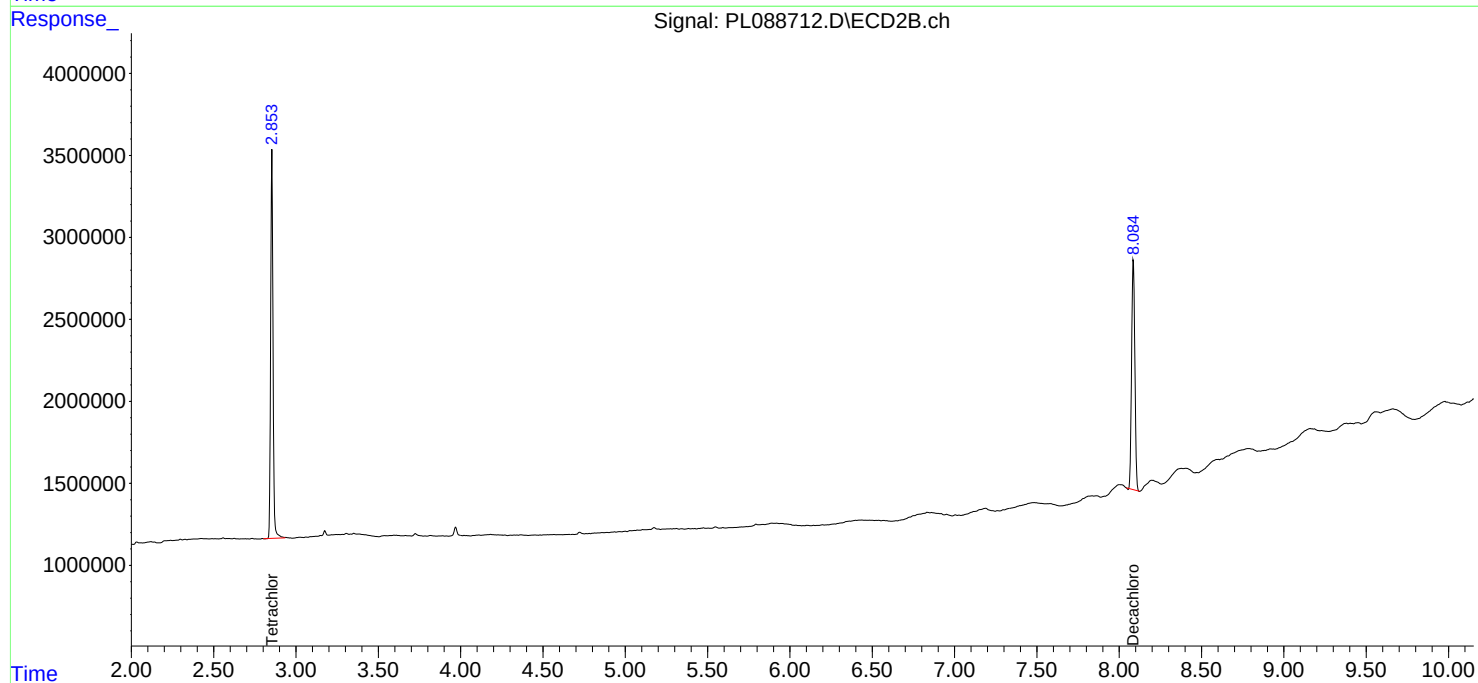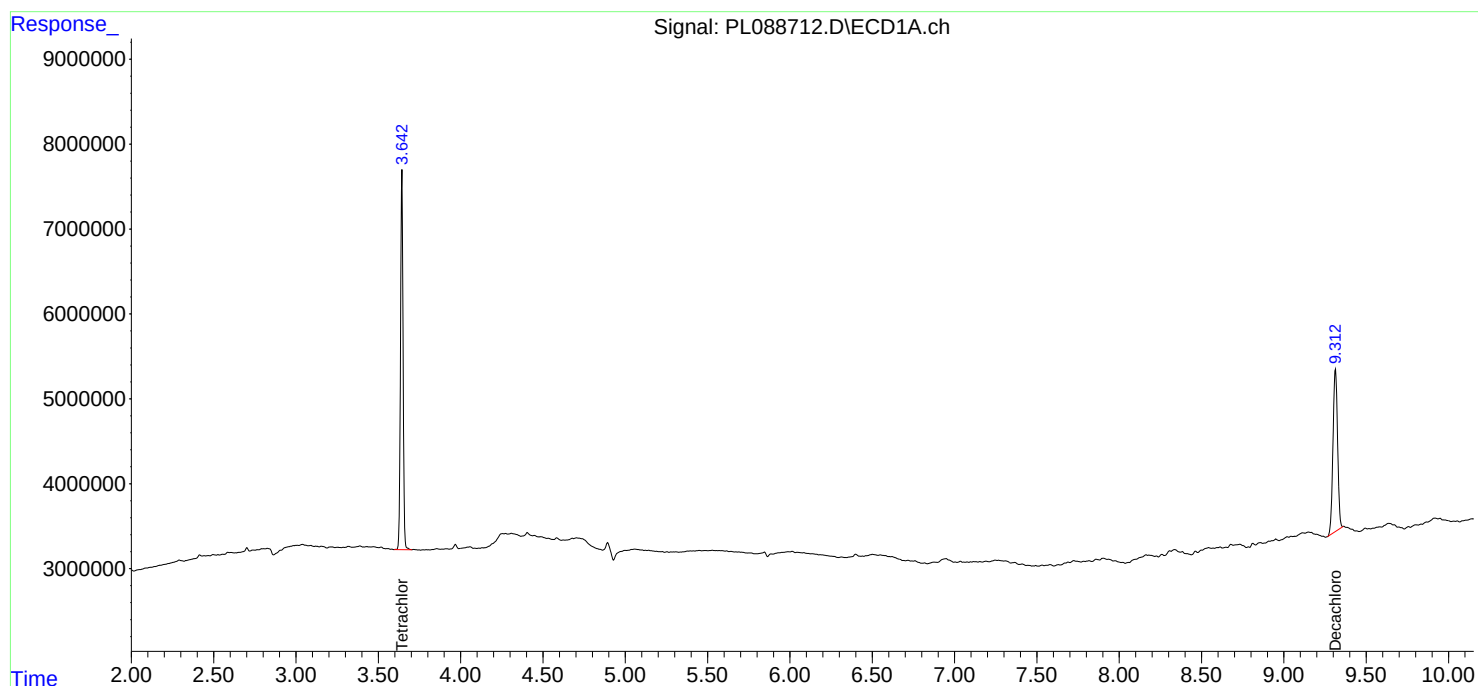

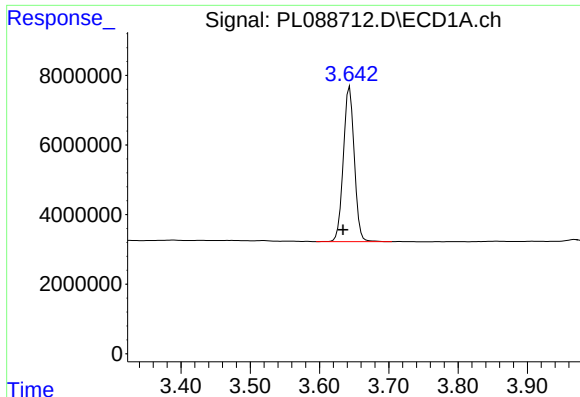


#1 Tetrachloro-m-xylene

R.T.: 3.644 min
Delta R.T.: 0.010 min
Response: 48805995
Conc: 18.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB159707BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/22/2024
Supervised By :Ankita Jodhani 03/22/2024

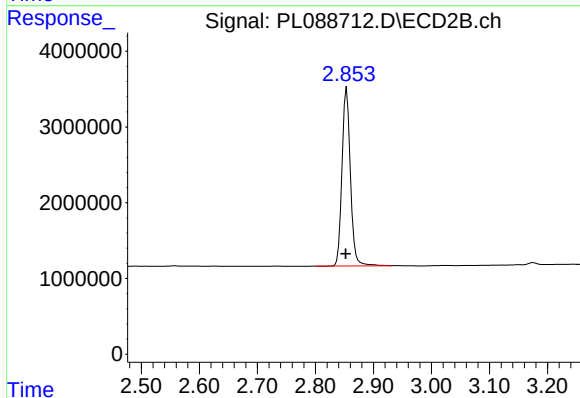


#1 Tetrachloro-m-xylene

R.T.: 2.854 min
Delta R.T.: 0.002 min
Response: 23849226
Conc: 17.89 ng/ml

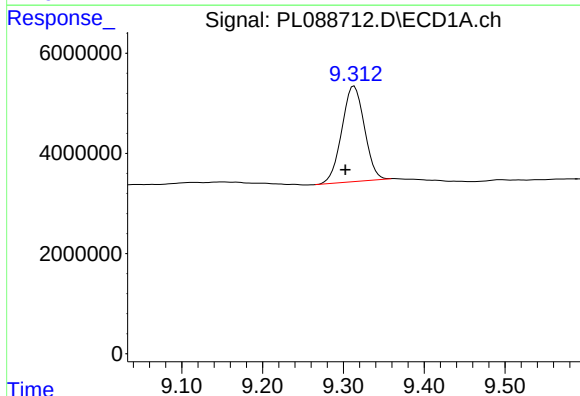

#28 Decachlorobiphenyl

R.T.: 9.312 min
Delta R.T.: 0.009 min
Response: 37052894
Conc: 14.99 ng/ml m

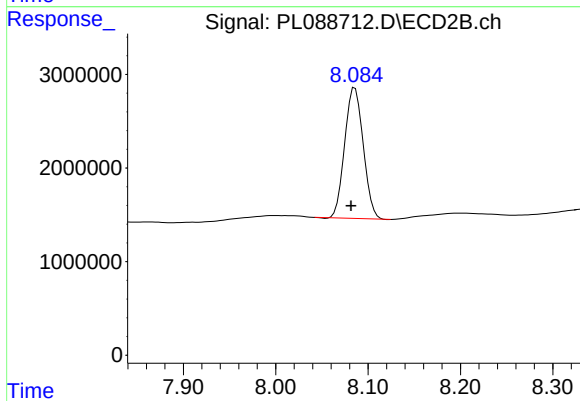

#28 Decachlorobiphenyl

R.T.: 8.086 min
Delta R.T.: 0.004 min
Response: 19457681
Conc: 14.35 ng/ml