

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032125\
 Data File : PL094793.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2025 15:12
 Operator : AR\AJ
 Sample : Q1607-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OR-03-031925

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 21 23:23:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
 Quant Title : GC Extractables
 QLast Update : Tue Mar 11 17:42:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.770	37877541	49316560	13.381	13.817
28)	SA Decachlor...	9.054	7.905	28175377	38660163	13.369	9.571 #
Target Compounds							
8)	B Heptachlo...	5.681	4.725	3600504	73859736	1.076	16.132 #
10)	B gamma-Chl...	5.937	4.973	9286177	20639386	2.756	4.275 #
11)	B alpha-Chl...	6.019	5.035	10038780	35682695	3.045	7.476 #
13)	MA Dieldrin	0.000	5.364	0	52894068	N.D.	10.902 #
14)	MA Endrin	0.000	5.648	0	47799062	N.D.	10.954 #
24)	Chlordane-2	0.000	4.343	0	8134998	N.D.	46.068 #
25)	Chlordane-3	5.937	4.973	9286177	20639386	18.579	38.796 #
26)	Chlordane-4	6.019	5.035	10038780	35682695	17.041	68.547 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031215\
Data File : PL094793.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2025 15:12
Operator : AR\AJ
Sample : Q1607-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OR-03-031925

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 21 23:23:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031125.M
Quant Title : GC Extractables
QLast Update : Tue Mar 11 17:42:21 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

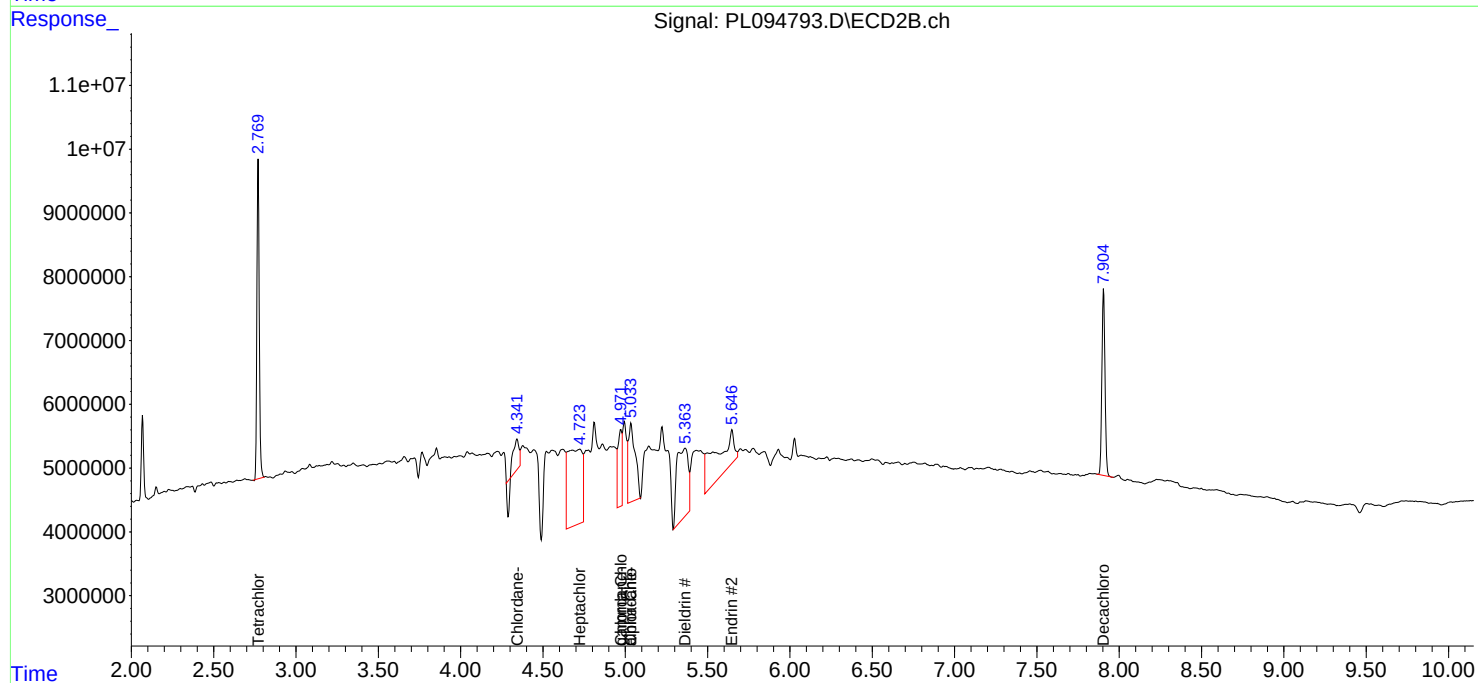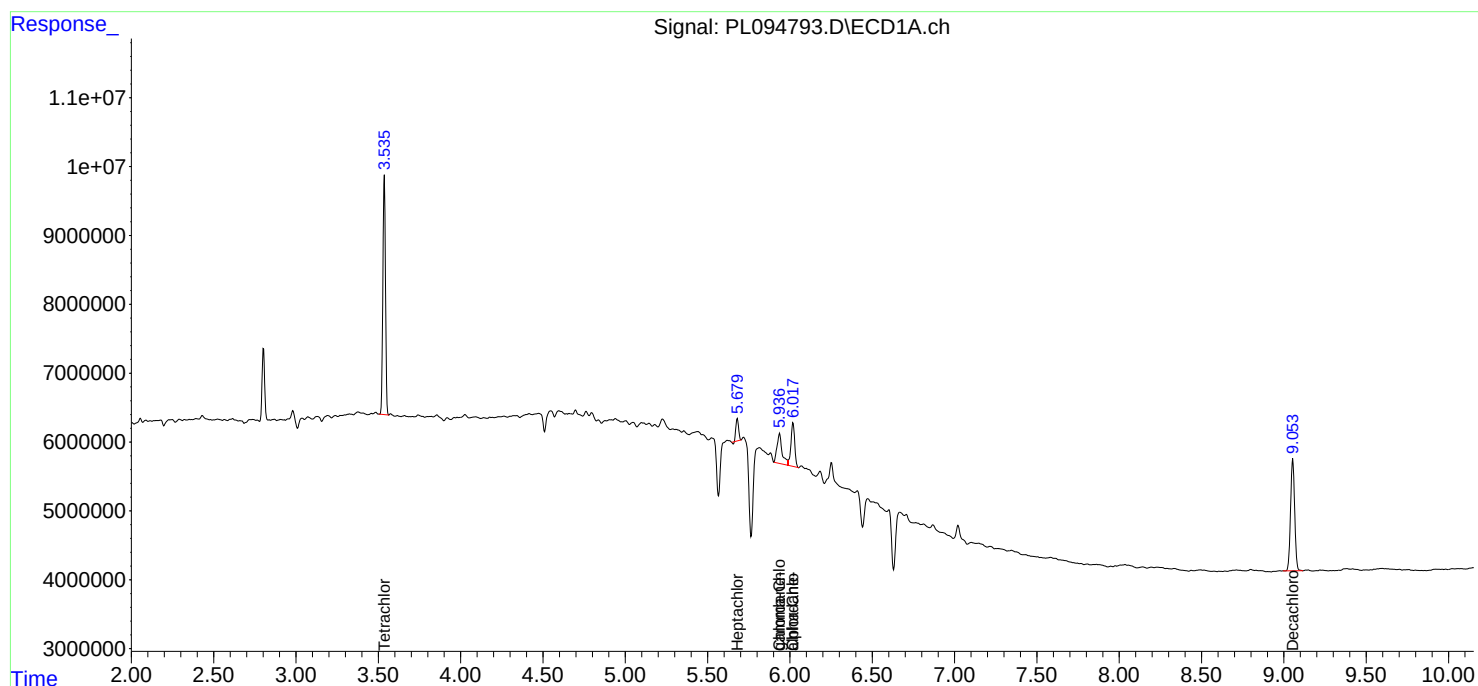


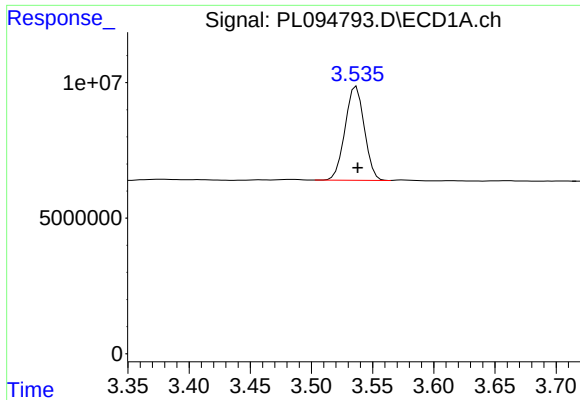

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: -0.001 min
Response: 37877541
Conc: 13.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-031925

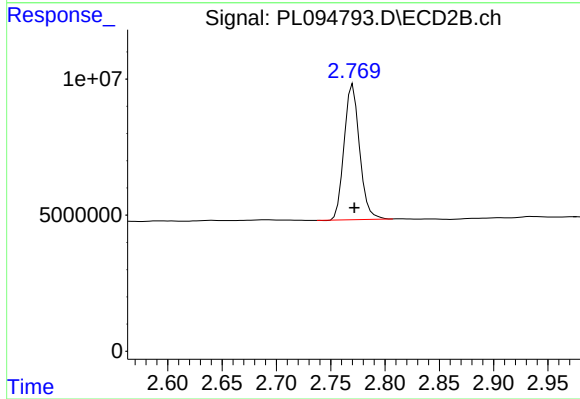


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: -0.001 min
Response: 49316560
Conc: 13.82 ng/ml

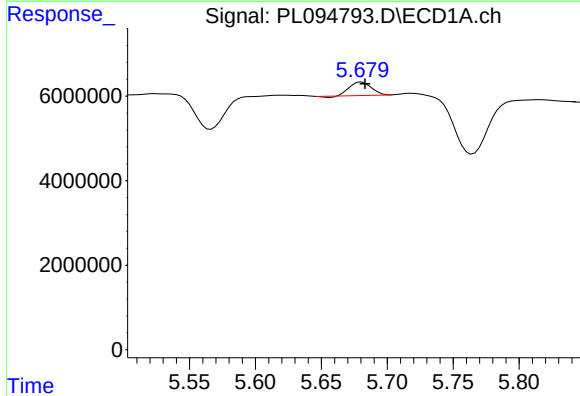


#8 Heptachlor epoxide

R.T.: 5.681 min
Delta R.T.: -0.002 min
Response: 3600504
Conc: 1.08 ng/ml

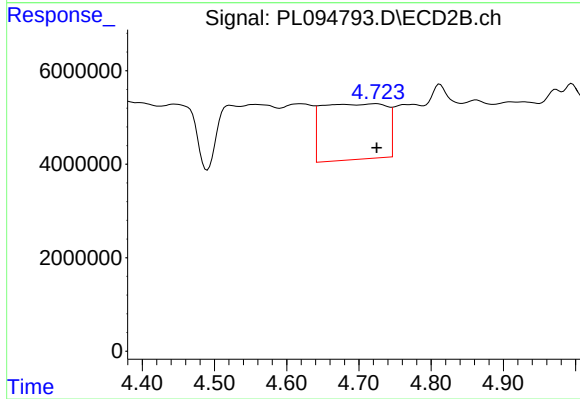

#8 Heptachlor epoxide


R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 73859736
Conc: 16.13 ng/ml

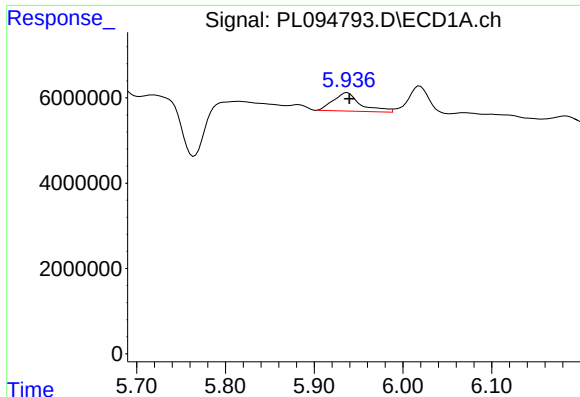

#10 gamma-Chlordane


R.T.: 5.937 min
Delta R.T.: -0.002 min
Response: 9286177
Conc: 2.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-031925

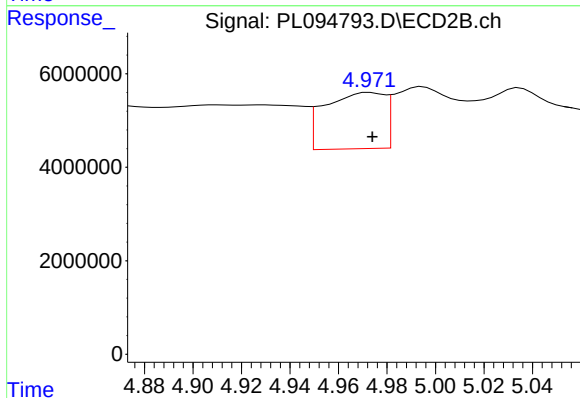


#10 gamma-Chlordane

R.T.: 4.973 min
Delta R.T.: 0.000 min
Response: 20639386
Conc: 4.27 ng/ml

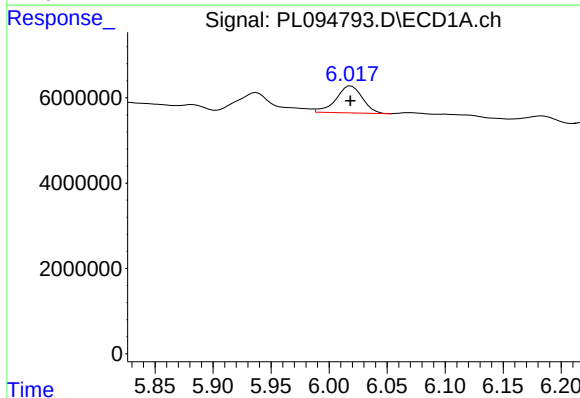


#11 alpha-Chlordane

R.T.: 6.019 min
Delta R.T.: 0.000 min
Response: 10038780
Conc: 3.04 ng/ml

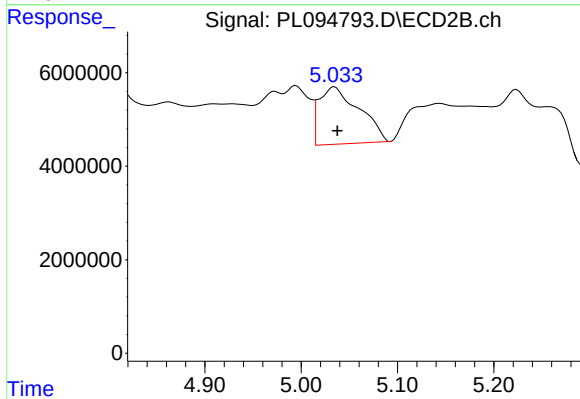

#11 alpha-Chlordane


R.T.: 5.035 min
Delta R.T.: -0.003 min
Response: 35682695
Conc: 7.48 ng/ml

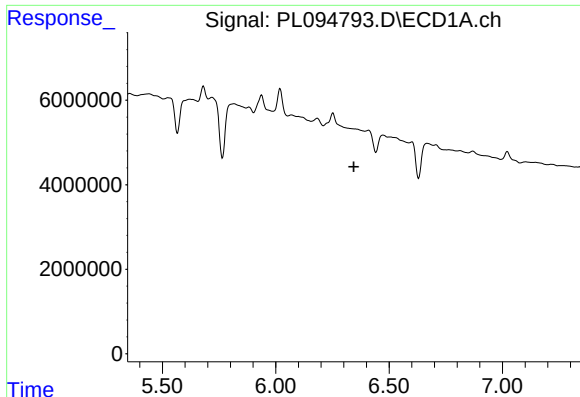

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.344 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-03-031925

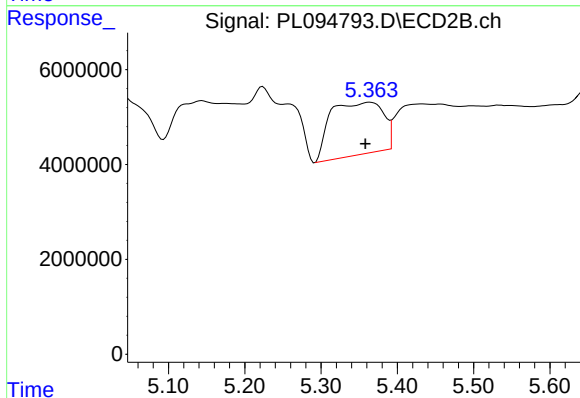


#13 Dieldrin

R.T.: 5.364 min
Delta R.T.: 0.006 min
Response: 52894068
Conc: 10.90 ng/ml

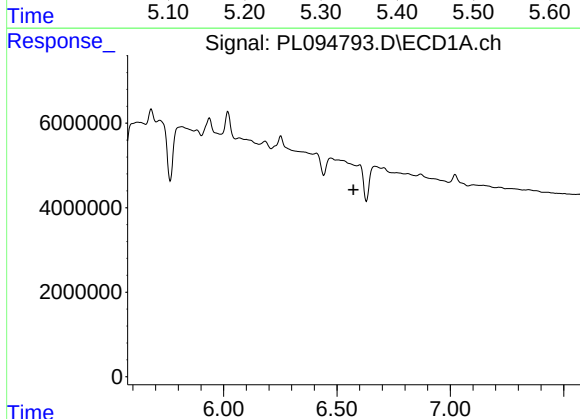


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.574 min
Response: 0
Conc: N.D.

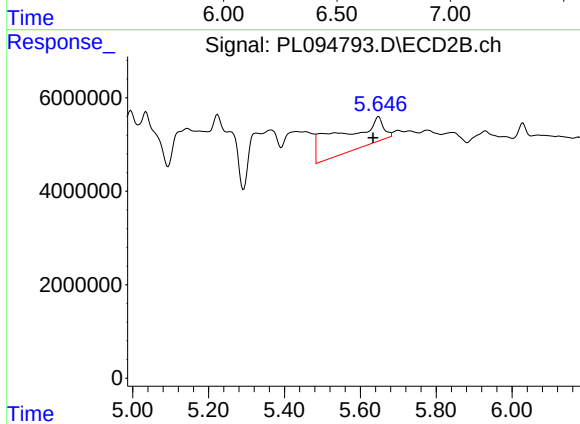

#14 Endrin


R.T.: 5.648 min
Delta R.T.: 0.015 min
Response: 47799062
Conc: 10.95 ng/ml

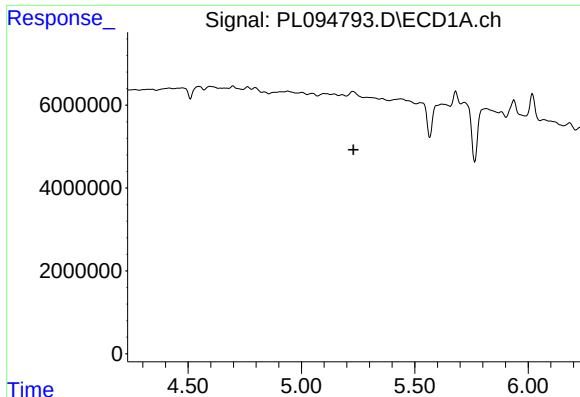

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.230 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OR-03-031925

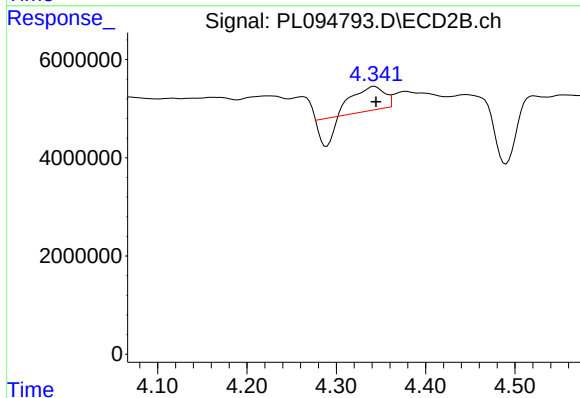


#24 Chlordane-2

R.T.: 4.343 min
Delta R.T.: -0.002 min
Response: 8134998
Conc: 46.07 ng/ml

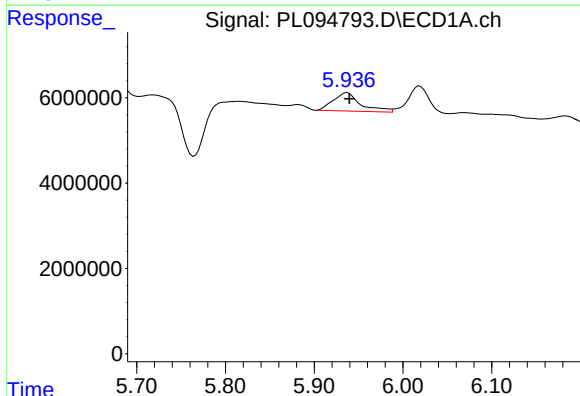


#25 Chlordane-3

R.T.: 5.937 min
Delta R.T.: -0.002 min
Response: 9286177
Conc: 18.58 ng/ml

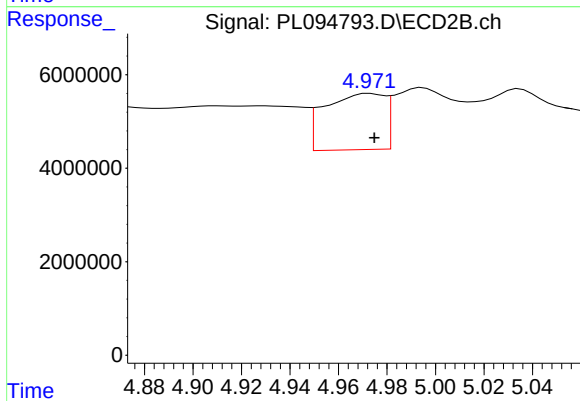

#25 Chlordane-3


R.T.: 4.973 min
Delta R.T.: -0.002 min
Response: 20639386
Conc: 38.80 ng/ml

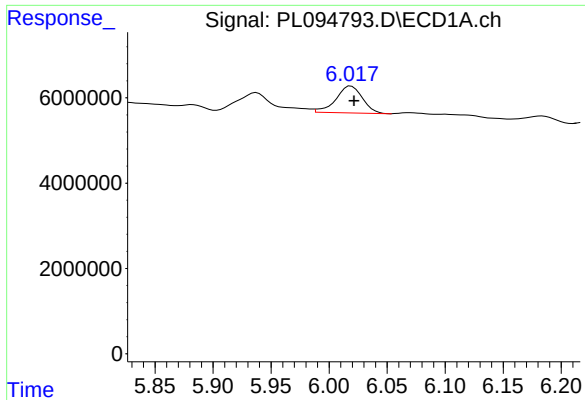

#26 Chlordane-4


R.T.: 6.019 min
Delta R.T.: -0.003 min
Response: 10038780
Conc: 17.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
OR-03-031925

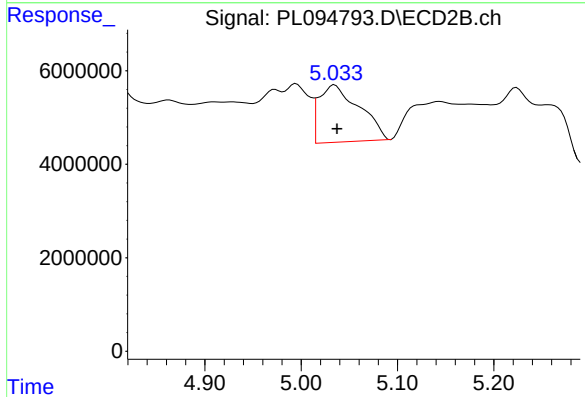


#26 Chlordane-4

R.T.: 5.035 min
Delta R.T.: -0.002 min
Response: 35682695
Conc: 68.55 ng/ml

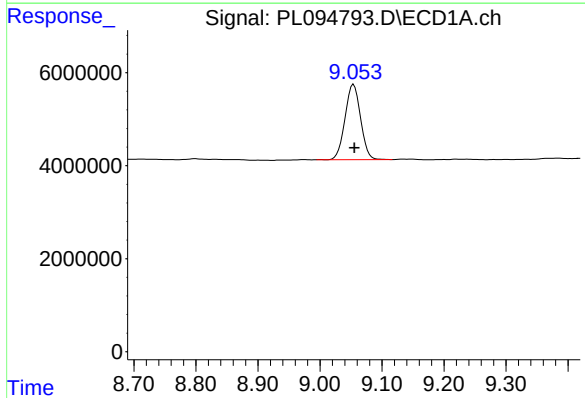

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: -0.001 min
Response: 28175377
Conc: 13.37 ng/ml

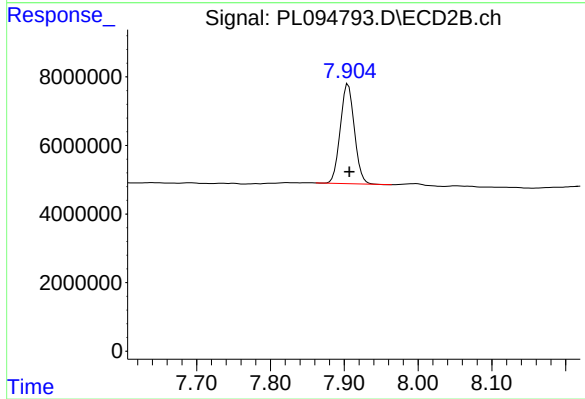

#28 Decachlorobiphenyl

R.T.: 7.905 min
Delta R.T.: -0.001 min
Response: 38660163
Conc: 9.57 ng/ml