

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
 Data File : PL046312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 11:04
 Operator : AJ\SJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 01:56:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.982	154.4E6	47963060	21.229	20.948
28)	SA Decachlor...	8.044	9.041	184.0E6	52448554	21.873	22.622
Target Compounds							
9)	A Endosulfan I	5.366	6.211	94364402	27139497	10.036	10.399
10)	B gamma-Chl...	5.257	6.088	102.8E6	29494115	10.006	10.392
12)	B 4,4'-DDE	5.481	6.319	192.4E6	50766236	20.897	20.451
13)	MA Dieldrin	5.606	6.468	212.5E6	57153527	21.173	21.085
19)	B Endosulfa...	6.513	7.242	169.7E6	49026655	20.670	20.783
20)	A Methoxychlor	6.773	7.566	453.9E6	129.8E6	106.792	101.794
21)	B Endrin ke...	6.997	7.713	167.5E6	45848363	18.117	18.453
25)	Chlordane-3	5.257	6.088	102.8E6	29494115	92.294	77.358



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
Data File : PL046312.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 11:04
Operator : AJ\SJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 01:56:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

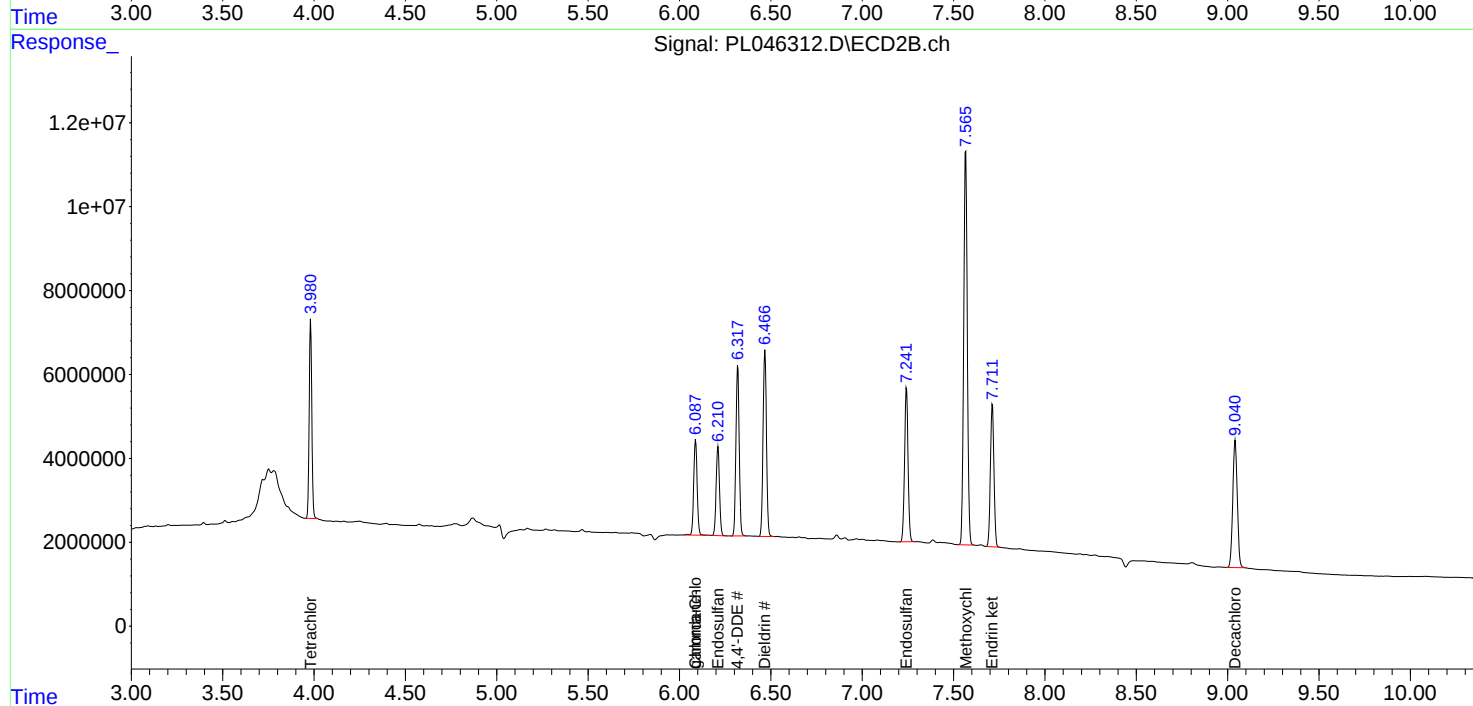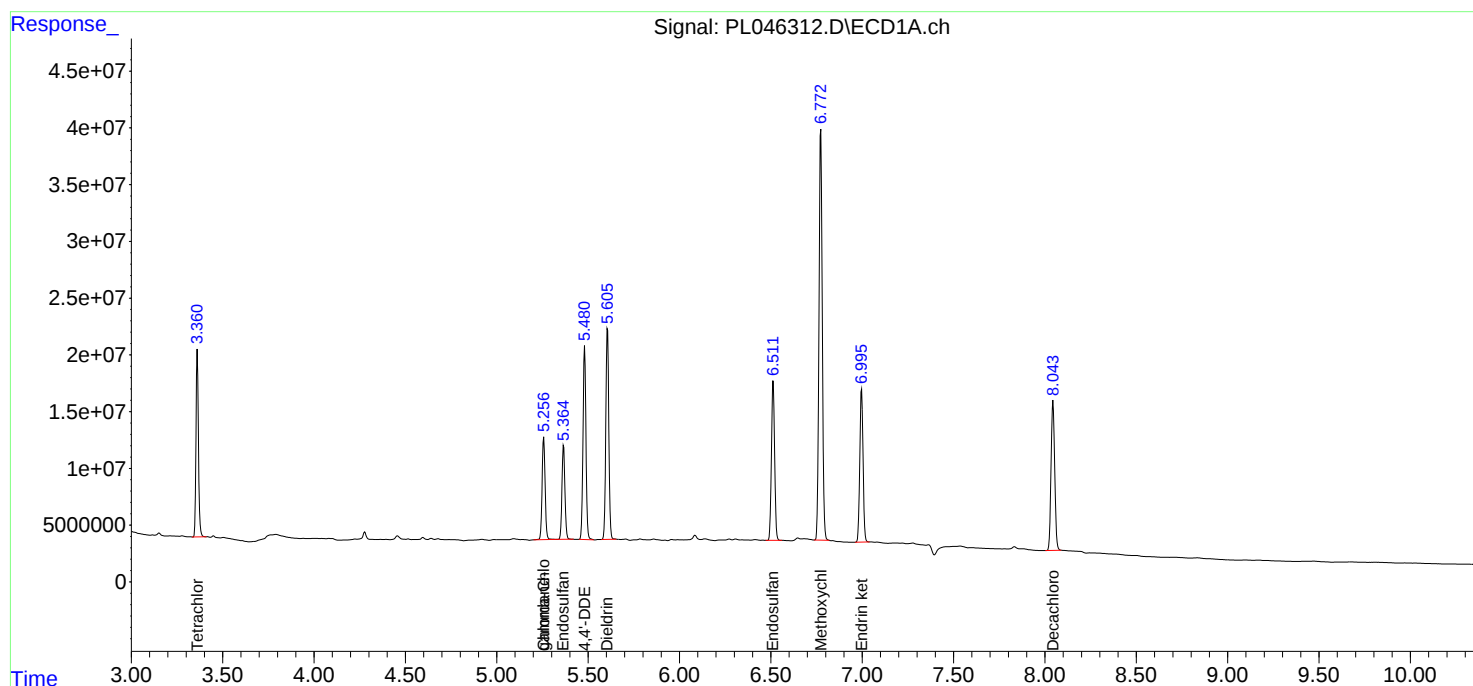


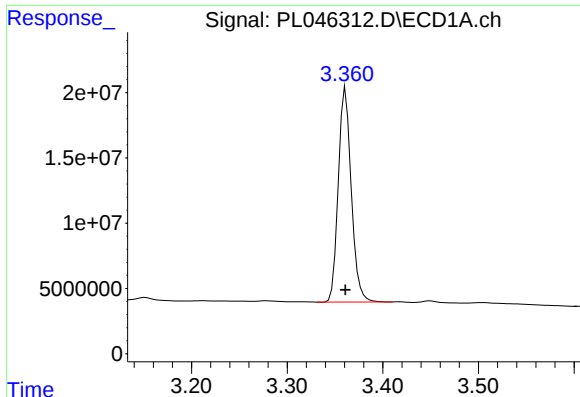

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: 0.000 min
Response: 154432790
Conc: 21.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

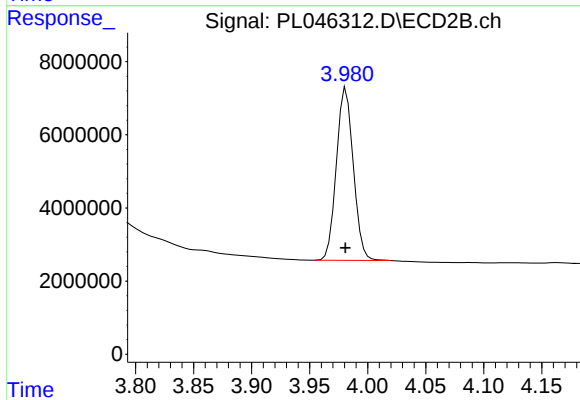


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 47963060
Conc: 20.95 ng/ml

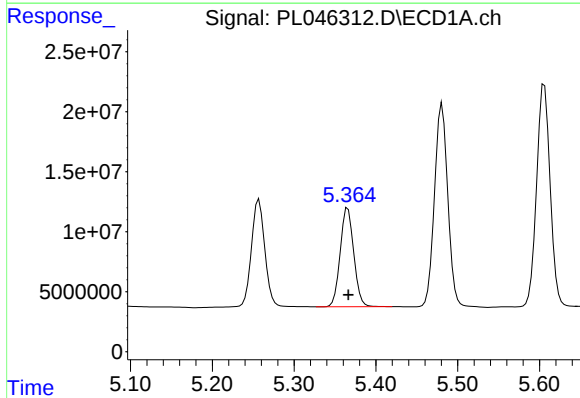


#9 Endosulfan I

R.T.: 5.366 min
Delta R.T.: 0.000 min
Response: 94364402
Conc: 10.04 ng/ml

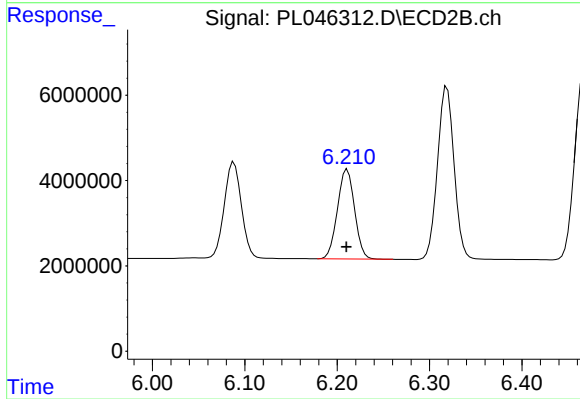

#9 Endosulfan I


R.T.: 6.211 min
Delta R.T.: 0.000 min
Response: 27139497
Conc: 10.40 ng/ml

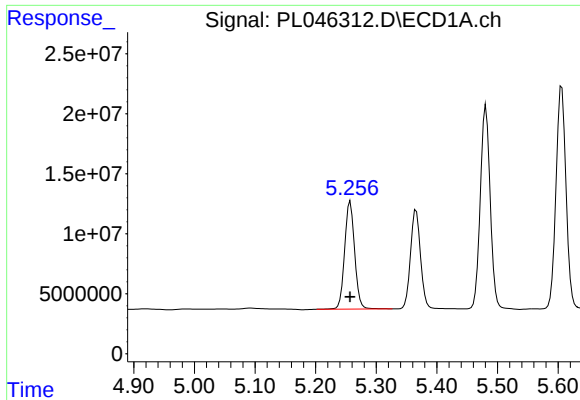

#10 gamma-Chlordane


R.T.: 5.257 min
Delta R.T.: 0.000 min
Response: 102784866
Conc: 10.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

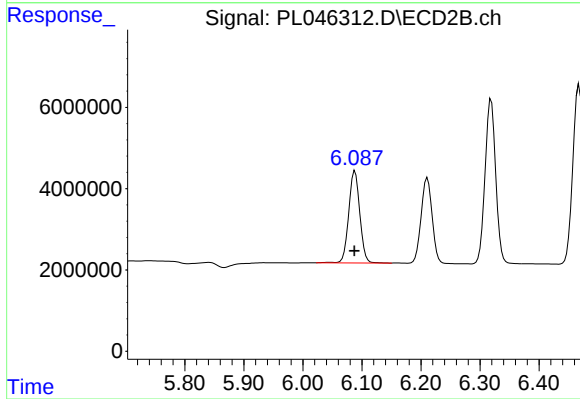


#10 gamma-Chlordane

R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 29494115
Conc: 10.39 ng/ml

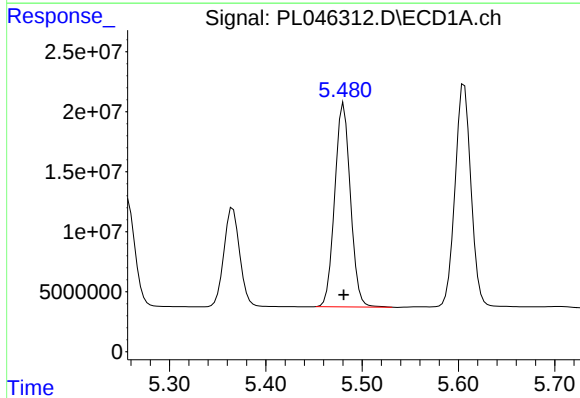


#12 4,4'-DDE

R.T.: 5.481 min
Delta R.T.: 0.000 min
Response: 192400754
Conc: 20.90 ng/ml

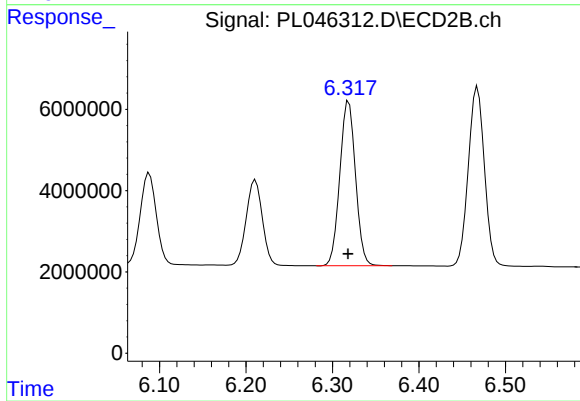

#12 4,4'-DDE


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 50766236
Conc: 20.45 ng/ml

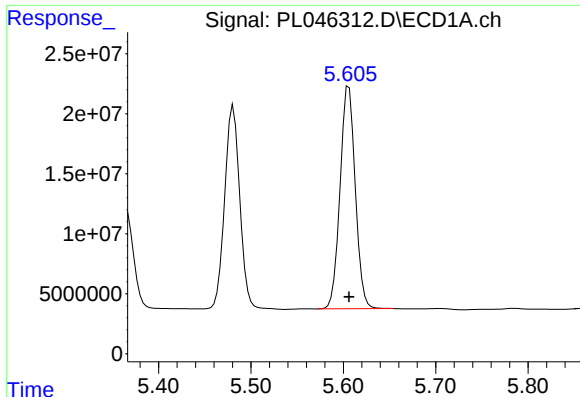

#13 Dieldrin


R.T.: 5.606 min
Delta R.T.: 0.000 min
Response: 212478249
Conc: 21.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

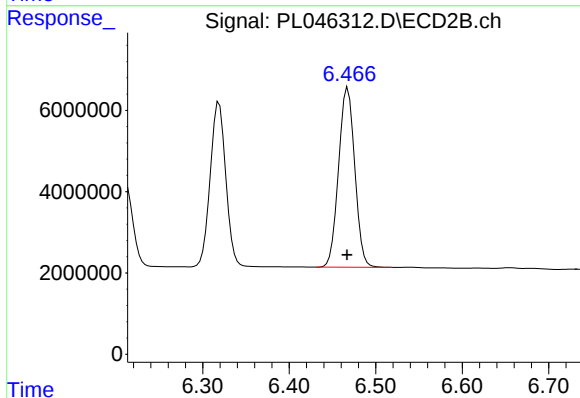


#13 Dieldrin

R.T.: 6.468 min
Delta R.T.: 0.000 min
Response: 57153527
Conc: 21.08 ng/ml

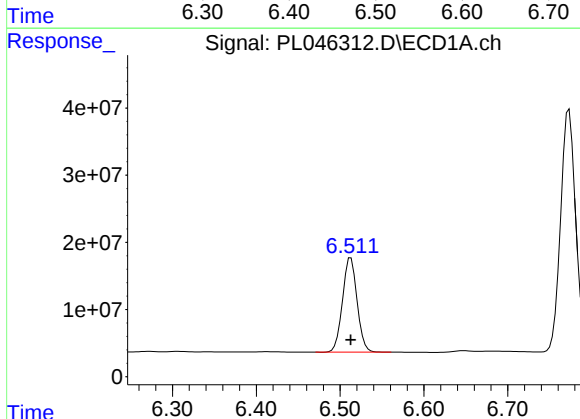


#19 Endosulfan Sulfate

R.T.: 6.513 min
Delta R.T.: 0.000 min
Response: 169724275
Conc: 20.67 ng/ml

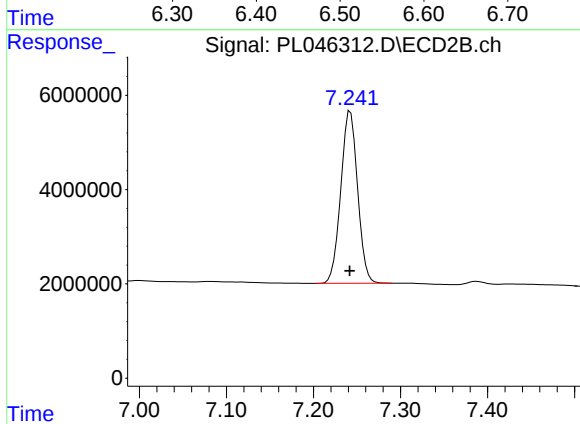

#19 Endosulfan Sulfate


R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 49026655
Conc: 20.78 ng/ml

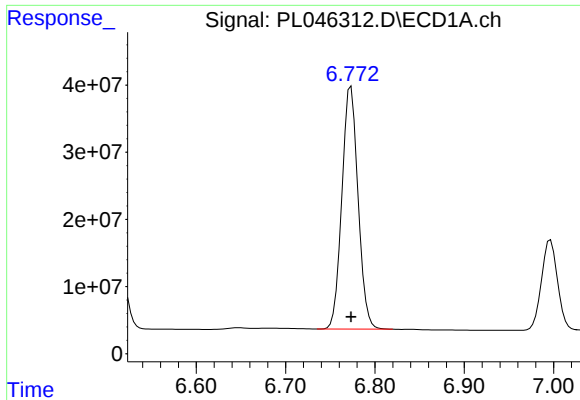

#20 Methoxychlor


R.T.: 6.773 min
Delta R.T.: 0.000 min
Response: 453853589
Conc: 106.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

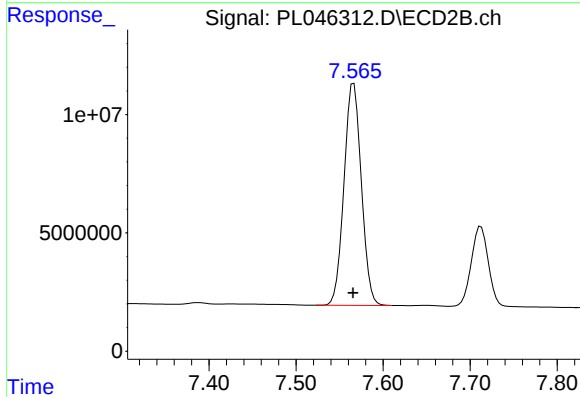


#20 Methoxychlor

R.T.: 7.566 min
Delta R.T.: 0.000 min
Response: 129763977
Conc: 101.79 ng/ml

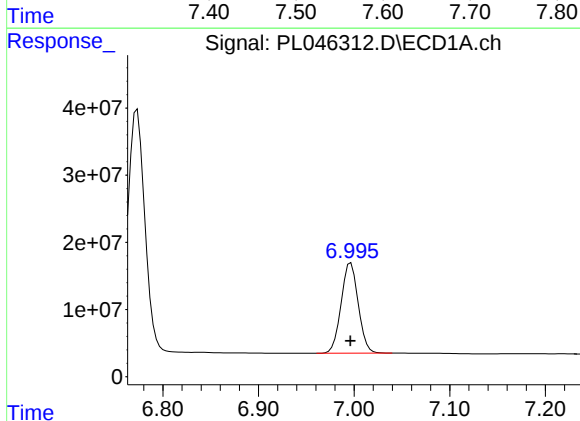


#21 Endrin ketone

R.T.: 6.997 min
Delta R.T.: 0.000 min
Response: 167520012
Conc: 18.12 ng/ml

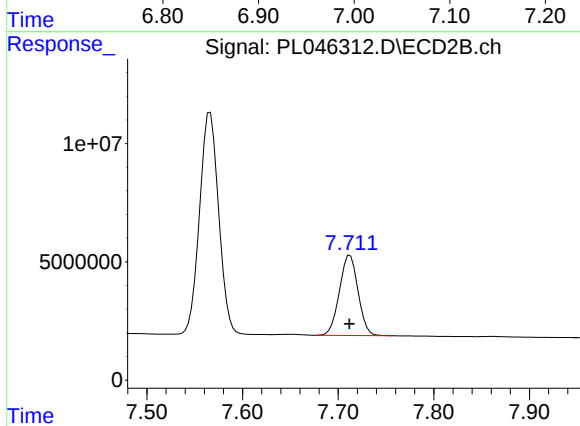

#21 Endrin ketone


R.T.: 7.713 min
Delta R.T.: 0.000 min
Response: 45848363
Conc: 18.45 ng/ml

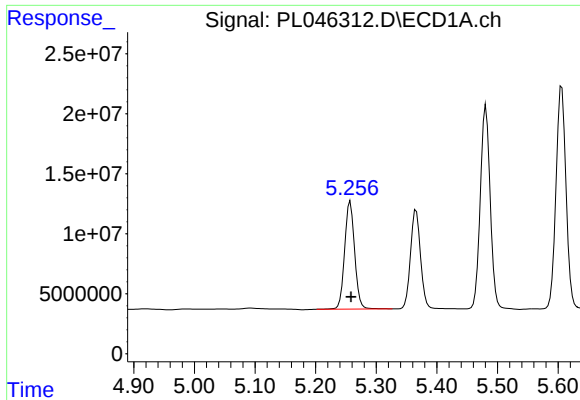

#25 Chlordane-3


R.T.: 5.257 min
Delta R.T.: -0.001 min
Response: 102784866
Conc: 92.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

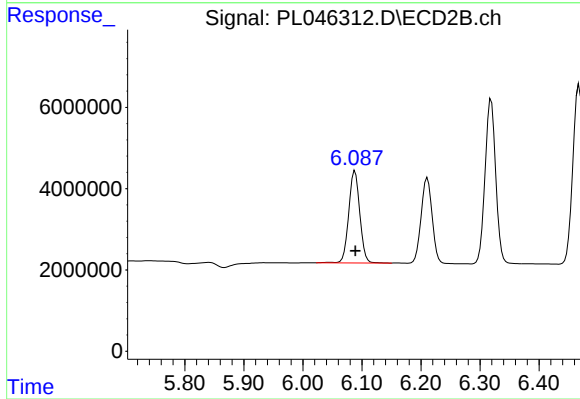


#25 Chlordane-3

R.T.: 6.088 min
Delta R.T.: 0.000 min
Response: 29494115
Conc: 77.36 ng/ml

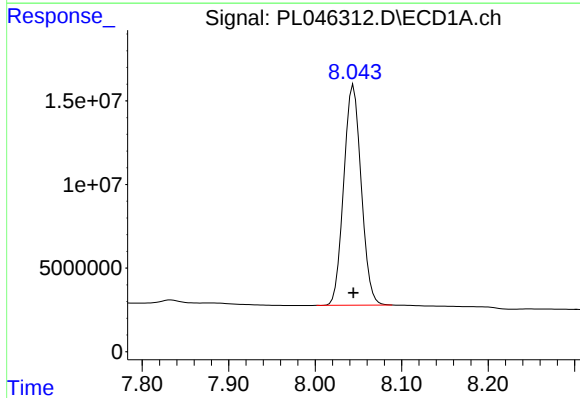

#28 Decachlorobiphenyl

R.T.: 8.044 min
Delta R.T.: 0.000 min
Response: 183973445
Conc: 21.87 ng/ml

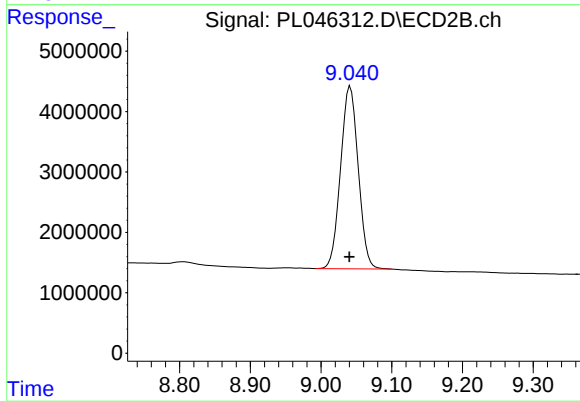

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.002 min
Response: 52448554
Conc: 22.62 ng/ml