

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
 Data File : PL046318.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 12:30
 Operator : AJ\SJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 13:15:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:15:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.982	793.0E6	229.5E6	101.433	102.174
28)	SA Decachlor...	8.045	9.043	805.3E6	216.8E6	96.616	93.282
Target Compounds							
23)	Chlordane-1	4.208	4.975	350.2E6	108.4E6	1029.553	1009.396
24)	Chlordane-2	4.701	5.443	369.9E6	110.1E6	993.778	969.255
25)	Chlordane-3	5.259	6.089	1170.2E6	388.2E6	1037.610	1031.405
26)	Chlordane-4	5.314	6.163	1072.5E6	460.7E6	1027.107	1015.788
27)	Chlordane-5	6.140	6.967	359.2E6	90936725	1044.283	1028.285


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
Data File : PL046318.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 12:30
Operator : AJ\SJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 13:15:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:15:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

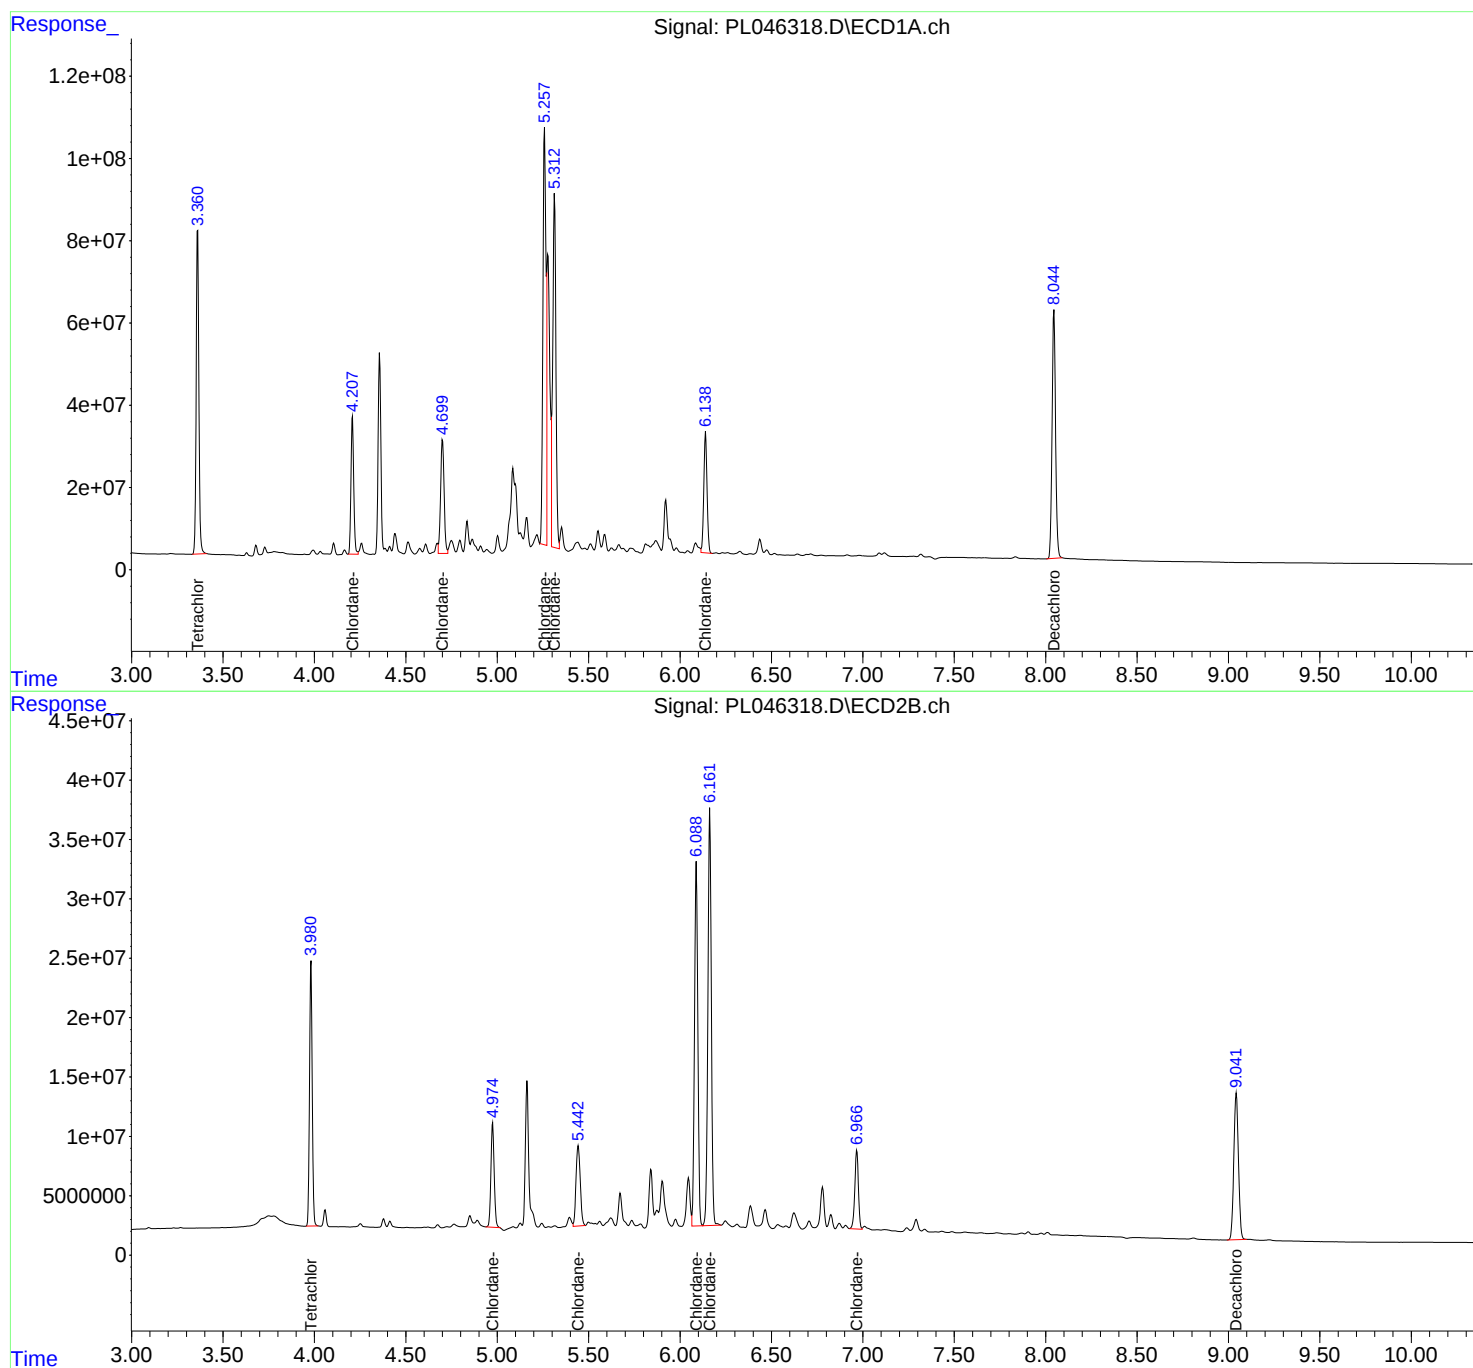


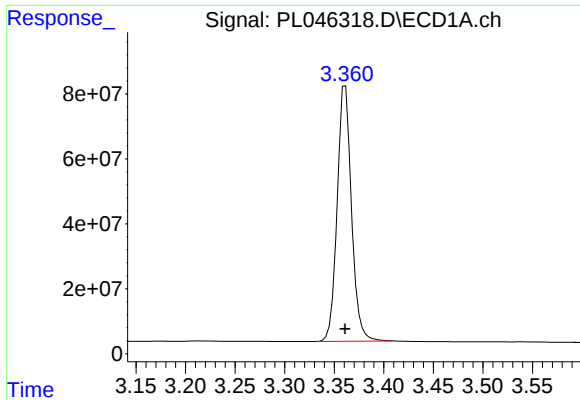

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: 0.000 min
Response: 792991248
Conc: 101.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

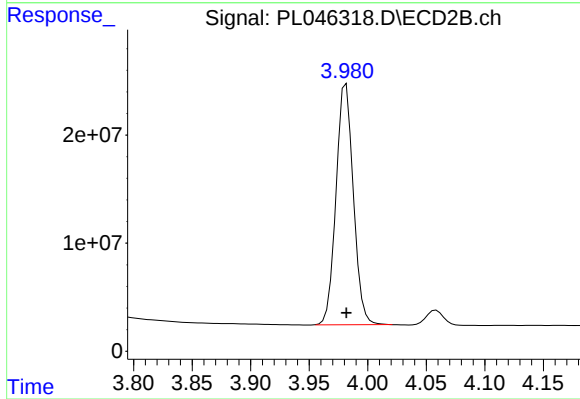


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 229471615
Conc: 102.17 ng/ml

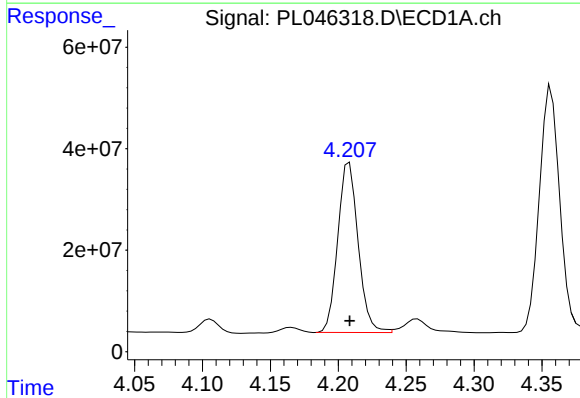


#23 Chlordane-1

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 350244680
Conc: 1029.55 ng/ml

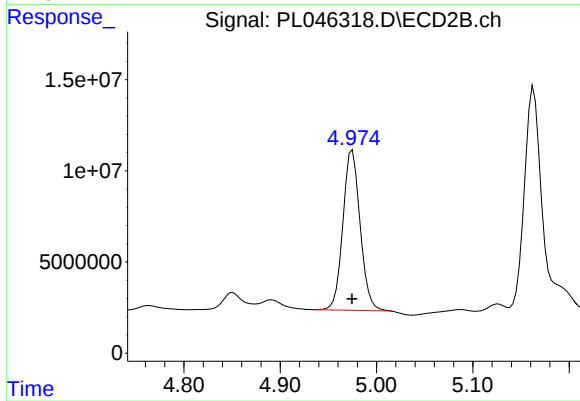

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 108357733
Conc: 1009.40 ng/ml

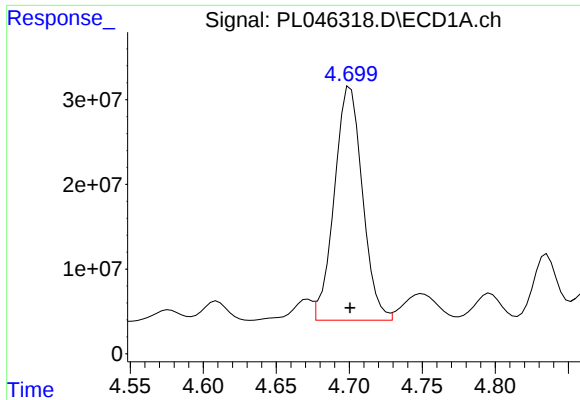

#24 Chlordane-2


R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 369942256
Conc: 993.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

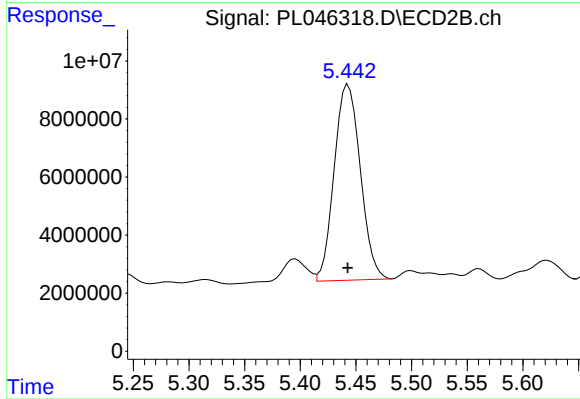


#24 Chlordane-2

R.T.: 5.443 min
Delta R.T.: 0.000 min
Response: 110084035
Conc: 969.26 ng/ml

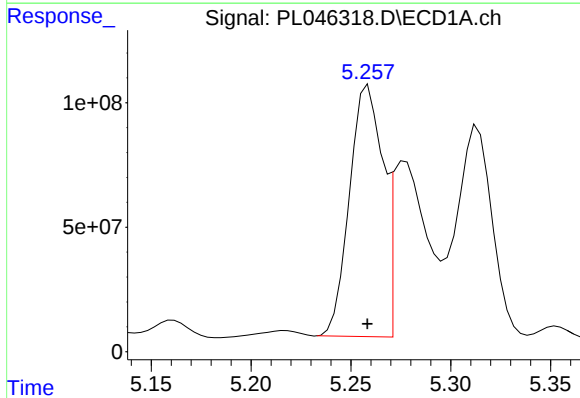


#25 Chlordane-3

R.T.: 5.259 min
Delta R.T.: 0.000 min
Response: 1170164080
Conc: 1037.61 ng/ml

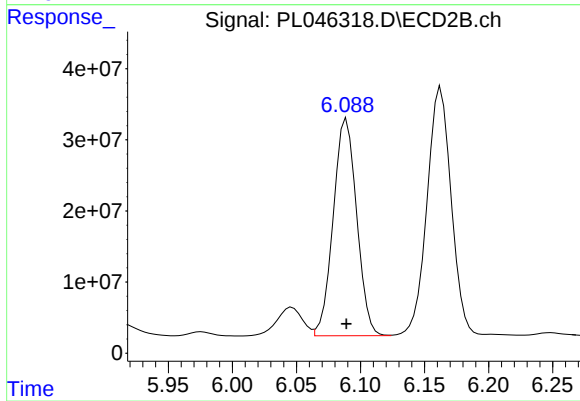

#25 Chlordane-3


R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 388215074
Conc: 1031.40 ng/ml

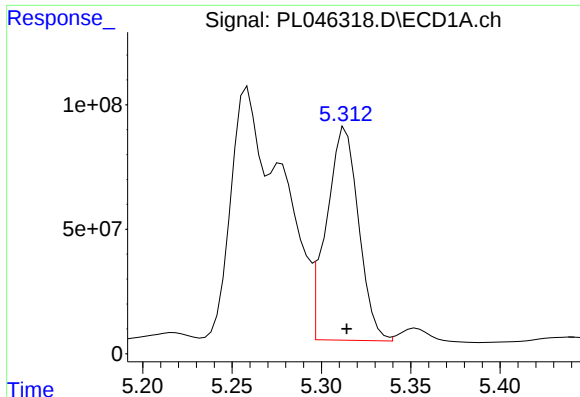

#26 Chlordane-4


R.T.: 5.314 min
Delta R.T.: 0.000 min
Response: 1072459419
Conc: 1027.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

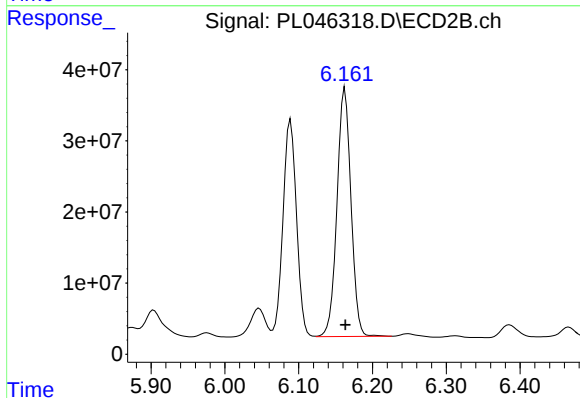


#26 Chlordane-4

R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 460679029
Conc: 1015.79 ng/ml

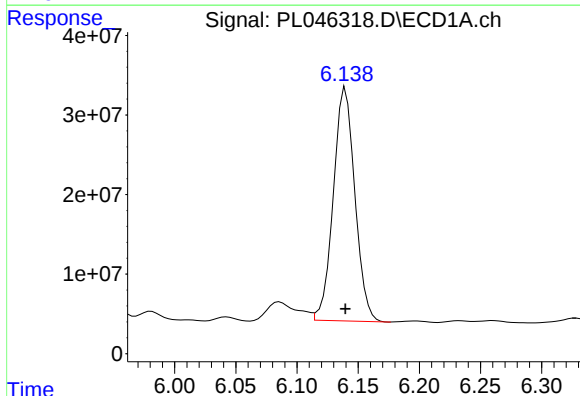


#27 Chlordane-5

R.T.: 6.140 min
Delta R.T.: 0.000 min
Response: 359165861
Conc: 1044.28 ng/ml

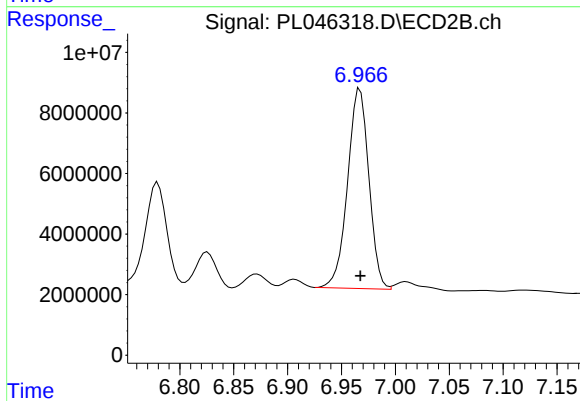

#27 Chlordane-5


R.T.: 6.967 min
Delta R.T.: 0.000 min
Response: 90936725
Conc: 1028.28 ng/ml

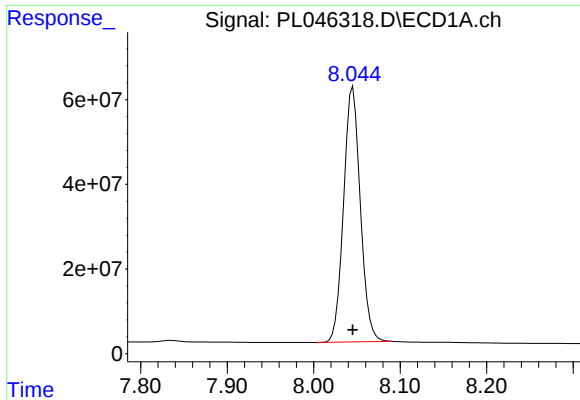

#28 Decachlorobiphenyl

R.T.: 8.045 min
Delta R.T.: 0.000 min
Response: 805314768
Conc: 96.62 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

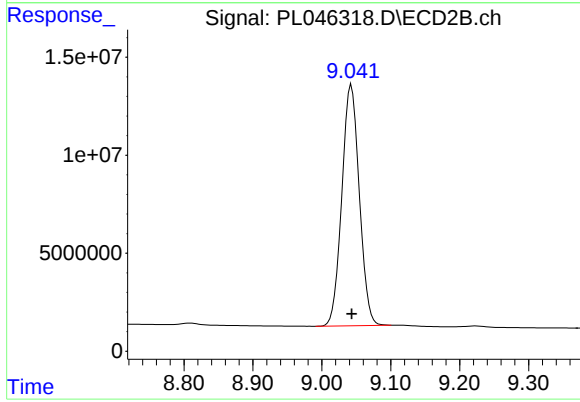

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 216835475
Conc: 93.28 ng/ml