

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
 Data File : PL046320.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 12:59
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 13:15:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:15:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.982	390.9E6	112.3E6	50.000	50.000
28)	SA Decachlor...	8.045	9.043	416.8E6	116.2E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.208	4.975	170.1E6	53674556	500.000	500.000
24)	Chlordane-2	4.701	5.443	186.1E6	56787941	500.000	500.000
25)	Chlordane-3	5.258	6.089	563.9E6	188.2E6	500.000	500.000
26)	Chlordane-4	5.314	6.163	522.1E6	226.8E6	500.000	500.000
27)	Chlordane-5	6.139	6.967	172.0E6	44217670	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
Data File : PL046320.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 12:59
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 13:15:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:15:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

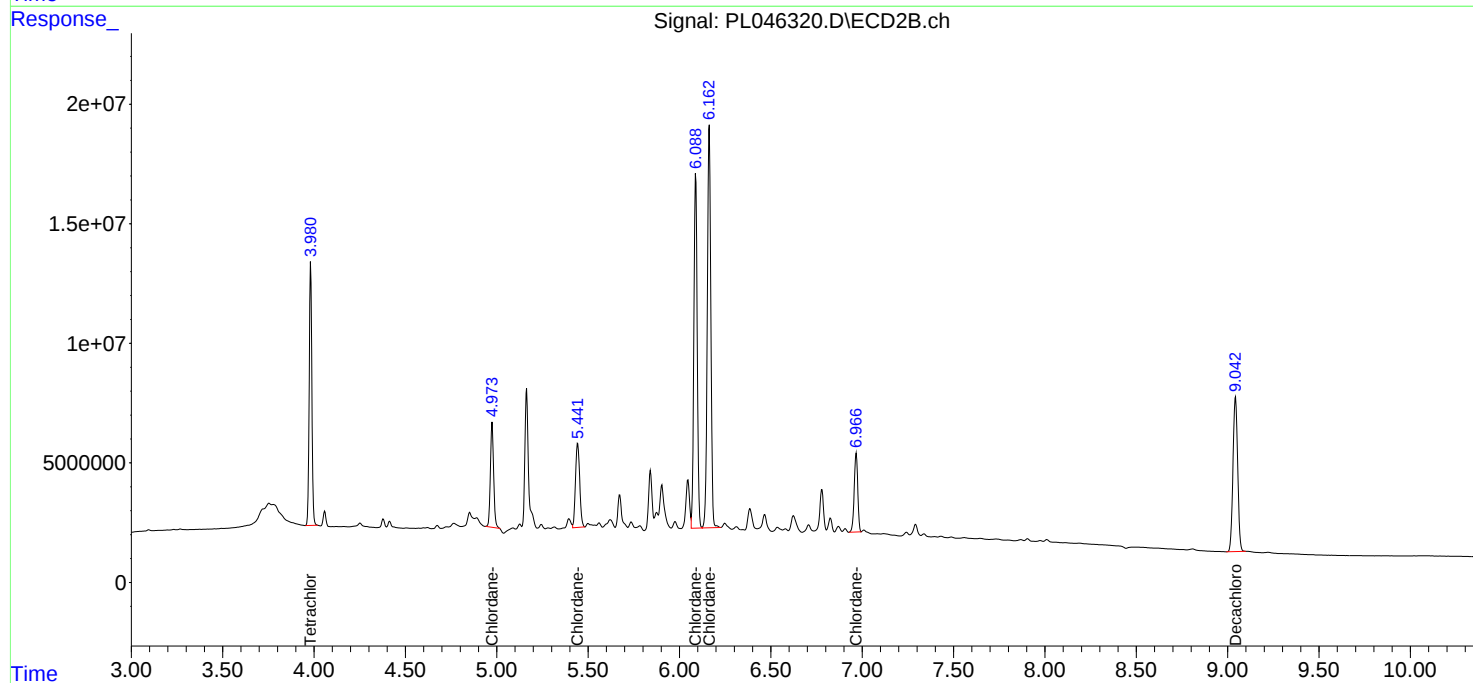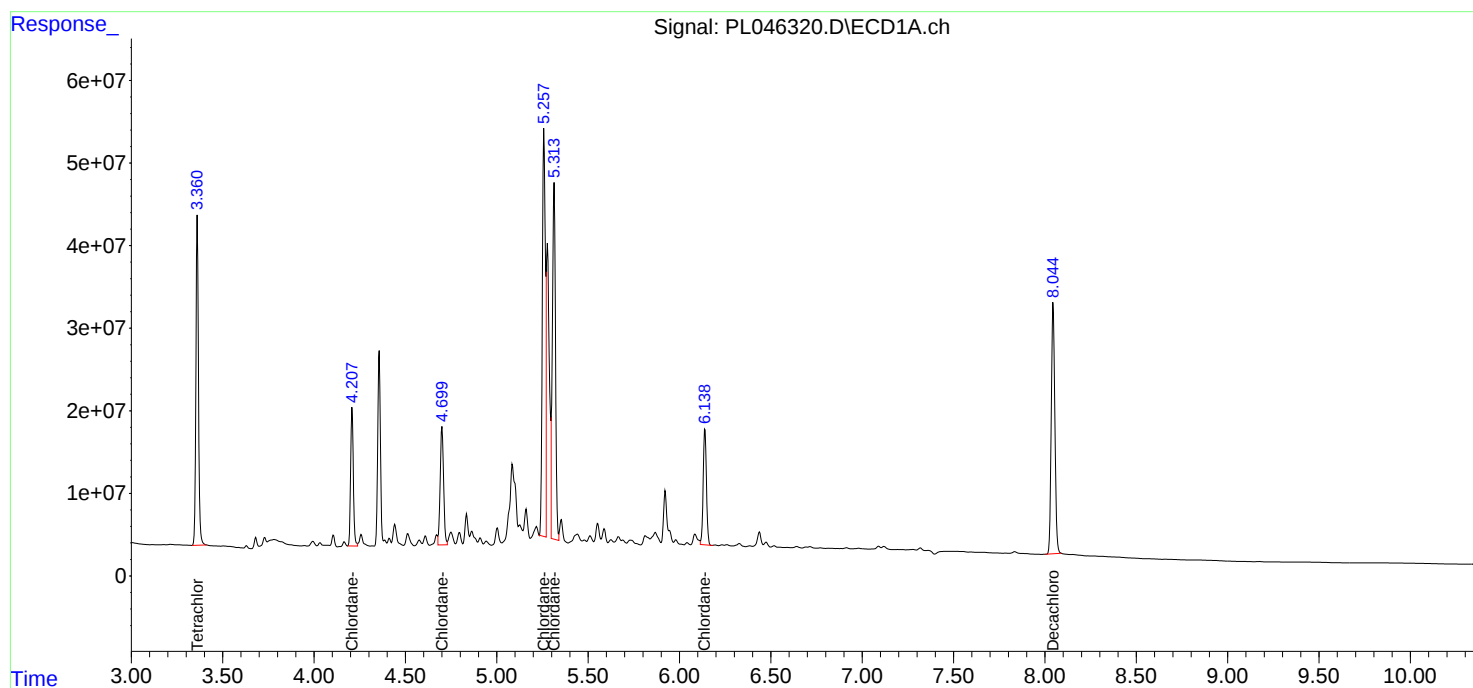


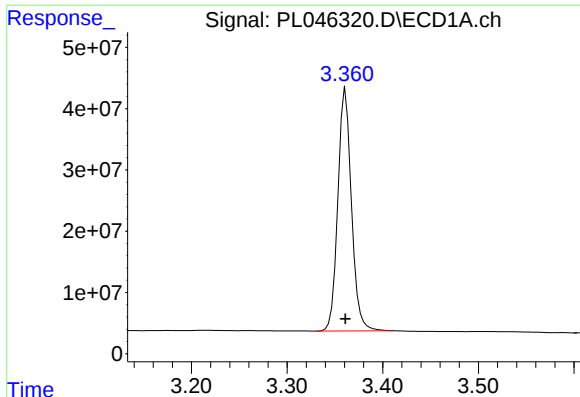

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: 0.000 min
Response: 390892638
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

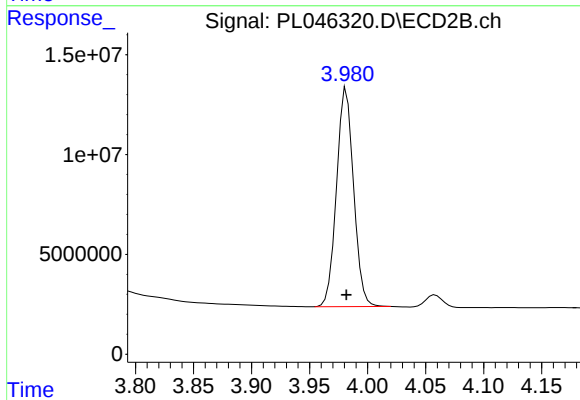


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 112294336
Conc: 50.00 ng/ml

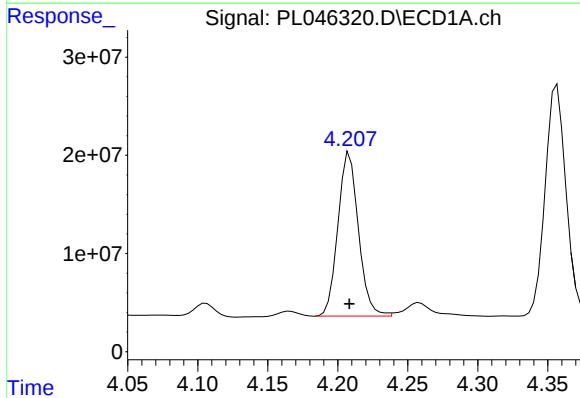


#23 Chlordane-1

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 170095554
Conc: 500.00 ng/ml

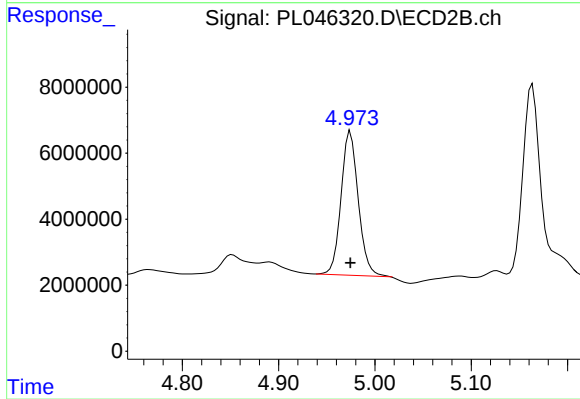

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 53674556
Conc: 500.00 ng/ml

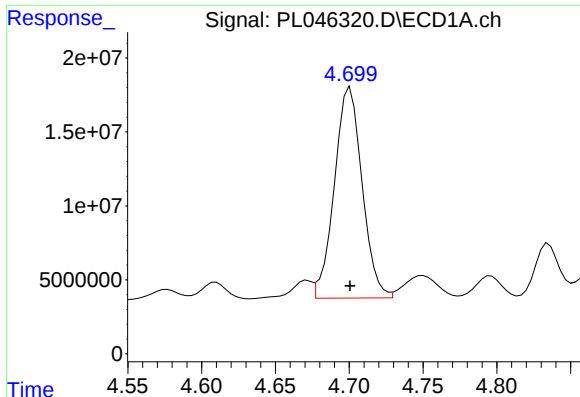

#24 Chlordane-2


R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 186129193
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

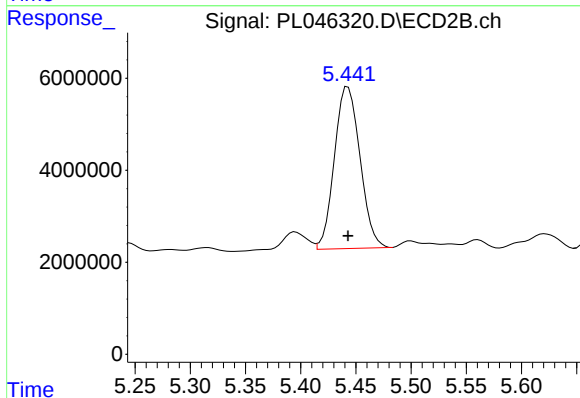


#24 Chlordane-2

R.T.: 5.443 min
Delta R.T.: 0.000 min
Response: 56787941
Conc: 500.00 ng/ml

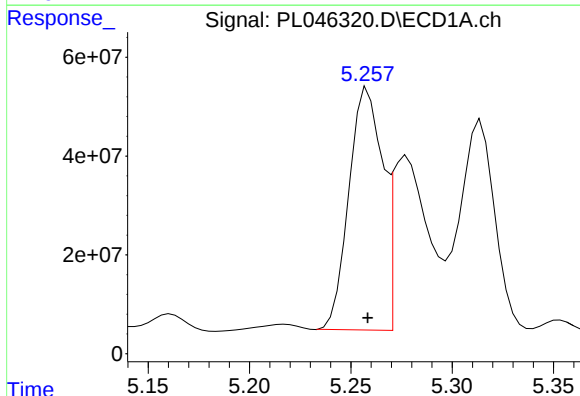


#25 Chlordane-3

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 563874476
Conc: 500.00 ng/ml

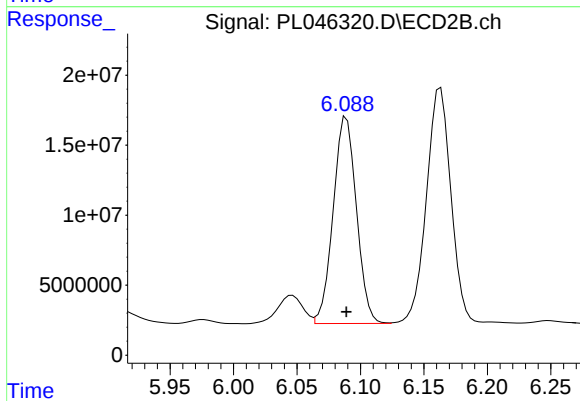

#25 Chlordane-3


R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 188197270
Conc: 500.00 ng/ml

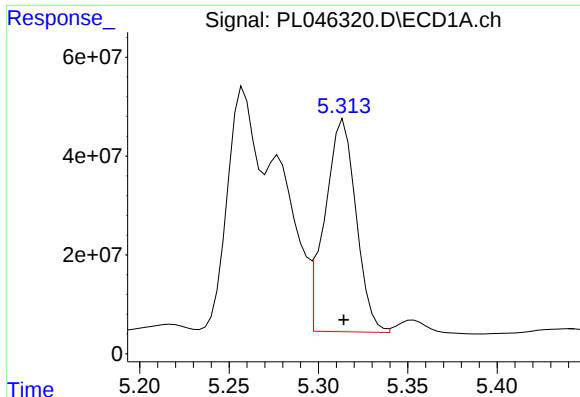

#26 Chlordane-4


R.T.: 5.314 min
Delta R.T.: 0.000 min
Response: 522077503
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

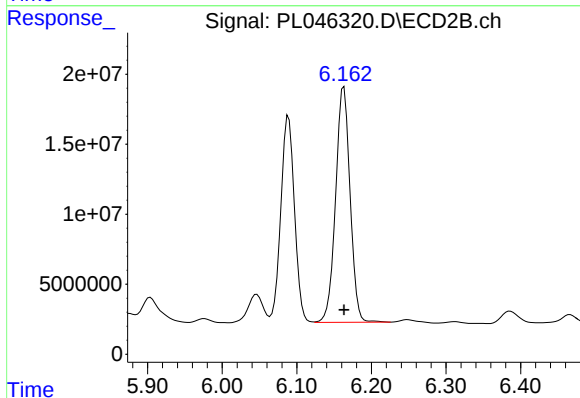


#26 Chlordane-4

R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 226759500
Conc: 500.00 ng/ml

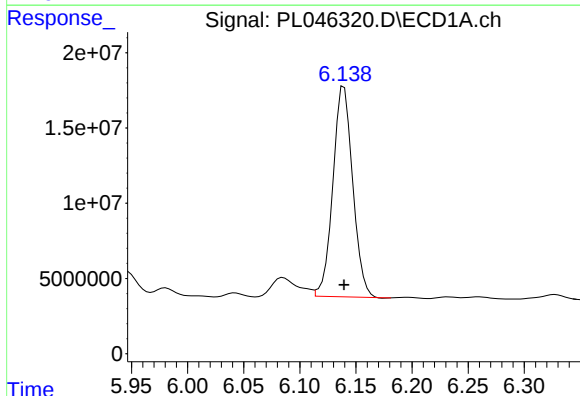


#27 Chlordane-5

R.T.: 6.139 min
Delta R.T.: 0.000 min
Response: 171967752
Conc: 500.00 ng/ml

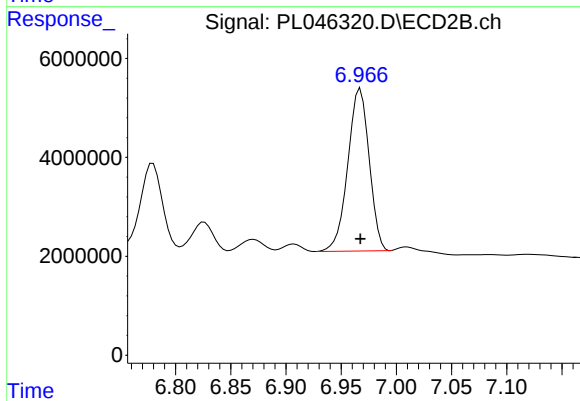

#27 Chlordane-5

R.T.: 6.967 min
Delta R.T.: 0.000 min
Response: 44217670
Conc: 500.00 ng/ml

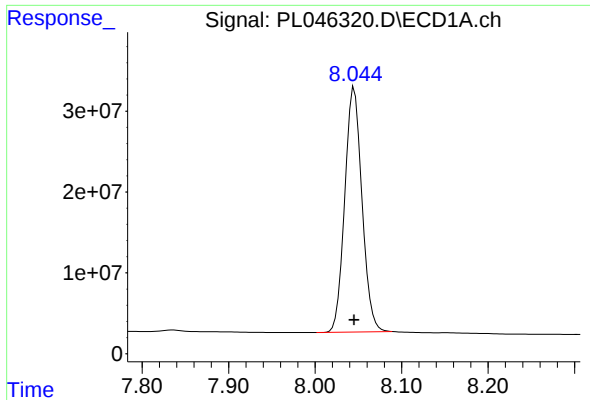

#28 Decachlorobiphenyl


R.T.: 8.045 min

Delta R.T.: 0.000 min

Response: 416761081

Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

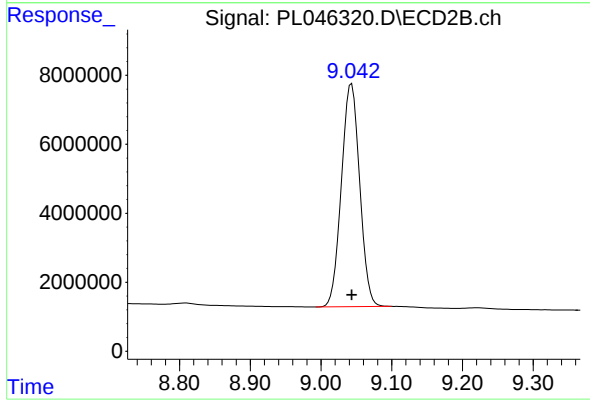

#28 Decachlorobiphenyl

R.T.: 9.043 min

Delta R.T.: 0.000 min

Response: 116225376

Conc: 50.00 ng/ml