

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
 Data File : PL046321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 13:13
 Operator : AJ\SJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 13:29:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:15:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.982	188.8E6	55322314	23.865	24.299
28)	SA Decachlor...	8.045	9.043	212.1E6	60321389	25.866	26.797
Target Compounds							
23)	Chlordane-1	4.208	4.975	81809959	26947813	236.173	249.208
24)	Chlordane-2	4.700	5.443	94075253	29180171	252.532	260.548
25)	Chlordane-3	5.258	6.089	268.9E6	91334612	232.394	238.086
26)	Chlordane-4	5.314	6.162	252.7E6	111.7E6	237.300	243.925
27)	Chlordane-5	6.140	6.967	81094154	21916371	229.753	242.629



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
Data File : PL046321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 13:13
Operator : AJ\SJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 13:29:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:15:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

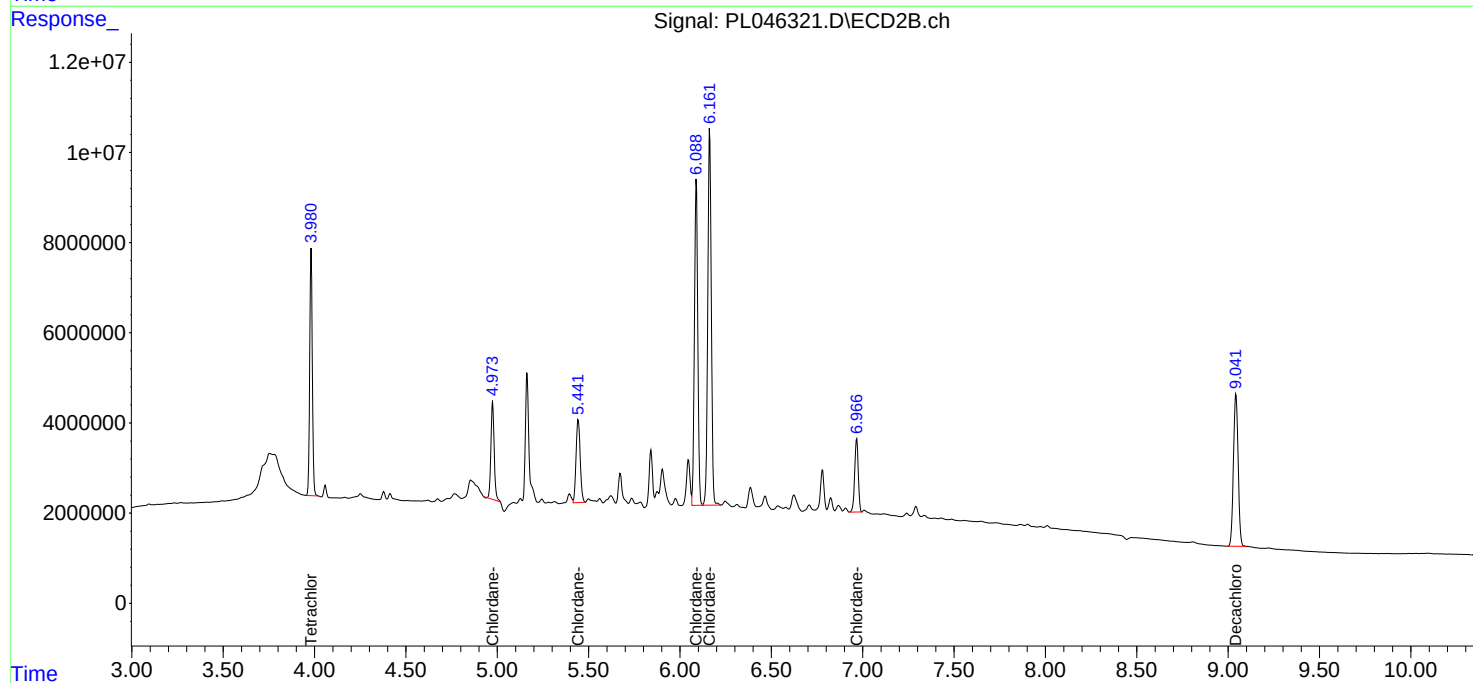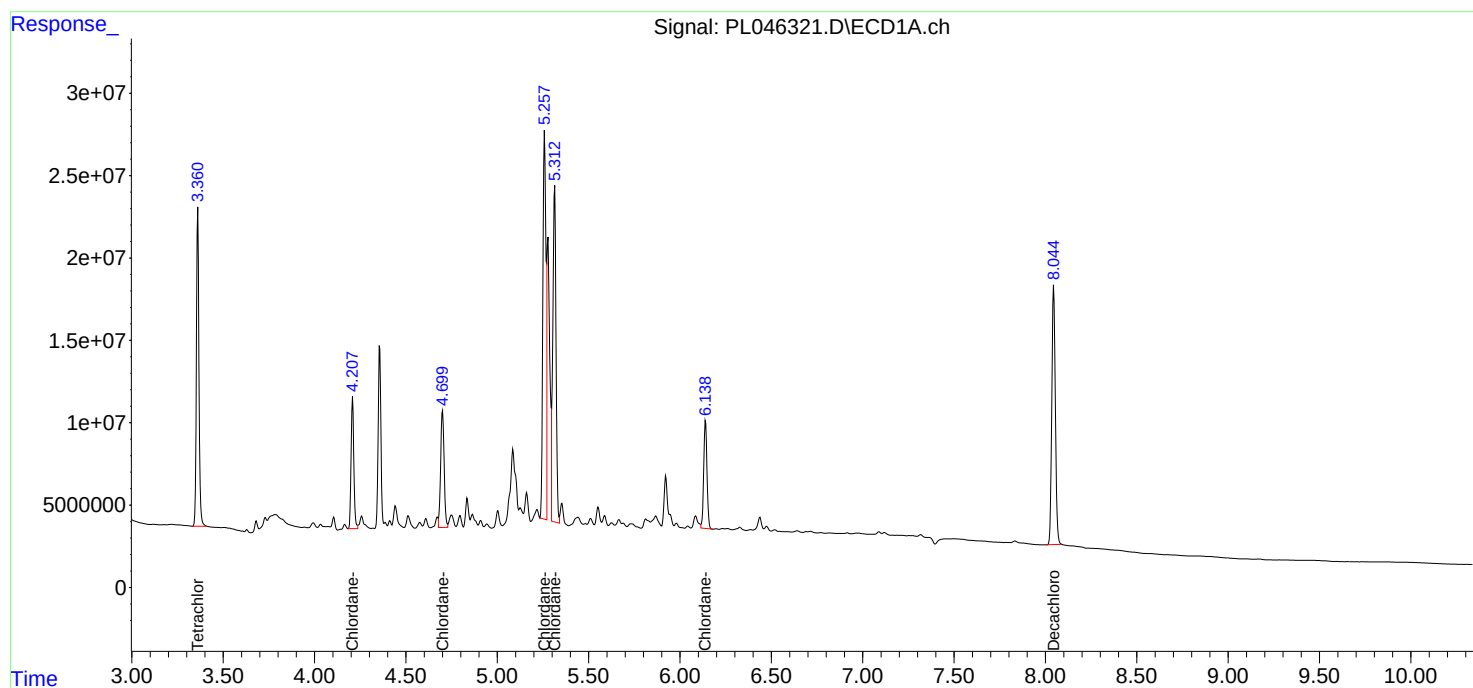


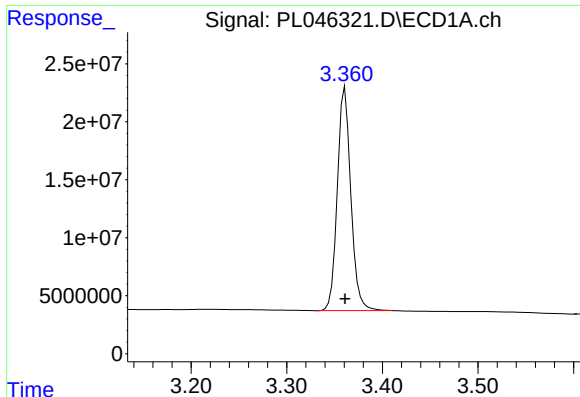

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: 0.000 min
Response: 188785417
Conc: 23.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

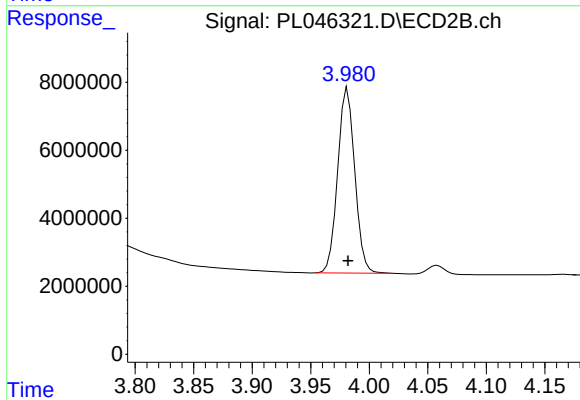


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 55322314
Conc: 24.30 ng/ml

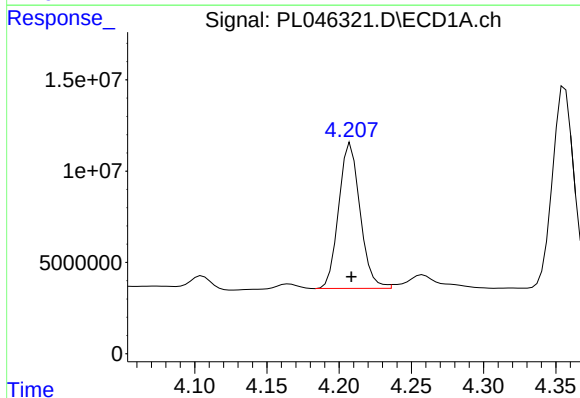


#23 Chlordane-1

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 81809959
Conc: 236.17 ng/ml

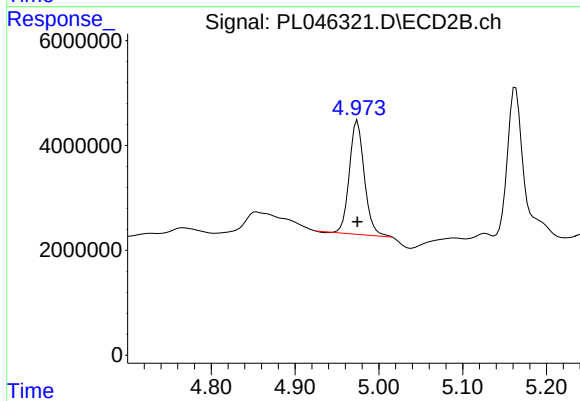

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 26947813
Conc: 249.21 ng/ml

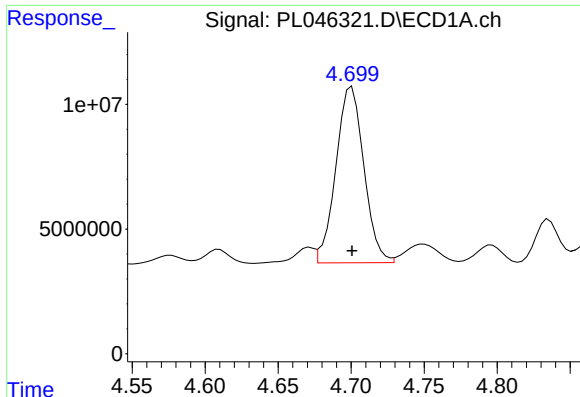

#24 Chlordane-2


R.T.: 4.700 min
Delta R.T.: 0.000 min
Response: 94075253
Conc: 252.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

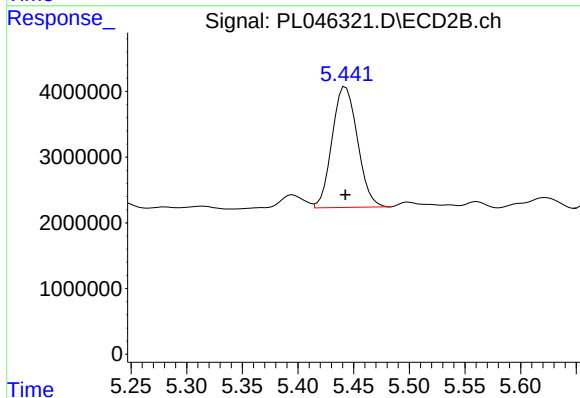


#24 Chlordane-2

R.T.: 5.443 min
Delta R.T.: 0.000 min
Response: 29180171
Conc: 260.55 ng/ml

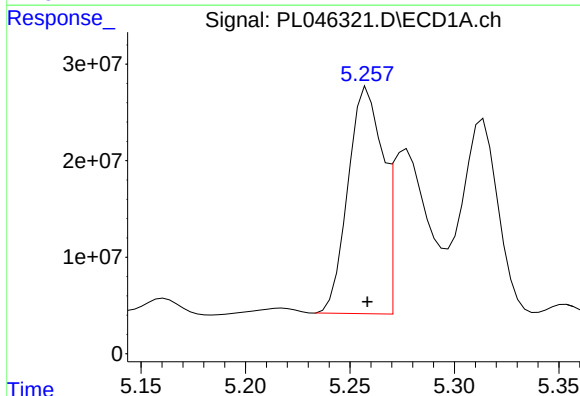


#25 Chlordane-3

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 268863314
Conc: 232.39 ng/ml

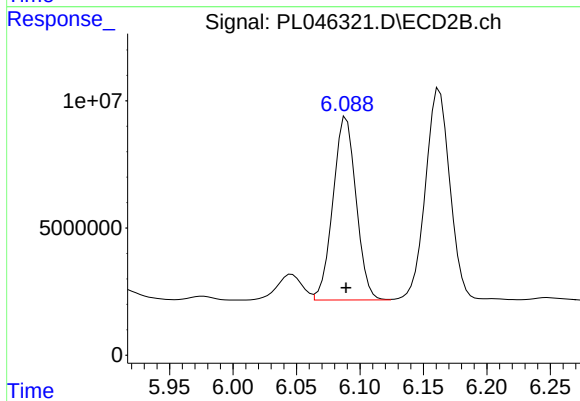

#25 Chlordane-3


R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 91334612
Conc: 238.09 ng/ml

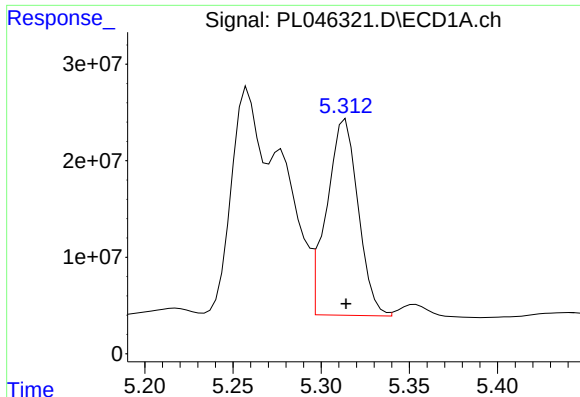

#26 Chlordane-4


R.T.: 5.314 min
Delta R.T.: 0.000 min
Response: 252717134
Conc: 237.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

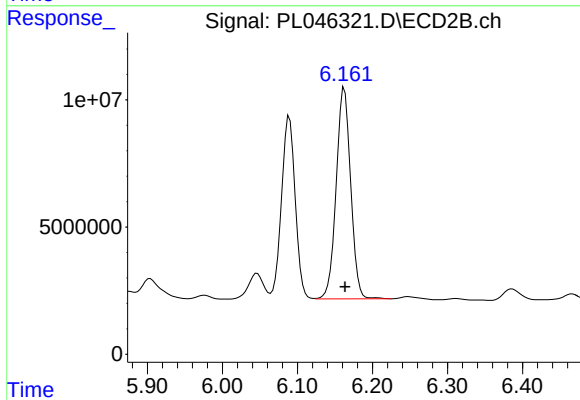


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 111675004
Conc: 243.93 ng/ml

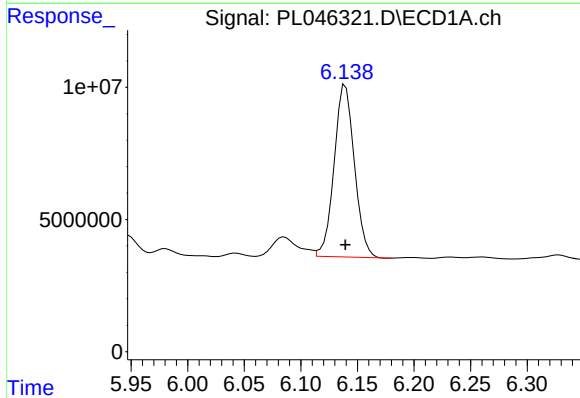


#27 Chlordane-5

R.T.: 6.140 min
Delta R.T.: 0.000 min
Response: 81094154
Conc: 229.75 ng/ml

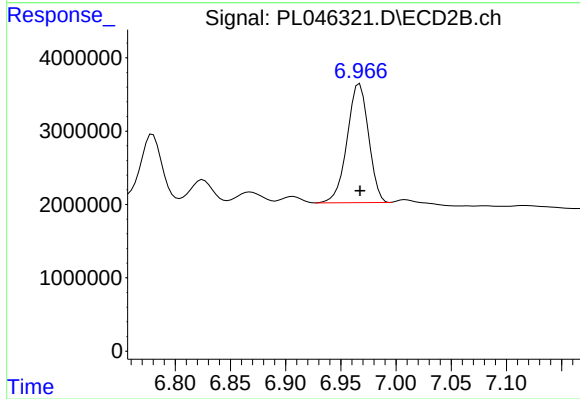

#27 Chlordane-5


R.T.: 6.967 min
Delta R.T.: 0.000 min
Response: 21916371
Conc: 242.63 ng/ml

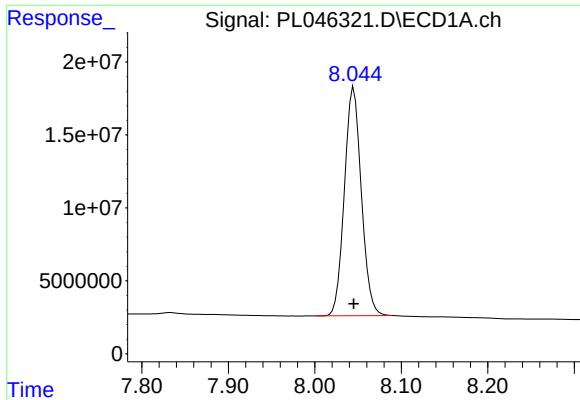

#28 Decachlorobiphenyl

R.T.: 8.045 min
Delta R.T.: 0.000 min
Response: 212070745
Conc: 25.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

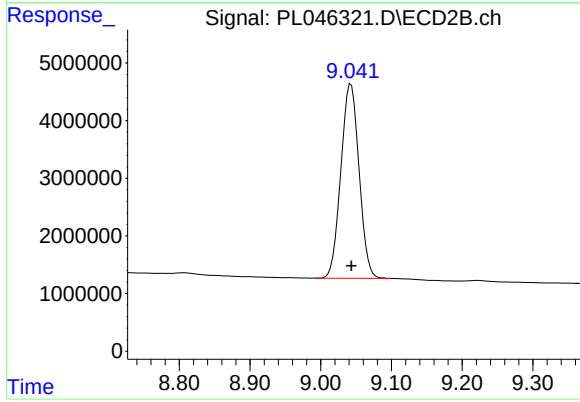

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 60321389
Conc: 26.80 ng/ml