

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
 Data File : PL046319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 12:45
 Operator : AJ\SJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 13:15:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:15:00 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.982	598.8E6	171.7E6	76.596	76.463
28)	SA Decachlor...	8.046	9.043	615.6E6	169.5E6	73.857	72.930
Target Compounds							
23)	Chlordane-1	4.208	4.975	261.6E6	81521028	768.893	759.401
24)	Chlordane-2	4.701	5.443	281.5E6	84244506	756.298	741.746
25)	Chlordane-3	5.259	6.089	879.7E6	289.7E6	780.011	769.640
26)	Chlordane-4	5.314	6.163	808.7E6	344.5E6	774.518	759.522
27)	Chlordane-5	6.140	6.967	266.8E6	68710537	775.842	776.958



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
Data File : PL046319.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 12:45
Operator : AJ\SJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 13:15:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:15:00 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

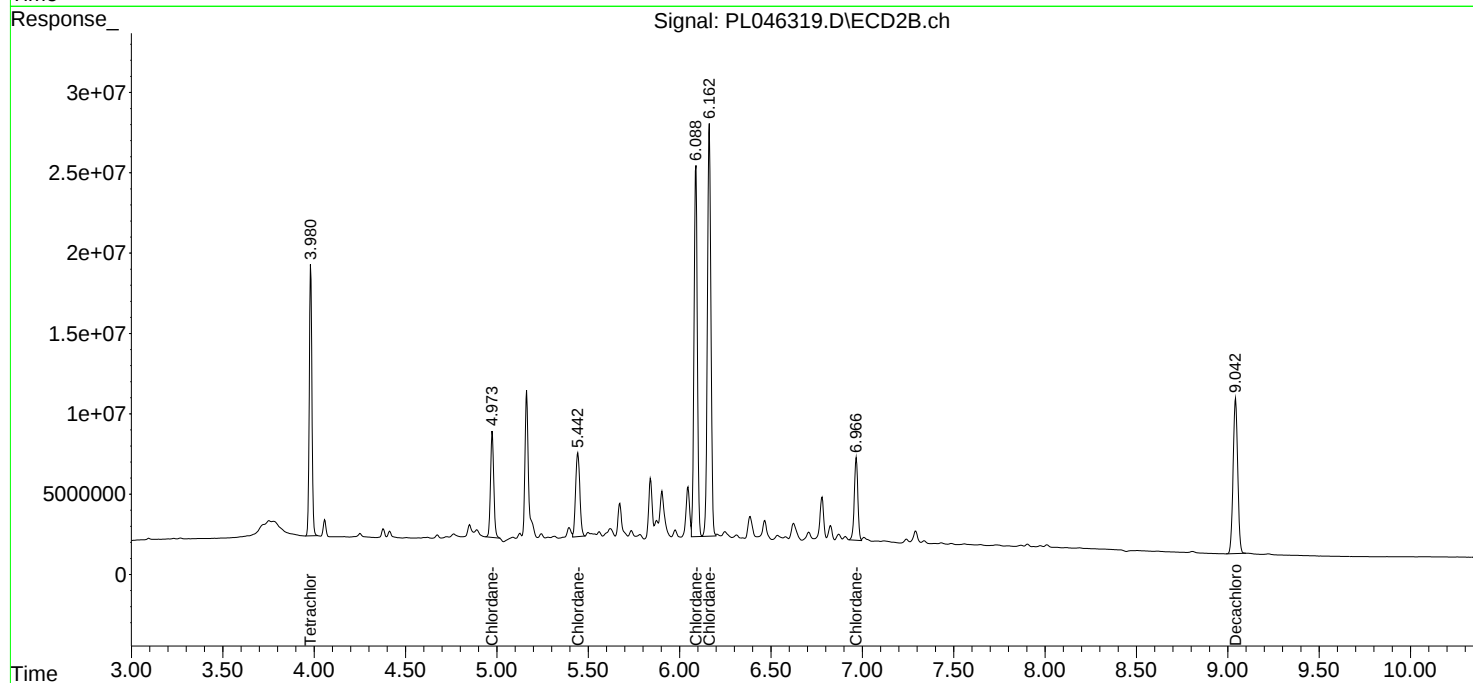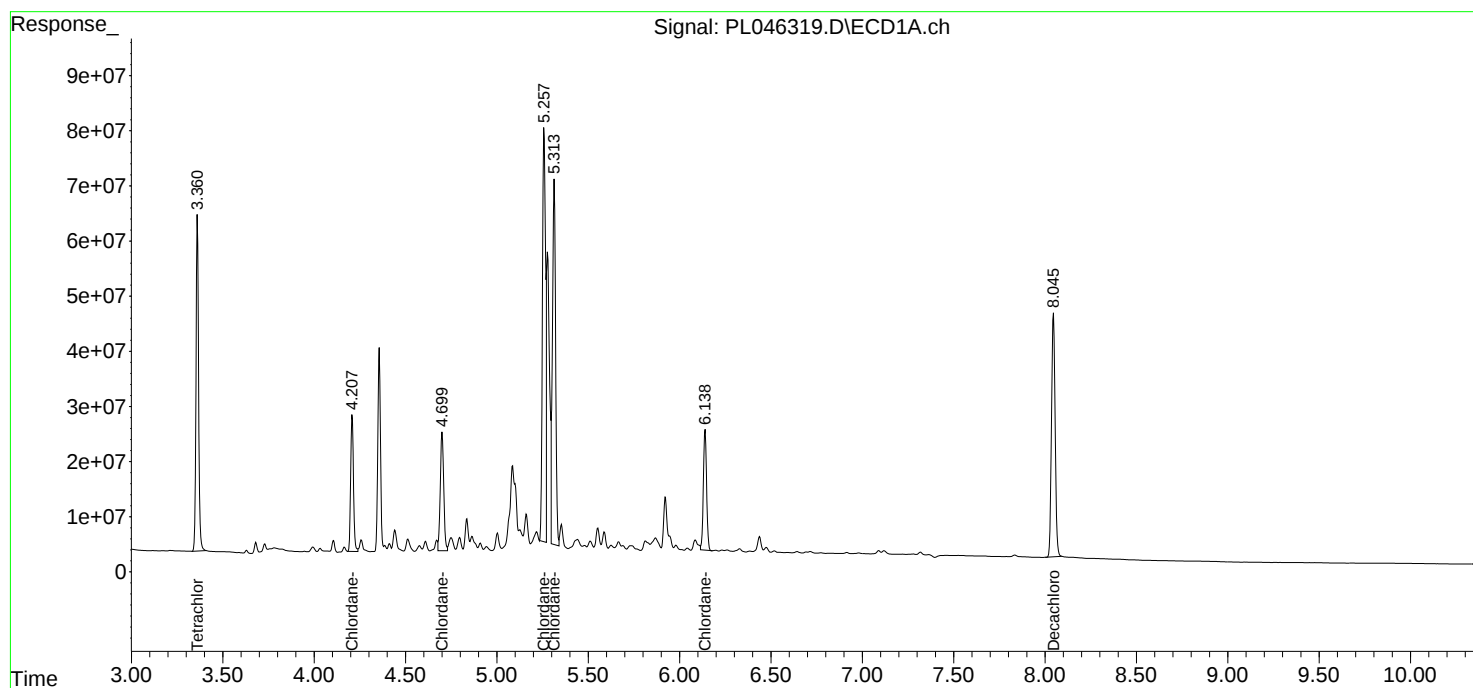


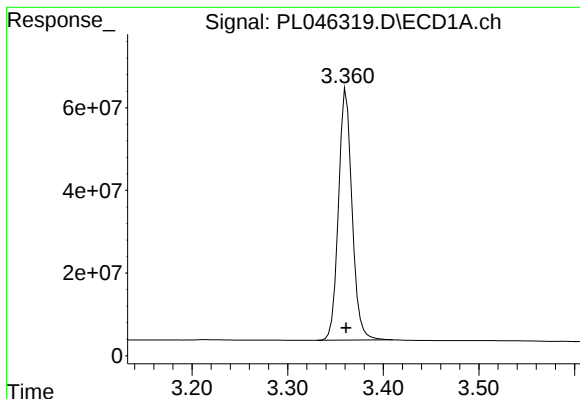

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: 0.000 min
Response: 598815301
Conc: 76.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

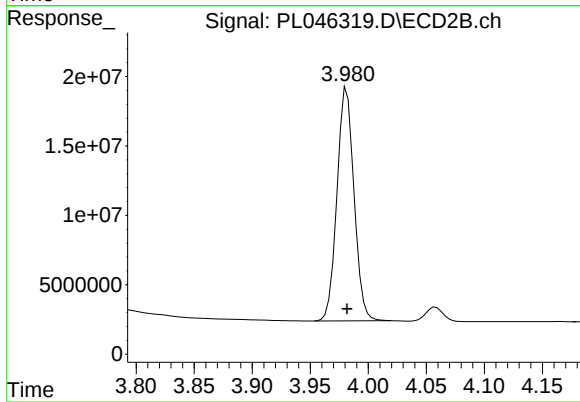


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 171726688
Conc: 76.46 ng/ml

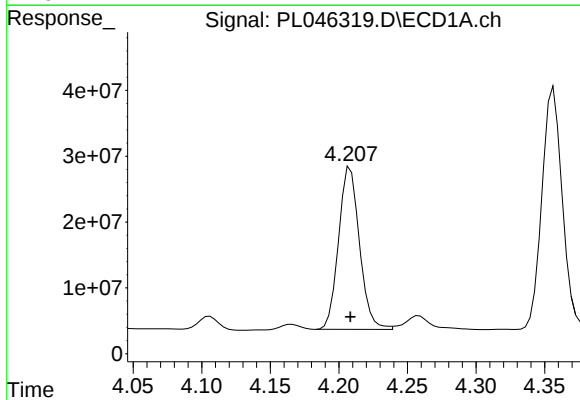


#23 Chlordane-1

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 261570483
Conc: 768.89 ng/ml

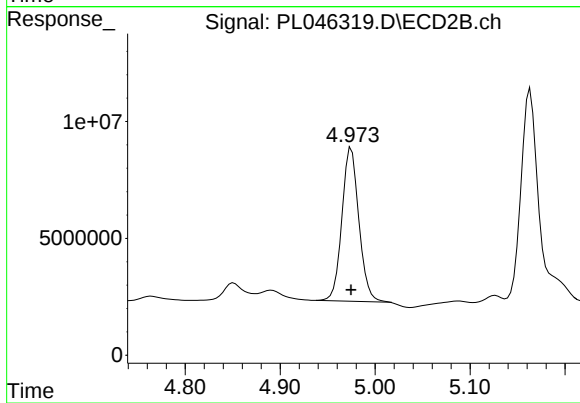

#23 Chlordane-1


R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 81521028
Conc: 759.40 ng/ml

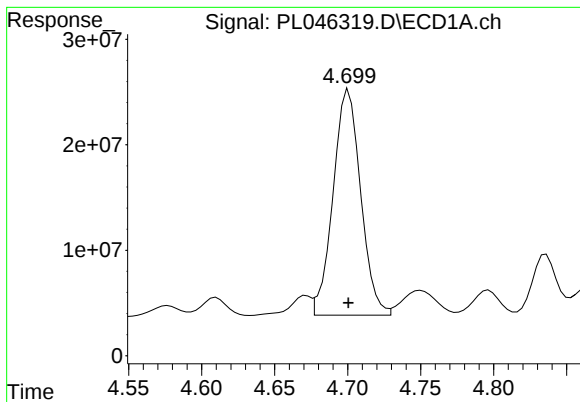

#24 Chlordane-2


R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 281538360
Conc: 756.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

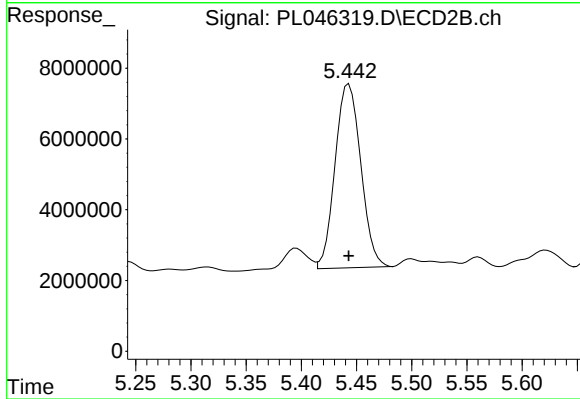


#24 Chlordane-2

R.T.: 5.443 min
Delta R.T.: 0.000 min
Response: 84244506
Conc: 741.75 ng/ml

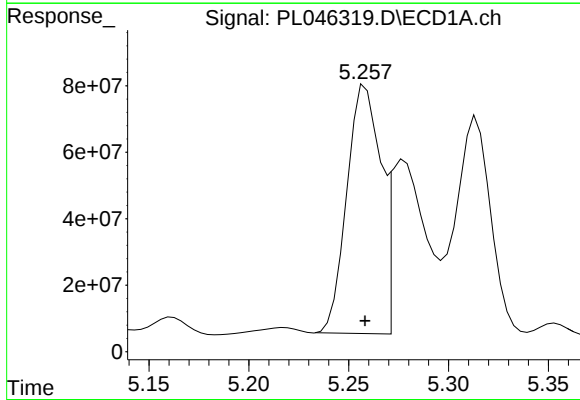


#25 Chlordane-3

R.T.: 5.259 min
Delta R.T.: 0.000 min
Response: 879656441
Conc: 780.01 ng/ml

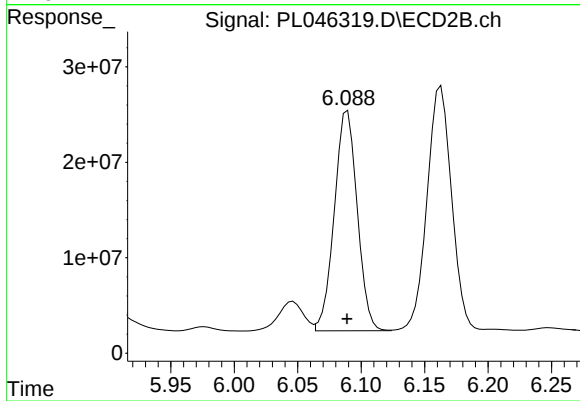

#25 Chlordane-3


R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 289688366
Conc: 769.64 ng/ml

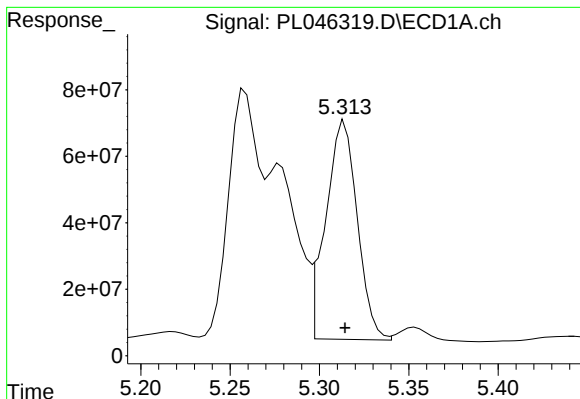

#26 Chlordane-4


R.T.: 5.314 min
Delta R.T.: 0.000 min
Response: 808716684
Conc: 774.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

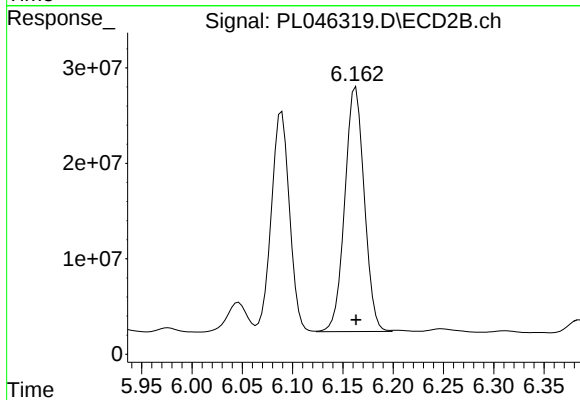


#26 Chlordane-4

R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 344457692
Conc: 759.52 ng/ml

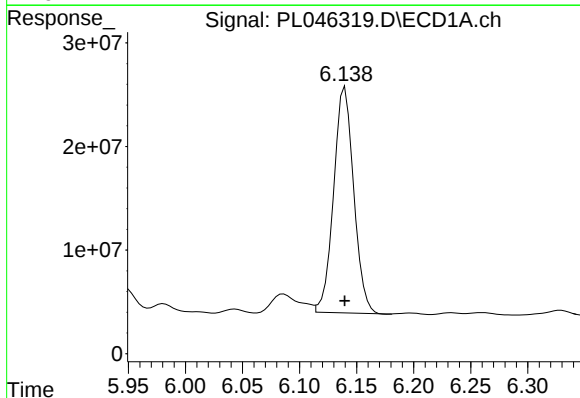


#27 Chlordane-5

R.T.: 6.140 min
Delta R.T.: 0.000 min
Response: 266839449
Conc: 775.84 ng/ml

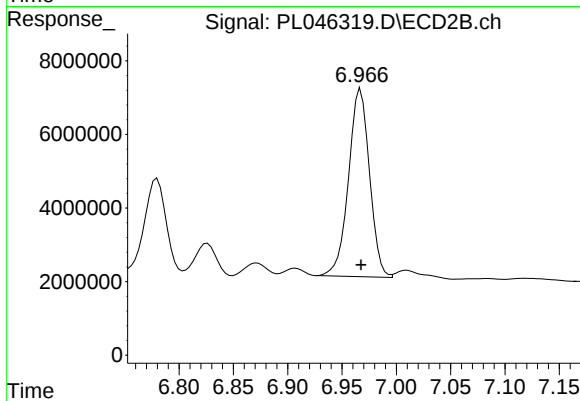

#27 Chlordane-5


R.T.: 6.967 min
Delta R.T.: 0.000 min
Response: 68710537
Conc: 776.96 ng/ml

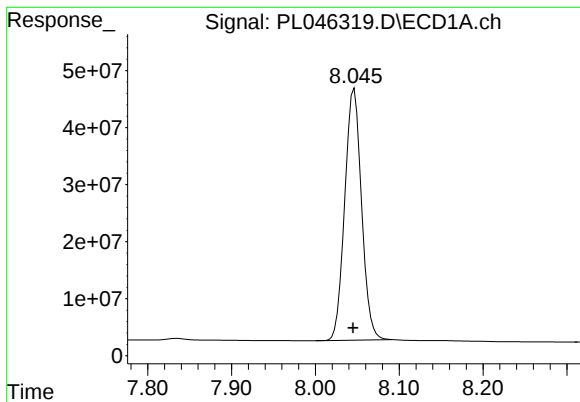

#28 Decachlorobiphenyl

R.T.: 8.046 min
Delta R.T.: 0.001 min
Response: 615617322
Conc: 73.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

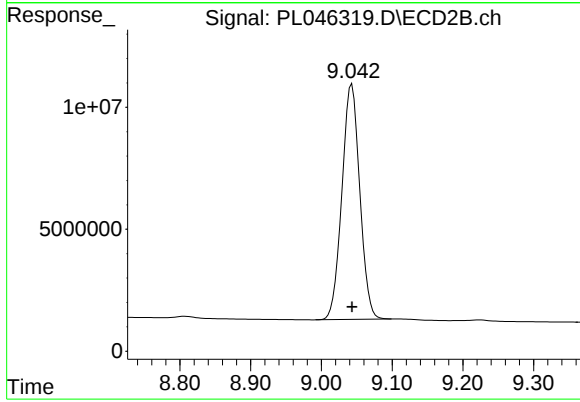

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 169525428
Conc: 72.93 ng/ml