

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
 Data File : PL046322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 13:27
 Operator : AJ\SJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Manual Integrations
 APPROVED

Sohil
 3/25/2019 9:37:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 13:38:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:30:23 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.981	38124220	11502561	4.875	5.088
28)	SA Decachlor...	8.046	9.043	49717677	13805587	6.012	6.025
Target Compounds							
23)	Chlordane-1	4.208	4.973	15752004	5444632	46.111	50.391m
24)	Chlordane-2	4.700	5.442	20160443	6566979	53.981	58.024
25)	Chlordane-3	5.258	6.089	51106244	19506960	44.966	51.463
26)	Chlordane-4	5.314	6.162	48226264	24347489	45.867	53.506
27)	Chlordane-5	6.139	6.967	16153567	4526851	46.711	50.487

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
Data File : PL046322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 13:27
Operator : AJ\SJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Sohil
3/25/2019 9:37:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 13:38:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:30:23 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

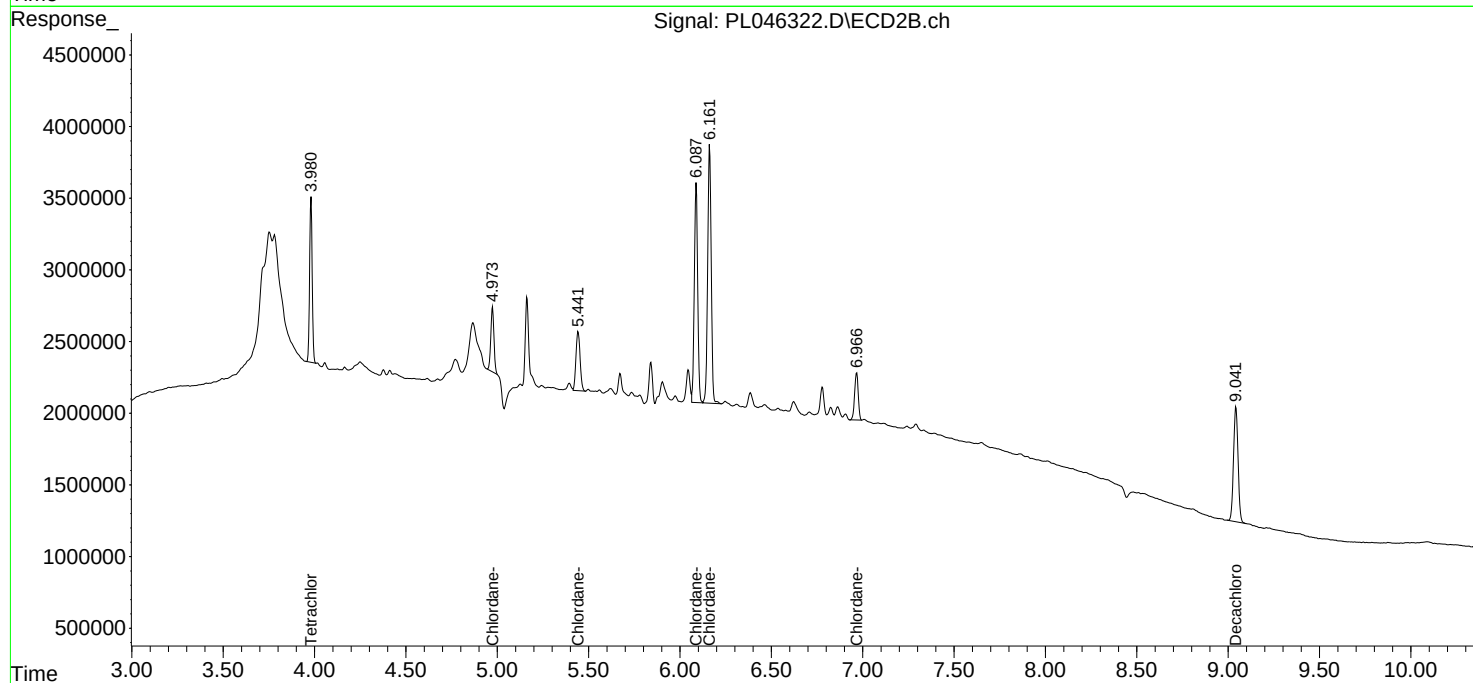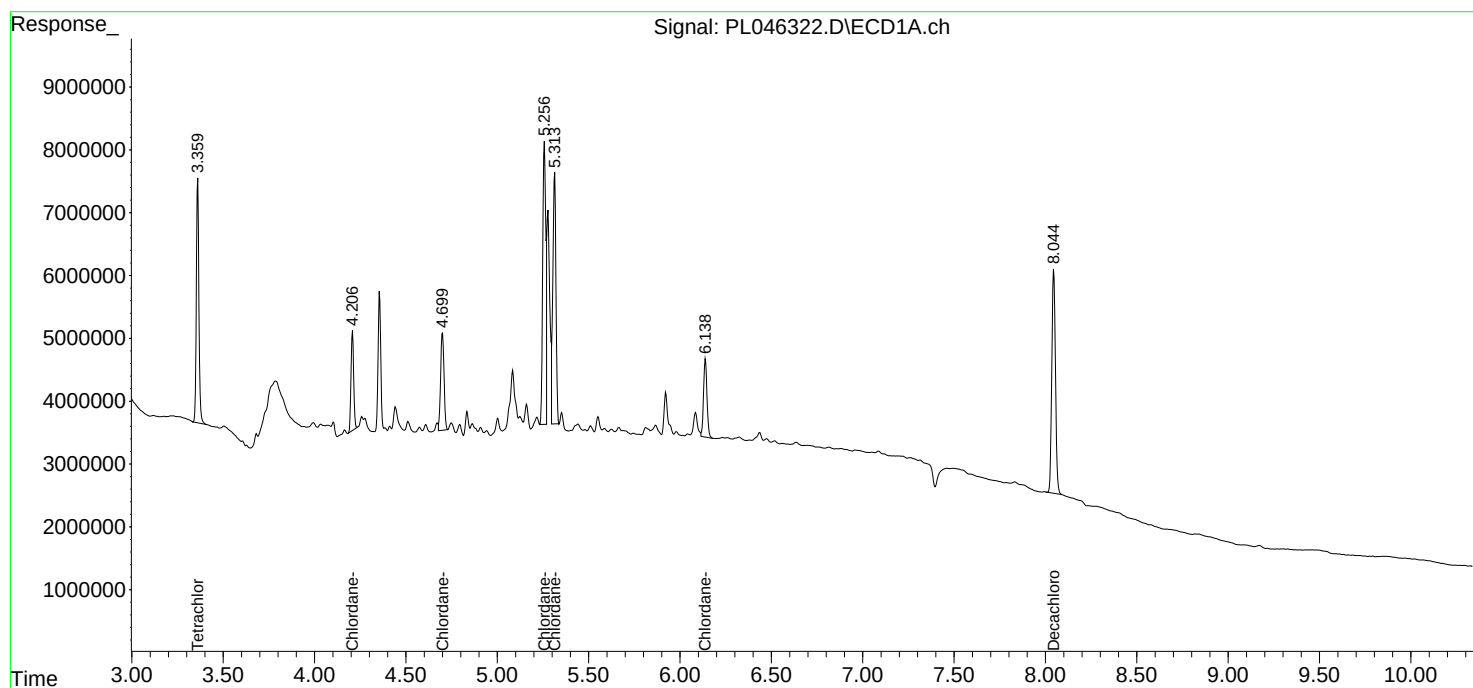

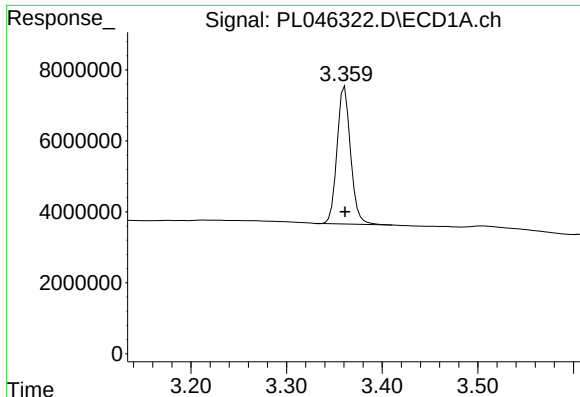


#1 Tetrachloro-m-xylene

R.T.: 3.361 min
Delta R.T.: 0.000 min
Response: 38124220
Conc: 4.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Sohil
3/25/2019 9:37:46 AM

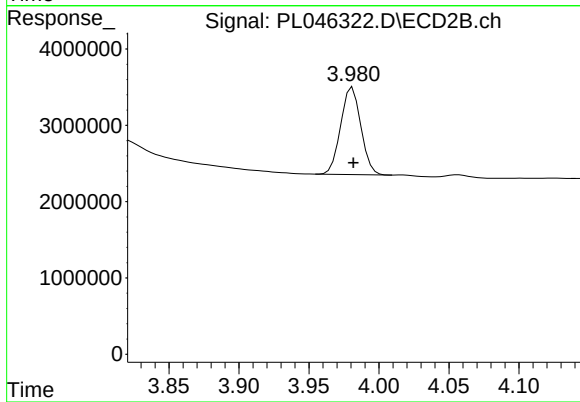


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 11502561
Conc: 5.09 ng/ml

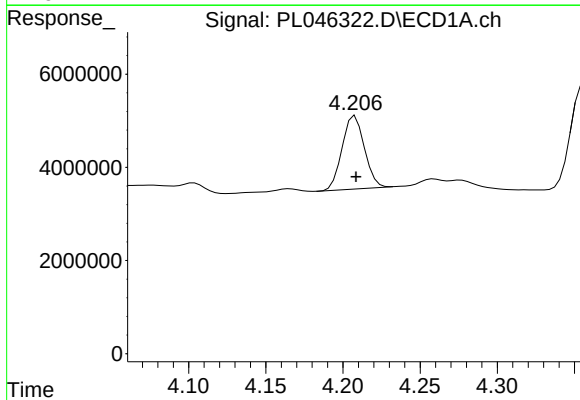


#23 Chlordane-1

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 15752004
Conc: 46.11 ng/ml

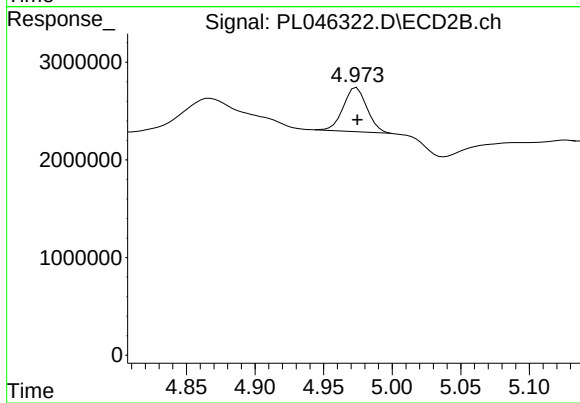

#23 Chlordane-1

R.T.: 4.973 min
Delta R.T.: -0.002 min
Response: 5444632
Conc: 50.39 ng/ml m

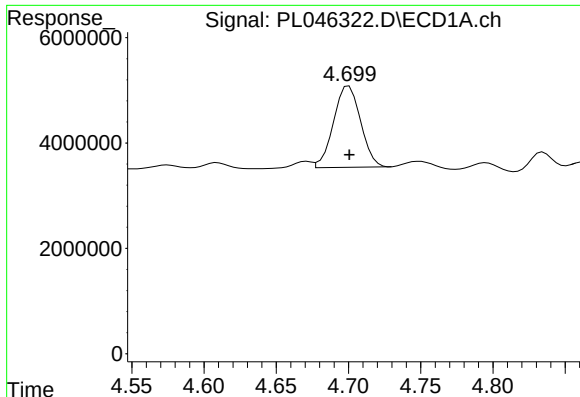


#24 Chlordane-2

R.T.: 4.700 min
Delta R.T.: 0.000 min
Response: 20160443
Conc: 53.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Sohil
3/25/2019 9:37:46 AM

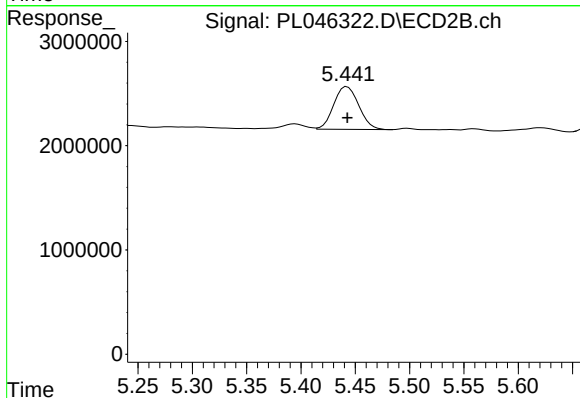


#24 Chlordane-2

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 6566979
Conc: 58.02 ng/ml

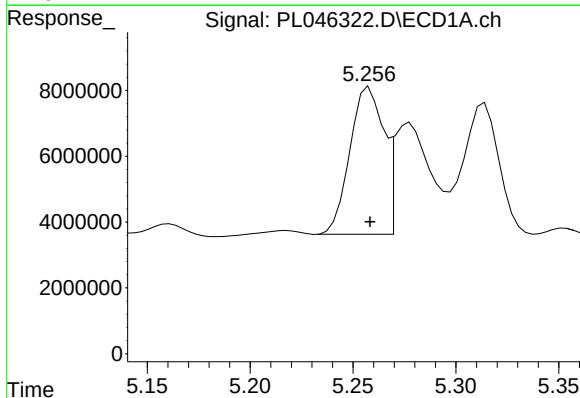


#25 Chlordane-3

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 51106244
Conc: 44.97 ng/ml

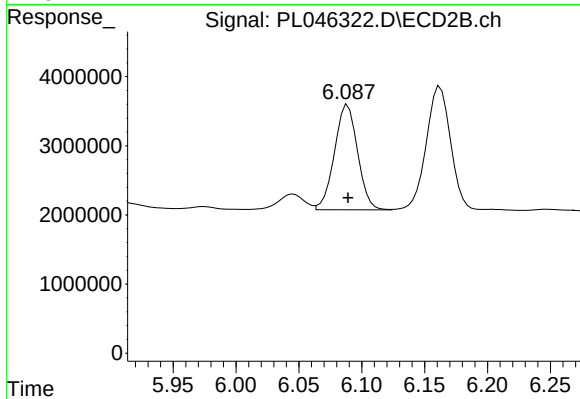

#25 Chlordane-3

R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 19506960
Conc: 51.46 ng/ml

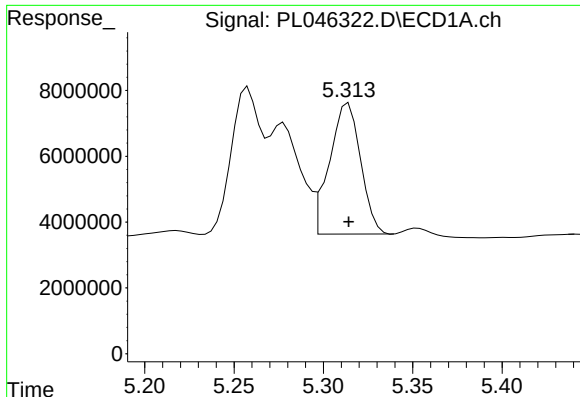


#26 Chlordane-4

R.T.: 5.314 min
Delta R.T.: 0.000 min
Response: 48226264
Conc: 45.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050


Manual Integrations
APPROVED

Sohil
3/25/2019 9:37:46 AM

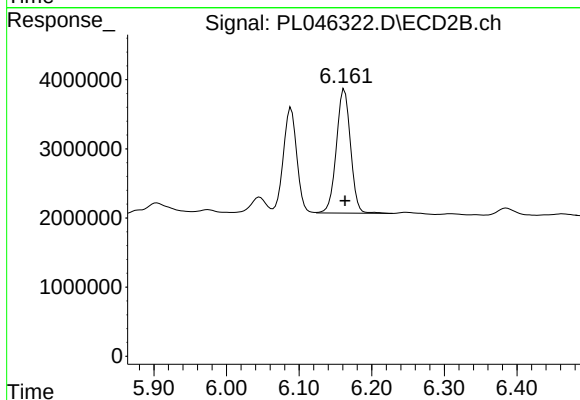


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 24347489
Conc: 53.51 ng/ml

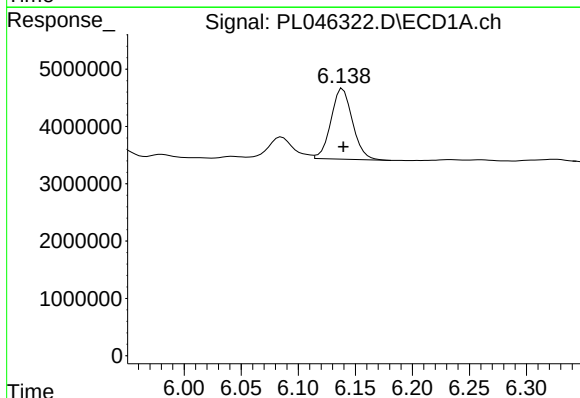


#27 Chlordane-5

R.T.: 6.139 min
Delta R.T.: 0.000 min
Response: 16153567
Conc: 46.71 ng/ml

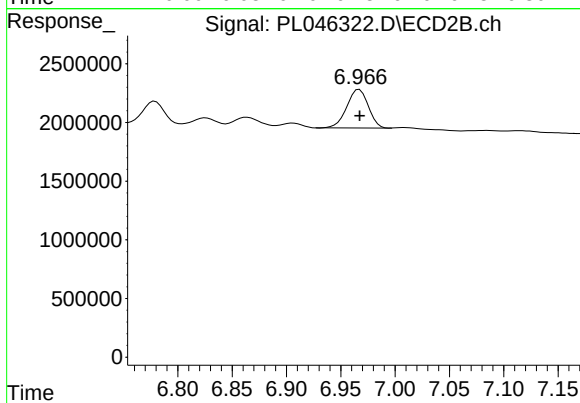

#27 Chlordane-5

R.T.: 6.967 min
Delta R.T.: 0.000 min
Response: 4526851
Conc: 50.49 ng/ml

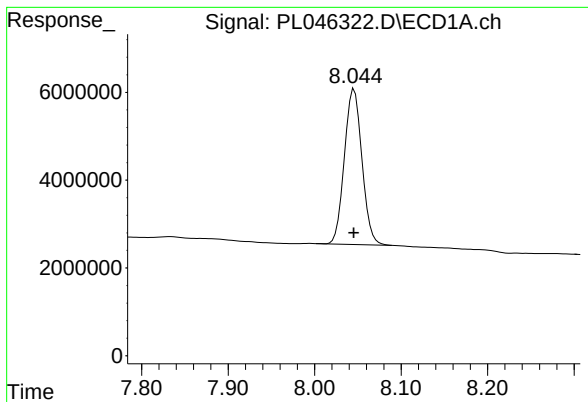


#28 Decachlorobiphenyl

R.T.: 8.046 min
Delta R.T.: 0.000 min
Response: 49717677
Conc: 6.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Manual Integrations
APPROVED

Sohil
3/25/2019 9:37:46 AM

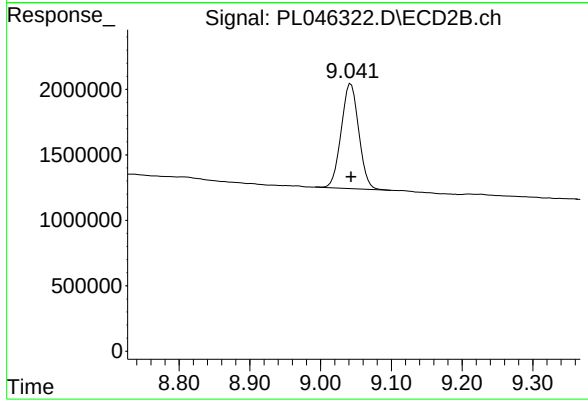

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 13805587
Conc: 6.02 ng/ml