

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
 Data File : PL046329.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 15:08
 Operator : AJ\SJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL032219CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 22 15:22:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.981	385.1E6	114.9E6	52.936	50.166
28)	SA Decachlor...	8.044	9.042	422.1E6	118.0E6	50.185	50.910
Target Compounds							
23)	Chlordane-1	4.208	4.974	168.6E6	54129653	501.331	500.195
24)	Chlordane-2	4.700	5.443	185.1E6	57930848	487.862	495.944
25)	Chlordane-3	5.258	6.089	566.6E6	193.9E6	508.744	508.686
26)	Chlordane-4	5.313	6.163	522.5E6	233.7E6	505.313	506.527
27)	Chlordane-5	6.139	6.967	170.8E6	45381900	500.351	505.154



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
Data File : PL046329.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 15:08
Operator : AJ\SJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL032219CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 22 15:22:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

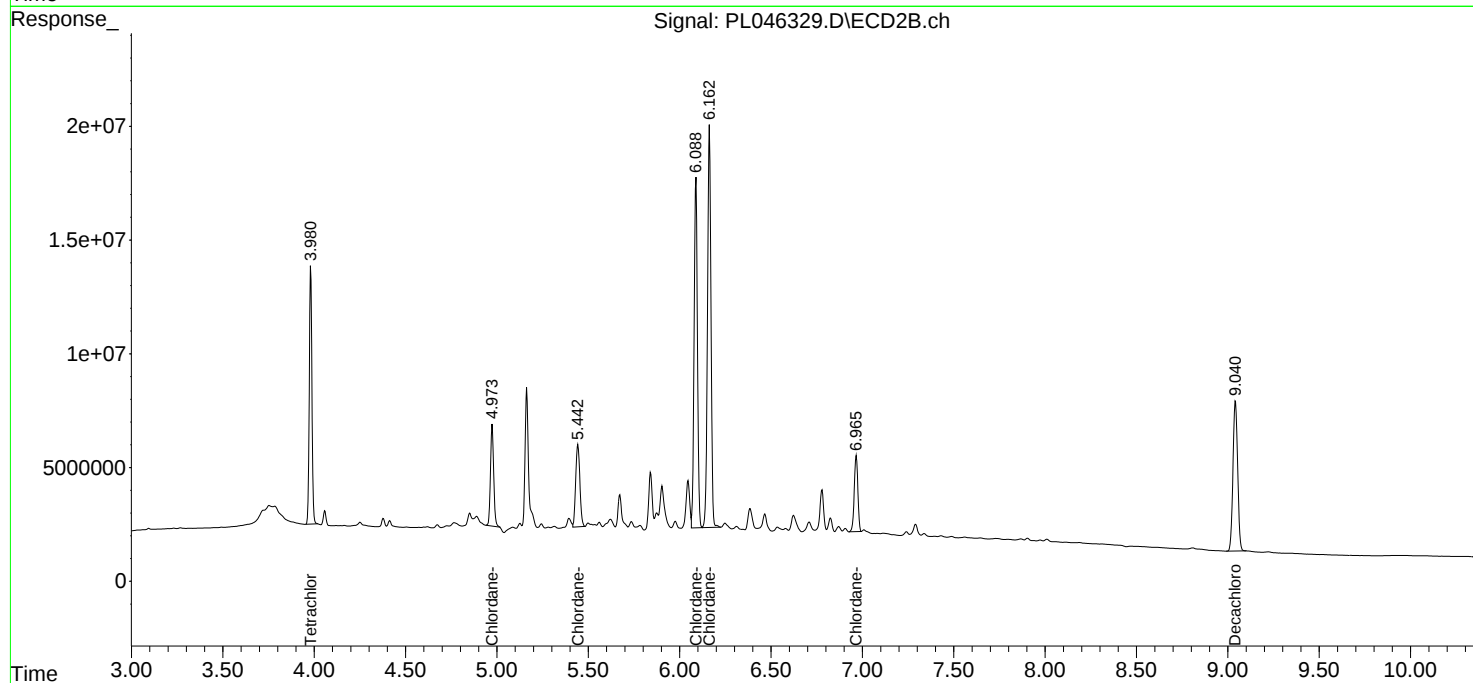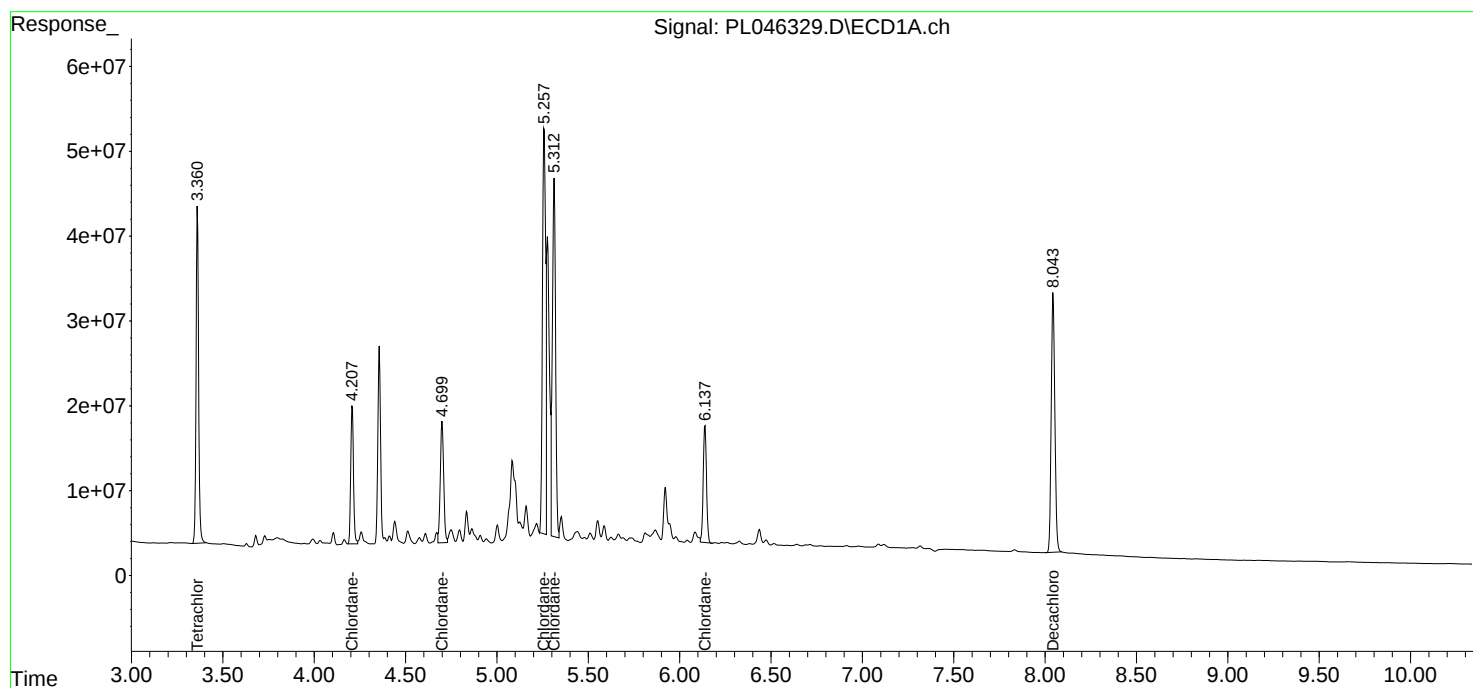


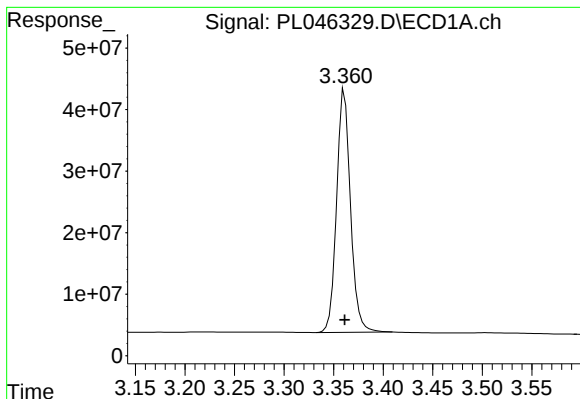

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: 0.000 min
Response: 385093647
Conc: 52.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL032219CHLOR

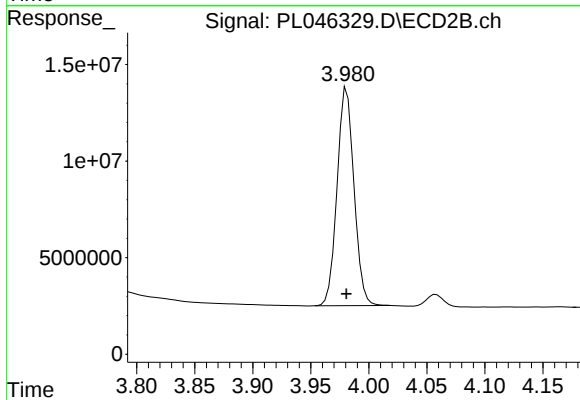


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 114859988
Conc: 50.17 ng/ml

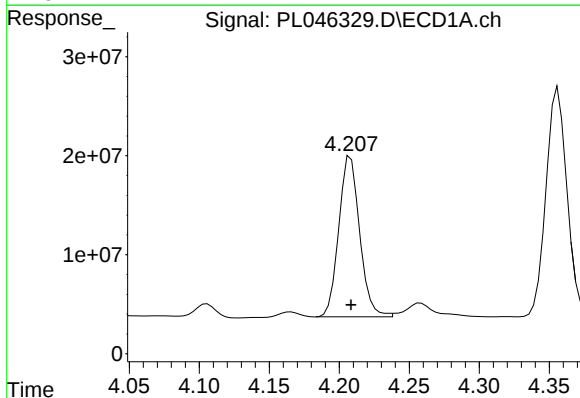


#23 Chlordane-1

R.T.: 4.208 min
Delta R.T.: 0.000 min
Response: 168595327
Conc: 501.33 ng/ml

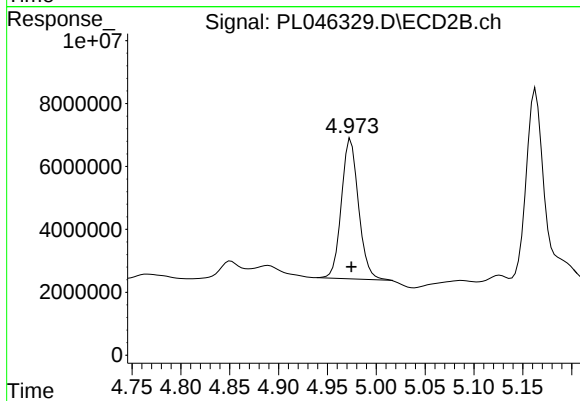

#23 Chlordane-1


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 54129653
Conc: 500.20 ng/ml

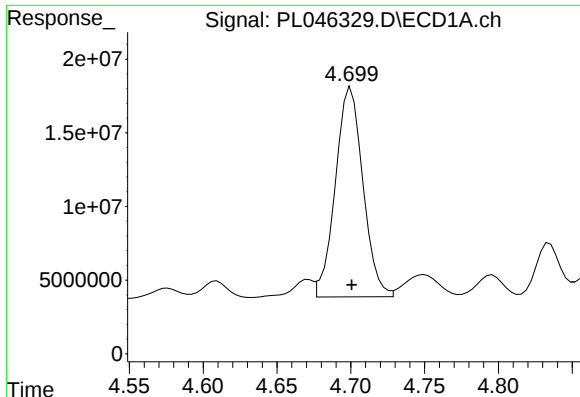

#24 Chlordane-2


R.T.: 4.700 min
Delta R.T.: 0.000 min
Response: 185104107
Conc: 487.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL032219CHLOR

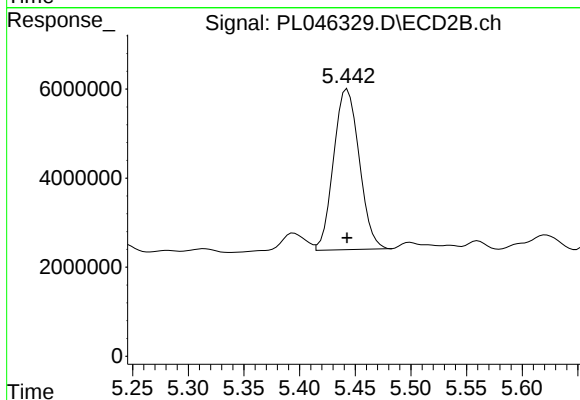


#24 Chlordane-2

R.T.: 5.443 min
Delta R.T.: 0.000 min
Response: 57930848
Conc: 495.94 ng/ml

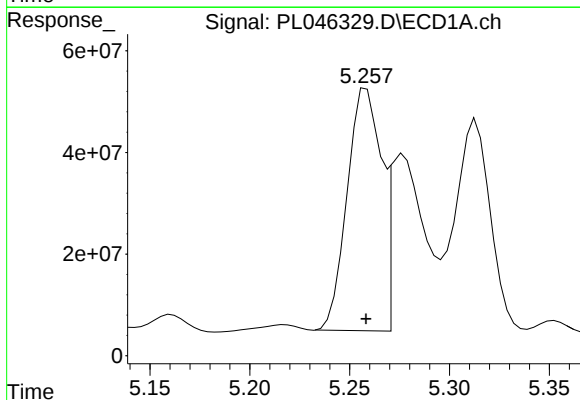


#25 Chlordane-3

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 566574359
Conc: 508.74 ng/ml

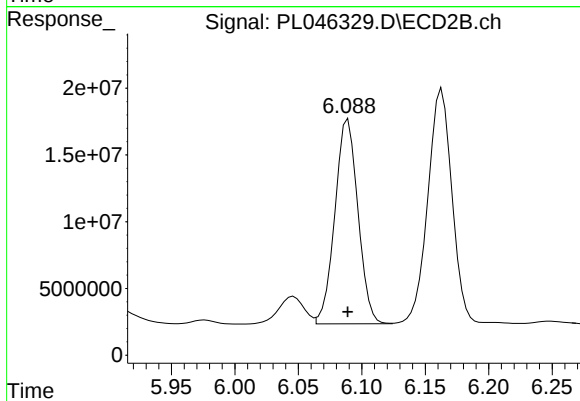

#25 Chlordane-3


R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 193945626
Conc: 508.69 ng/ml

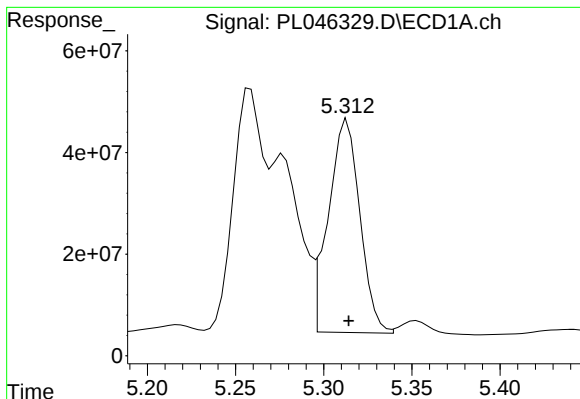

#26 Chlordane-4


R.T.: 5.313 min
Delta R.T.: 0.000 min
Response: 522523544
Conc: 505.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL032219CHLOR

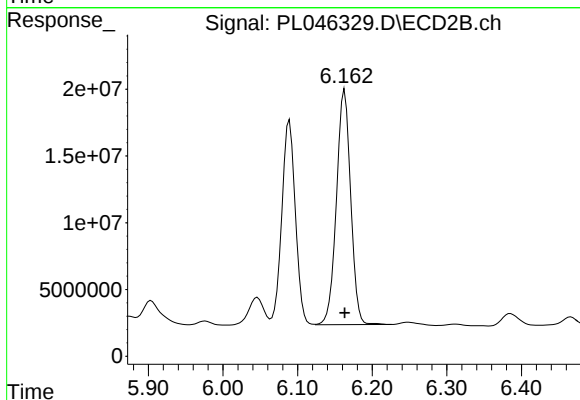


#26 Chlordane-4

R.T.: 6.163 min
Delta R.T.: 0.000 min
Response: 233724144
Conc: 506.53 ng/ml

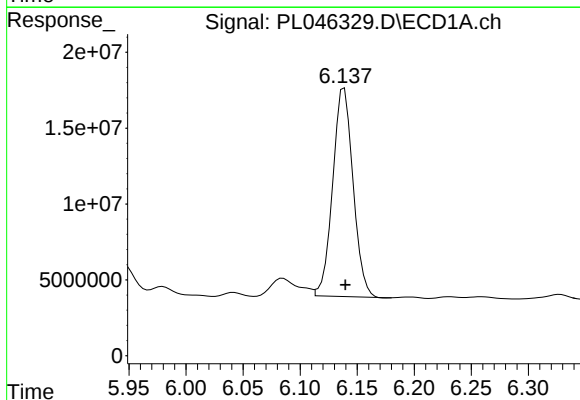


#27 Chlordane-5

R.T.: 6.139 min
Delta R.T.: 0.000 min
Response: 170753470
Conc: 500.35 ng/ml

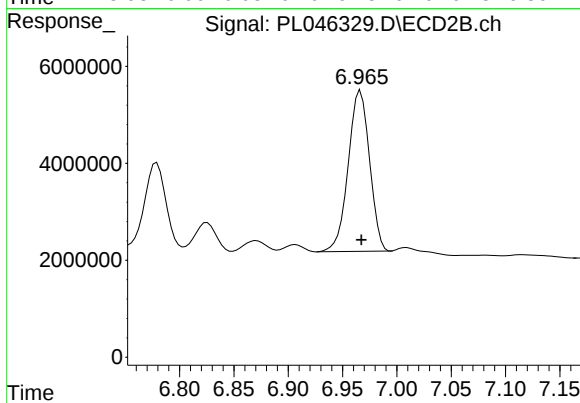

#27 Chlordane-5

R.T.: 6.967 min
Delta R.T.: 0.000 min
Response: 45381900
Conc: 505.15 ng/ml

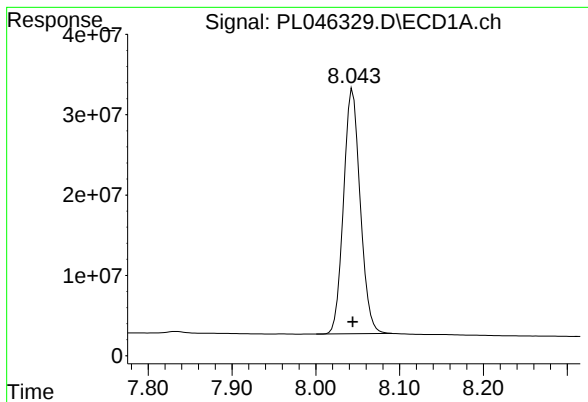

#28 Decachlorobiphenyl


R.T.: 8.044 min

Delta R.T.: 0.000 min

Response: 422107714

Conc: 50.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL032219CHLOR

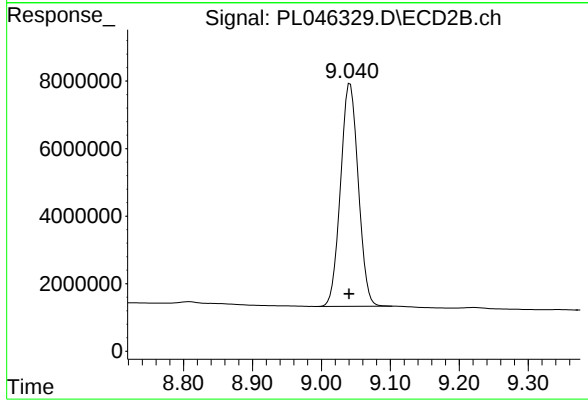

#28 Decachlorobiphenyl

R.T.: 9.042 min

Delta R.T.: 0.002 min

Response: 118032571

Conc: 50.91 ng/ml