

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
 Data File : PL046334.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2019 16:20
 Operator : AJ\SJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 04:00:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 22 13:40:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.981	387.2E6	115.8E6	53.226	50.561
28)	SA Decachlor...	8.045	9.042	426.5E6	119.9E6	50.710	51.707
Target Compounds							
23)	Chlordane-1	4.207	4.974	168.8E6	55480666	502.011	512.679
24)	Chlordane-2	4.700	5.442	187.7E6	58784654	494.778	503.253
25)	Chlordane-3	5.258	6.089	557.3E6	195.9E6	500.382	513.880
26)	Chlordane-4	5.313	6.162	524.5E6	235.0E6	507.249	509.375
27)	Chlordane-5	6.139	6.968	170.2E6	45720408	498.666	508.922



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032219\
Data File : PL046334.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2019 16:20
Operator : AJ\SJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 04:00:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL032219.M
Quant Title : GC Extractables
QLast Update : Fri Mar 22 13:40:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

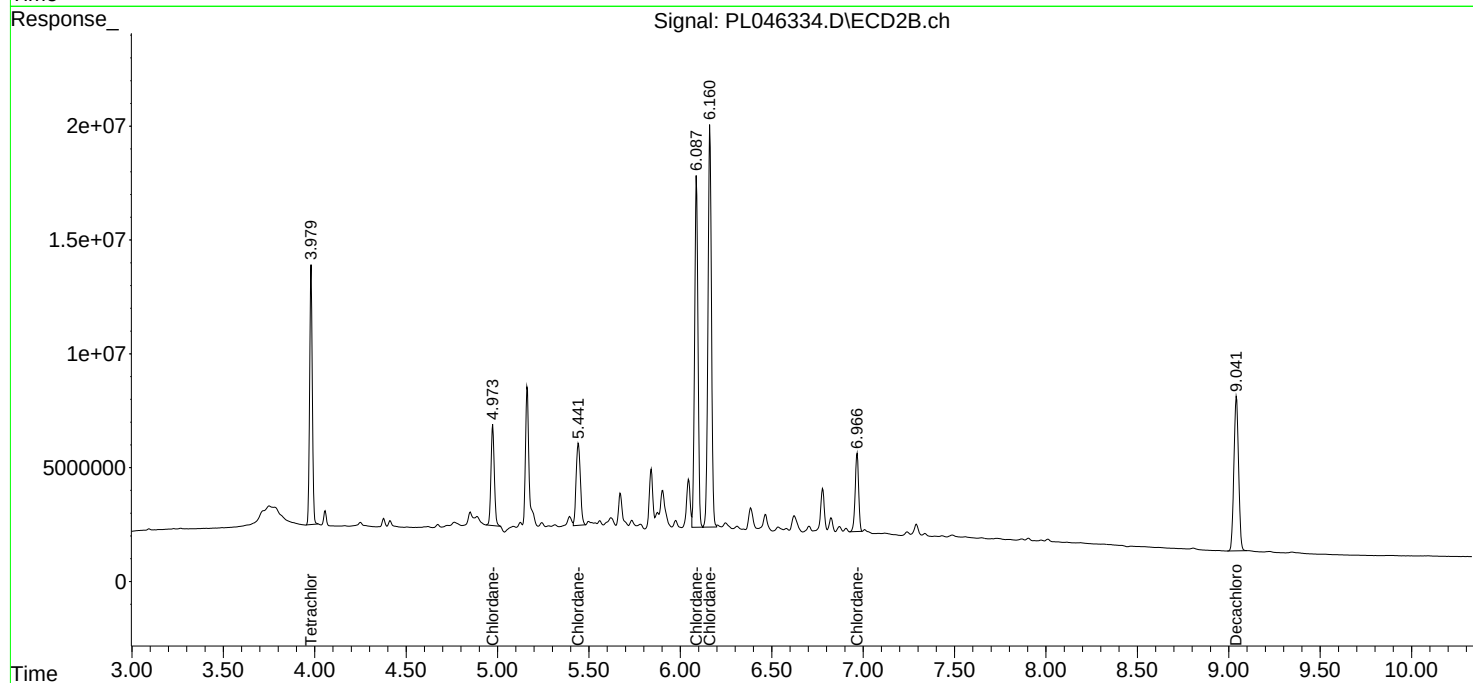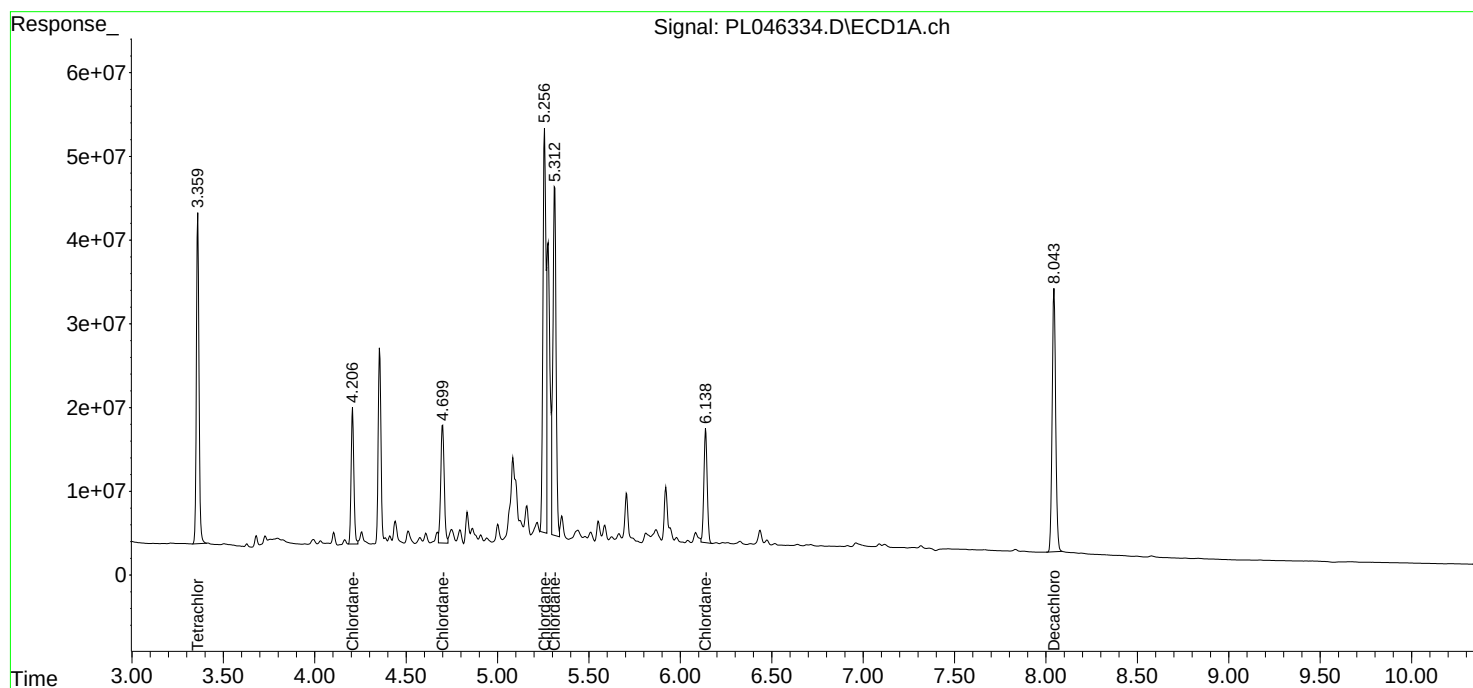


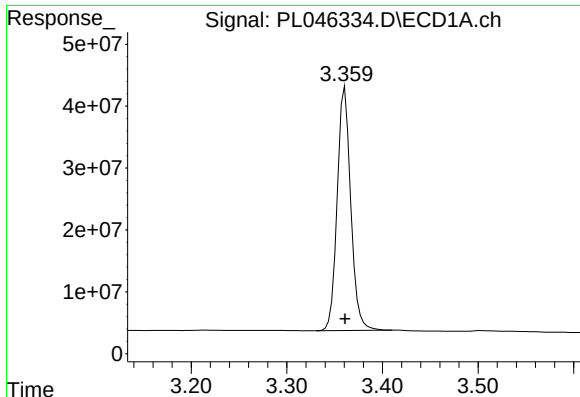

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: 0.000 min
Response: 387202124
Conc: 53.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

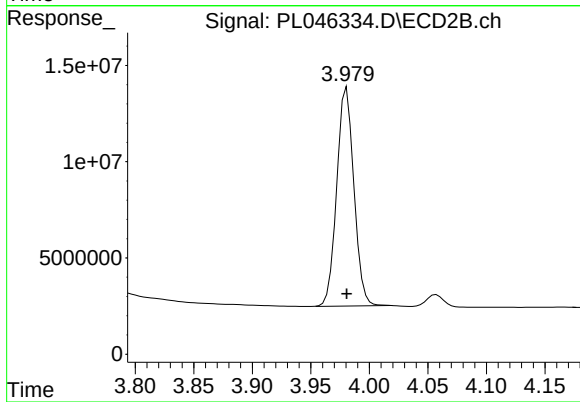


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 115765660
Conc: 50.56 ng/ml

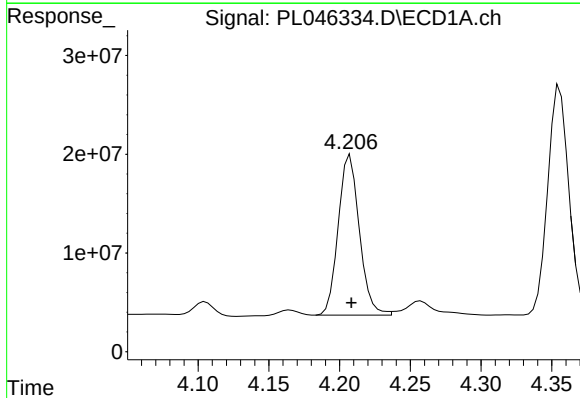


#23 Chlordane-1

R.T.: 4.207 min
Delta R.T.: 0.000 min
Response: 168824012
Conc: 502.01 ng/ml

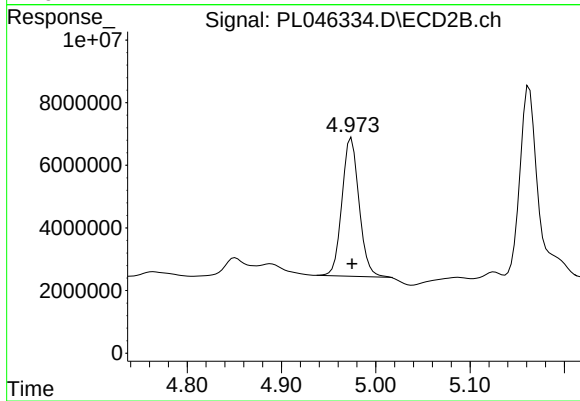

#23 Chlordane-1


R.T.: 4.974 min
Delta R.T.: 0.000 min
Response: 55480666
Conc: 512.68 ng/ml

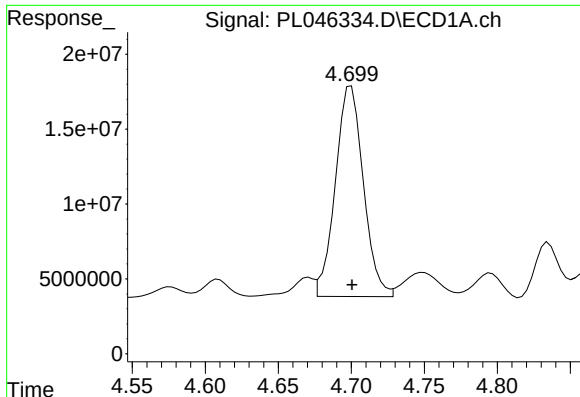

#24 Chlordane-2


R.T.: 4.700 min
Delta R.T.: 0.000 min
Response: 187728217
Conc: 494.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

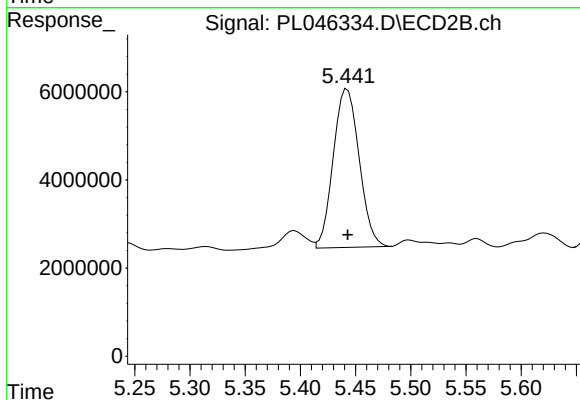


#24 Chlordane-2

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 58784654
Conc: 503.25 ng/ml

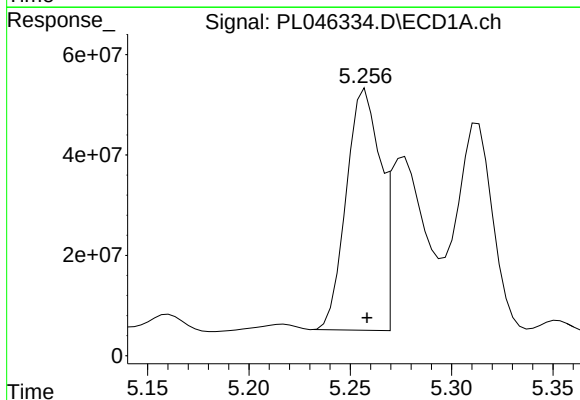


#25 Chlordane-3

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 557261849
Conc: 500.38 ng/ml

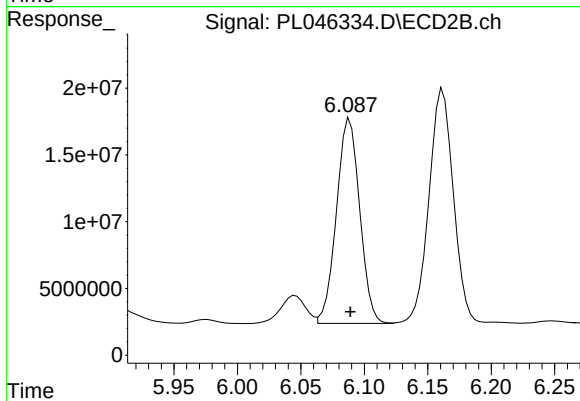

#25 Chlordane-3


R.T.: 6.089 min
Delta R.T.: 0.000 min
Response: 195925994
Conc: 513.88 ng/ml

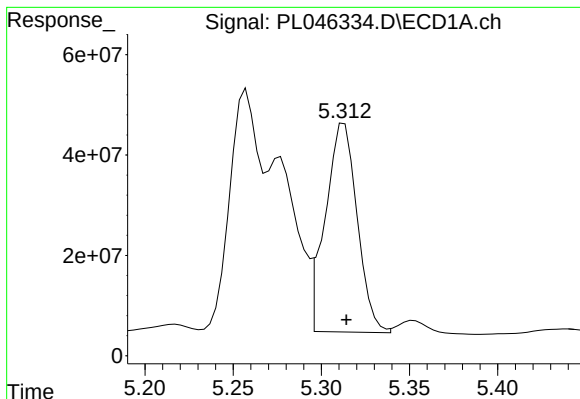

#26 Chlordane-4


R.T.: 5.313 min
Delta R.T.: -0.001 min
Response: 524525671
Conc: 507.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

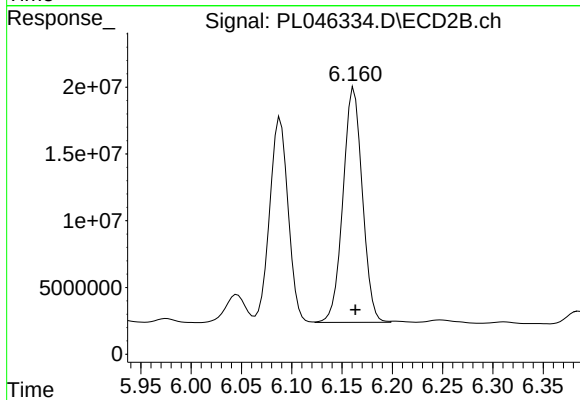


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: -0.001 min
Response: 235038301
Conc: 509.37 ng/ml

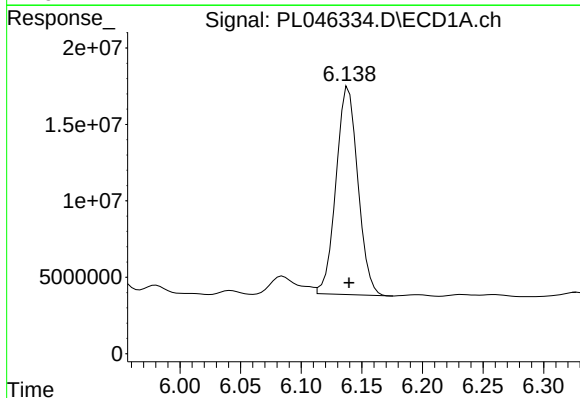


#27 Chlordane-5

R.T.: 6.139 min
Delta R.T.: 0.000 min
Response: 170178217
Conc: 498.67 ng/ml

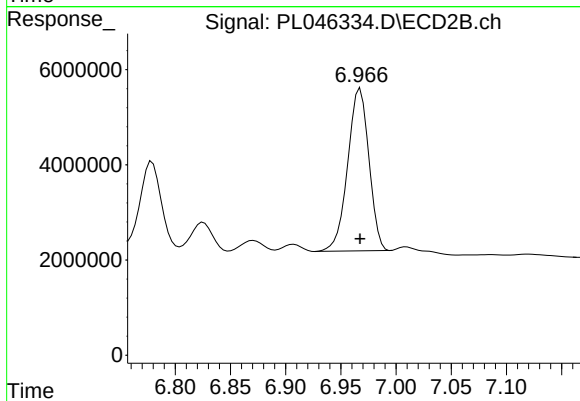

#27 Chlordane-5


R.T.: 6.968 min
Delta R.T.: 0.000 min
Response: 45720408
Conc: 508.92 ng/ml

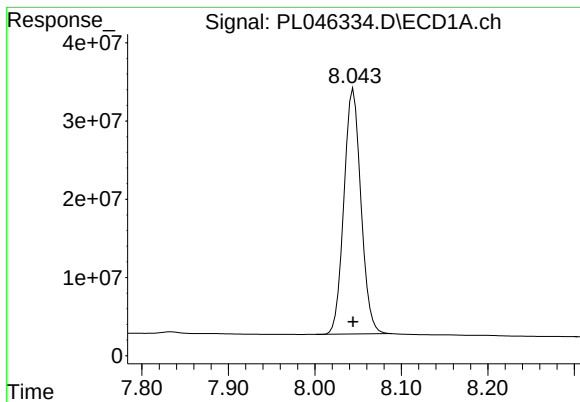

#28 Decachlorobiphenyl

R.T.: 8.045 min
Delta R.T.: 0.000 min
Response: 426523845
Conc: 50.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

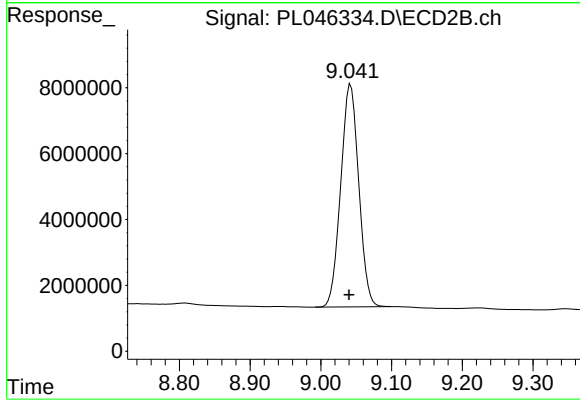

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.002 min
Response: 119882142
Conc: 51.71 ng/ml