

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032221\
 Data File : PL065472.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Mar 2021 15:33
 Operator : AR\AJ
 Sample : M1718-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BACKFILL-ASHCROFT-REAR-04

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 23 02:03:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 19 02:14:11 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.286	3.785	28742922	28909682	12.103	10.533
28)	SA Decachlor...	7.925	8.733	28988809	24318914	11.998	12.269
Target Compounds							
4)	MA Heptachlor	0.000	4.944	0	519566	N.D.	0.156 #
6)	B beta-BHC	0.000	4.637	0	4125305	N.D.	2.395 #
8)	B Heptachlo...	0.000	5.641f	0	947341	N.D.	0.328 #
9)	A Endosulfan I	0.000	5.997f	0	956446	N.D.	0.363 #
10)	B gamma-Chl...	0.000	5.831f	0	548545	N.D.	0.197 #
11)	B alpha-Chl...	0.000	5.924	0	275281	N.D.	0.099 #
16)	A 4,4'-DDD	0.000	6.589	0	1005445	N.D.	0.457 #
25)	Chlordane-3	0.000	5.831f	0	548545	N.D.	1.346 #
26)	Chlordane-4	0.000	5.924	0	275281	N.D.	0.572 #
27)	Chlordane-5	0.000	6.698f	0	1475330	N.D.	18.437 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL032221\
Data File : PL065472.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Mar 2021 15:33
Operator : AR\AJ
Sample : M1718-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BACKFILL-ASHCROFT-REAR-04

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 23 02:03:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031821.M
Quant Title : GC Extractables
QLast Update : Fri Mar 19 02:14:11 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

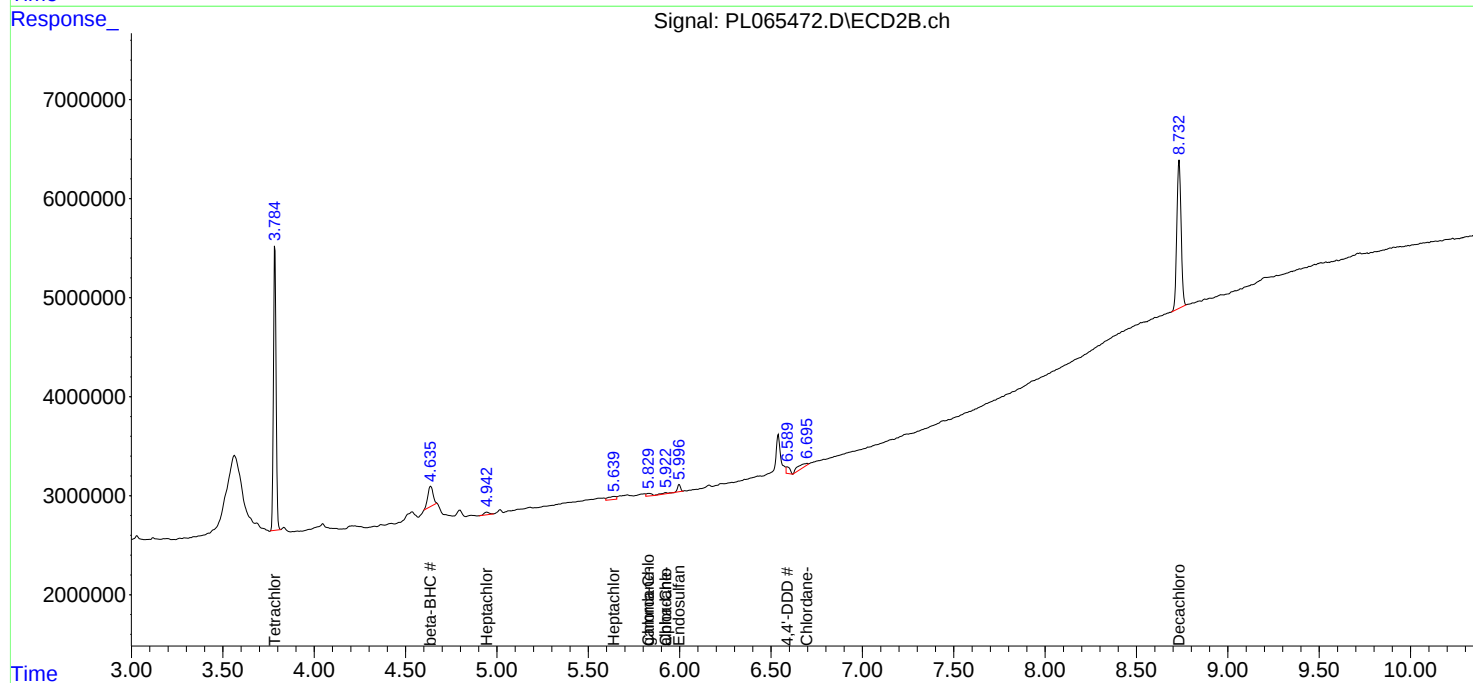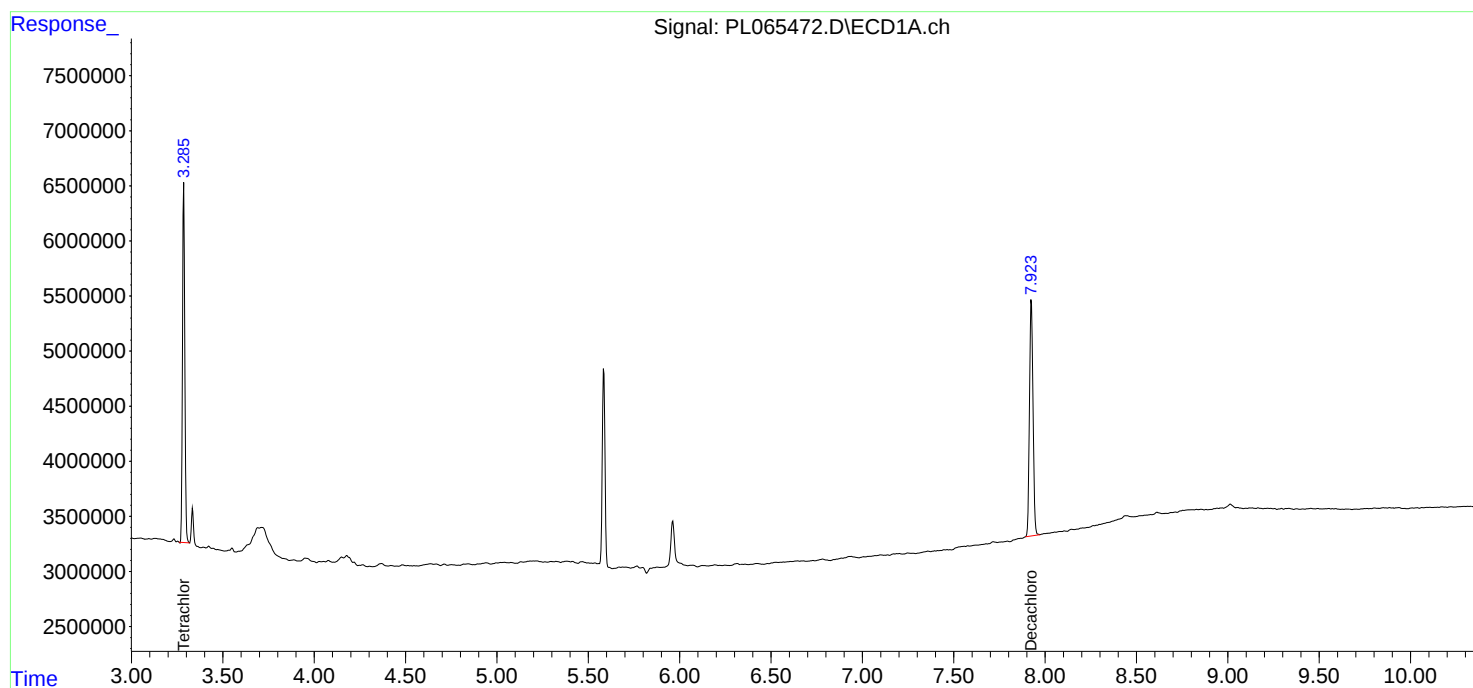


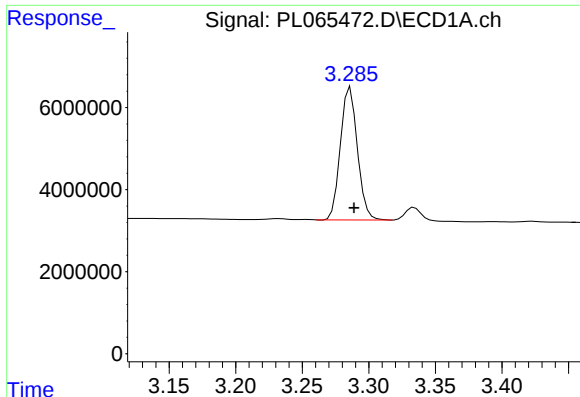

#1 Tetrachloro-m-xylene


R.T.: 3.286 min
Delta R.T.: -0.003 min
Response: 28742922
Conc: 12.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
BACKFILL-ASHCROFT-REAR-04

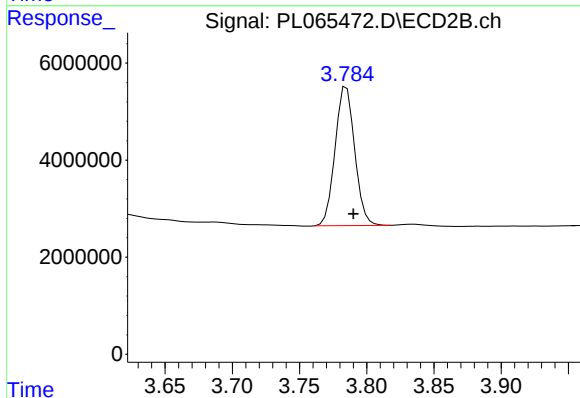


#1 Tetrachloro-m-xylene

R.T.: 3.785 min
Delta R.T.: -0.005 min
Response: 28909682
Conc: 10.53 ng/ml

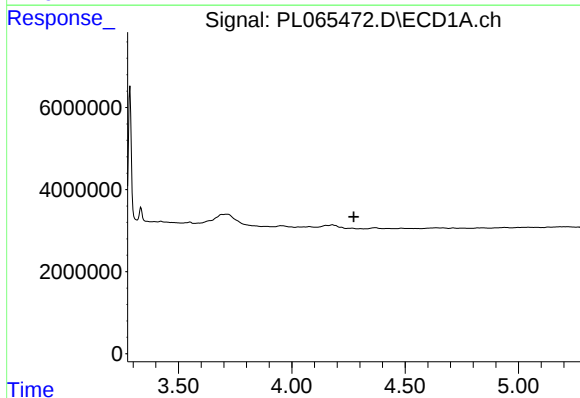


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.274 min
Response: 0
Conc: N.D.

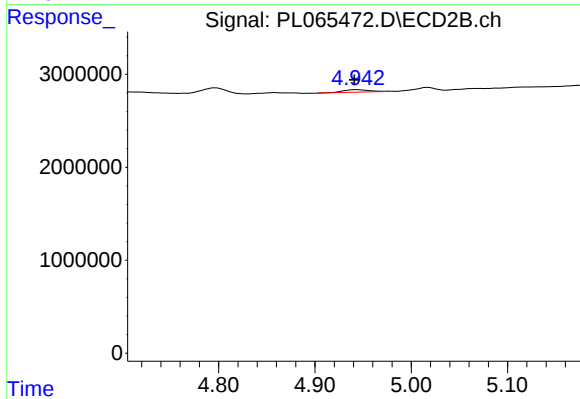

#4 Heptachlor


R.T.: 4.944 min
Delta R.T.: 0.003 min
Response: 519566
Conc: 0.16 ng/ml

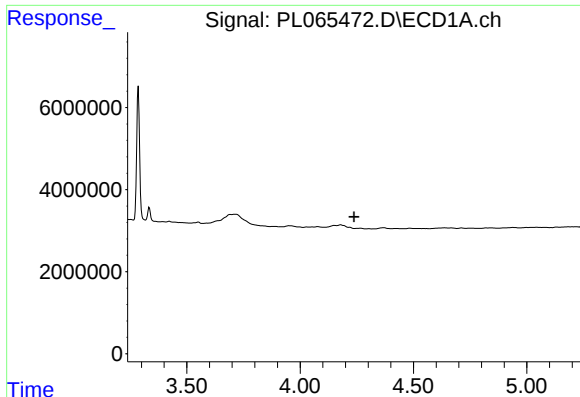

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.238 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BACKFILL-ASHCROFT-REAR-04

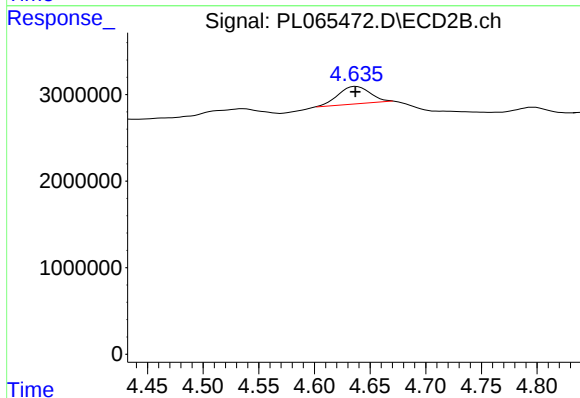


#6 beta-BHC

R.T.: 4.637 min
Delta R.T.: 0.000 min
Response: 4125305
Conc: 2.39 ng/ml

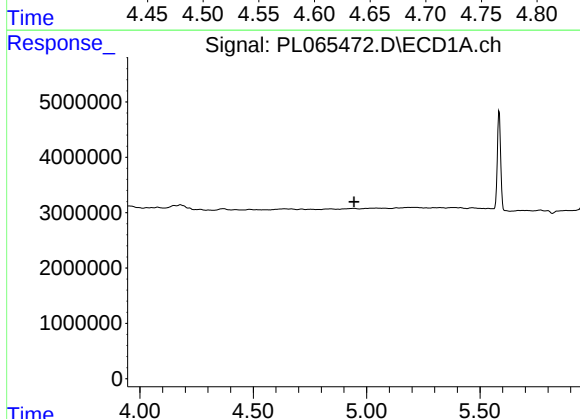


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 4.944 min
Response: 0
Conc: N.D.

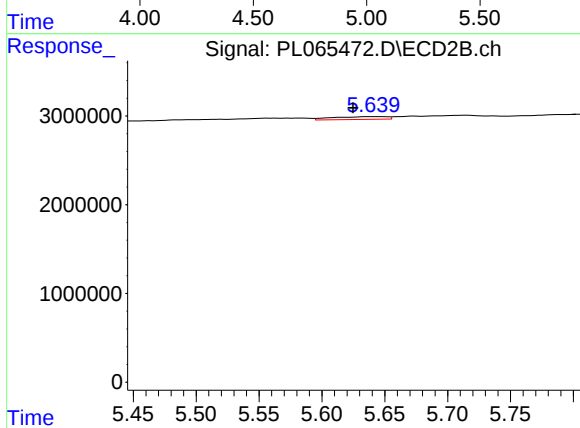

#8 Heptachlor epoxide


R.T.: 5.641 min
Delta R.T.: 0.016 min
Response: 947341
Conc: 0.33 ng/ml

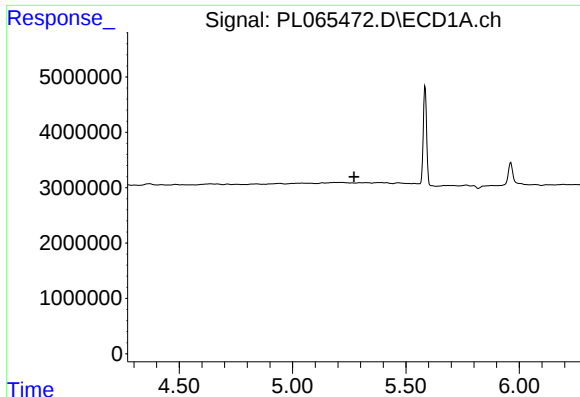

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.271 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BACKFILL-ASHCROFT-REAR-04

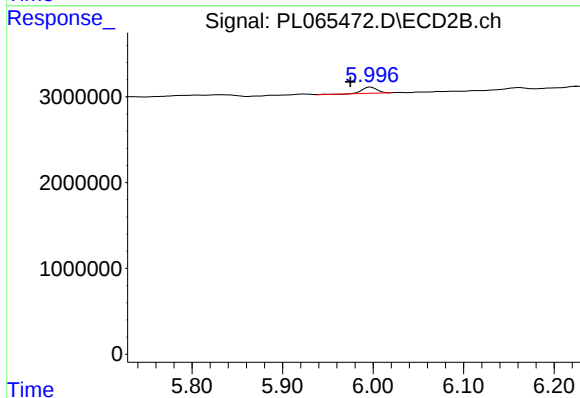


#9 Endosulfan I

R.T.: 5.997 min
Delta R.T.: 0.022 min
Response: 956446
Conc: 0.36 ng/ml

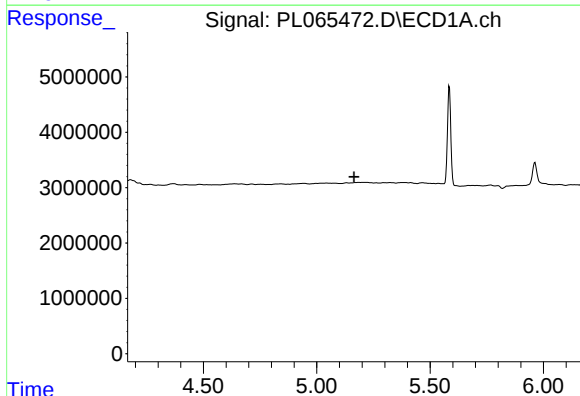


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.165 min
Response: 0
Conc: N.D.

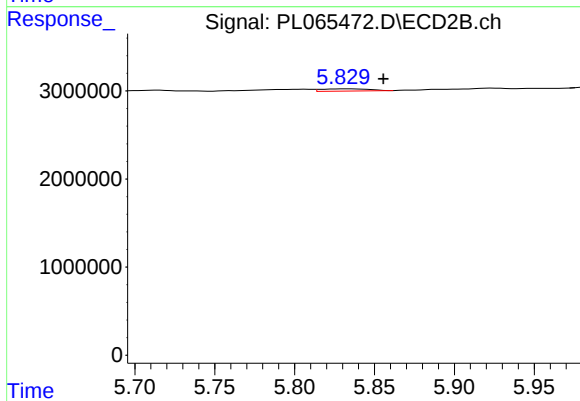

#10 gamma-Chlordane


R.T.: 5.831 min
Delta R.T.: -0.025 min
Response: 548545
Conc: 0.20 ng/ml

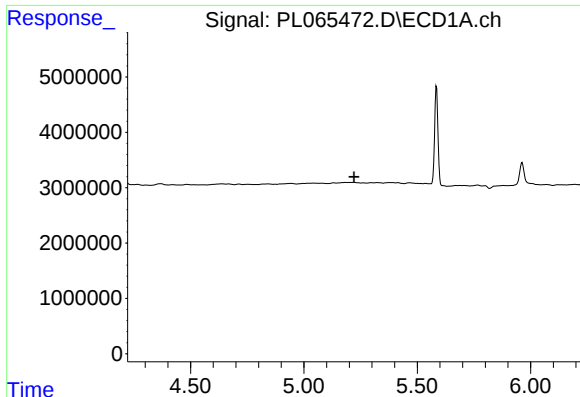

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BACKFILL-ASHCROFT-REAR-04

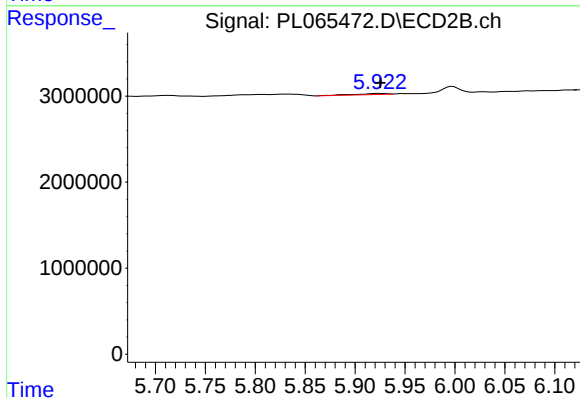


#11 alpha-Chlordane

R.T.: 5.924 min
Delta R.T.: -0.001 min
Response: 275281
Conc: 0.10 ng/ml

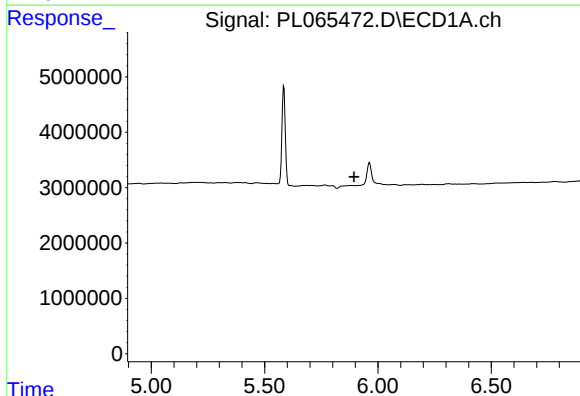


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.894 min
Response: 0
Conc: N.D.

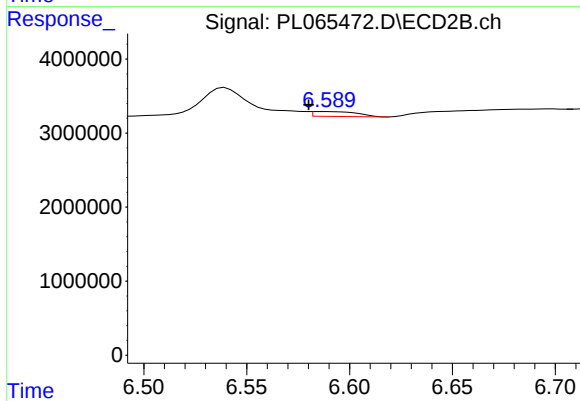

#16 4,4'-DDD


R.T.: 6.589 min
Delta R.T.: 0.008 min
Response: 1005445
Conc: 0.46 ng/ml

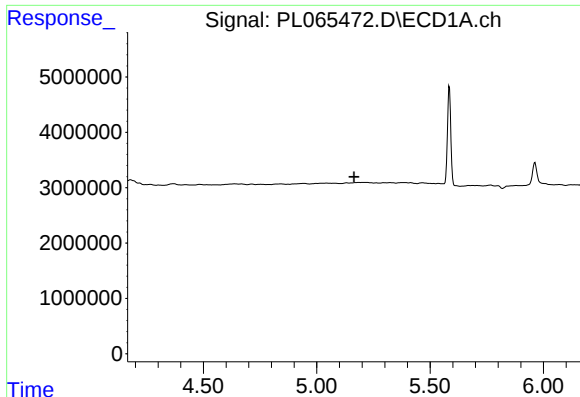

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.165 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BACKFILL-ASHCROFT-REAR-04

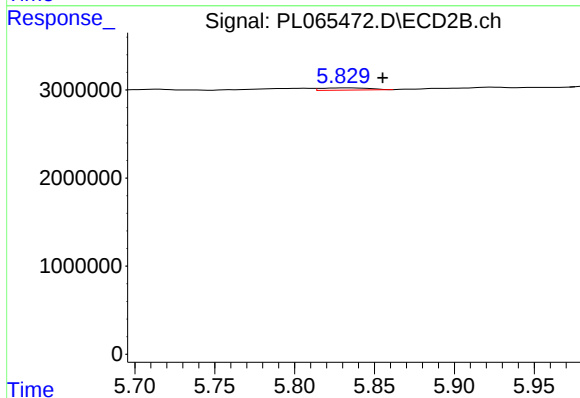


#25 Chlordane-3

R.T.: 5.831 min
Delta R.T.: -0.024 min
Response: 548545
Conc: 1.35 ng/ml

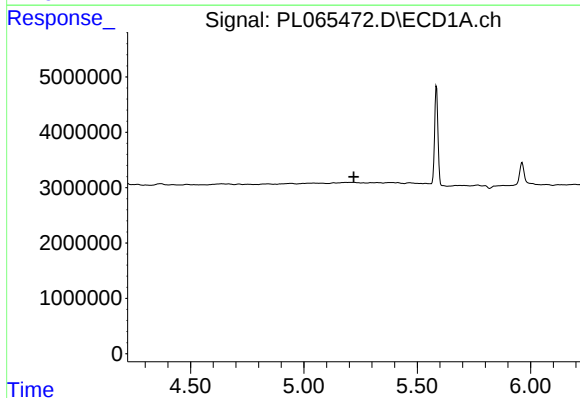


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.220 min
Response: 0
Conc: N.D.

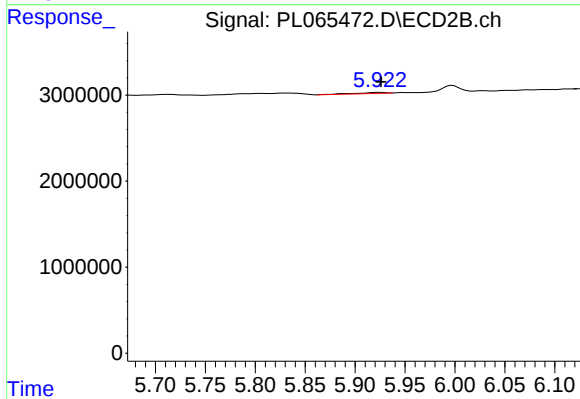

#26 Chlordane-4


R.T.: 5.924 min
Delta R.T.: -0.002 min
Response: 275281
Conc: 0.57 ng/ml

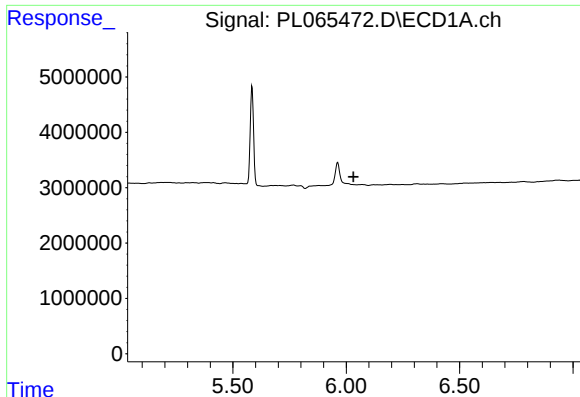

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.033 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
BACKFILL-ASHCROFT-REAR-04

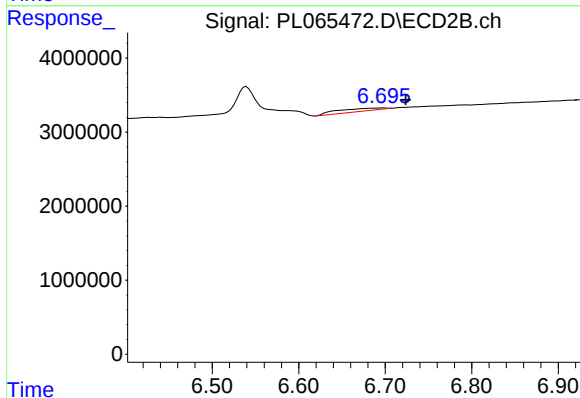


#27 Chlordane-5

R.T.: 6.698 min
Delta R.T.: -0.026 min
Response: 1475330
Conc: 18.44 ng/ml

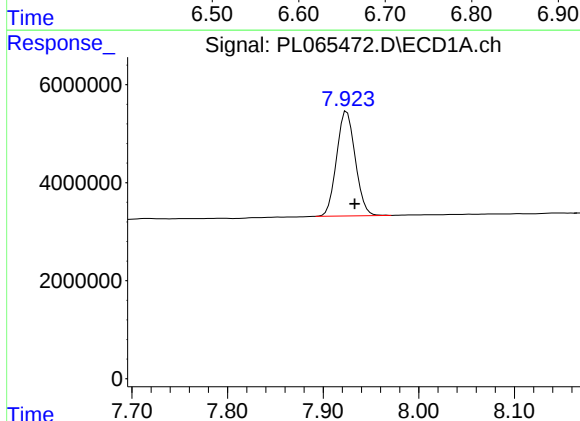

#28 Decachlorobiphenyl

R.T.: 7.925 min
Delta R.T.: -0.008 min
Response: 28988809
Conc: 12.00 ng/ml

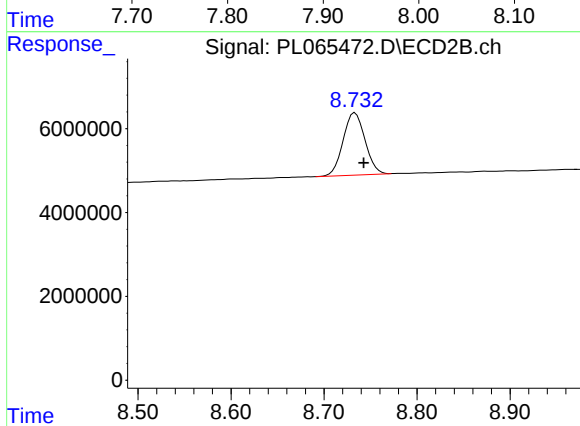

#28 Decachlorobiphenyl

R.T.: 8.733 min
Delta R.T.: -0.009 min
Response: 24318914
Conc: 12.27 ng/ml